

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032023\
 Data File : BN024447.D
 Acq On : 21 Mar 2023 13:53
 Operator : CG/JU
 Sample : 01884-08
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB916

Quant Time: Mar 21 17:39:28 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 21 02:42:36 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.034	152	9007	0.400	ng/ul	0.00
4) Naphthalene-d8	10.850	136	27588	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.666	164	16771	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.413	188	33778	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.600	240	28504	0.400	ng/ul	# 0.00
23) Perylene-d12	24.085	264	28537	0.400	ng/ul	#-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	37108	3.744	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.429	152	11208	0.342	ng/ul	0.00
18) Fluoranthene-d10	19.436	212	24508	0.323	ng/ul	0.00
Target Compounds						
						Qvalue
10) Acenaphthylene	14.398	152	2474	0.035	ng/ul#	54
16) Anthracene	17.544	178	7281	0.086	ng/ul#	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032023\
Data File : BN024447.D
Acq On : 21 Mar 2023 13:53
Operator : CG/JU
Sample : 01884-08
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB916

Quant Time: Mar 21 17:39:28 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 21 02:42:36 2023
Response via : Initial Calibration




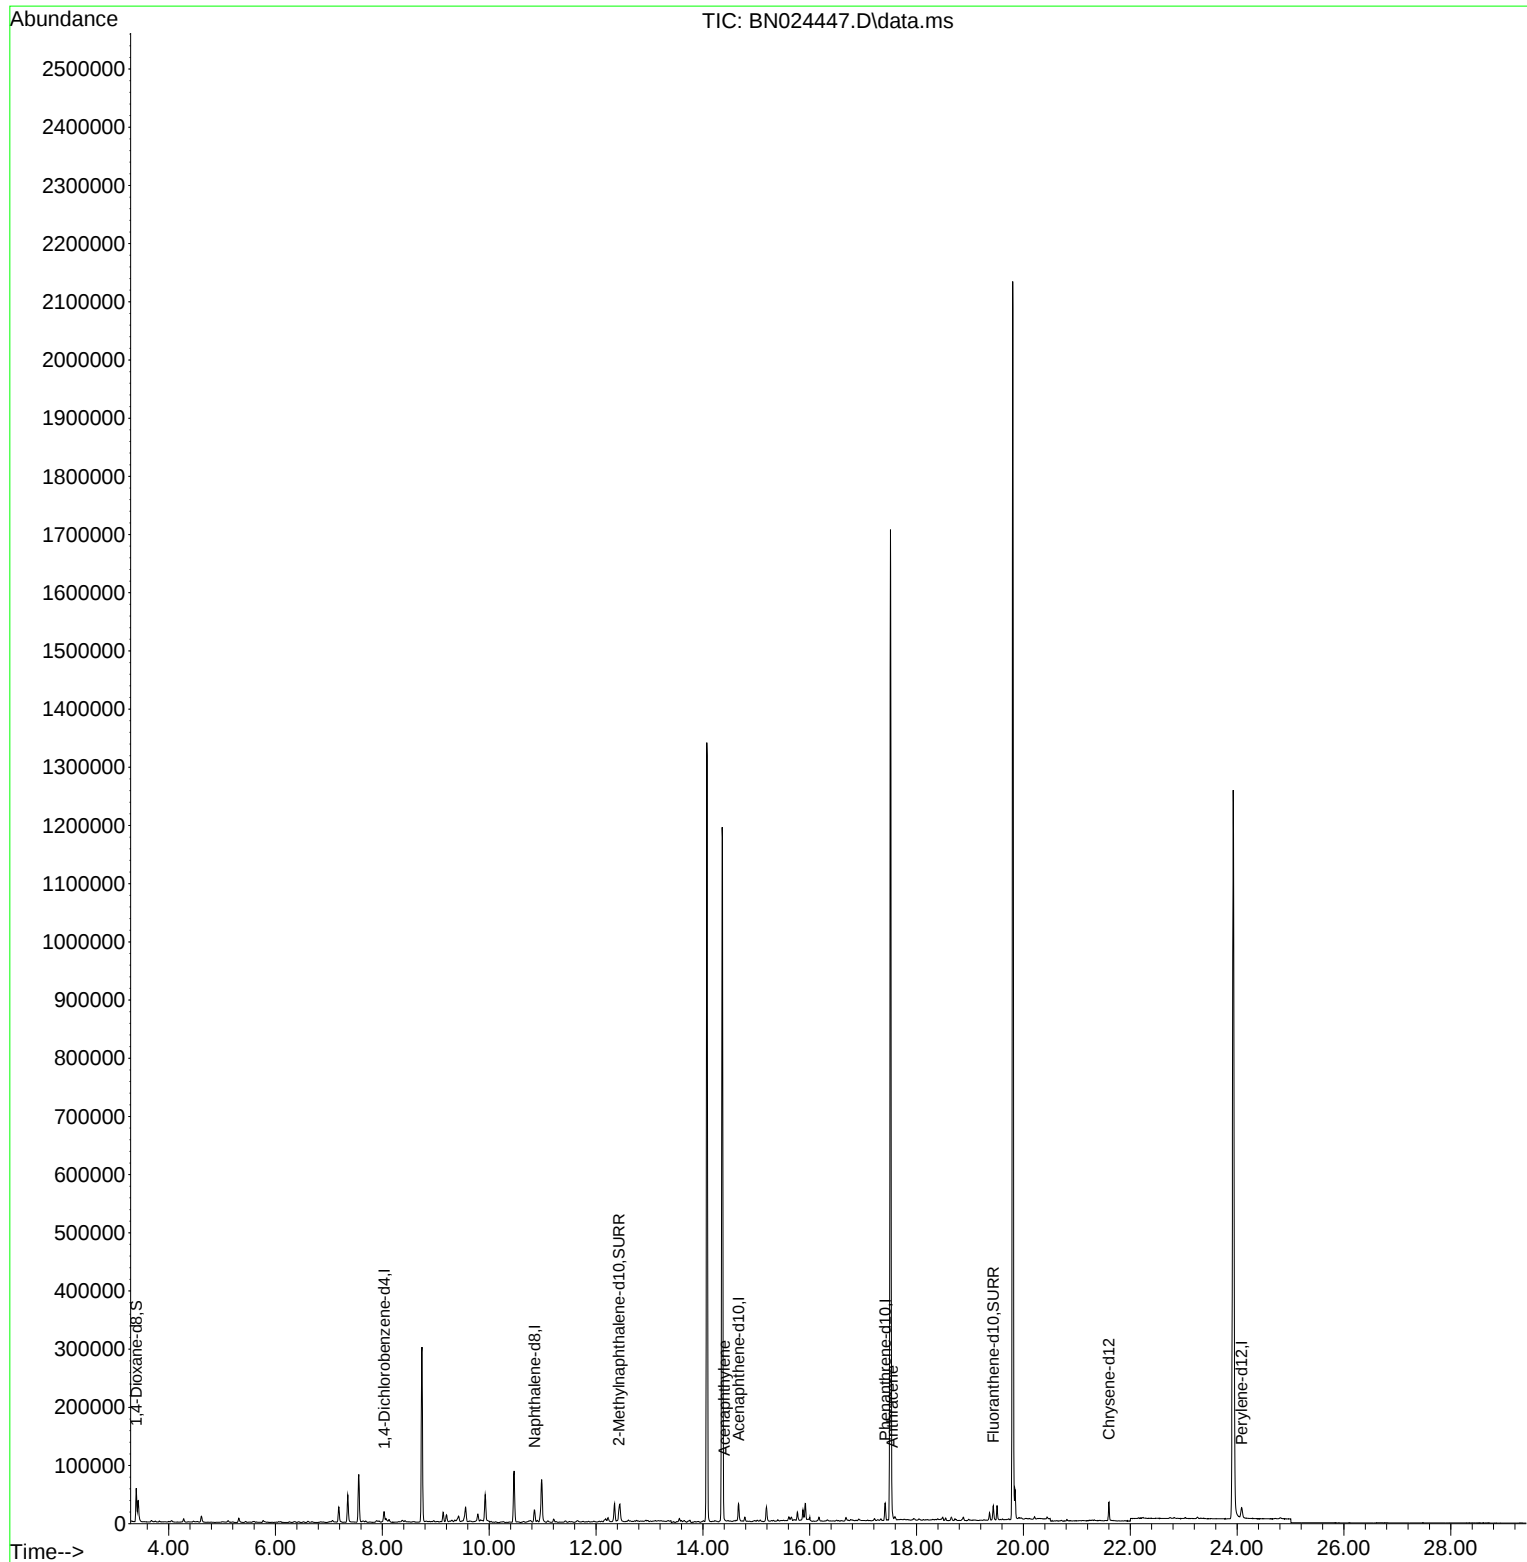


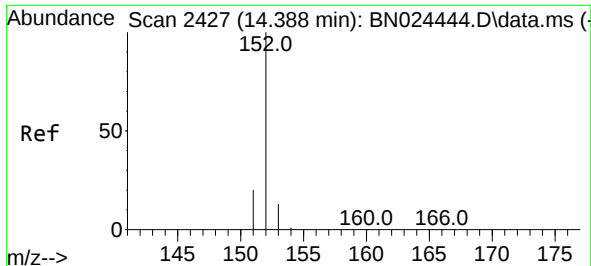

#10
Acenaphthylene
Concen: 0.035 ng/ul
RT: 14.398 min Scan# 2429
Delta R.T. 0.005 min
Lab File: BN024447.D
Acq: 21 Mar 2023 13:53

Instrument :
BNA_N
ClientSampleId :
CB916

Tgt Ion:152 Resp: 2474
Ion Ratio Lower Upper
152 100
151 39.4 15.9 23.9#
153 34.1 10.6 16.0#

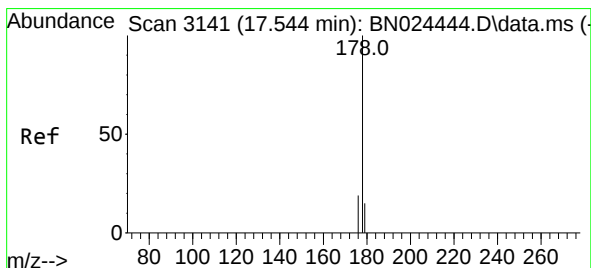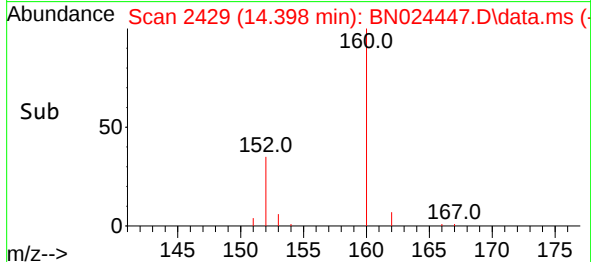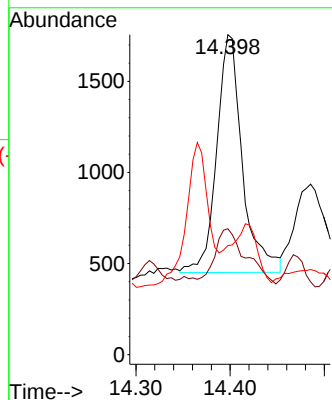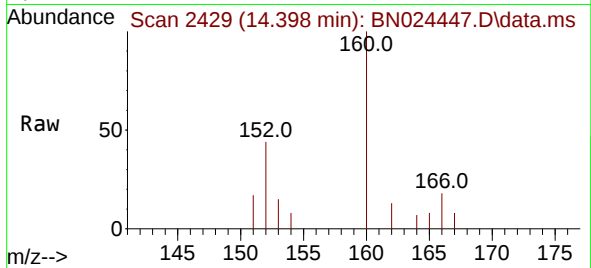

#16
Anthracene
Concen: 0.086 ng/ul
RT: 17.544 min Scan# 3141
Delta R.T. -0.004 min
Lab File: BN024447.D
Acq: 21 Mar 2023 13:53

Tgt Ion:178 Resp: 7281
Ion Ratio Lower Upper
178 100
179 32.2 12.3 18.5#
176 32.4 15.3 22.9#

