

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032023\
 Data File : BN024448.D
 Acq On : 21 Mar 2023 14:30
 Operator : CG/JU
 Sample : 01884-10
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB919

Quant Time: Mar 21 17:39:33 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 21 02:42:36 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.034	152	9333	0.400	ng/ul	0.00
4) Naphthalene-d8	10.850	136	28472	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.666	164	18171	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.413	188	35171	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.595	240	29557	0.400	ng/ul	# 0.00
23) Perylene-d12	24.091	264	29375	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	40156	3.910	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.429	152	14588	0.431	ng/ul	0.00
18) Fluoranthene-d10	19.436	212	32816	0.417	ng/ul	0.00
Target Compounds						
					Qvalue	
15) Phenanthrene	17.456	178	3722	0.037	ng/ul#	52
16) Anthracene	17.548	178	6492	0.073	ng/ul#	67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032023\
Data File : BN024448.D
Acq On : 21 Mar 2023 14:30
Operator : CG/JU
Sample : 01884-10
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB919

Quant Time: Mar 21 17:39:33 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 21 02:42:36 2023
Response via : Initial Calibration




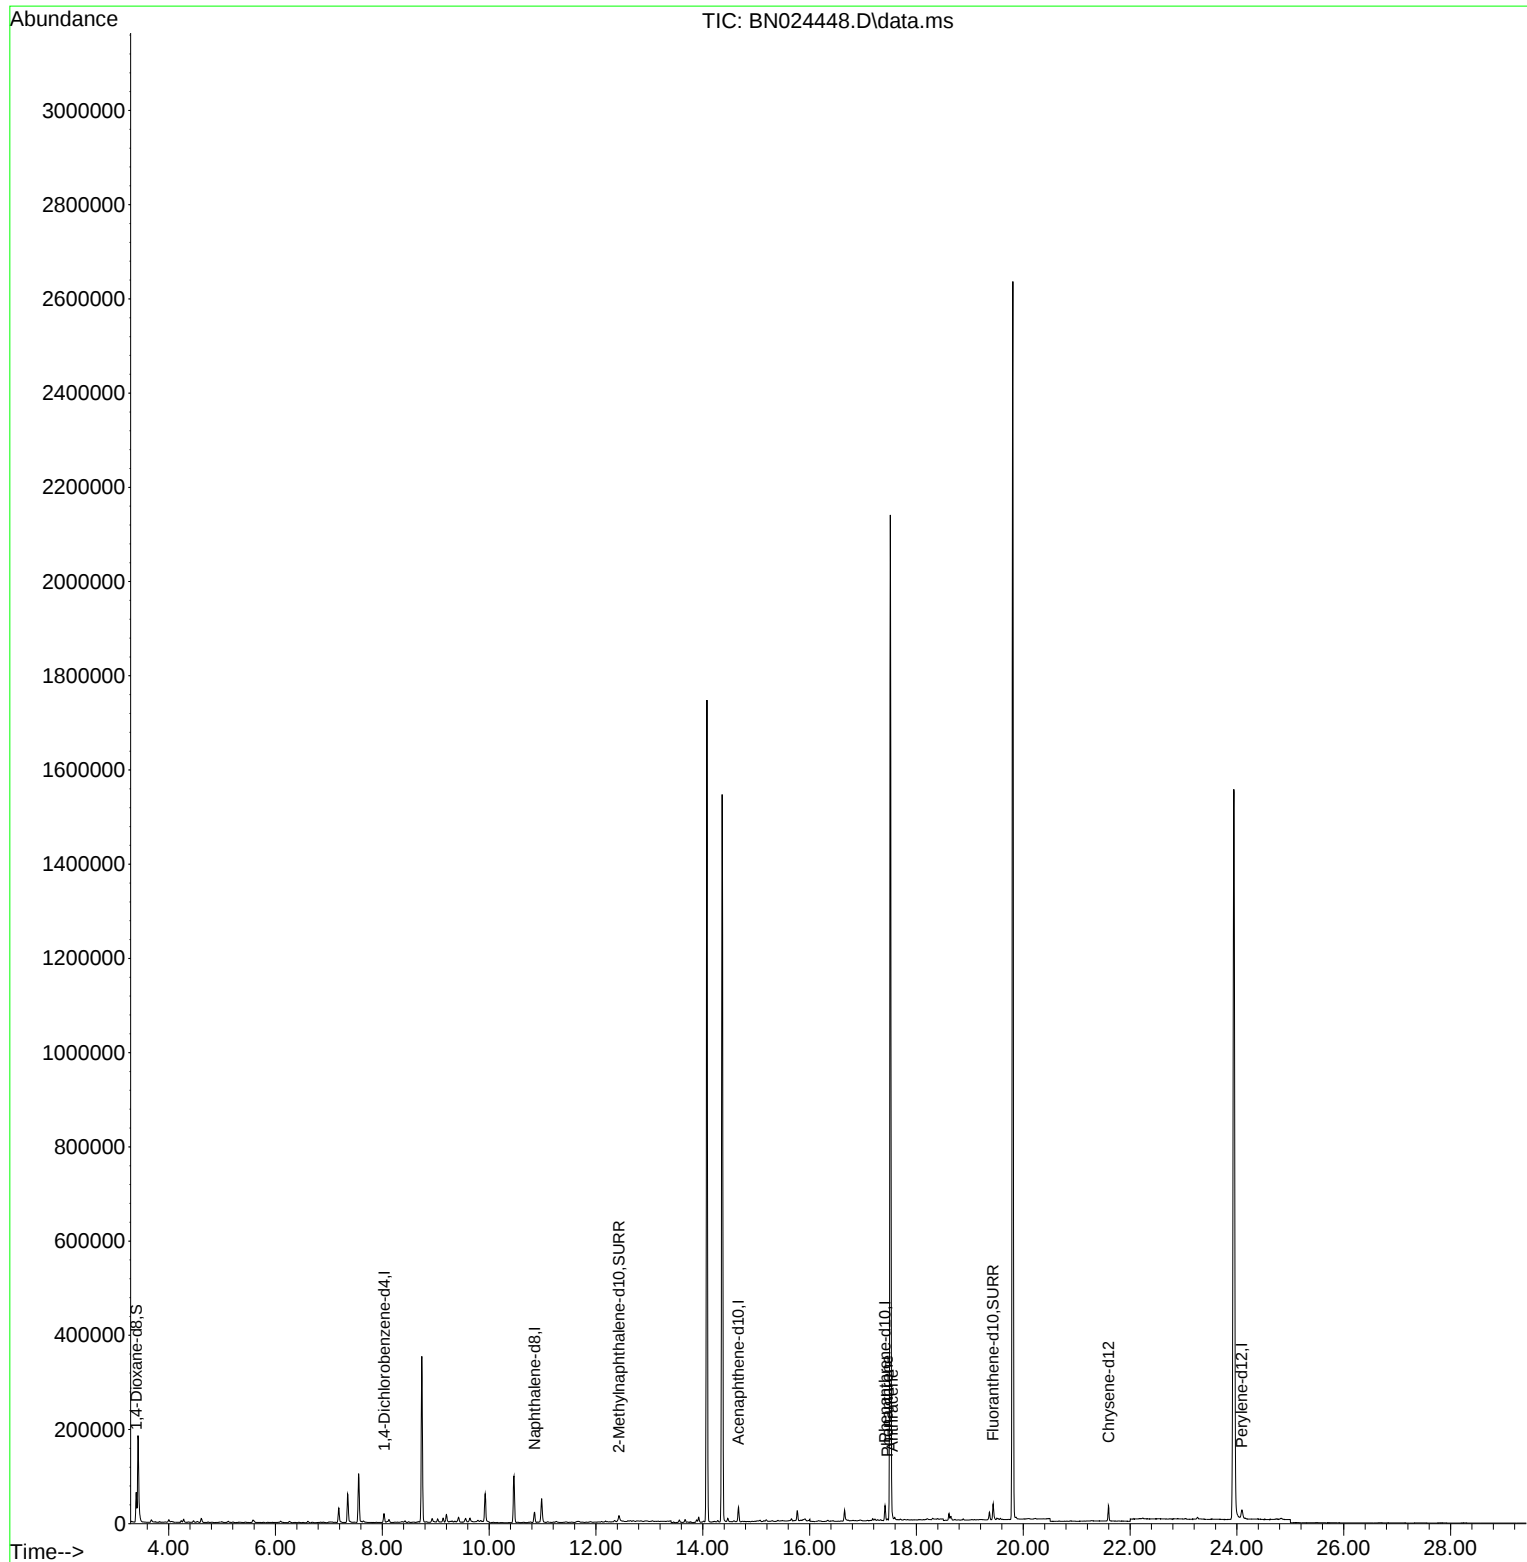


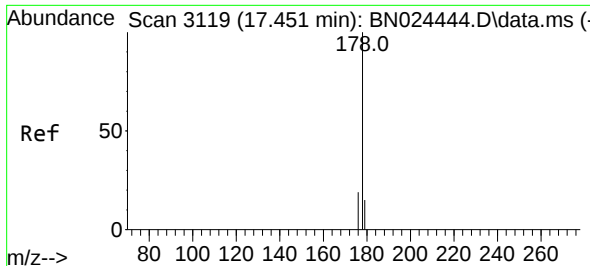

#15
Phenanthrene
Concen: 0.037 ng/u1
RT: 17.456 min Scan# 3119
Delta R.T. 0.000 min
Lab File: BN024448.D
Acq: 21 Mar 2023 14:30

Instrument :
BNA_N
ClientSampleId :
CB919

Tgt Ion:178 Resp: 3722
Ion Ratio Lower Upper
178 100
179 41.4 12.2 18.2#
176 36.7 15.7 23.5#

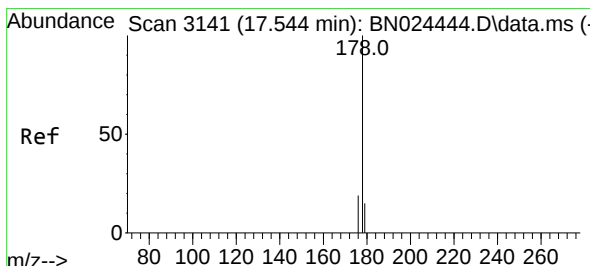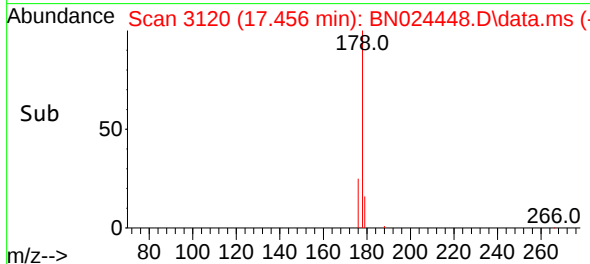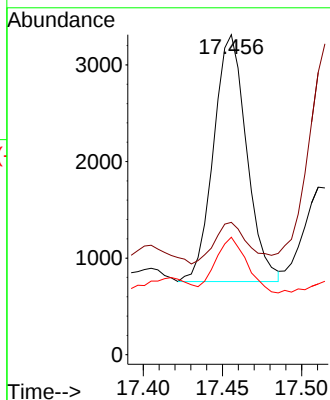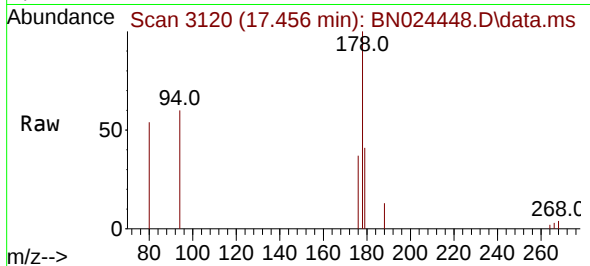

#16
Anthracene
Concen: 0.073 ng/u1
RT: 17.548 min Scan# 3142
Delta R.T. 0.000 min
Lab File: BN024448.D
Acq: 21 Mar 2023 14:30

Tgt Ion:178 Resp: 6492
Ion Ratio Lower Upper
178 100
179 36.1 12.3 18.5#
176 28.3 15.3 22.9#

