

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032023\
 Data File : BN024449.D
 Acq On : 21 Mar 2023 15:07
 Operator : CG/JU
 Sample : 01884-11
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB921

Quant Time: Mar 21 17:39:38 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 21 02:42:36 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.034	152	7720	0.400	ng/ul	0.00
4) Naphthalene-d8	10.850	136	23586	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.670	164	13633	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.413	188	28623	0.400	ng/ul	0.00
17) Chrysene-d12	21.600	240	24566	0.400	ng/ul	0.00
23) Perylene-d12	24.088	264	26133	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	35214	4.145	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.428	152	11730	0.419	ng/ul	0.00
18) Fluoranthene-d10	19.436	212	26454	0.405	ng/ul	0.00
Target Compounds						
					Qvalue	
15) Phenanthrene	17.455	178	2531	0.031	ng/ul#	83
20) Pyrene	19.831	202	4046	0.041	ng/ul#	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032023\
Data File : BN024449.D
Acq On : 21 Mar 2023 15:07
Operator : CG/JU
Sample : 01884-11
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB921

Quant Time: Mar 21 17:39:38 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 21 02:42:36 2023
Response via : Initial Calibration




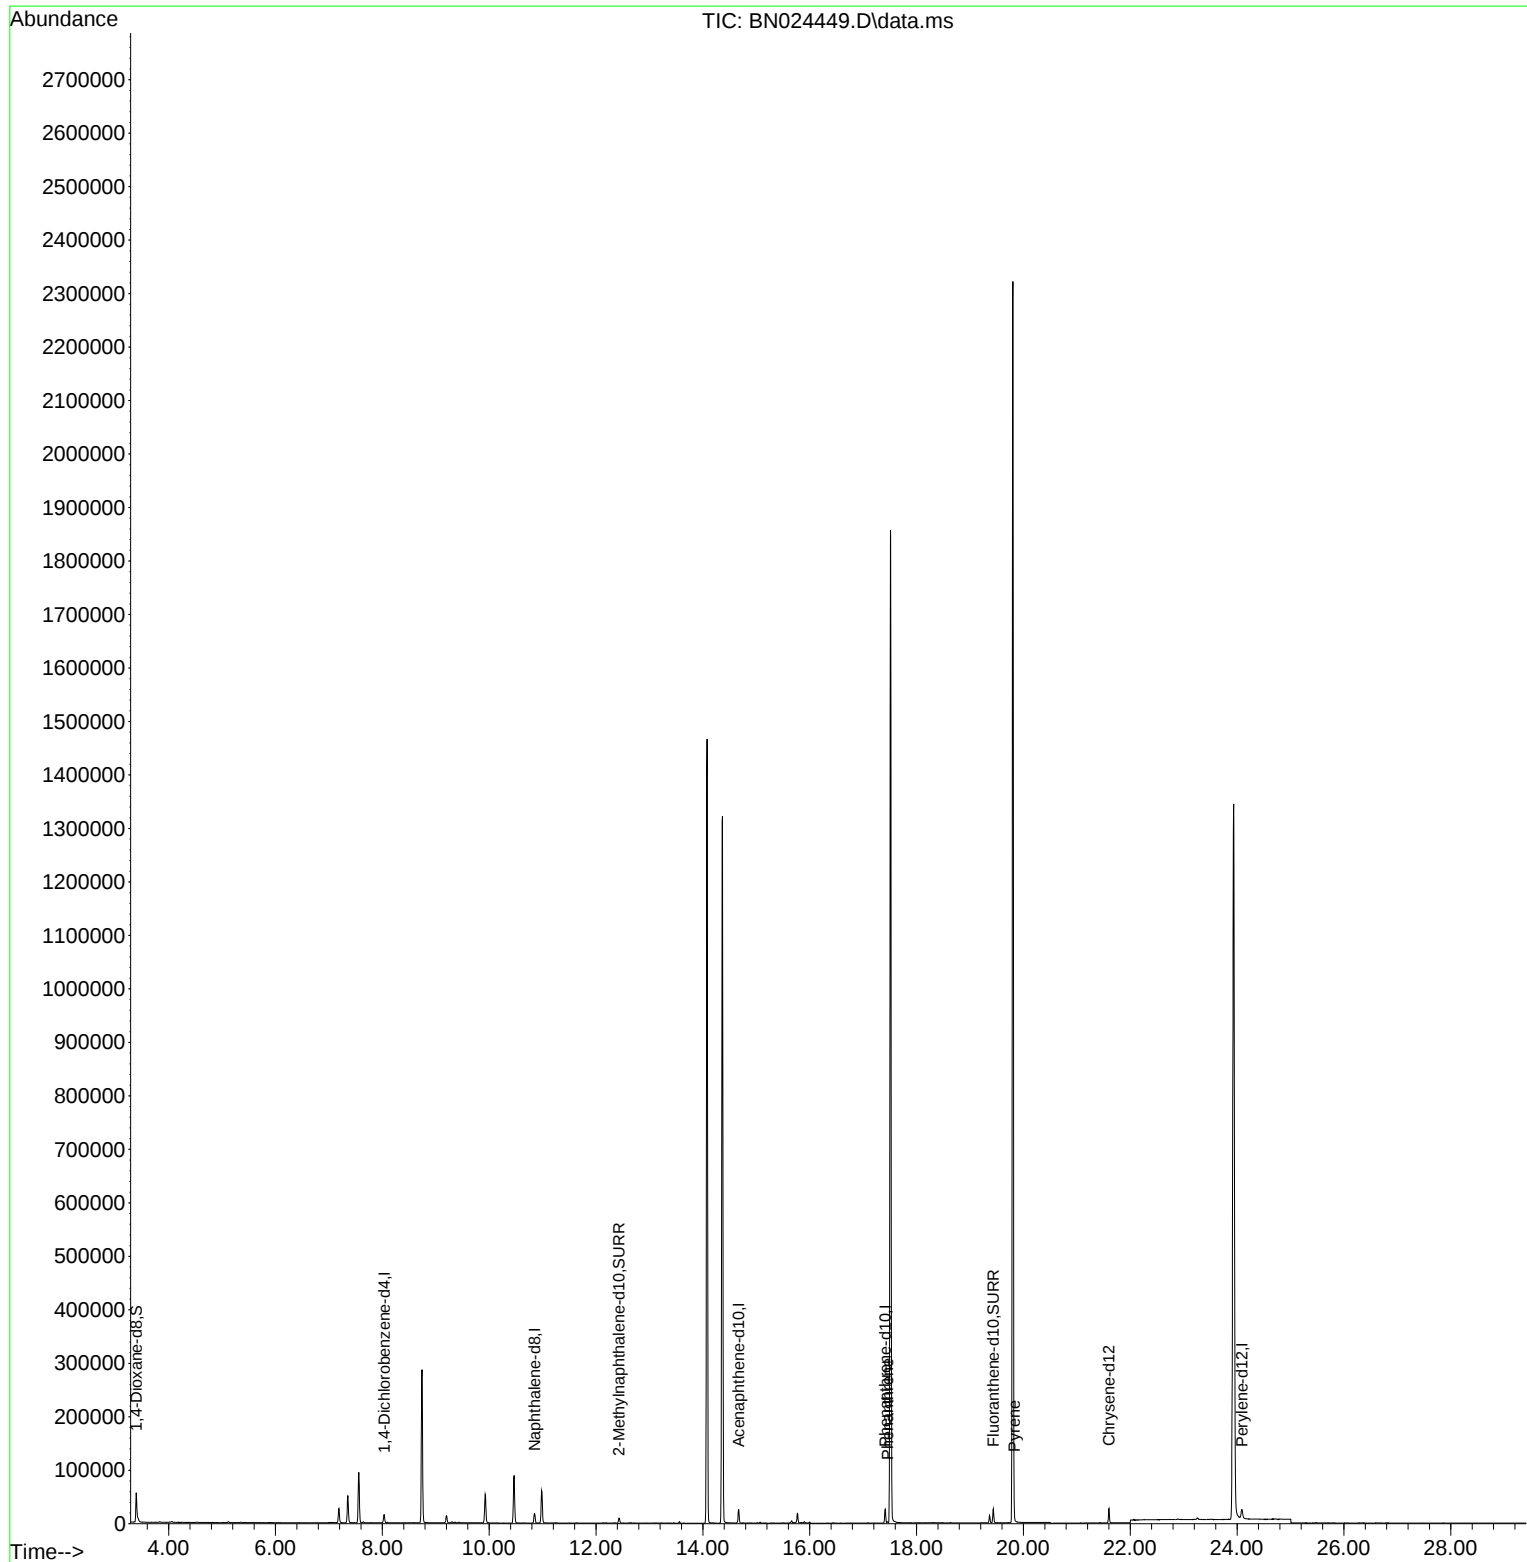


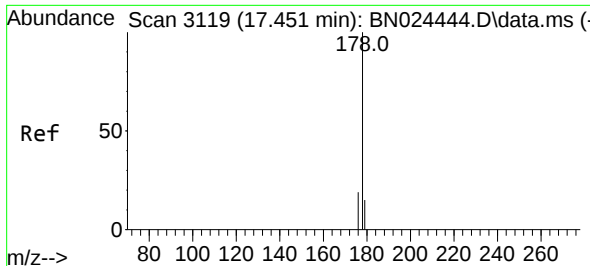

#15
Phenanthrene
Concen: 0.031 ng/ul
RT: 17.455 min Scan# 3119
Delta R.T. -0.000 min
Lab File: BN024449.D
Acq: 21 Mar 2023 15:07

Instrument :
BNA_N
ClientSampleId :
CB921

Tgt Ion:178 Resp: 2531
Ion Ratio Lower Upper
178 100
179 25.8 12.2 18.2#
176 24.5 15.7 23.5#

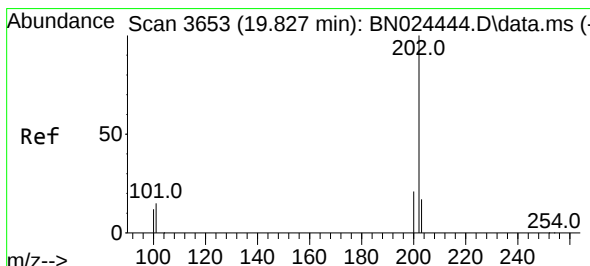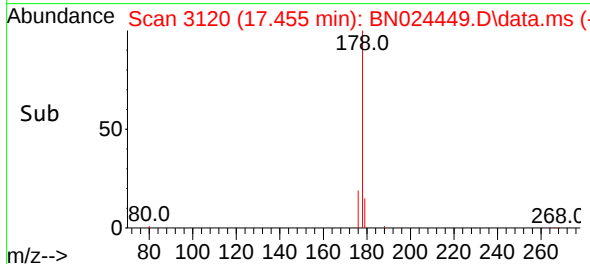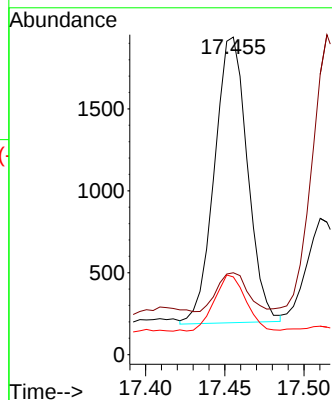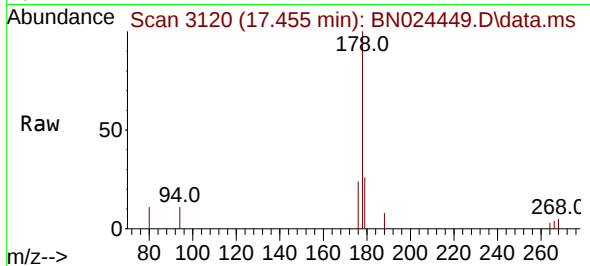

#20
Pyrene
Concen: 0.041 ng/ul
RT: 19.831 min Scan# 3654
Delta R.T. -0.000 min
Lab File: BN024449.D
Acq: 21 Mar 2023 15:07

Tgt Ion:202 Resp: 4046
Ion Ratio Lower Upper
202 100
101 19.7 12.1 18.1#
100 17.2 9.4 14.0#

