
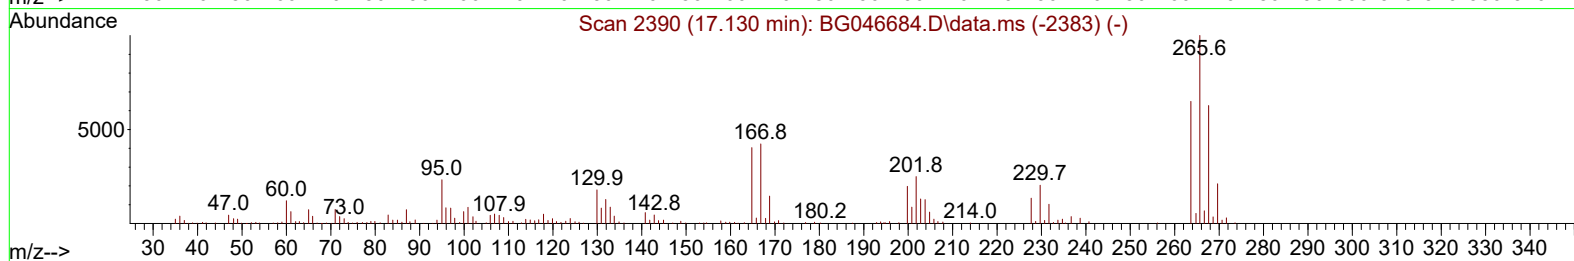
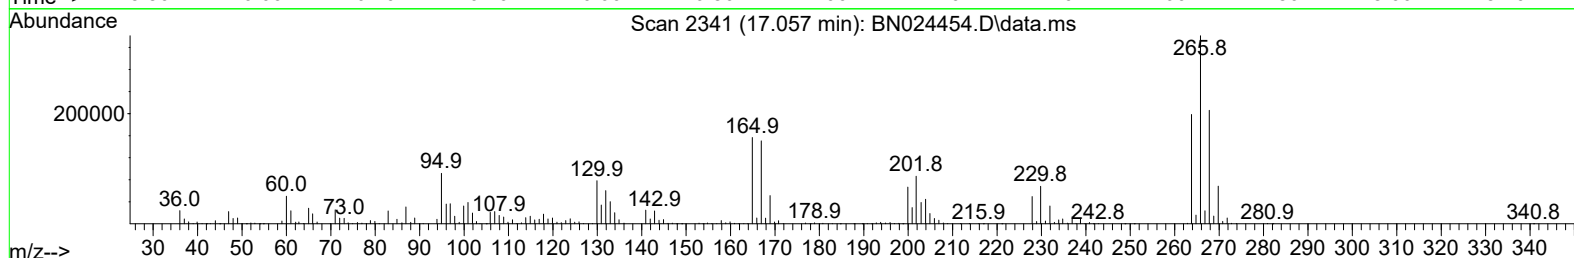


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032123\
Data File : BN024454.D
Acq On : 21 Mar 2023 19:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 22 05:58:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 22 05:58:11 2023
Response via : Initial Calibration

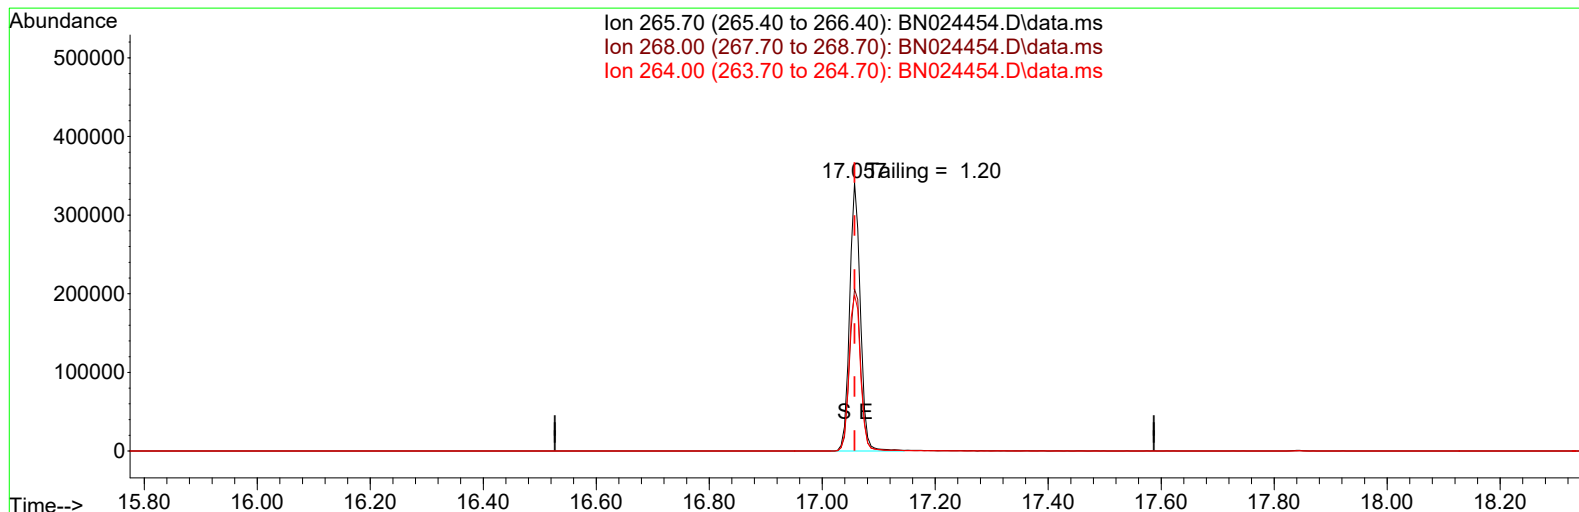

TIC: BN024454.D\data.ms

(70) Pentachlorophenol (C)




17.057min (0.000) 26371.65 ng

response 454480

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.32
264.00	61.60	58.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032123\
Data File : BN024454.D
Acq On : 21 Mar 2023 19:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 22 05:58:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 22 05:58:11 2023
Response via : Initial Calibration

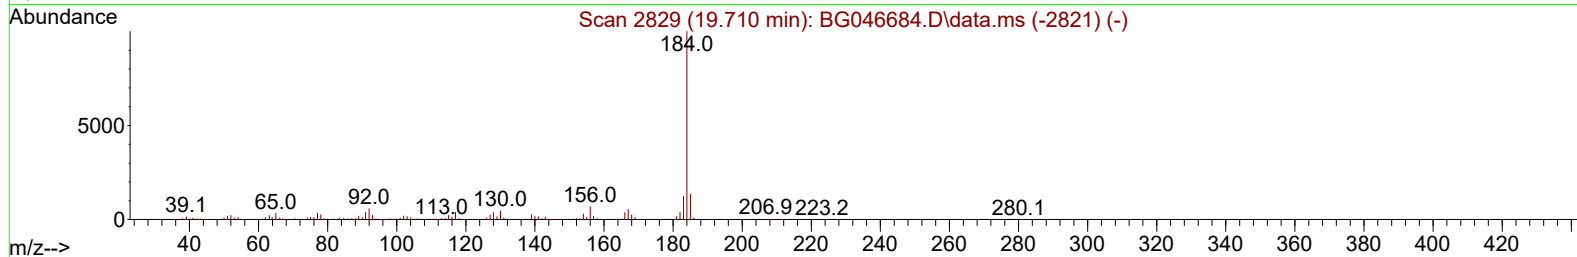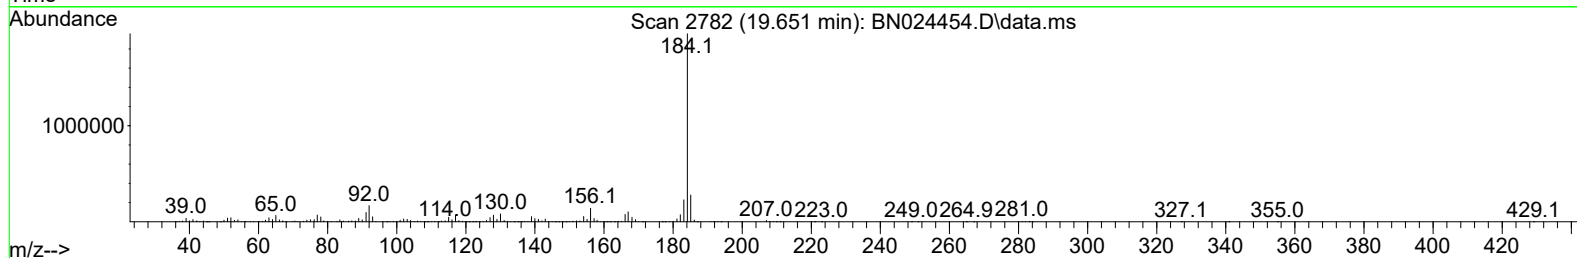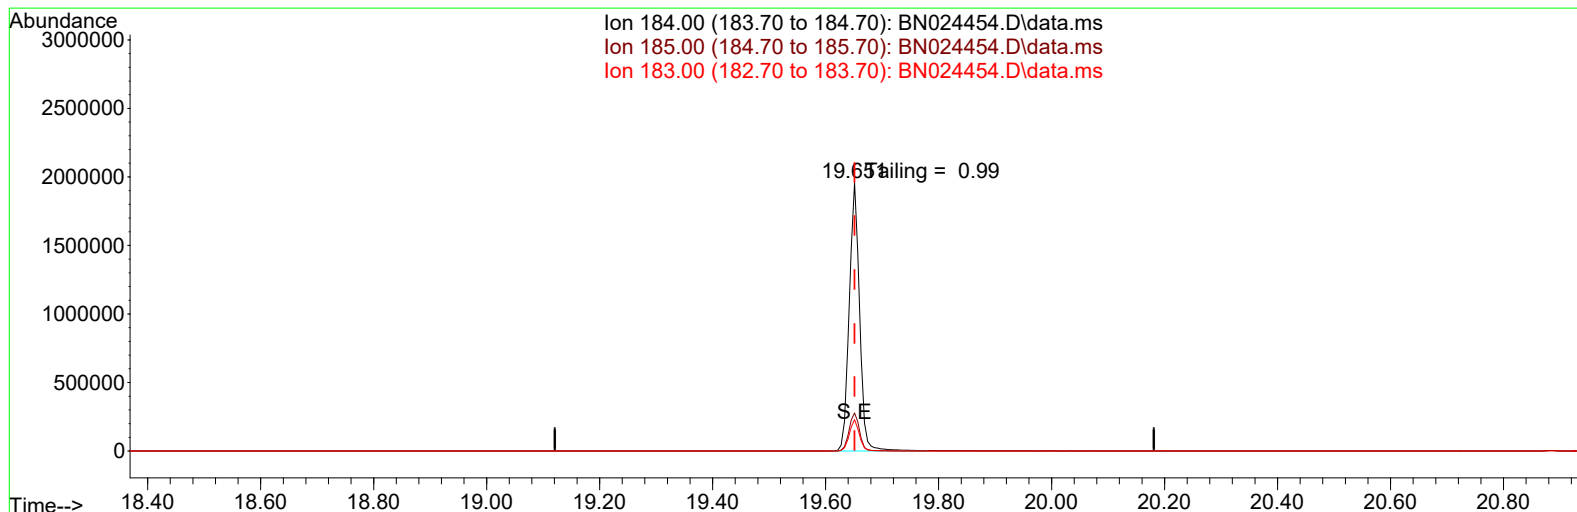

TIC: BN024454.D\data.ms

(77) Benzidine

19.651min (0.000) 0.00 ng

response 2511950

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.23
183.00	13.20	11.71
0.00	0.00	0.00