
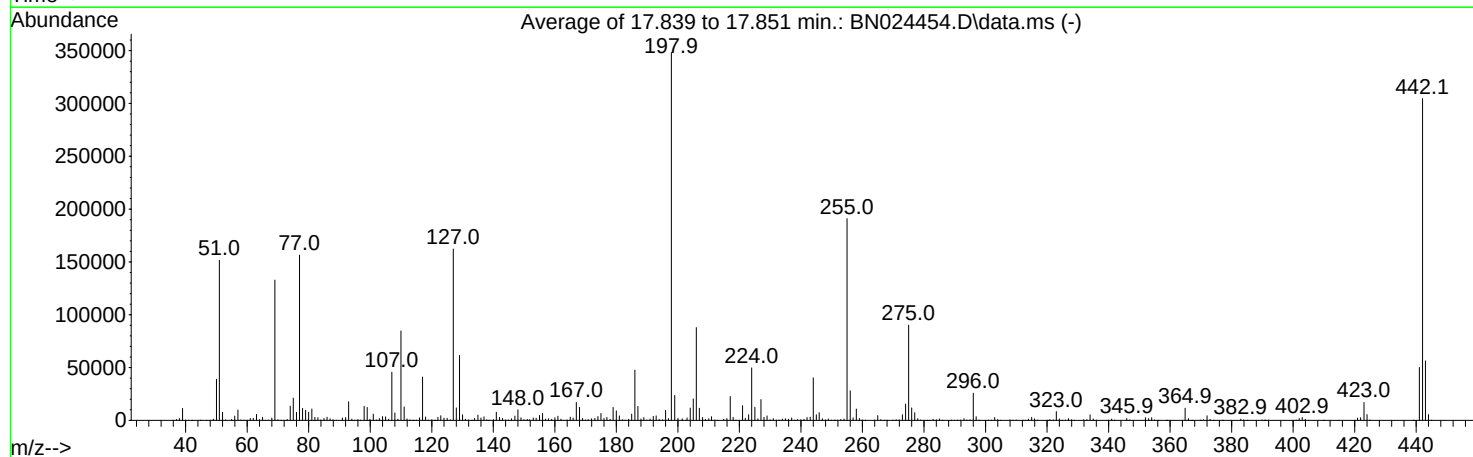


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032123\
 Data File : BN024454.D
 Acq On : 21 Mar 2023 19:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN031323.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 22 04:14:21 2023

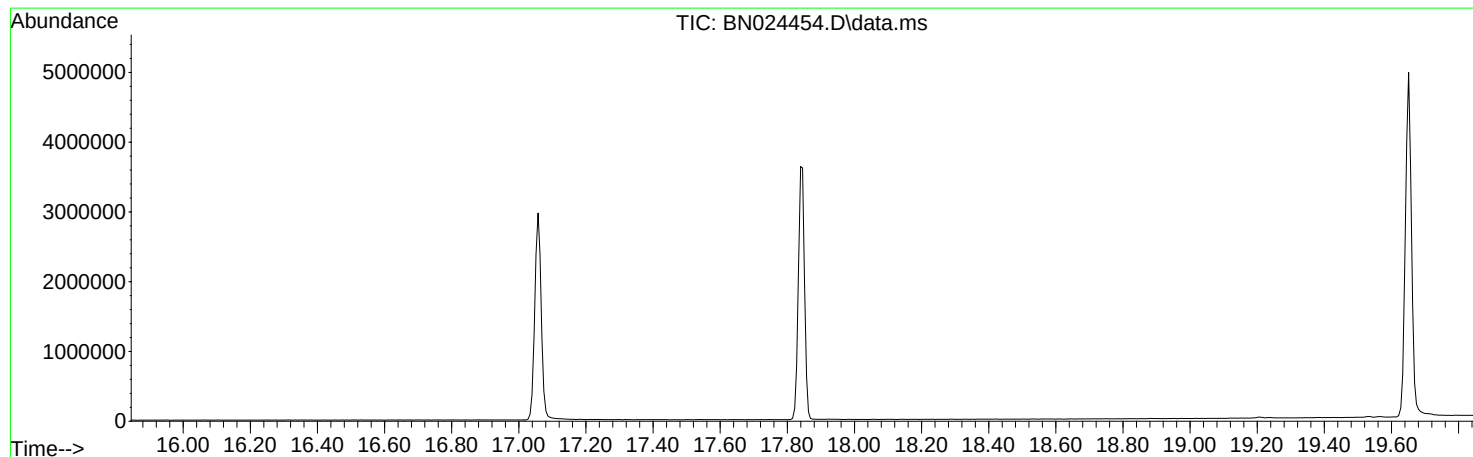




AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.5	151606	PASS
68	69	0.00	2	1.7	2228	PASS
69	198	0.00	100	38.2	132851	PASS
70	69	0.00	2	0.5	644	PASS
127	198	10	80	46.6	162275	PASS
197	198	0.00	2	0.5	1749	PASS
198	198	100	100	100.0	348224	PASS
199	198	5	9	6.8	23649	PASS
275	198	10	60	25.9	90096	PASS
365	198	1	100	3.3	11529	PASS
441	198	0.01	100	14.4	50208	PASS
442	442	50	100	100.0	304597	PASS
443	442	15	24	18.5	56421	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032123\
Data File : BN024454.D
Acq On : 21 Mar 2023 19:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 22 05:58:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 22 05:58:11 2023
Response via : Initial Calibration

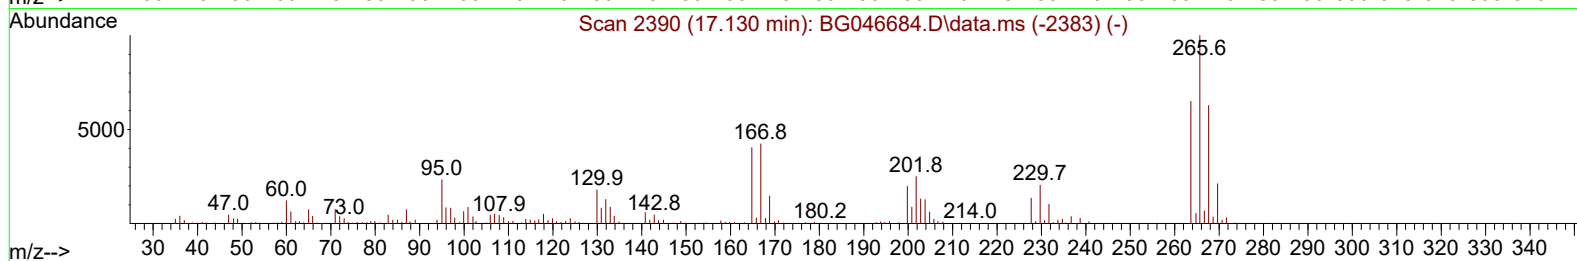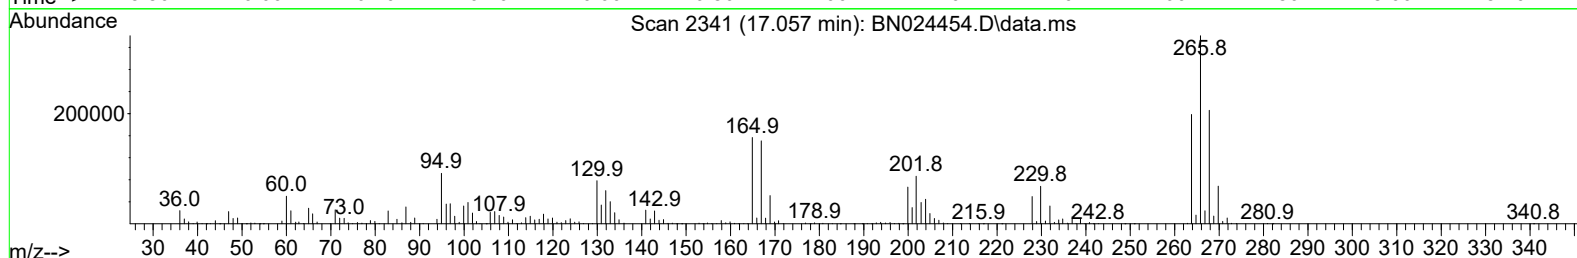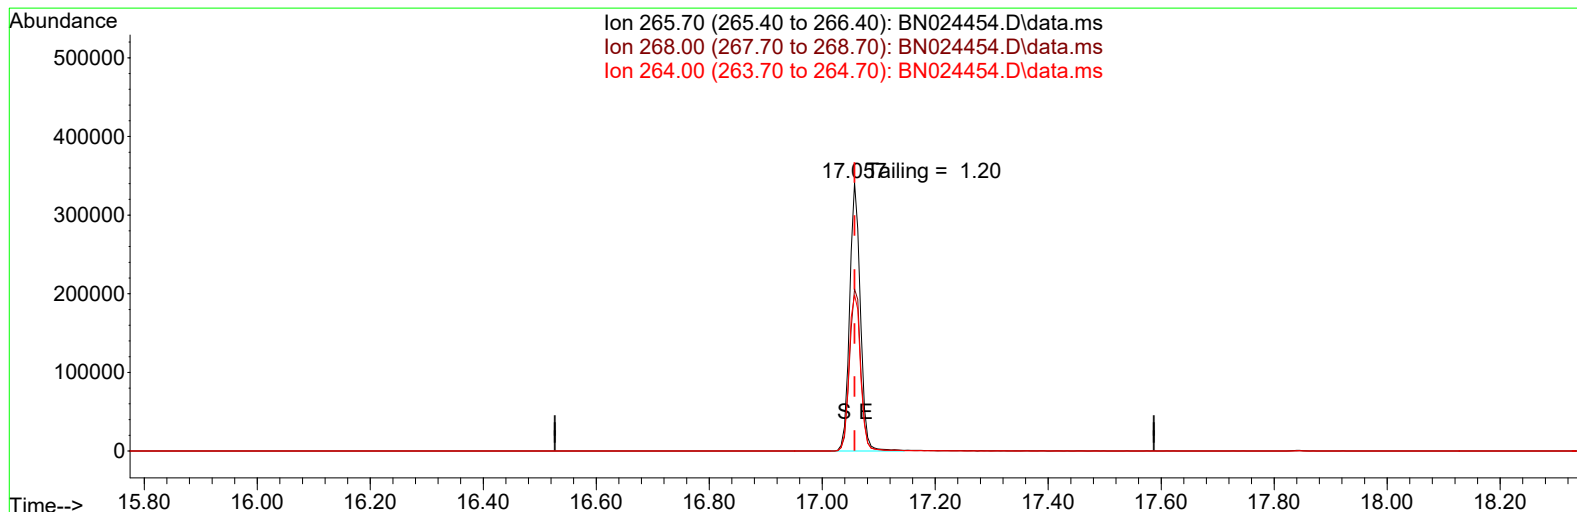

TIC: BN024454.D\data.ms

(70) Pentachlorophenol (C)

17.057min (0.000) 26371.65 ng




response 454480

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.32
264.00	61.60	58.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032123\
Data File : BN024454.D
Acq On : 21 Mar 2023 19:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 22 05:58:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 22 05:58:11 2023
Response via : Initial Calibration

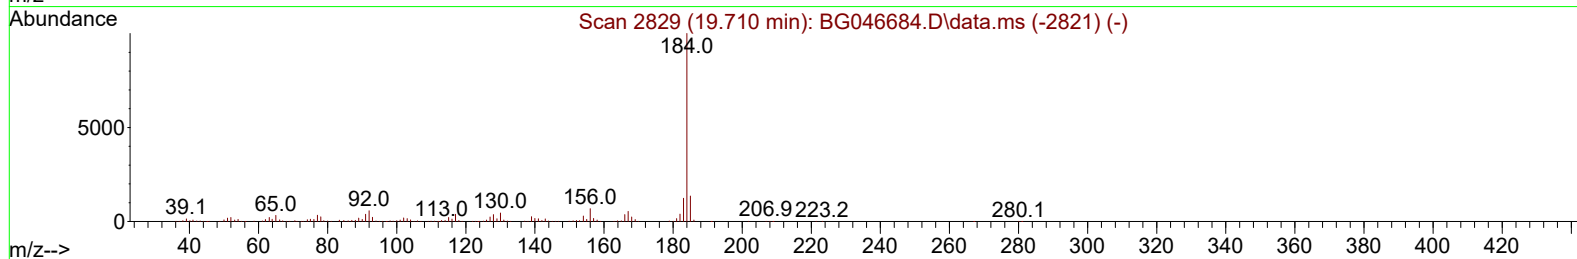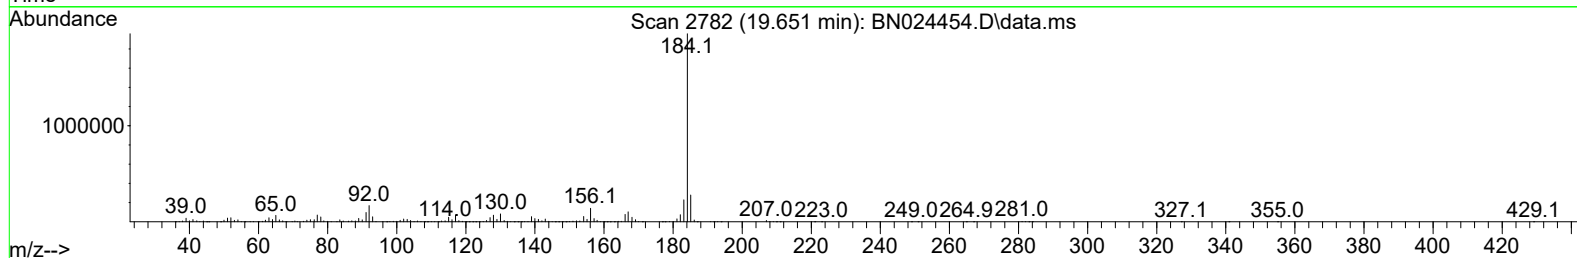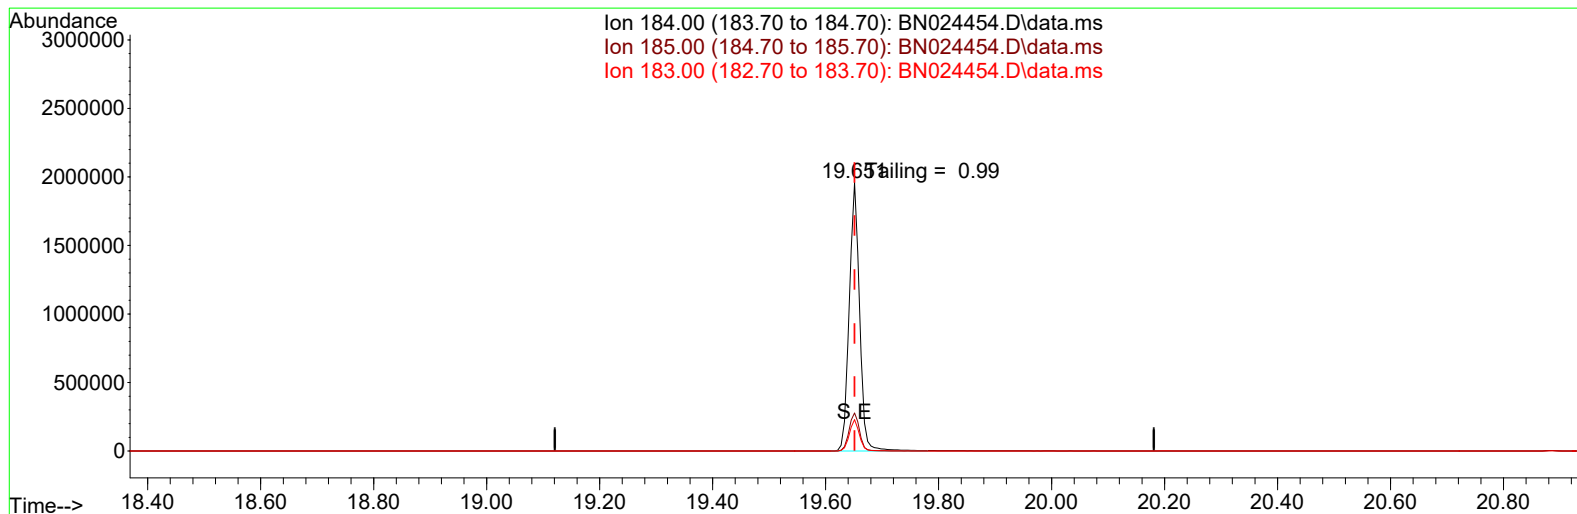

TIC: BN024454.D\data.ms

(77) Benzidine

19.651min (0.000) 0.00 ng

response 2511950

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.23
183.00	13.20	11.71
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/21/2023	BNA_N	<u>BN024454.D</u>
Compound Name	Response	Retention Time
DDT	1192418	20.886
DDD	85240	20.439
DDE	4744	19.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
89984	1282402	7.02

Instrument :
BNA_N
ClientSampleId :
DFTPP