

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032421\
 Data File : BN014079.D
 Acq On : 24 Mar 2021 20:23
 Operator : CG/JU
 Sample : M1787-10
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 RE-125D3-20210319

Quant Time: Mar 25 05:38:13 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN032021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 23 11:06:27 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.700	152	5104	0.40	ng	0.00
7) Naphthalene-d8	10.467	136	19781	0.40	ng	#-0.01
13) Acenaphthene-d10	14.321	164	11413	0.40	ng	0.00
19) Phenanthrene-d10	17.055	188	25006	0.40	ng	-0.01
29) Chrysene-d12	21.239	240	23500	0.40	ng	# 0.00
36) Perylene-d12	23.441	264	19082	0.40	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.292	112	1803	0.15	ng	0.00
5) Phenol-d6	6.863	99	1291	0.09	ng	0.00
8) Nitrobenzene-d5	8.832	82	4497	0.34	ng	-0.01
11) 2-Methylnaphthalene-d10	12.062	152	11330	0.37	ng	0.00
14) 2,4,6-Tribromophenol	15.818	330	1229	0.33	ng	0.00
15) 2-Fluorobiphenyl	12.938	172	15224	0.36	ng	-0.01
27) Fluoranthene-d10	19.089	212	28452	0.41	ng	0.00
31) Terphenyl-d14	19.690	244	27490	0.53	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.239	88	13859	2.06	ng	# 93
34) Bis(2-ethylhexyl)phtha...	21.154	149	1431	0.06	ng	# 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032421\
Data File : BN014079.D
Acq On : 24 Mar 2021 20:23
Operator : CG/JU
Sample : M1787-10
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
RE-125D3-20210319

Quant Time: Mar 25 05:38:13 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN032021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 23 11:06:27 2021
Response via : Initial Calibration




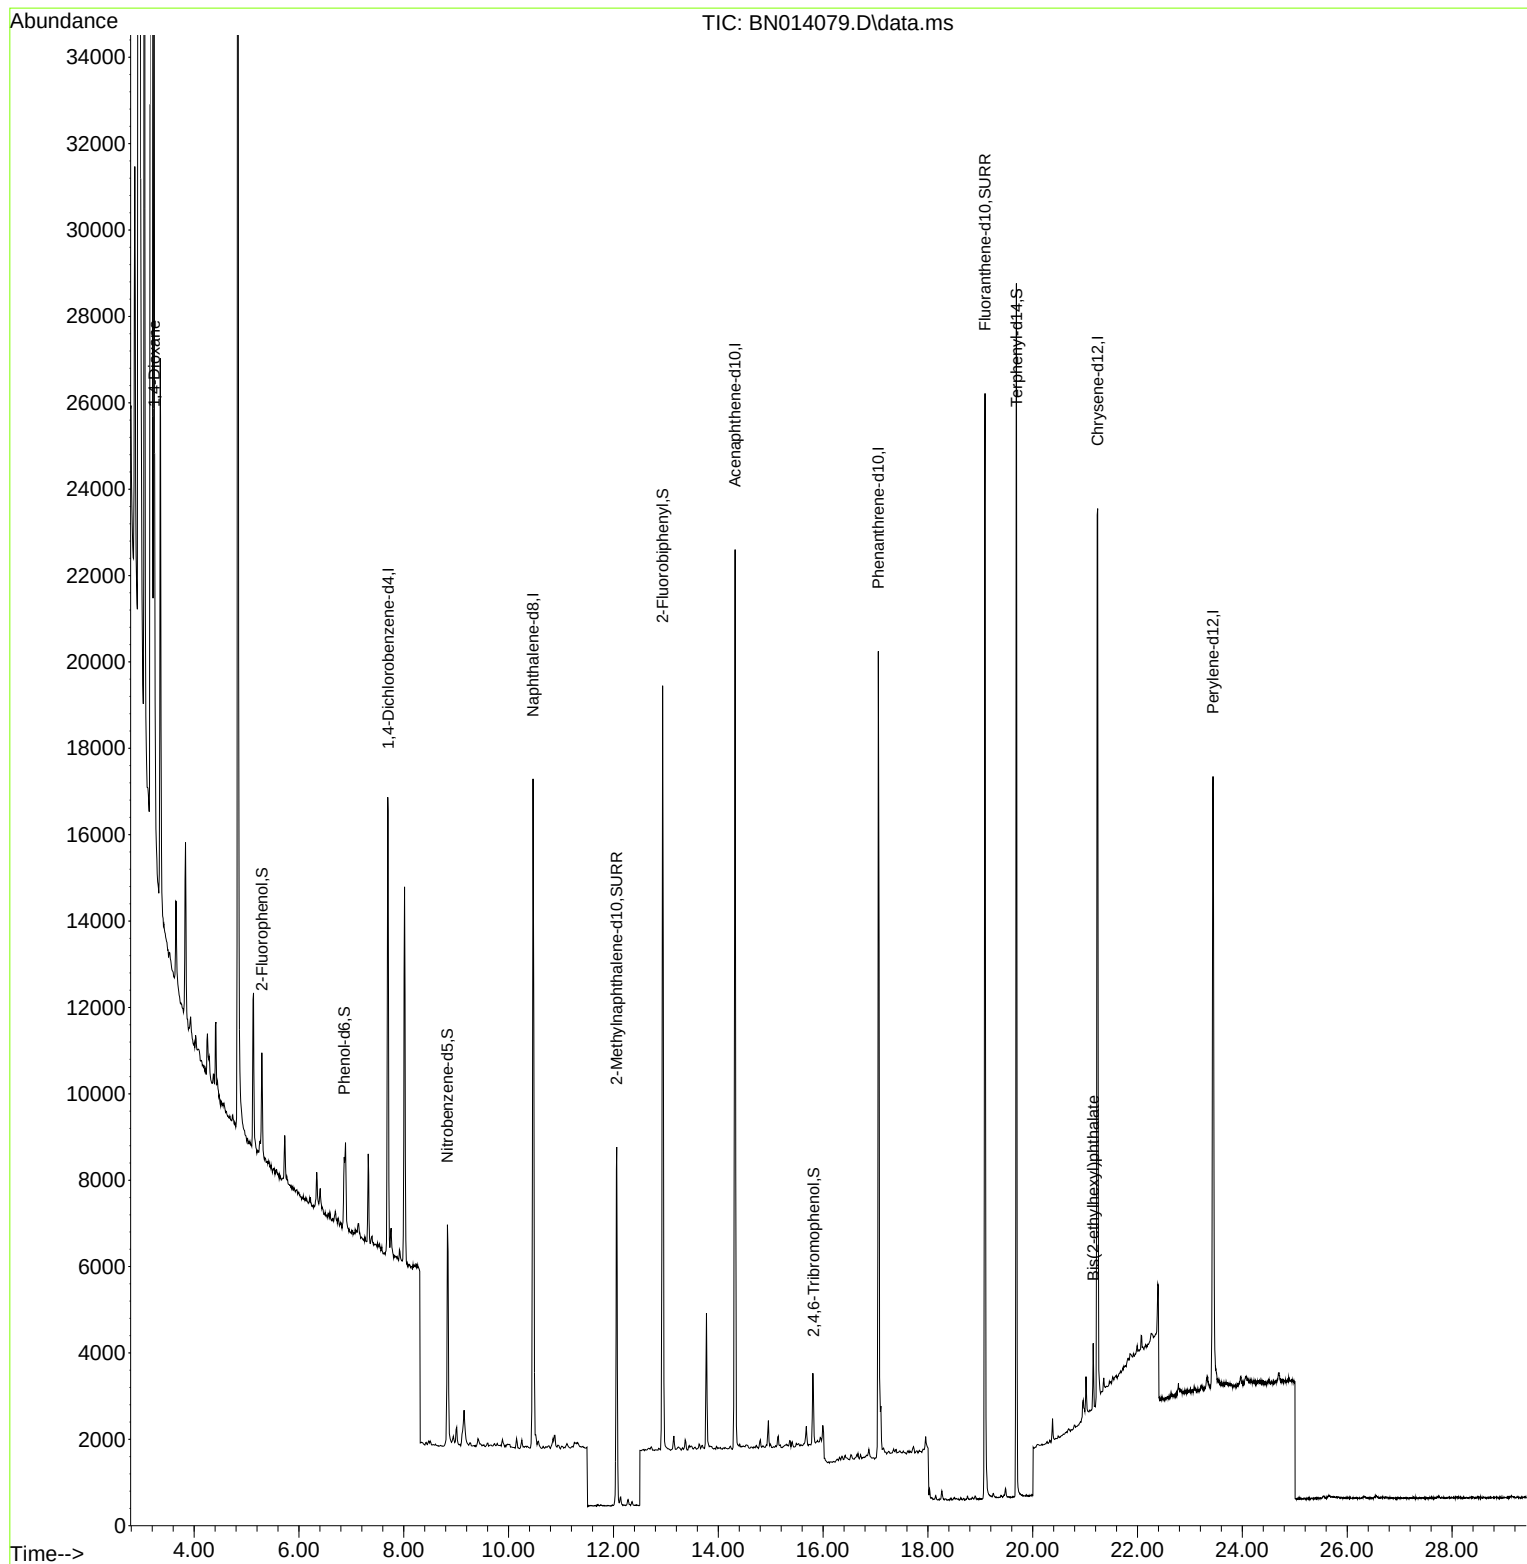


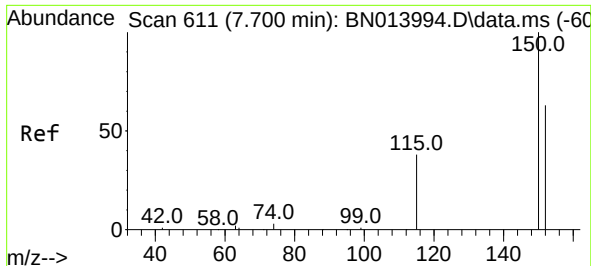

#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.700 min Scan# 611
 Delta R.T. 0.000 min
 Lab File: BN014079.D
 Acq: 24 Mar 2021 20:23




Instrument :
 BNA_N
 ClientSampleId :
 RE-125D3-20210319


Tgt Ion:152 Resp: 5104
 Ion Ratio Lower Upper
 152 100
 150 154.1 121.8 182.8
 115 58.1 46.6 69.8

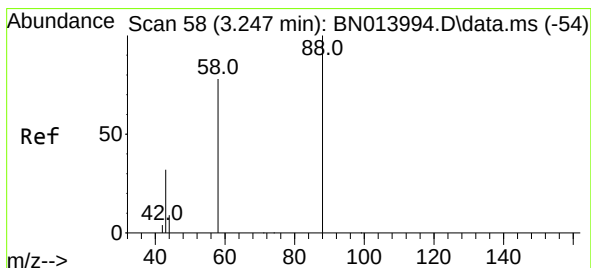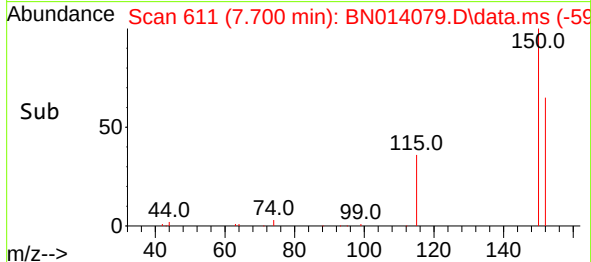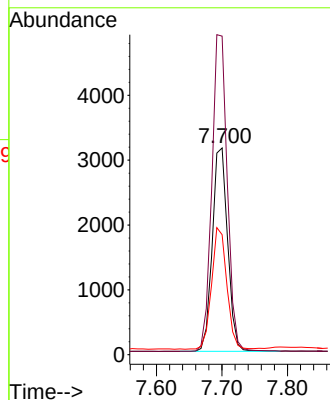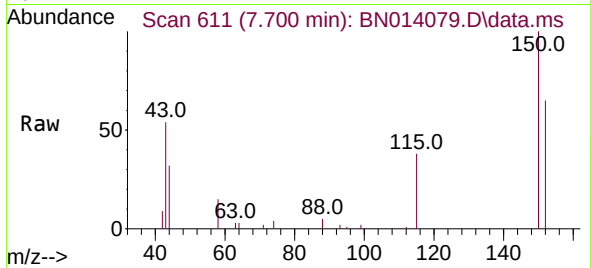

#2
 1,4-Dioxane
 Concen: 2.06 ng
 RT: 3.239 min Scan# 57
 Delta R.T. -0.008 min
 Lab File: BN014079.D
 Acq: 24 Mar 2021 20:23

Tgt Ion: 88 Resp: 13859
 Ion Ratio Lower Upper
 88 100
 58 81.2 64.6 96.8
 43 46.4 26.6 40.0#


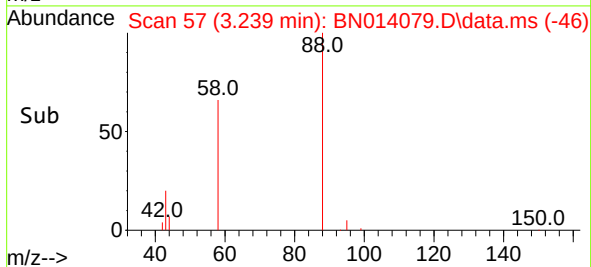
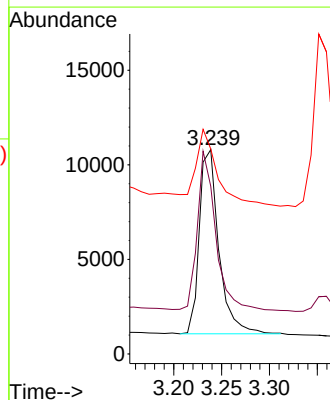
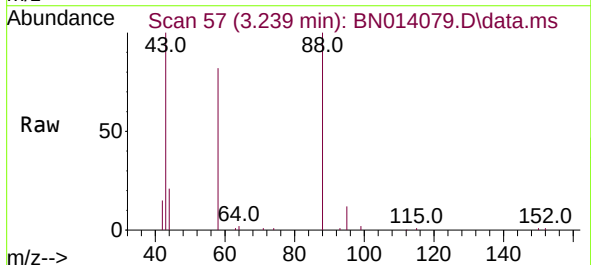


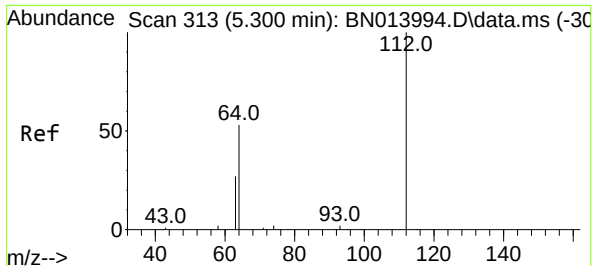

#4
2-Fluorophenol
Concen: 0.15 ng
RT: 5.292 min Scan# 312
Delta R.T. 0.000 min
Lab File: BN014079.D
Acq: 24 Mar 2021 20:23




Instrument :
BNA_N
ClientSampleId :
RE-125D3-20210319


Tgt Ion:112 Resp: 1803
Ion Ratio Lower Upper
112 100
64 59.3 44.3 66.5
63 32.0 23.0 34.6

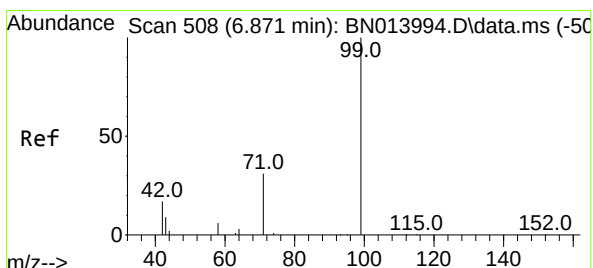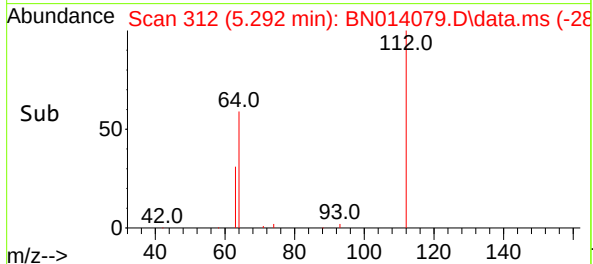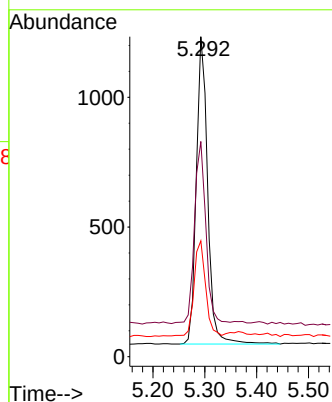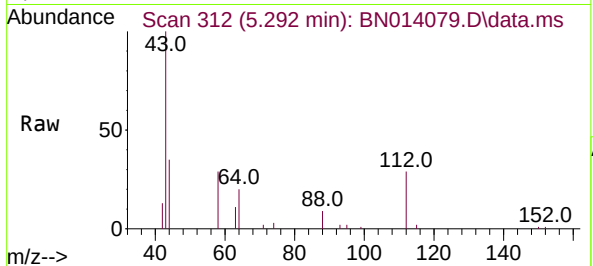

#5
Phenol-d6
Concen: 0.09 ng
RT: 6.863 min Scan# 507
Delta R.T. 0.000 min
Lab File: BN014079.D
Acq: 24 Mar 2021 20:23

Tgt Ion: 99 Resp: 1291
Ion Ratio Lower Upper
99 100
42 41.5 15.2 22.8#
71 38.3 26.1 39.1


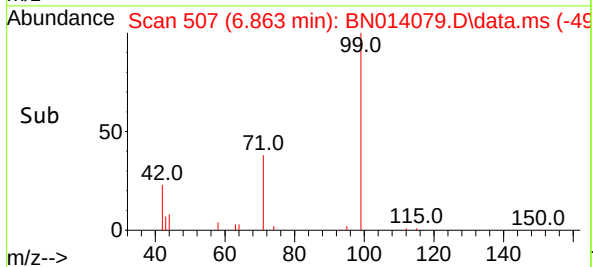
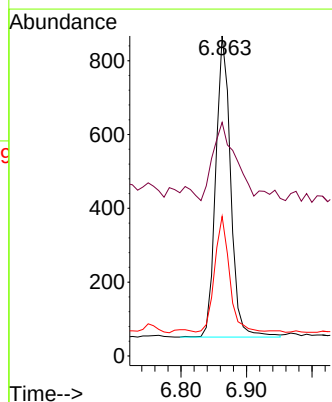
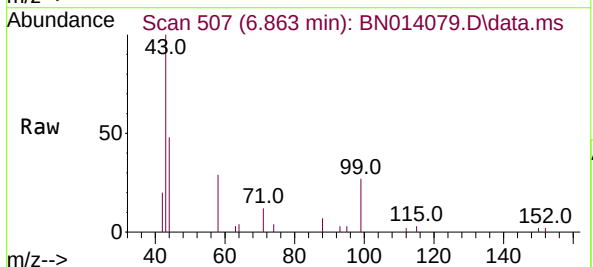


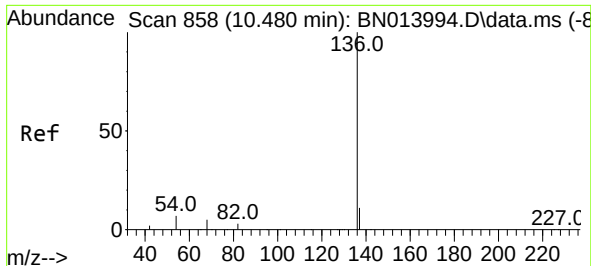

#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.467 min Scan# 857
Delta R.T. -0.012 min
Lab File: BN014079.D
Acq: 24 Mar 2021 20:23




Instrument :
BNA_N
ClientSampleId :
RE-125D3-20210319


Tgt Ion:	136	Resp:	19781
Ion Ratio	Lower	Upper	
136	100		
137	11.2	9.0	13.6
54	9.3	6.4	9.6
68	6.8	4.5	6.7

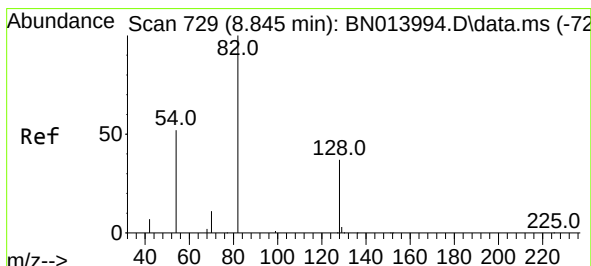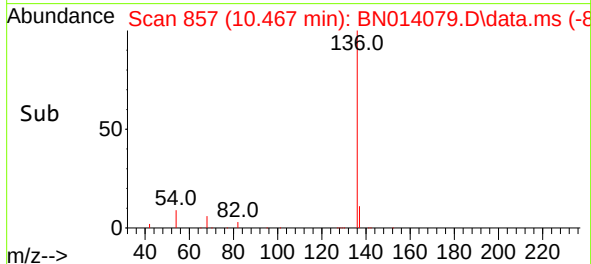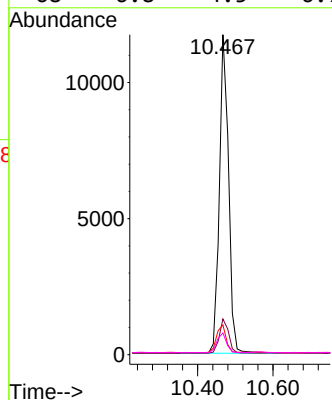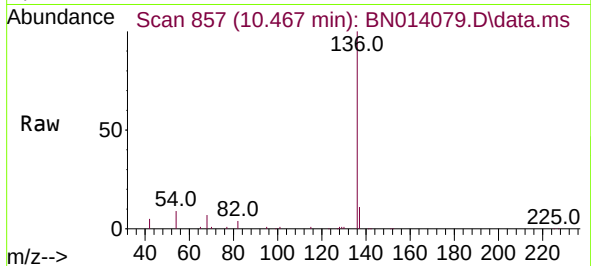

#8
Nitrobenzene-d5
Concen: 0.34 ng
RT: 8.832 min Scan# 728
Delta R.T. -0.012 min
Lab File: BN014079.D
Acq: 24 Mar 2021 20:23

Tgt Ion:	82	Resp:	4497
Ion Ratio	Lower	Upper	
82	100		
128	32.3	39.2	58.8
54	60.0	40.1	60.1


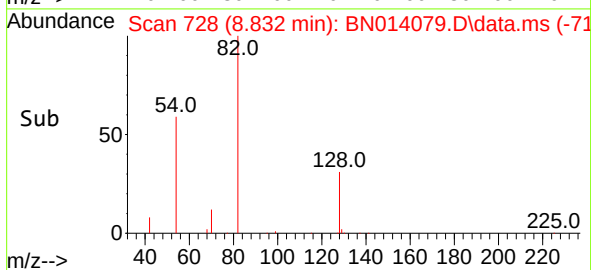
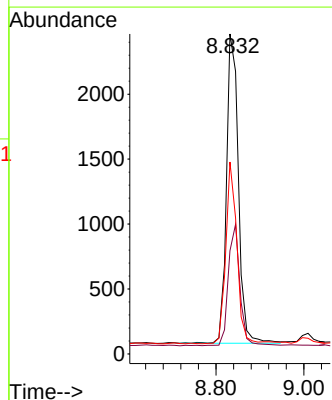
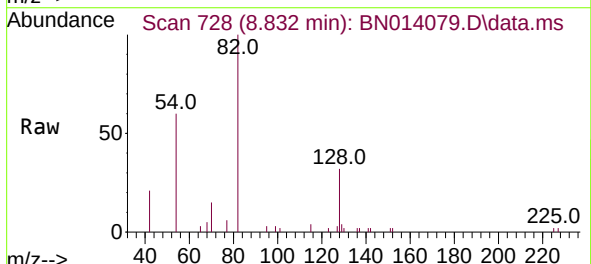


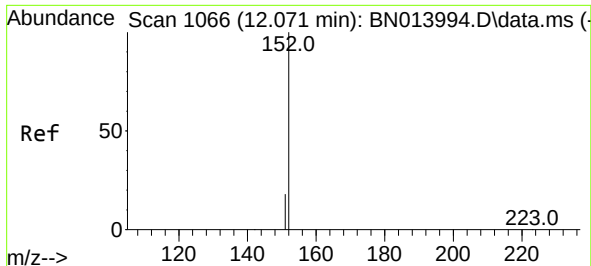

#11
2-Methylnaphthalene-d10
Concen: 0.37 ng
RT: 12.062 min Scan# 1064
Delta R.T. -0.004 min
Lab File: BN014079.D
Acq: 24 Mar 2021 20:23




Instrument :
BNA_N
ClientSampleId :
RE-125D3-20210319


Tgt Ion:152 Resp: 11330
Ion Ratio Lower Upper
152 100
151 19.8 16.2 24.2

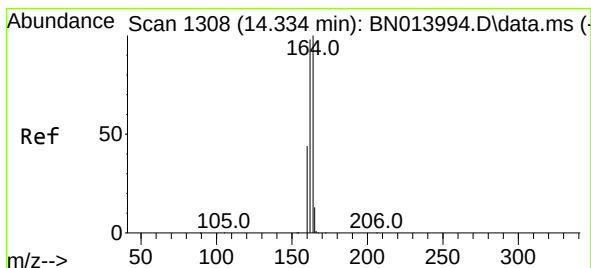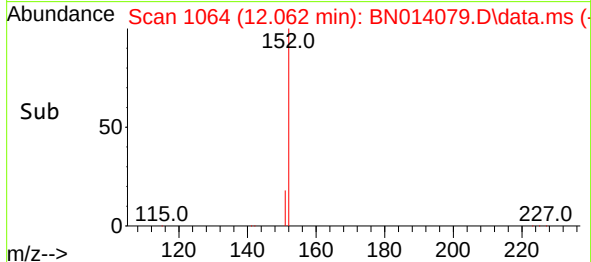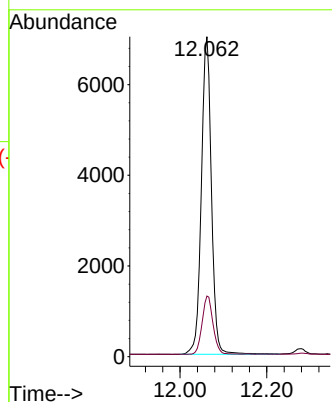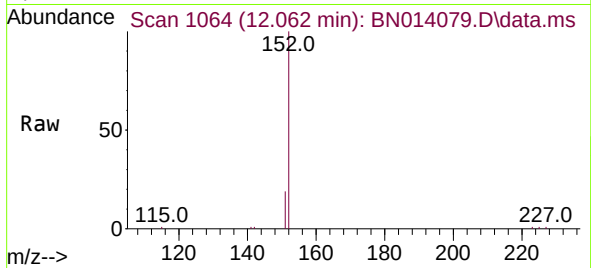

#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.321 min Scan# 1307
Delta R.T. 0.000 min
Lab File: BN014079.D
Acq: 24 Mar 2021 20:23

Tgt Ion:164 Resp: 11413
Ion Ratio Lower Upper
164 100
162 99.8 79.6 119.4
160 45.0 36.0 54.0


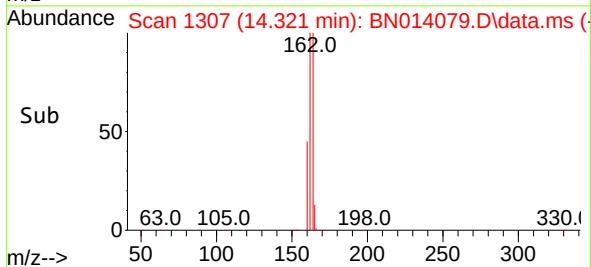
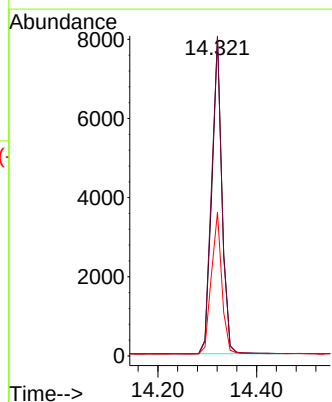
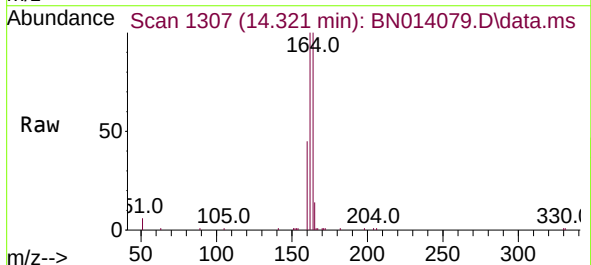


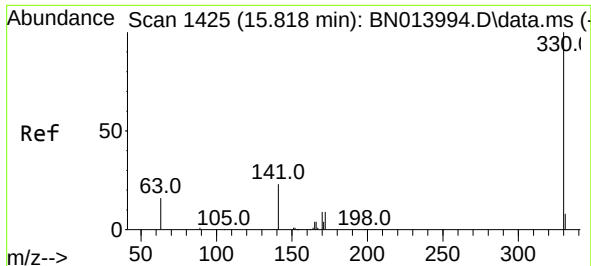

#14
2,4,6-Tribromophenol
Concen: 0.33 ng
RT: 15.818 min Scan# 1425
Delta R.T. 0.000 min
Lab File: BN014079.D
Acq: 24 Mar 2021 20:23




Instrument :
BNA_N
ClientSampleId :
RE-125D3-20210319


Tgt Ion:330 Resp: 1229
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 38.2 26.8 40.2

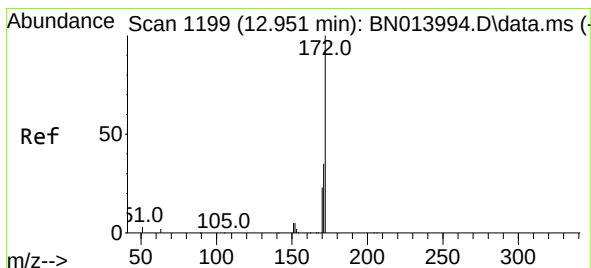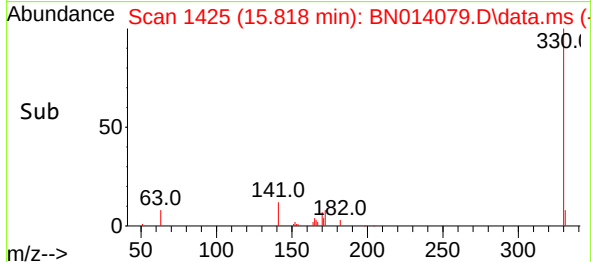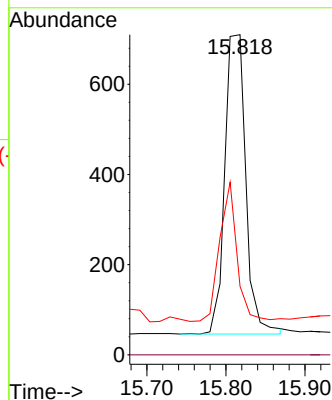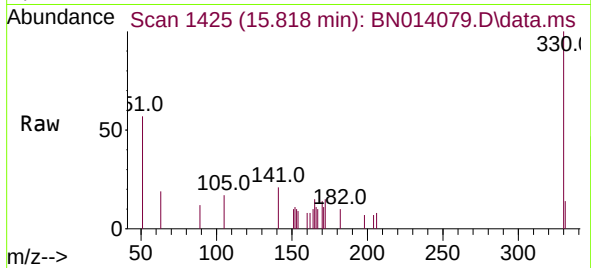

#15
2-Fluorobiphenyl
Concen: 0.36 ng
RT: 12.938 min Scan# 1198
Delta R.T. -0.012 min
Lab File: BN014079.D
Acq: 24 Mar 2021 20:23

Tgt Ion:172 Resp: 15224
Ion Ratio Lower Upper
172 100
171 35.4 28.6 42.8
170 24.5 18.9 28.3


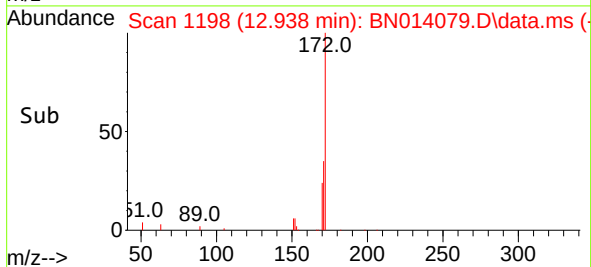
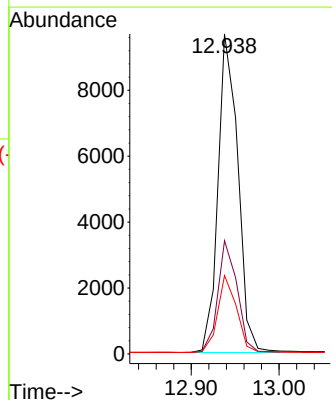
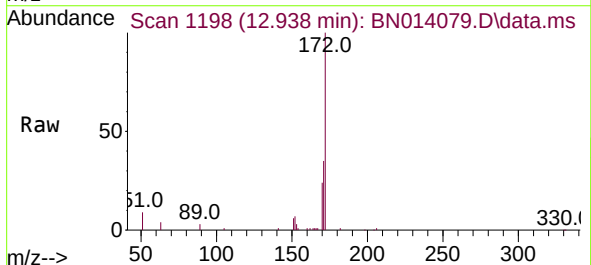


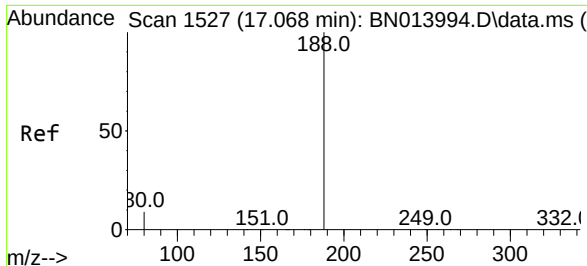

#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.055 min Scan# 1526
Delta R.T. -0.012 min
Lab File: BN014079.D
Acq: 24 Mar 2021 20:23




Instrument :
BNA_N
ClientSampleId :
RE-125D3-20210319


Tgt Ion:188	Resp:	25006
Ion Ratio	Lower	Upper
188	100	
94	0.0	0.0
80	11.4	9.0

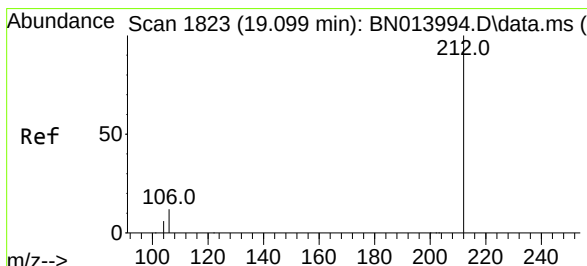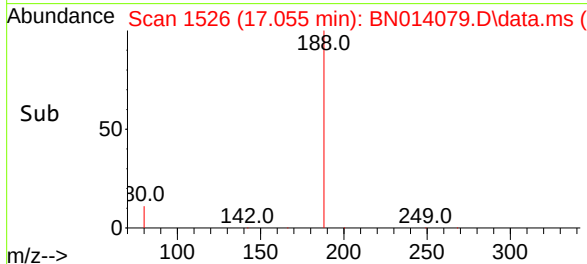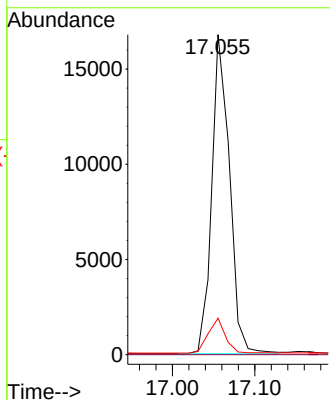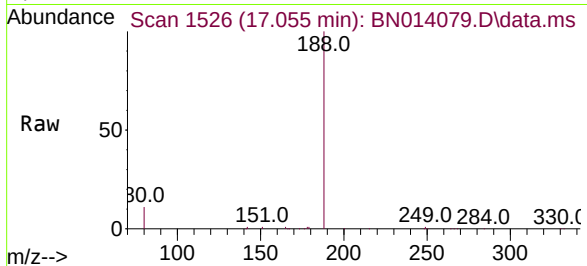

#27
Fluoranthene-d10
Concen: 0.41 ng
RT: 19.089 min Scan# 1821
Delta R.T. 0.000 min
Lab File: BN014079.D
Acq: 24 Mar 2021 20:23

Tgt Ion:212	Resp:	28452
Ion Ratio	Lower	Upper
212	100	
106	12.7	9.7
104	7.3	5.5


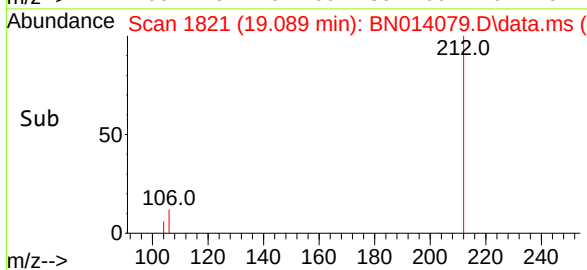
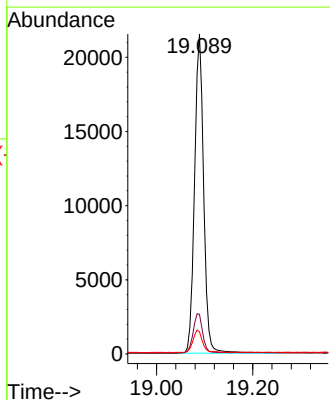
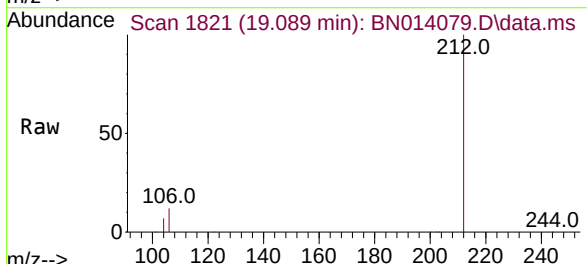


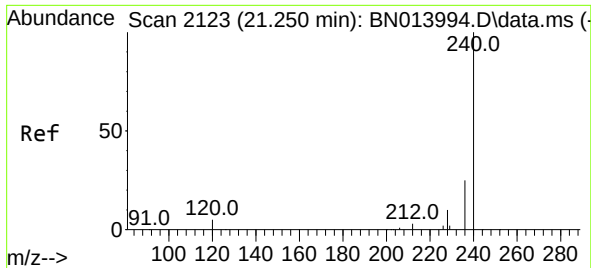

#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.239 min Scan# 2122
Delta R.T. 0.000 min
Lab File: BN014079.D
Acq: 24 Mar 2021 20:23




Instrument :
BNA_N
ClientSampleId :
RE-125D3-20210319


Tgt Ion:240 Resp: 23500
Ion Ratio Lower Upper
240 100
120 6.0 10.2 15.4#
236 25.1 21.3 31.9

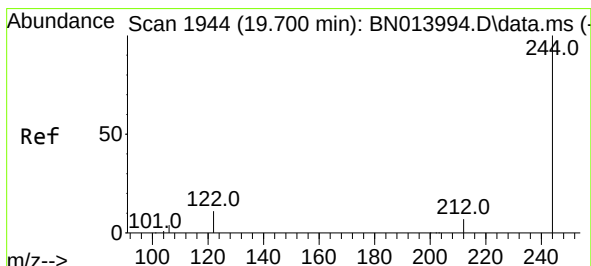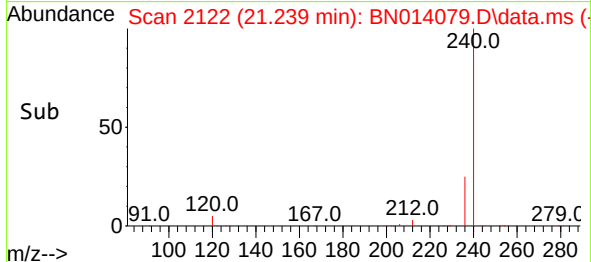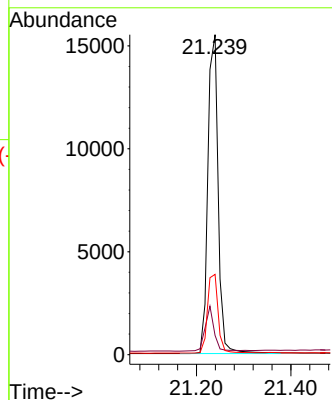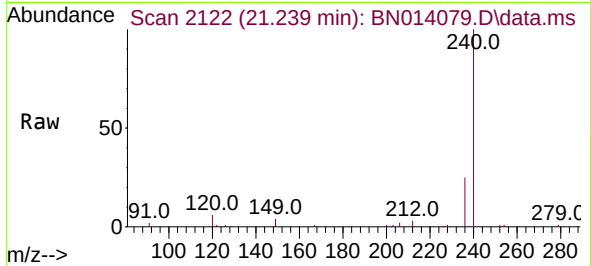

#31
Terphenyl-d14
Concen: 0.53 ng
RT: 19.690 min Scan# 1942
Delta R.T. 0.000 min
Lab File: BN014079.D
Acq: 24 Mar 2021 20:23

Tgt Ion:244 Resp: 27490
Ion Ratio Lower Upper
244 100
212 7.5 6.1 9.1
122 10.9 9.8 14.8


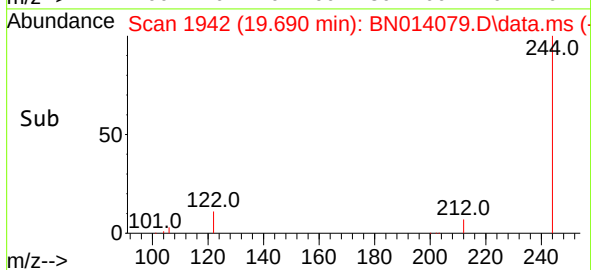
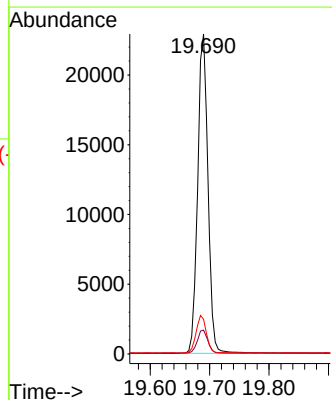
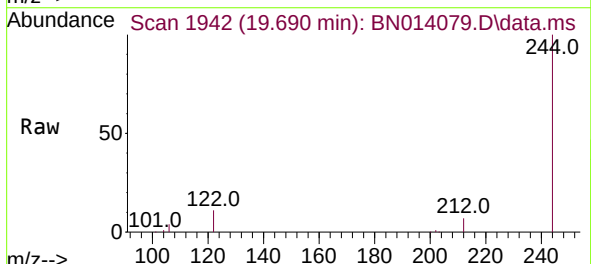


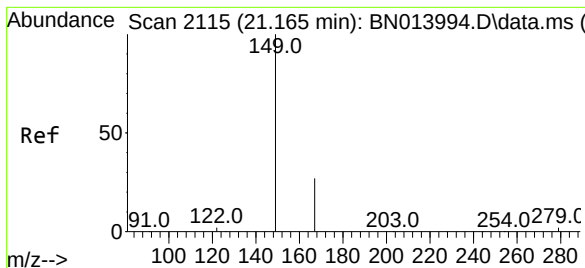

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.06 ng
 RT: 21.154 min Scan# 2114
 Delta R.T. 0.000 min
 Lab File: BN014079.D
 Acq: 24 Mar 2021 20:23

Instrument :
 BNA_N
 ClientSampleId :
 RE-125D3-20210319

Tgt Ion:149 Resp: 1431
 Ion Ratio Lower Upper
 149 100
 167 26.1 22.1 33.1
 279 6.6 3.5 5.3#

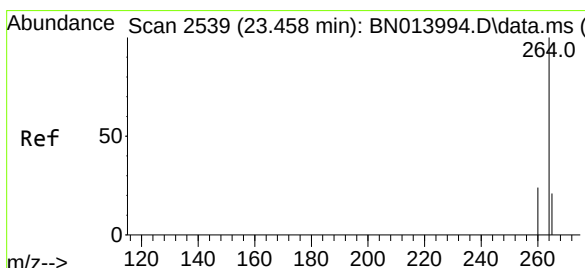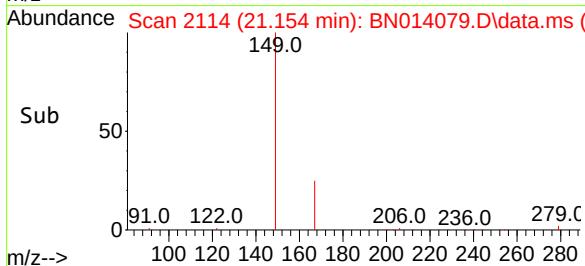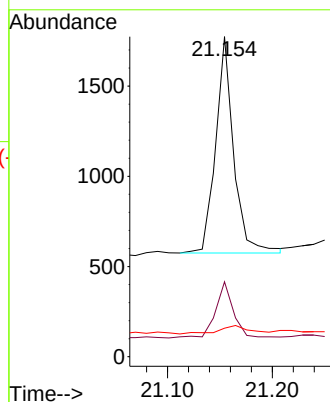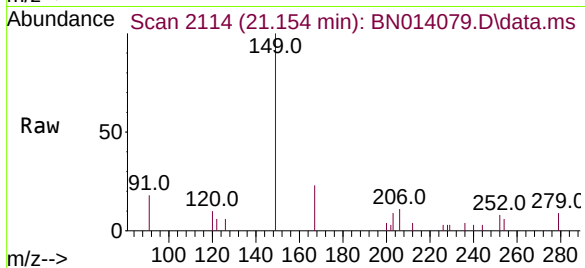

#36
 Perylene-d12
 Concen: 0.40 ng
 RT: 23.441 min Scan# 2534
 Delta R.T. -0.006 min
 Lab File: BN014079.D
 Acq: 24 Mar 2021 20:23

Tgt Ion:264 Resp: 19082
 Ion Ratio Lower Upper
 264 100
 260 25.2 19.3 28.9
 265 36.3 66.2 99.4#

