
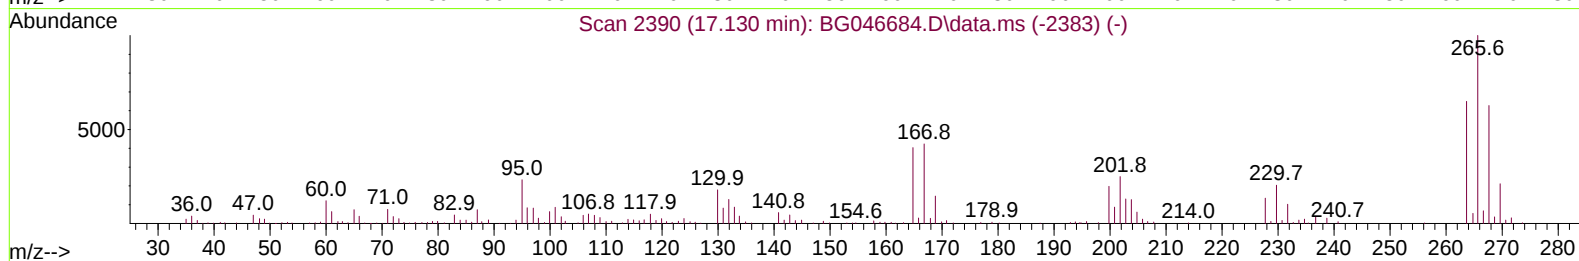
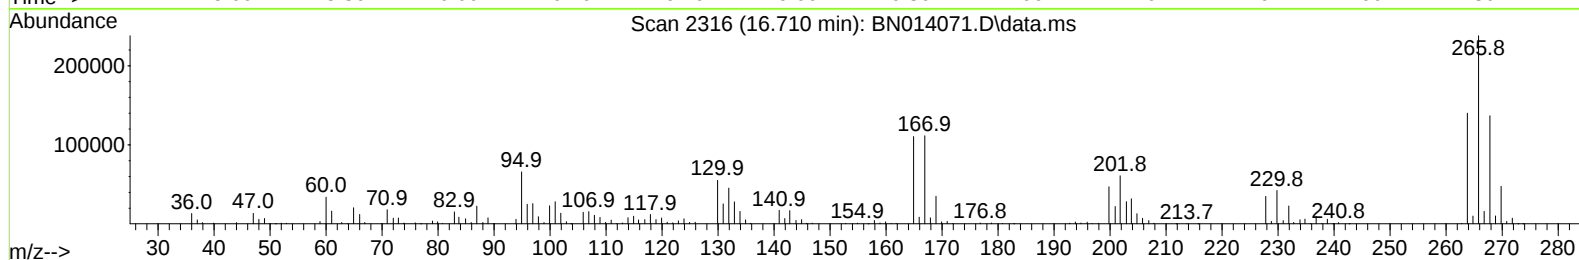


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032421\
Data File : BN014071.D
Acq On : 24 Mar 2021 15:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 25 09:14:13 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 25 09:00:06 2021
Response via : Initial Calibration

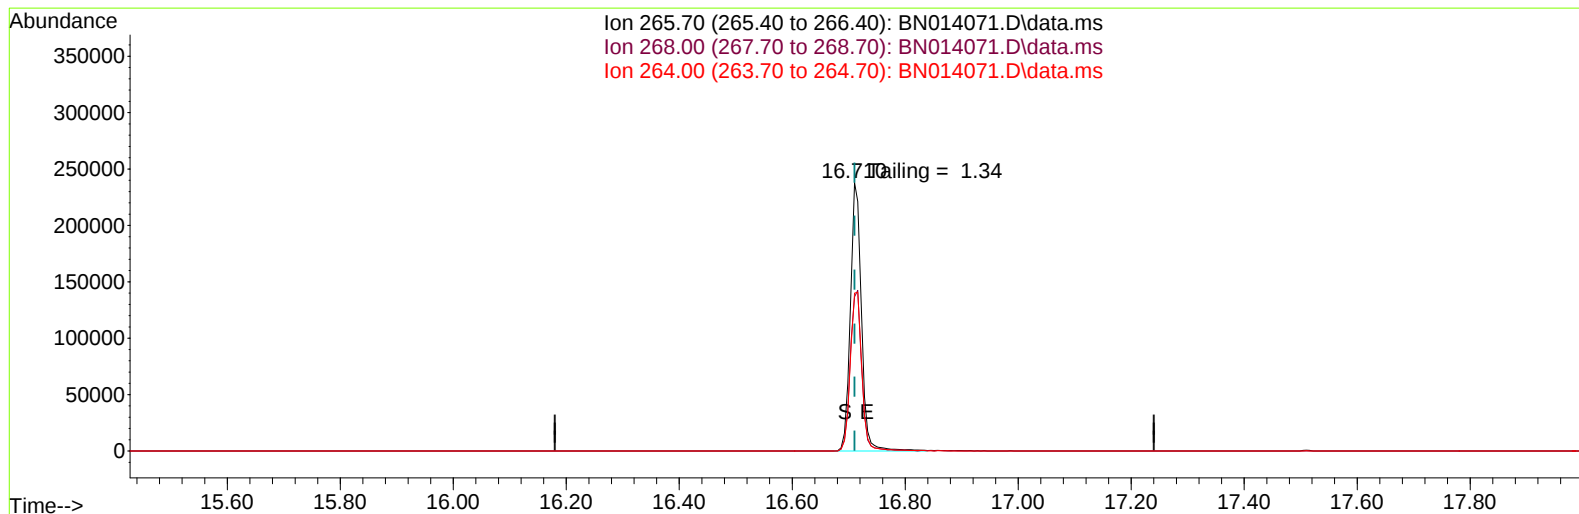

TIC: BN014071.D\data.ms

(70) Pentachlorophenol (C)




16.710min (+ 0.000) 22122.39 ng

response 326215

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	57.50
264.00	61.60	58.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032421\
Data File : BN014071.D
Acq On : 24 Mar 2021 15:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 25 09:14:13 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 25 09:00:06 2021
Response via : Initial Calibration

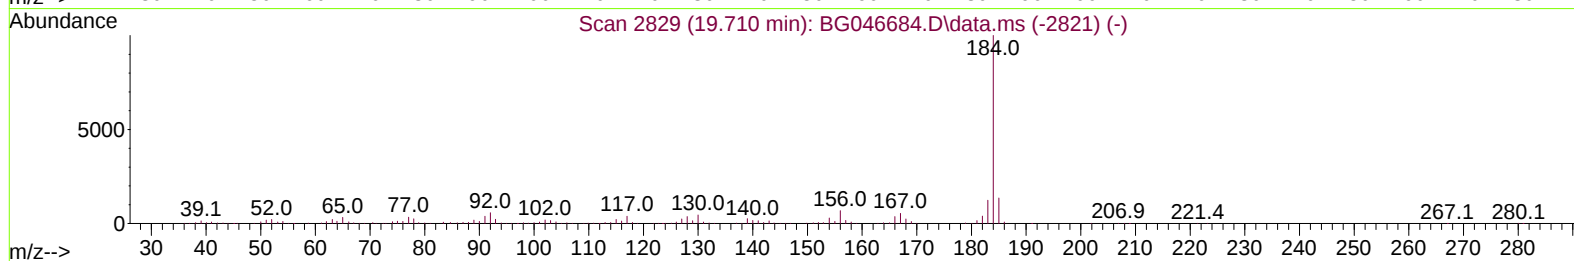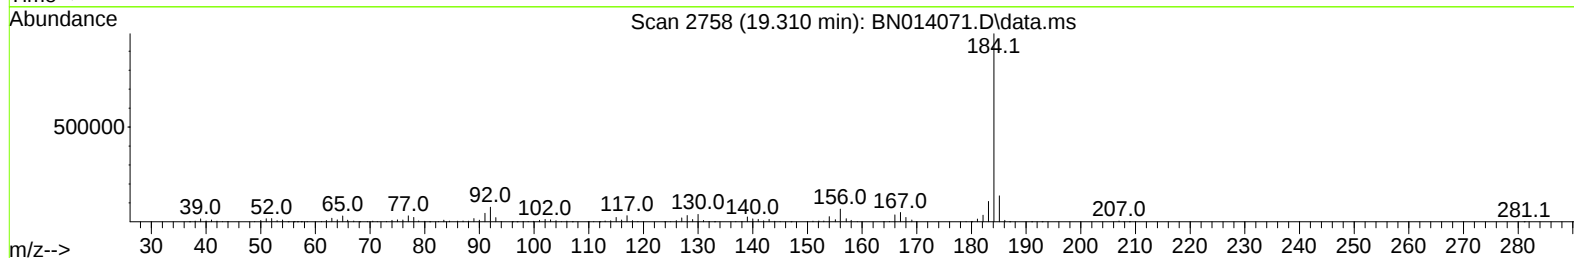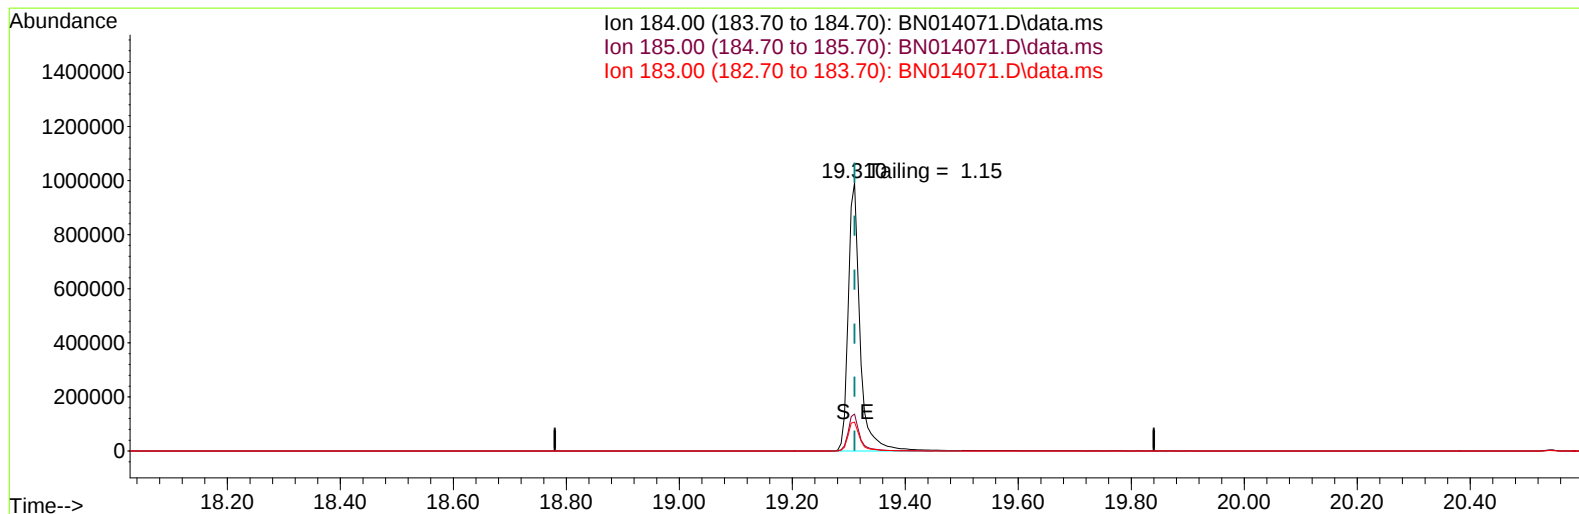

TIC: BN014071.D\data.ms

(77) Benzidine

19.310min (+ 0.000) 0.00 ng m

response 1446742

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.81
183.00	13.20	10.83
0.00	0.00	0.00