
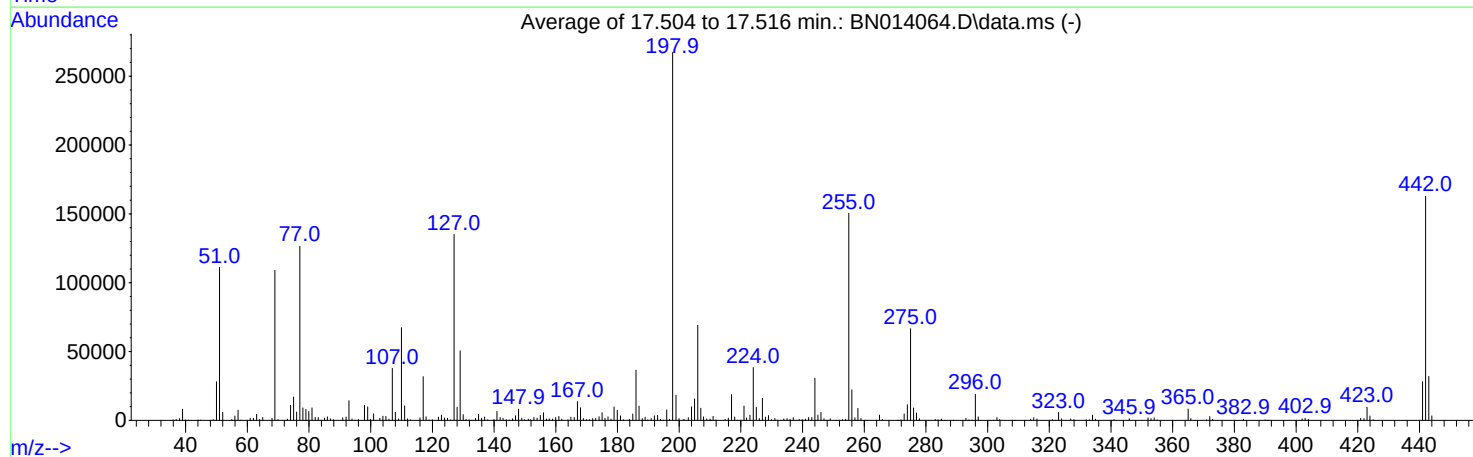


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032421\
 Data File : BN014064.D
 Acq On : 24 Mar 2021 08:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN032021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 23 11:06:27 2021

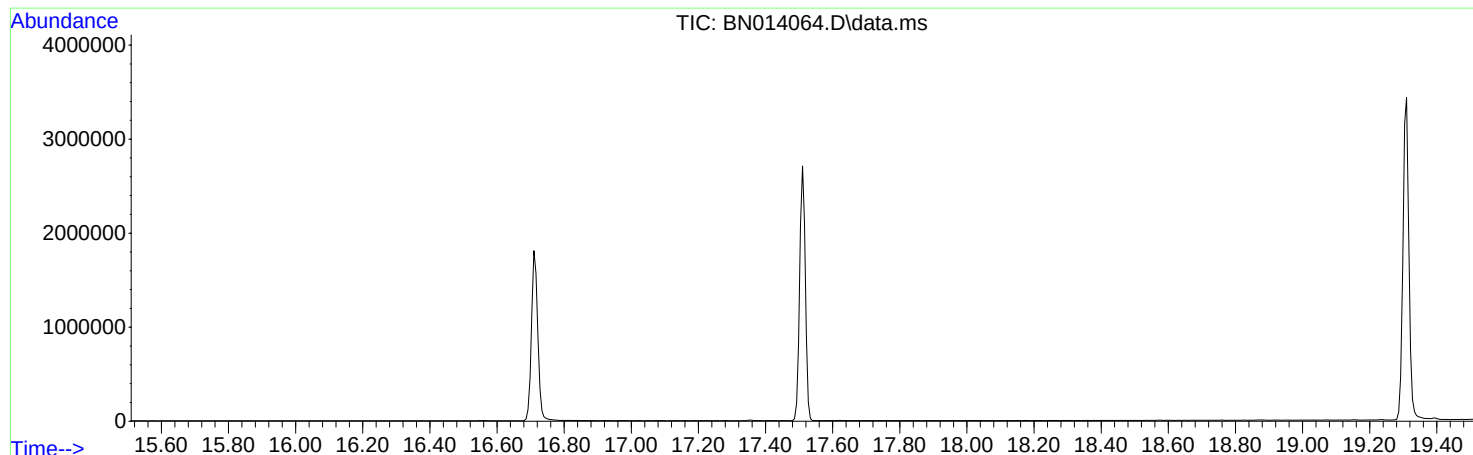




AutoFind: Scans 2451, 2452, 2453; Background Corrected with Scan 2445

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.6	111088	PASS
68	69	0.00	2	1.5	1581	PASS
69	198	0.00	100	40.7	108877	PASS
70	69	0.00	2	0.5	541	PASS
127	198	10	80	50.5	135048	PASS
197	198	0.00	2	0.3	821	PASS
198	198	100	100	100.0	267243	PASS
199	198	5	9	6.8	18267	PASS
275	198	10	60	24.9	66584	PASS
365	198	1	100	3.1	8259	PASS
441	198	0.01	100	10.5	28160	PASS
442	442	50	100	100.0	162808	PASS
443	442	15	24	19.6	31923	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032421\
Data File : BN014064.D
Acq On : 24 Mar 2021 08:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 25 09:00:25 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 25 09:00:06 2021
Response via : Initial Calibration

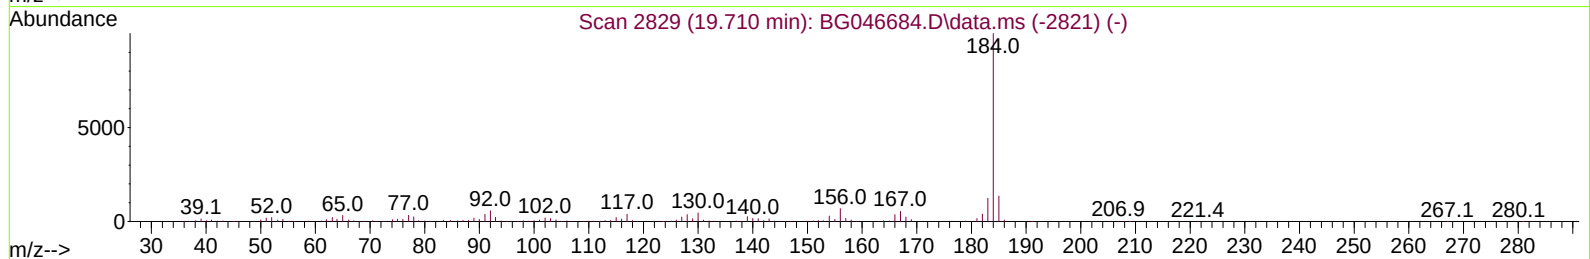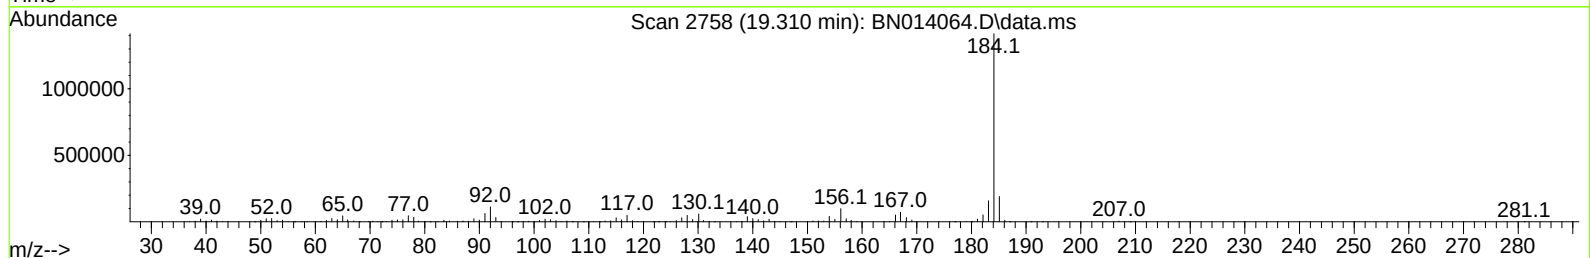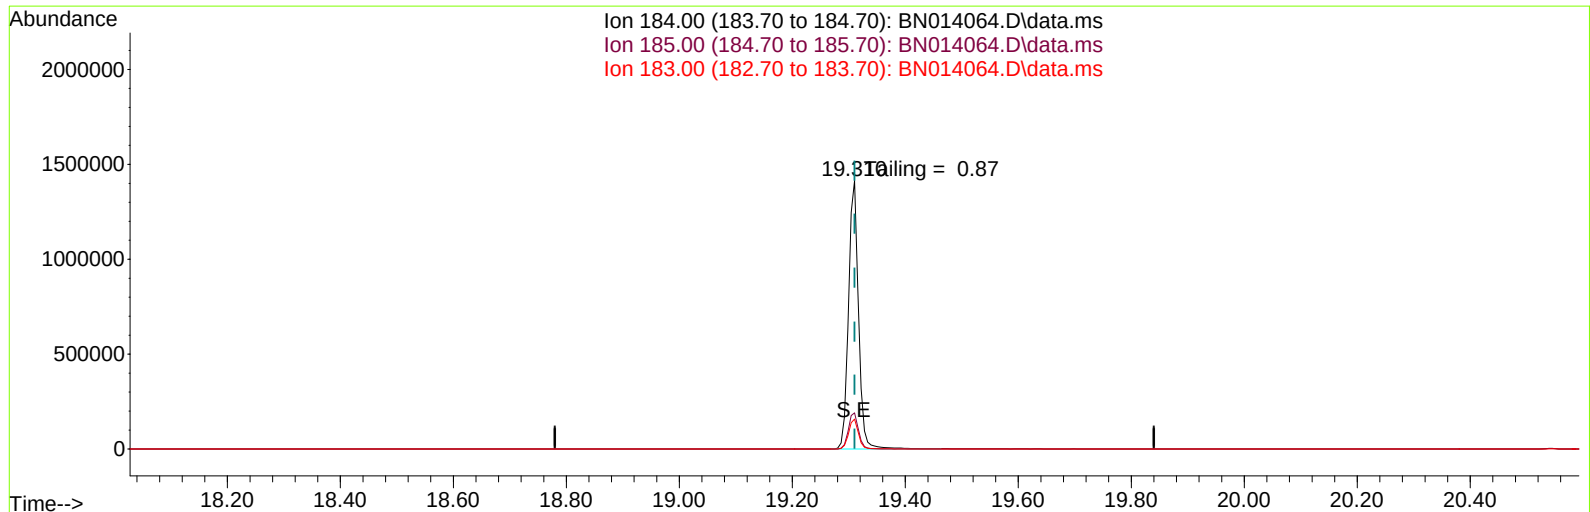

TIC: BN014064.D\data.ms

(77) Benzidine

19.310min (0.000) 0.00 ng




response 1740182

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.50
183.00	13.20	11.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032421\
Data File : BN014064.D
Acq On : 24 Mar 2021 08:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 25 09:00:25 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 25 09:00:06 2021
Response via : Initial Calibration

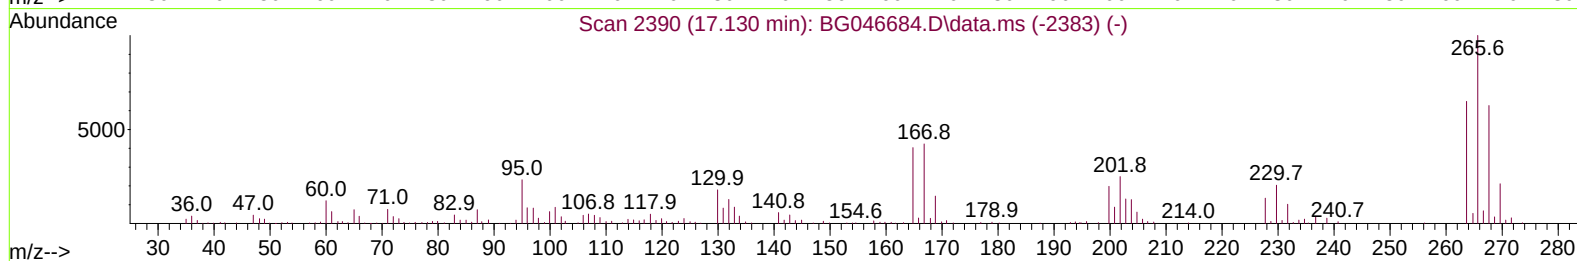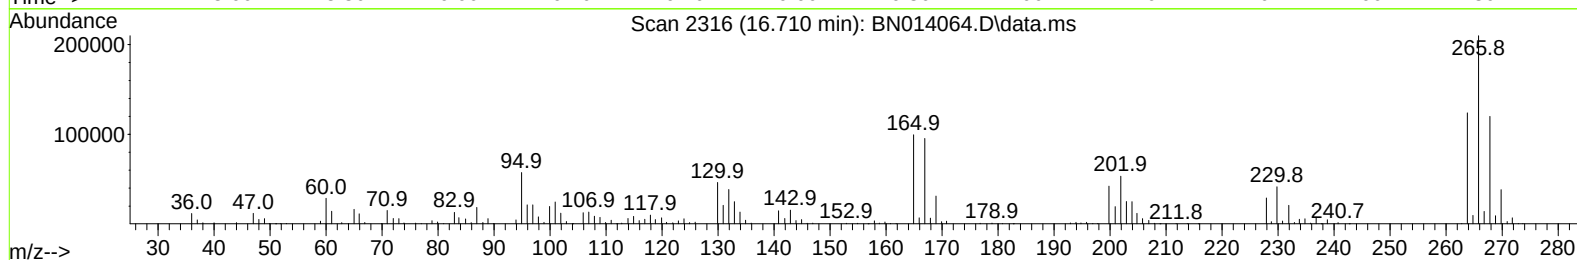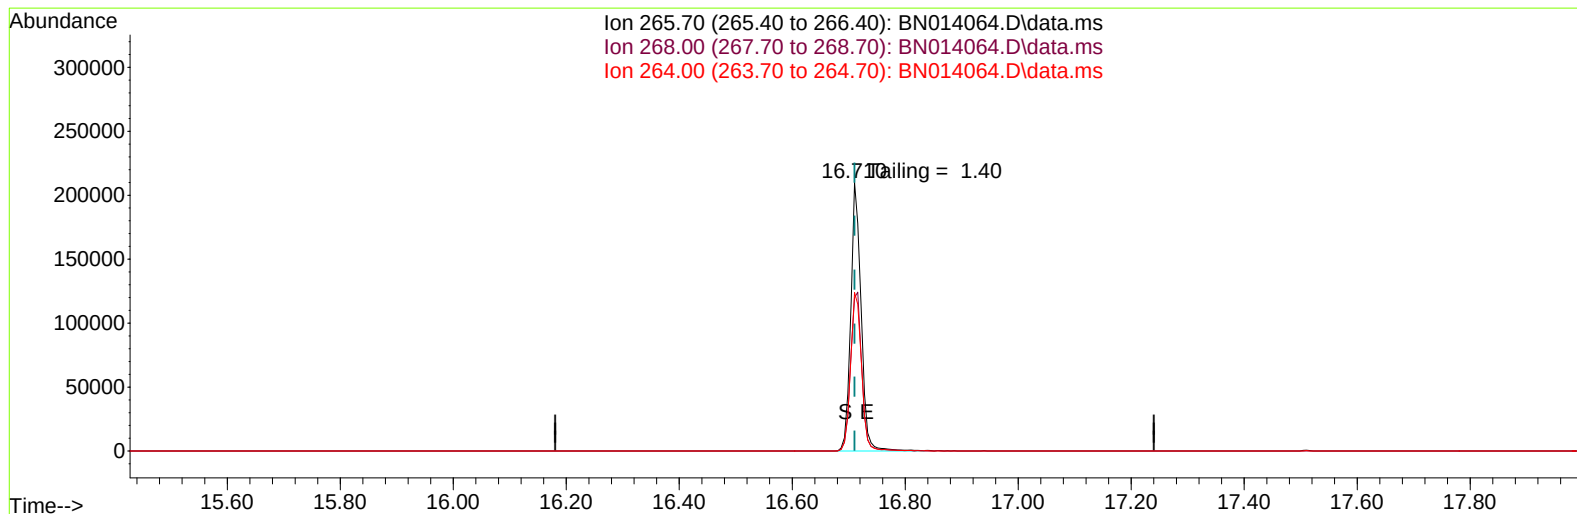

TIC: BN014064.D\data.ms

(70) Pentachlorophenol (C)

16.710min (0.000) 19727.91 ng

response 268767

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	57.13
264.00	61.60	59.03
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
03/24/2021	BNA_N	<u>BN014064.D</u>
Compound Name	Response	Retention Time
DDT	873986	20.545
DDD	8044	20.104
DDE	1484	19.598
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9528	883514	1.08