
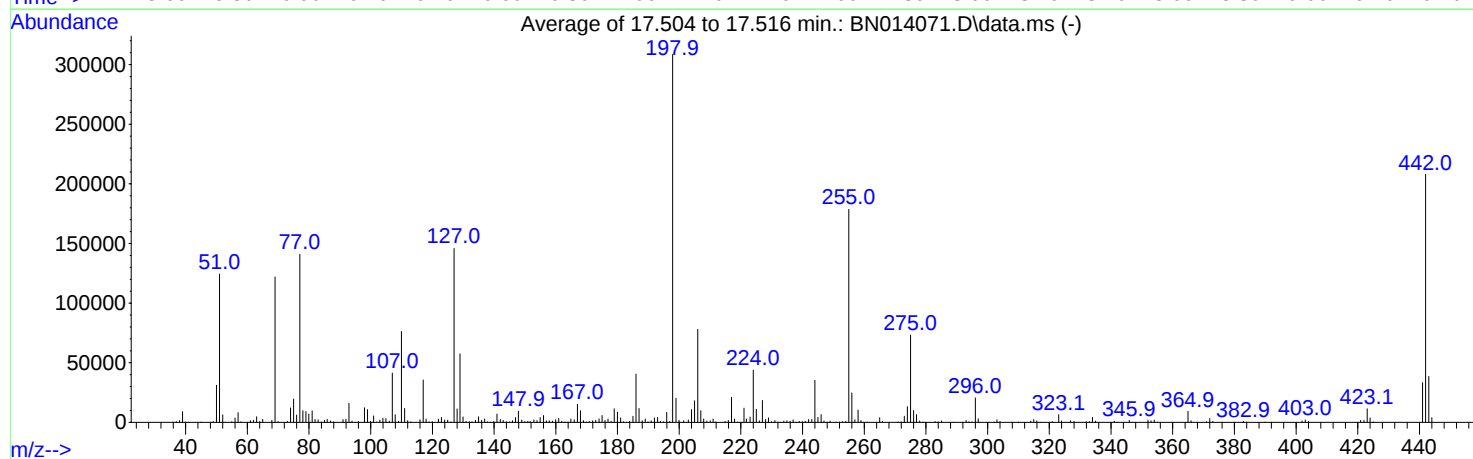


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032421\
 Data File : BN014071.D
 Acq On : 24 Mar 2021 15:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN032021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 23 11:06:27 2021

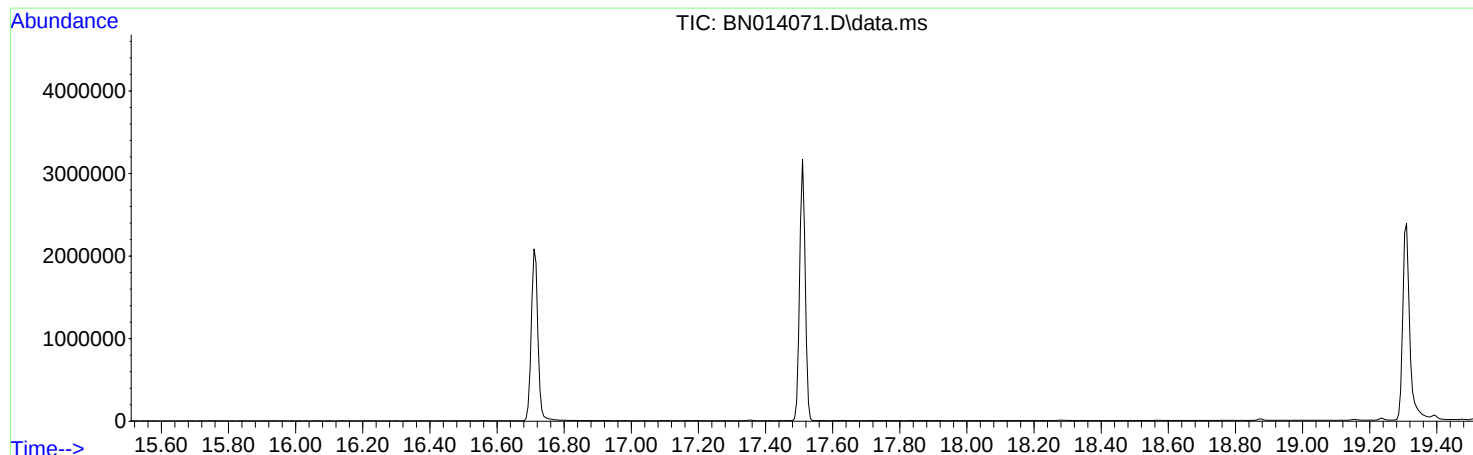




AutoFind: Scans 2451, 2452, 2453; Background Corrected with Scan 2444

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.3	124445	PASS
68	69	0.00	2	1.5	1805	PASS
69	198	0.00	100	39.5	121979	PASS
70	69	0.00	2	0.6	678	PASS
127	198	10	80	47.3	145867	PASS
197	198	0.00	2	0.3	868	PASS
198	198	100	100	100.0	308480	PASS
199	198	5	9	6.6	20312	PASS
275	198	10	60	23.8	73272	PASS
365	198	1	100	3.0	9233	PASS
441	198	0.01	100	10.8	33304	PASS
442	442	50	100	100.0	207957	PASS
443	442	15	24	18.5	38493	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032421\
Data File : BN014071.D
Acq On : 24 Mar 2021 15:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 25 09:14:13 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 25 09:00:06 2021
Response via : Initial Calibration

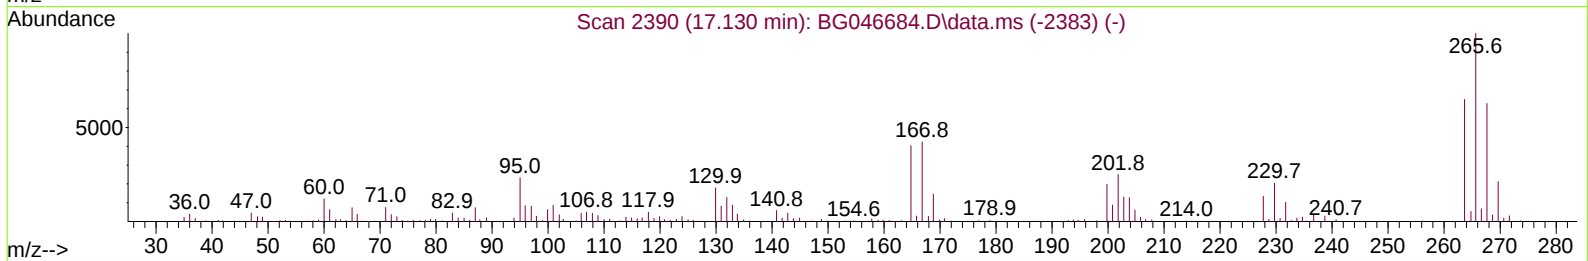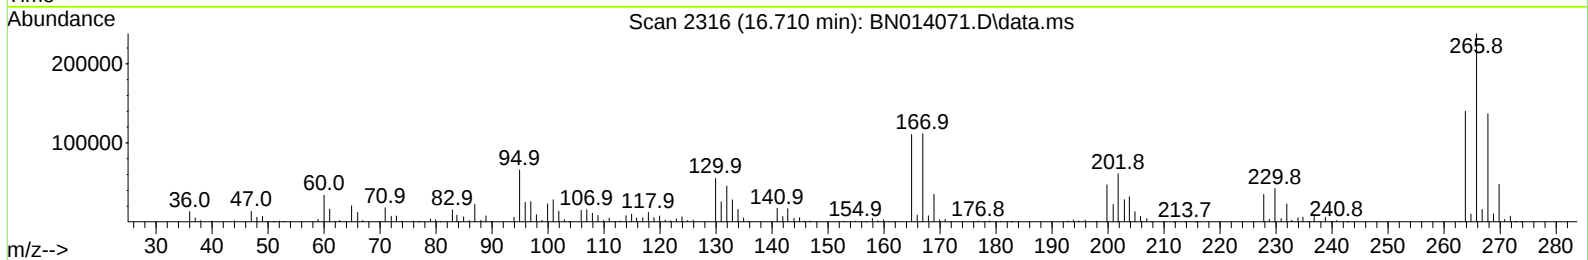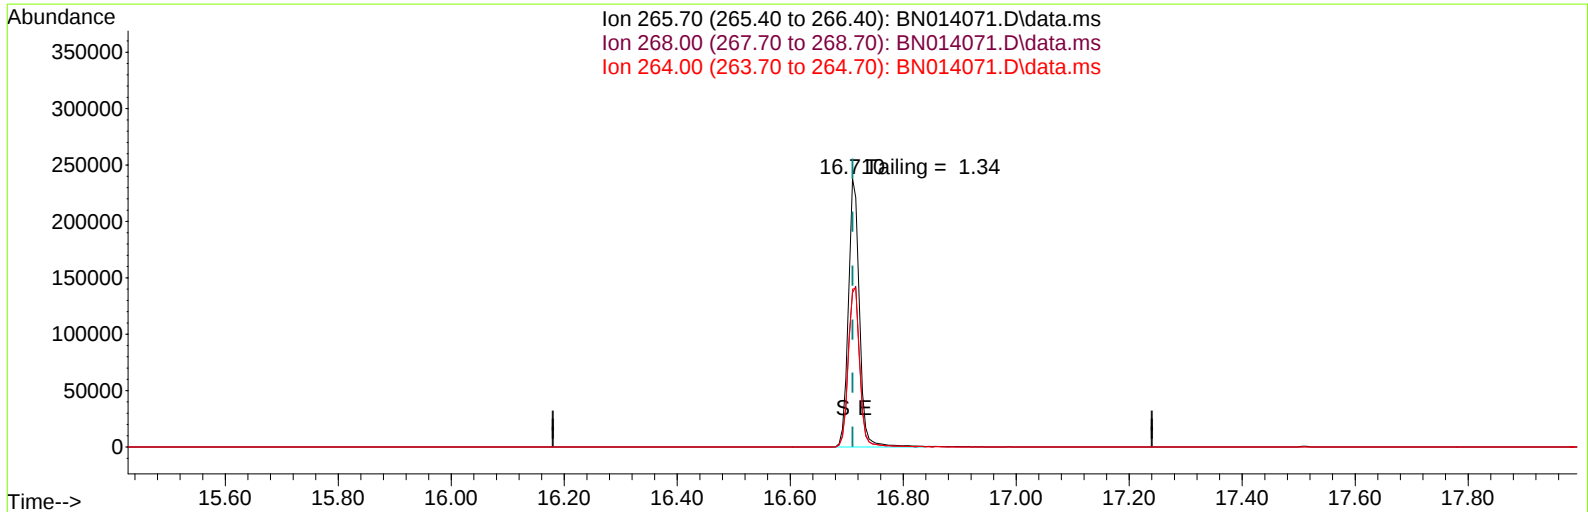

TIC: BN014071.D\data.ms

(70) Pentachlorophenol (C)

16.710min (+ 0.000) 22122.39 ng




response 326215

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	57.50
264.00	61.60	58.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032421\
 Data File : BN014071.D
 Acq On : 24 Mar 2021 15:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Mar 25 09:14:13 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 25 09:00:06 2021
 Response via : Initial Calibration

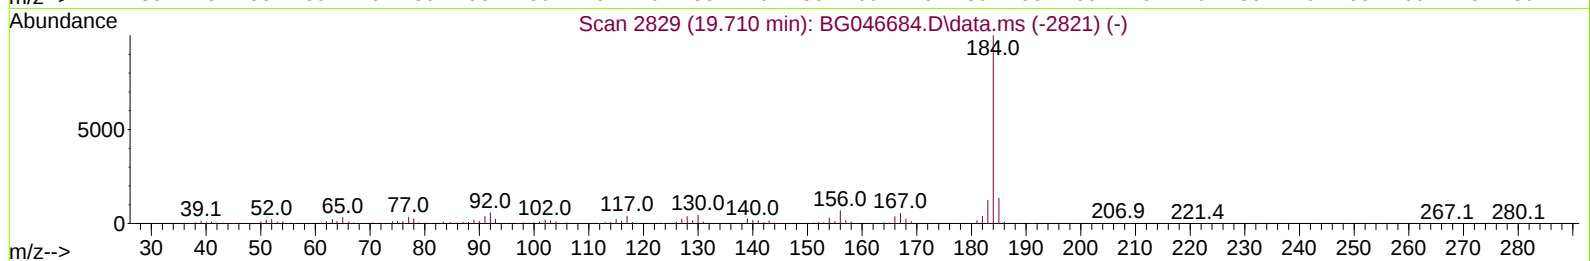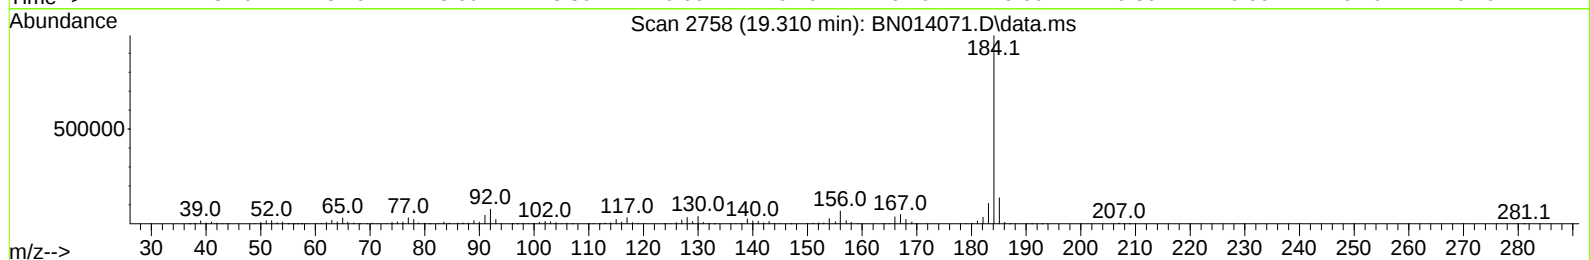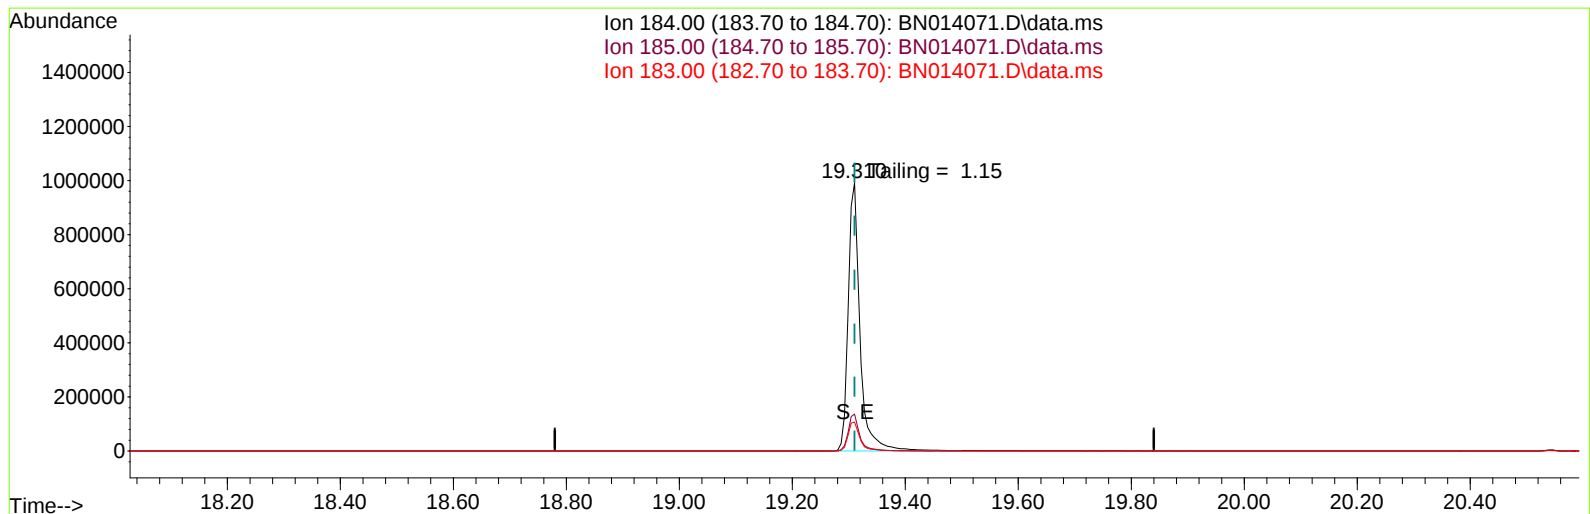

TIC: BN014071.D\data.ms

(77) Benzidine

19.310min (+ 0.000) 0.00 ng m

response 1446742

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.81
183.00	13.20	10.83
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_N
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
03/24/2021	BNA_N	<u>BN014071.D</u>
Compound Name	Response	Retention Time
DDT	1036114	20.545
DDD	10399	20.104
DDE	3026	19.598
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13425	1049539	1.28