
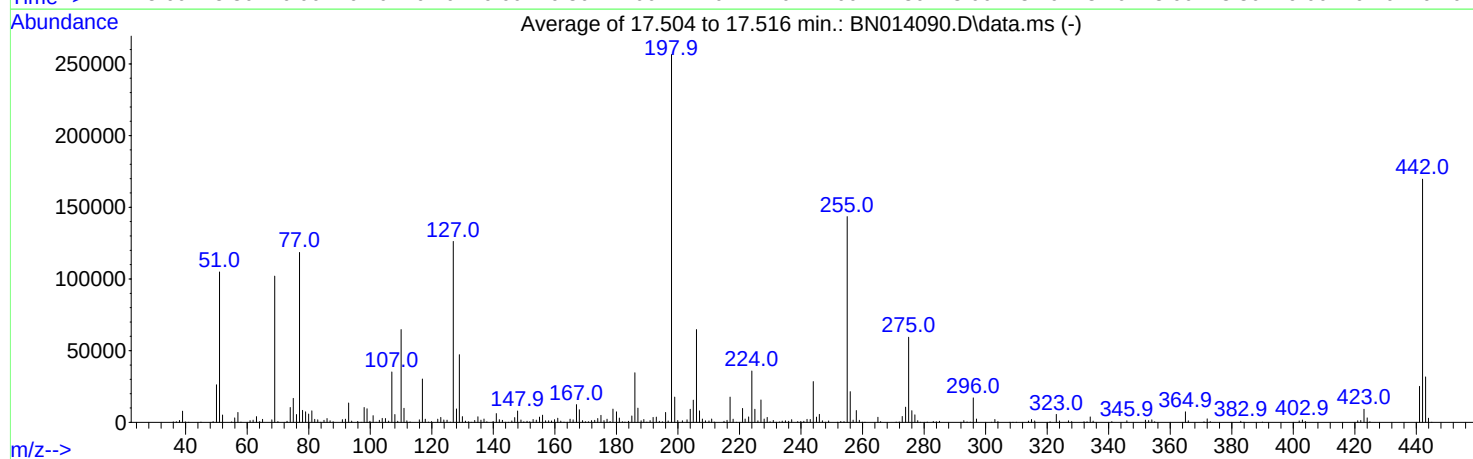


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032421\
 Data File : BN014090.D
 Acq On : 25 Mar 2021 03:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN032021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 23 11:06:27 2021

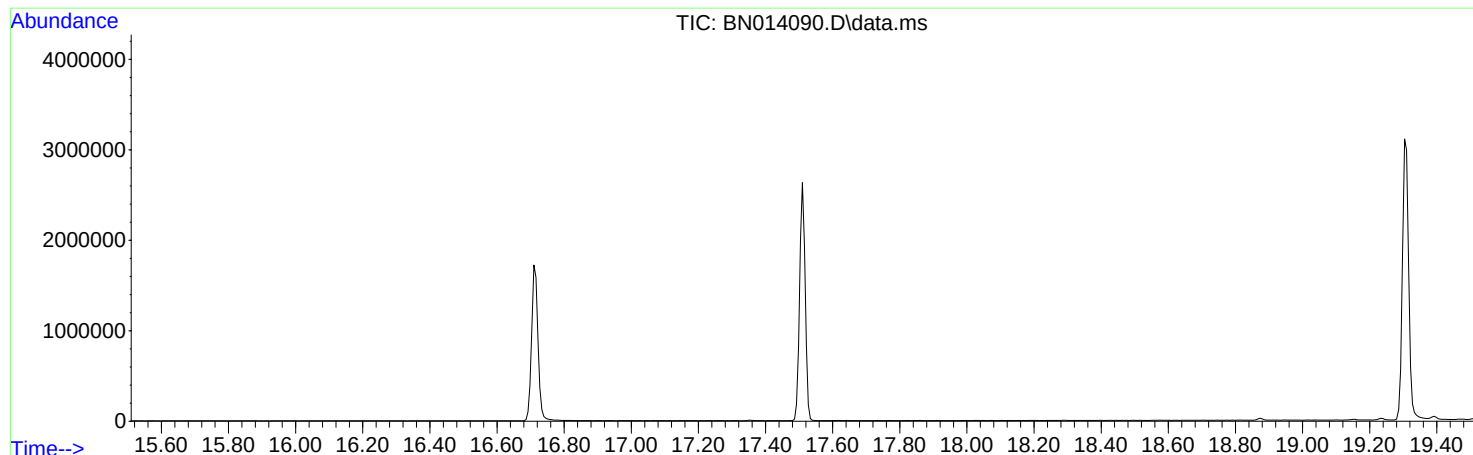




AutoFind: Scans 2451, 2452, 2453; Background Corrected with Scan 2445

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.9	104931	PASS
68	69	0.00	2	1.7	1762	PASS
69	198	0.00	100	39.7	101965	PASS
70	69	0.00	2	0.6	576	PASS
127	198	10	80	49.2	126200	PASS
197	198	0.00	2	0.4	1017	PASS
198	198	100	100	100.0	256555	PASS
199	198	5	9	6.9	17622	PASS
275	198	10	60	23.2	59408	PASS
365	198	1	100	2.9	7344	PASS
441	198	0.01	100	9.8	25149	PASS
442	442	50	100	100.0	169648	PASS
443	442	15	24	18.7	31661	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032421\
Data File : BN014090.D
Acq On : 25 Mar 2021 03:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 25 09:50:36 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 25 09:00:06 2021
Response via : Initial Calibration

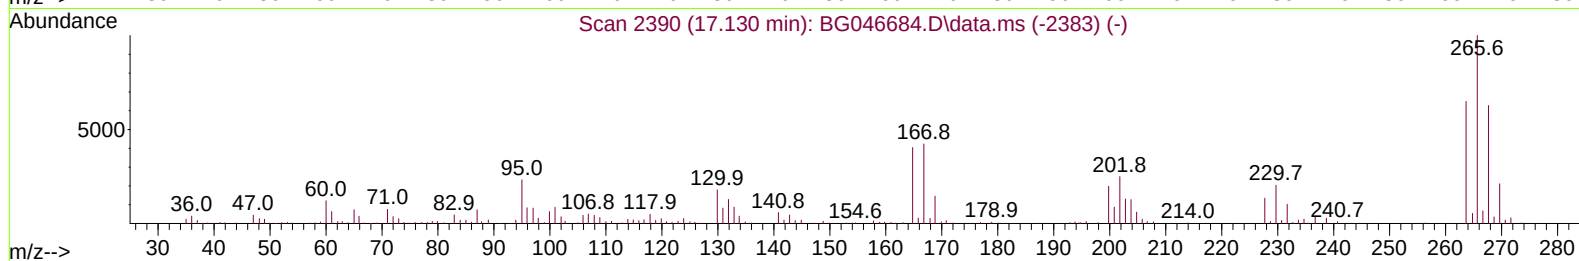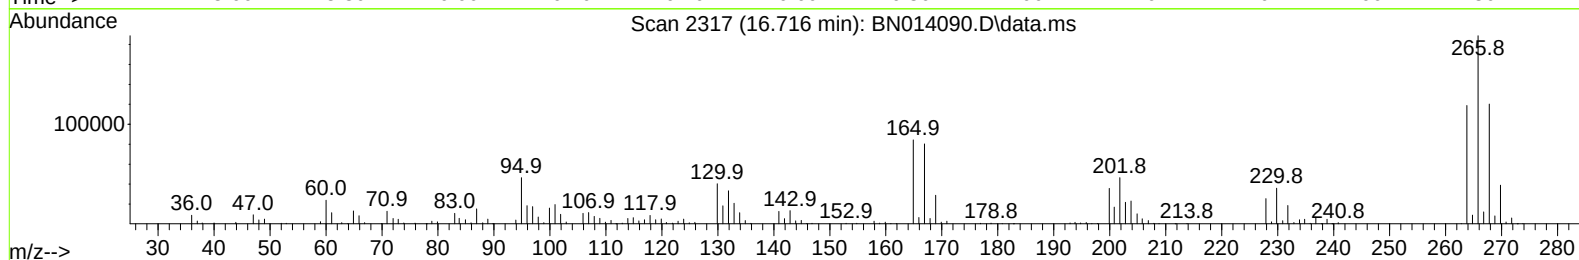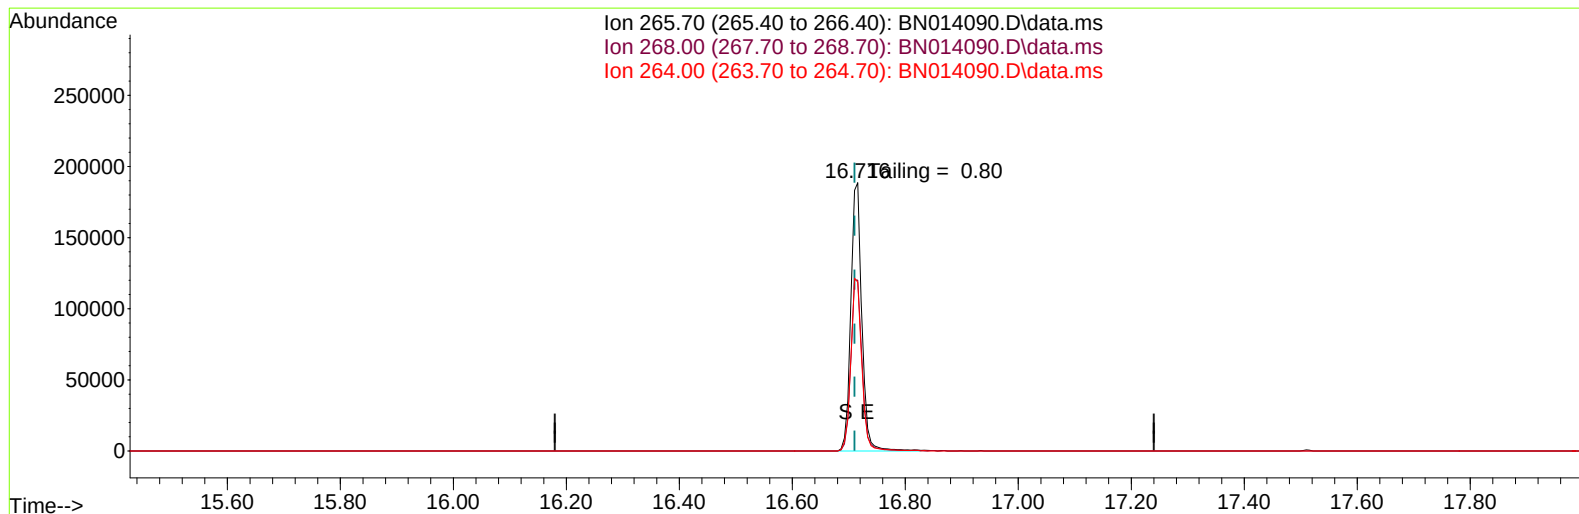

TIC: BN014090.D\data.ms

(70) Pentachlorophenol (C)

16.716min (+ 0.006) 21399.25 ng




response 256942

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.69
264.00	61.60	62.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032421\
Data File : BN014090.D
Acq On : 25 Mar 2021 03:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 25 09:50:36 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 25 09:00:06 2021
Response via : Initial Calibration

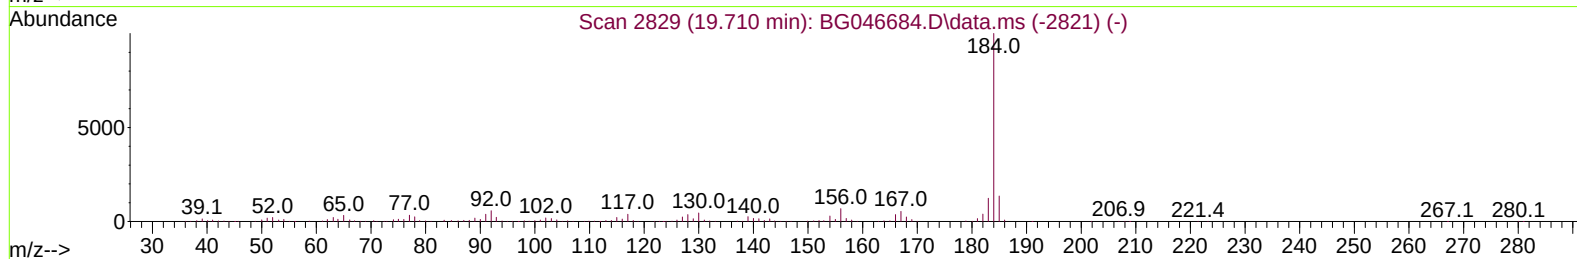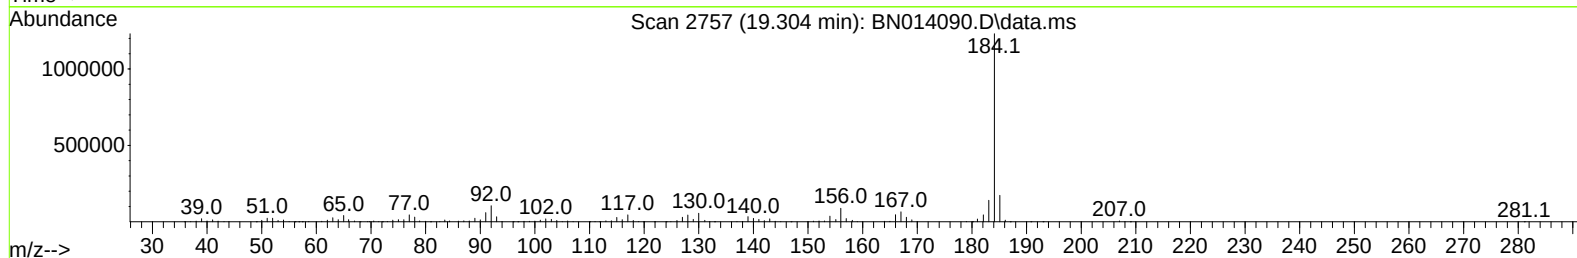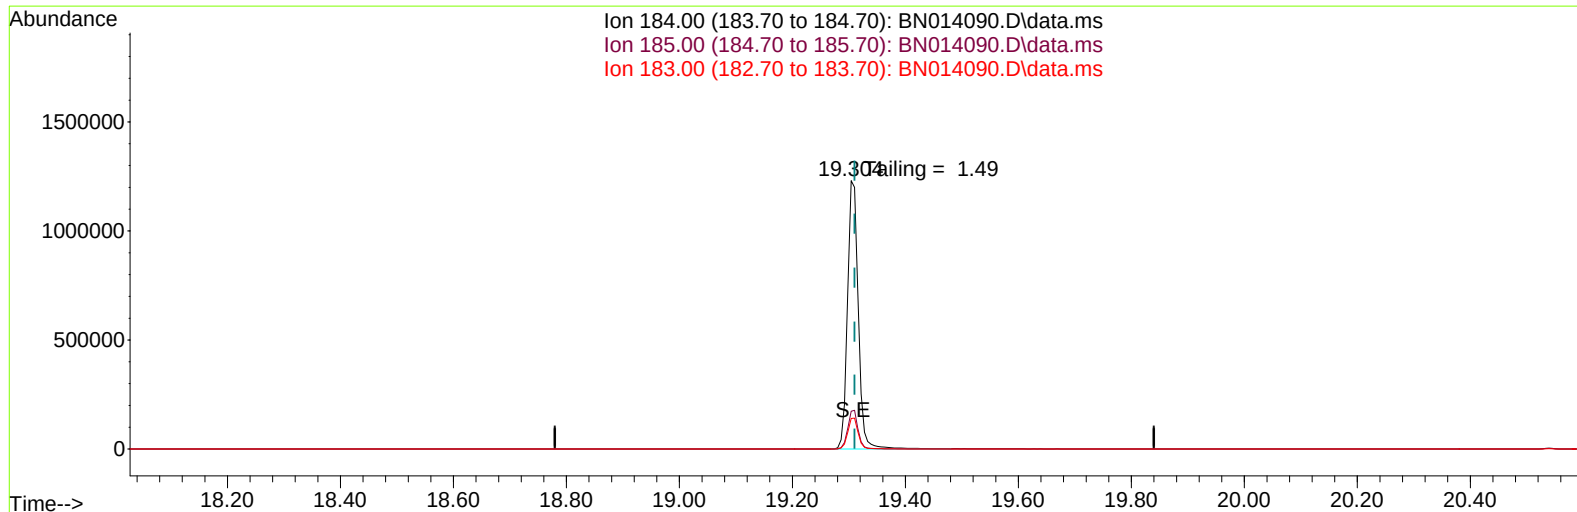

TIC: BN014090.D\data.ms

(77) Benzidine

19.304min (-0.006) 0.00 ng

response 1637066

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.06
183.00	13.20	11.40
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_N
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
03/24/2021	BNA_N	<u>BN014090.D</u>
Compound Name	Response	Retention Time
DDT	877104	20.539
DDD	7535	20.098
DDE	1399	19.598
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8934	886038	1.01