
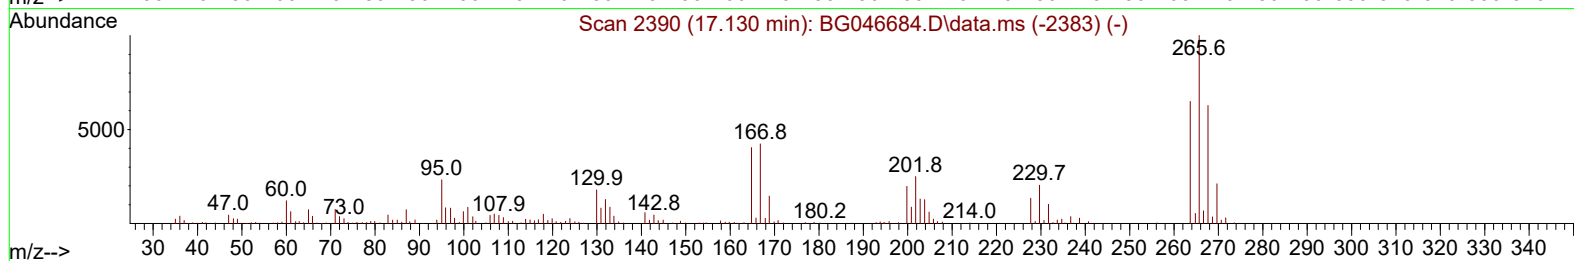
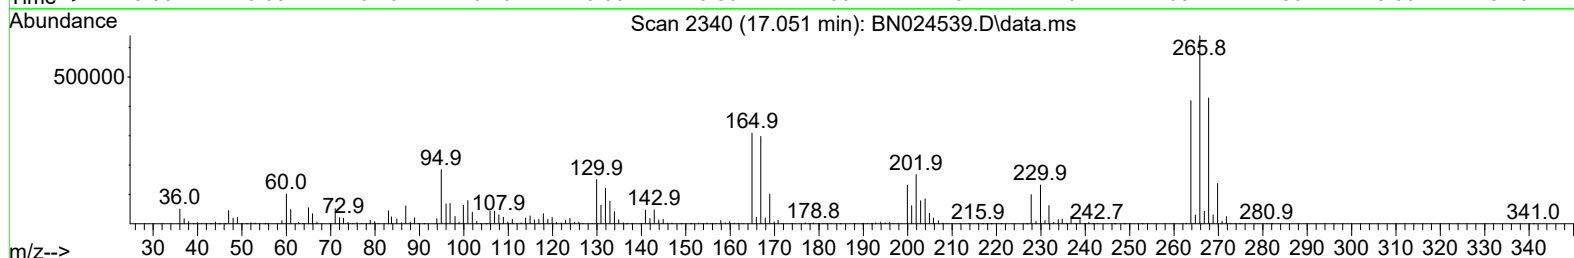


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032423\
Data File : BN024539.D
Acq On : 24 Mar 2023 10:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 25 04:06:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 25 04:06:45 2023
Response via : Initial Calibration

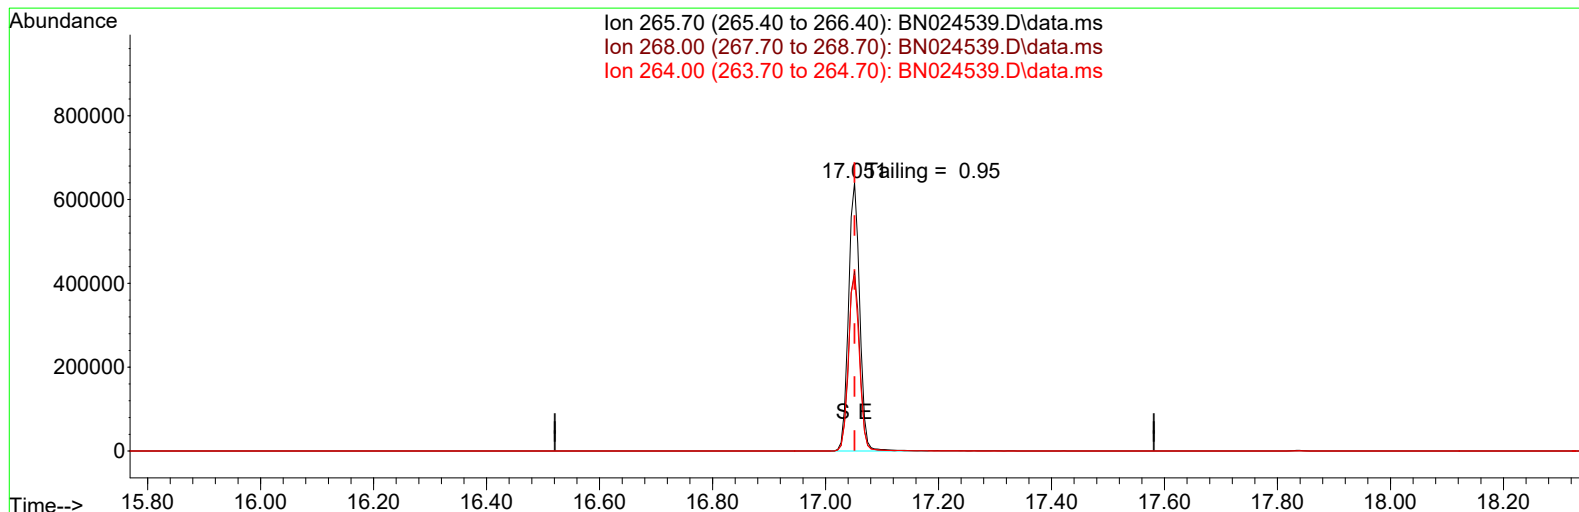

TIC: BN024539.D\data.ms

(70) Pentachlorophenol (C)




17.051min (0.000) 26179.58 ng

response 884260

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.87
264.00	61.60	65.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032423\
Data File : BN024539.D
Acq On : 24 Mar 2023 10:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 25 04:06:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 25 04:06:45 2023
Response via : Initial Calibration

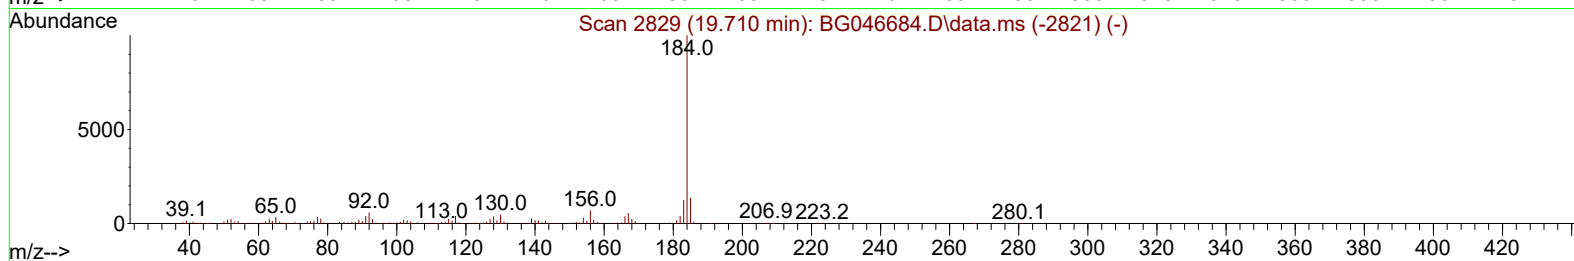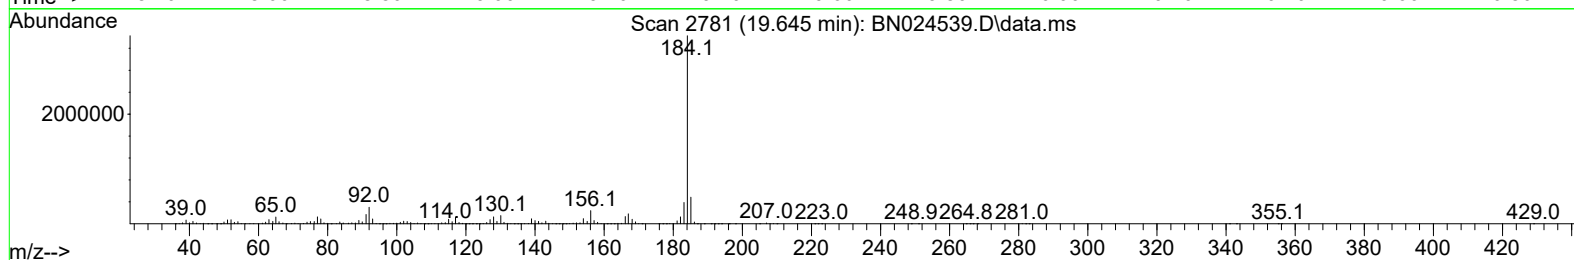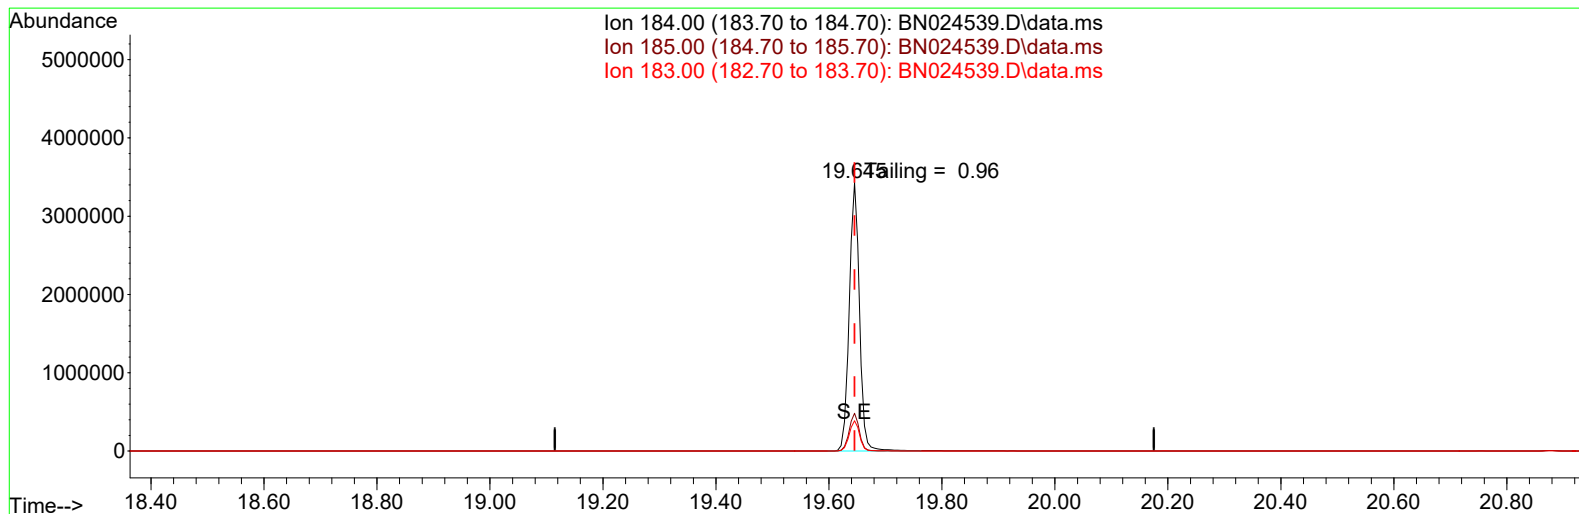

TIC: BN024539.D\data.ms

(77) Benzidine**19.645min (0.000) 1151438.80 ng****response 4294717**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.10
183.00	13.20	11.30
0.00	0.00	0.00