
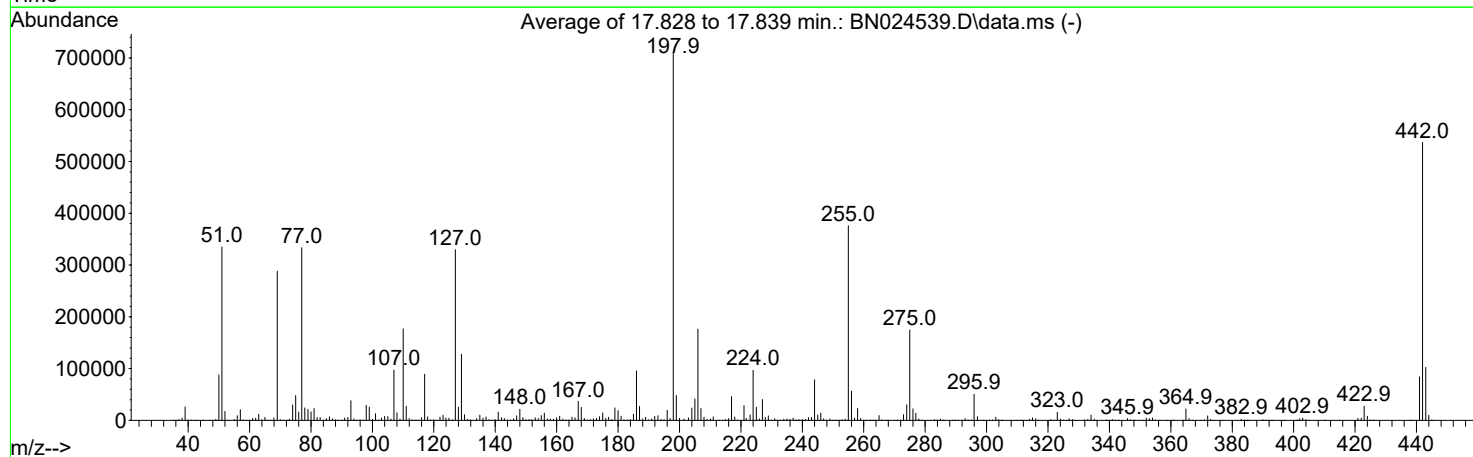


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN032423\  
 Data File : BN024539.D  
 Acq On : 24 Mar 2023 10:10  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN031323.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Sat Mar 25 00:22:43 2023

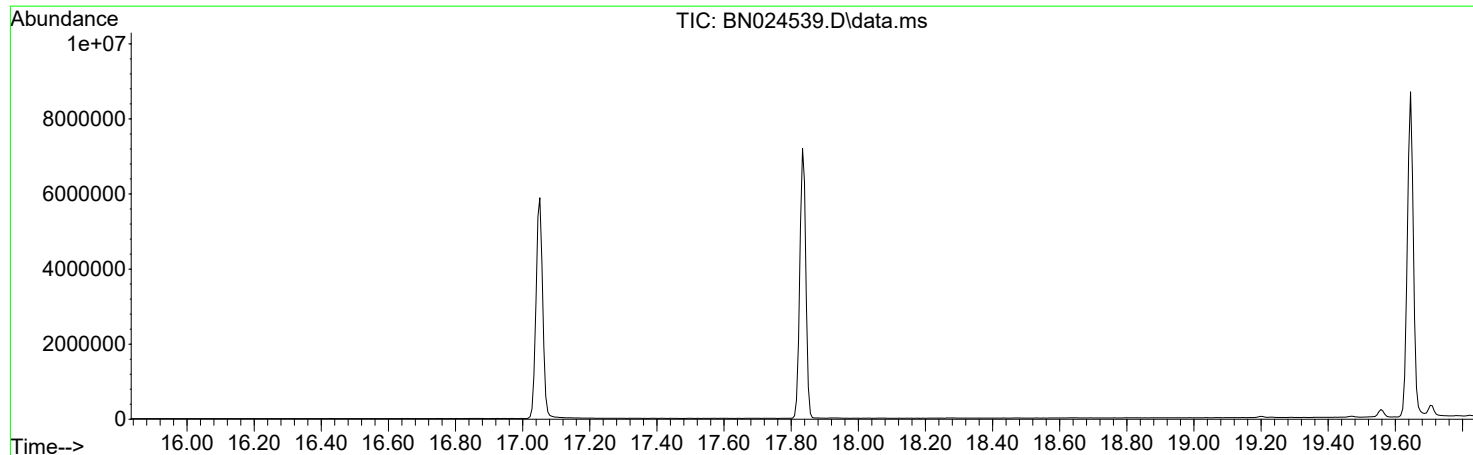

AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2465

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 47.1         | 334869     | PASS                |
| 68             | 69              | 0.00            | 2               | 1.6          | 4723       | PASS                |
| 69             | 198             | 0.00            | 100             | 40.6         | 288149     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 1542       | PASS                |
| 127            | 198             | 10              | 80              | 46.4         | 329877     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.5          | 3643       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 710485     | PASS                |
| 199            | 198             | 5               | 9               | 6.8          | 48323      | PASS                |
| 275            | 198             | 10              | 60              | 24.6         | 174571     | PASS                |
| 365            | 198             | 1               | 100             | 3.1          | 21872      | PASS                |
| 441            | 198             | 0.01            | 100             | 11.8         | 84005      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 536789     | PASS                |
| 443            | 442             | 15              | 24              | 19.0         | 102211     | PASS                |

# DDT Breakdown




| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 3/24/2023     | BNA_N            | <u>BN024539.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 2267344          | 20.88              |
| DDD           | 163939           | 20.433             |
| DDE           | 8204             | 19.928             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 172143        | 2439487          | 7.06               |
|               |                  |                    |

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN032423\  
Data File : BN024539.D  
Acq On : 24 Mar 2023 10:10  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Quant Time: Mar 25 04:06:49 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Mar 25 04:06:45 2023  
Response via : Initial Calibration

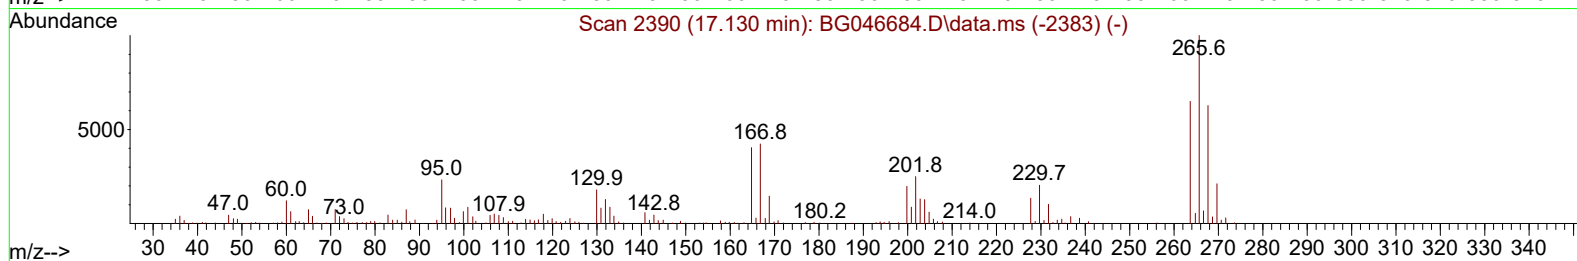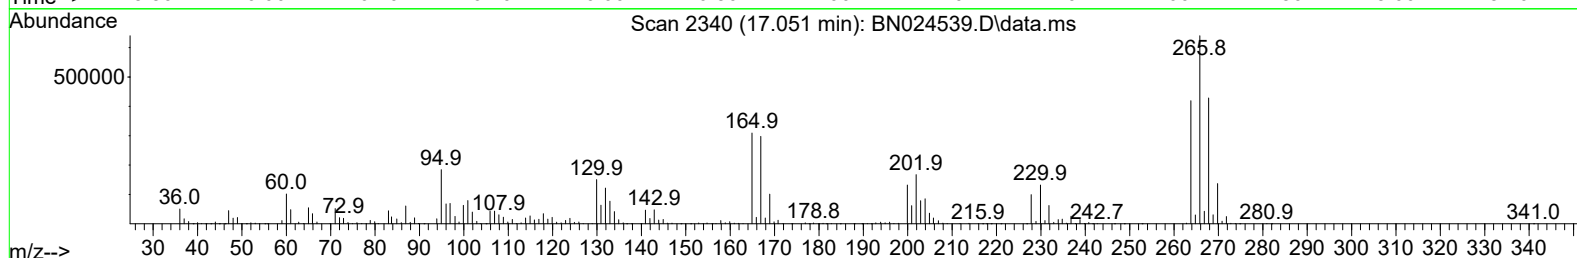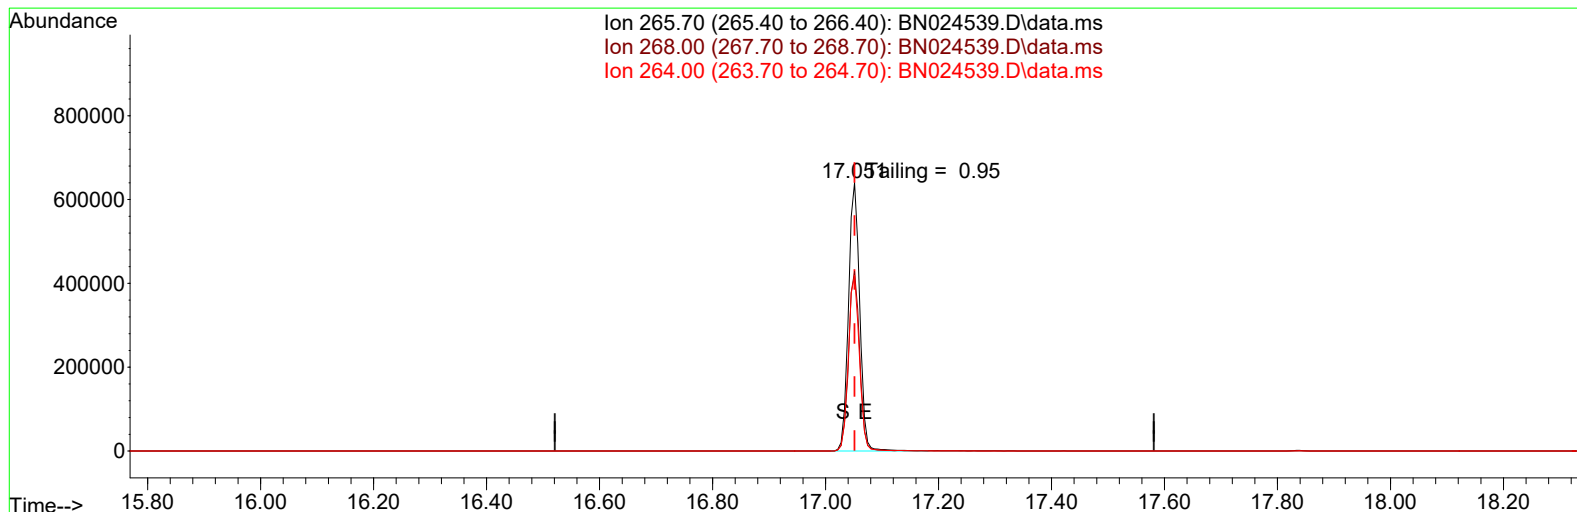

TIC: BN024539.D\data.ms

**(70) Pentachlorophenol (C)**

17.051min ( 0.000) 26179.58 ng




response 884260

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 66.87  |
| 264.00 | 61.60  | 65.47  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN032423\  
 Data File : BN024539.D  
 Acq On : 24 Mar 2023 10:10  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Quant Time: Mar 25 04:06:49 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Sat Mar 25 04:06:45 2023  
 Response via : Initial Calibration

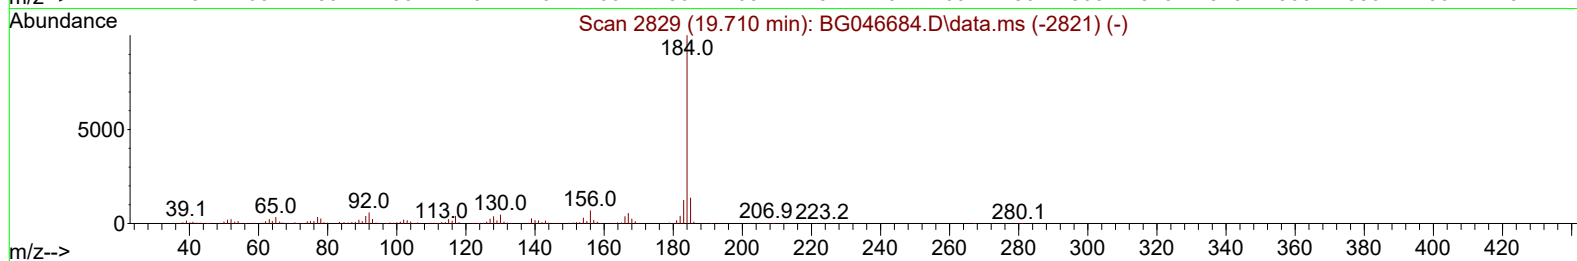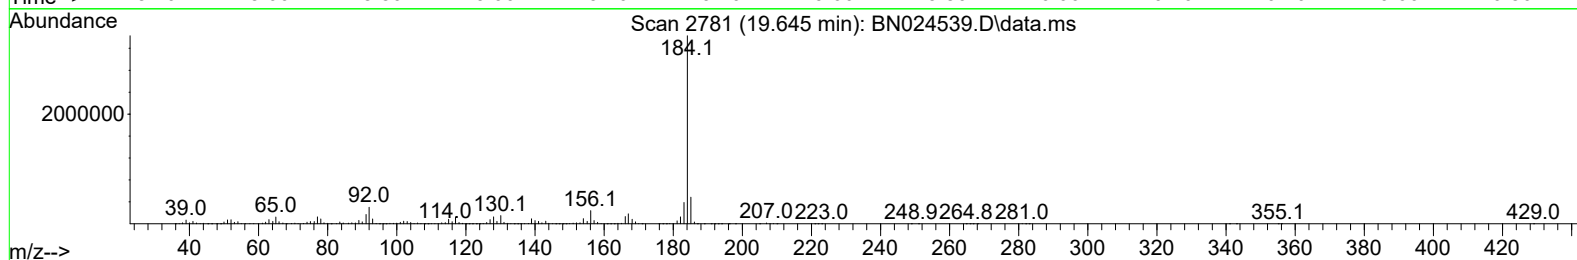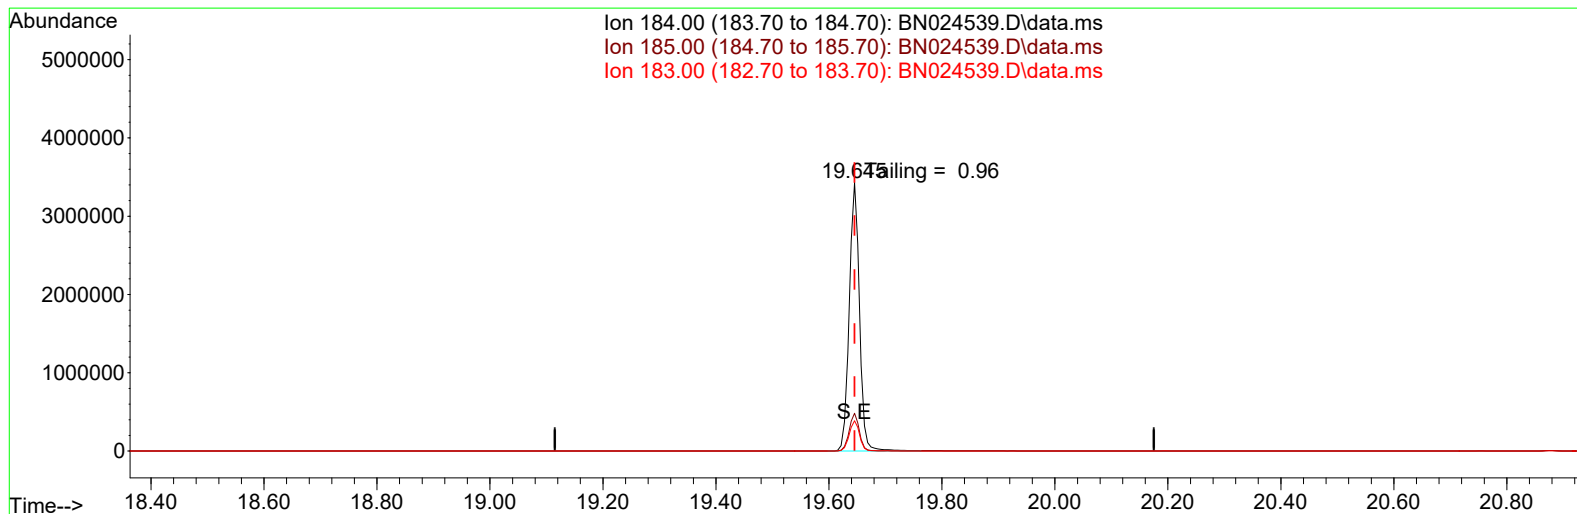

TIC: BN024539.D\data.ms

**(77) Benzidine**

19.645min ( 0.000) 1151438.80 ng

response 4294717

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 14.10  |
| 183.00 | 13.20  | 11.30  |
| 0.00   | 0.00   | 0.00   |