

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033122\
 Data File : BN019294.D
 Acq On : 01 Apr 2022 19:08
 Operator : CG/JU
 Sample : N2220-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A04015

Quant Time: Apr 01 21:58:47 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN033122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 31 12:41:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.840	152	3936	0.400	ng	0.00
7) Naphthalene-d8	10.637	136	11556	0.400	ng	# 0.00
13) Acenaphthene-d10	14.474	164	7481	0.400	ng	0.00
19) Phenanthrene-d10	17.215	188	14795	0.400	ng	0.00
29) Chrysene-d12	21.404	240	11882	0.400	ng	# 0.00
35) Perylene-d12	23.764	264	9860	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.392	112	2729	0.317	ng	0.00
5) Phenol-d6	7.002	99	2539	0.278	ng	0.00
8) Nitrobenzene-d5	9.003	82	1871	0.225	ng	0.01
11) 2-Methylnaphthalene-d10	12.231	152	5245	0.286	ng	0.00
14) 2,4,6-Tribromophenol	15.974	330	693	0.198	ng	0.01
15) 2-Fluorobiphenyl	13.105	172	7209	0.240	ng	0.00
27) Fluoranthene-d10	19.248	212	12650	0.285	ng	0.00
31) Terphenyl-d14	19.843	244	6839	0.259	ng	0.00
Target Compounds						
20) 4,6-Dinitro-2-methylph...	15.618	198	5	0.092	ng	# 1
25) Phenanthrene	17.256	178	1072	0.023	ng	98
34) Bis(2-ethylhexyl)phtha...	21.315	149	3020	0.121	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033122\
Data File : BN019294.D
Acq On : 01 Apr 2022 19:08
Operator : CG/JU
Sample : N2220-10
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A04015


Quant Time: Apr 01 21:58:47 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN033122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 31 12:41:03 2022
Response via : Initial Calibration

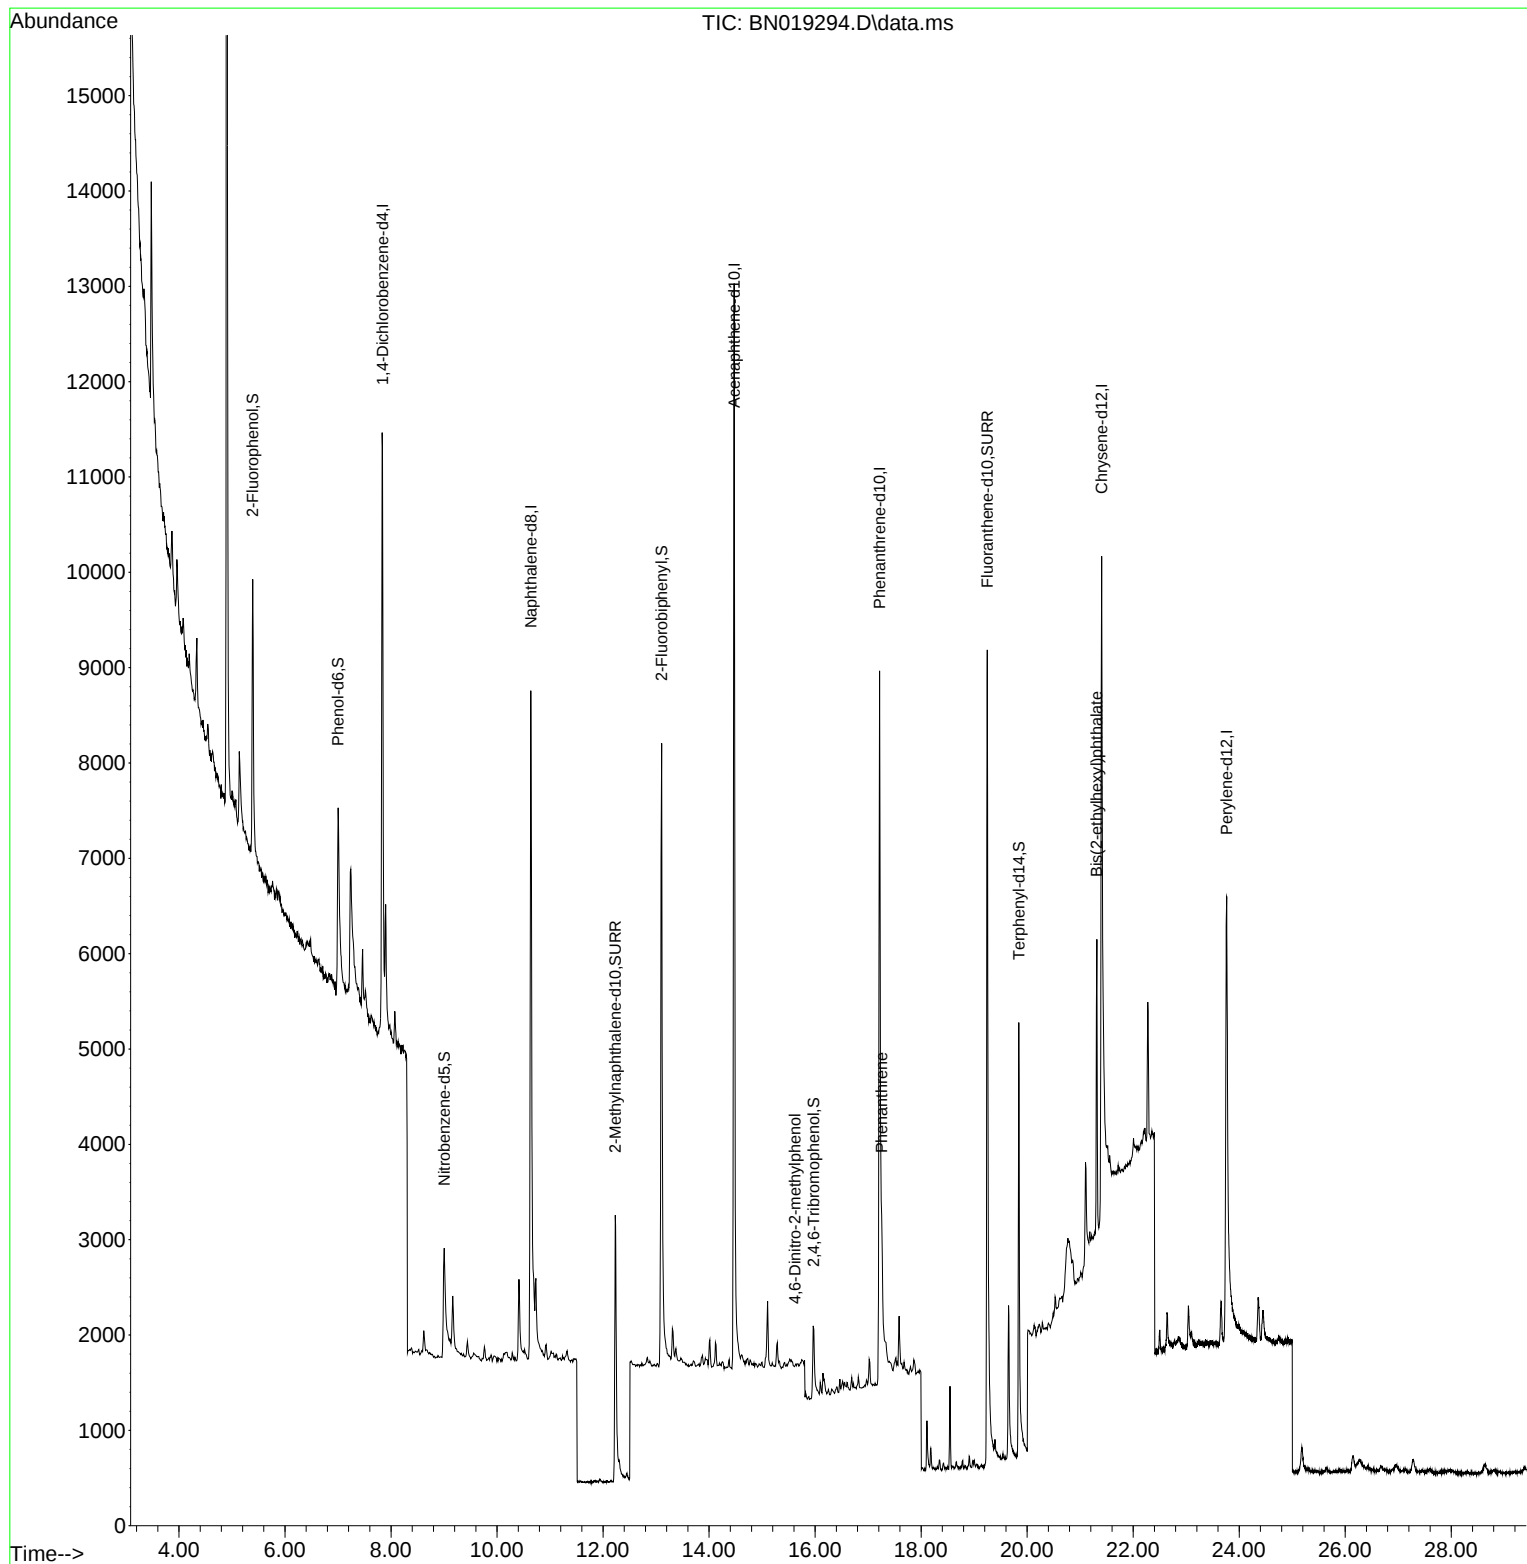



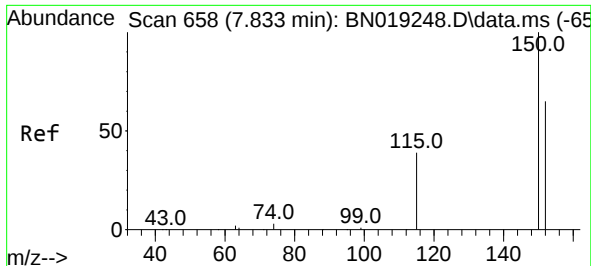


#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.840 min Scan# 61
Delta R.T. 0.007 min
Lab File: BN019294.D
Acq: 01 Apr 2022 19:08

Instrument :
BNA_N
ClientSampleId :
A04015



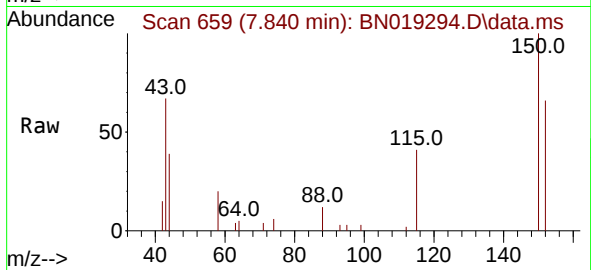



Tgt Ion:152 Resp: 3936
Ion Ratio Lower Upper
152 100
150 150.9 123.9 185.9
115 61.3 48.2 72.4

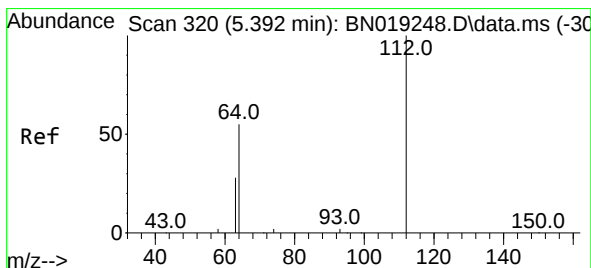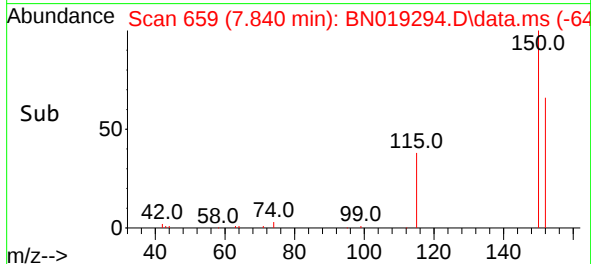

#4
2-Fluorophenol
Concen: 0.317 ng
RT: 5.392 min Scan# 320
Delta R.T. -0.000 min
Lab File: BN019294.D
Acq: 01 Apr 2022 19:08

Tgt Ion:112 Resp: 2729
Ion Ratio Lower Upper
112 100
64 65.2 47.8 71.8
63 34.8 25.7 38.5


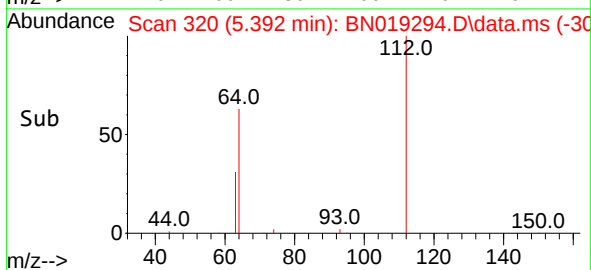

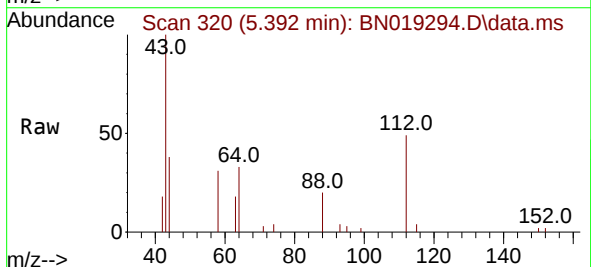


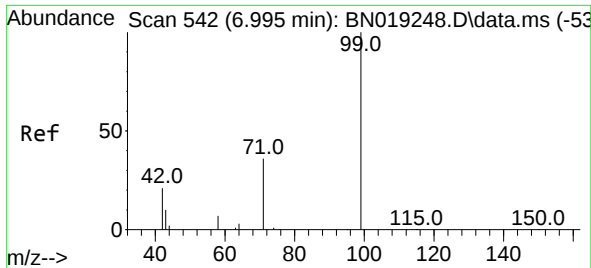

#5
Phenol-d6
Concen: 0.278 ng
RT: 7.002 min Scan# 542
Delta R.T. 0.007 min
Lab File: BN019294.D
Acq: 01 Apr 2022 19:08




Instrument :
BNA_N
ClientSampleId :
A04015


Tgt Ion: 99 Resp: 2539
Ion Ratio Lower Upper
99 100
42 21.3 16.2 24.4
71 36.7 27.7 41.5

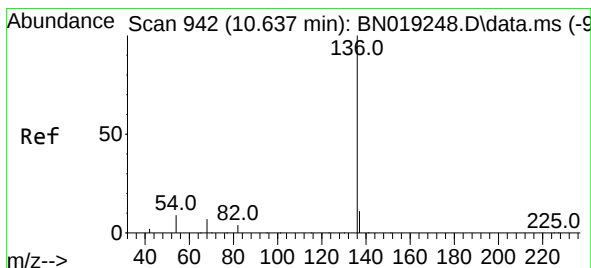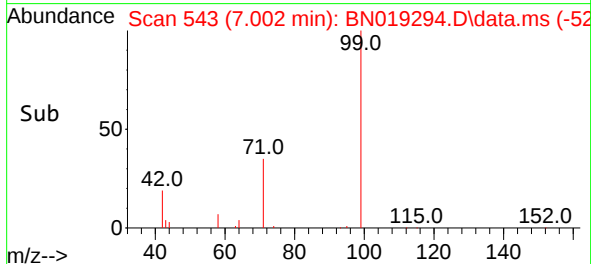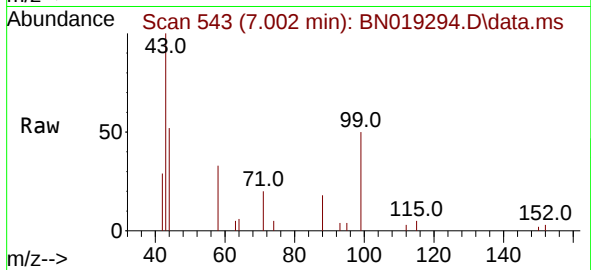

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.637 min Scan# 942
Delta R.T. -0.000 min
Lab File: BN019294.D
Acq: 01 Apr 2022 19:08

Tgt Ion: 136 Resp: 11556
Ion Ratio Lower Upper
136 100
137 11.8 9.0 13.4
54 11.2 5.8 8.6#
68 8.3 4.6 7.0#


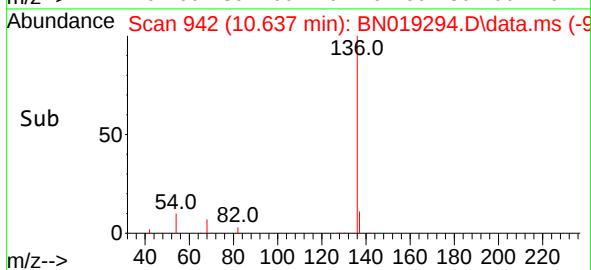

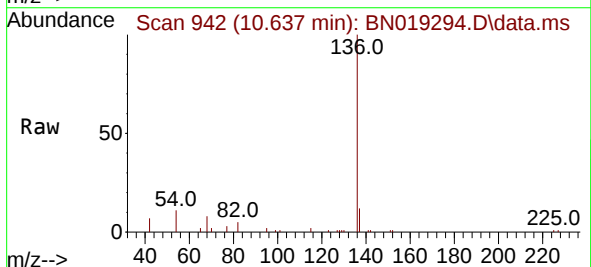


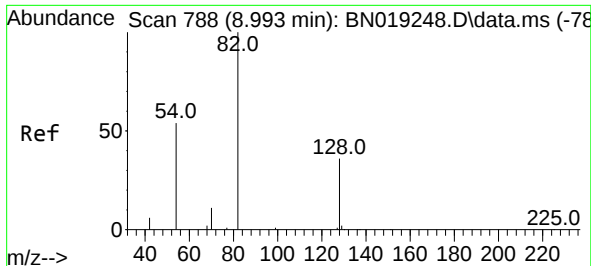

#8
Nitrobenzene-d5
Concen: 0.225 ng
RT: 9.003 min Scan# 788
Delta R.T. 0.011 min
Lab File: BN019294.D
Acq: 01 Apr 2022 19:08




Instrument :
BNA_N
ClientSampleId :
A04015


Tgt Ion: 82 Resp: 1871
Ion Ratio Lower Upper
82 100
128 43.1 33.0 49.6
54 59.6 42.5 63.7

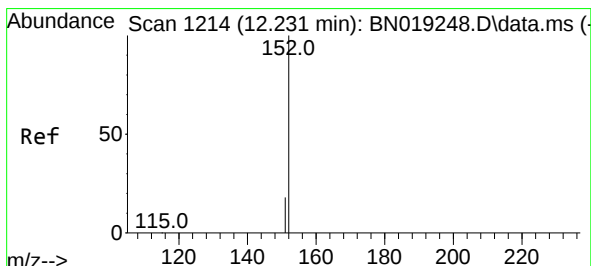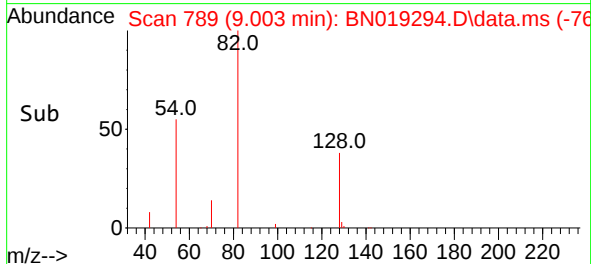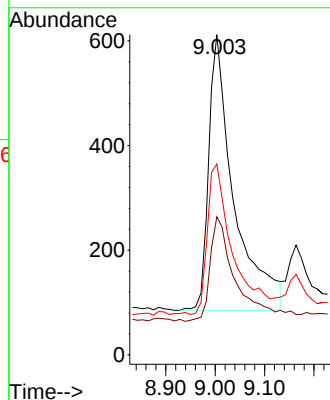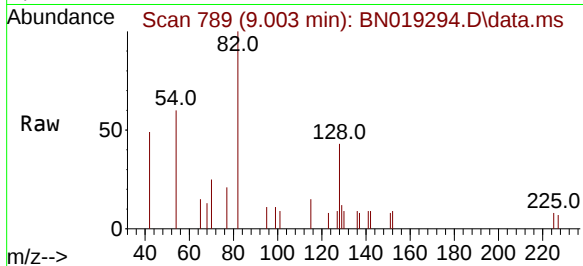

#11
2-Methylnaphthalene-d10
Concen: 0.286 ng
RT: 12.231 min Scan# 1214
Delta R.T. -0.000 min
Lab File: BN019294.D
Acq: 01 Apr 2022 19:08

Tgt Ion: 152 Resp: 5245
Ion Ratio Lower Upper
152 100
151 20.3 16.5 24.7


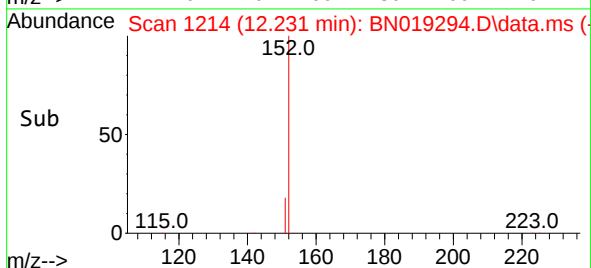
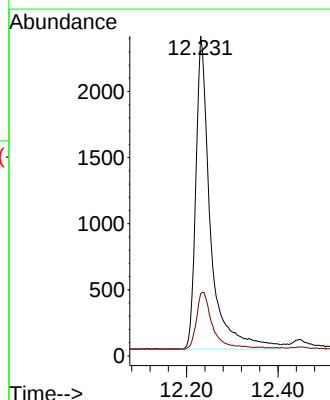
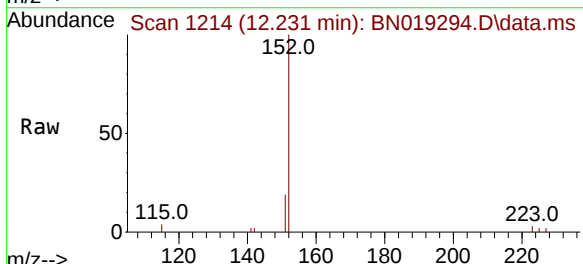


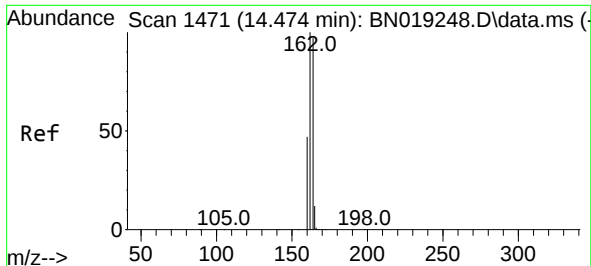

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.474 min Scan# 1471
Delta R.T. -0.000 min
Lab File: BN019294.D
Acq: 01 Apr 2022 19:08




Instrument :
BNA_N
ClientSampleId :
A04015


Tgt Ion:164 Resp: 7481
Ion Ratio Lower Upper
164 100
162 103.4 85.2 127.8
160 47.6 41.5 62.3

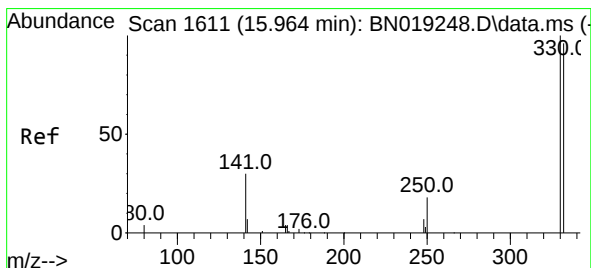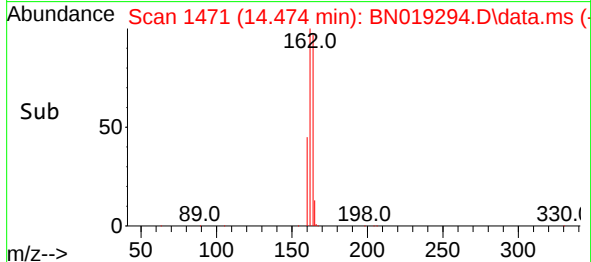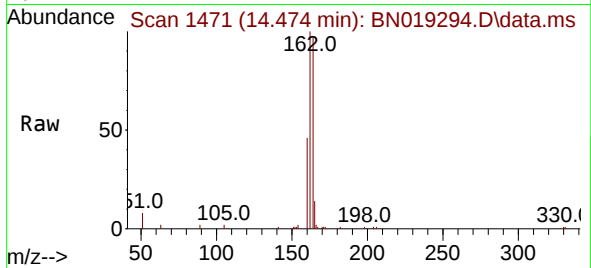

#14
2,4,6-Tribromophenol
Concen: 0.198 ng
RT: 15.974 min Scan# 1612
Delta R.T. 0.010 min
Lab File: BN019294.D
Acq: 01 Apr 2022 19:08

Tgt Ion:330 Resp: 693
Ion Ratio Lower Upper
330 100
332 92.9 76.8 115.2
141 42.0 32.2 48.2


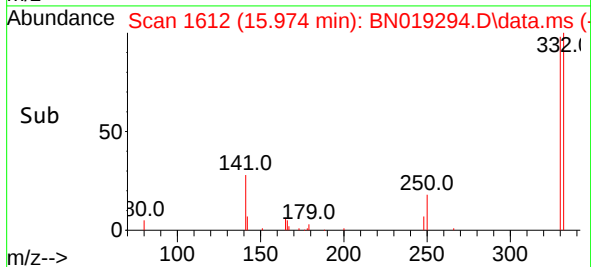

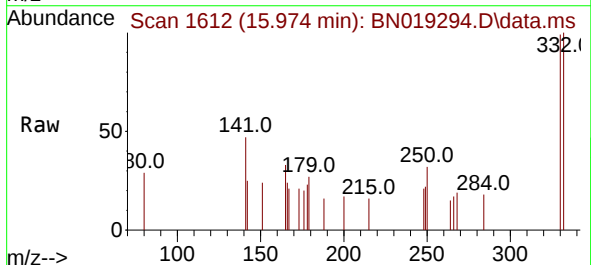


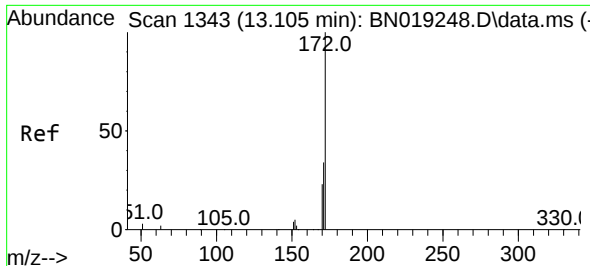

#15
2-Fluorobiphenyl
Concen: 0.240 ng
RT: 13.105 min Scan# 11
Delta R.T. -0.000 min
Lab File: BN019294.D
Acq: 01 Apr 2022 19:08




Instrument :
BNA_N
ClientSampleId :
A04015


Tgt Ion:172 Resp: 7209
Ion Ratio Lower Upper
172 100
171 35.2 28.2 42.2
170 22.9 18.7 28.1

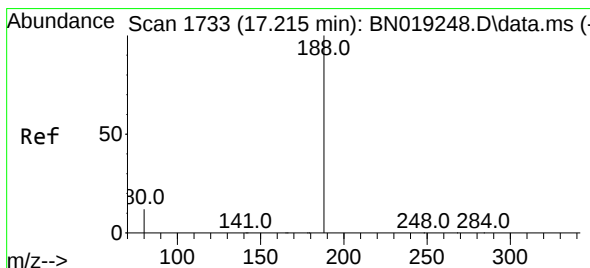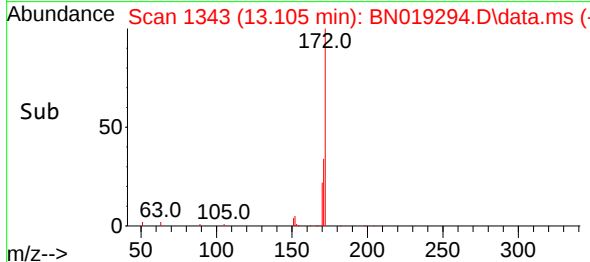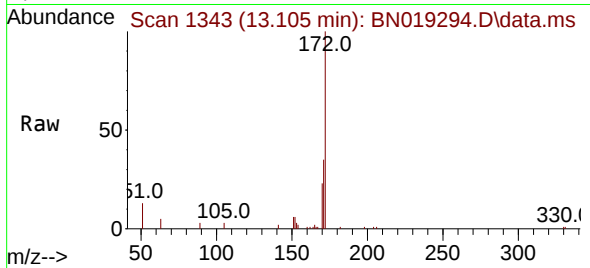

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.215 min Scan# 1733
Delta R.T. 0.000 min
Lab File: BN019294.D
Acq: 01 Apr 2022 19:08

Tgt Ion:188 Resp: 14795
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 13.7 11.8 17.8


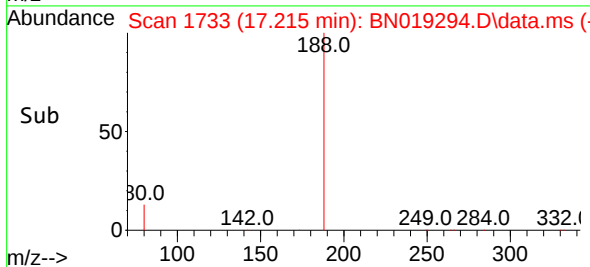

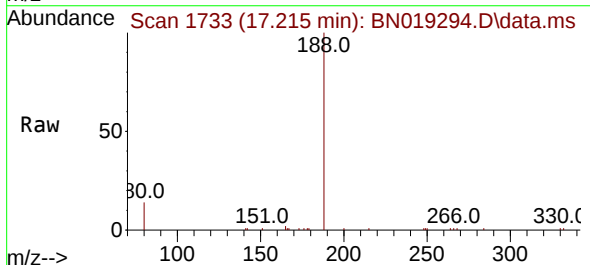


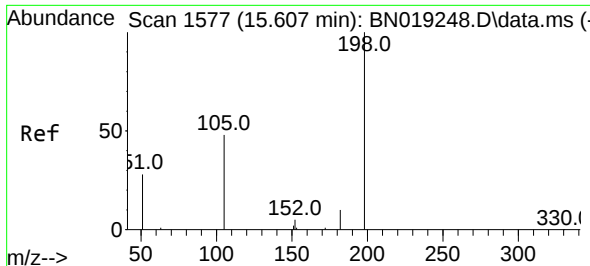

#20
4,6-Dinitro-2-methylphenol
Concen: 0.092 ng
RT: 15.618 min Scan# 1577
Delta R.T. 0.011 min
Lab File: BN019294.D
Acq: 01 Apr 2022 19:08




Instrument :
BNA_N
ClientSampleId :
A04015


Tgt Ion:198 Resp: 5
Ion Ratio Lower Upper
198 100
182 106.1 13.0 19.4#
77 0.0 0.0 0.0

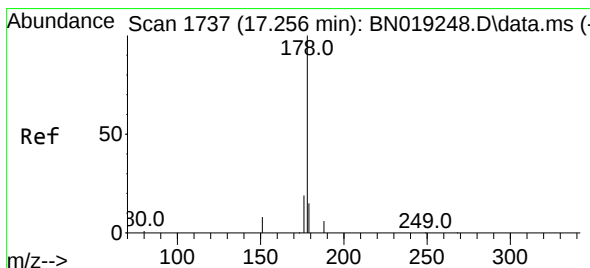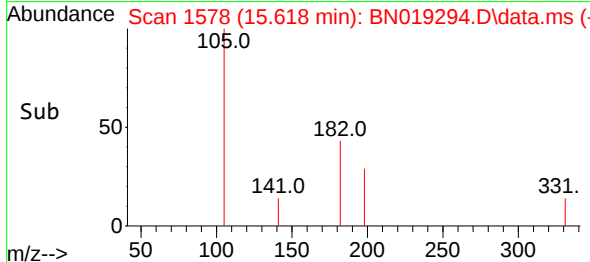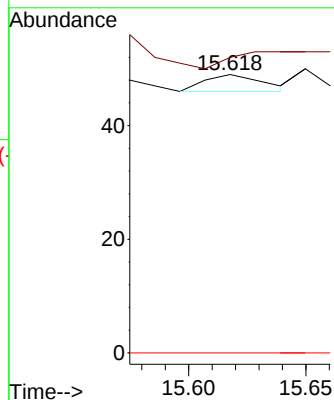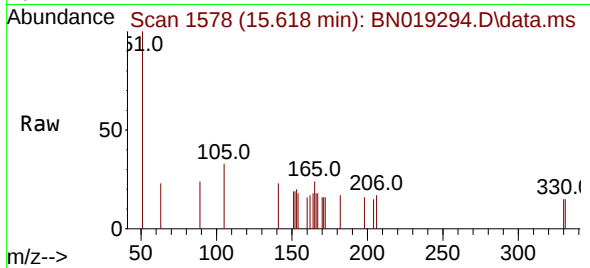

#25
Phenanthrene
Concen: 0.023 ng
RT: 17.256 min Scan# 1737
Delta R.T. -0.000 min
Lab File: BN019294.D
Acq: 01 Apr 2022 19:08

Tgt Ion:178 Resp: 1072
Ion Ratio Lower Upper
178 100
176 19.2 15.4 23.0
179 17.4 12.2 18.2


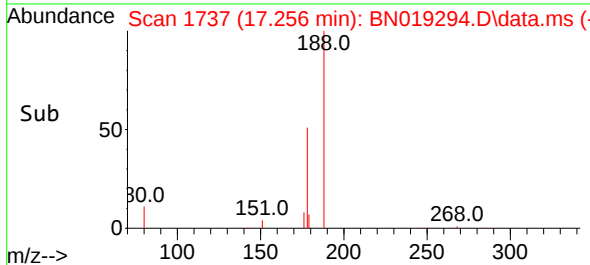
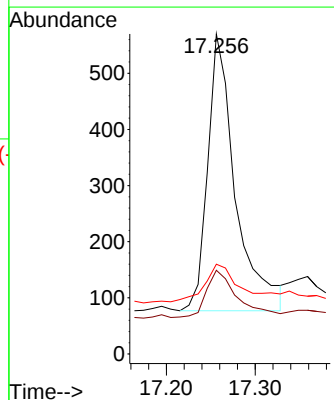
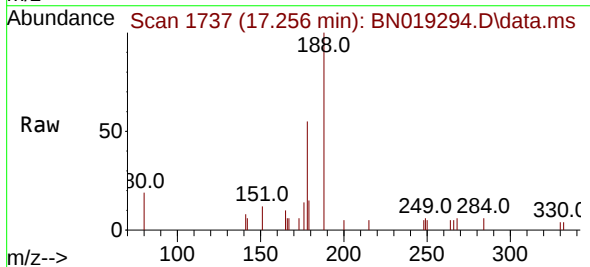


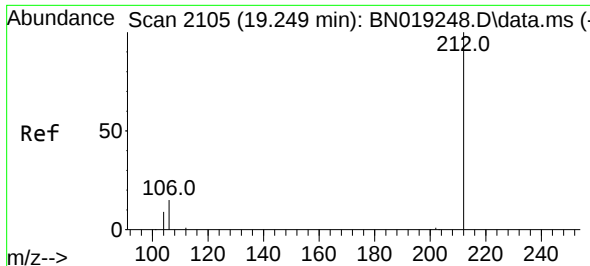

#27
Fluoranthene-d10
Concen: 0.285 ng
RT: 19.248 min Scan# 2105
Delta R.T. -0.000 min
Lab File: BN019294.D
Acq: 01 Apr 2022 19:08




Instrument :
BNA_N
ClientSampleId :
A04015


Tgt Ion:212 Resp: 12650
Ion Ratio Lower Upper
212 100
106 15.0 12.7 19.1
104 8.6 7.1 10.7

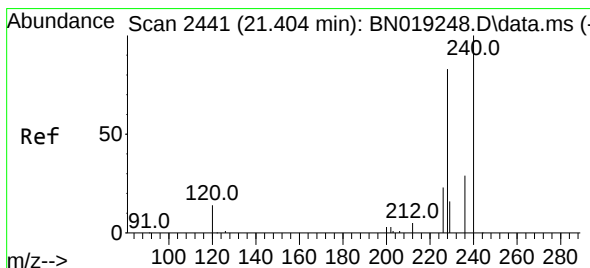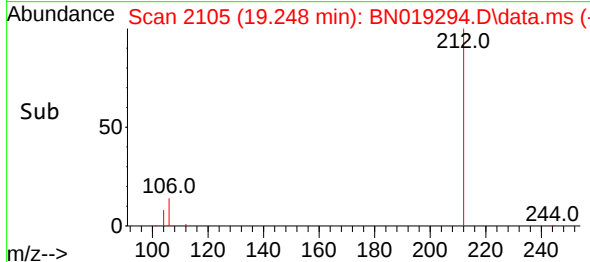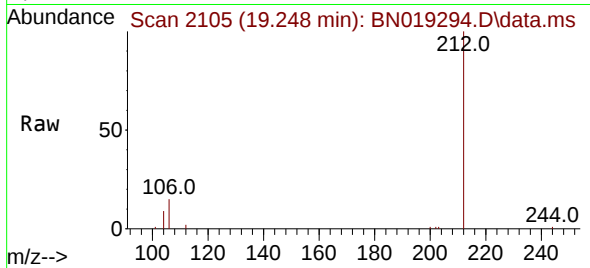

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.404 min Scan# 2441
Delta R.T. -0.000 min
Lab File: BN019294.D
Acq: 01 Apr 2022 19:08

Tgt Ion:240 Resp: 11882
Ion Ratio Lower Upper
240 100
120 16.2 8.5 12.7#
236 28.7 22.4 33.6


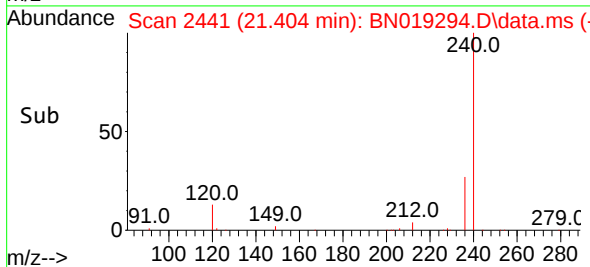

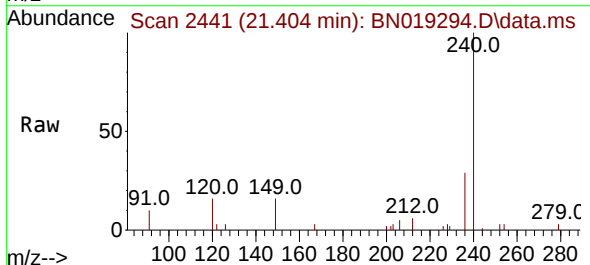


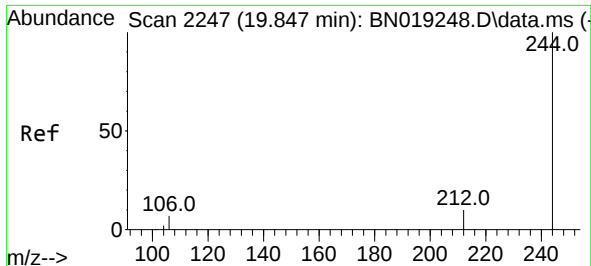

#31
 Terphenyl-d14
 Concen: 0.259 ng
 RT: 19.843 min Scan# 21
 Delta R.T. -0.004 min
 Lab File: BN019294.D
 Acq: 01 Apr 2022 19:08




Instrument :
 BNA_N
 ClientSampleId :
 A04015


Tgt Ion:244 Resp: 6839
 Ion Ratio Lower Upper
 244 100
 212 11.1 8.2 12.4
 122 0.0 0.0 0.0

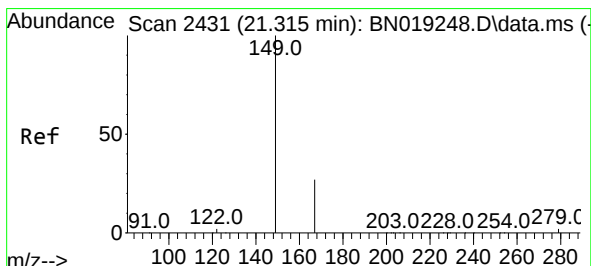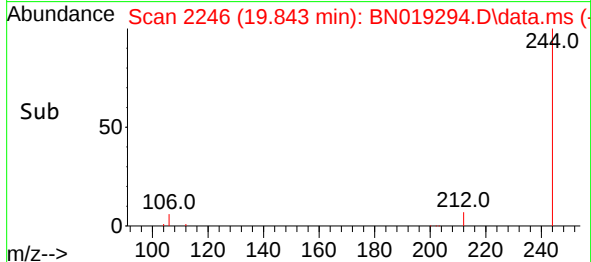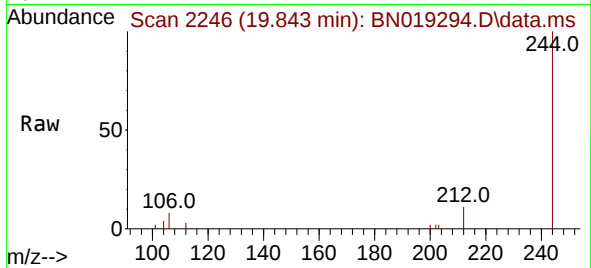

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.121 ng
 RT: 21.315 min Scan# 2431
 Delta R.T. -0.000 min
 Lab File: BN019294.D
 Acq: 01 Apr 2022 19:08

Tgt Ion:149 Resp: 3020
 Ion Ratio Lower Upper
 149 100
 167 27.5 21.8 32.8
 279 2.8 2.0 3.0

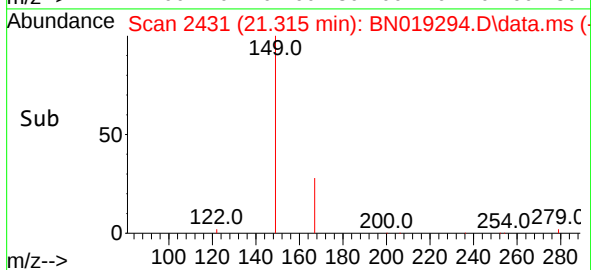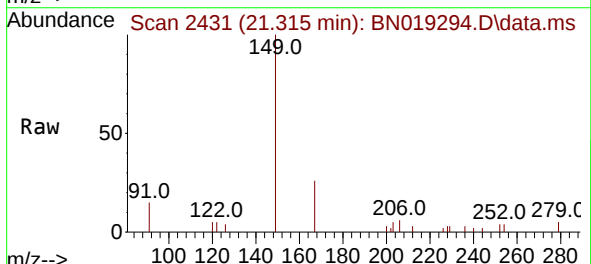

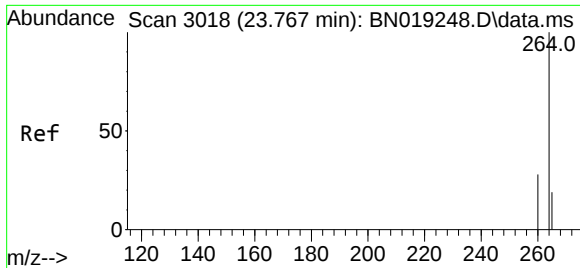

#35

Perylene-d12

Concen: 0.400 ng

RT: 23.764 min Scan# 30

Delta R.T. -0.003 min

Lab File: BN019294.D


Acq: 01 Apr 2022 19:08

Instrument :

BNA_N

ClientSampleId :

A04015

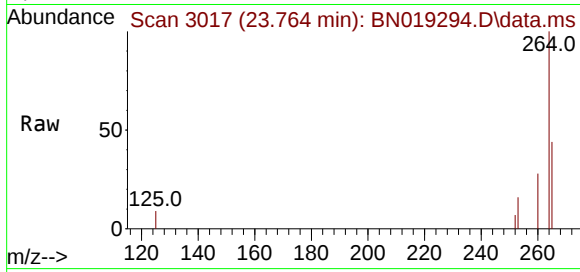

Tgt Ion:264 Resp: 9860

Ion Ratio Lower Upper

264 100

260 27.9 22.4 33.6

265 44.2 25.3 37.9#

