
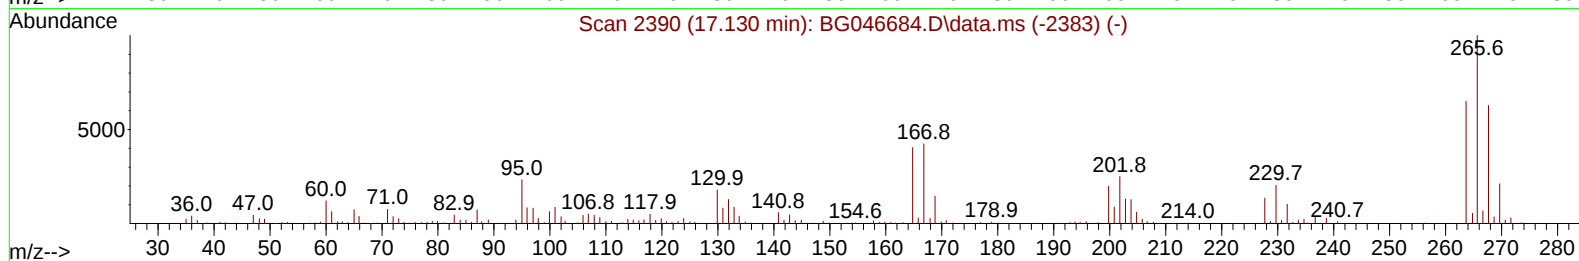
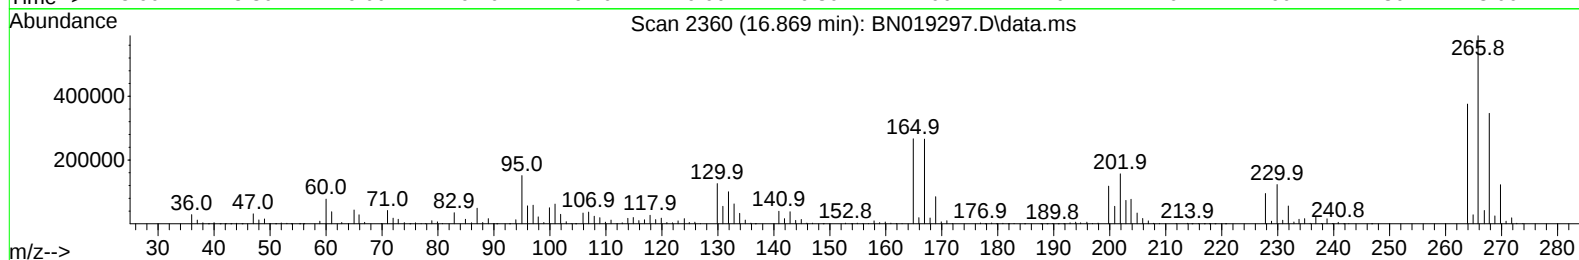


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033122\
 Data File : BN019297.D
 Acq On : 01 Apr 2022 21:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 02 02:16:40 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 23 16:56:32 2022
 Response via : Initial Calibration

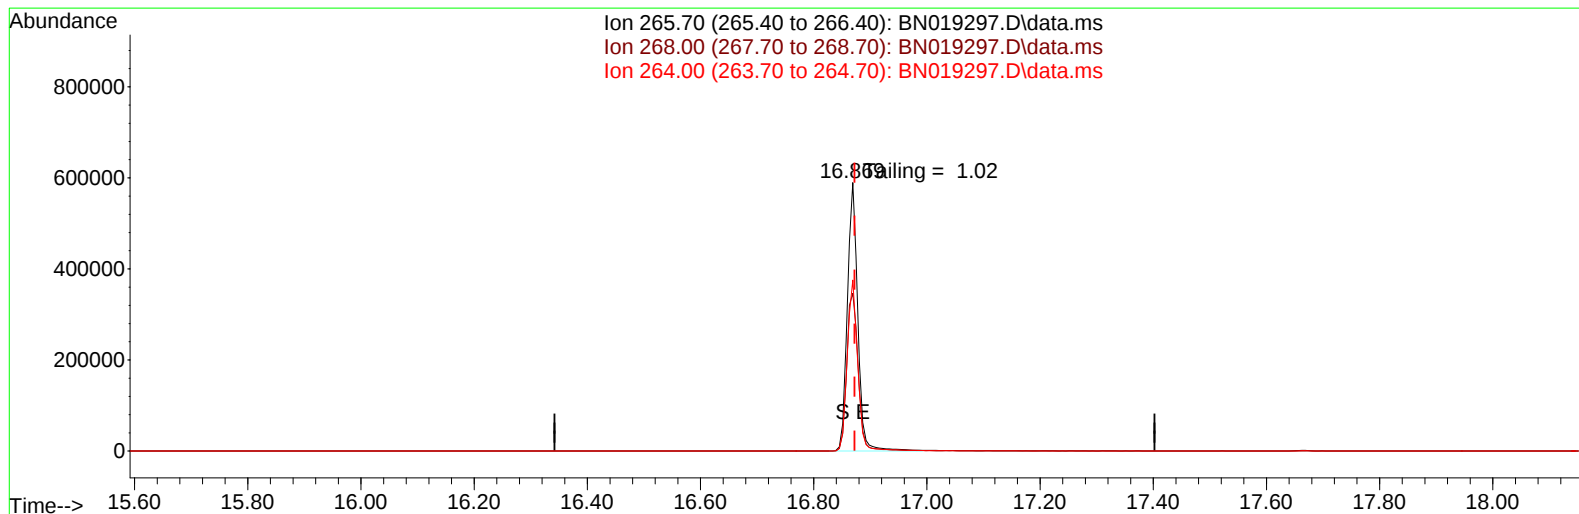

TIC: BN019297.D\data.ms

(70) Pentachlorophenol (C)




16.869min (-0.003) 21197.05 ng

response 761380

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	58.71
264.00	61.60	63.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033122\
Data File : BN019297.D
Acq On : 01 Apr 2022 21:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 02 02:16:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

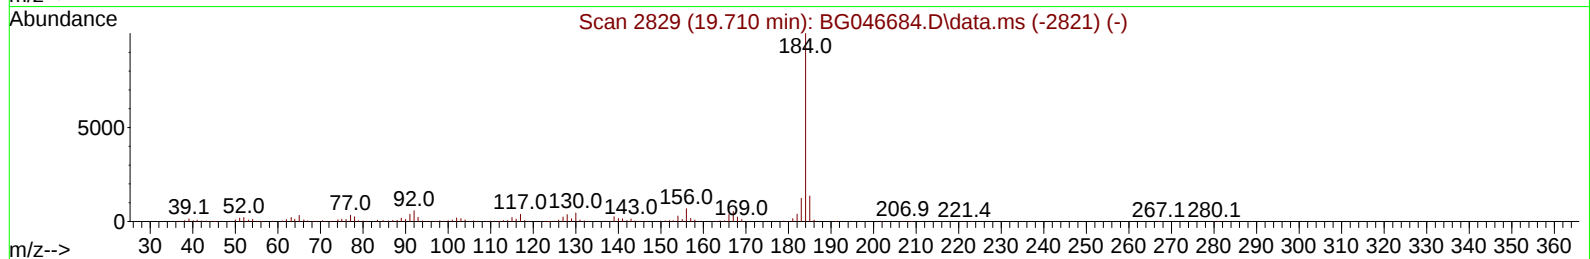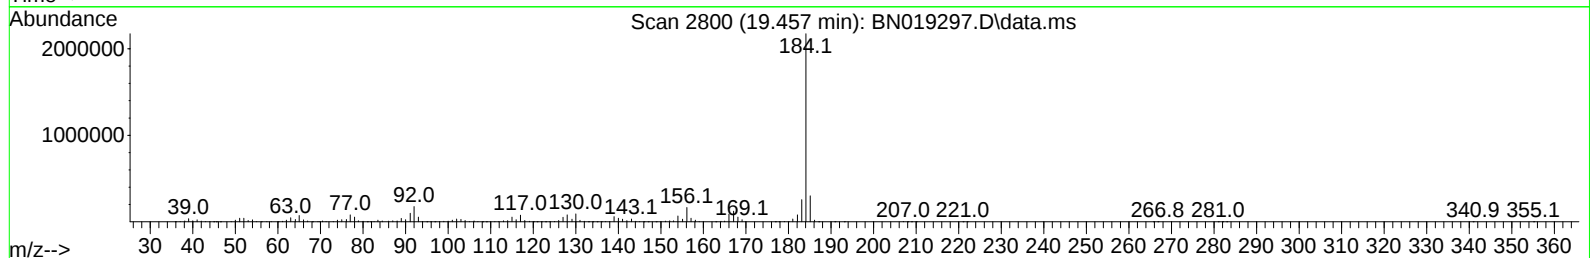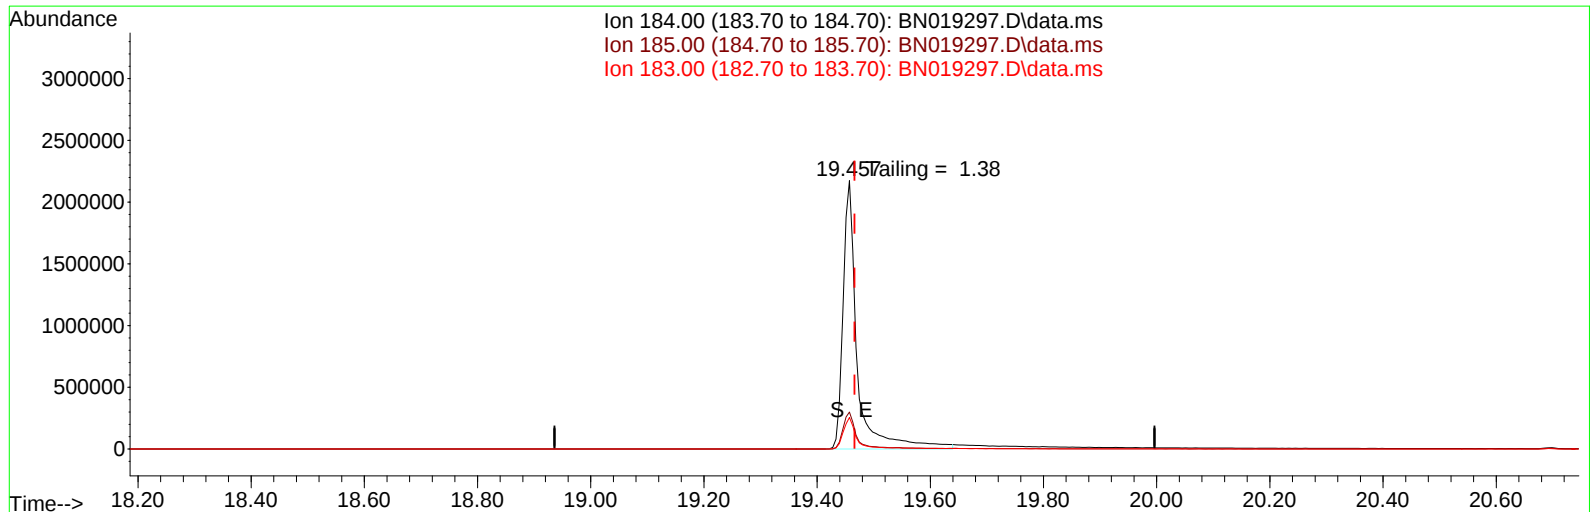

TIC: BN019297.D\data.ms

(77) Benzidine

19.457min (-0.009) 0.00 ng

response 3928217

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.81
183.00	13.20	11.79
0.00	0.00	0.00