


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033122\
 Data File : BN019245.D
 Acq On : 31 Mar 2022 07:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN033122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 31 12:41:03 2022

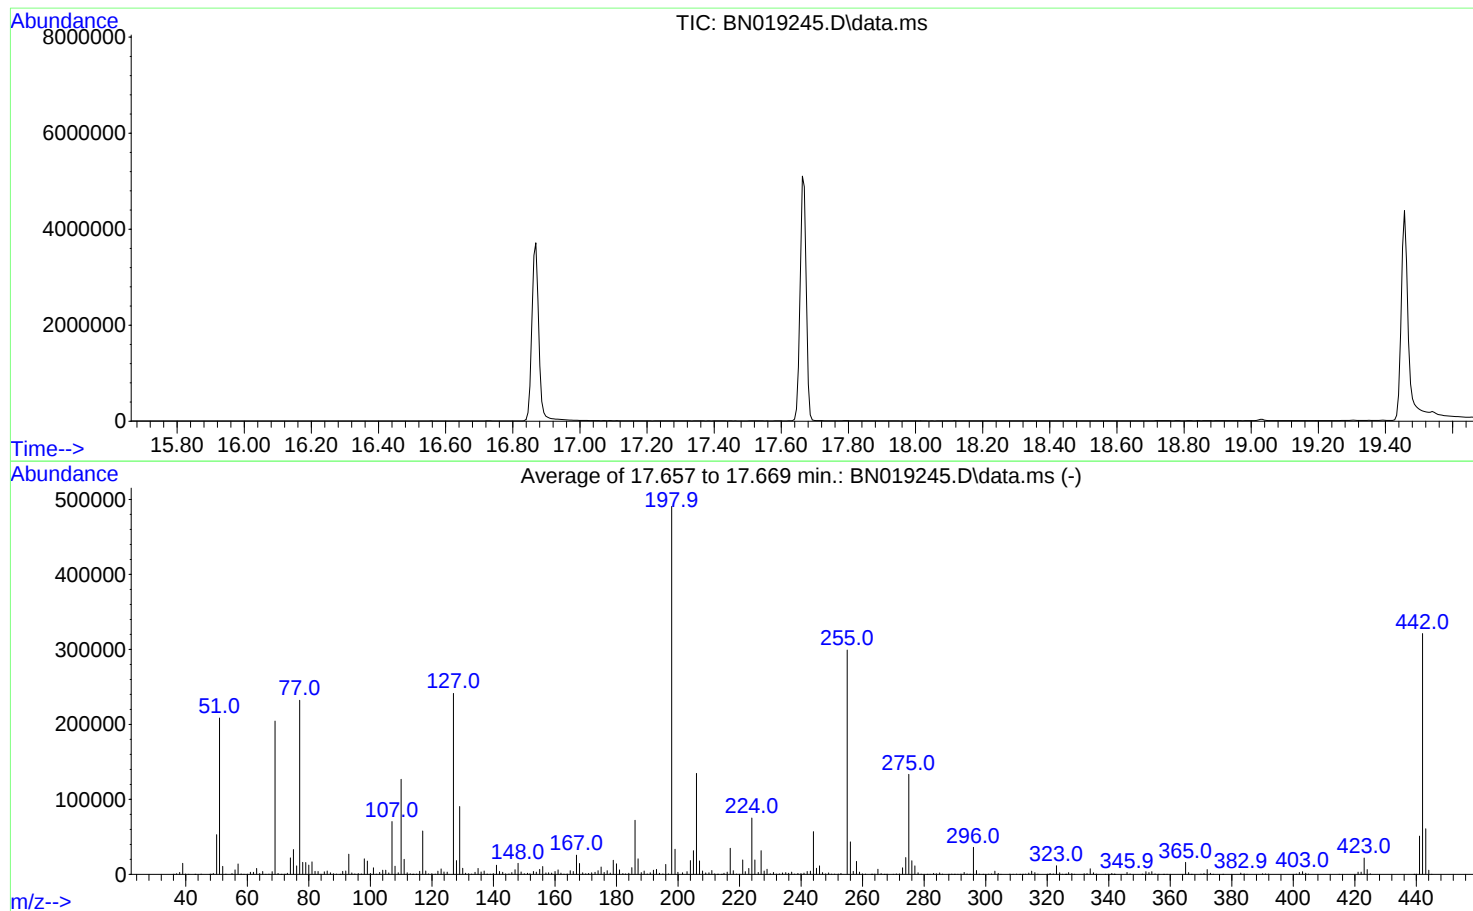




AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.5	208381	PASS
68	69	0.00	2	1.8	3627	PASS
69	198	0.00	100	41.7	204459	PASS
70	69	0.00	2	0.6	1218	PASS
127	198	10	80	49.2	241429	PASS
197	198	0.00	2	0.1	624	PASS
198	198	100	100	100.0	490560	PASS
199	198	5	9	6.8	33557	PASS
275	198	10	60	27.2	133288	PASS
365	198	1	100	3.3	15997	PASS
441	198	0.01	100	10.4	51008	PASS
442	442	50	100	100.0	321045	PASS
443	442	15	24	19.0	60864	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033122\
 Data File : BN019245.D
 Acq On : 31 Mar 2022 07:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Mar 31 12:05:24 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 23 16:56:32 2022
 Response via : Initial Calibration

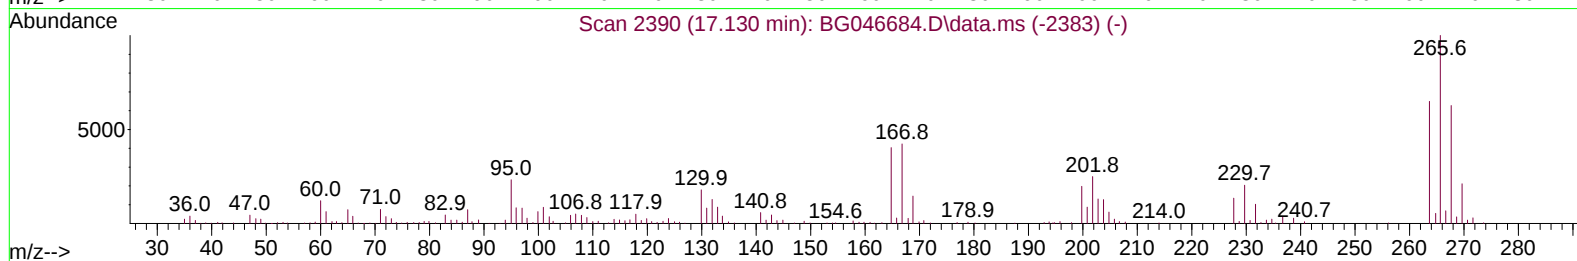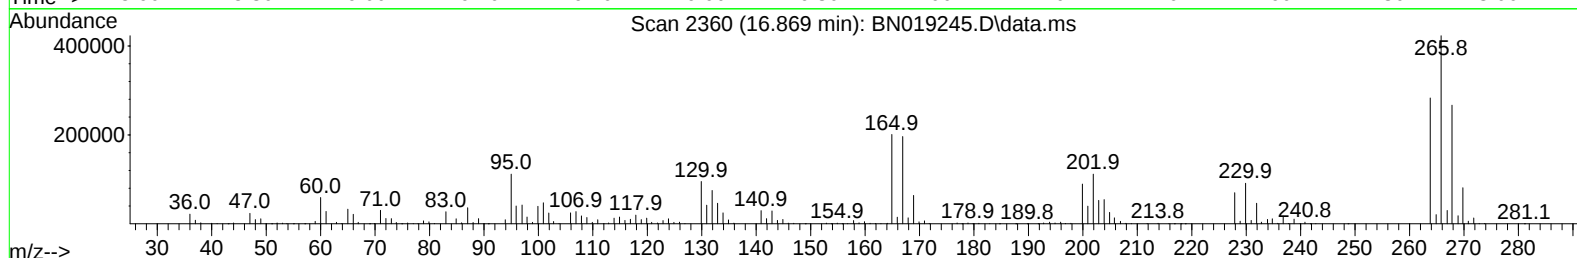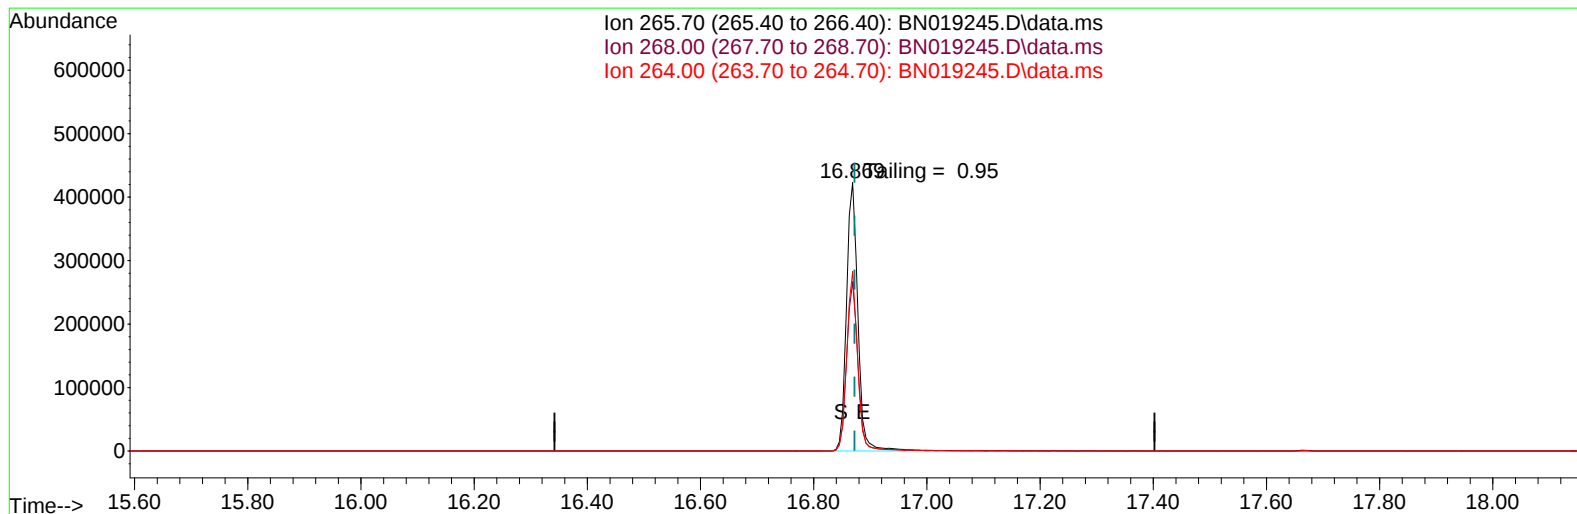

TIC: BN019245.D\data.ms

(70) Pentachlorophenol (C)

16.869min (-0.003) 22843.55 ng




response 597867

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.08
264.00	61.60	66.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033122\
 Data File : BN019245.D
 Acq On : 31 Mar 2022 07:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Mar 31 12:05:24 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 23 16:56:32 2022
 Response via : Initial Calibration

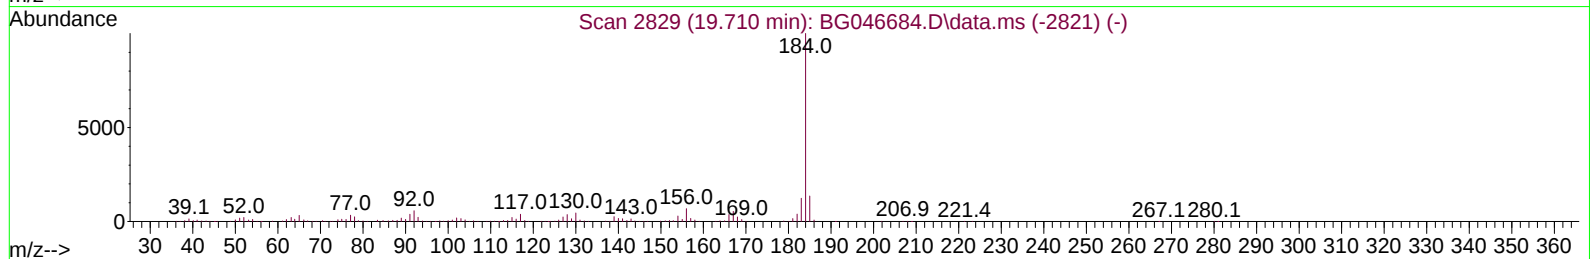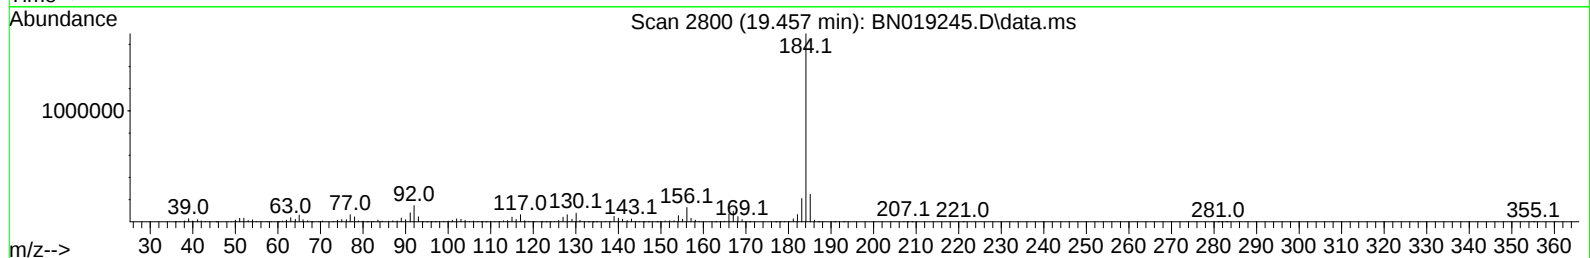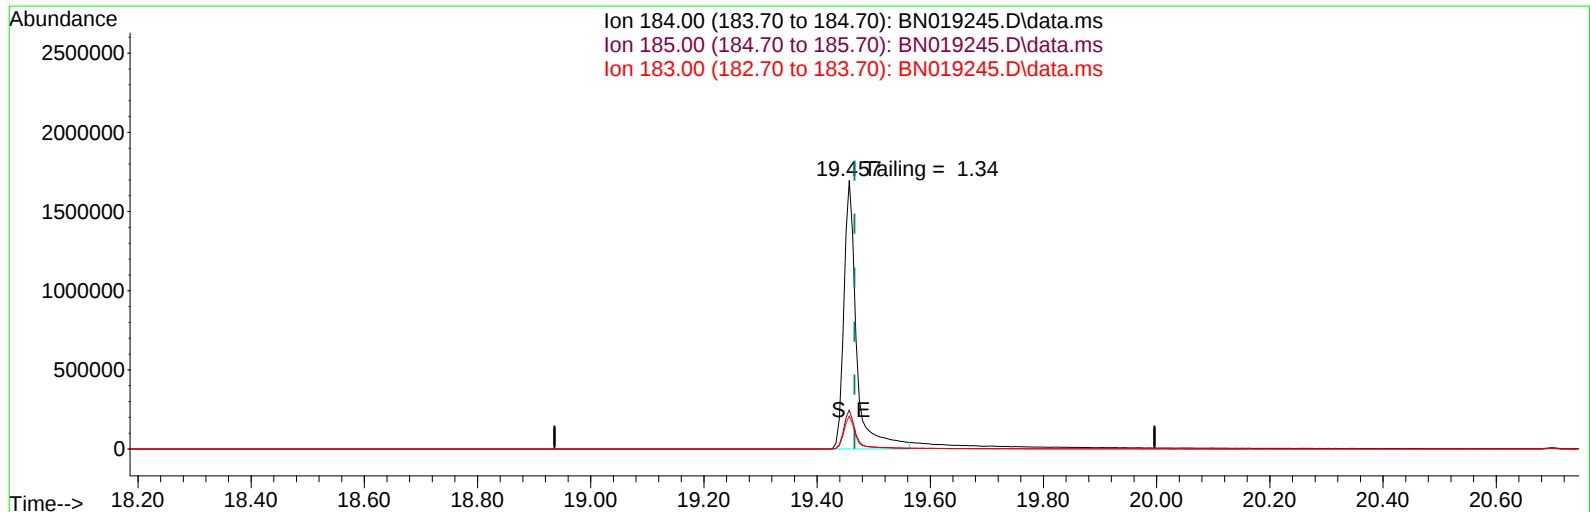

TIC: BN019245.D\data.ms

(77) Benzidine

19.457min (-0.009) 0.00 ng

response 2874559

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.61
183.00	13.20	12.38
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/31/2022	BNA_N	<u>BN019245.D</u>
Compound Name	Response	Retention Time
DDT	1772851	20.69
DDD	13572	20.25
DDE	1646	19.75
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15218	1788069	0.85

Instrument :
BNA_N
ClientSampleId :
DFTPP