
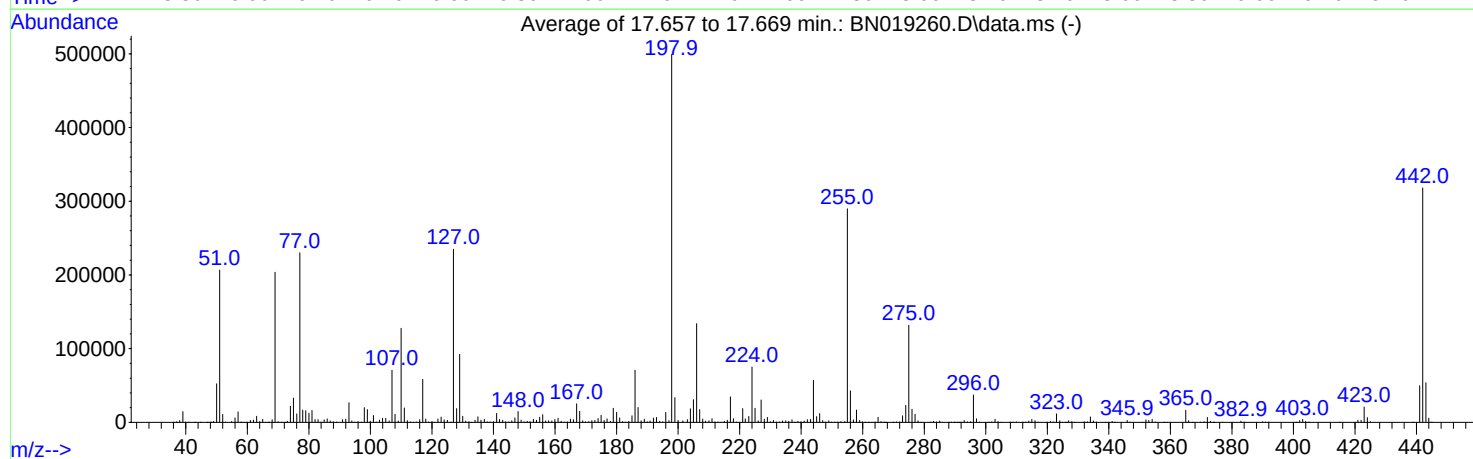


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033122\
 Data File : BN019260.D
 Acq On : 31 Mar 2022 20:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN033122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 31 12:41:03 2022

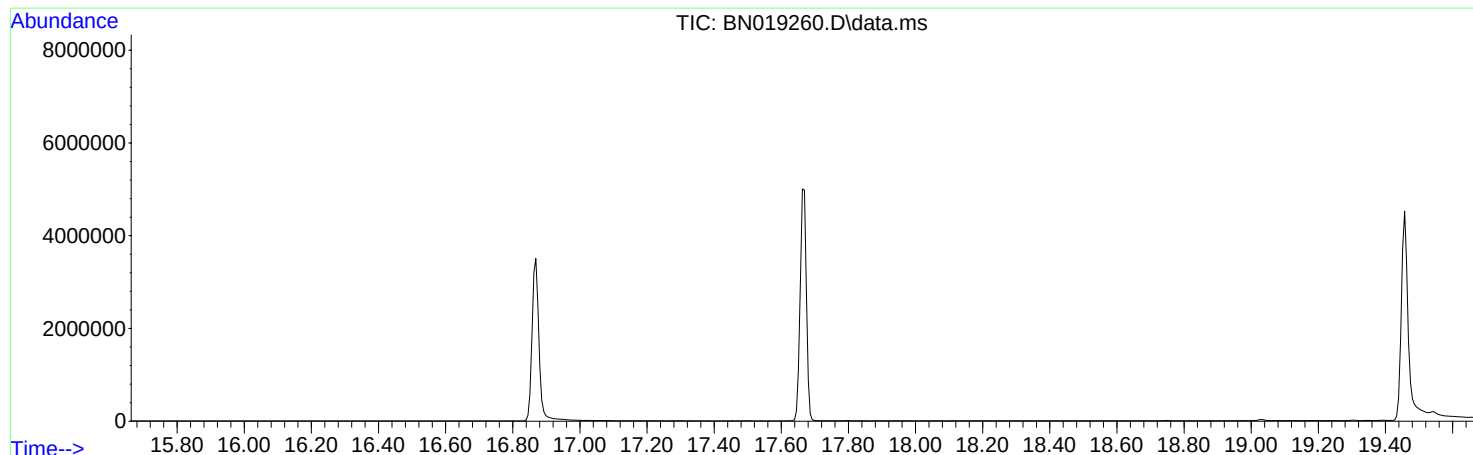




AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.4	206733	PASS
68	69	0.00	2	1.8	3761	PASS
69	198	0.00	100	40.8	203584	PASS
70	69	0.00	2	0.5	1114	PASS
127	198	10	80	47.1	234901	PASS
197	198	0.00	2	0.5	2500	PASS
198	198	100	100	100.0	499072	PASS
199	198	5	9	6.7	33581	PASS
275	198	10	60	26.4	131683	PASS
365	198	1	100	3.3	16444	PASS
441	198	0.01	100	10.0	49733	PASS
442	442	50	100	100.0	317973	PASS
443	442	15	24	17.0	53939	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033122\
Data File : BN019260.D
Acq On : 31 Mar 2022 20:05
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 01 06:10:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

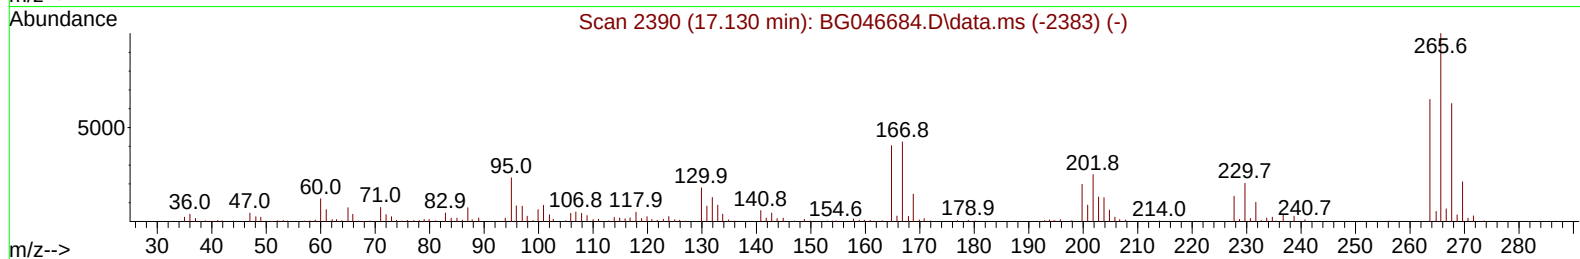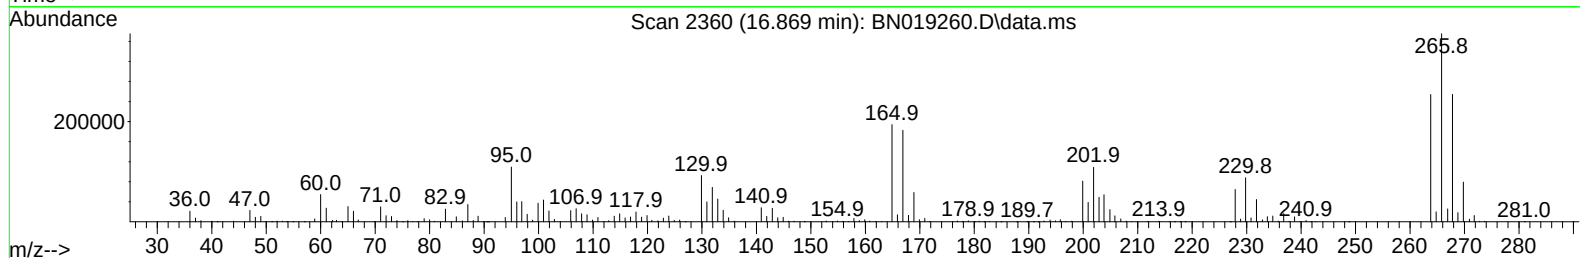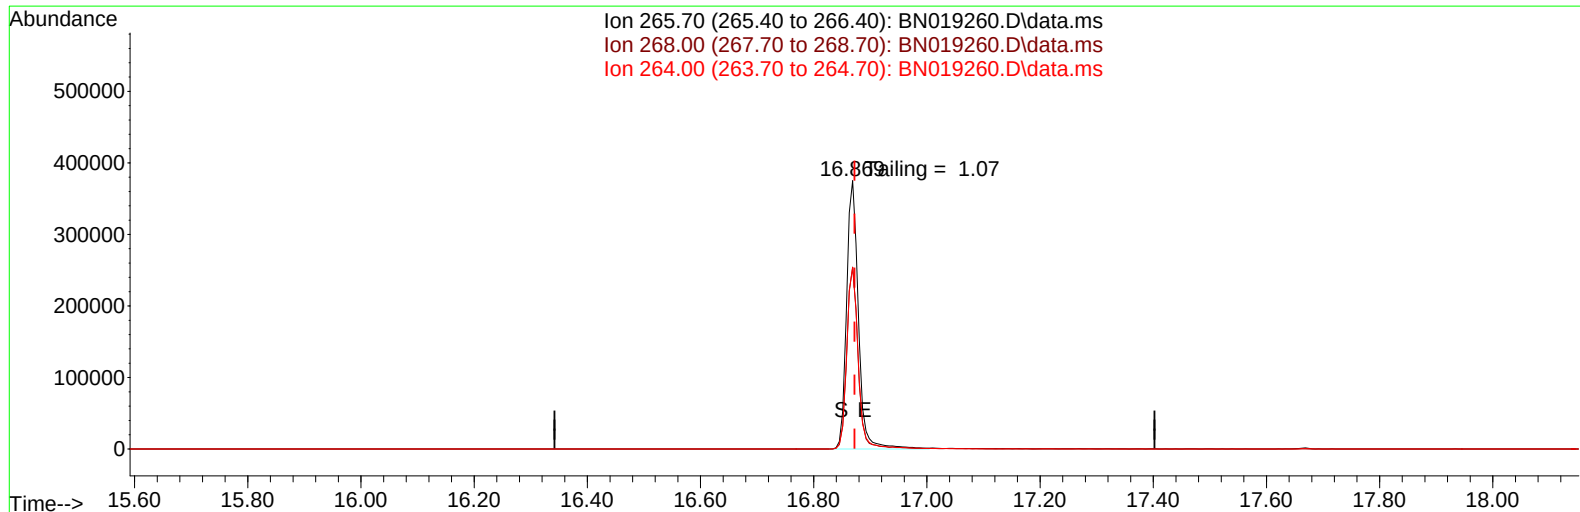

TIC: BN019260.D\data.ms

(70) Pentachlorophenol (C)

16.869min (-0.003) 21778.23 ng




response 549134

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	67.80
264.00	61.60	67.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033122\
Data File : BN019260.D
Acq On : 31 Mar 2022 20:05
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 01 06:10:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

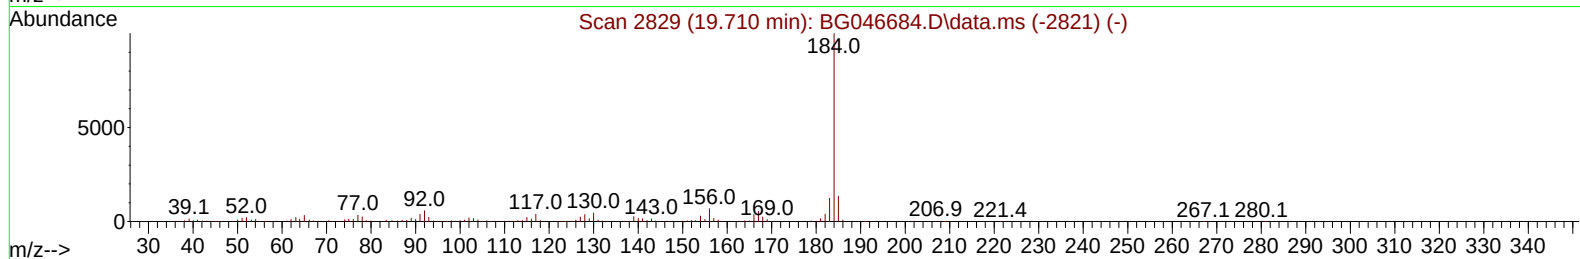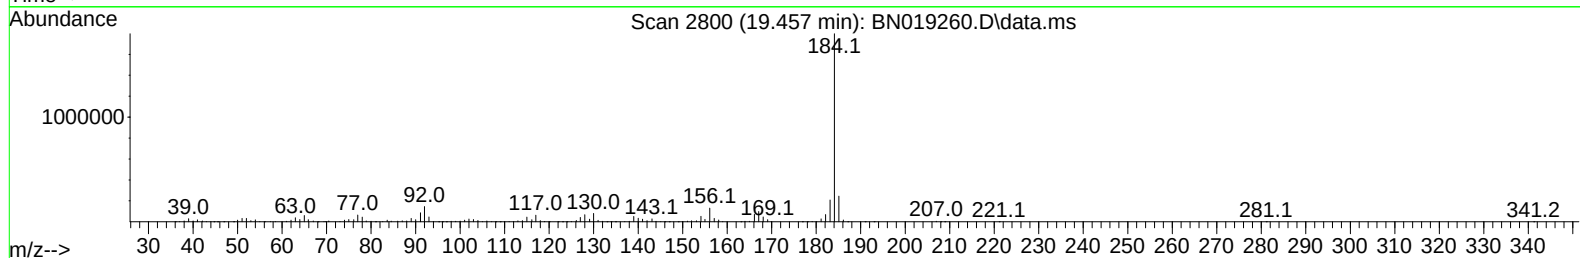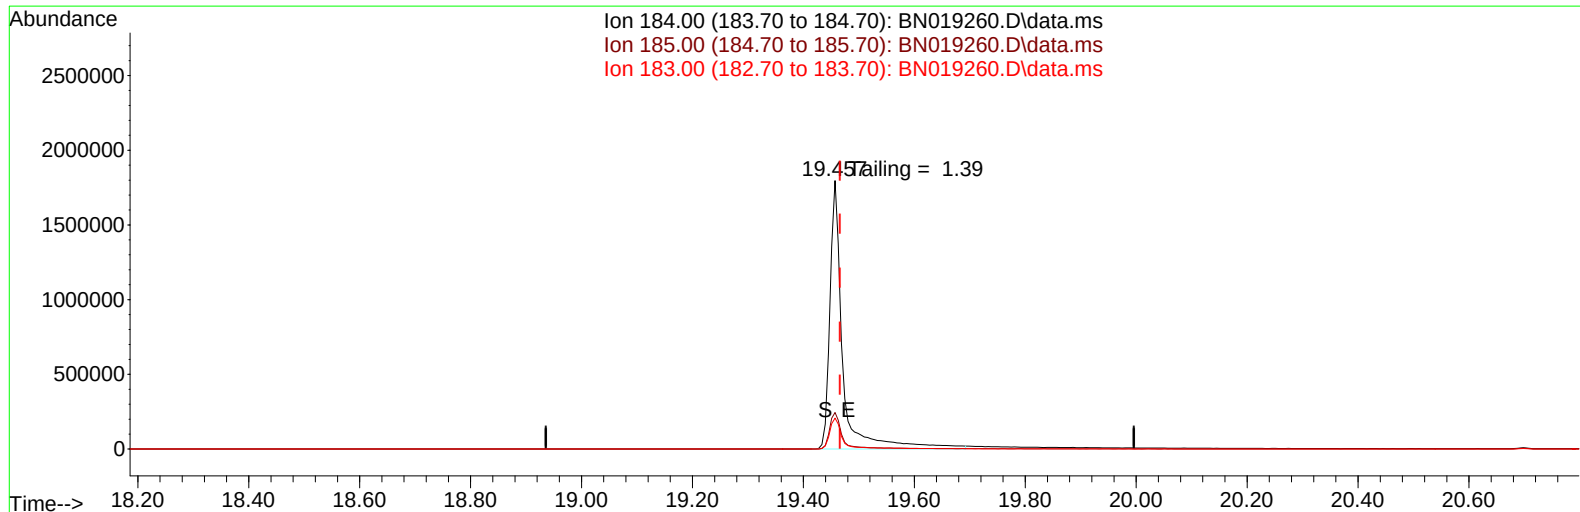

TIC: BN019260.D\data.ms

(77) Benzidine

19.457min (-0.009) 0.00 ng

response 3014587

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.63
183.00	13.20	11.55
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/31/2022	BNA_N	<u>BN019260.D</u>
Compound Name	Response	Retention Time
DDT	1818689	20.698
DDD	27366	20.257
DDE	1730	19.751
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
29096	1847785	1.57

Instrument :
BNA_N
ClientSampleId :
DFTPP