
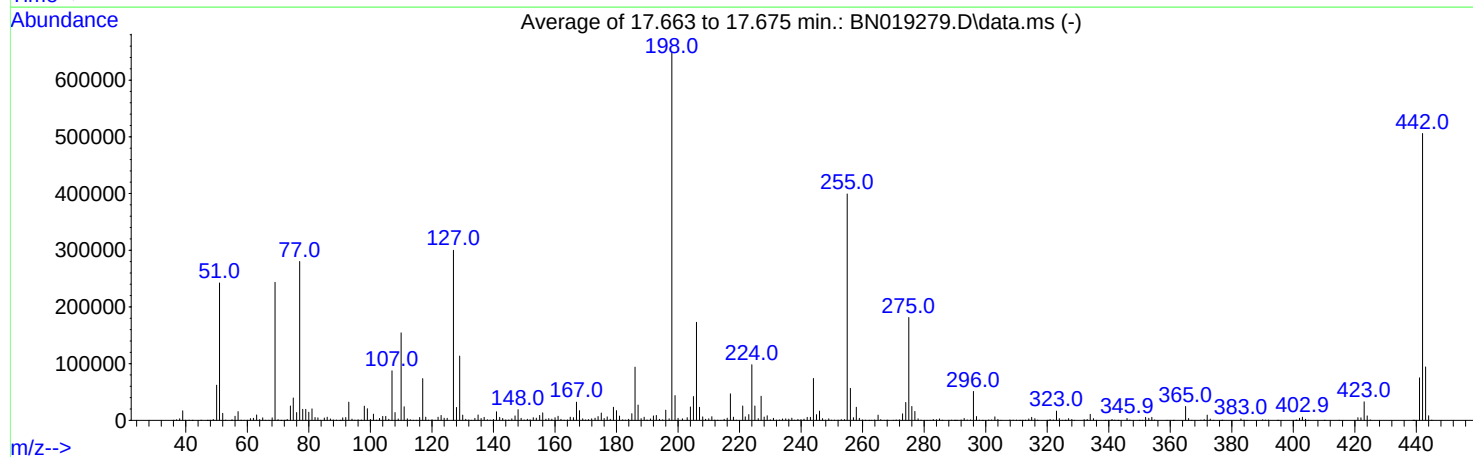


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033122\
 Data File : BN019279.D
 Acq On : 01 Apr 2022 09:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN033122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 31 12:41:03 2022

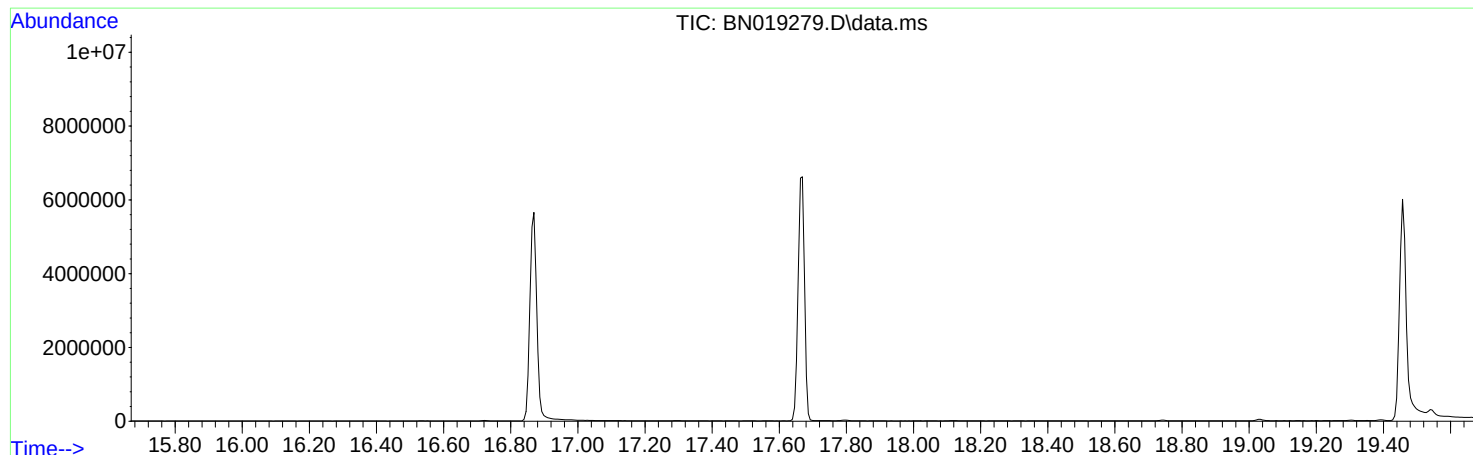




AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.4	242449	PASS
68	69	0.00	2	1.9	4663	PASS
69	198	0.00	100	37.5	243584	PASS
70	69	0.00	2	0.6	1376	PASS
127	198	10	80	46.2	299968	PASS
197	198	0.00	2	0.4	2919	PASS
198	198	100	100	100.0	648704	PASS
199	198	5	9	6.7	43776	PASS
275	198	10	60	28.0	181376	PASS
365	198	1	100	3.8	24501	PASS
441	198	0.01	100	11.6	75016	PASS
442	442	50	100	100.0	505813	PASS
443	442	15	24	18.6	94272	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033122\
 Data File : BN019279.D
 Acq On : 01 Apr 2022 09:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Apr 01 16:37:47 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 23 16:56:32 2022
 Response via : Initial Calibration

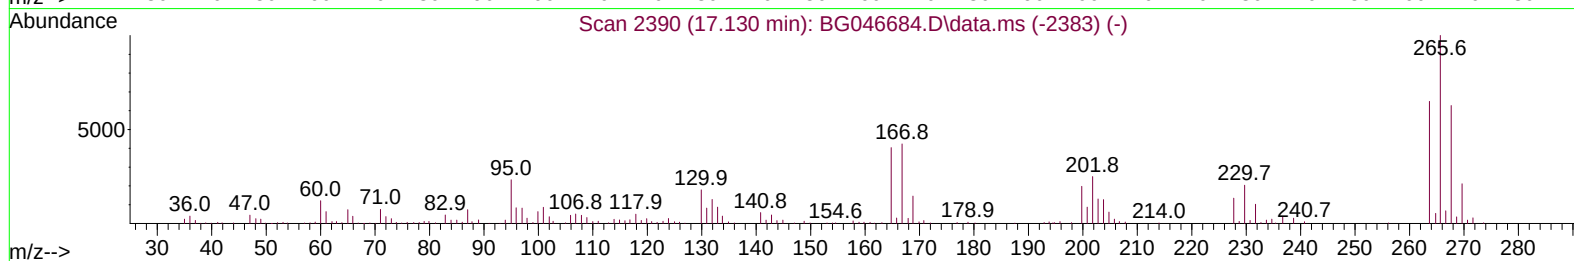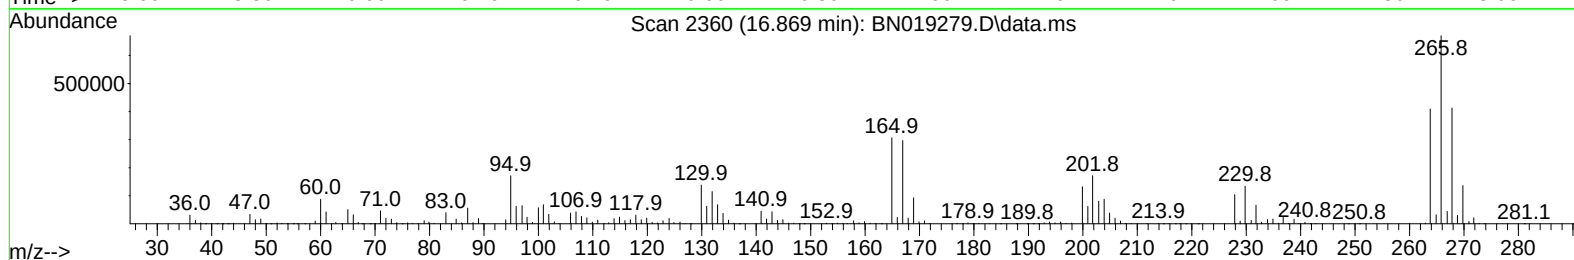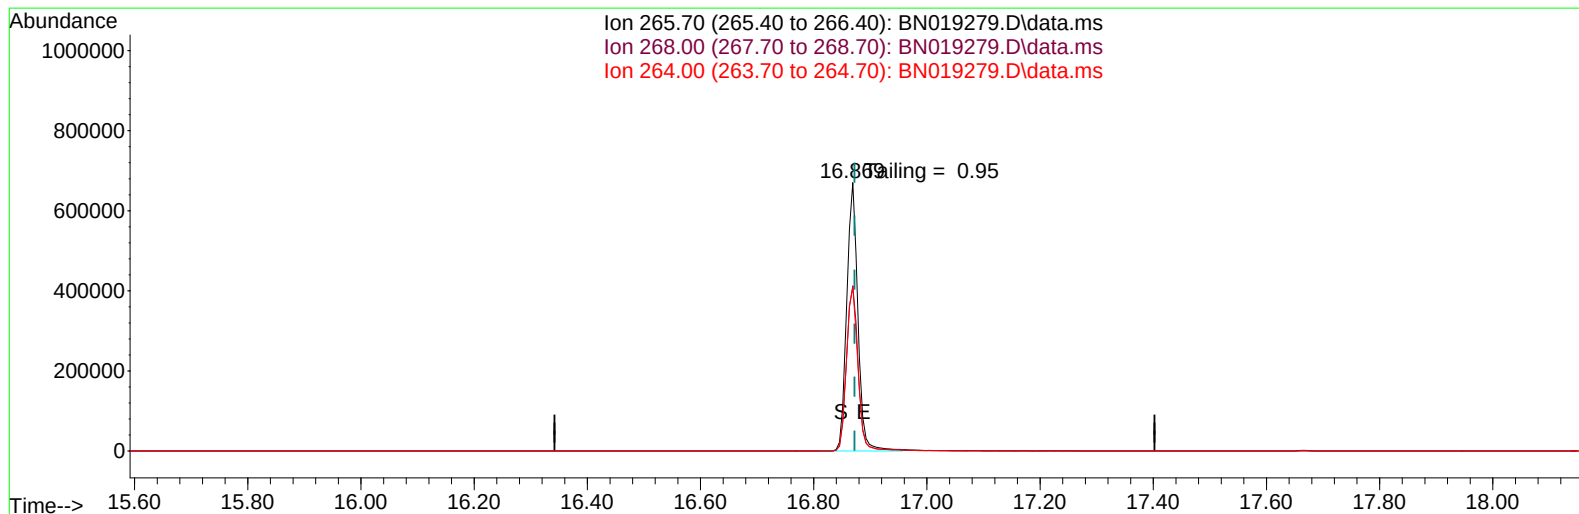

TIC: BN019279.D\data.ms

(70) Pentachlorophenol (C)

16.869min (-0.003) 24783.07 ng




response 931030

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.55
264.00	61.60	61.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033122\
Data File : BN019279.D
Acq On : 01 Apr 2022 09:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 01 16:37:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

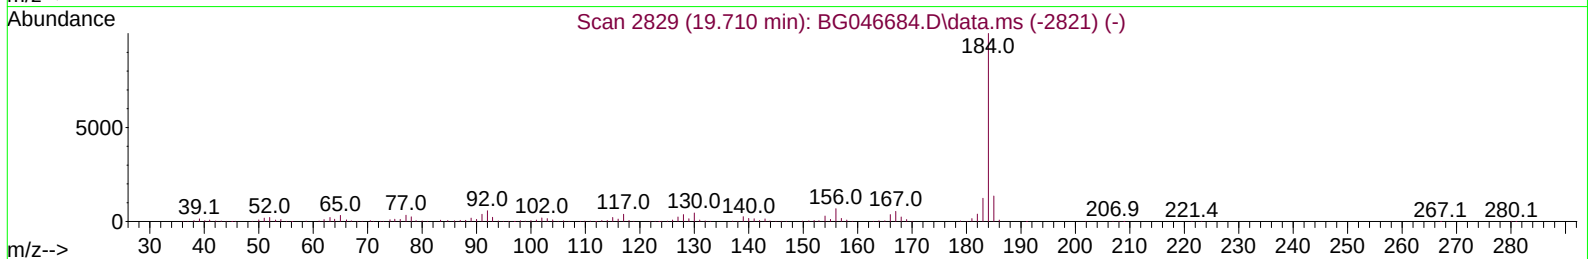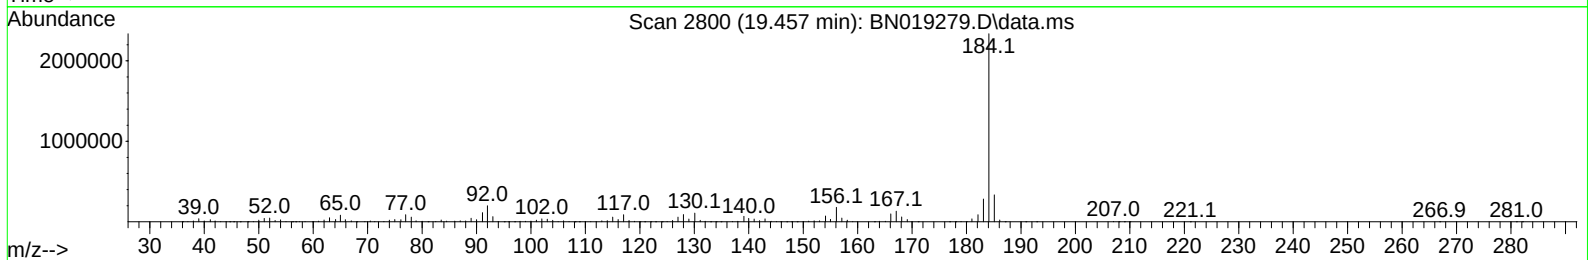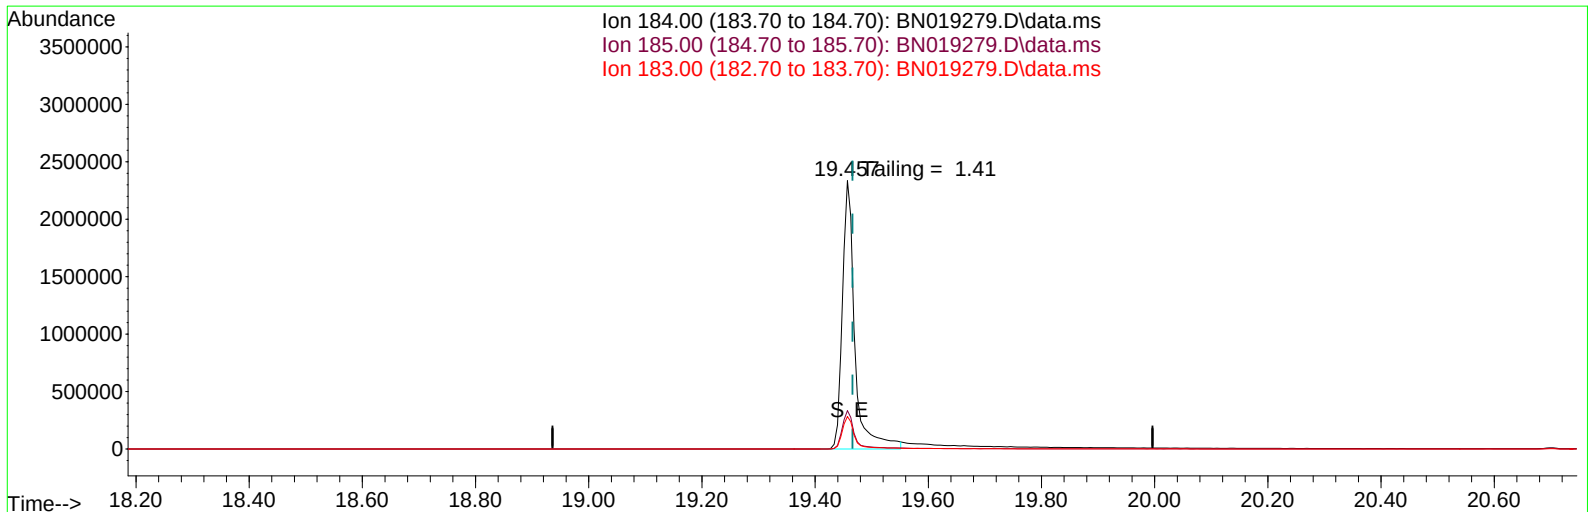

TIC: BN019279.D\data.ms

(77) Benzidine

19.457min (-0.009) 0.00 ng

response 3907303

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.31
183.00	13.20	12.09
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/31/2022	BNA_N	<u>BN019279.D</u>
Compound Name	Response	Retention Time
DDT	2414897	20.69
DDD	39746	20.25
DDE	2014	19.75
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
41760	2456657	1.70

Instrument :
BNA_N
ClientSampleId :
DFTPP