
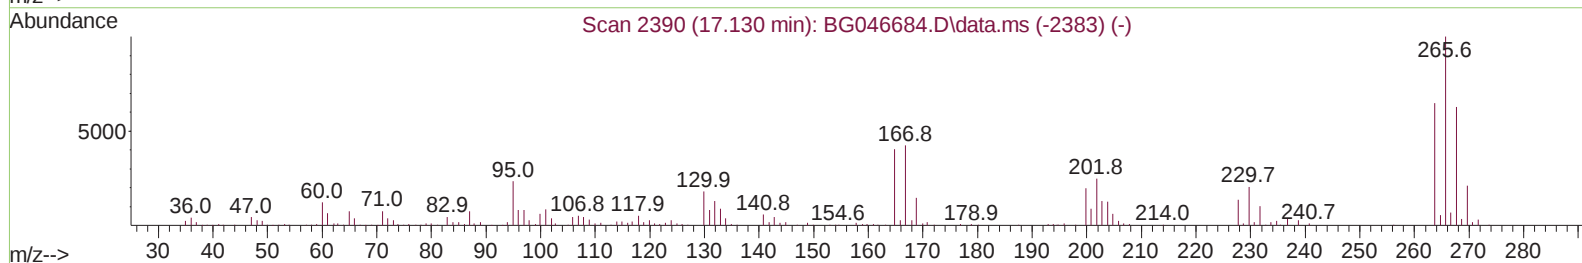
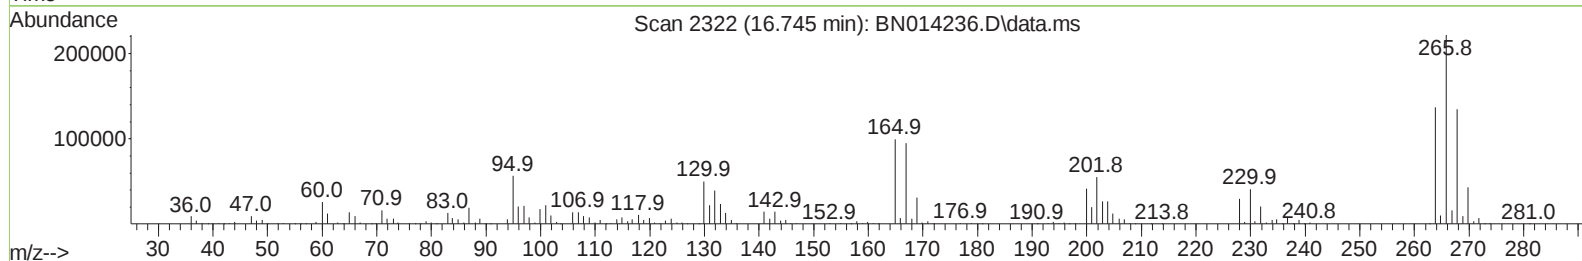


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040821\
Data File : BN014236.D
Acq On : 08 Apr 2021 08:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 08 10:52:35 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 26 11:50:50 2021
Response via : Initial Calibration

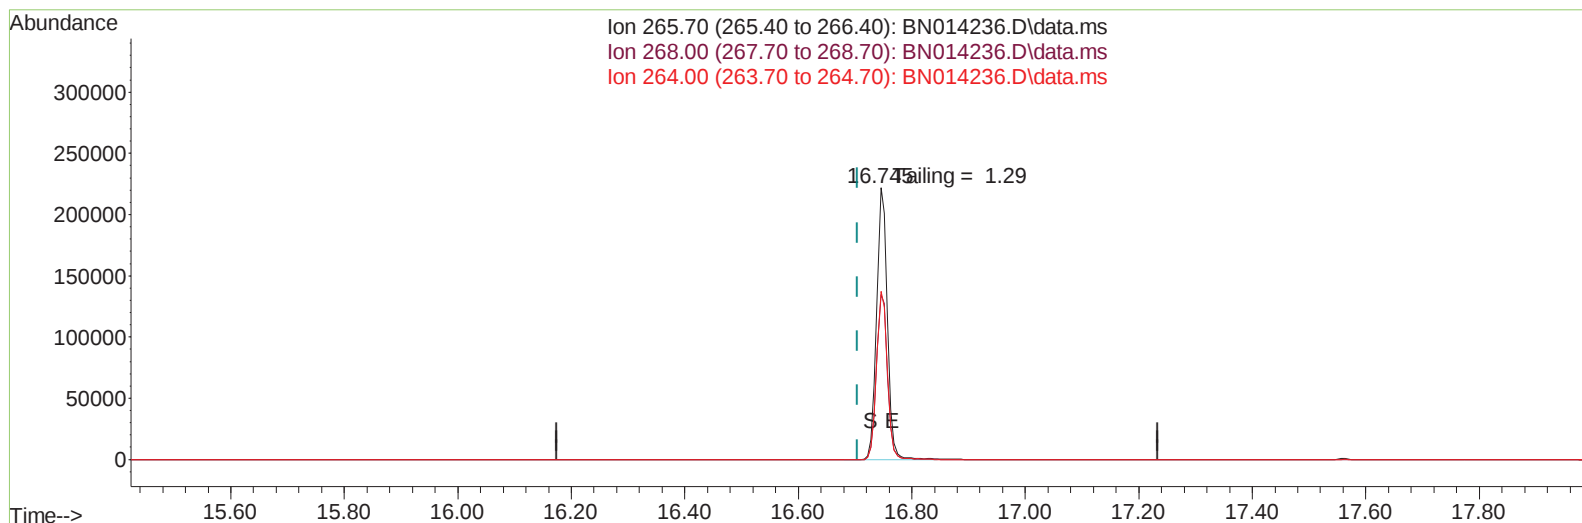

TIC: BN014236.D\data.ms

(70) Pentachlorophenol (C)




16.745min (+ 0.041) 23437.08 ng

response 289871

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.84
264.00	61.60	61.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040821\
Data File : BN014236.D
Acq On : 08 Apr 2021 08:49
Operator : CG/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 08 10:52:35 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 26 11:50:50 2021
Response via : Initial Calibration

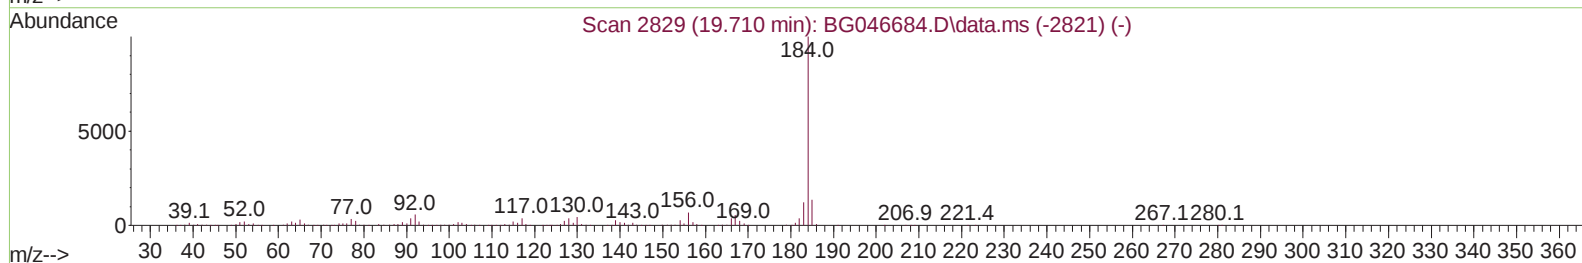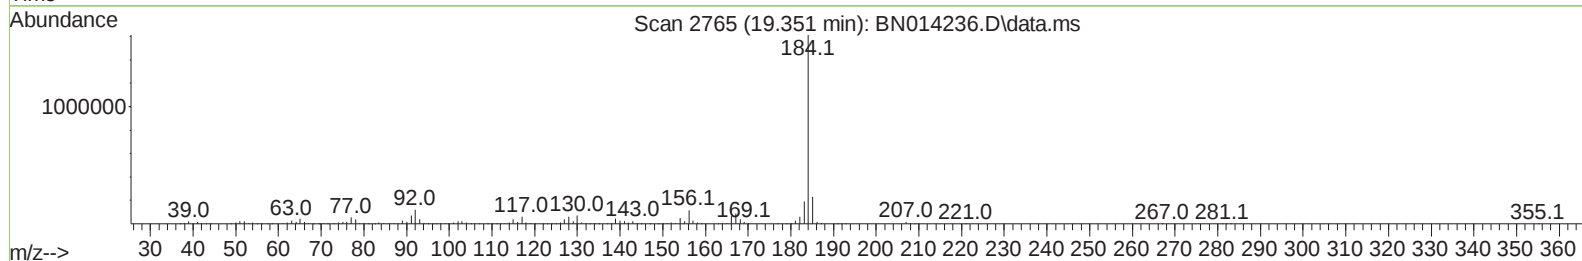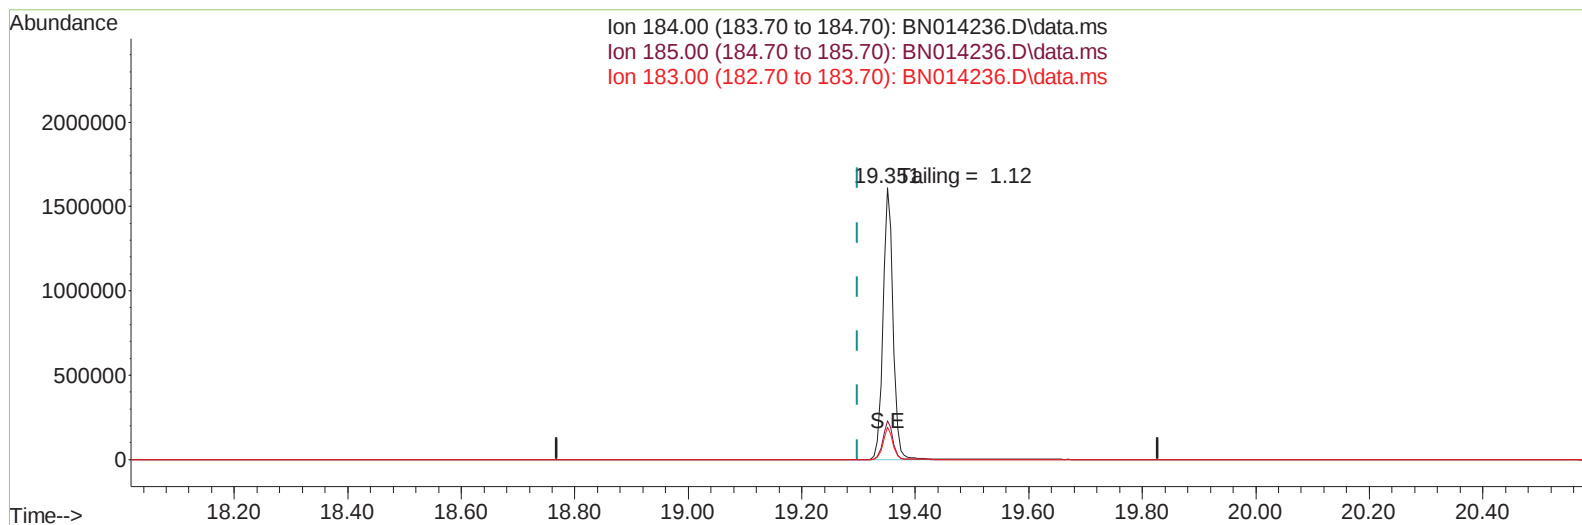

TIC: BN014236.D\data.ms

(77) Benzidine**19.351min (+ 0.053) 0.00 ng****response 1998070**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.29
183.00	13.20	11.86
0.00	0.00	0.00