

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040821\
 Data File : BN014237.D
 Acq On : 08 Apr 2021 10:09
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Manual Integrations
 APPROVED

mohammad
 4/8/2021 1:37:24 PM

Quant Time: Apr 08 10:47:22 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN040821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 08 01:18:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.724	152	9260	0.40	ng	0.00
7) Naphthalene-d8	10.505	136	37272	0.40	ng	# 0.00
13) Acenaphthene-d10	14.346	164	23079	0.40	ng	-0.01
19) Phenanthrene-d10	17.091	188	49699	0.40	ng	#-0.01
29) Chrysene-d12	21.290	240	50085	0.40	ng	#-0.01
36) Perylene-d12	23.531	264	51051	0.40	ng	#-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.324	112	9830	0.40	ng	0.00
5) Phenol-d6	6.887	99	12884	0.38	ng	0.00
8) Nitrobenzene-d5	8.870	82	9103	0.35	ng	0.00
11) 2-Methylnaphthalene-d10	12.093	152	25930	0.41	ng	0.00
14) 2,4,6-Tribromophenol	15.843	330	3850	0.32	ng	0.00
15) 2-Fluorobiphenyl	12.976	172	34737	0.43	ng	0.00
27) Fluoranthene-d10	19.131	212	59771	0.41	ng	0.00
31) Terphenyl-d14	19.736	244	46974	0.42	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.295	88	4647	0.45	ng	# 77
3) n-Nitrosodimethylamine	3.649	42	1707	0.35	ng	# 53
6) bis(2-Chloroethyl)ether	7.161	93	9859	0.43	ng	92
9) Naphthalene	10.556	128	38766	0.41	ng	99
10) Hexachlorobutadiene	10.847	225	7687	0.42	ng	# 99
12) 2-Methylnaphthalene	12.168	142	27609	0.41	ng	99
16) Acenaphthylene	14.067	152	36815	0.35	ng	100
17) Acenaphthene	14.410	154	26558	0.41	ng	99
18) Fluorene	15.399	166	33846	0.40	ng	100
20) 4,6-Dinitro-2-methylph...	15.475	198	1924	0.43	ng	96
21) 4-Bromophenyl-phenylether	16.300	248	11077	0.41	ng	# 84
22) Hexachlorobenzene	16.410	284	13156	0.44	ng	95
23) Atrazine	16.568	200	7900	0.29	ng	95
24) Pentachlorophenol	16.751	266	4155m	0.34	ng	
25) Phenanthrene	17.140	178	55567	0.42	ng	99
26) Anthracene	17.225	178	48423	0.38	ng	99
28) Fluoranthene	19.161	202	64509	0.42	ng	99
30) Pyrene	19.523	202	65867	0.41	ng	100
32) Benzo(a)anthracene	21.268	228	62779	0.40	ng	97
33) Chrysene	21.321	228	66378	0.43	ng	98
34) Bis(2-ethylhexyl)phtha...	21.226	149	20507	0.21	ng	99
35) Indeno(1,2,3-cd)pyrene	25.790	276	87870	0.47	ng	100
37) Benzo(b)fluoranthene	22.860	252	71582	0.43	ng	97
38) Benzo(k)fluoranthene	22.901	252	73069m	0.45	ng	
39) Benzo(a)pyrene	23.432	252	62920	0.41	ng	# 91
40) Dibenzo(a,h)anthracene	25.804	278	73559	0.46	ng	98
41) Benzo(g,h,i)perylene	26.478	276	72936	0.45	ng	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040821\
Data File : BN014237.D
Acq On : 08 Apr 2021 10:09
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Manual Integrations
APPROVED


mohammad
4/8/2021 1:37:24 PM

Quant Time: Apr 08 10:47:22 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN040821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 08 01:18:45 2021
Response via : Initial Calibration



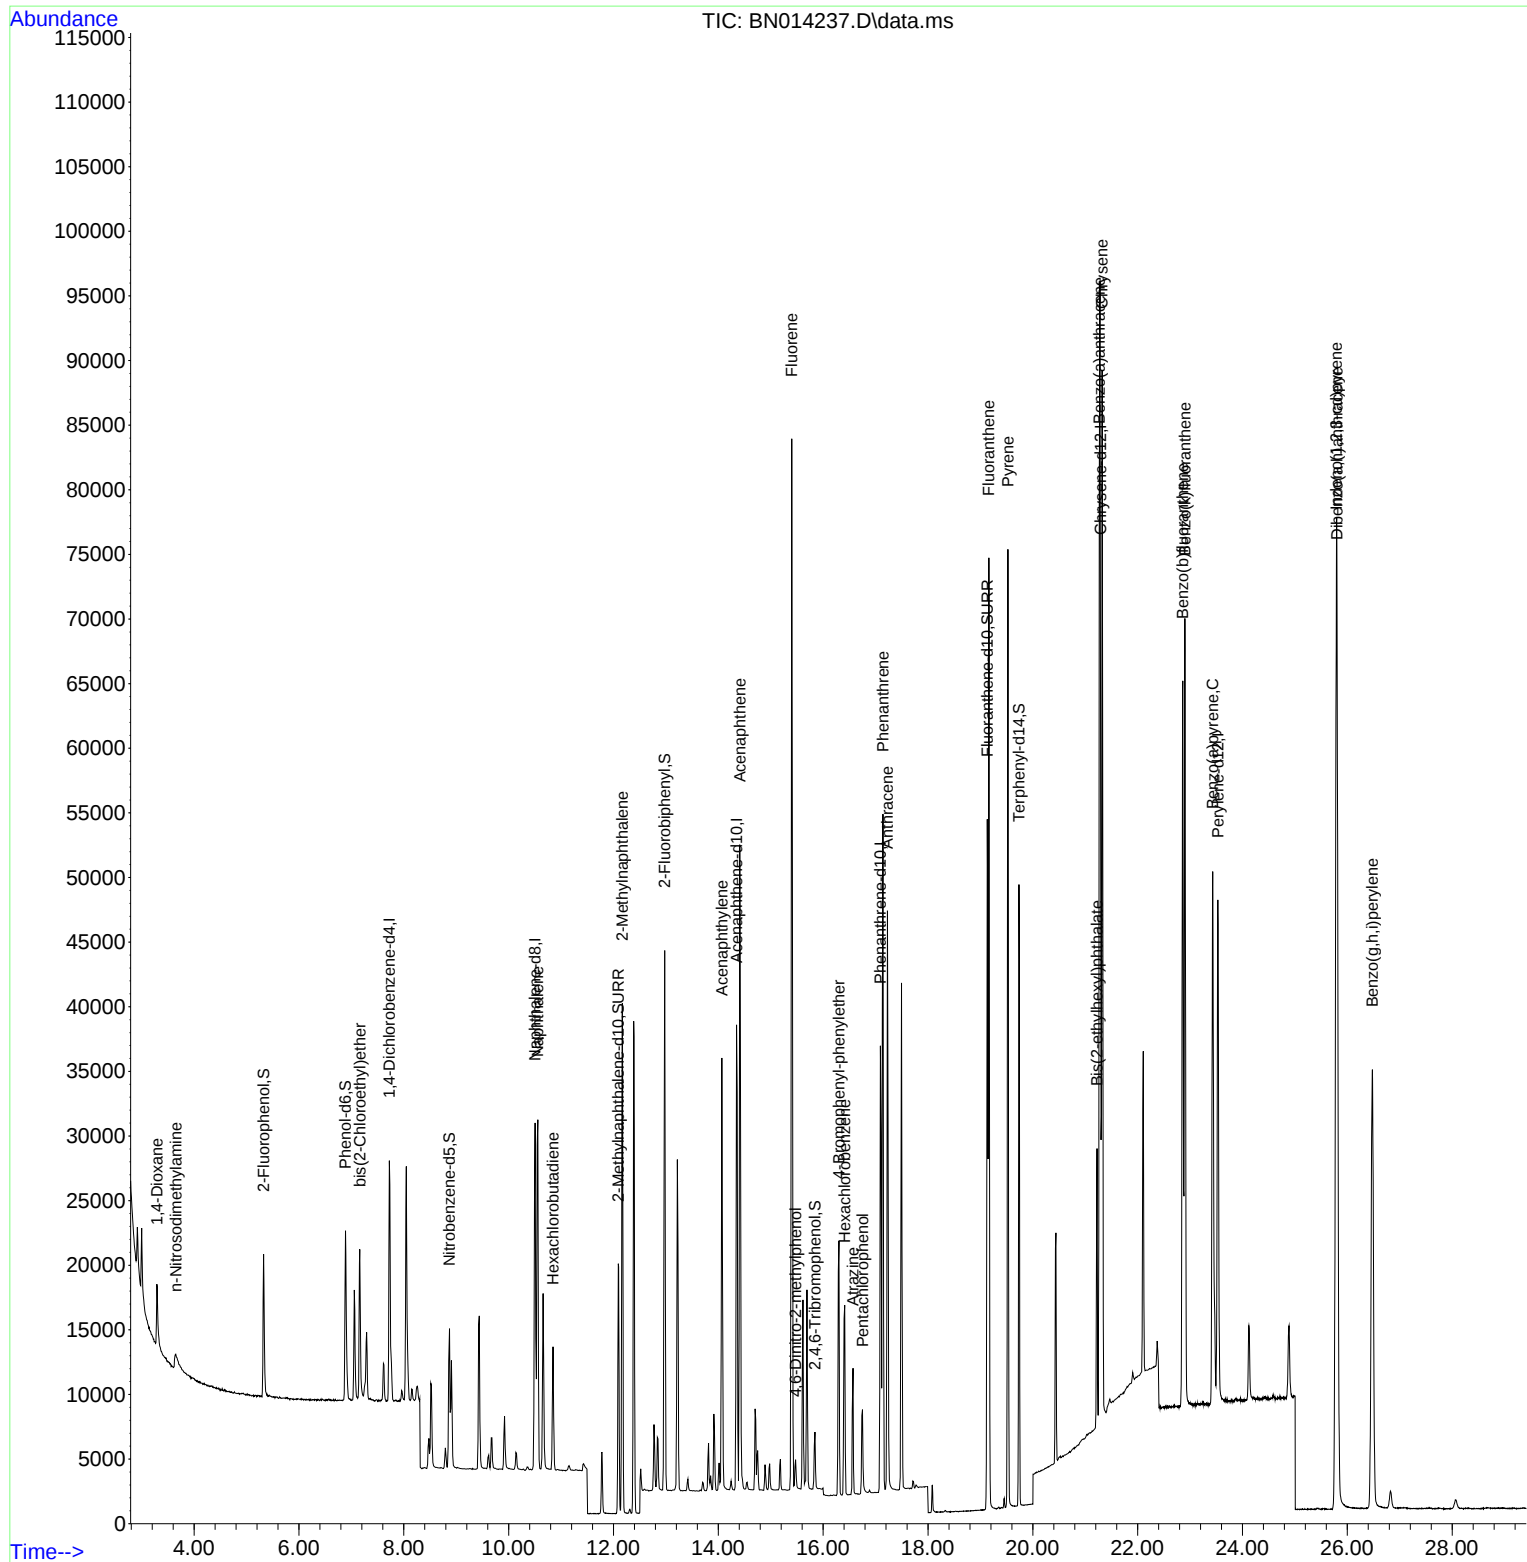





#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.724 min Scan# 614
 Delta R.T. -0.008 min
 Lab File: BN014237.D
 Acq: 08 Apr 2021 10:09





Tgt Ion: 152 Resp: 9260
 Ion Ratio Lower Upper
 152 100
 150 157.3 126.2 189.2
 115 61.4 49.4 74.0

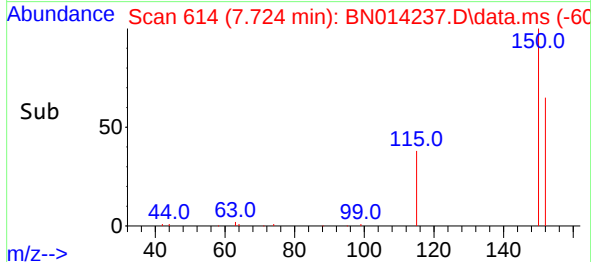

#2
 1,4-Dioxane
 Concen: 0.45 ng
 RT: 3.295 min Scan# 64
 Delta R.T. -0.000 min
 Lab File: BN014237.D
 Acq: 08 Apr 2021 10:09




Tgt Ion: 88 Resp: 4647
 Ion Ratio Lower Upper
 88 100
 58 64.5 70.0 105.0#
 43 24.9 28.3 42.5#

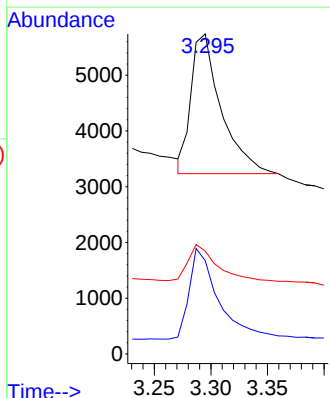


Instrument :
 BNA_N
 ClientSampled :
 SSTDCCC0.4

Manual Integrations
 APPROVED




mohammad
 4/8/2021 1:37:24 PM




#3
n-Nitrosodimethylamine
Concen: 0.35 ng
RT: 3.649 min Scan# 108
Delta R.T. 0.000 min
Lab File: BN014237.D
Acq: 08 Apr 2021 10:09





Tgt Ion: 42 Resp: 1707
Ion Ratio Lower Upper
42 100
74 157.2 85.0 127.6#
44 0.0 9.4 14.0#

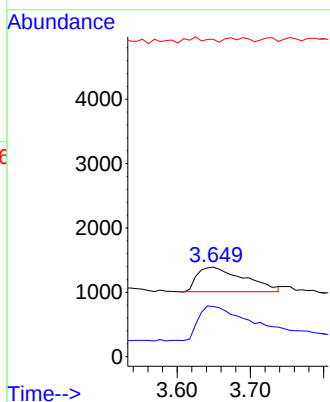

#4
2-Fluorophenol
Concen: 0.40 ng
RT: 5.324 min Scan# 316
Delta R.T. -0.008 min
Lab File: BN014237.D
Acq: 08 Apr 2021 10:09




Tgt Ion: 112 Resp: 9830
Ion Ratio Lower Upper
112 100
64 54.0 48.4 72.6
63 28.5 26.1 39.1

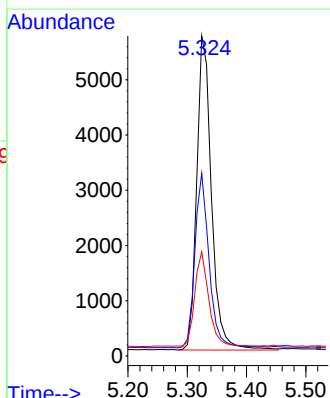

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Manual Integrations
APPROVED

mohammad
4/8/2021 1:37:24 PM







#5
Phenol-d6
Concen: 0.38 ng
RT: 6.887 min Scan# 510
Delta R.T. -0.008 min
Lab File: BN014237.D
Acq: 08 Apr 2021 10:09

Tgt Ion:	99	Resp:	12884
Ion	Ratio	Lower	Upper
99	100		
42	18.6	17.9	26.9
71	34.2	27.0	40.6

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4




Manual Integrations
APPROVED


mohammad
4/8/2021 1:37:24 PM

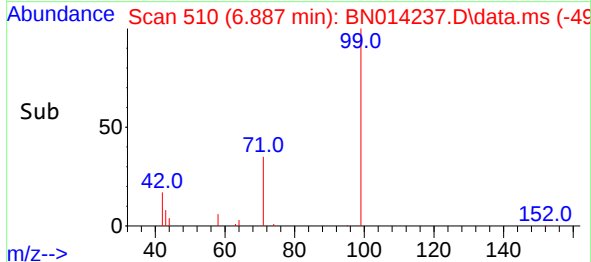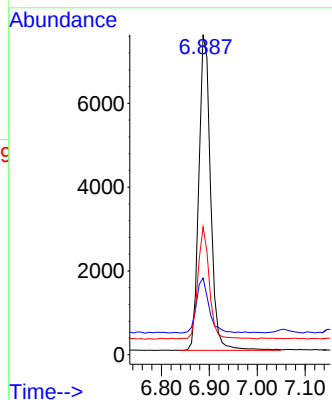

#6
bis(2-Chloroethyl)ether
Concen: 0.43 ng
RT: 7.161 min Scan# 544
Delta R.T. -0.000 min
Lab File: BN014237.D
Acq: 08 Apr 2021 10:09


Tgt Ion:	93	Resp:	9859
Ion	Ratio	Lower	Upper
93	100		
63	71.4	65.3	97.9
95	33.4	26.3	39.5

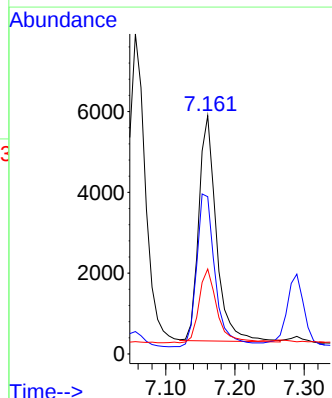



#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.505 min Scan# 860
Delta R.T. -0.000 min
Lab File: BN014237.D
Acq: 08 Apr 2021 10:09




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4




Tgt Ion:136 Resp: 37272
Ion Ratio Lower Upper
136 100
137 11.2 8.9 13.3
54 5.4 8.4 12.6#
68 5.2 5.8 8.8#

Manual Integrations
APPROVED



mohammad
4/8/2021 1:37:24 PM

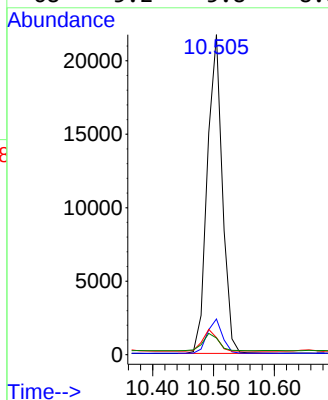


#8
Nitrobenzene-d5
Concen: 0.35 ng
RT: 8.870 min Scan# 731
Delta R.T. -0.000 min
Lab File: BN014237.D
Acq: 08 Apr 2021 10:09




Tgt Ion: 82 Resp: 9103
Ion Ratio Lower Upper
82 100
128 42.9 36.1 54.1
54 42.2 39.1 58.7

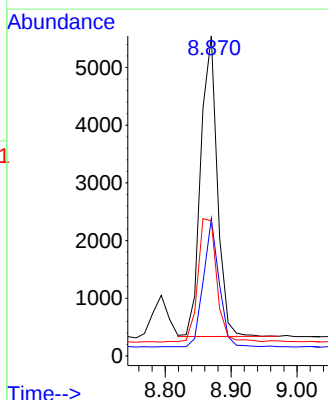



#9
Naphthalene
Concen: 0.41 ng
RT: 10.556 min Scan# 864
Delta R.T. -0.000 min
Lab File: BN014237.D
Acq: 08 Apr 2021 10:09




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4



Tgt Ion:128 Resp: 38766
Ion Ratio Lower Upper
128 100
129 11.5 8.9 13.3
127 13.0 10.6 16.0




Manual Integrations
APPROVED


mohammad
4/8/2021 1:37:24 PM

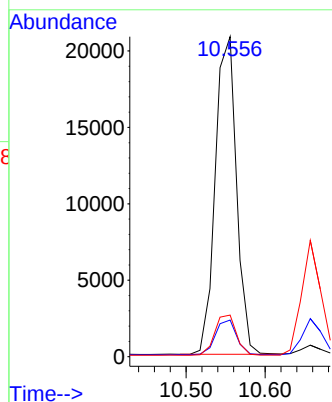

#10
Hexachlorobutadiene
Concen: 0.42 ng
RT: 10.847 min Scan# 887
Delta R.T. -0.000 min
Lab File: BN014237.D
Acq: 08 Apr 2021 10:09

Tgt Ion:225 Resp: 7687
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 64.3 50.6 75.8

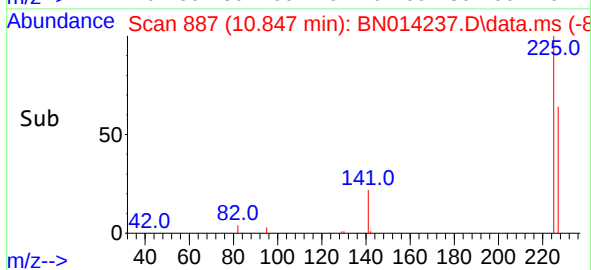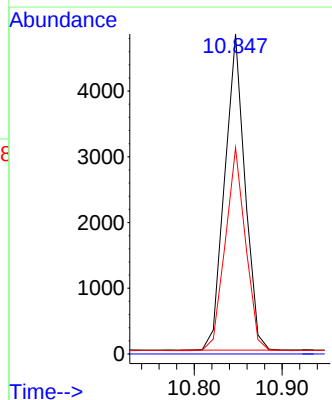







#11
2-Methylnaphthalene-d10
Concen: 0.41 ng
RT: 12.093 min Scan# 1071
Delta R.T. -0.009 min
Lab File: BN014237.D
Acq: 08 Apr 2021 10:09

Tgt Ion:152 Resp: 25930
Ion Ratio Lower Upper
152 100
151 20.1 16.2 24.2

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4




Manual Integrations
APPROVED


mohammad
4/8/2021 1:37:24 PM




#12
2-Methylnaphthalene
Concen: 0.41 ng
RT: 12.168 min Scan# 1088
Delta R.T. -0.004 min
Lab File: BN014237.D
Acq: 08 Apr 2021 10:09

Tgt Ion:142 Resp: 27609
Ion Ratio Lower Upper
142 100
141 88.2 71.4 107.2
115 35.5 29.1 43.7









#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.346 min Scan# 1309
Delta R.T. -0.013 min
Lab File: BN014237.D
Acq: 08 Apr 2021 10:09





Tgt Ion:164 Resp: 23079
Ion Ratio Lower Upper
164 100
162 103.9 80.4 120.6
160 48.5 36.0 54.0

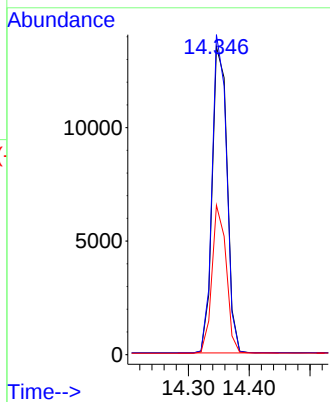

#14
2,4,6-Tribromophenol
Concen: 0.32 ng
RT: 15.843 min Scan# 1427
Delta R.T. -0.000 min
Lab File: BN014237.D
Acq: 08 Apr 2021 10:09

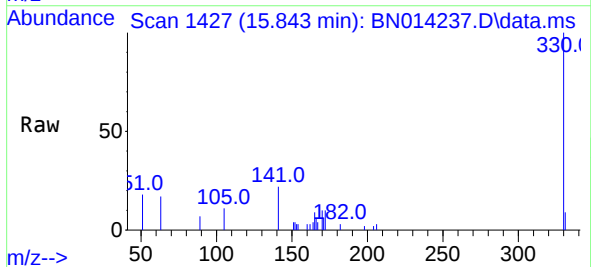


Tgt Ion:330 Resp: 3850
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 32.5 30.6 45.8

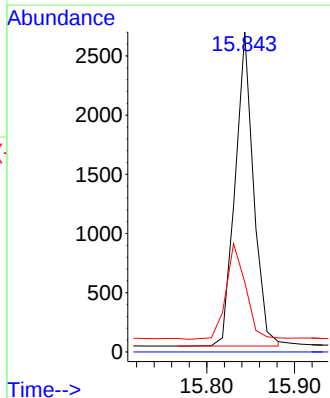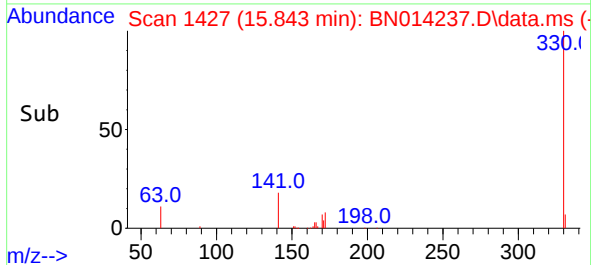

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Manual Integrations
APPROVED

mohammad
4/8/2021 1:37:24 PM







#15
2-Fluorobiphenyl
Concen: 0.43 ng
RT: 12.976 min Scan# 1201
Delta R.T. -0.000 min
Lab File: BN014237.D
Acq: 08 Apr 2021 10:09

Tgt Ion:172 Resp: 34737
Ion Ratio Lower Upper
172 100
171 34.5 27.8 41.6
170 23.1 18.7 28.1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4




Manual Integrations
APPROVED


mohammad
4/8/2021 1:37:24 PM

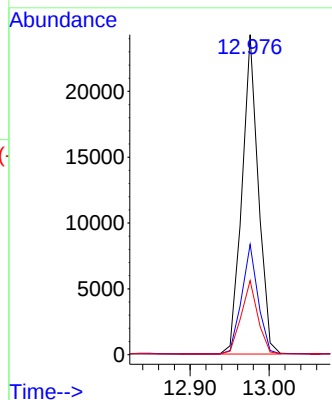

#16
Acenaphthylene
Concen: 0.35 ng
RT: 14.067 min Scan# 1287
Delta R.T. -0.000 min
Lab File: BN014237.D
Acq: 08 Apr 2021 10:09


Tgt Ion:152 Resp: 36815
Ion Ratio Lower Upper
152 100
151 19.3 15.5 23.3
153 12.8 10.5 15.7

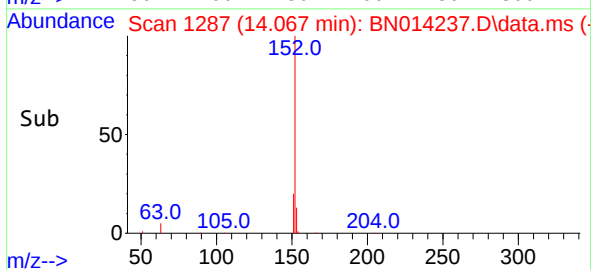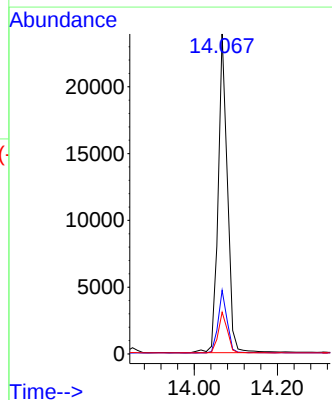



#17
Acenaphthene
Concen: 0.41 ng
RT: 14.410 min Scan# 1314
Delta R.T. -0.013 min
Lab File: BN014237.D
Acq: 08 Apr 2021 10:09




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

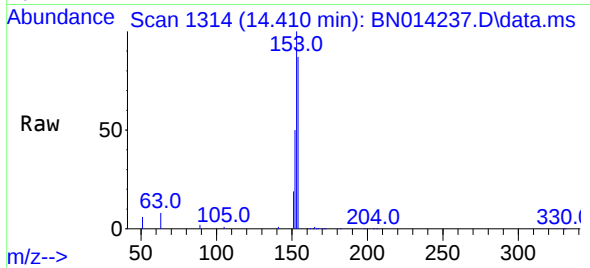

Tgt Ion:154 Resp: 26558
Ion Ratio Lower Upper
154 100
153 110.2 88.8 133.2
152 54.0 43.8 65.6




Manual Integrations
APPROVED


mohammad
4/8/2021 1:37:24 PM

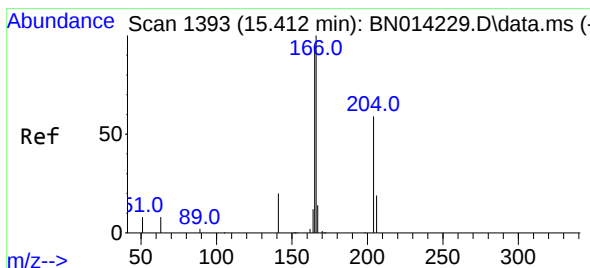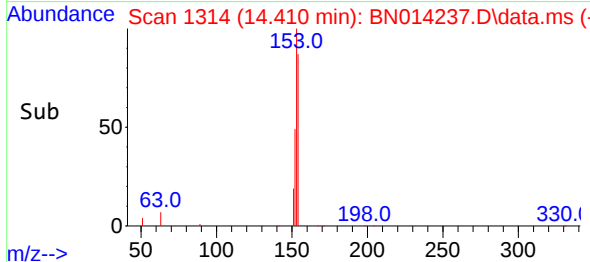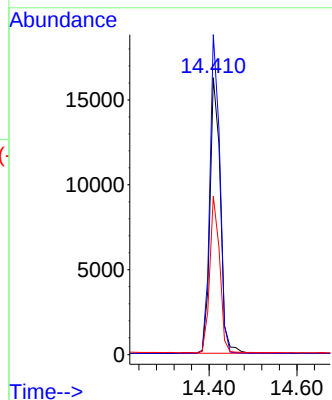

#18
Fluorene
Concen: 0.40 ng
RT: 15.399 min Scan# 1392
Delta R.T. -0.013 min
Lab File: BN014237.D
Acq: 08 Apr 2021 10:09

Tgt Ion:166 Resp: 33846
Ion Ratio Lower Upper
166 100
165 98.4 78.6 118.0
167 13.5 10.7 16.1

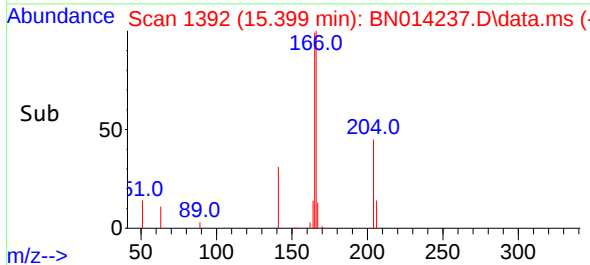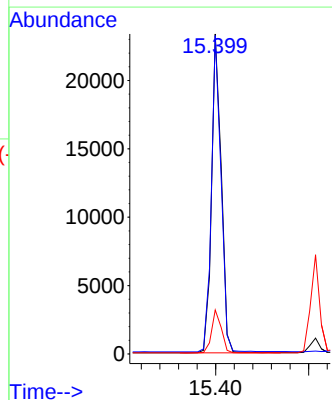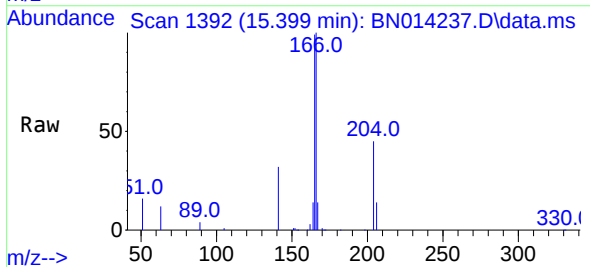







#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.091 min Scan# 1529
Delta R.T. -0.012 min
Lab File: BN014237.D
Acq: 08 Apr 2021 10:09

Tgt Ion:188 Resp: 49699
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 11.0 6.2 9.2#

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4




Manual Integrations
APPROVED


mohammad
4/8/2021 1:37:24 PM



#20
4,6-Dinitro-2-methylphenol
Concen: 0.43 ng
RT: 15.475 min Scan# 1398
Delta R.T. 0.000 min
Lab File: BN014237.D
Acq: 08 Apr 2021 10:09


Tgt Ion:198 Resp: 1924
Ion Ratio Lower Upper
198 100
51 59.7 46.3 69.5
105 48.2 35.5 53.3

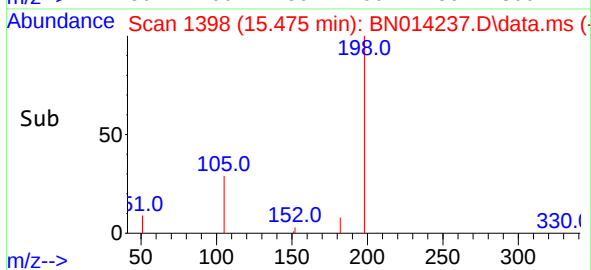



#21
4-Bromophenyl-phenylether
Concen: 0.41 ng
RT: 16.300 min Scan# 1464
Delta R.T. -0.000 min
Lab File: BN014237.D
Acq: 08 Apr 2021 10:09




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

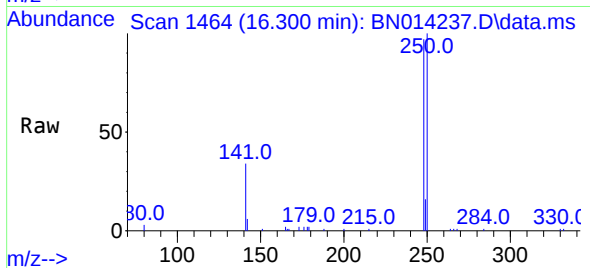


Tgt Ion:248 Resp: 11077
Ion Ratio Lower Upper
248 100
250 103.2 76.1 114.1
141 35.3 45.5 68.3#

Manual Integrations
APPROVED



mohammad
4/8/2021 1:37:24 PM

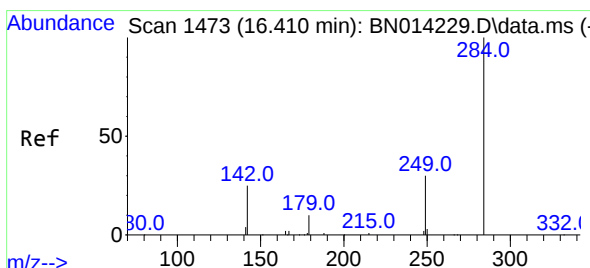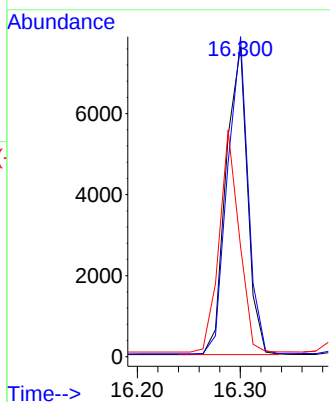


#22
Hexachlorobenzene
Concen: 0.44 ng
RT: 16.410 min Scan# 1473
Delta R.T. -0.000 min
Lab File: BN014237.D
Acq: 08 Apr 2021 10:09




Tgt Ion:284 Resp: 13156
Ion Ratio Lower Upper
284 100
142 32.3 28.9 43.3
249 28.9 25.0 37.4

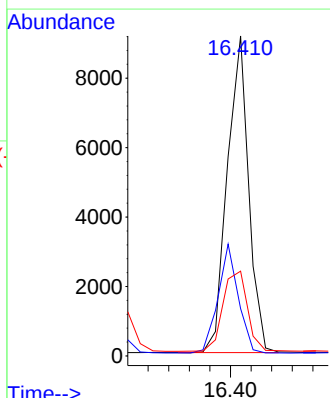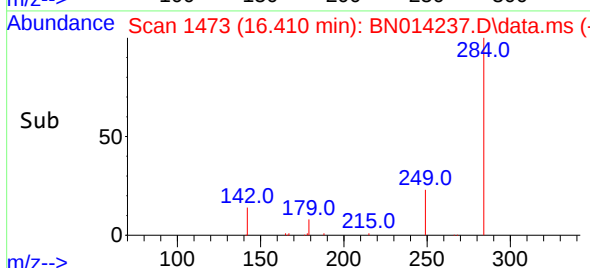

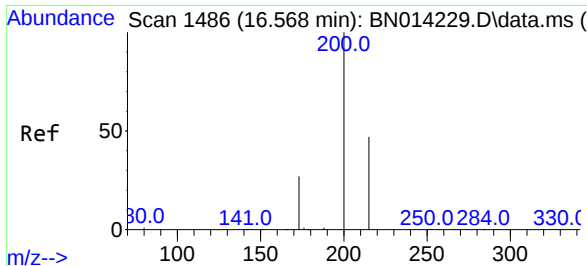

#23
Atrazine
Concen: 0.29 ng
RT: 16.568 min Scan# 1486
Delta R.T. -0.000 min
Lab File: BN014237.D
Acq: 08 Apr 2021 10:09




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

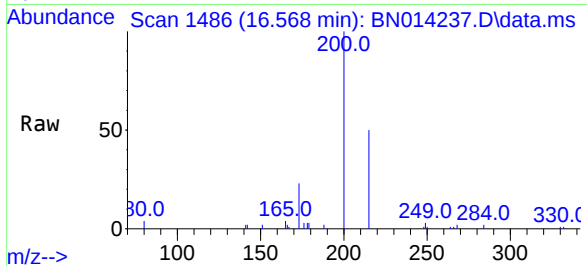


Tgt Ion:200 Resp: 7900
Ion Ratio Lower Upper
200 100
173 22.7 21.9 32.9
215 49.8 38.1 57.1

Manual Integrations
APPROVED



mohammad
4/8/2021 1:37:24 PM

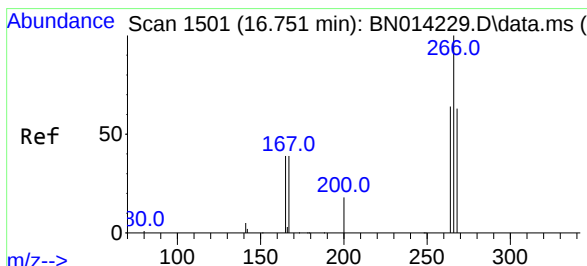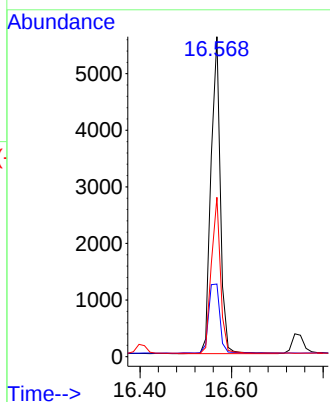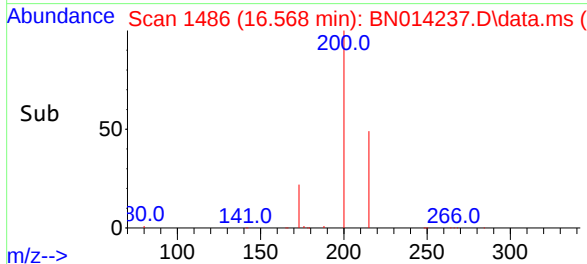


#24
Pentachlorophenol
Concen: 0.34 ng m
RT: 16.751 min Scan# 1501
Delta R.T. -0.000 min
Lab File: BN014237.D
Acq: 08 Apr 2021 10:09

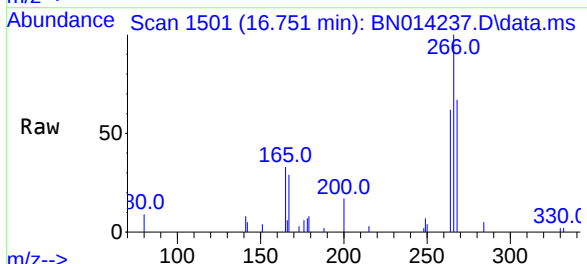


Tgt Ion:266 Resp: 4155
Ion Ratio Lower Upper
266 100
264 57.3 48.8 73.2
268 57.6 48.8 73.2

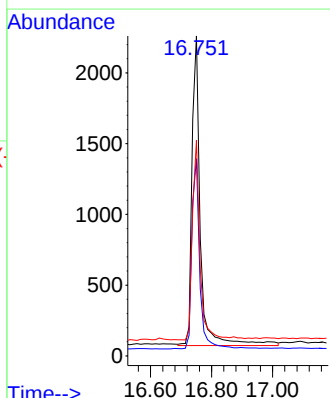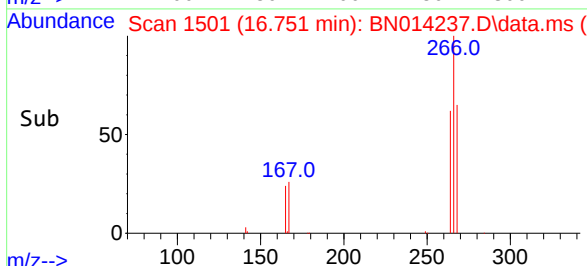



#25
Phenanthrene
Concen: 0.42 ng
RT: 17.140 min Scan# 1533
Delta R.T. -0.000 min
Lab File: BN014237.D
Acq: 08 Apr 2021 10:09




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4




Tgt Ion:178 Resp: 55567
Ion Ratio Lower Upper
178 100
176 19.3 15.0 22.6
179 15.4 12.2 18.4

Manual Integrations
APPROVED



mohammad
4/8/2021 1:37:24 PM

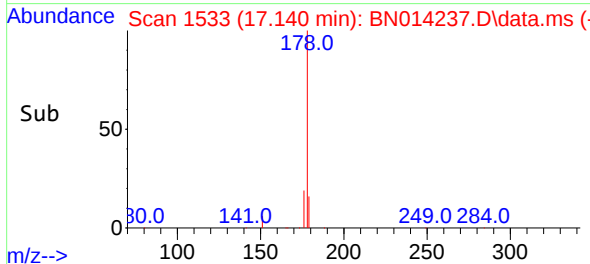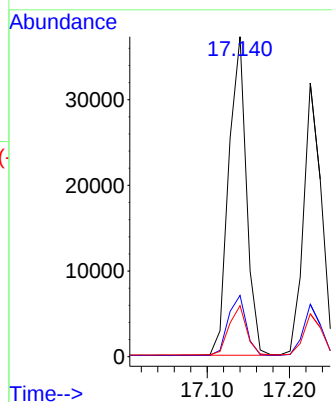


#26
Anthracene
Concen: 0.38 ng
RT: 17.225 min Scan# 1540
Delta R.T. -0.012 min
Lab File: BN014237.D
Acq: 08 Apr 2021 10:09

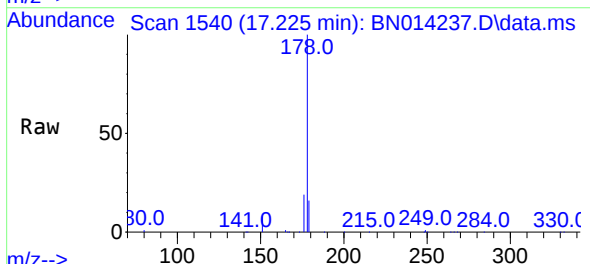

Tgt Ion:178 Resp: 48423
Ion Ratio Lower Upper
178 100
176 18.6 14.6 21.8
179 15.4 12.3 18.5

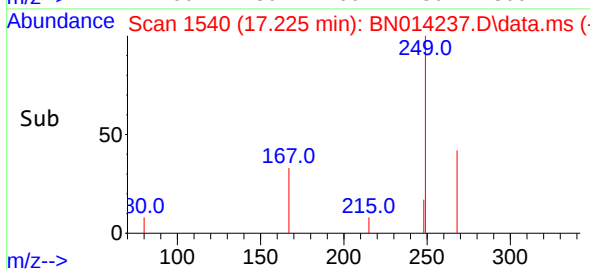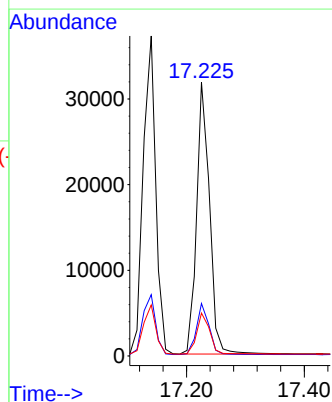







#27
Fluoranthene-d10
Concen: 0.41 ng
RT: 19.131 min Scan# 1831
Delta R.T. -0.005 min
Lab File: BN014237.D
Acq: 08 Apr 2021 10:09

Tgt Ion: 212 Resp: 59771
Ion Ratio Lower Upper
212 100
106 11.3 10.1 15.1
104 6.3 5.6 8.4

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4




Manual Integrations
APPROVED


mohammad
4/8/2021 1:37:24 PM

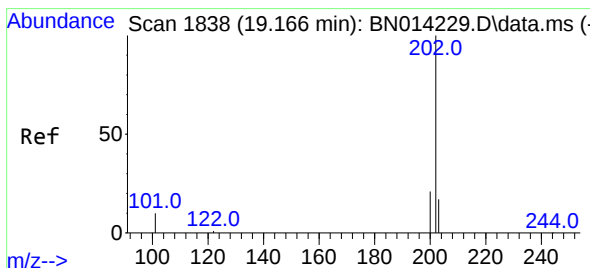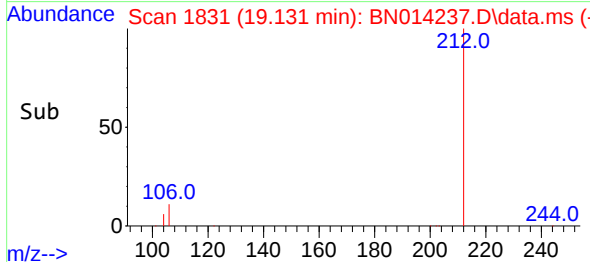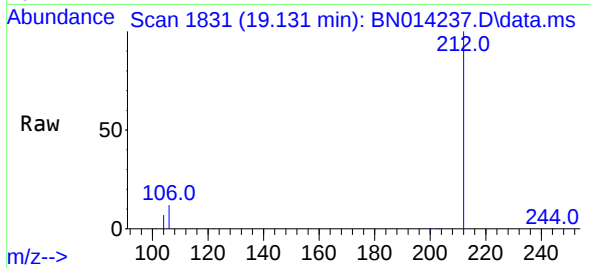

#28
Fluoranthene
Concen: 0.42 ng
RT: 19.161 min Scan# 1837
Delta R.T. -0.005 min
Lab File: BN014237.D
Acq: 08 Apr 2021 10:09

Tgt Ion: 202 Resp: 64509
Ion Ratio Lower Upper
202 100
101 9.8 8.6 13.0
203 17.3 13.8 20.6

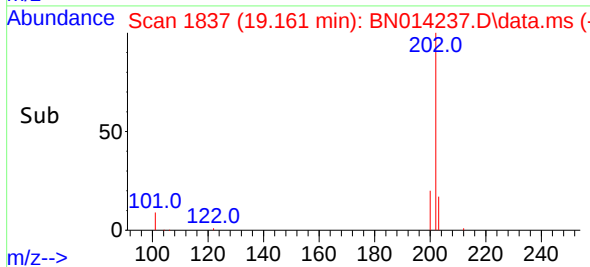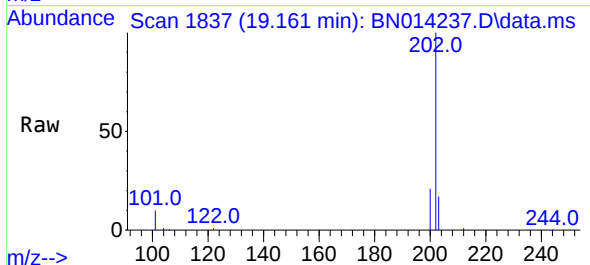







#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.290 min Scan# 2128
Delta R.T. -0.011 min
Lab File: BN014237.D
Acq: 08 Apr 2021 10:09

Tgt Ion:240 Resp: 50085
Ion Ratio Lower Upper
240 100
120 8.6 10.8 16.2#
236 26.2 21.4 32.2

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4




Manual Integrations
APPROVED


mohammad
4/8/2021 1:37:24 PM

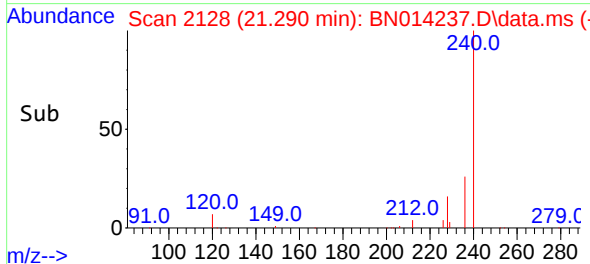


#30
Pyrene
Concen: 0.41 ng
RT: 19.523 min Scan# 1910
Delta R.T. -0.005 min
Lab File: BN014237.D
Acq: 08 Apr 2021 10:09

Tgt Ion:202 Resp: 65867
Ion Ratio Lower Upper
202 100
200 20.6 16.3 24.5
203 17.5 13.9 20.9

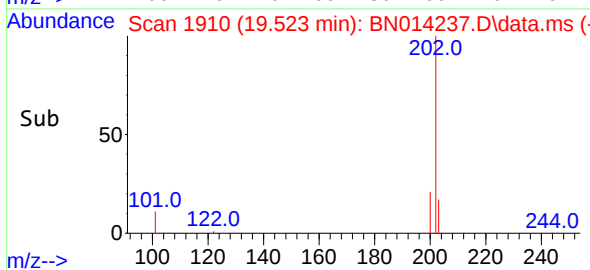

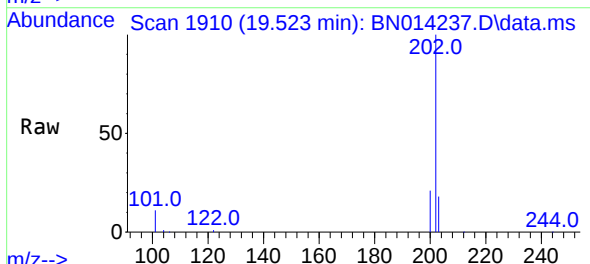


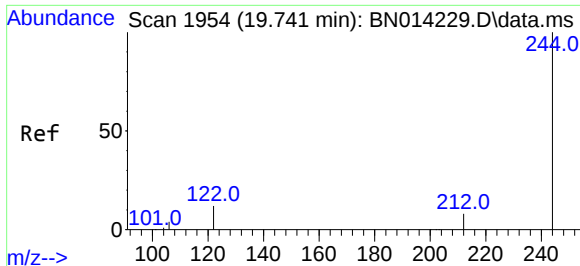


#31
Terphenyl-d14
Concen: 0.42 ng
RT: 19.736 min Scan# 1953
Delta R.T. -0.005 min
Lab File: BN014237.D
Acq: 08 Apr 2021 10:09

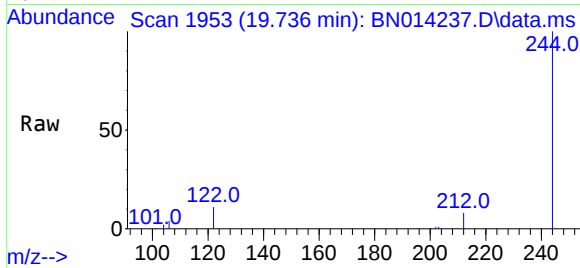



Tgt Ion:244 Resp: 46974
Ion Ratio Lower Upper
244 100
212 7.7 5.9 8.9
122 11.2 9.2 13.8

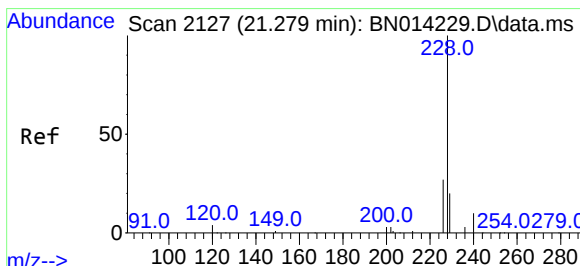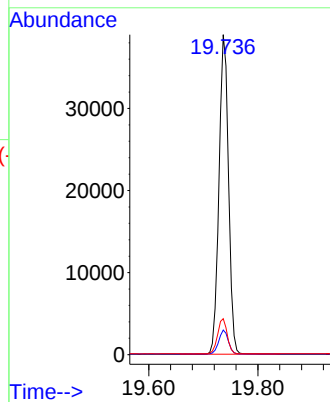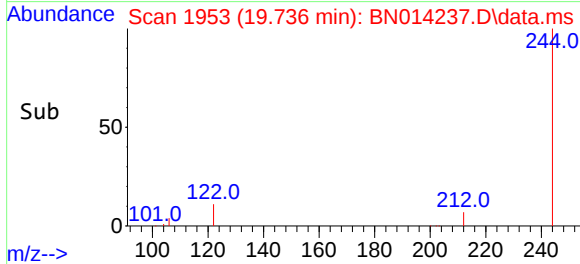

#32
Benzo(a)anthracene
Concen: 0.40 ng
RT: 21.268 min Scan# 2126
Delta R.T. -0.011 min
Lab File: BN014237.D
Acq: 08 Apr 2021 10:09

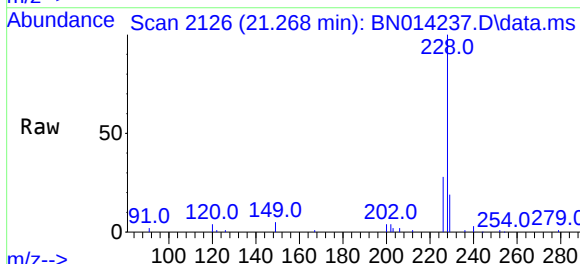


Tgt Ion:228 Resp: 62779
Ion Ratio Lower Upper
228 100
226 28.0 21.1 31.7
229 19.0 15.8 23.8

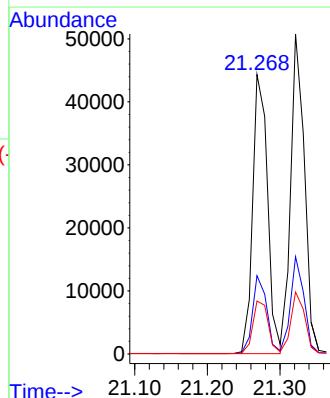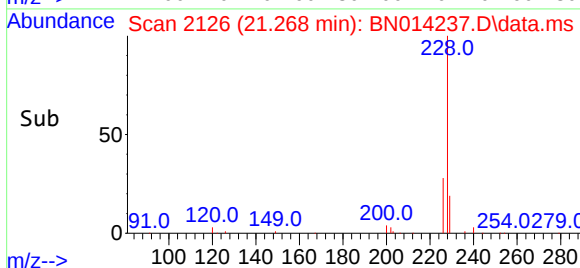

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Manual Integrations
APPROVED

mohammad
4/8/2021 1:37:24 PM

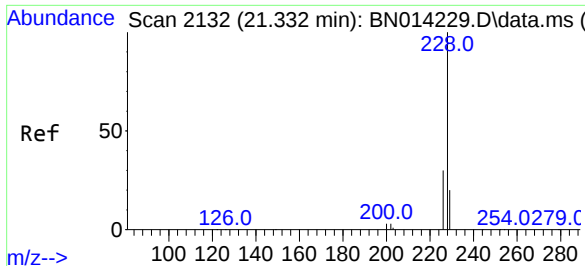





#33
Chrysene
Concen: 0.43 ng
RT: 21.321 min Scan# 2131
Delta R.T. -0.011 min
Lab File: BN014237.D
Acq: 08 Apr 2021 10:09

Tgt Ion: 228 Resp: 66378
Ion Ratio Lower Upper
228 100
226 30.4 23.0 34.6
229 19.4 15.8 23.8

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4




Manual Integrations
APPROVED


mohammad
4/8/2021 1:37:24 PM

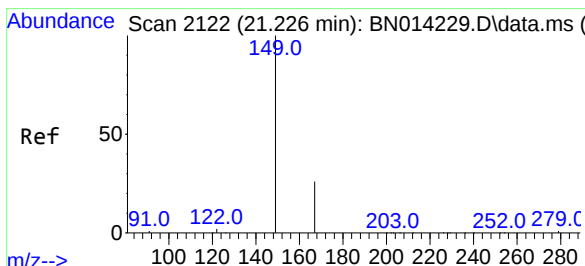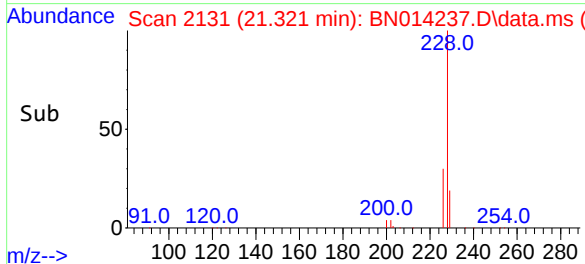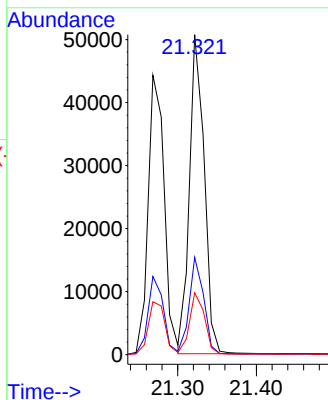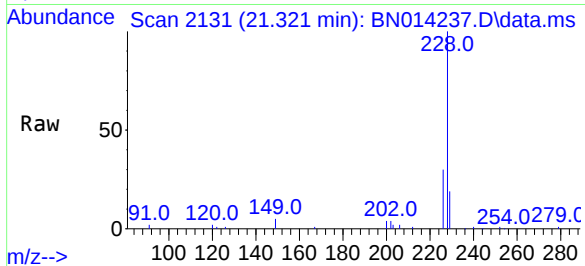

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.21 ng
RT: 21.226 min Scan# 2122
Delta R.T. -0.000 min
Lab File: BN014237.D
Acq: 08 Apr 2021 10:09

Tgt Ion: 149 Resp: 20507
Ion Ratio Lower Upper
149 100
167 26.3 21.4 32.0
279 4.2 3.1 4.7

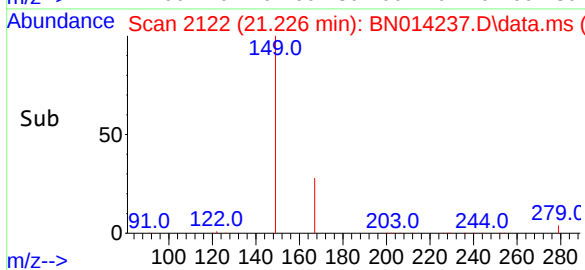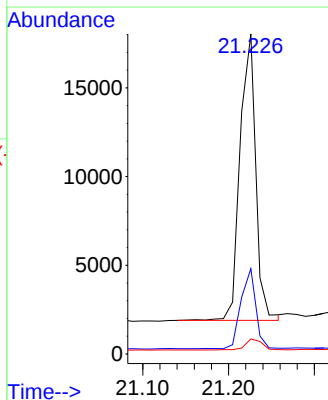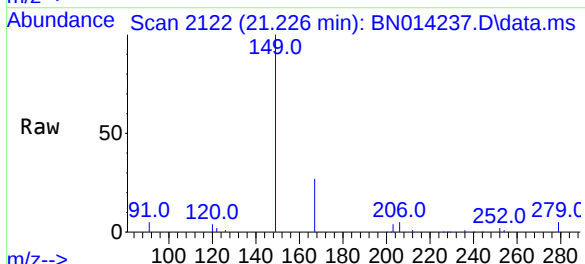







#35
Indeno(1,2,3-cd)pyrene
Concen: 0.47 ng
RT: 25.790 min Scan# 3222
Delta R.T. -0.014 min
Lab File: BN014237.D
Acq: 08 Apr 2021 10:09

Tgt Ion: 276 Resp: 87870
Ion Ratio Lower Upper
276 100
138 23.4 18.6 27.8
277 24.8 19.8 29.8

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4




Manual Integrations
APPROVED


mohammad
4/8/2021 1:37:24 PM

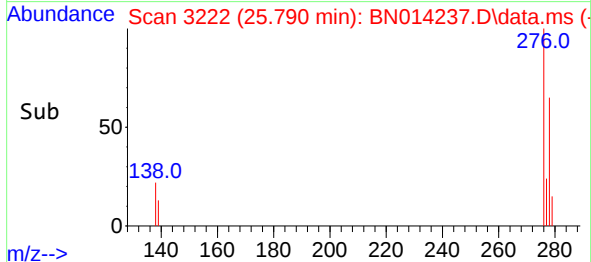

#36
Perylene-d12
Concen: 0.40 ng
RT: 23.531 min Scan# 2562
Delta R.T. -0.010 min
Lab File: BN014237.D
Acq: 08 Apr 2021 10:09

Tgt Ion: 264 Resp: 51051
Ion Ratio Lower Upper
264 100
260 24.4 19.7 29.5
265 43.6 19.2 28.8#

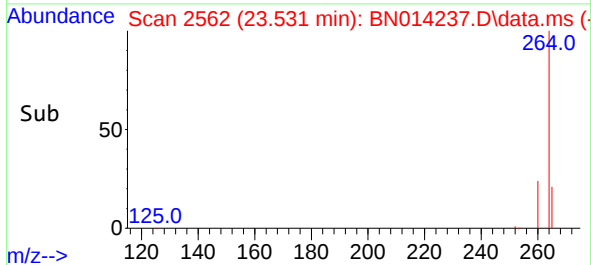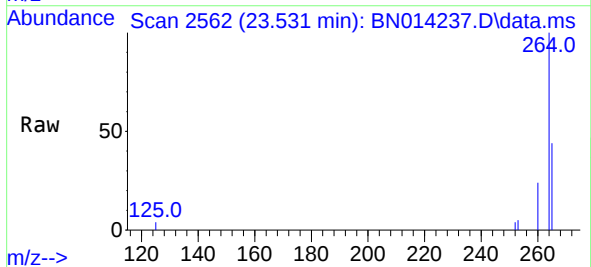







#37
Benzo(b)fluoranthene
Concen: 0.43 ng
RT: 22.860 min Scan# 2366
Delta R.T. -0.007 min
Lab File: BN014237.D
Acq: 08 Apr 2021 10:09

Tgt Ion:	252	Resp:	71582
Ion Ratio	Lower	Upper	
252	100		
253	24.0	18.5	27.7
125	11.0	10.3	15.5

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4




Manual Integrations
APPROVED


mohammad
4/8/2021 1:37:24 PM

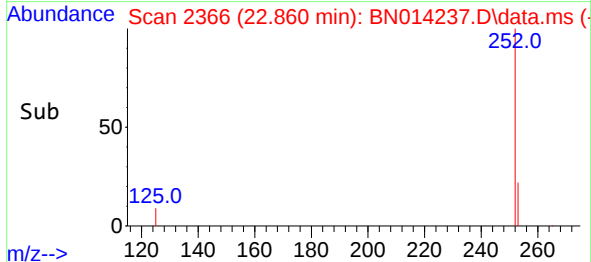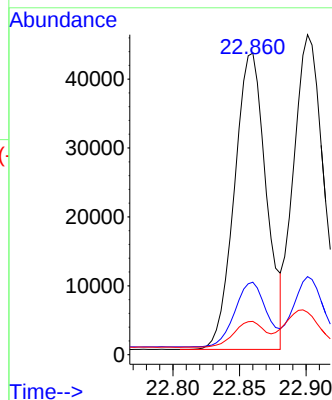


#38
Benzo(k)fluoranthene
Concen: 0.45 ng m
RT: 22.901 min Scan# 2378
Delta R.T. -0.010 min
Lab File: BN014237.D
Acq: 08 Apr 2021 10:09

Tgt Ion:	252	Resp:	73069
Ion Ratio	Lower	Upper	
252	100		
253	24.4	18.1	27.1
125	13.3	7.8	11.6#

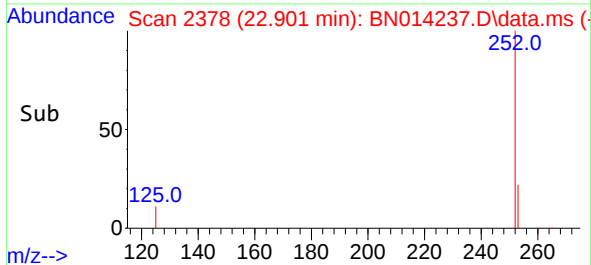
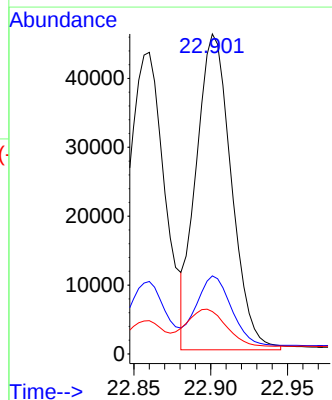
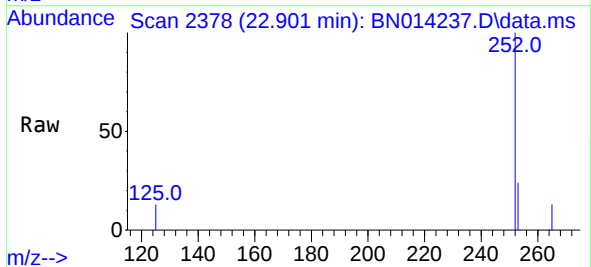





#39
Benzo(a)pyrene
Concen: 0.41 ng
RT: 23.432 min Scan# 2533
Delta R.T. -0.010 min
Lab File: BN014237.D
Acq: 08 Apr 2021 10:09





Tgt Ion:252 Resp: 62920
Ion Ratio Lower Upper
252 100
253 25.0 19.4 29.2
125 12.8 16.6 24.8#

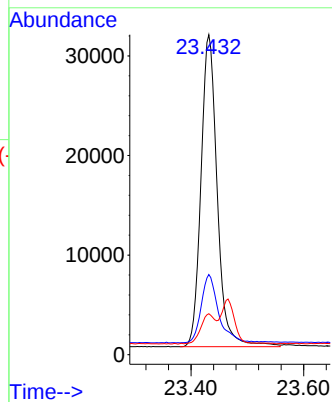

#40
Dibenzo(a,h)anthracene
Concen: 0.46 ng
RT: 25.804 min Scan# 3226
Delta R.T. -0.017 min
Lab File: BN014237.D
Acq: 08 Apr 2021 10:09




Tgt Ion:278 Resp: 73559
Ion Ratio Lower Upper
278 100
139 16.2 12.6 19.0
279 25.2 19.4 29.0

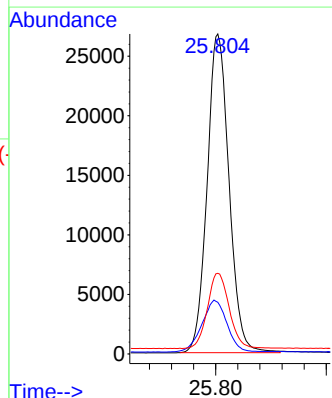

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Manual Integrations
APPROVED

mohammad
4/8/2021 1:37:24 PM

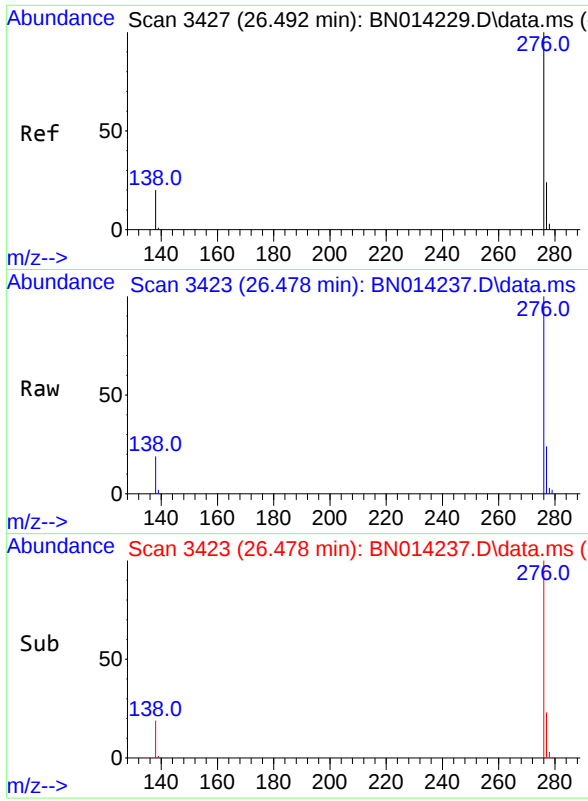

#41
Benzo(g,h,i)perylene
Concen: 0.45 ng
RT: 26.478 min Scan# 3423
Delta R.T. -0.014 min
Lab File: BN014237.D
Acq: 08 Apr 2021 10:09

Tgt Ion:	276	Resp:	72936
Ion Ratio	Lower	Upper	
276	100		
277	24.0	18.9	28.3
138	19.4	16.4	24.6

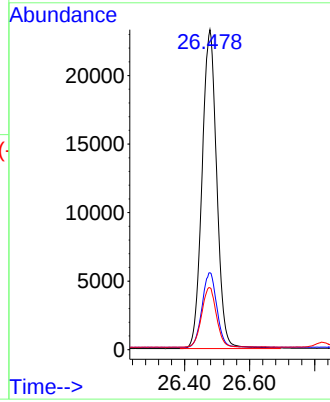

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Manual Integrations
APPROVED

mohammad
4/8/2021 1:37:24 PM