
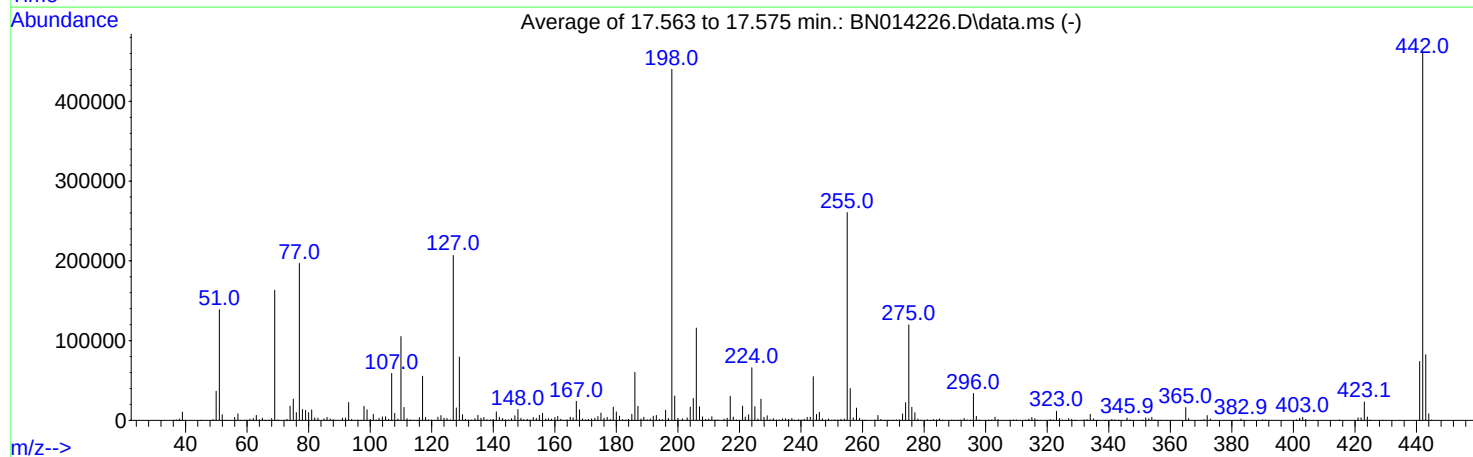


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040821\
 Data File : BN014226.D
 Acq On : 07 Apr 2021 15:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN040821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 08 01:18:45 2021

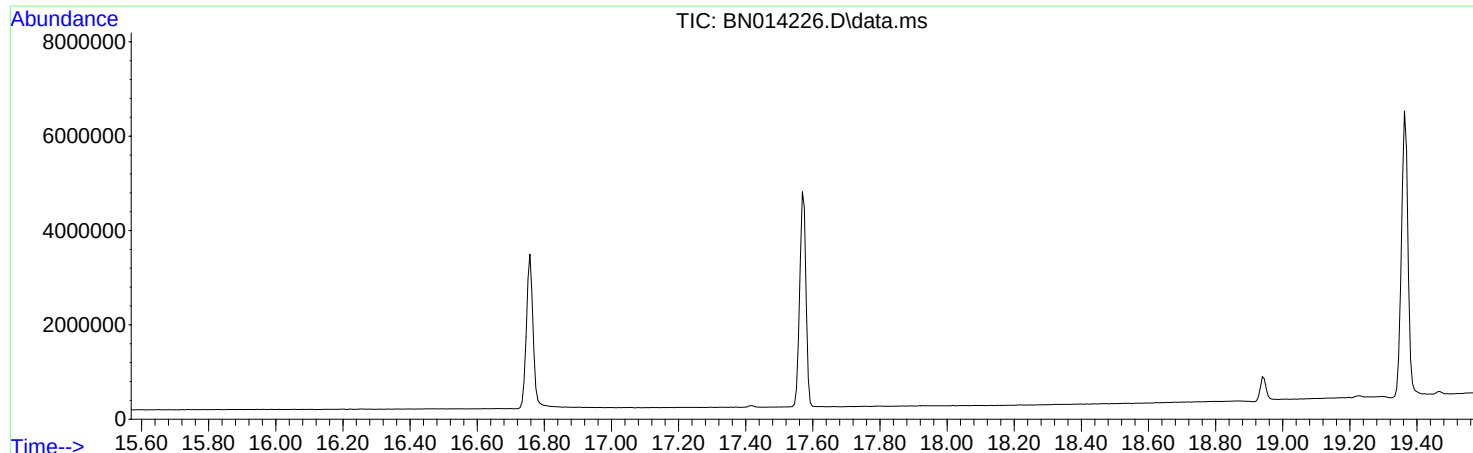




AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2454

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.5	138833	PASS
68	69	0.00	2	1.4	2242	PASS
69	198	0.00	100	37.1	163261	PASS
70	69	0.00	2	0.4	714	PASS
127	198	10	80	47.0	206886	PASS
197	198	0.00	2	0.5	2387	PASS
198	198	100	100	100.0	440128	PASS
199	198	5	9	6.9	30507	PASS
275	198	10	60	27.2	119717	PASS
365	198	1	100	3.7	16065	PASS
441	198	0.01	100	16.8	73923	PASS
442	442	50	100	100.0	461227	PASS
443	442	15	24	17.8	82243	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040821\
 Data File : BN014226.D
 Acq On : 07 Apr 2021 15:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Apr 07 17:07:28 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 26 11:50:50 2021
 Response via : Initial Calibration

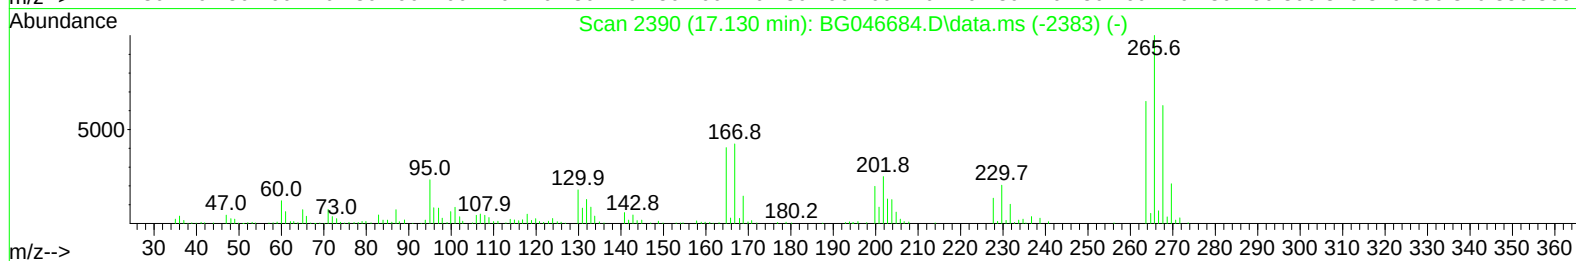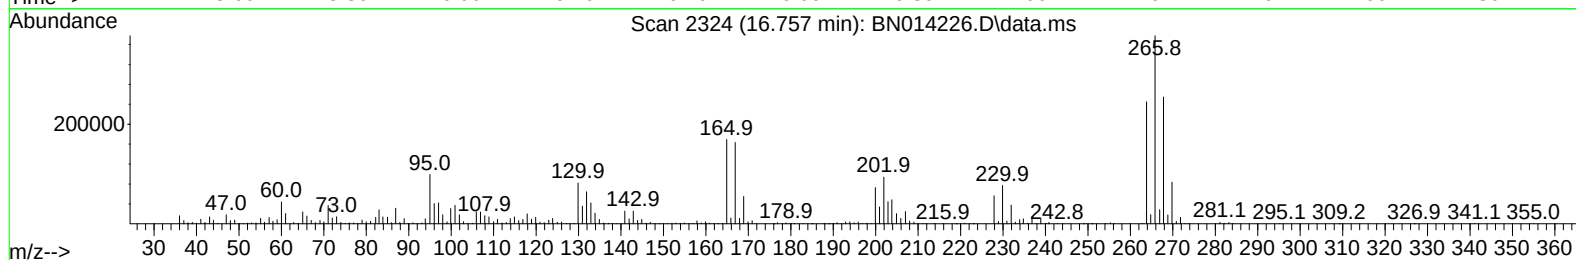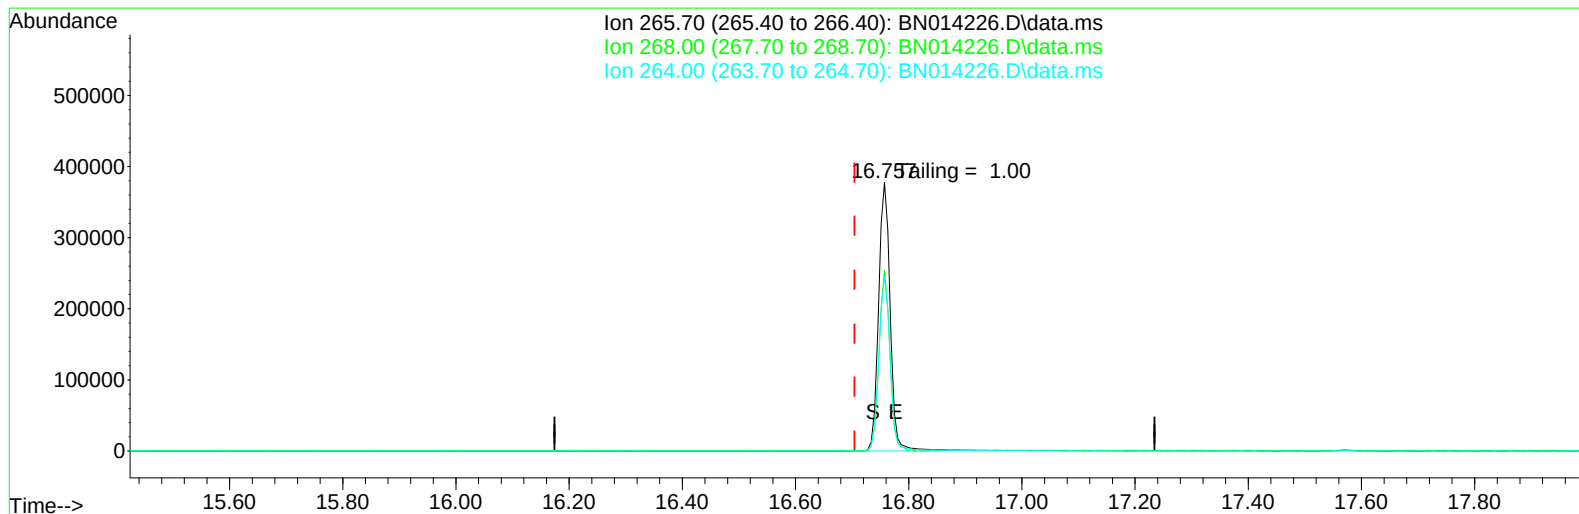

TIC: BN014226.D\data.ms

(70) Pentachlorophenol (C)

16.757min (+ 0.053) 26108.66 ng




response 536413

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	67.42
264.00	61.60	64.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040821\
Data File : BN014226.D
Acq On : 07 Apr 2021 15:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 07 17:07:28 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 26 11:50:50 2021
Response via : Initial Calibration

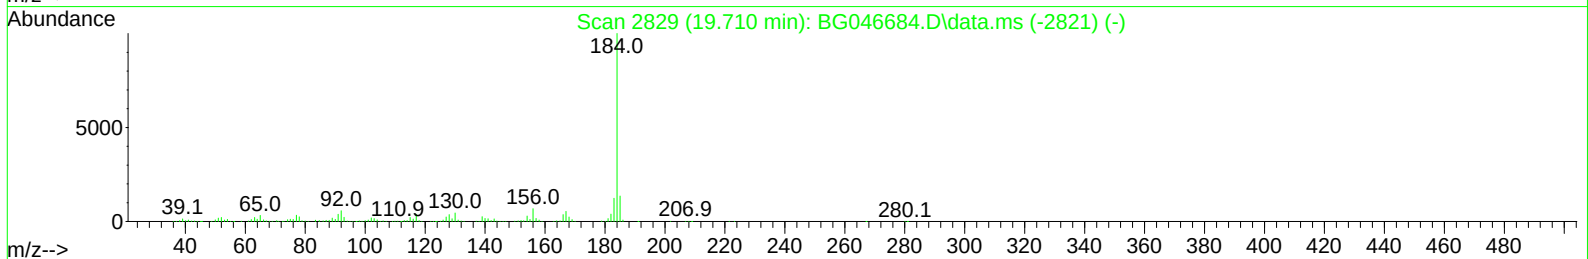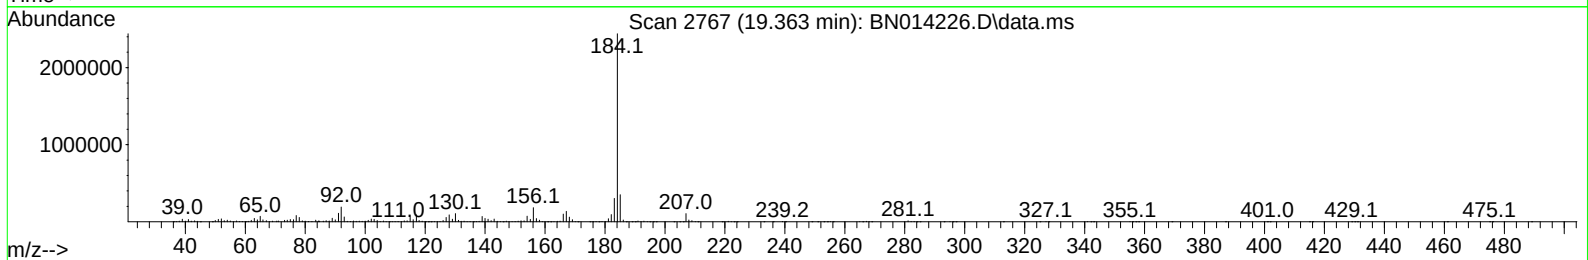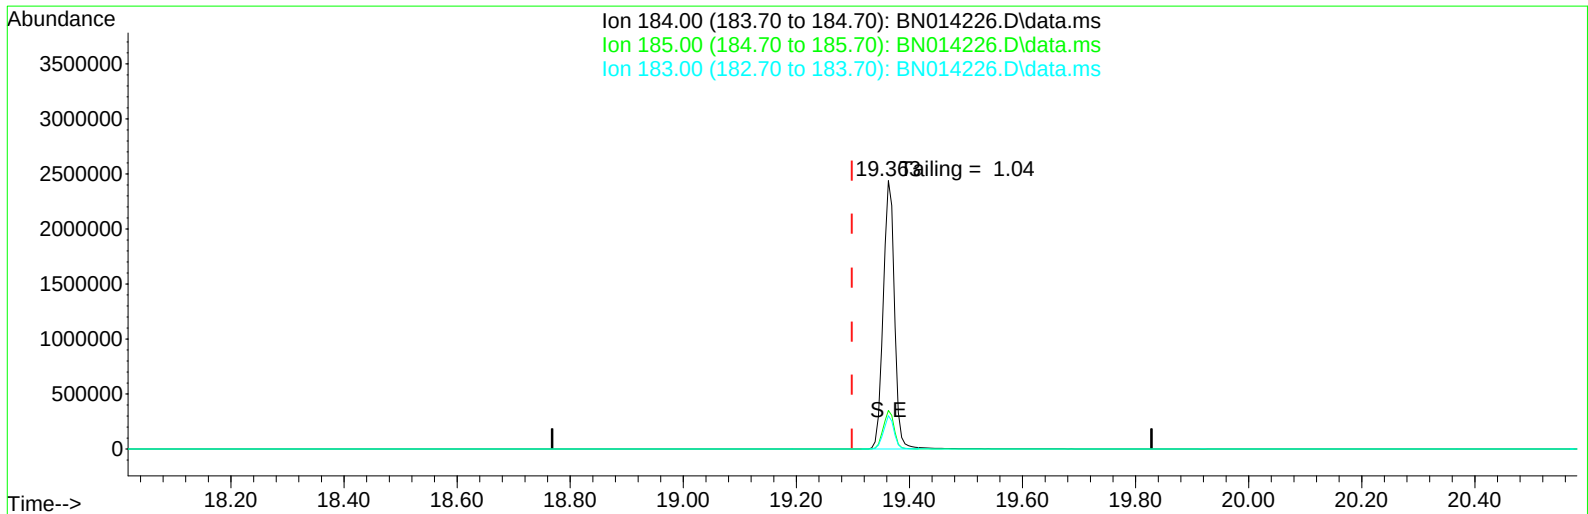

TIC: BN014226.D\data.ms

(77) Benzidine

19.363min (+ 0.065) 394889.18 ng

response 3396157

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.38
183.00	13.20	12.42
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/8/2021	BNA_N	<u>BN014226.D</u>
Compound Name	Response	Retention Time
DDT	1592280	20.61
DDD	9722	20.16
DDE	2055	19.65
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11777	1604057	0.73