
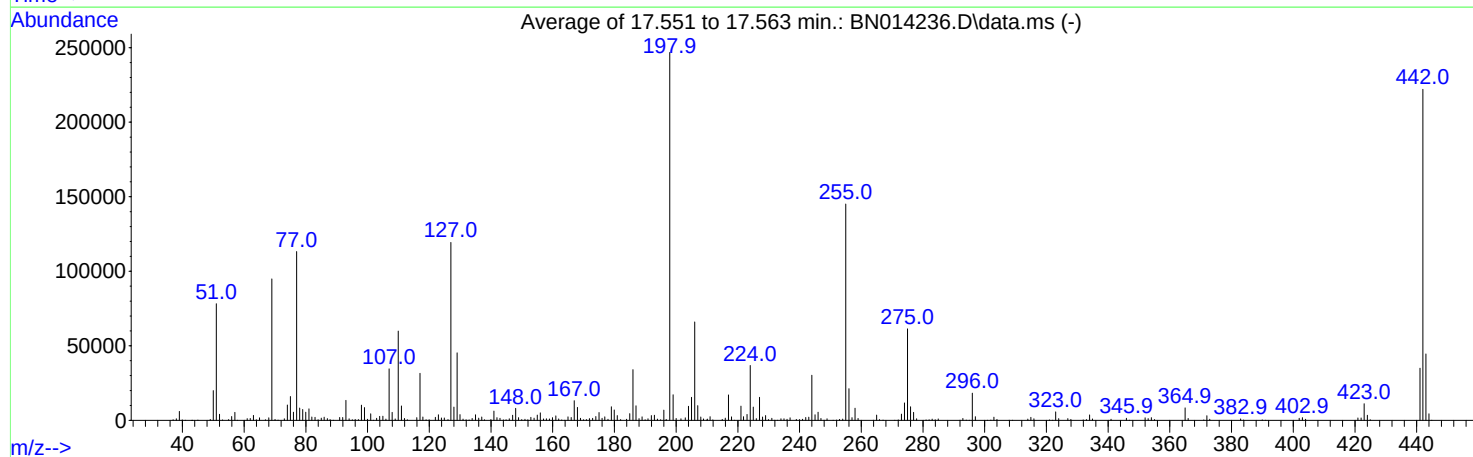


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040821\
 Data File : BN014236.D
 Acq On : 08 Apr 2021 08:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN040821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 08 01:18:45 2021

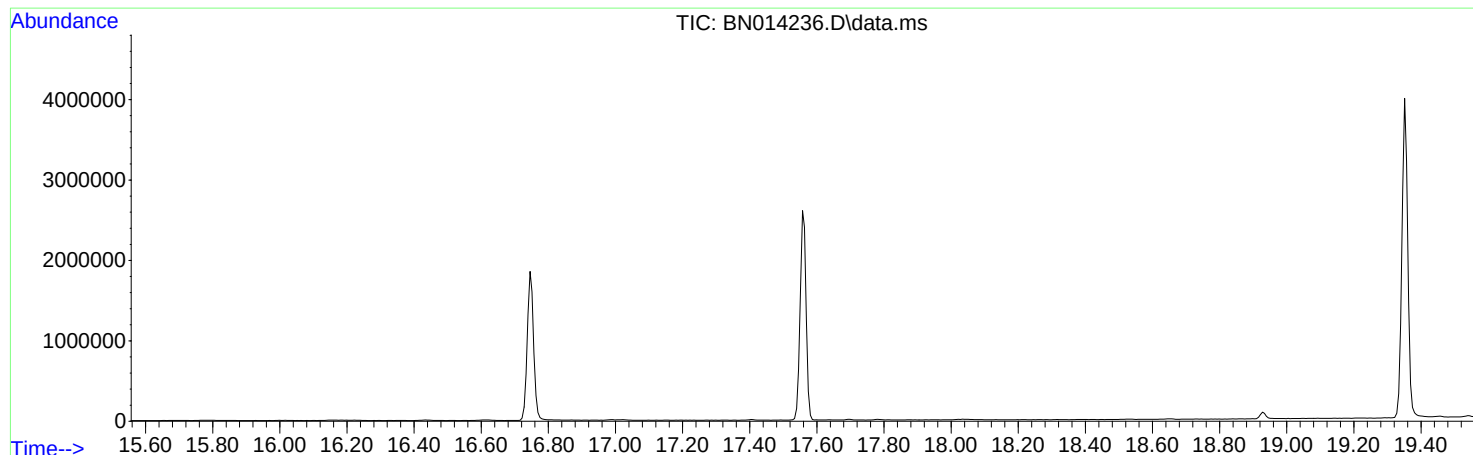




AutoFind: Scans 2459, 2460, 2461; Background Corrected with Scan 2453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.7	78227	PASS
68	69	0.00	2	1.8	1683	PASS
69	198	0.00	100	38.4	94853	PASS
70	69	0.00	2	0.7	693	PASS
127	198	10	80	48.4	119381	PASS
197	198	0.00	2	0.2	439	PASS
198	198	100	100	100.0	246741	PASS
199	198	5	9	7.0	17213	PASS
275	198	10	60	24.9	61429	PASS
365	198	1	100	3.4	8367	PASS
441	198	0.01	100	14.2	35040	PASS
442	442	50	100	100.0	222077	PASS
443	442	15	24	20.1	44568	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040821\
Data File : BN014236.D
Acq On : 08 Apr 2021 08:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 08 10:52:35 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 26 11:50:50 2021
Response via : Initial Calibration

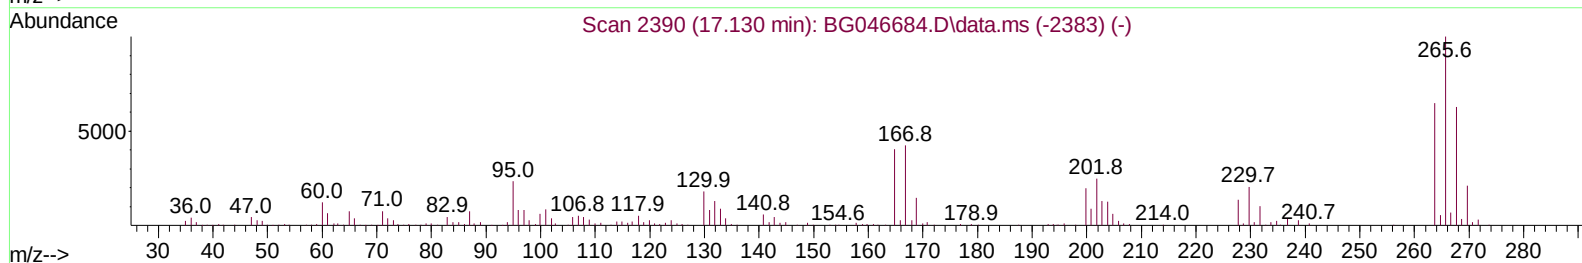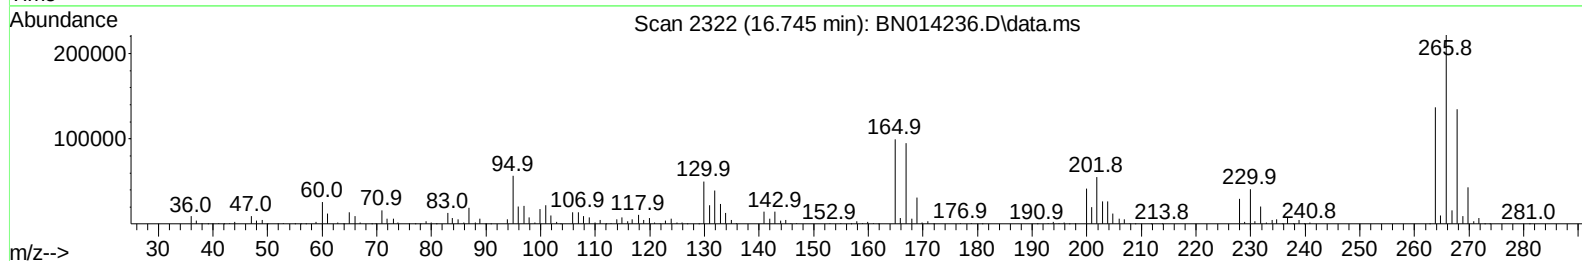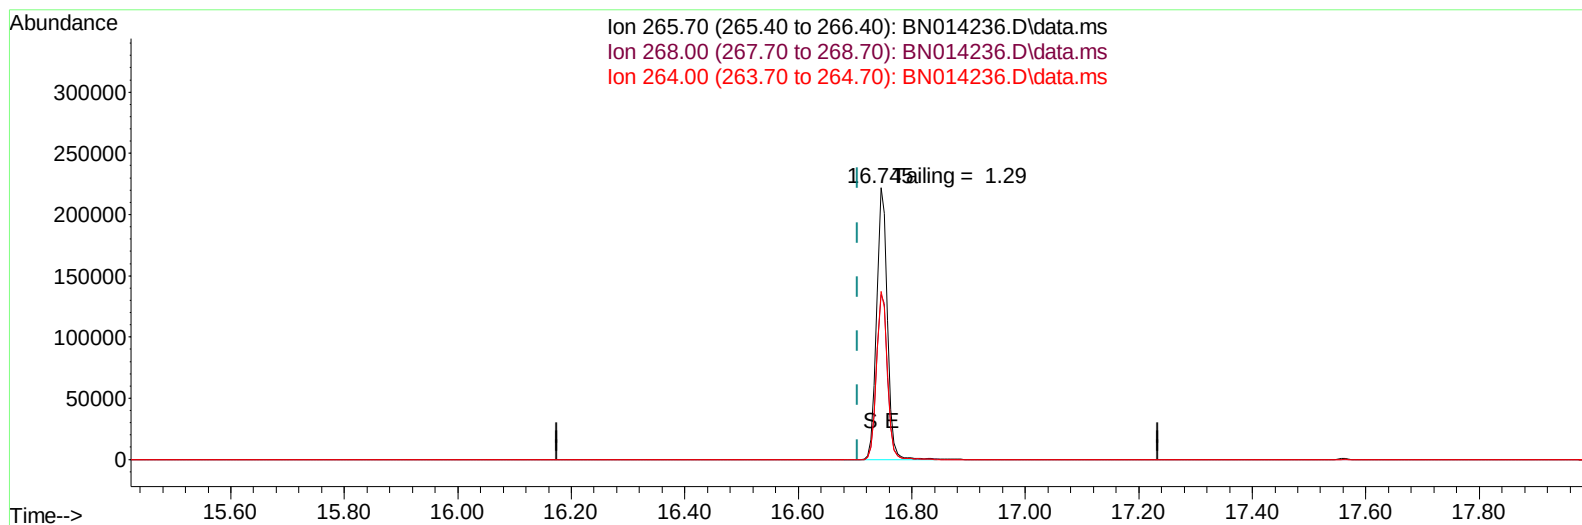

TIC: BN014236.D\data.ms

(70) Pentachlorophenol (C)

16.745min (+ 0.041) 23437.08 ng




response 289871

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.84
264.00	61.60	61.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040821\
Data File : BN014236.D
Acq On : 08 Apr 2021 08:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 08 10:52:35 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 26 11:50:50 2021
Response via : Initial Calibration

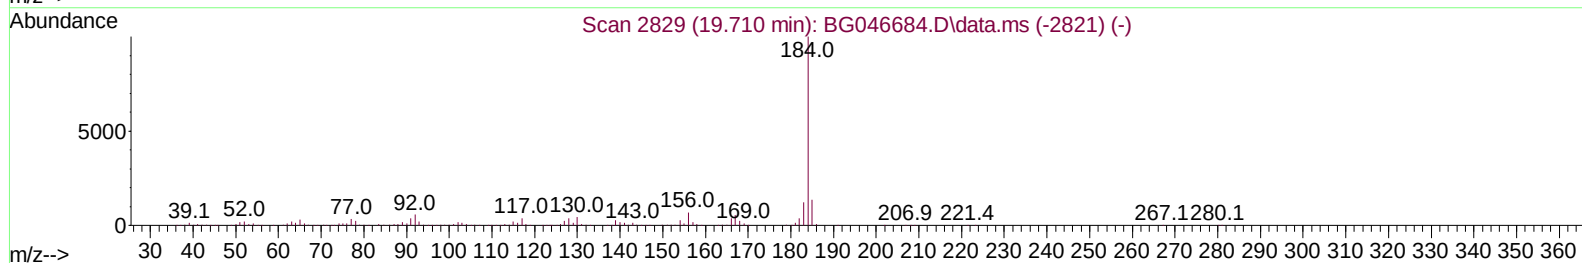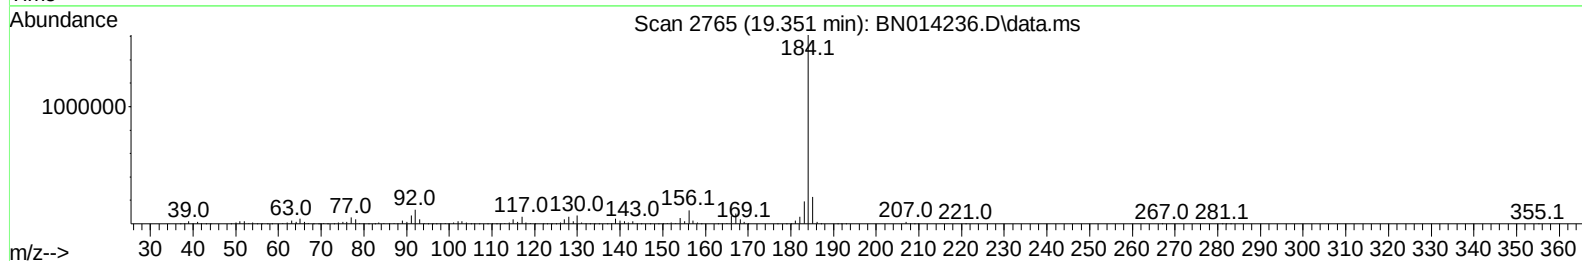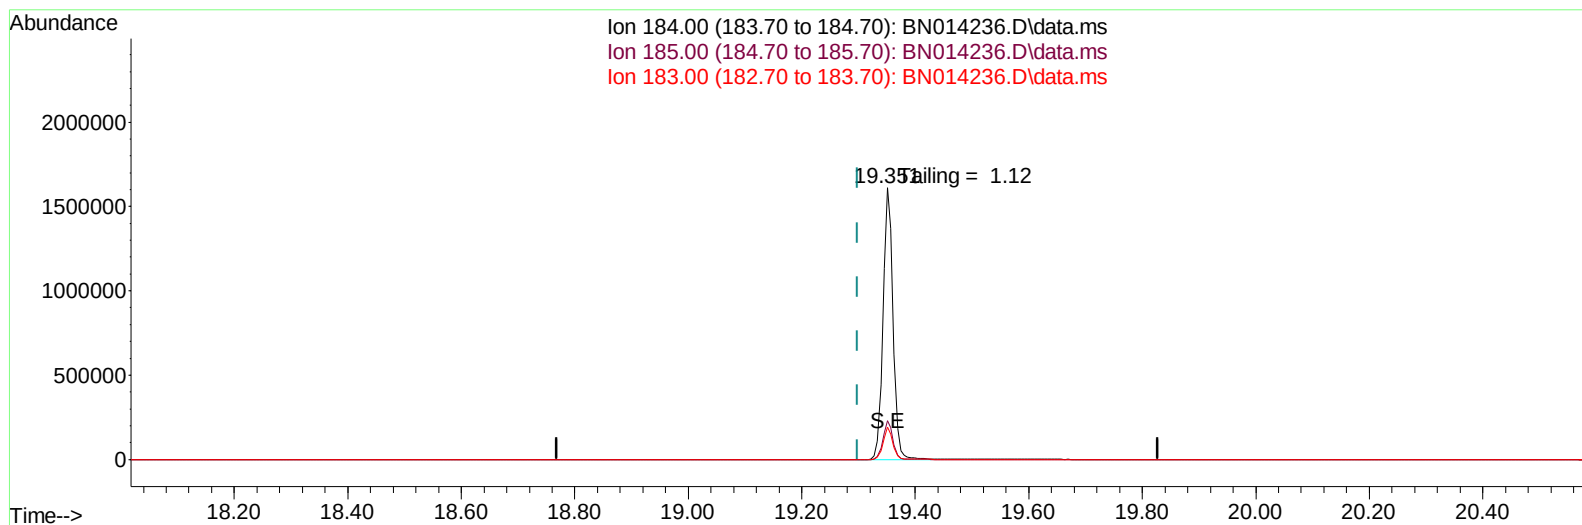

TIC: BN014236.D\data.ms

(77) Benzidine

19.351min (+ 0.053) 0.00 ng

response 1998070

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.29
183.00	13.20	11.86
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/8/2021	BNA_N	<u>BN014236.D</u>
Compound Name	Response	Retention Time
DDT	990216	20.598
DDD	4279	20.157
DDE	892	19.651
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5171	995387	0.52