

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041621\
 Data File : BN014308.D
 Acq On : 16 Apr 2021 14:09
 Operator : CG/JU
 Sample : SSTDICC0.8
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8

Quant Time: Apr 16 15:05:30 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN041621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 16 14:08:36 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.700	152	7119	0.40	ng	0.00
7) Naphthalene-d8	10.479	136	25632	0.40	ng	0.00
13) Acenaphthene-d10	14.333	164	12817	0.40	ng	0.00
19) Phenanthrene-d10	17.080	188	26365	0.40	ng	# 0.01
29) Chrysene-d12	21.271	240	28162	0.40	ng	0.00
36) Perylene-d12	23.499	264	22700	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.300	112	12317	0.73	ng	0.00
5) Phenol-d6	6.871	99	15228	0.72	ng	0.00
8) Nitrobenzene-d5	8.844	82	12951	0.80	ng	0.00
11) 2-Methylnaphthalene-d10	12.066	152	31217	0.78	ng	0.00
14) 2,4,6-Tribromophenol	15.818	330	3492	0.70	ng	0.00
15) 2-Fluorobiphenyl	12.950	172	43050	0.92	ng	0.00
27) Fluoranthene-d10	19.109	212	56803	0.74	ng	0.00
31) Terphenyl-d14	19.714	244	48319	0.78	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.263	88	6905	0.76	ng	91
3) n-Nitrosodimethylamine	3.601	42	3837	0.90	ng	99
6) bis(2-Chloroethyl)ether	7.128	93	14492	0.84	ng	99
9) Naphthalene	10.517	128	51679	0.81	ng	100
10) Hexachlorobutadiene	10.822	225	10298	0.81	ng	# 100
12) 2-Methylnaphthalene	12.142	142	33644	0.79	ng	100
16) Acenaphthylene	14.041	152	37804	0.77	ng	99
17) Acenaphthene	14.397	154	29359	0.81	ng	99
18) Fluorene	15.374	166	35603	0.78	ng	99
20) 4,6-Dinitro-2-methylph...	15.450	198	2173	0.70	ng	# 71
21) 4-Bromophenyl-phenylether	16.276	248	11193	0.83	ng	98
22) Hexachlorobenzene	16.386	284	14566	0.85	ng	100
23) Atrazine	16.544	200	6459	0.64	ng	99
24) Pentachlorophenol	16.727	266	3537	0.67	ng	99
25) Phenanthrene	17.116	178	58529	0.80	ng	100
26) Anthracene	17.201	178	45835	0.76	ng	100
28) Fluoranthene	19.139	202	64237	0.77	ng	100
30) Pyrene	19.506	202	63083	0.71	ng	100
32) Benzo(a)anthracene	21.250	228	56285	0.70	ng	100
33) Chrysene	21.303	228	68601	0.79	ng	100
34) Bis(2-ethylhexyl)phtha...	21.197	149	15173	0.53	ng	100
35) Indeno(1,2,3-cd)pyrene	25.741	276	79566	0.78	ng	99
37) Benzo(b)fluoranthene	22.828	252	73962	0.92	ng	98
38) Benzo(k)fluoranthene	22.873	252	71918	0.89	ng	98
39) Benzo(a)pyrene	23.400	252	55924	0.82	ng	96
40) Dibenzo(a,h)anthracene	25.755	278	66492	0.85	ng	99
41) Benzo(g,h,i)perylene	26.426	276	71068	0.89	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041621\
Data File : BN014308.D
Acq On : 16 Apr 2021 14:09
Operator : CG/JU
Sample : SSTDICC0.8
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8

Quant Time: Apr 16 15:05:30 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN041621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 16 14:08:36 2021
Response via : Initial Calibration




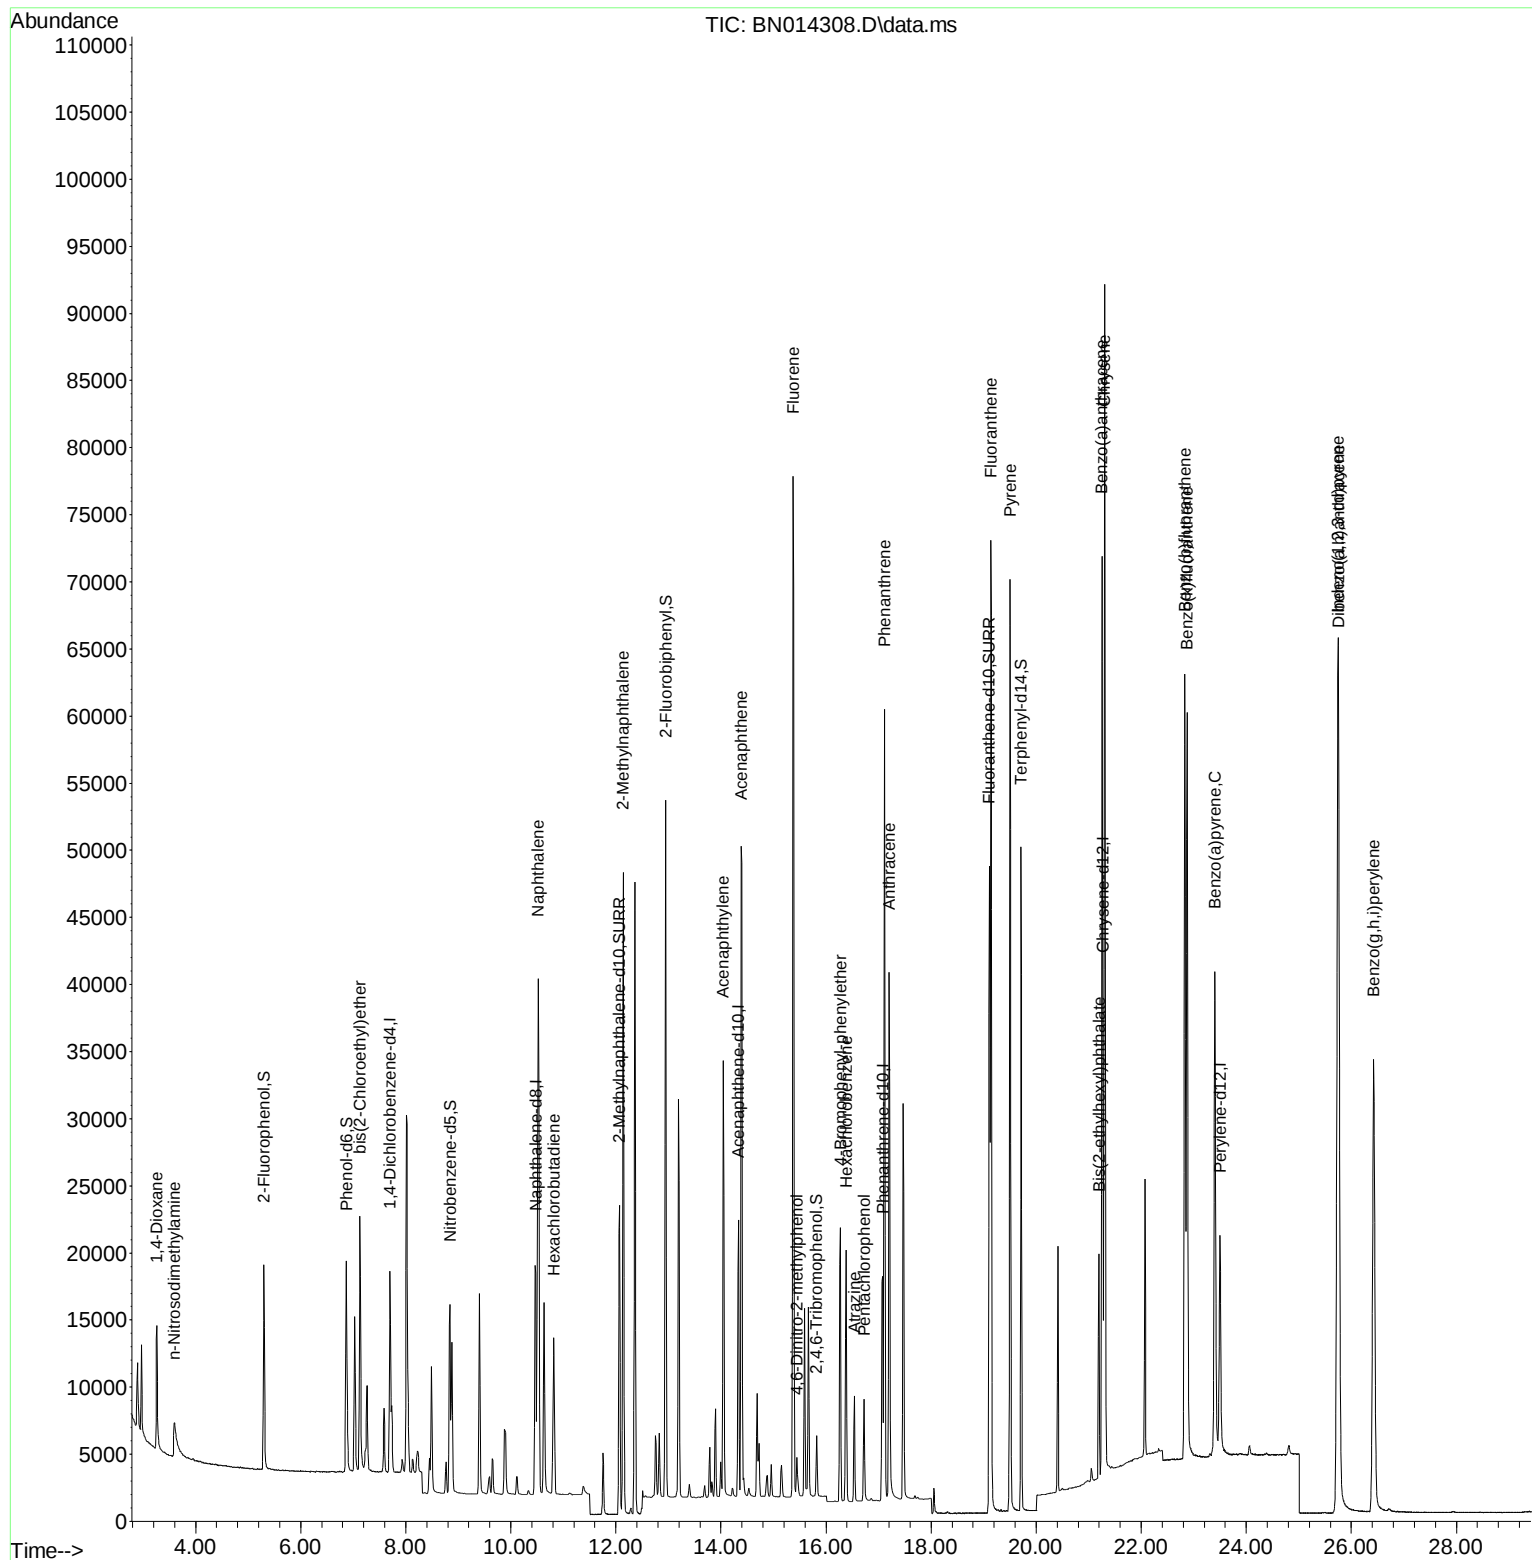


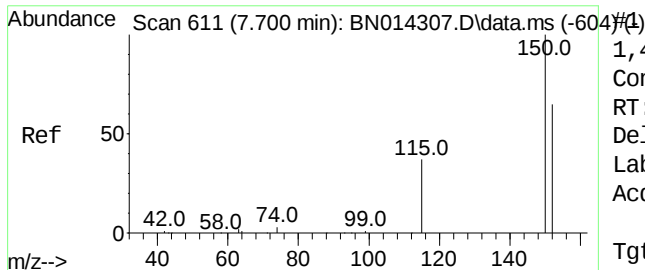

1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.700 min Scan# 611
 Delta R.T. 0.000 min
 Lab File: BN014308.D
 Acq: 16 Apr 2021 14:09




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8


Tgt Ion:	152	Resp:	7119
Ion	Ratio	Lower	Upper
152	100		
150	152.9	123.0	184.4
115	59.1	47.6	71.4

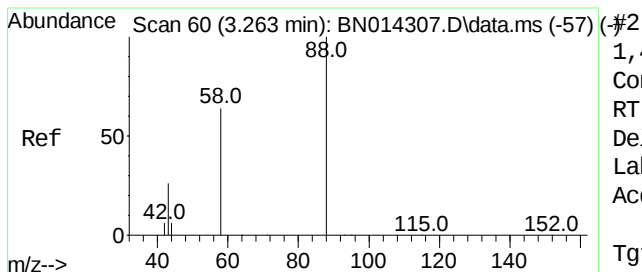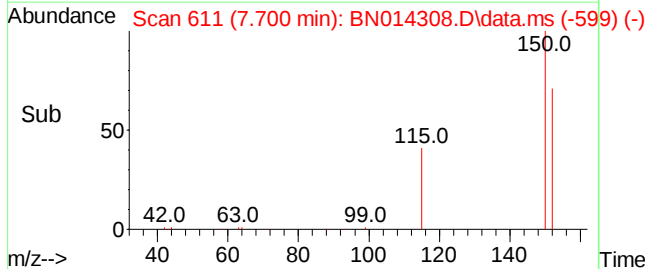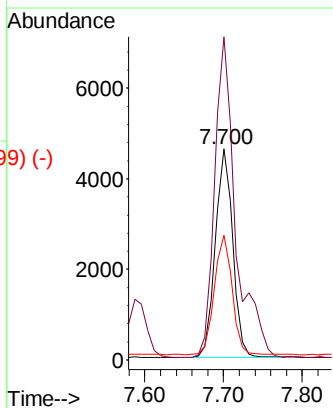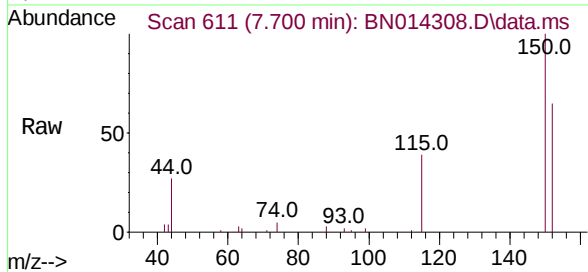

1,4-Dioxane
 Concen: 0.76 ng
 RT: 3.263 min Scan# 60
 Delta R.T. -0.000 min
 Lab File: BN014308.D
 Acq: 16 Apr 2021 14:09

Tgt Ion:	88	Resp:	6905
Ion	Ratio	Lower	Upper
88	100		
58	67.8	47.3	70.9
43	26.7	20.6	31.0


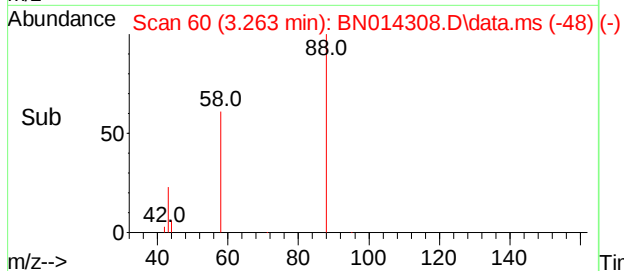

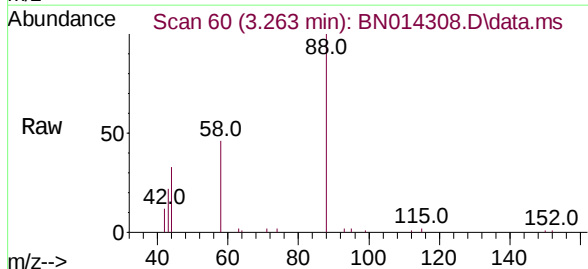


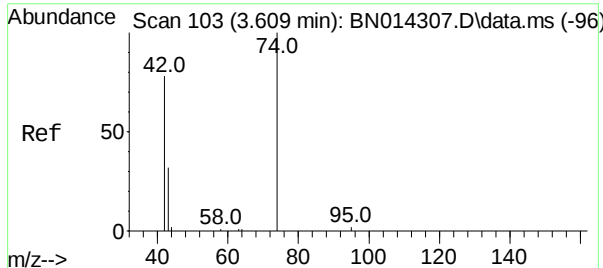

n-Nitrosodimethylamine
Concen: 0.90 ng
RT: 3.601 min Scan# 102
Delta R.T. -0.008 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion: 42 Resp: 3837
Ion Ratio Lower Upper
42 100
74 131.9 104.6 157.0
44 3.3 2.4 3.6

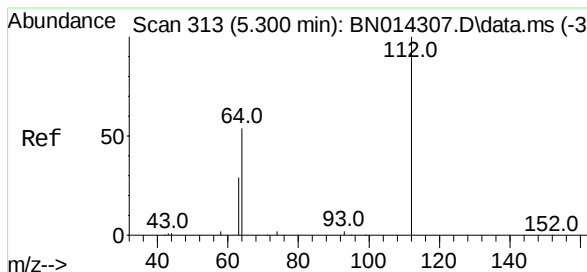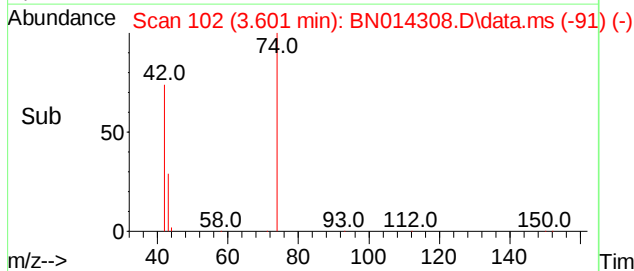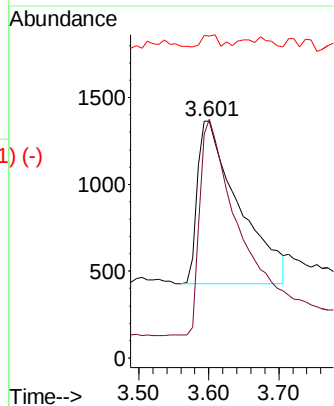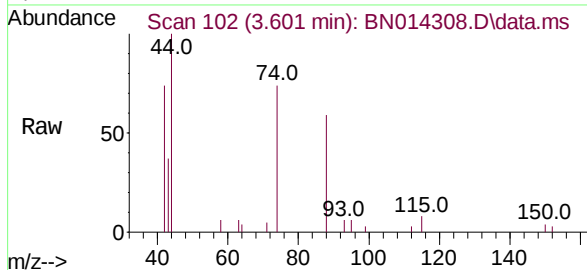

2-Fluorophenol
Concen: 0.73 ng
RT: 5.300 min Scan# 313
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09

Tgt Ion:112 Resp: 12317
Ion Ratio Lower Upper
112 100
64 55.0 43.7 65.5
63 29.7 23.8 35.8


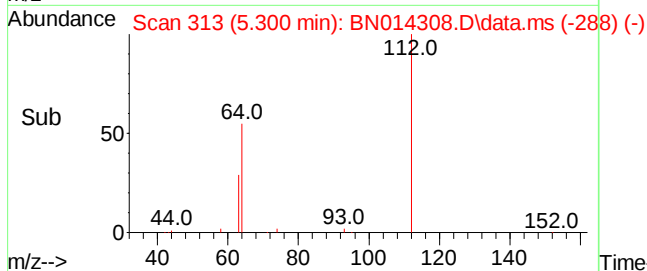
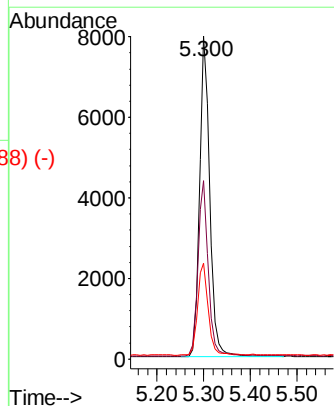
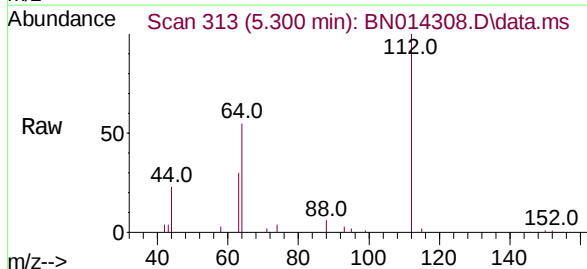


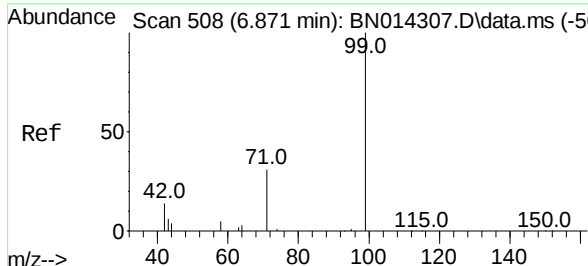

Phenol-d6
 Concen: 0.72 ng
 RT: 6.871 min Scan# 508
 Delta R.T. -0.000 min
 Lab File: BN014308.D
 Acq: 16 Apr 2021 14:09




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8

Tgt Ion:	99	Resp:	15228
Ion	Ratio	Lower	Upper
99	100		
42	19.3	15.7	23.5
71	34.6	27.6	41.4

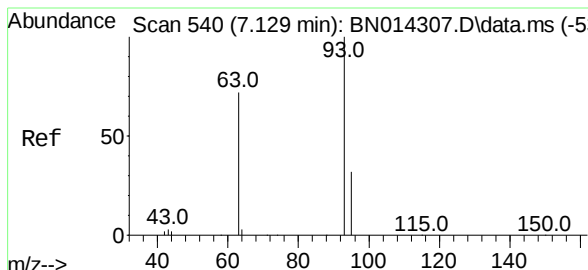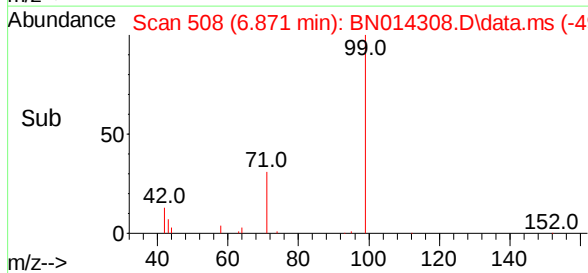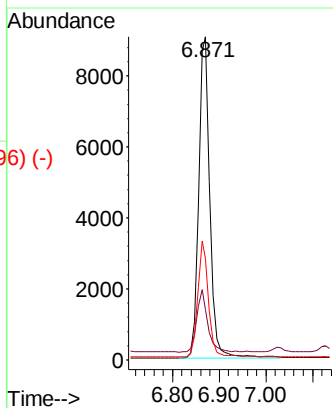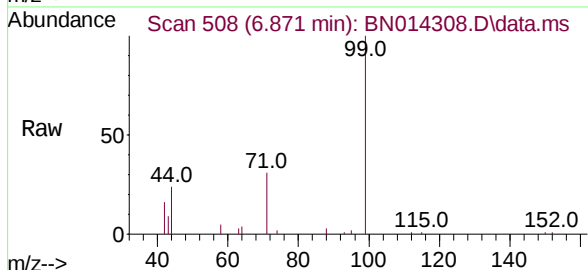


bis(2-Chloroethyl)ether
 Concen: 0.84 ng
 RT: 7.128 min Scan# 540
 Delta R.T. -0.000 min
 Lab File: BN014308.D
 Acq: 16 Apr 2021 14:09

Tgt Ion:	93	Resp:	14492
Ion	Ratio	Lower	Upper
93	100		
63	73.8	58.2	87.4
95	33.4	26.7	40.1

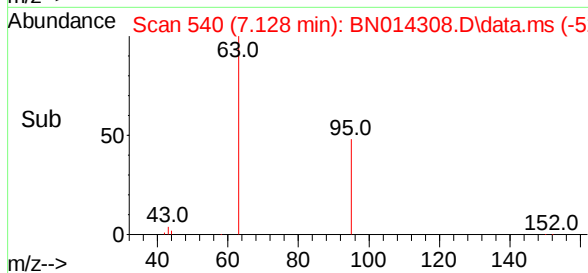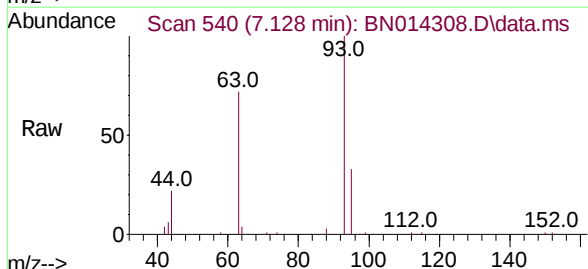




Abundance Scan 858 (10.480 min): BN014307.D\data.ms (-857-)

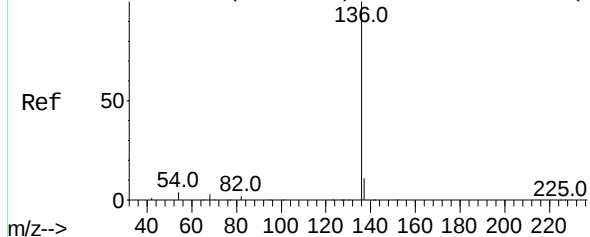


Naphthalene-d8
Concen: 0.40 ng
RT: 10.479 min Scan# 858
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8

Tgt Ion:	136	Resp:	25632
Ion	Ratio	Lower	Upper
136	100		
137	11.1	9.0	13.6
54	4.6	3.5	5.3
68	4.1	3.4	5.2

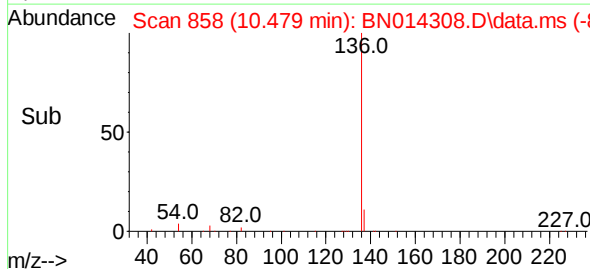
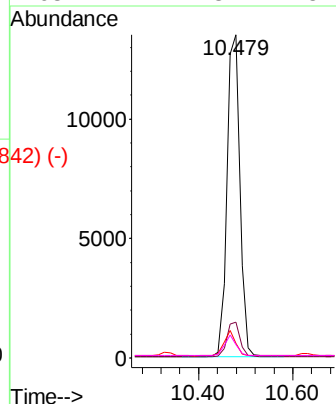
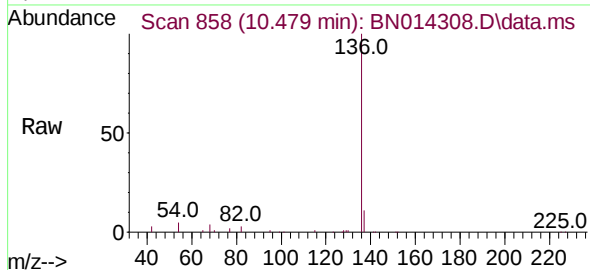


Abundance Scan 729 (8.845 min): BN014307.D\data.ms (-725#)

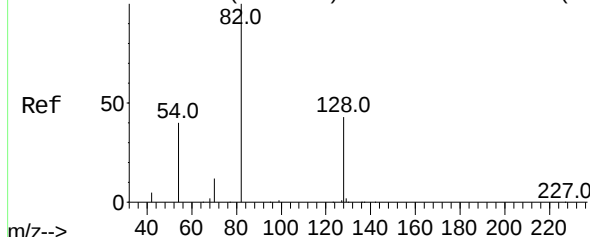

Nitrobenzene-d5
Concen: 0.80 ng
RT: 8.844 min Scan# 729
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09


Tgt Ion:	82	Resp:	12951
Ion	Ratio	Lower	Upper
82	100		
128	42.6	35.3	52.9
54	40.4	33.4	50.2

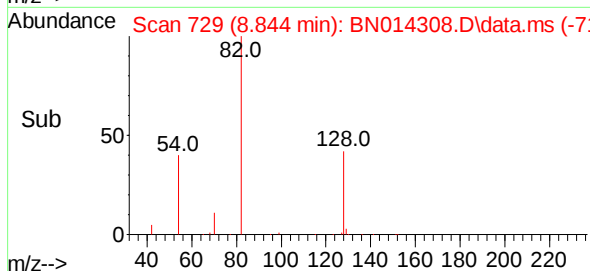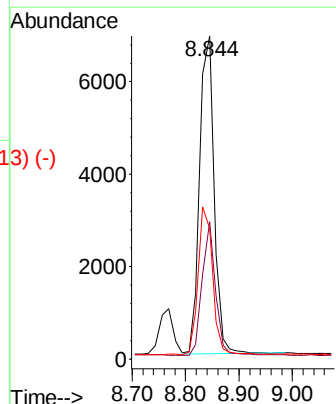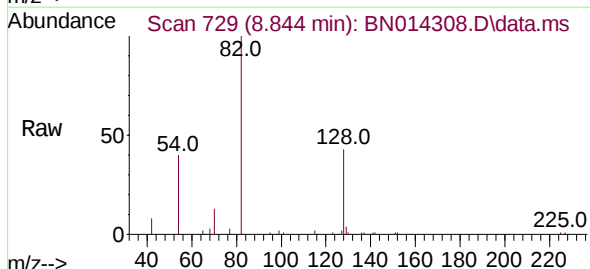




Abundance Scan 861 (10.518 min): BN014307.D\data.ms (-856) (-)

Naphthalene
Concen: 0.81 ng
RT: 10.517 min Scan# 861
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09

Instrument :
BNA_N
ClientSampled :
SSTDIC0.8

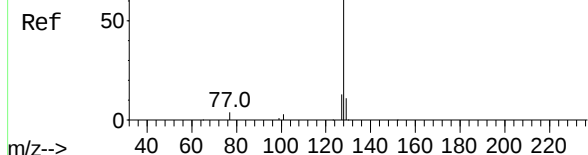


Tgt Ion:	128	Resp:	51679
Ion	Ratio	Lower	Upper
128	100		
129	11.1	9.0	13.4
127	13.2	10.7	16.1

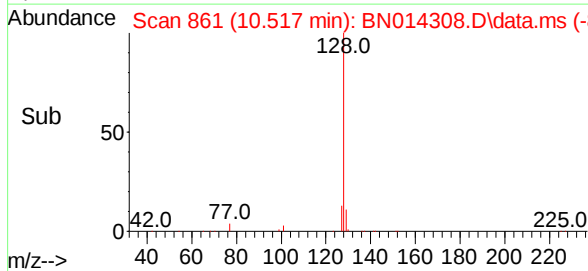
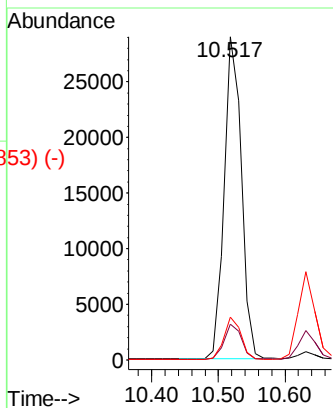
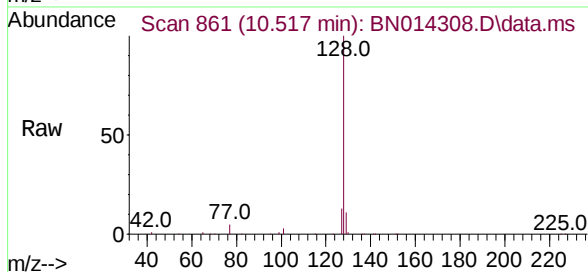


Abundance Scan 885 (10.822 min): BN014307.D\data.ms (-886) (-)

Hexachlorobutadiene
Concen: 0.81 ng
RT: 10.822 min Scan# 885
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09

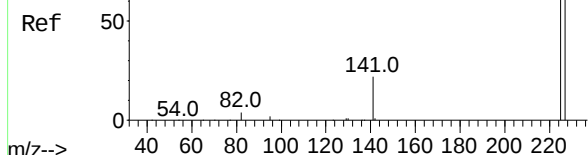


Tgt Ion:	225	Resp:	10298
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	63.6	50.9	76.3

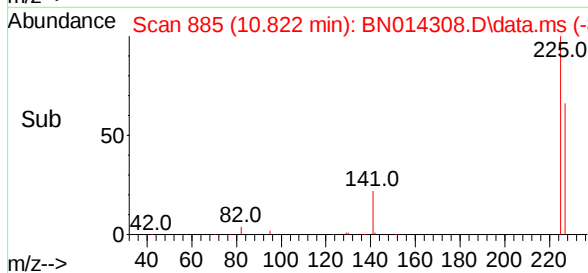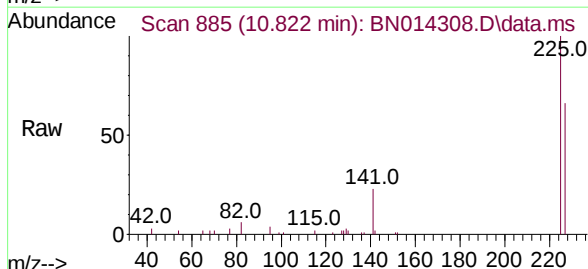



Abundance Scan 1065 (12.066 min): BN014307.D\data.ms (-1032) (-)

2-Methylnaphthalene-d10
Concen: 0.78 ng
RT: 12.066 min Scan# 1065
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09


Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8

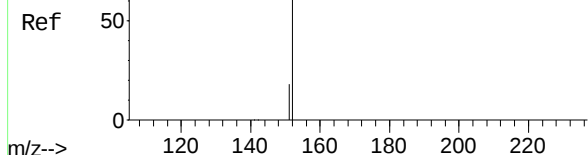

Tgt Ion:152 Resp: 31217
Ion Ratio Lower Upper
152 100
151 20.2 16.2 24.4

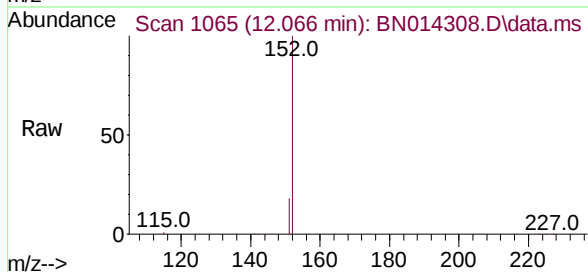




Abundance Scan 1065 (12.066 min): BN014308.D\data.ms (-1020) (-)

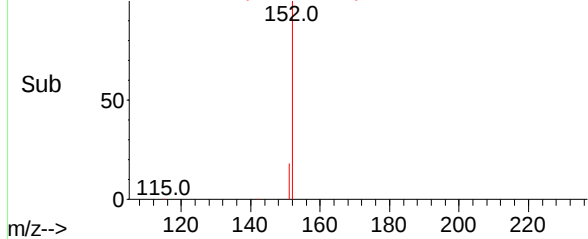


Abundance Scan 1082 (12.142 min): BN014307.D\data.ms (-1070) (-)

2-Methylnaphthalene
Concen: 0.79 ng
RT: 12.142 min Scan# 1082
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09

Tgt Ion:142 Resp: 33644
Ion Ratio Lower Upper
142 100
141 87.8 70.0 105.0
115 35.5 28.8 43.2

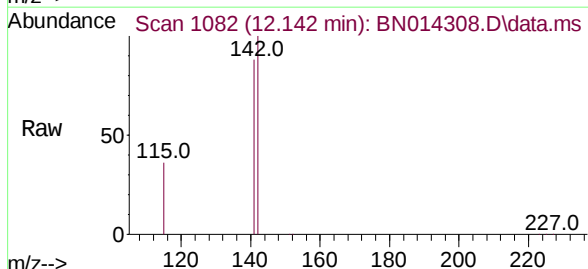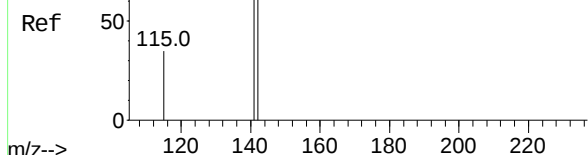


Abundance Scan 1082 (12.142 min): BN014308.D\data.ms (-1060) (-)

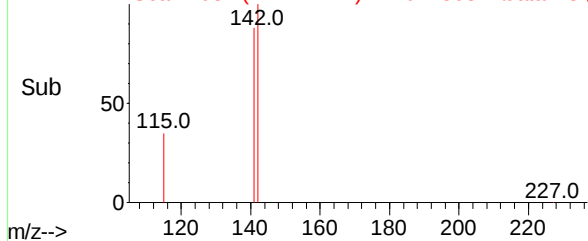



Abundance Scan 1308 (14.334 min): BN014307.D\data.ms (-1219) (-)

Acenaphthene-d10
Concen: 0.40 ng
RT: 14.333 min Scan# 1308
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09


Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8

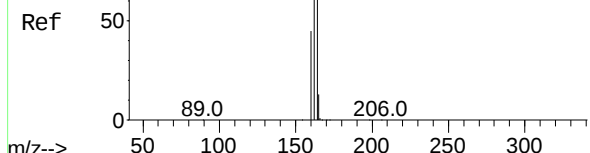

Tgt Ion:	164	Resp:	12817
Ion Ratio	Lower	Upper	
164	100		
162	99.5	78.6	117.8
160	45.2	36.2	54.4

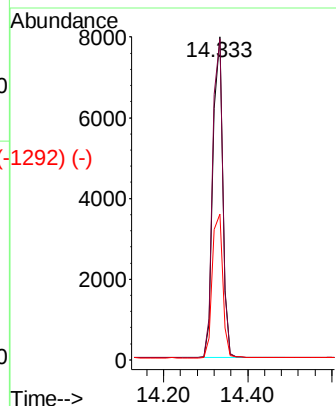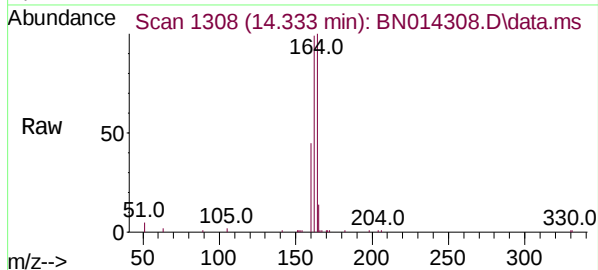



Abundance Scan 1308 (14.333 min): BN014308.D\data.ms (-1292) (-)

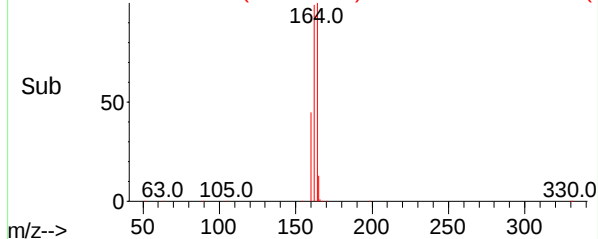


Abundance Scan 1425 (15.818 min): BN014307.D\data.ms (-1417) (-)


2,4,6-Tribromophenol
Concen: 0.70 ng
RT: 15.818 min Scan# 1425
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09

Tgt Ion:	330	Resp:	3492
Ion Ratio	Lower	Upper	
330	100		
332	0.0	0.0	0.0
141	33.6	28.8	43.2

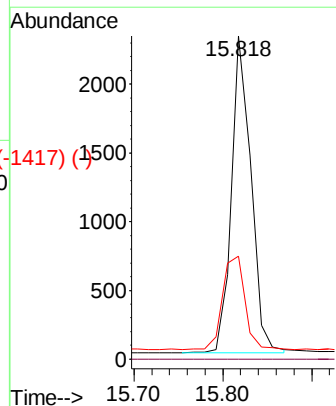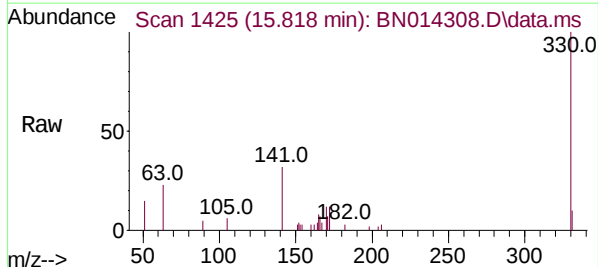

Abundance Scan 1425 (15.818 min): BN014308.D\data.ms (-1417) (-)




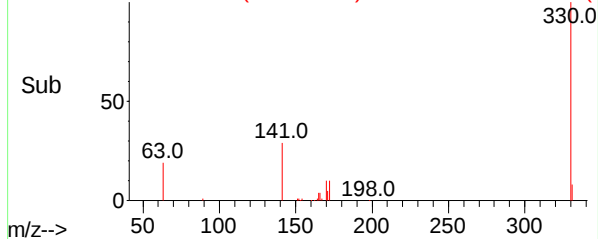


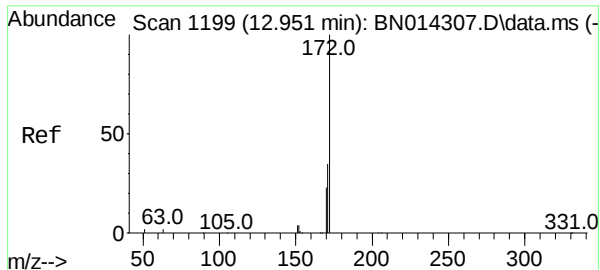

2-Fluorobiphenyl
Concen: 0.92 ng
RT: 12.950 min Scan# 1199
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8

Tgt Ion:	172	Resp:	43050
Ion	Ratio	Lower	Upper
172	100		
171	34.2	27.9	41.9
170	23.2	18.8	28.2

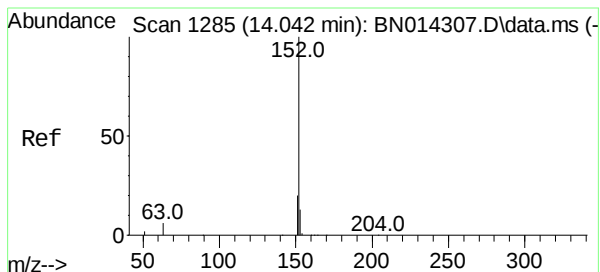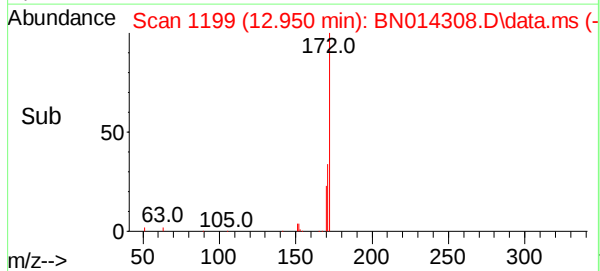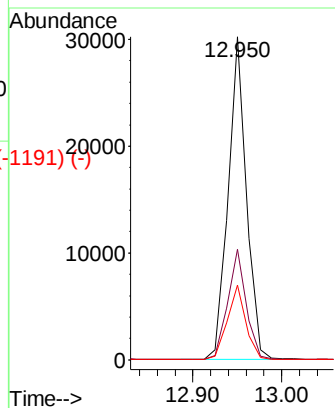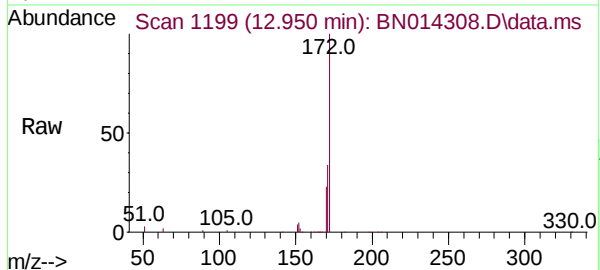

Acenaphthylene
Concen: 0.77 ng
RT: 14.041 min Scan# 1285
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09


Tgt Ion:	152	Resp:	37804
Ion	Ratio	Lower	Upper
152	100		
151	19.5	15.9	23.9
153	13.0	10.6	15.8

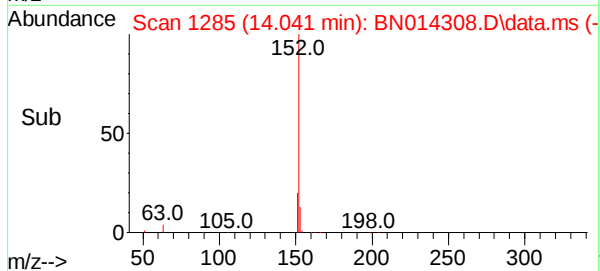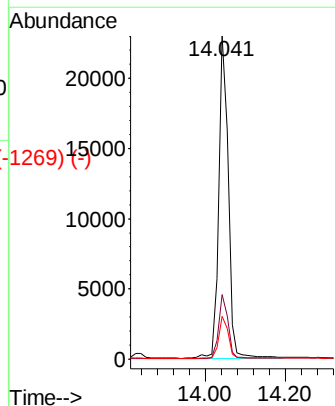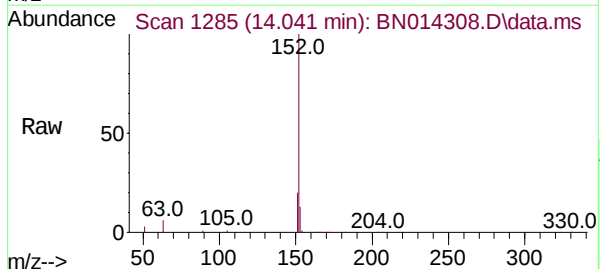




Abundance Scan 1312 (14.384 min): BN014307.D\data.ms (-1304) (-)

Acenaphthene
Concen: 0.81 ng
RT: 14.397 min Scan# 1313
Delta R.T. 0.012 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09

Instrument :
BNA_N
ClientSampled :
SSTDIC0.8

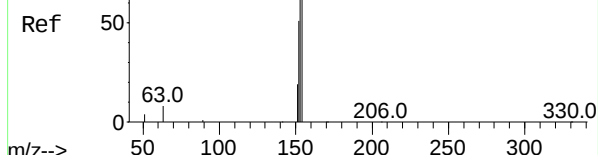


Tgt Ion	Ratio	Lower	Upper
154	100		
153	110.2	89.4	134.2
152	55.0	44.7	67.1

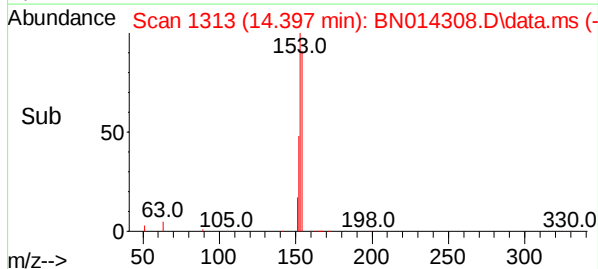

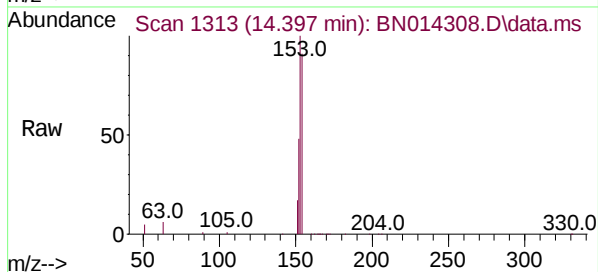


Abundance Scan 1390 (15.374 min): BN014307.D\data.ms (-1374) (-)

Fluorene
Concen: 0.78 ng
RT: 15.374 min Scan# 1390
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09

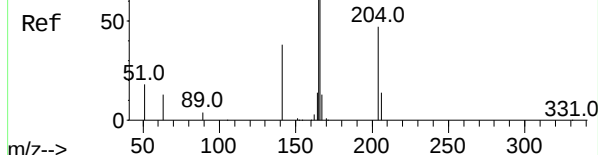


Tgt Ion	Ratio	Lower	Upper
166	100		
165	98.5	78.2	117.2
167	13.4	10.9	16.3

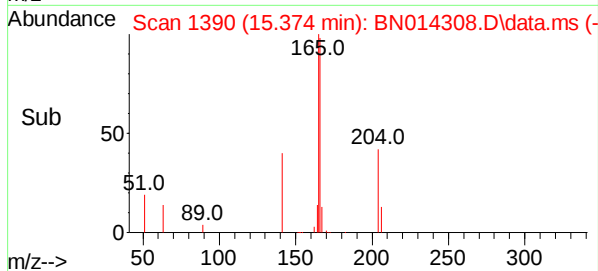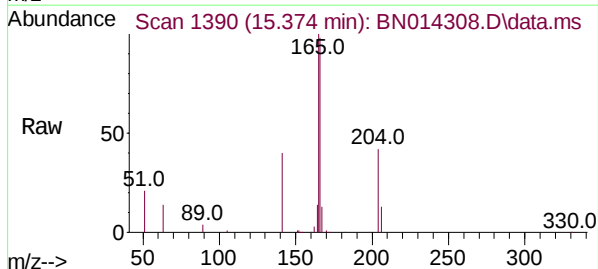




Abundance Scan 1527 (17.068 min): BN014307.D\data.ms (-1511) (-)

Phenanthrene-d10
Concen: 0.40 ng
RT: 17.080 min Scan# 1528
Delta R.T. 0.012 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09

Instrument :
BNA_N
ClientSampled :
SSTDIC0.8

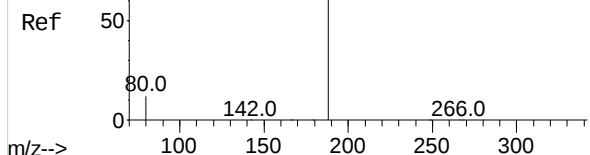


Tgt Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	6.2	10.2	15.4#

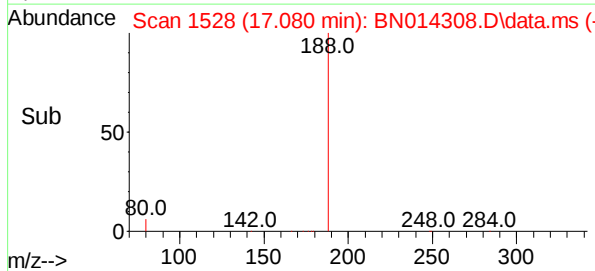
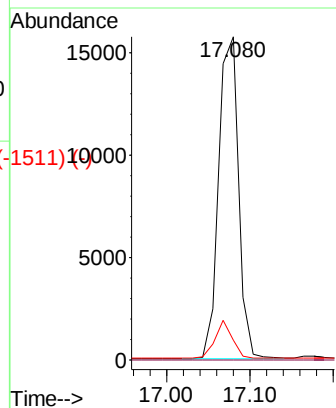
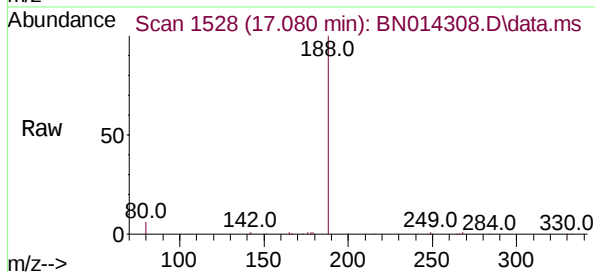


Abundance Scan 1396 (15.450 min): BN014307.D\data.ms (-1322) (-)


4,6-Dinitro-2-methylphenol
Concen: 0.70 ng
RT: 15.450 min Scan# 1396
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09

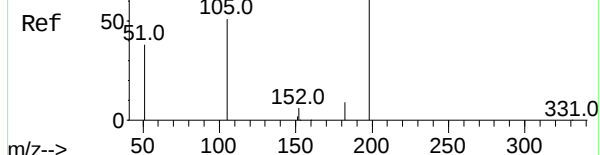

Tgt Ion	Ratio	Lower	Upper
198	100		
51	65.2	82.6	123.8#
105	56.0	56.1	84.1#

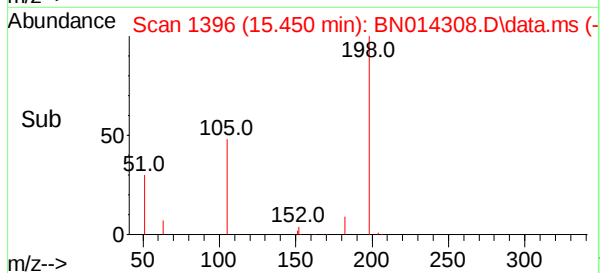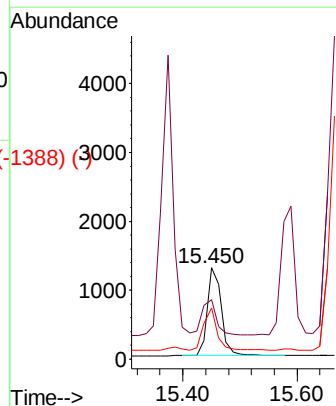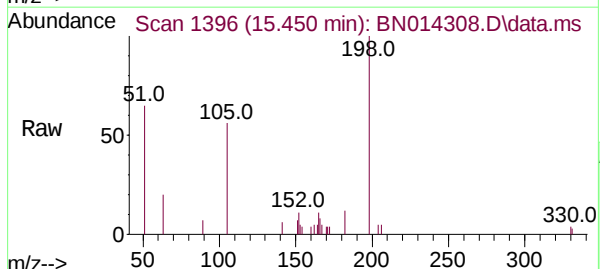



Abundance Scan 1462 (16.277 min): BN014307.D\data.ms (-1425) (-)

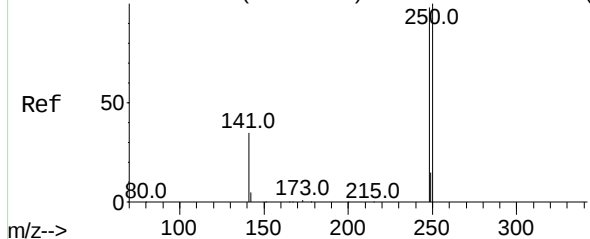


4-Bromophenyl-phenylether
Concen: 0.83 ng
RT: 16.276 min Scan# 1462
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion	Ratio	Lower	Upper
248	100		
250	104.5	81.9	122.9
141	36.8	29.3	43.9

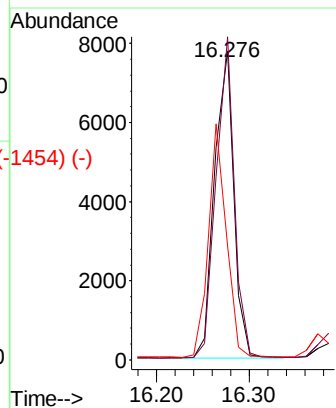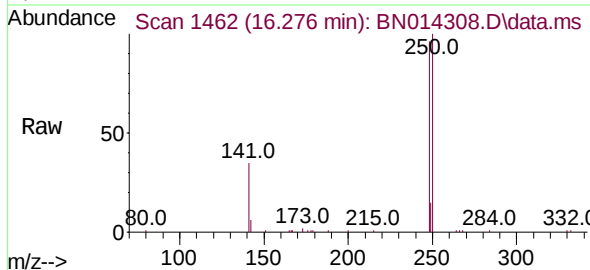

Abundance Scan 1462 (16.276 min): BN014308.D\data.ms (-1454) (-)


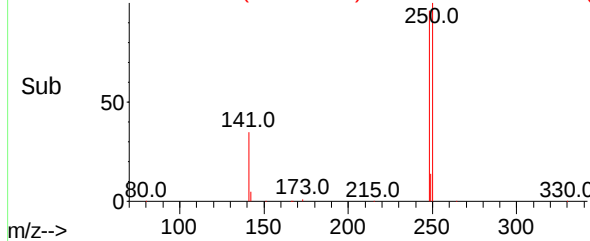


Abundance Scan 1471 (16.386 min): BN014307.D\data.ms (-1422) (-)

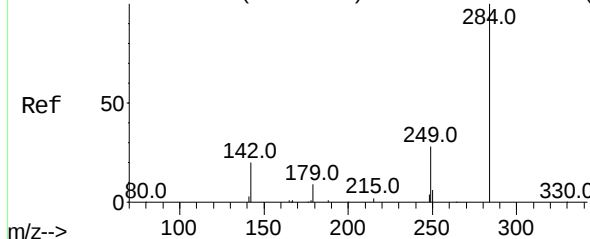


Hexachlorobenzene
Concen: 0.85 ng
RT: 16.386 min Scan# 1471
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09

Tgt Ion	Ratio	Lower	Upper
284	100		
142	33.7	27.0	40.6
249	29.6	23.7	35.5

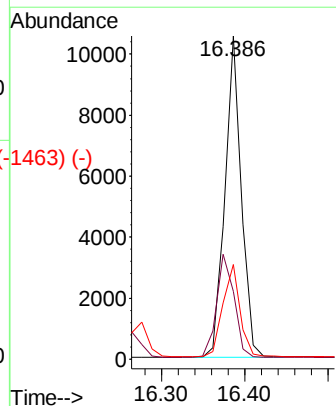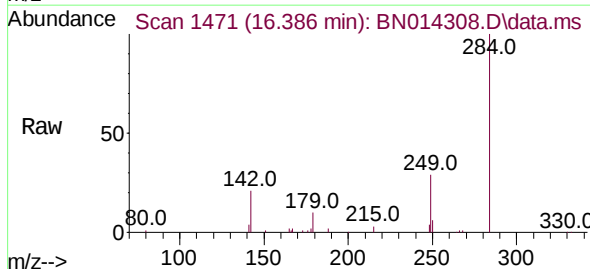


Abundance Scan 1471 (16.386 min): BN014308.D\data.ms (-1463) (-)

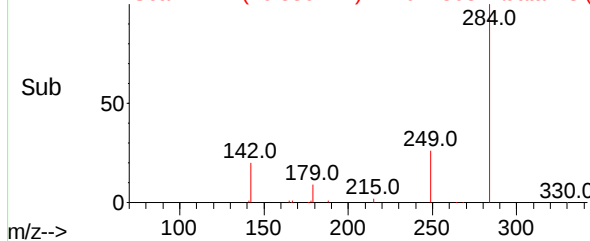



Abundance Scan 1484 (16.544 min): BN014307.D\data.ms (-1428) (-)

Atrazine
Concen: 0.64 ng
RT: 16.544 min Scan# 1484
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09


Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8

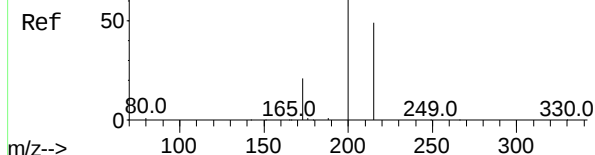

Tgt Ion:	200	Resp:	6459
Ion Ratio	Lower	Upper	
200	100		
173	22.6	18.5	27.7
215	49.4	40.0	60.0

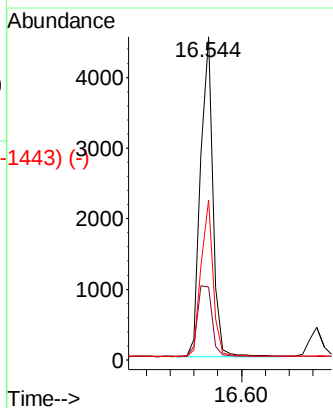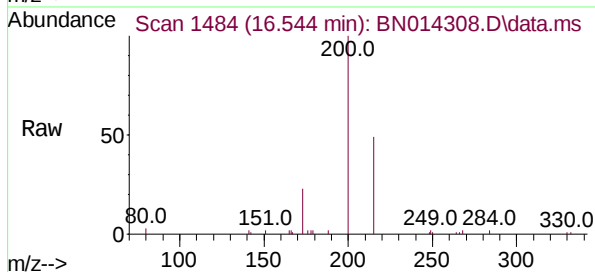




Abundance Scan 1484 (16.544 min): BN014308.D\data.ms (-1443) (-)

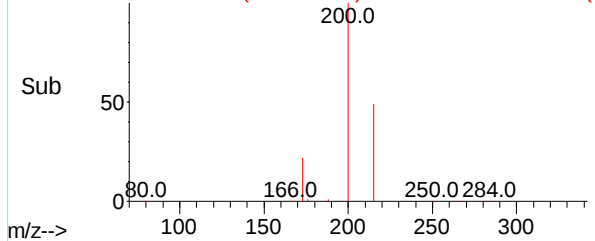

Abundance Scan 1499 (16.727 min): BN014307.D\data.ms (-1424) (-)


Pentachlorophenol
Concen: 0.67 ng
RT: 16.727 min Scan# 1499
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09

Tgt Ion:	266	Resp:	3537
Ion Ratio	Lower	Upper	
266	100		
264	62.8	49.8	74.8
268	63.8	50.7	76.1

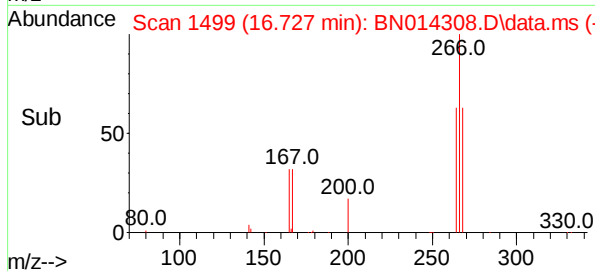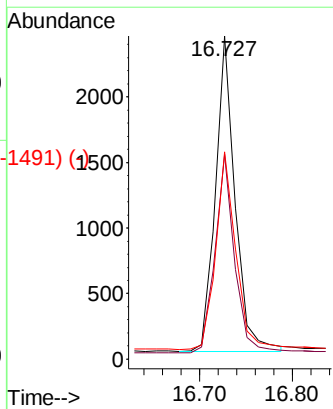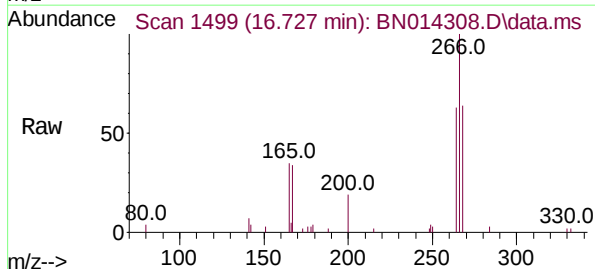

Abundance Scan 1499 (16.727 min): BN014308.D\data.ms (-1491) (-)







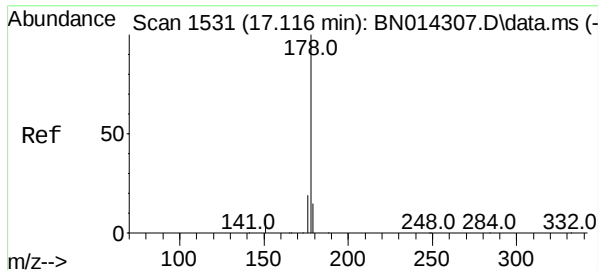

Phenanthrene
Concen: 0.80 ng
RT: 17.116 min Scan# 1531
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8

Tgt Ion:	178	Resp:	58529
Ion	Ratio	Lower	Upper
178	100		
176	19.3	15.3	22.9
179	15.3	12.2	18.4

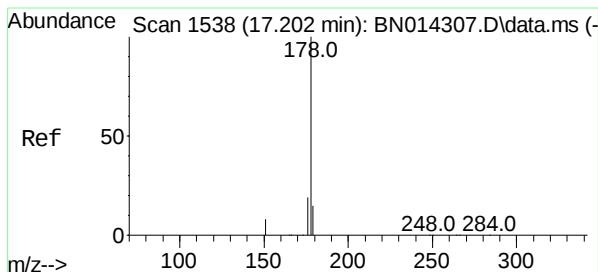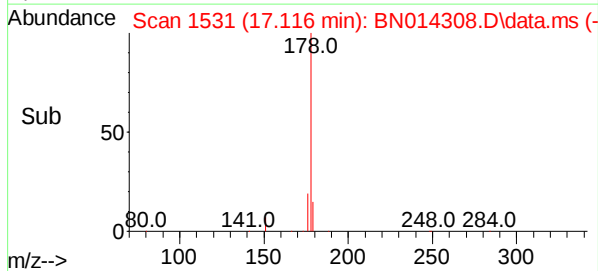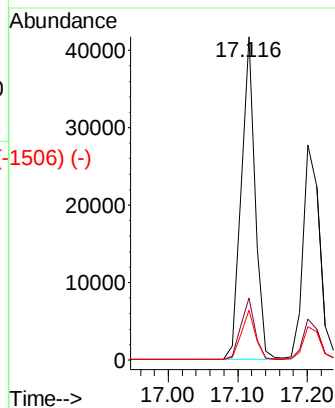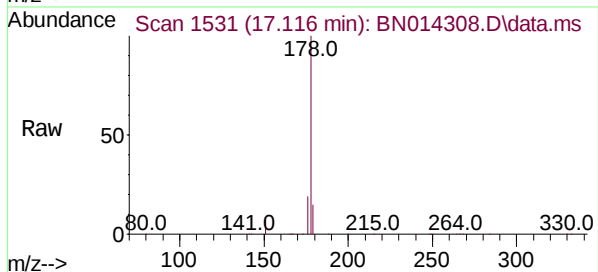

Anthracene
Concen: 0.76 ng
RT: 17.201 min Scan# 1538
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09


Tgt Ion:	178	Resp:	45835
Ion	Ratio	Lower	Upper
178	100		
176	18.5	14.8	22.2
179	15.4	12.2	18.4

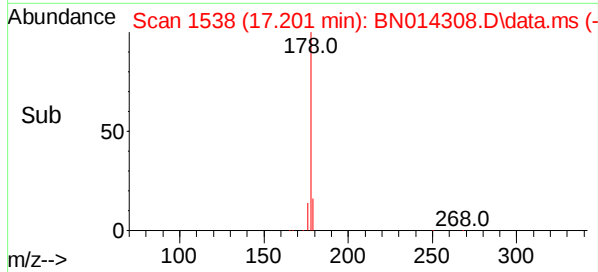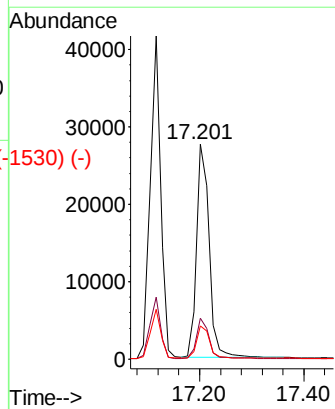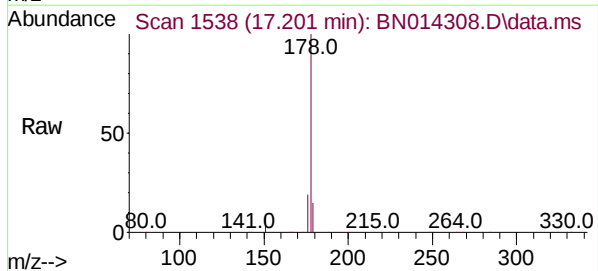



Abundance Scan 1825 (19.109 min): BN014307.D\data.ms (-1825) (-)

Fluoranthene-d10
Concen: 0.74 ng
RT: 19.109 min Scan# 1825
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09


Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8

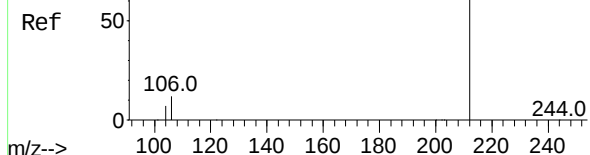

Tgt Ion:	212	Resp:	56803
Ion Ratio	Lower	Upper	
212	100		
106	12.0	9.7	14.5
104	6.7	5.5	8.3

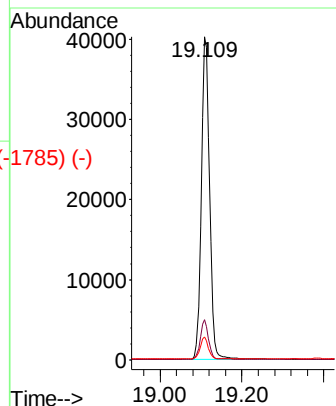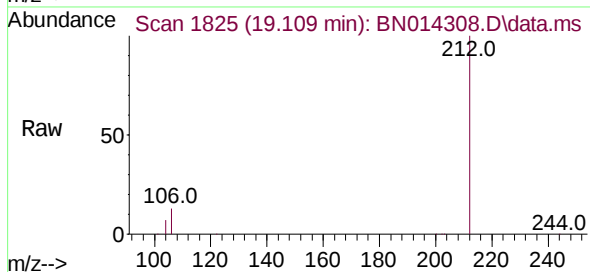



Abundance Scan 1825 (19.109 min): BN014308.D\data.ms (-1785) (-)

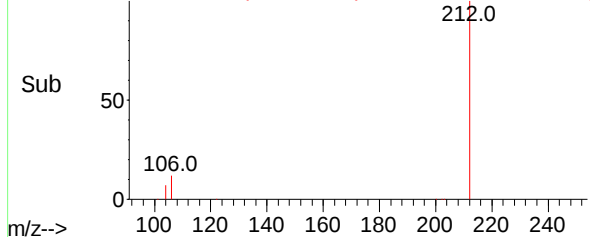


Abundance Scan 1831 (19.139 min): BN014307.D\data.ms (-1823) (-)

Fluoranthene
Concen: 0.77 ng
RT: 19.139 min Scan# 1831
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09

Tgt Ion:	202	Resp:	64237
Ion Ratio	Lower	Upper	
202	100		
101	10.2	8.3	12.5
203	17.2	13.8	20.6

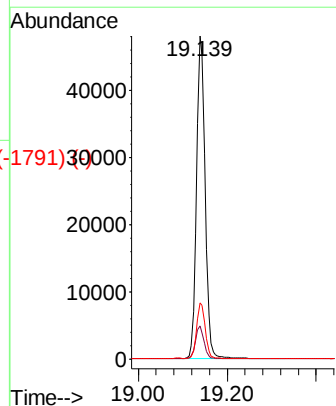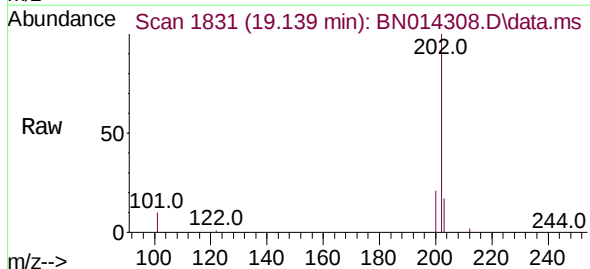


Abundance Scan 1831 (19.139 min): BN014308.D\data.ms (-1791) (-)

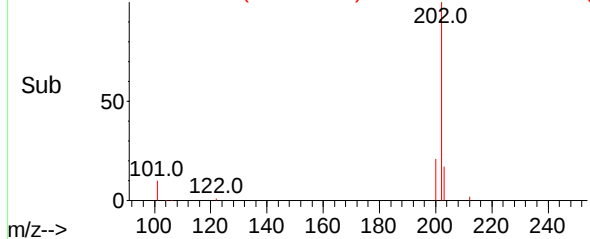



Abundance Scan 2125 (21.271 min): BN014307.D\data.ms (-2106) (-)

Chrysene-d12
Concen: 0.40 ng
RT: 21.271 min Scan# 2125
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09


Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8

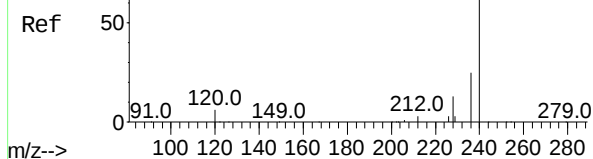

Tgt Ion:	240	Resp:	28162
Ion Ratio	Lower	Upper	
240	100		
120	6.7	5.4	8.0
236	26.0	20.4	30.6

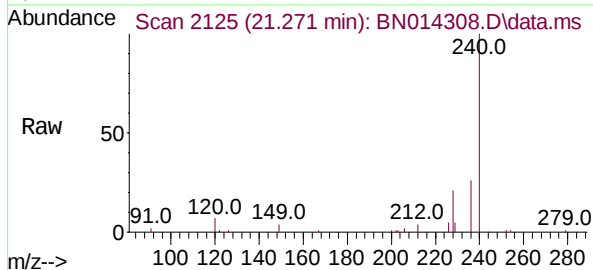




Abundance Scan 2125 (21.271 min): BN014308.D\data.ms (-2106) (-)

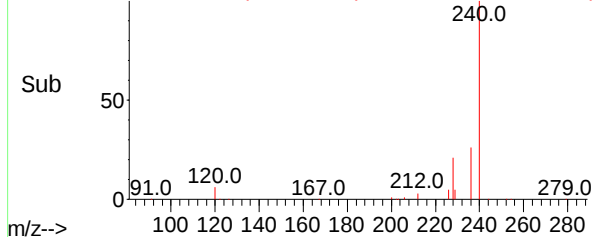


Abundance Scan 1904 (19.501 min): BN014307.D\data.ms (-1864) (-)

Pyrene
Concen: 0.71 ng
RT: 19.506 min Scan# 1905
Delta R.T. 0.005 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09


Tgt Ion:	202	Resp:	63083
Ion Ratio	Lower	Upper	
202	100		
200	20.7	16.6	24.8
203	17.4	14.0	21.0

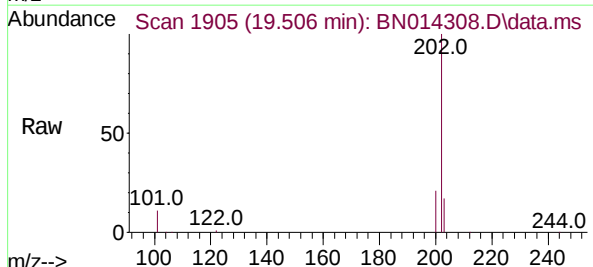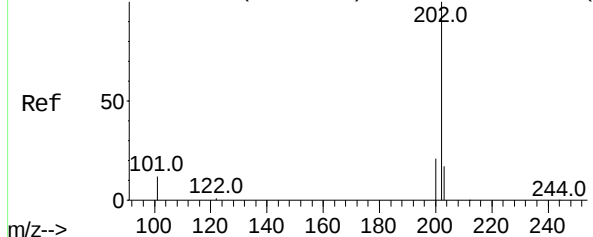

Abundance Scan 1905 (19.506 min): BN014308.D\data.ms (-1864) (-)

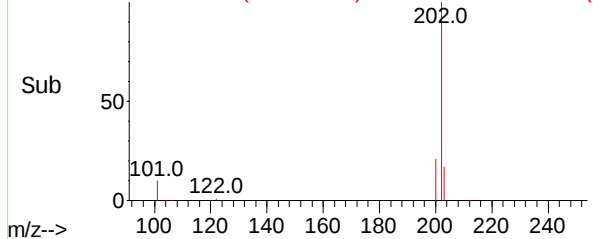



Abundance Scan 1947 (19.715 min): BN014307.D\data.ms (-1929) (-)

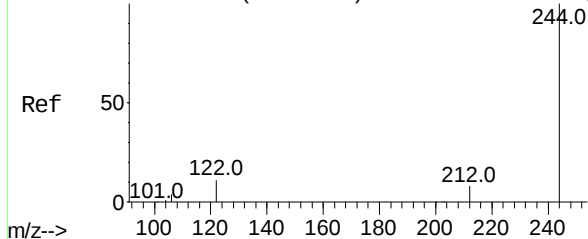


Terphenyl-d14
Concen: 0.78 ng
RT: 19.714 min Scan# 1947
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion	Ratio	Lower	Upper
244	100		
212	7.7	6.2	9.4
122	11.3	9.0	13.6

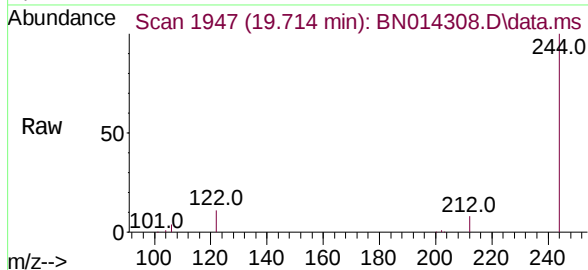

Abundance Scan 1947 (19.714 min): BN014308.D\data.ms (-1917) (-)


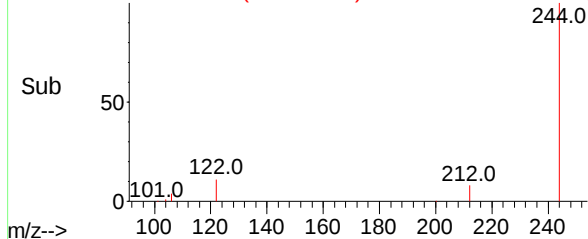


Abundance Scan 2123 (21.250 min): BN014307.D\data.ms (-2134) (-)

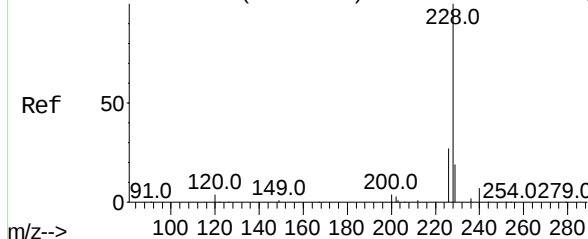


Benzo(a)anthracene
Concen: 0.70 ng
RT: 21.250 min Scan# 2123
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09


Tgt Ion	Ratio	Lower	Upper
228	100		
226	27.4	21.7	32.5
229	19.5	15.7	23.5

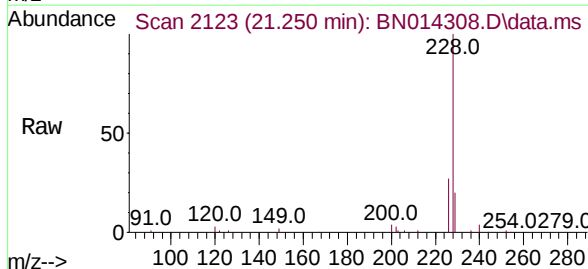

Abundance Scan 2123 (21.250 min): BN014308.D\data.ms (-2104) (-)

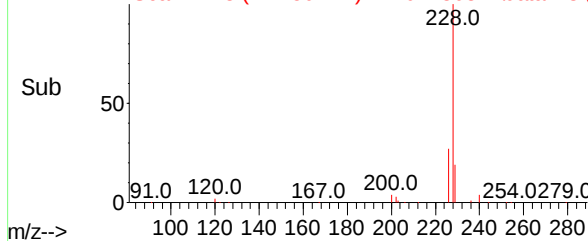




Abundance Scan 2128 (21.303 min): BN014307.D\data.ms (-2128) (-)

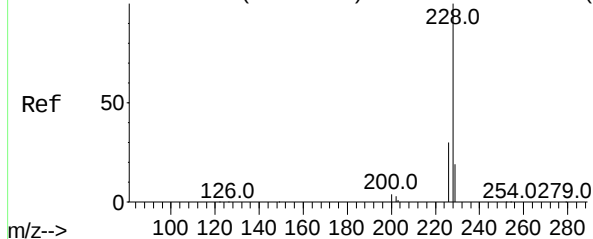


Chrysene
Concen: 0.79 ng
RT: 21.303 min Scan# 2128
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8

Tgt Ion:	228	Resp:	68601
Ion	Ratio	Lower	Upper
228	100		
226	29.8	23.8	35.6
229	19.5	15.6	23.4

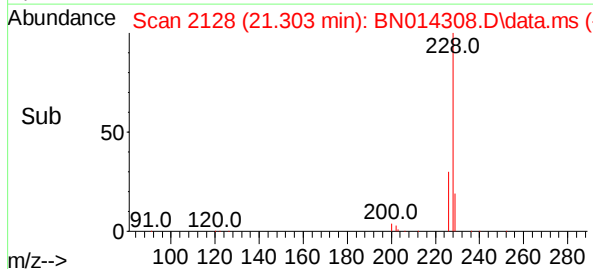

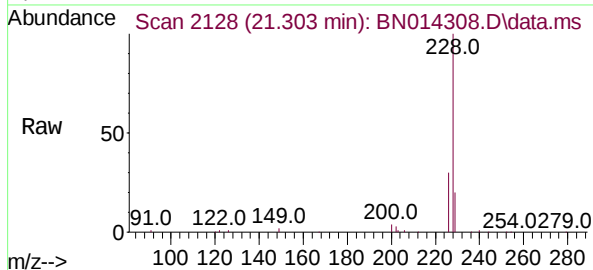


Abundance Scan 2118 (21.197 min): BN014307.D\data.ms (-2118) (-)

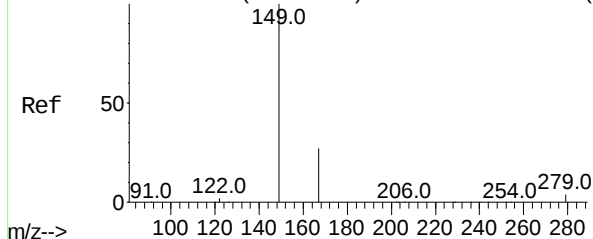

Bis(2-ethylhexyl)phthalate
Concen: 0.53 ng
RT: 21.197 min Scan# 2118
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09


Tgt Ion:	149	Resp:	15173
Ion	Ratio	Lower	Upper
149	100		
167	26.4	21.0	31.4
279	4.0	3.3	4.9

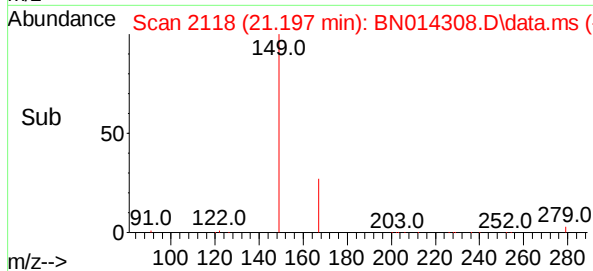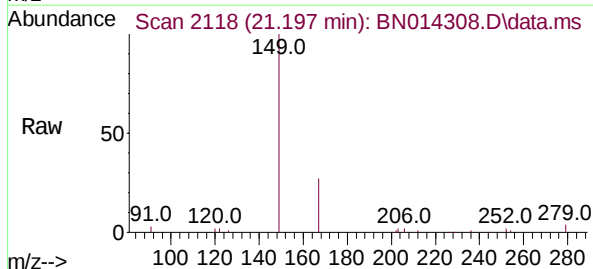




Abundance Scan 3205 (25.738 min): BN014307.D\data.ms (-3185) (-)

Indeno(1,2,3-cd)pyrene
Concen: 0.78 ng
RT: 25.741 min Scan# 3206
Delta R.T. 0.003 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8

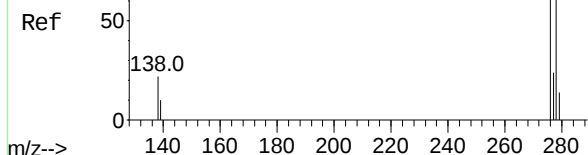


Tgt Ion	Ratio	Lower	Upper
276	100		
138	23.6	18.3	27.5
277	24.8	19.9	29.9

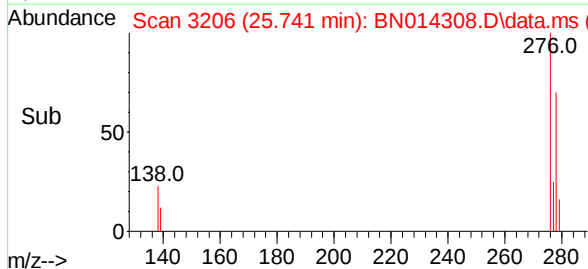

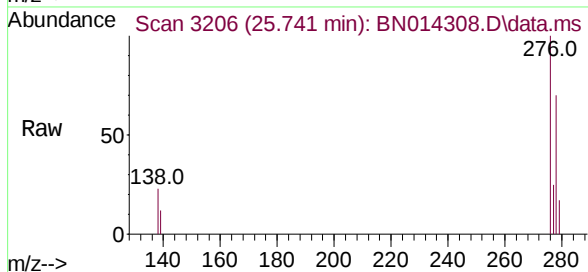


Abundance Scan 2551 (23.500 min): BN014307.D\data.ms (-2536) (-)


Perylene-d12
Concen: 0.40 ng
RT: 23.499 min Scan# 2551
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09

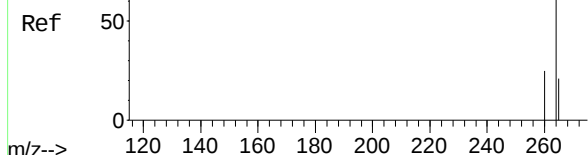

Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.4	20.0	30.0
265	47.4	37.8	56.8

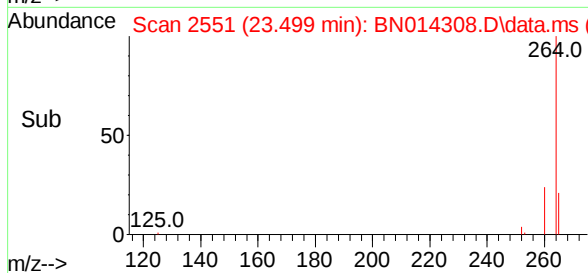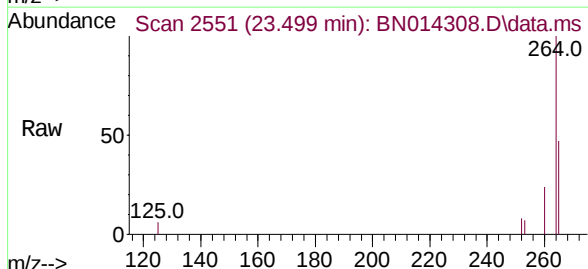



Abundance Scan 2355 (22.829 min): BN014307.D\data.ms (-2355) (-)

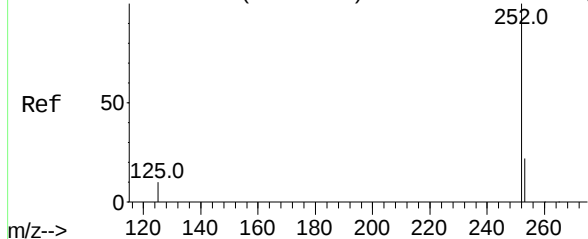


Benzo(b)fluoranthene
Concen: 0.92 ng
RT: 22.828 min Scan# 2355
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09

Tgt Ion:	252	Resp:	73962
Ion	Ratio	Lower	Upper
252	100		
253	22.9	19.0	28.6
125	10.7	9.3	13.9


Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8

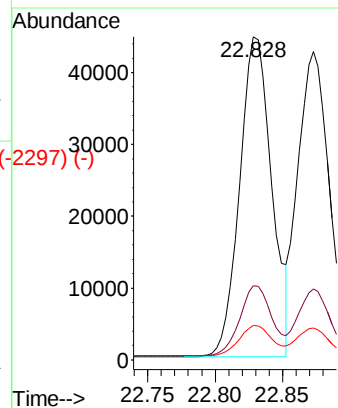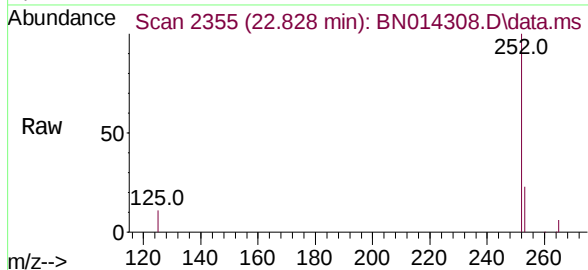

Abundance Scan 2355 (22.828 min): BN014308.D\data.ms (-2297) (-)


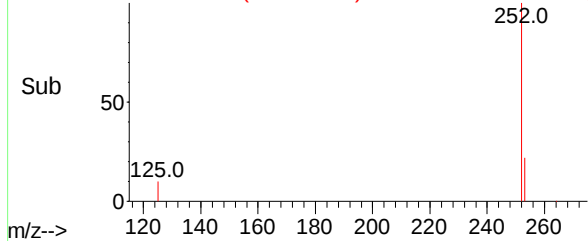


Abundance Scan 2368 (22.873 min): BN014307.D\data.ms (-2368) (-)

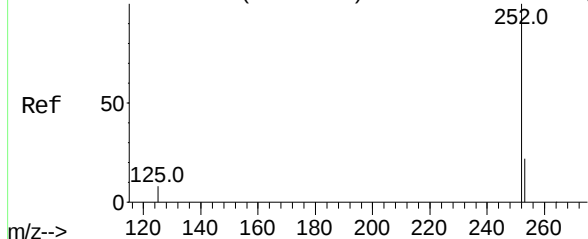


Benzo(k)fluoranthene
Concen: 0.89 ng
RT: 22.873 min Scan# 2368
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09

Tgt Ion:	252	Resp:	71918
Ion	Ratio	Lower	Upper
252	100		
253	22.9	19.1	28.7
125	10.4	9.1	13.7

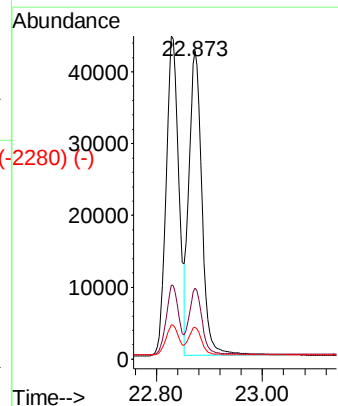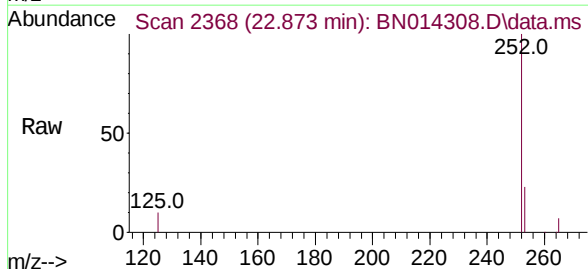


Abundance Scan 2368 (22.873 min): BN014308.D\data.ms (-2280) (-)

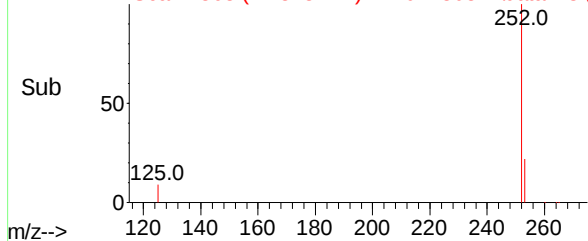




Abundance Scan 2522 (23.400 min): BN014307.D\data.ms (-2539) (-)

Benzo(a)pyrene
Concen: 0.82 ng
RT: 23.400 min Scan# 2522
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8

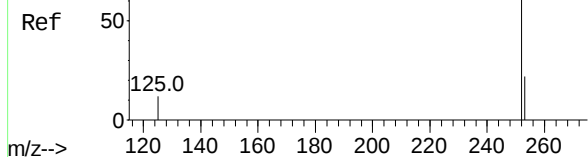




Tgt Ion:	252	Resp:	55924
Ion Ratio	Lower	Upper	
252	100		
253	24.0	20.2	30.2
125	13.3	12.4	18.6

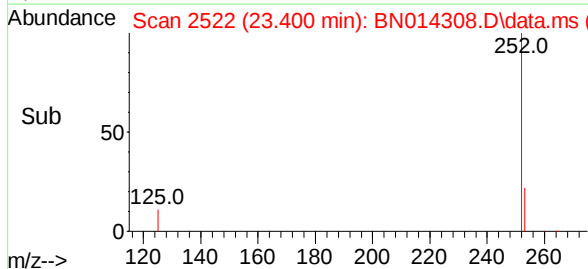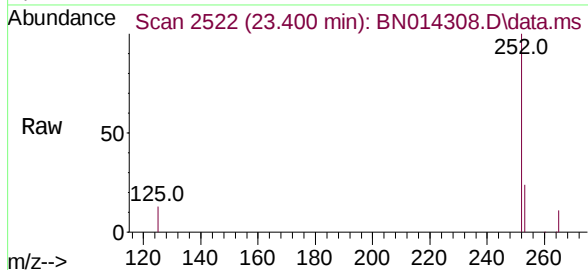


Abundance Scan 3210 (25.755 min): BN014307.D\data.ms (-3186) (-)

Dibenzo(a,h)anthracene
Concen: 0.85 ng
RT: 25.755 min Scan# 3210
Delta R.T. 0.003 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09

Tgt Ion:	278	Resp:	66492
Ion Ratio	Lower	Upper	
278	100		
139	15.7	12.8	19.2
279	24.4	20.0	30.0

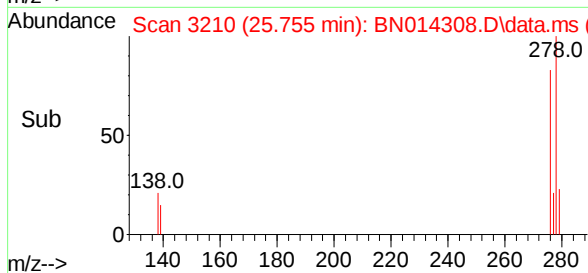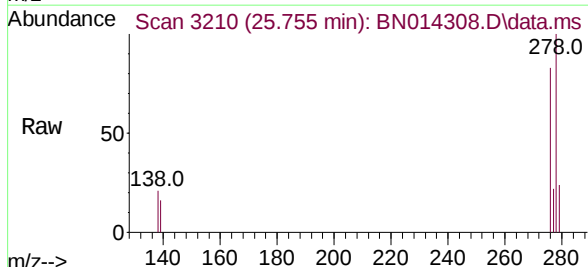


Abundance Scan 3405 (26.423 min): BN014307.D\data.ms (-3374) (-)

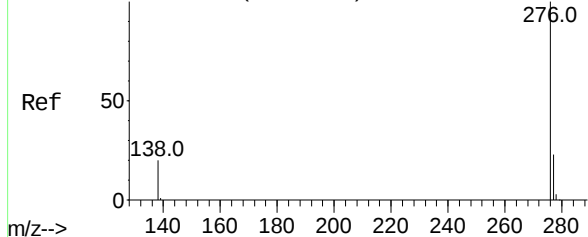

Benzo(g,h,i)perylene
 Concen: 0.89 ng
 RT: 26.426 min Scan# 3406
 Delta R.T. 0.003 min
 Lab File: BN014308.D
 Acq: 16 Apr 2021 14:09

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8

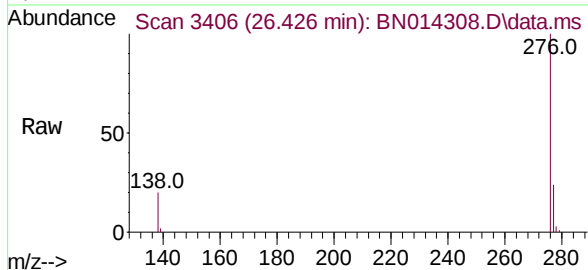

Tgt Ion:	276	Resp:	71068
Ion Ratio	Lower	Upper	
276	100		
277	24.0	18.9	28.3
138	20.4	16.6	24.8

