

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041621\
 Data File : BN014311.D
 Acq On : 16 Apr 2021 15:57
 Operator : CG/JU
 Sample : SSTDICC5.0
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Quant Time: Apr 16 16:26:32 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN041621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 16 14:08:36 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.700	152	9657	0.40	ng	0.00
7) Naphthalene-d8	10.467	136	31911	0.40	ng	#-0.01
13) Acenaphthene-d10	14.334	164	16793	0.40	ng	0.00
19) Phenanthrene-d10	17.080	188	33787	0.40	ng	# 0.01
29) Chrysene-d12	21.271	240	39834	0.40	ng	0.00
36) Perylene-d12	23.500	264	30839	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.300	112	99291	4.31	ng	0.00
5) Phenol-d6	6.863	99	131405	4.57	ng	0.00
8) Nitrobenzene-d5	8.832	82	105762	5.22	ng	-0.01
11) 2-Methylnaphthalene-d10	12.066	152	240044	4.83	ng	0.00
14) 2,4,6-Tribromophenol	15.818	330	34484	5.26	ng	0.00
15) 2-Fluorobiphenyl	12.951	172	307785	5.00	ng	0.00
27) Fluoranthene-d10	19.109	212	488066	4.98	ng	0.00
31) Terphenyl-d14	19.715	244	375765	4.27	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.255	88	50937	4.14	ng	93
3) n-Nitrosodimethylamine	3.569	42	37718	6.56	ng	# 99
6) bis(2-Chloroethyl)ether	7.129	93	109167	4.68	ng	100
9) Naphthalene	10.518	128	383976	4.84	ng	99
10) Hexachlorobutadiene	10.822	225	74747	4.71	ng	# 100
12) 2-Methylnaphthalene	12.142	142	253792	4.77	ng	99
16) Acenaphthylene	14.042	152	355644	5.51	ng	99
17) Acenaphthene	14.397	154	237073	5.02	ng	97
18) Fluorene	15.374	166	291551	4.86	ng	100
20) 4,6-Dinitro-2-methylph...	15.450	198	24629	6.15	ng	# 49
21) 4-Bromophenyl-phenylether	16.277	248	88587	5.12	ng	99
22) Hexachlorobenzene	16.386	284	110313	5.01	ng	100
23) Atrazine	16.544	200	66573	5.15	ng	98
24) Pentachlorophenol	16.727	266	37664	5.57	ng	99
25) Phenanthrene	17.116	178	466255	4.99	ng	100
26) Anthracene	17.201	178	412798	5.33	ng	100
28) Fluoranthene	19.139	202	537515	5.01	ng	99
30) Pyrene	19.506	202	543400	4.33	ng	100
32) Benzo(a)anthracene	21.250	228	543731	4.79	ng	99
33) Chrysene	21.303	228	562065	4.57	ng	99
34) Bis(2-ethylhexyl)phtha...	21.197	149	159226	3.91	ng	99
35) Indeno(1,2,3-cd)pyrene	25.742	276	647785	4.47	ng	99
37) Benzo(b)fluoranthene	22.832	252	569409	5.19	ng	96
38) Benzo(k)fluoranthene	22.877	252	570950	5.20	ng	95
39) Benzo(a)pyrene	23.404	252	498920	5.39	ng	# 92
40) Dibenzo(a,h)anthracene	25.759	278	542111	5.09	ng	98
41) Benzo(g,h,i)perylene	26.426	276	553834	5.13	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041621\
Data File : BN014311.D
Acq On : 16 Apr 2021 15:57
Operator : CG/JU
Sample : SSTDIC5.0
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Quant Time: Apr 16 16:26:32 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN041621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 16 14:08:36 2021
Response via : Initial Calibration







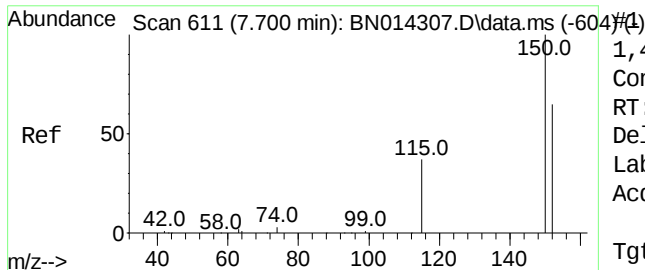

1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.700 min Scan# 611
 Delta R.T. 0.000 min
 Lab File: BN014311.D
 Acq: 16 Apr 2021 15:57




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0


Tgt Ion:152 Resp: 9657
 Ion Ratio Lower Upper
 152 100
 150 154.3 123.0 184.4
 115 58.7 47.6 71.4

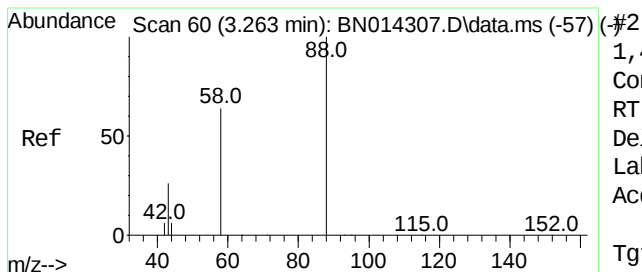

1,4-Dioxane
 Concen: 4.14 ng
 RT: 3.255 min Scan# 59
 Delta R.T. -0.008 min
 Lab File: BN014311.D
 Acq: 16 Apr 2021 15:57

Tgt Ion: 88 Resp: 50937
 Ion Ratio Lower Upper
 88 100
 58 66.3 47.3 70.9
 43 26.8 20.6 31.0







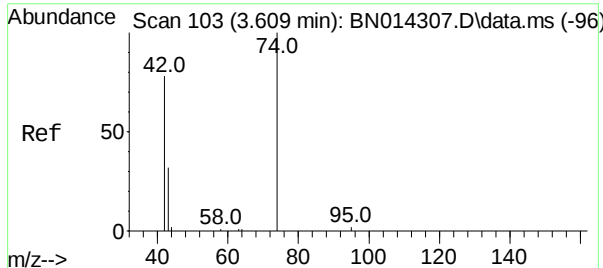

n-Nitrosodimethylamine
Concen: 6.56 ng
RT: 3.569 min Scan# 98
Delta R.T. -0.040 min
Lab File: BN014311.D
Acq: 16 Apr 2021 15:57




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion: 42 Resp: 37718
Ion Ratio Lower Upper
42 100
74 131.8 104.6 157.0
44 5.4 2.4 3.6#

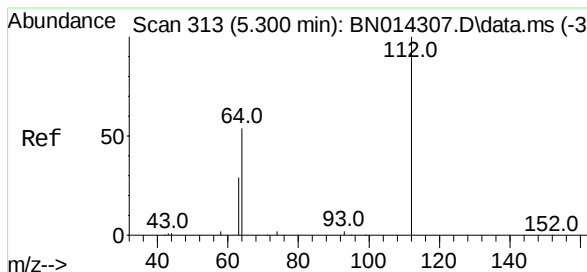

2-Fluorophenol
Concen: 4.31 ng
RT: 5.300 min Scan# 313
Delta R.T. -0.000 min
Lab File: BN014311.D
Acq: 16 Apr 2021 15:57

Tgt Ion: 112 Resp: 99291
Ion Ratio Lower Upper
112 100
64 54.4 43.7 65.5
63 29.7 23.8 35.8







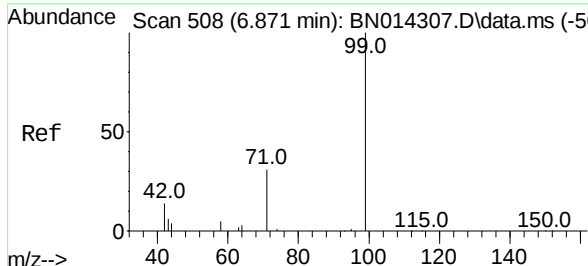

Phenol-d6
 Concen: 4.57 ng
 RT: 6.863 min Scan# 507
 Delta R.T. -0.008 min
 Lab File: BN014311.D
 Acq: 16 Apr 2021 15:57




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Tgt Ion:	99	Resp:	131405
Ion	Ratio	Lower	Upper
99	100		
42	18.7	15.7	23.5
71	34.4	27.6	41.4




bis(2-Chloroethyl)ether
 Concen: 4.68 ng
 RT: 7.129 min Scan# 540
 Delta R.T. -0.000 min
 Lab File: BN014311.D
 Acq: 16 Apr 2021 15:57

Tgt Ion:	93	Resp:	109167
Ion	Ratio	Lower	Upper
93	100		
63	72.8	58.2	87.4
95	32.9	26.7	40.1



Abundance Scan 858 (10.480 min): BN014307.D\data.ms (-857#7-)



Naphthalene-d8
Concen: 0.40 ng
RT: 10.467 min Scan# 857
Delta R.T. -0.013 min
Lab File: BN014311.D
Acq: 16 Apr 2021 15:57

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

m/z-->

Tgt Ion:136 Resp: 31911

Ion Ratio Lower Upper


136 100

137 11.2 9.0 13.6


54 8.3 3.5 5.3#

68 7.0 3.4 5.2#


Abundance Scan 857 (10.467 min): BN014311.D\data.ms



m/z-->




Abundance Scan 857 (10.467 min): BN014311.D\data.ms (-842) (-)



m/z-->

Abundance Scan 729 (8.845 min): BN014307.D\data.ms (-725#8)



Nitrobenzene-d5
Concen: 5.22 ng
RT: 8.832 min Scan# 728
Delta R.T. -0.013 min
Lab File: BN014311.D
Acq: 16 Apr 2021 15:57

Tgt Ion: 82 Resp: 105762


Ion Ratio Lower Upper

82 100


128 30.8 35.3 52.9#

54 50.5 33.4 50.2#


Abundance Scan 728 (8.832 min): BN014311.D\data.ms




m/z-->



Abundance Scan 728 (8.832 min): BN014311.D\data.ms (-713) (-)







m/z-->



Naphthalene
Concen: 4.84 ng
RT: 10.518 min Scan# 861
Delta R.T. -0.000 min
Lab File: BN014311.D
Acq: 16 Apr 2021 15:57




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:	128	Resp:	383976
Ion	Ratio	Lower	Upper
128	100		
129	10.9	9.0	13.4
127	13.0	10.7	16.1



Hexachlorobutadiene
Concen: 4.71 ng
RT: 10.822 min Scan# 885
Delta R.T. -0.000 min
Lab File: BN014311.D
Acq: 16 Apr 2021 15:57


Tgt Ion:	225	Resp:	74747
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	64.0	50.9	76.3





Abundance Scan 1065 (12.066 min): BN014307.D\data.ms (-1032) (-)

2-Methylnaphthalene-d10
Concen: 4.83 ng
RT: 12.066 min Scan# 1065
Delta R.T. -0.000 min
Lab File: BN014311.D
Acq: 16 Apr 2021 15:57


Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

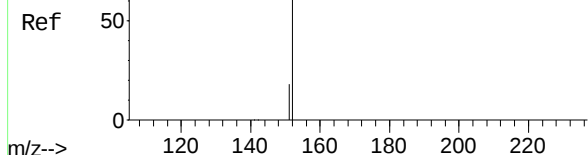

Tgt Ion:152 Resp: 240044
Ion Ratio Lower Upper
152 100
151 20.2 16.2 24.4






Abundance Scan 1065 (12.066 min): BN014311.D\data.ms (-1020) (-)




Abundance Scan 1082 (12.142 min): BN014307.D\data.ms (-1070) (-)

2-Methylnaphthalene
Concen: 4.77 ng
RT: 12.142 min Scan# 1082
Delta R.T. -0.000 min
Lab File: BN014311.D
Acq: 16 Apr 2021 15:57

Tgt Ion:142 Resp: 253792
Ion Ratio Lower Upper
142 100
141 87.6 70.0 105.0
115 35.0 28.8 43.2

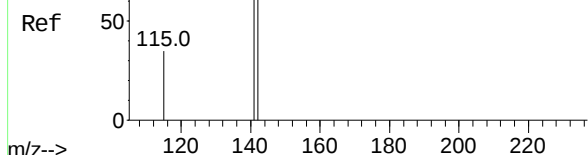


Abundance Scan 1082 (12.142 min): BN014311.D\data.ms (-1060) (-)






Abundance Scan 1308 (14.334 min): BN014307.D\data.ms (-1219) (-)

Acenaphthene-d10
Concen: 0.40 ng
RT: 14.334 min Scan# 1308
Delta R.T. -0.000 min
Lab File: BN014311.D
Acq: 16 Apr 2021 15:57

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

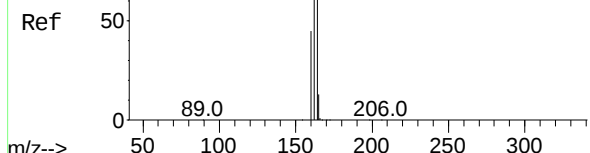


Tgt Ion:	164	Resp:	16793
Ion Ratio	Lower	Upper	
164	100		
162	99.9	78.6	117.8
160	45.2	36.2	54.4







Abundance Scan 1425 (15.818 min): BN014307.D\data.ms (-1417) (-)

2,4,6-Tribromophenol
Concen: 5.26 ng
RT: 15.818 min Scan# 1425
Delta R.T. -0.000 min
Lab File: BN014311.D
Acq: 16 Apr 2021 15:57



Tgt Ion:	330	Resp:	34484
Ion Ratio	Lower	Upper	
330	100		
332	0.0	0.0	0.0
141	34.2	28.8	43.2







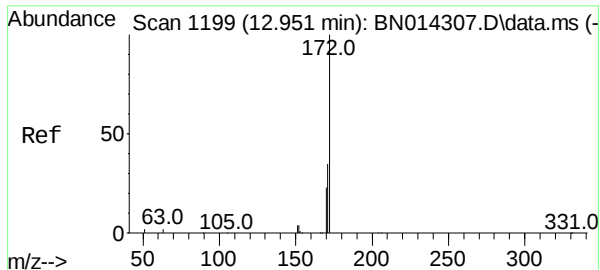

2-Fluorobiphenyl
Concen: 5.00 ng
RT: 12.951 min Scan# 1199
Delta R.T. -0.000 min
Lab File: BN014311.D
Acq: 16 Apr 2021 15:57




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:	172	Resp:	307785
Ion	Ratio	Lower	Upper
172	100		
171	33.8	27.9	41.9
170	22.5	18.8	28.2




Acenaphthylene
Concen: 5.51 ng
RT: 14.042 min Scan# 1285
Delta R.T. -0.000 min
Lab File: BN014311.D
Acq: 16 Apr 2021 15:57

Tgt Ion:	152	Resp:	355644
Ion	Ratio	Lower	Upper
152	100		
151	19.4	15.9	23.9
153	13.0	10.6	15.8





Abundance Scan 1312 (14.384 min): BN014307.D\data.ms (-1304) (-)




Acenaphthene
Concen: 5.02 ng
RT: 14.397 min Scan# 1313
Delta R.T. 0.013 min
Lab File: BN014311.D
Acq: 16 Apr 2021 15:57

Instrument :
BNA_N
ClientSampled :
SSTDICC5.0


Tgt Ion:	154	Resp:	237073
Ion	Ratio	Lower	Upper
154	100		
153	108.3	89.4	134.2
152	53.2	44.7	67.1



Abundance Scan 1313 (14.397 min): BN014311.D\data.ms (-1304) (-)





Abundance Scan 1390 (15.374 min): BN014307.D\data.ms (-1316) (-)




Fluorene
Concen: 4.86 ng
RT: 15.374 min Scan# 1390
Delta R.T. -0.000 min
Lab File: BN014311.D
Acq: 16 Apr 2021 15:57

Tgt Ion:	166	Resp:	291551
Ion	Ratio	Lower	Upper
166	100		
165	98.0	78.2	117.2
167	13.5	10.9	16.3




Abundance Scan 1390 (15.374 min): BN014311.D\data.ms (-1374) (-)





Abundance Scan 1527 (17.068 min): BN014307.D\data.ms (-1511) (-)

Phenanthrene-d10
Concen: 0.40 ng
RT: 17.080 min Scan# 1528
Delta R.T. 0.012 min
Lab File: BN014311.D
Acq: 16 Apr 2021 15:57


Instrument :
BNA_N
ClientSampled :
SSTDICC5.0

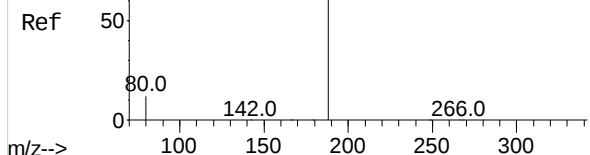

Tgt Ion:	188	Resp:	33787
Ion Ratio	Lower	Upper	
188	100		
94	0.0	0.0	0.0
80	5.8	10.2	15.4#







Abundance Scan 1528 (17.080 min): BN014311.D\data.ms (-1511) (-)



Abundance Scan 1396 (15.450 min): BN014307.D\data.ms (-1388) (-)

4,6-Dinitro-2-methylphenol
Concen: 6.15 ng
RT: 15.450 min Scan# 1396
Delta R.T. -0.000 min
Lab File: BN014311.D
Acq: 16 Apr 2021 15:57


Tgt Ion:	198	Resp:	24629
Ion Ratio	Lower	Upper	
198	100		
51	37.9	82.6	123.8#
105	43.9	56.1	84.1#





Abundance Scan 1462 (16.277 min): BN014307.D\data.ms (-1425) (-)

4-Bromophenyl-phenylether
Concen: 5.12 ng
RT: 16.277 min Scan# 1462
Delta R.T. -0.000 min
Lab File: BN014311.D
Acq: 16 Apr 2021 15:57


Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0



Tgt Ion:	248	Resp:	88587
Ion	Ratio	Lower	Upper
248	100		
250	103.1	81.9	122.9
141	34.4	29.3	43.9





Abundance Scan 1462 (16.277 min): BN014311.D\data.ms (-1454) (-)




Abundance Scan 1471 (16.386 min): BN014307.D\data.ms (-1426) (-)

Hexachlorobenzene
Concen: 5.01 ng
RT: 16.386 min Scan# 1471
Delta R.T. -0.000 min
Lab File: BN014311.D
Acq: 16 Apr 2021 15:57

Tgt Ion:	284	Resp:	110313
Ion	Ratio	Lower	Upper
284	100		
142	33.7	27.0	40.6
249	29.6	23.7	35.5




Abundance Scan 1471 (16.386 min): BN014311.D\data.ms (-1463) (-)






Abundance Scan 1484 (16.544 min): BN014307.D\data.ms (-1423) (-)

Atrazine
Concen: 5.15 ng
RT: 16.544 min Scan# 1484
Delta R.T. -0.000 min
Lab File: BN014311.D
Acq: 16 Apr 2021 15:57

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

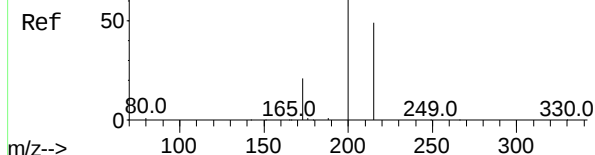





Tgt Ion	Ratio	Lower	Upper
200	100		
173	22.1	18.5	27.7
215	49.2	40.0	60.0




Abundance Scan 1499 (16.727 min): BN014307.D\data.ms (-1424) (-)

Pentachlorophenol
Concen: 5.57 ng
RT: 16.727 min Scan# 1499
Delta R.T. -0.000 min
Lab File: BN014311.D
Acq: 16 Apr 2021 15:57

Tgt Ion	Ratio	Lower	Upper
266	100		
264	62.6	49.8	74.8
268	63.9	50.7	76.1









Phenanthrene
Concen: 4.99 ng
RT: 17.116 min Scan# 1531
Delta R.T. -0.000 min
Lab File: BN014311.D
Acq: 16 Apr 2021 15:57




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:	178	Resp:	466255
Ion	Ratio	Lower	Upper
178	100		
176	19.0	15.3	22.9
179	15.3	12.2	18.4




Anthracene
Concen: 5.33 ng
RT: 17.201 min Scan# 1538
Delta R.T. -0.000 min
Lab File: BN014311.D
Acq: 16 Apr 2021 15:57

Tgt Ion:	178	Resp:	412798
Ion	Ratio	Lower	Upper
178	100		
176	18.5	14.8	22.2
179	15.3	12.2	18.4





Abundance Scan 1825 (19.109 min): BN014307.D\data.ms (-1825) (-)




Fluoranthene-d10
Concen: 4.98 ng
RT: 19.109 min Scan# 1825
Delta R.T. -0.000 min
Lab File: BN014311.D
Acq: 16 Apr 2021 15:57

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:	212	Resp:	488066
Ion Ratio	Lower	Upper	
212	100		
106	11.9	9.7	14.5
104	6.7	5.5	8.3



Abundance Scan 1825 (19.109 min): BN014311.D\data.ms (-1785) (-)





Abundance Scan 1831 (19.139 min): BN014307.D\data.ms (-1823) (-)




Fluoranthene
Concen: 5.01 ng
RT: 19.139 min Scan# 1831
Delta R.T. -0.000 min
Lab File: BN014311.D
Acq: 16 Apr 2021 15:57

Tgt Ion:	202	Resp:	537515
Ion Ratio	Lower	Upper	
202	100		
101	10.2	8.3	12.5
203	17.4	13.8	20.6




Abundance Scan 1831 (19.139 min): BN014311.D\data.ms (-1791) (-)






Abundance Scan 2125 (21.271 min): BN014307.D\data.ms (-1129) (-)

Chrysene-d12
Concen: 0.40 ng
RT: 21.271 min Scan# 2125
Delta R.T. -0.000 min
Lab File: BN014311.D
Acq: 16 Apr 2021 15:57

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0




Tgt Ion	Ratio	Lower	Upper
240	100		
120	6.6	5.4	8.0
236	25.7	20.4	30.6






Abundance Scan 1904 (19.501 min): BN014307.D\data.ms (-1129) (-)

Pyrene
Concen: 4.33 ng
RT: 19.506 min Scan# 1905
Delta R.T. 0.005 min
Lab File: BN014311.D
Acq: 16 Apr 2021 15:57




Tgt Ion	Ratio	Lower	Upper
202	100		
200	20.6	16.6	24.8
203	17.5	14.0	21.0






Abundance Scan 1947 (19.715 min): BN014307.D\data.ms (-1929) (-)

Terphenyl-d14
Concen: 4.27 ng
RT: 19.715 min Scan# 1947
Delta R.T. -0.000 min
Lab File: BN014311.D
Acq: 16 Apr 2021 15:57

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0




Tgt Ion	Ratio	Lower	Upper
244	100		
212	7.6	6.2	9.4
122	11.2	9.0	13.6






Abundance Scan 2123 (21.250 min): BN014307.D\data.ms (-2134) (-)


Benzo(a)anthracene
Concen: 4.79 ng
RT: 21.250 min Scan# 2123
Delta R.T. -0.000 min
Lab File: BN014311.D
Acq: 16 Apr 2021 15:57



Tgt Ion	Ratio	Lower	Upper
228	100		
226	27.7	21.7	32.5
229	19.3	15.7	23.5




Abundance Scan 2128 (21.303 min): BN014307.D\data.ms (-2128) (-)


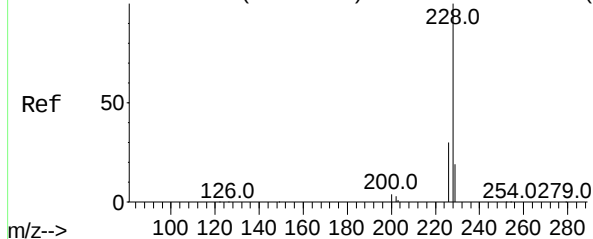


Chrysene
Concen: 4.57 ng
RT: 21.303 min Scan# 2128
Delta R.T. -0.000 min
Lab File: BN014311.D
Acq: 16 Apr 2021 15:57


Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0




Tgt Ion	Ratio	Lower	Upper
228	100		
226	30.1	23.8	35.6
229	19.3	15.6	23.4





Abundance Scan 2118 (21.197 min): BN014307.D\data.ms (-2118) (-)

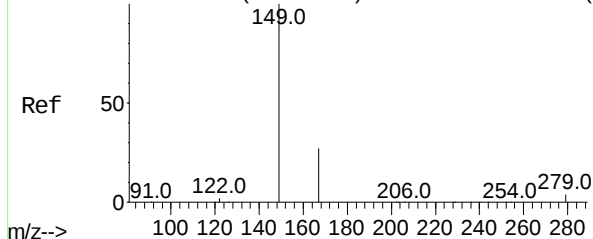


Bis(2-ethylhexyl)phthalate
Concen: 3.91 ng
RT: 21.197 min Scan# 2118
Delta R.T. -0.000 min
Lab File: BN014311.D
Acq: 16 Apr 2021 15:57



Tgt Ion	Ratio	Lower	Upper
149	100		
167	26.6	21.0	31.4
279	3.7	3.3	4.9





Abundance Scan 3205 (25.738 min): BN014307.D\data.ms (-3185) (-)




Indeno(1,2,3-cd)pyrene
Concen: 4.47 ng
RT: 25.742 min Scan# 3206
Delta R.T. 0.003 min
Lab File: BN014311.D
Acq: 16 Apr 2021 15:57

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion	Ratio	Lower	Upper
276	100		
138	23.6	18.3	27.5
277	24.9	19.9	29.9



Abundance Scan 3206 (25.742 min): BN014311.D\data.ms (-3176) (-)





Abundance Scan 2551 (23.500 min): BN014307.D\data.ms (-2536) (-)




Perylene-d12
Concen: 0.40 ng
RT: 23.500 min Scan# 2551
Delta R.T. -0.000 min
Lab File: BN014311.D
Acq: 16 Apr 2021 15:57


Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.5	20.0	30.0
265	40.3	37.8	56.8



Abundance Scan 2551 (23.500 min): BN014311.D\data.ms (-2507) (-)





Abundance Scan 2355 (22.829 min): BN014307.D\data.ms (-2355) (-)

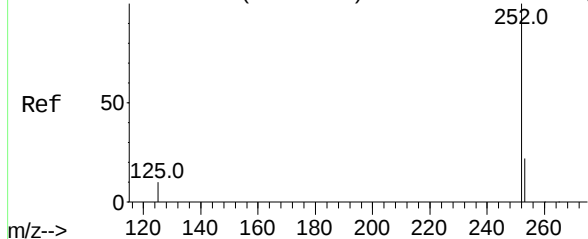


Benzo(b)fluoranthene
Concen: 5.19 ng
RT: 22.832 min Scan# 2356
Delta R.T. 0.003 min
Lab File: BN014311.D
Acq: 16 Apr 2021 15:57

Tgt Ion:	252	Resp:	569409
Ion	Ratio	Lower	Upper
252	100		
253	22.1	19.0	28.6
125	9.4	9.3	13.9


Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0



Abundance Scan 2356 (22.832 min): BN014311.D\data.ms (-2297) (-)





Abundance Scan 2368 (22.873 min): BN014307.D\data.ms (-2368) (-)




Benzo(k)fluoranthene
Concen: 5.20 ng
RT: 22.877 min Scan# 2369
Delta R.T. 0.003 min
Lab File: BN014311.D
Acq: 16 Apr 2021 15:57


Tgt Ion:	252	Resp:	570950
Ion	Ratio	Lower	Upper
252	100		
253	21.9	19.1	28.7
125	9.2	9.1	13.7



Abundance Scan 2369 (22.877 min): BN014311.D\data.ms (-2280) (-)





Abundance Scan 2522 (23.400 min): BN014307.D\data.ms (-2539) (-)




Benzo(a)pyrene
Concen: 5.39 ng
RT: 23.404 min Scan# 2523
Delta R.T. 0.003 min
Lab File: BN014311.D
Acq: 16 Apr 2021 15:57

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:	252	Resp:	498920
Ion	Ratio	Lower	Upper
252	100		
253	22.2	20.2	30.2
125	10.4	12.4	18.6#



Abundance Scan 2523 (23.404 min): BN014311.D\data.ms (-2464) (-)





Abundance Scan 3209 (25.752 min): BN014307.D\data.ms (-3140) (-)




Dibenzo(a,h)anthracene
Concen: 5.09 ng
RT: 25.759 min Scan# 3211
Delta R.T. 0.007 min
Lab File: BN014311.D
Acq: 16 Apr 2021 15:57


Tgt Ion:	278	Resp:	542111
Ion	Ratio	Lower	Upper
278	100		
139	15.1	12.8	19.2
279	23.6	20.0	30.0



Abundance Scan 3211 (25.759 min): BN014311.D\data.ms (-3186) (-)




Abundance Scan 3405 (26.423 min): BN014307.D\data.ms (-3374) (-)



Benzo(g,h,i)perylene
Concen: 5.13 ng
RT: 26.426 min Scan# 3406
Delta R.T. 0.003 min
Lab File: BN014311.D
Acq: 16 Apr 2021 15:57

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Abundance Scan 3406 (26.426 min): BN014311.D\data.ms



Tgt Ion:276 Resp: 553834
Ion Ratio Lower Upper
276 100
277 23.7 18.9 28.3
138 20.1 16.6 24.8

Abundance Scan 3406 (26.426 min): BN014311.D\data.ms (-3347) (-)

