
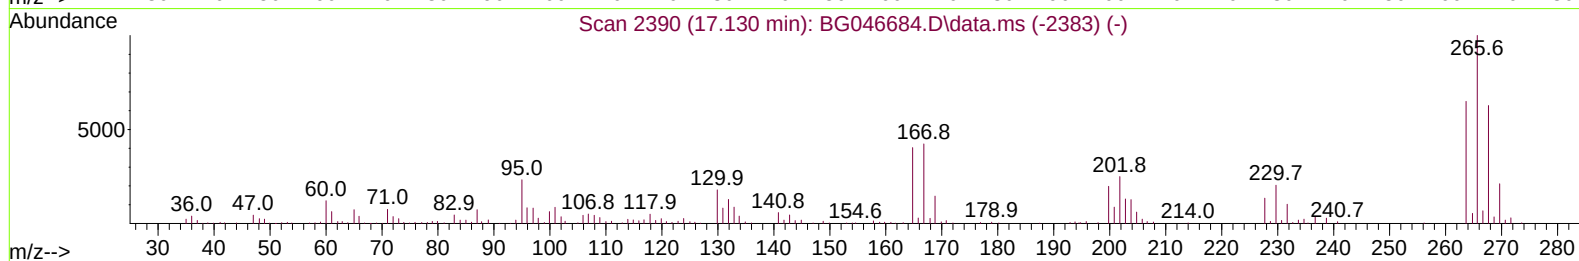
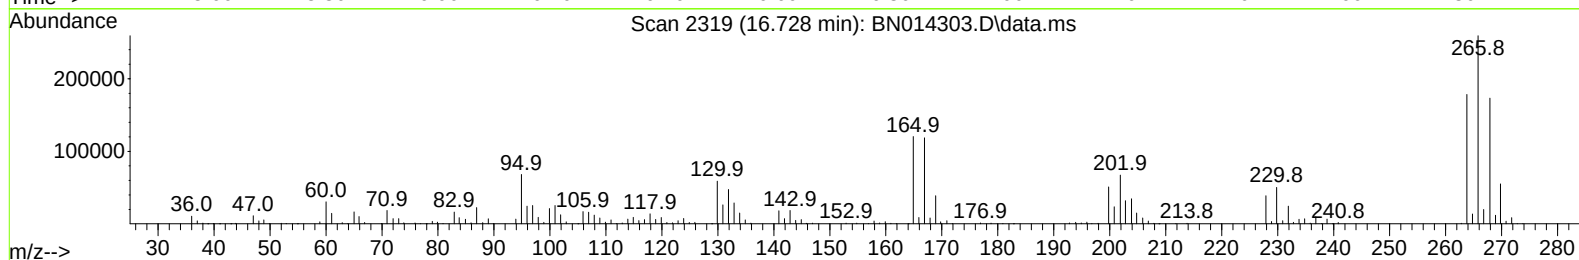


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041621\
Data File : BN014303.D
Acq On : 16 Apr 2021 10:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 19 01:18:25 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 09 09:55:03 2021
Response via : Initial Calibration

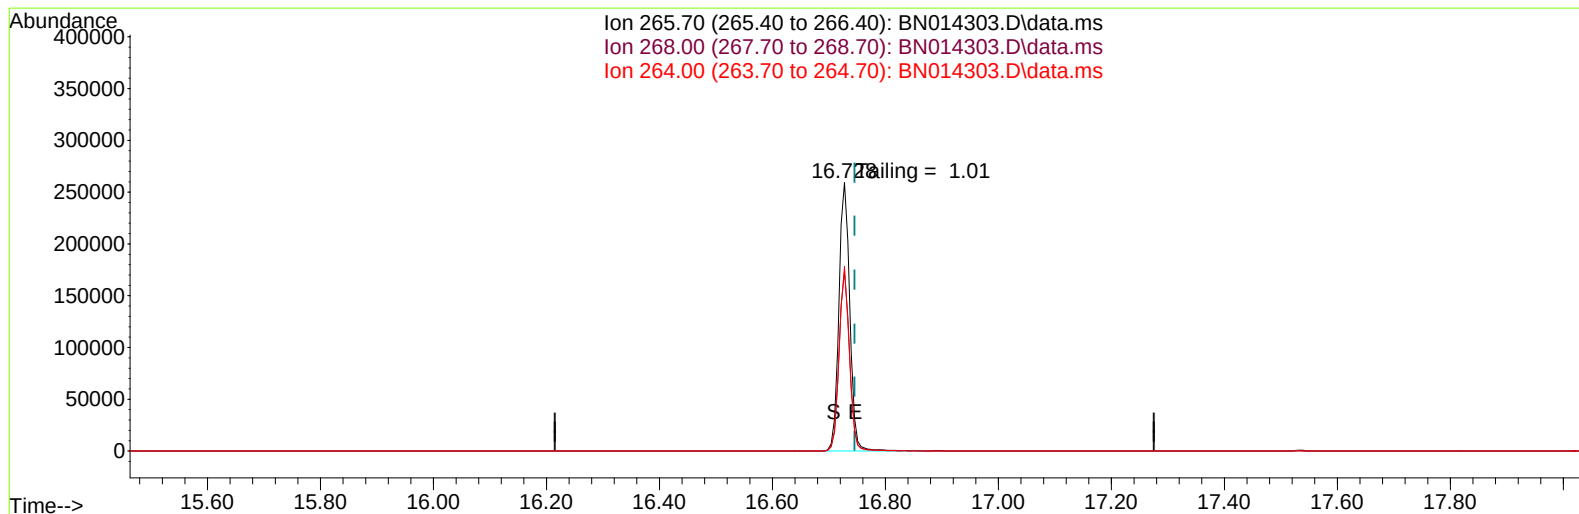

TIC: BN014303.D\data.ms

(70) Pentachlorophenol (C)




16.728min (-0.018) 26163.40 ng

response 344944

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.84
264.00	61.60	68.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041621\
Data File : BN014303.D
Acq On : 16 Apr 2021 10:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 19 01:18:25 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 09 09:55:03 2021
Response via : Initial Calibration

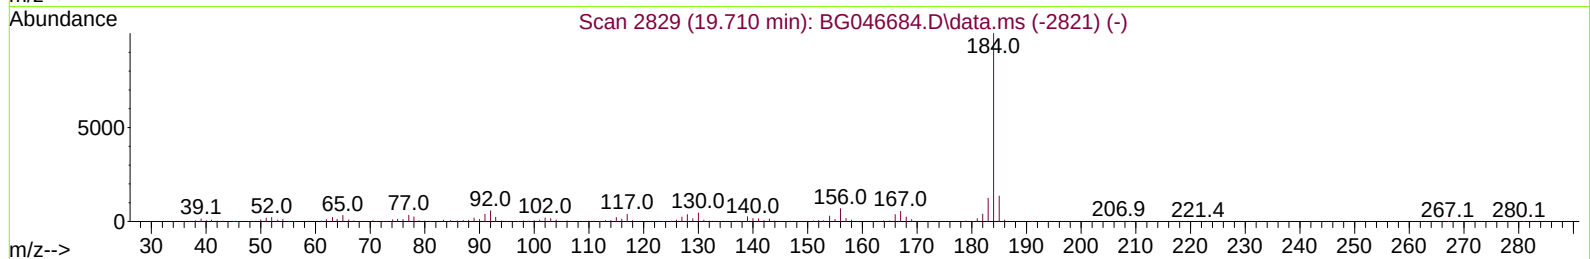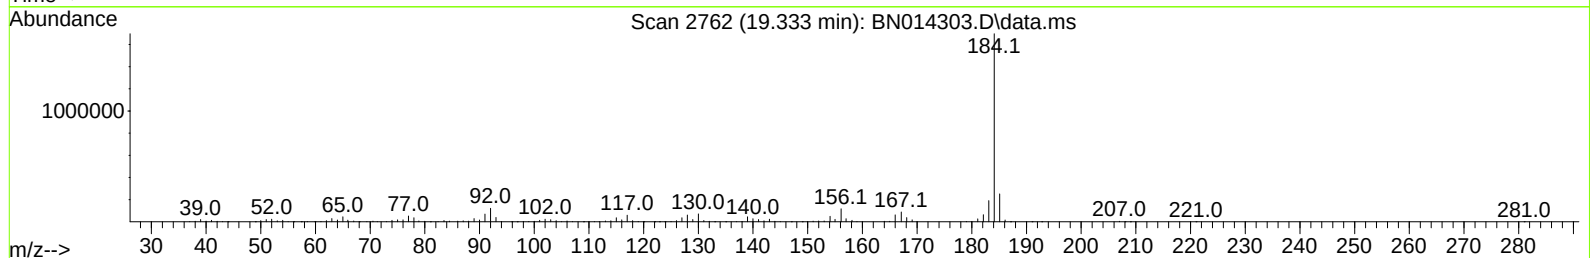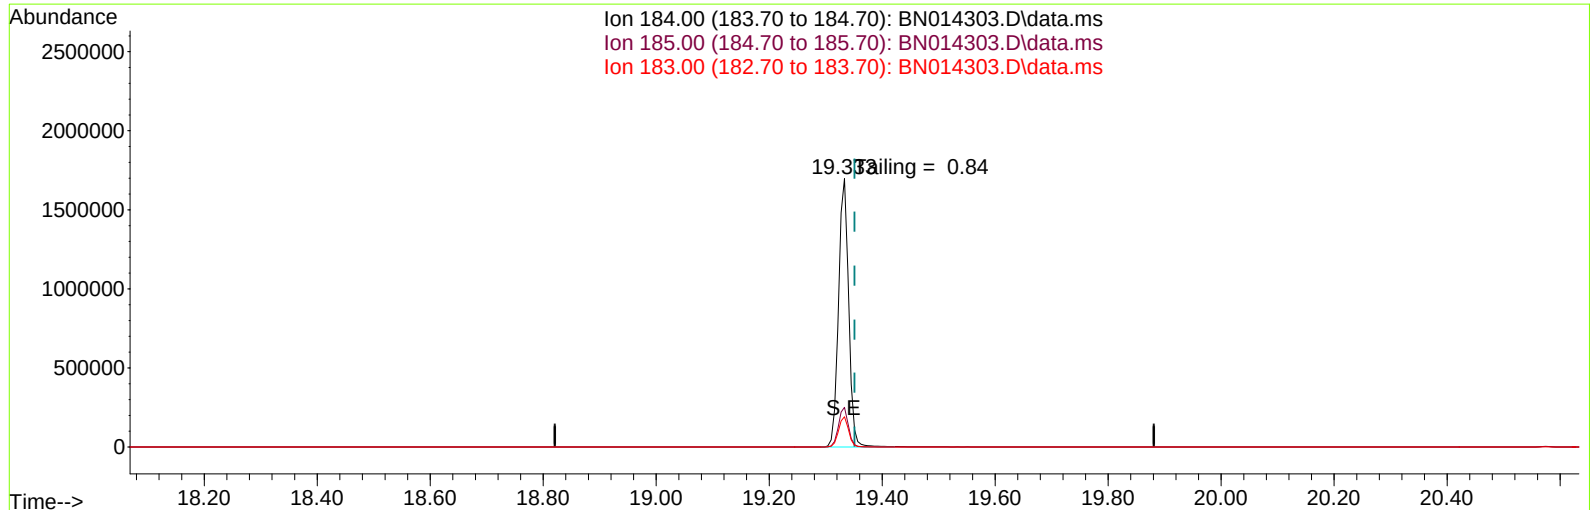

TIC: BN014303.D\data.ms

(77) Benzidine**19.333min (-0.018) 2683.88 ng****response 2096085**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.80
183.00	13.20	11.26
0.00	0.00	0.00