

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041621\
 Data File : BN014308.D
 Acq On : 16 Apr 2021 14:09
 Operator : CG/JU
 Sample : SSTDIC0.8
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDIC0.8

Quant Time: Apr 16 15:05:30 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN041621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 16 14:08:36 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.700	152	7119	0.40	ng	0.00
7) Naphthalene-d8	10.479	136	25632	0.40	ng	0.00
13) Acenaphthene-d10	14.333	164	12817	0.40	ng	0.00
19) Phenanthrene-d10	17.080	188	26365	0.40	ng	# 0.01
29) Chrysene-d12	21.271	240	28162	0.40	ng	0.00
36) Perylene-d12	23.499	264	22700	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.300	112	12317	0.73	ng	0.00
5) Phenol-d6	6.871	99	15228	0.72	ng	0.00
8) Nitrobenzene-d5	8.844	82	12951	0.80	ng	0.00
11) 2-Methylnaphthalene-d10	12.066	152	31217	0.78	ng	0.00
14) 2,4,6-Tribromophenol	15.818	330	3492	0.70	ng	0.00
15) 2-Fluorobiphenyl	12.950	172	43050	0.92	ng	0.00
27) Fluoranthene-d10	19.109	212	56803	0.74	ng	0.00
31) Terphenyl-d14	19.714	244	48319	0.78	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.263	88	6905	0.76	ng	91
3) n-Nitrosodimethylamine	3.601	42	3837	0.90	ng	99
6) bis(2-Chloroethyl)ether	7.128	93	14492	0.84	ng	99
9) Naphthalene	10.517	128	51679	0.81	ng	100
10) Hexachlorobutadiene	10.822	225	10298	0.81	ng	# 100
12) 2-Methylnaphthalene	12.142	142	33644	0.79	ng	100
16) Acenaphthylene	14.041	152	37804	0.77	ng	99
17) Acenaphthene	14.397	154	29359	0.81	ng	99
18) Fluorene	15.374	166	35603	0.78	ng	99
20) 4,6-Dinitro-2-methylph...	15.450	198	2173	0.70	ng	# 71
21) 4-Bromophenyl-phenylether	16.276	248	11193	0.83	ng	98
22) Hexachlorobenzene	16.386	284	14566	0.85	ng	100
23) Atrazine	16.544	200	6459	0.64	ng	99
24) Pentachlorophenol	16.727	266	3537	0.67	ng	99
25) Phenanthrene	17.116	178	58529	0.80	ng	100
26) Anthracene	17.201	178	45835	0.76	ng	100
28) Fluoranthene	19.139	202	64237	0.77	ng	100
30) Pyrene	19.506	202	63083	0.71	ng	100
32) Benzo(a)anthracene	21.250	228	56285	0.70	ng	100
33) Chrysene	21.303	228	68601	0.79	ng	100
34) Bis(2-ethylhexyl)phtha...	21.197	149	15173	0.53	ng	100
35) Indeno(1,2,3-cd)pyrene	25.741	276	79566	0.78	ng	99
37) Benzo(b)fluoranthene	22.828	252	73962	0.92	ng	98
38) Benzo(k)fluoranthene	22.873	252	71918	0.89	ng	98
39) Benzo(a)pyrene	23.400	252	55924	0.82	ng	96
40) Dibenzo(a,h)anthracene	25.755	278	66492	0.85	ng	99
41) Benzo(g,h,i)perylene	26.426	276	71068	0.89	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041621\
Data File : BN014308.D
Acq On : 16 Apr 2021 14:09
Operator : CG/JU
Sample : SSTDIC0.8
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8

Quant Time: Apr 16 15:05:30 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN041621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 16 14:08:36 2021
Response via : Initial Calibration

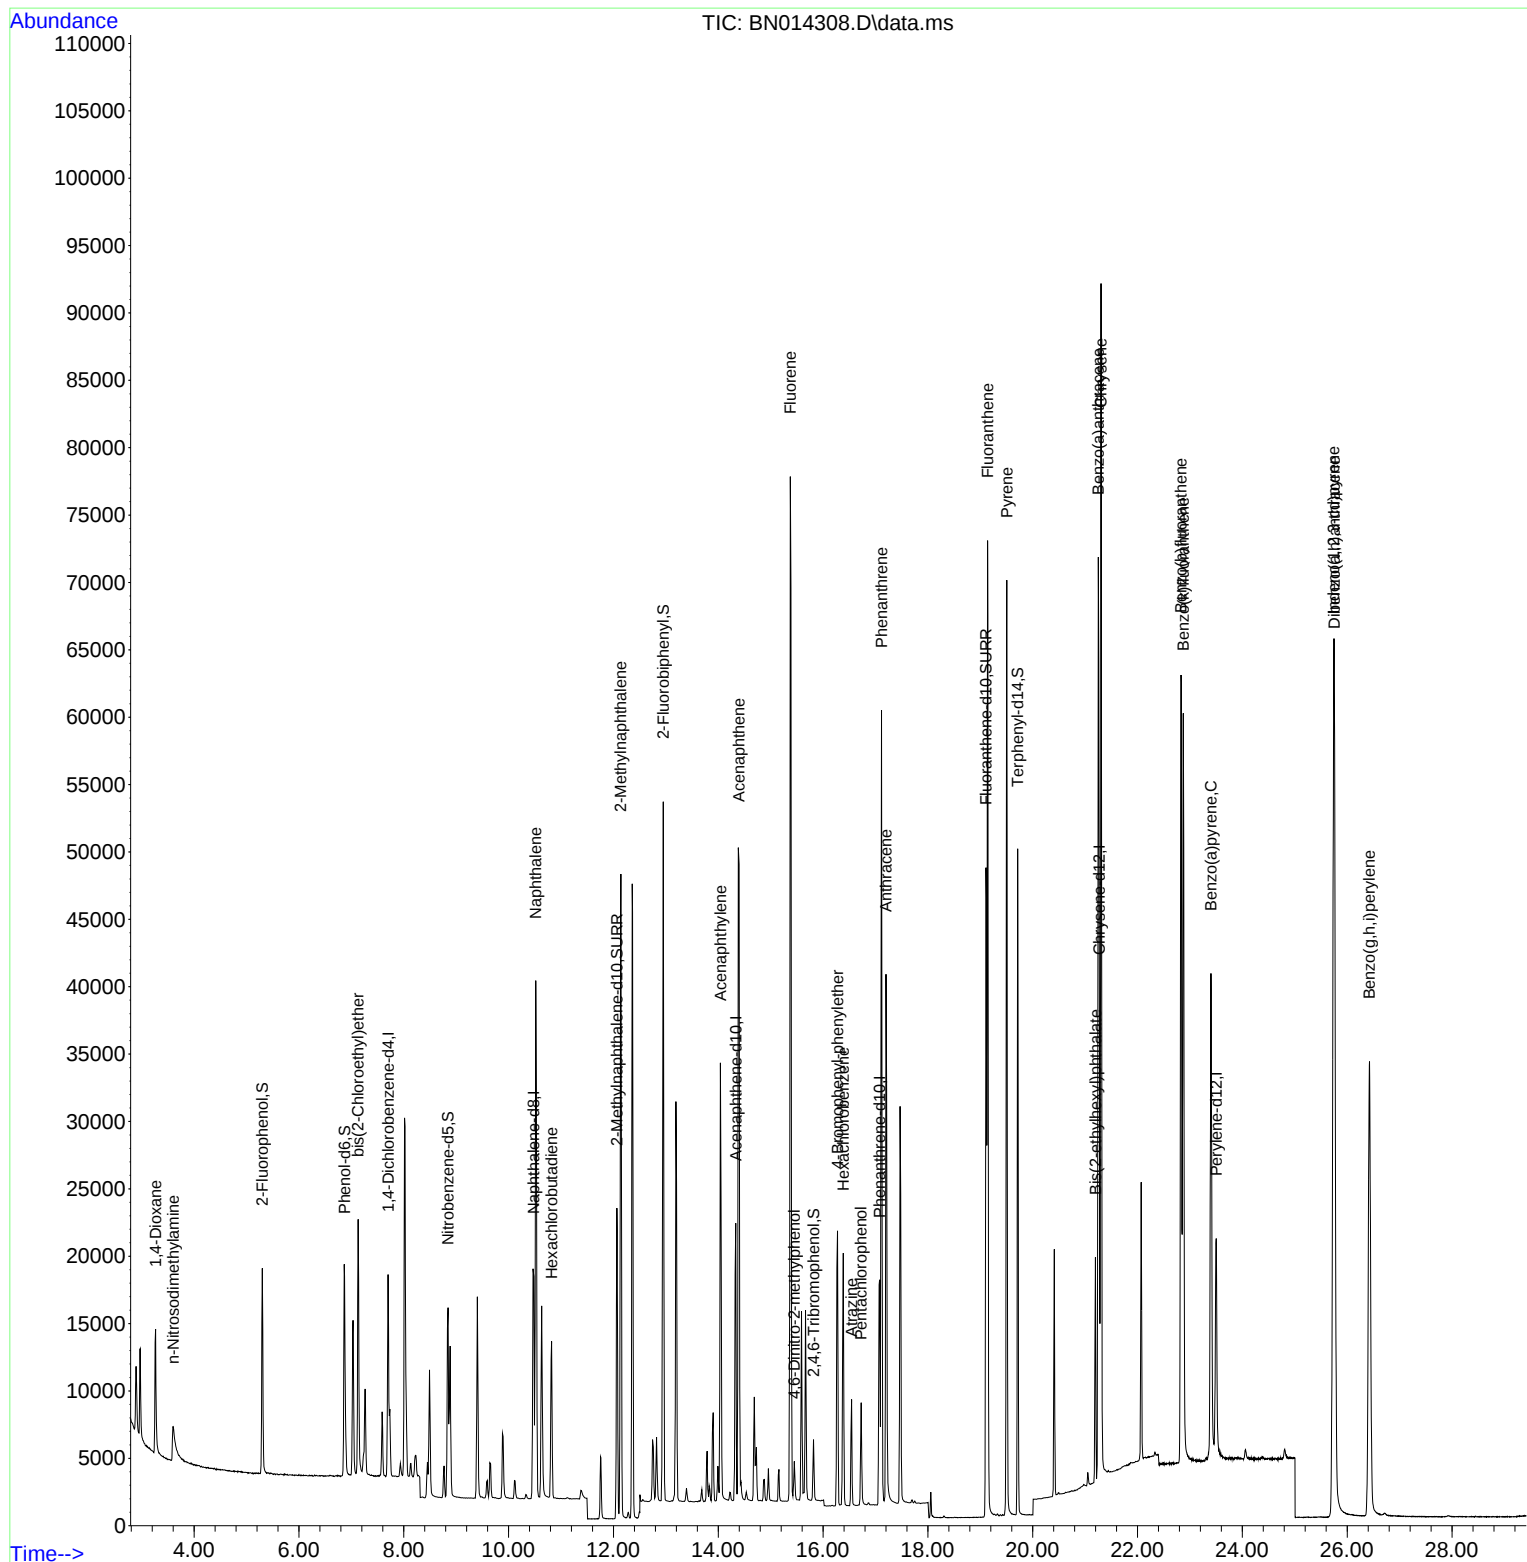







#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.700 min Scan# 611
 Delta R.T. 0.000 min
 Lab File: BN014308.D
 Acq: 16 Apr 2021 14:09

Instrument :
 BNA_N
 ClientSampled :
 SSTDICC0.8

Tgt Ion: 152 Resp: 7119




Ion	Ratio	Lower	Upper
152	100		
150	152.9	123.0	184.4
115	59.1	47.6	71.4

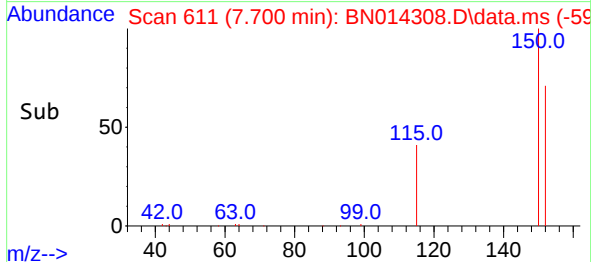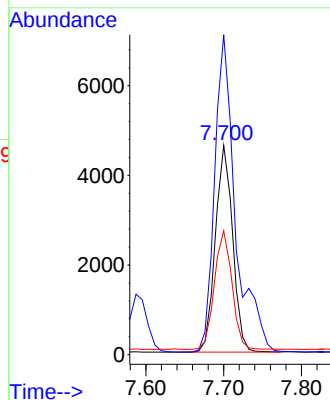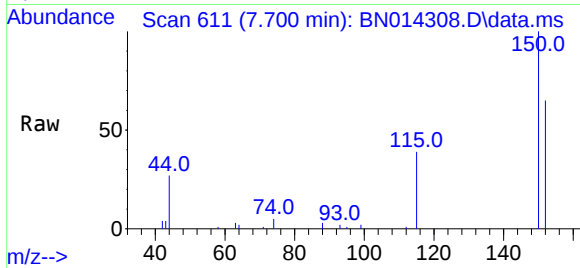


#2
 1,4-Dioxane
 Concen: 0.76 ng
 RT: 3.263 min Scan# 60
 Delta R.T. -0.000 min
 Lab File: BN014308.D
 Acq: 16 Apr 2021 14:09

Tgt Ion: 88 Resp: 6905

Ion	Ratio	Lower	Upper
88	100		
58	67.8	47.3	70.9
43	26.7	20.6	31.0


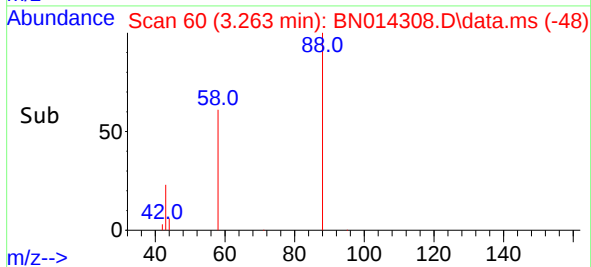
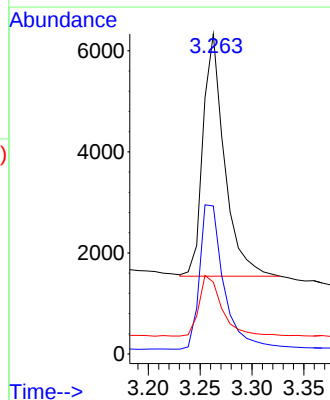
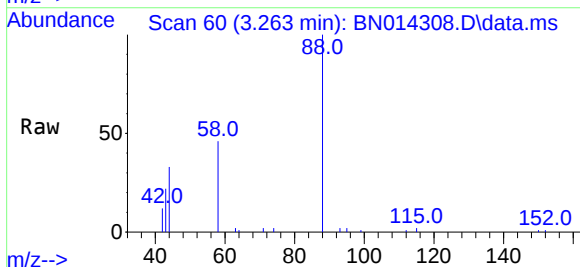


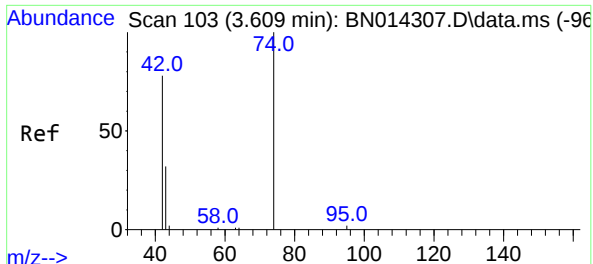

#3
n-Nitrosodimethylamine
Concen: 0.90 ng
RT: 3.601 min Scan# 102
Delta R.T. -0.008 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09




Instrument :
BNA_N
ClientSampled :
SSTDIC0.8


Tgt Ion: 42 Resp: 3837
Ion Ratio Lower Upper
42 100
74 131.9 104.6 157.0
44 3.3 2.4 3.6

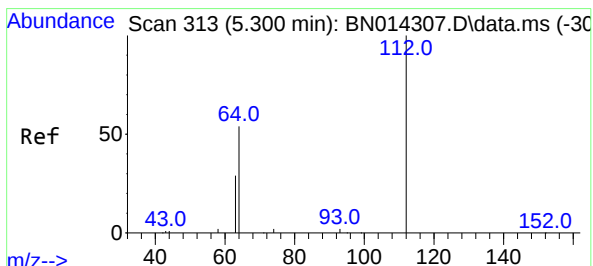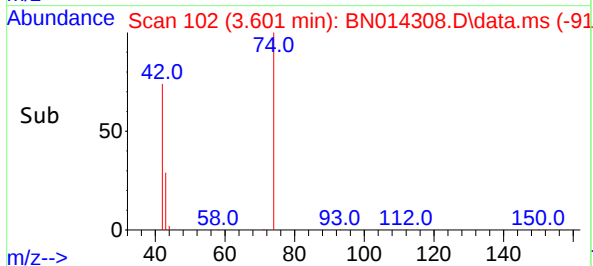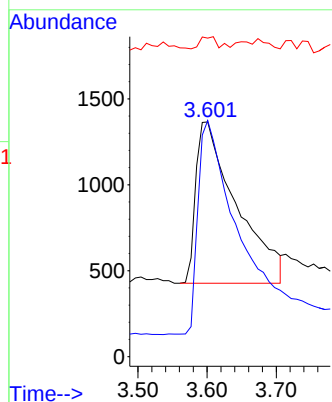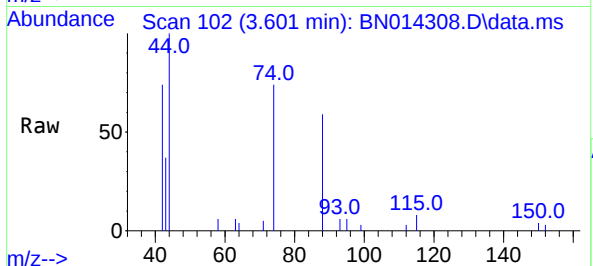

#4
2-Fluorophenol
Concen: 0.73 ng
RT: 5.300 min Scan# 313
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09

Tgt Ion: 112 Resp: 12317
Ion Ratio Lower Upper
112 100
64 55.0 43.7 65.5
63 29.7 23.8 35.8


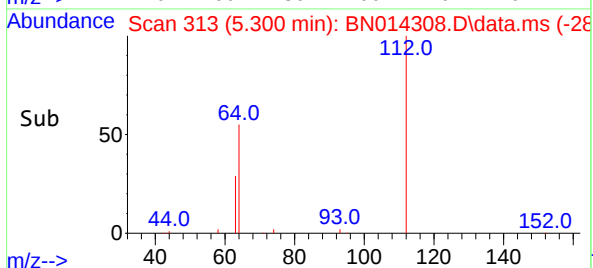

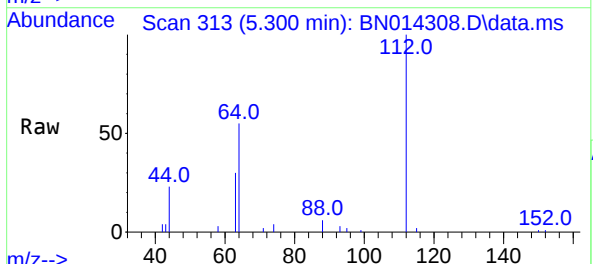




#5
Phenol-d6
Concen: 0.72 ng
RT: 6.871 min Scan# 508
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09




Instrument :
BNA_N
ClientSampled :
SSTDICC0.8


Tgt Ion: 99 Resp: 15228
Ion Ratio Lower Upper
99 100
42 19.3 15.7 23.5
71 34.6 27.6 41.4

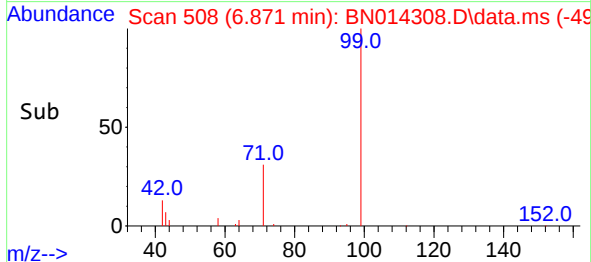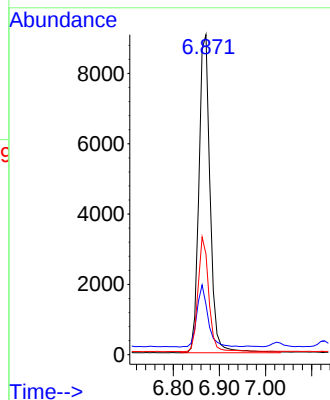

#6
bis(2-Chloroethyl)ether
Concen: 0.84 ng
RT: 7.128 min Scan# 540
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09

Tgt Ion: 93 Resp: 14492
Ion Ratio Lower Upper
93 100
63 73.8 58.2 87.4
95 33.4 26.7 40.1



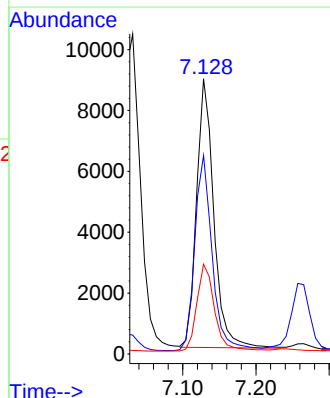





#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.479 min Scan# 858
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:	136	Resp:	25632
Ion Ratio	Lower	Upper	
136	100		
137	11.1	9.0	13.6
54	4.6	3.5	5.3
68	4.1	3.4	5.2

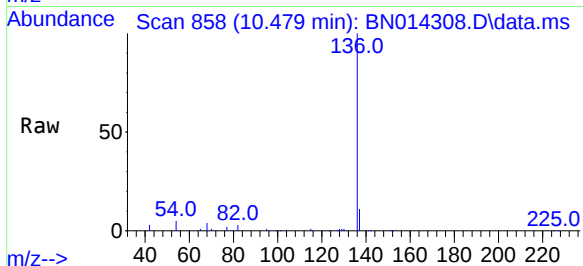

#8
Nitrobenzene-d5
Concen: 0.80 ng
RT: 8.844 min Scan# 729
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09

Tgt Ion:	82	Resp:	12951
Ion Ratio	Lower	Upper	
82	100		
128	42.6	35.3	52.9
54	40.4	33.4	50.2




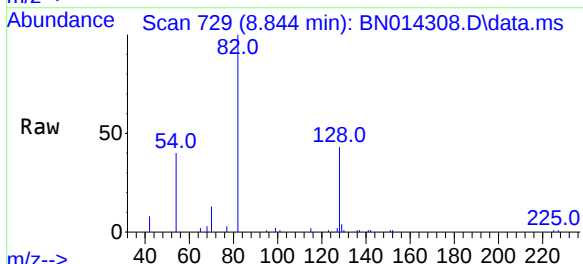


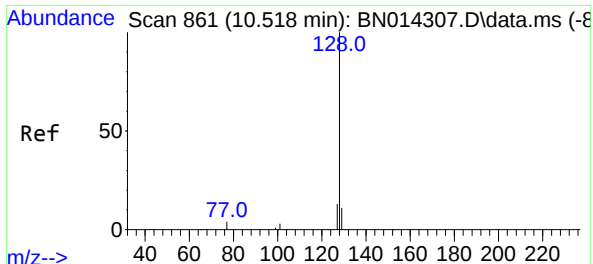

#9
Naphthalene
Concen: 0.81 ng
RT: 10.517 min Scan# 861
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09




Instrument :
BNA_N
ClientSampled :
SSTDIC0.8


Tgt Ion:128 Resp: 51679
Ion Ratio Lower Upper
128 100
129 11.1 9.0 13.4
127 13.2 10.7 16.1

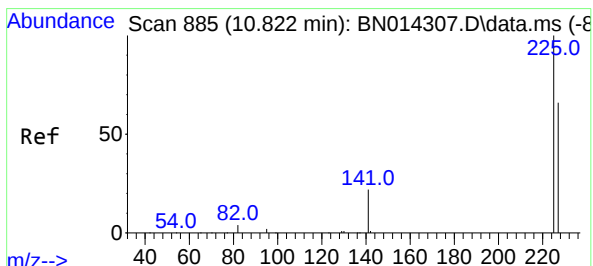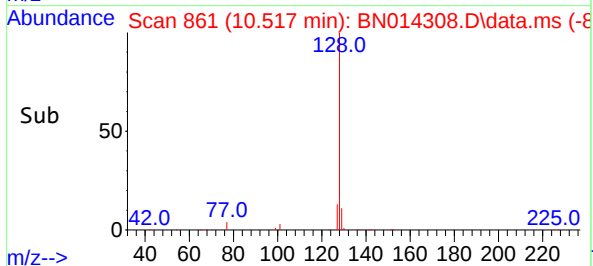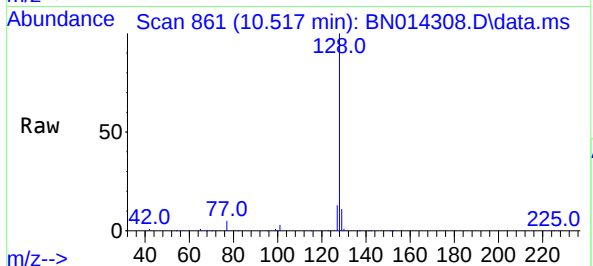

#10
Hexachlorobutadiene
Concen: 0.81 ng
RT: 10.822 min Scan# 885
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09

Tgt Ion:225 Resp: 10298
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 63.6 50.9 76.3


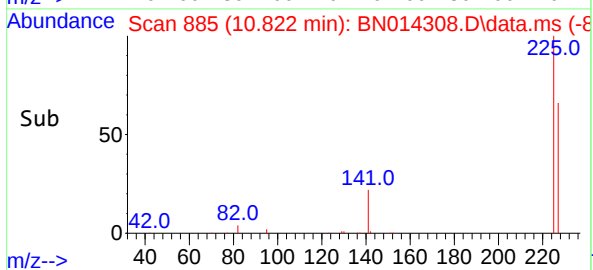

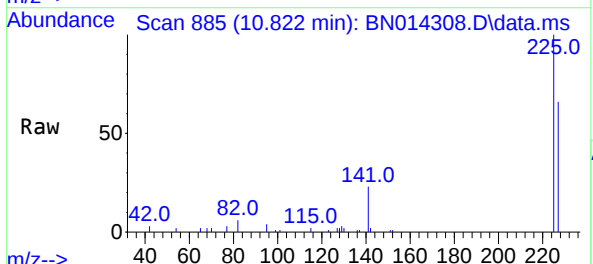




#11
2-Methylnaphthalene-d10
Concen: 0.78 ng
RT: 12.066 min Scan# 1065
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09




Instrument :
BNA_N
ClientSampled :
SSTDICC0.8


Tgt Ion:152 Resp: 31217
Ion Ratio Lower Upper
152 100
151 20.2 16.2 24.4

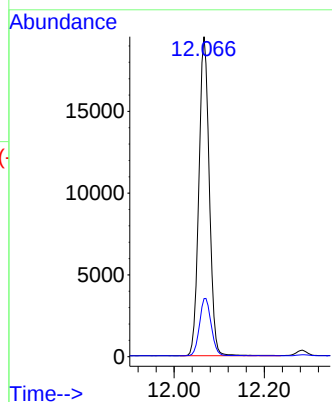

#12
2-Methylnaphthalene
Concen: 0.79 ng
RT: 12.142 min Scan# 1082
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09

Tgt Ion:142 Resp: 33644
Ion Ratio Lower Upper
142 100
141 87.8 70.0 105.0
115 35.5 28.8 43.2









#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.333 min Scan# 1308
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:164 Resp: 12817
Ion Ratio Lower Upper
164 100
162 99.5 78.6 117.8
160 45.2 36.2 54.4

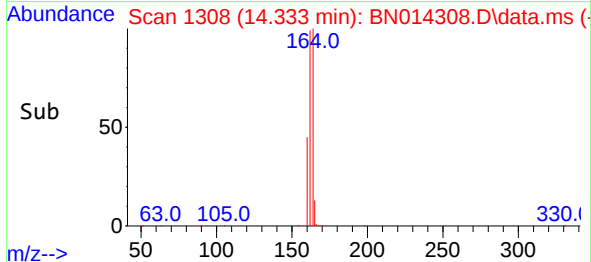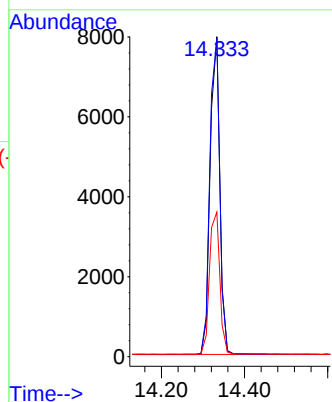

#14
2,4,6-Tribromophenol
Concen: 0.70 ng
RT: 15.818 min Scan# 1425
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09

Tgt Ion:330 Resp: 3492
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 33.6 28.8 43.2


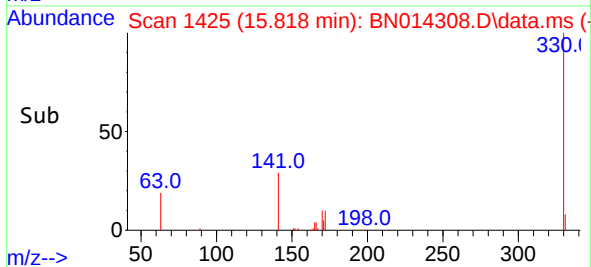

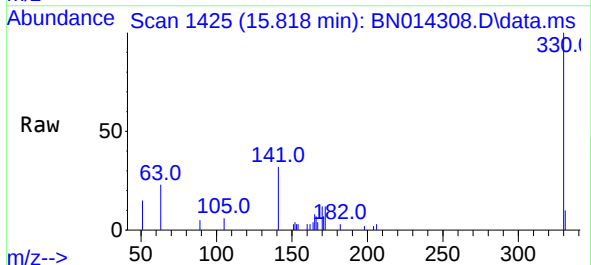




#15
2-Fluorobiphenyl
Concen: 0.92 ng
RT: 12.950 min Scan# 1199
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:172	Resp:	43050
Ion	Ratio	Lower Upper
172	100	
171	34.2	27.9 41.9
170	23.2	18.8 28.2

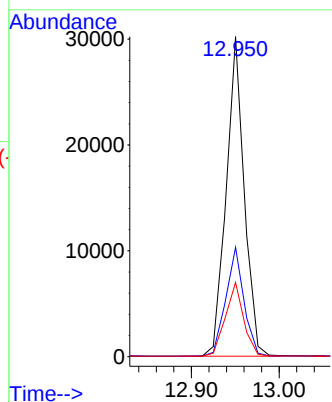

#16
Acenaphthylene
Concen: 0.77 ng
RT: 14.041 min Scan# 1285
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09

Tgt Ion:152	Resp:	37804
Ion	Ratio	Lower Upper
152	100	
151	19.5	15.9 23.9
153	13.0	10.6 15.8


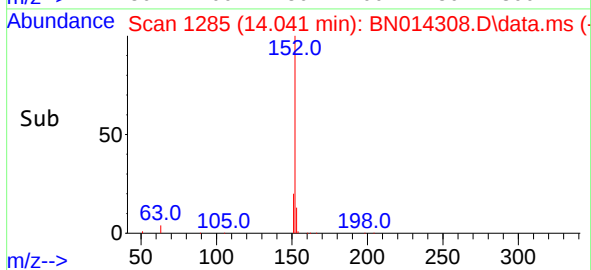
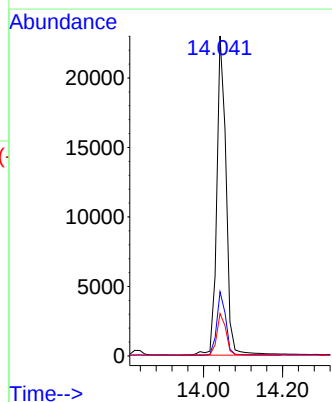





#17
Acenaphthene
Concen: 0.81 ng
RT: 14.397 min Scan# 1313
Delta R.T. 0.012 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:154 Resp: 29359
Ion Ratio Lower Upper
154 100
153 110.2 89.4 134.2
152 55.0 44.7 67.1

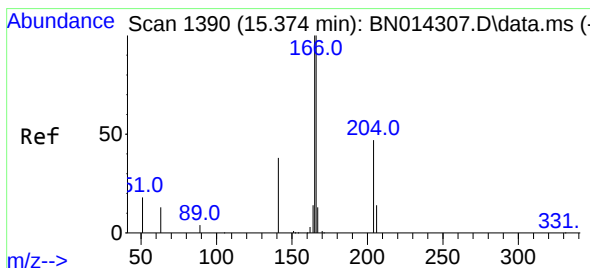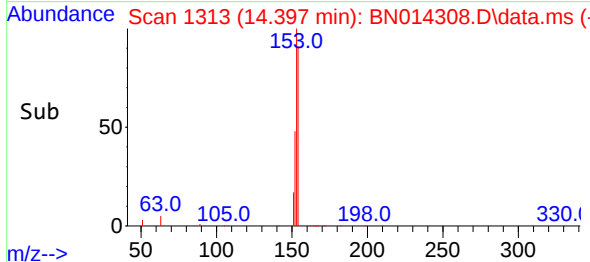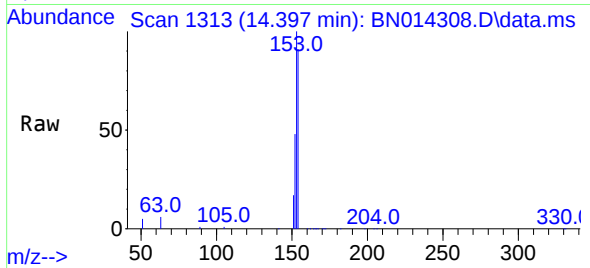

#18
Fluorene
Concen: 0.78 ng
RT: 15.374 min Scan# 1390
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09

Tgt Ion:166 Resp: 35603
Ion Ratio Lower Upper
166 100
165 98.5 78.2 117.2
167 13.4 10.9 16.3


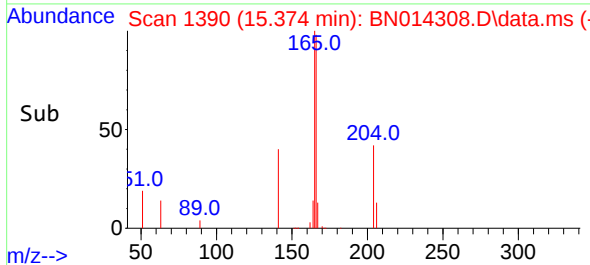

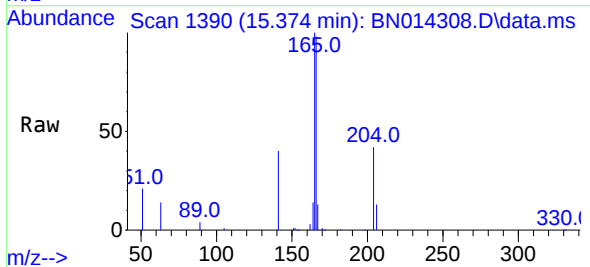




#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.080 min Scan# 1528
Delta R.T. 0.012 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:188 Resp: 26365
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 6.2 10.2 15.4#



#20
4,6-Dinitro-2-methylphenol
Concen: 0.70 ng
RT: 15.450 min Scan# 1396
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09

Tgt Ion:198 Resp: 2173
Ion Ratio Lower Upper
198 100
51 65.2 82.6 123.8#
105 56.0 56.1 84.1#


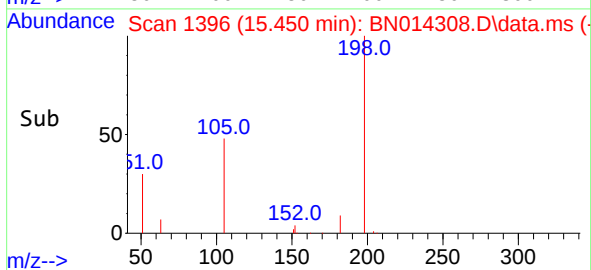






#21
4-Bromophenyl-phenylether
Concen: 0.83 ng
RT: 16.276 min Scan# 1462
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09




Instrument :
BNA_N
ClientSampled :
SSTDIC0.8


Tgt Ion:	248	Resp:	11193
Ion	Ratio	Lower	Upper
248	100		
250	104.5	81.9	122.9
141	36.8	29.3	43.9

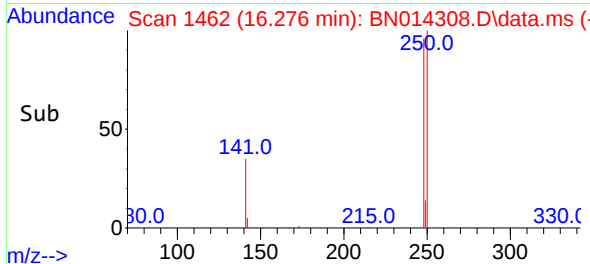

#22
Hexachlorobenzene
Concen: 0.85 ng
RT: 16.386 min Scan# 1471
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09

Tgt Ion:	284	Resp:	14566
Ion	Ratio	Lower	Upper
284	100		
142	33.7	27.0	40.6
249	29.6	23.7	35.5


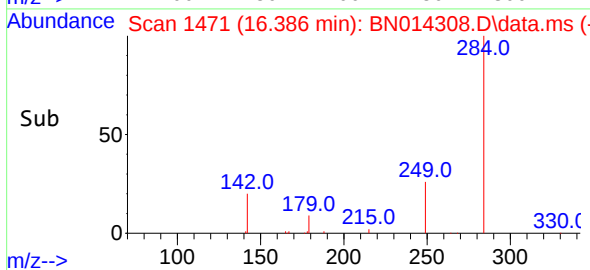

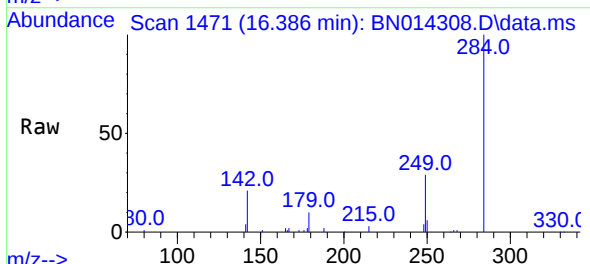


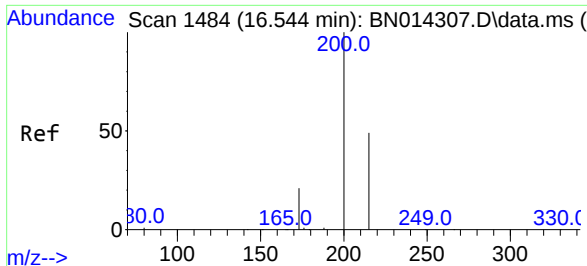

#23
Atrazine
Concen: 0.64 ng
RT: 16.544 min Scan# 1484
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:	200	Resp:	6459
Ion Ratio	Lower	Upper	
200	100		
173	22.6	18.5	27.7
215	49.4	40.0	60.0

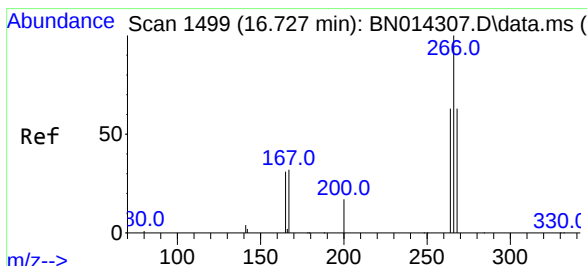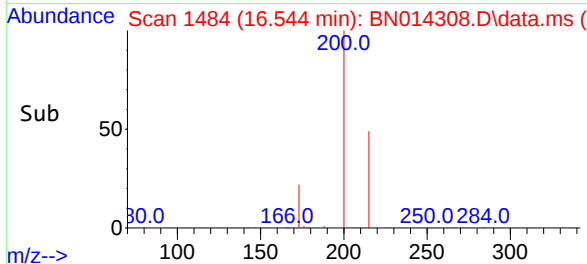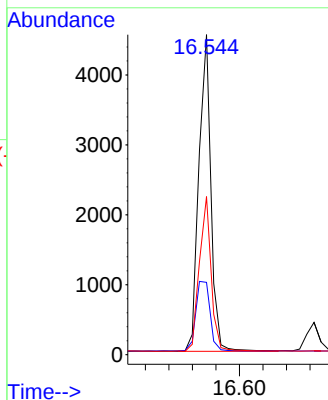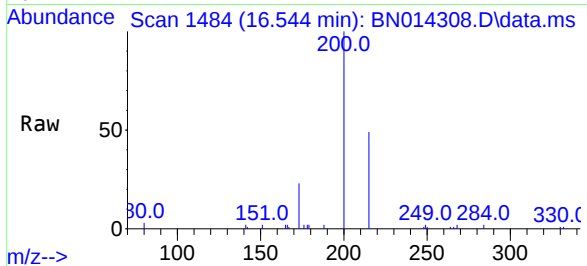

#24
Pentachlorophenol
Concen: 0.67 ng
RT: 16.727 min Scan# 1499
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09

Tgt Ion:	266	Resp:	3537
Ion Ratio	Lower	Upper	
266	100		
264	62.8	49.8	74.8
268	63.8	50.7	76.1


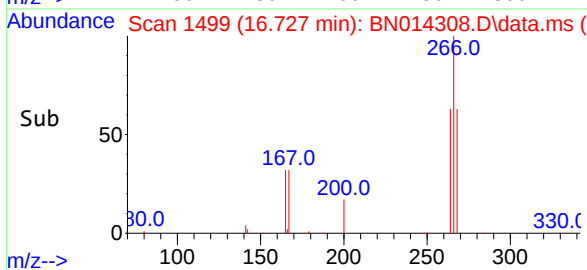
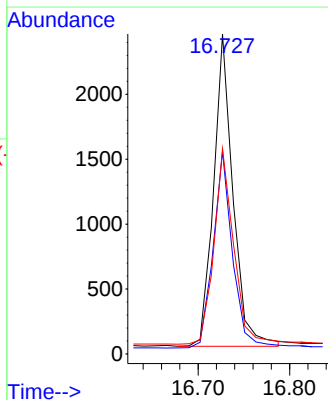
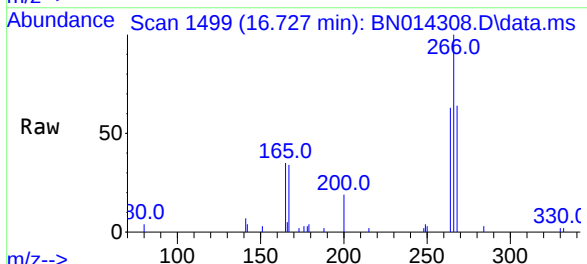




#25
Phenanthrene
Concen: 0.80 ng
RT: 17.116 min Scan# 1531
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:178 Resp: 58529
Ion Ratio Lower Upper
178 100
176 19.3 15.3 22.9
179 15.3 12.2 18.4

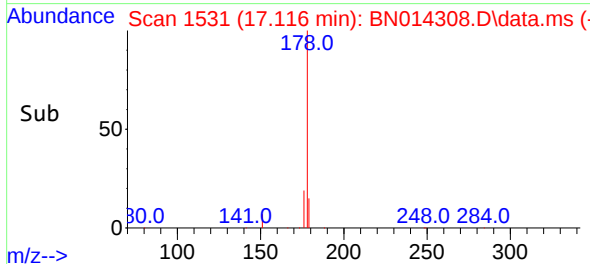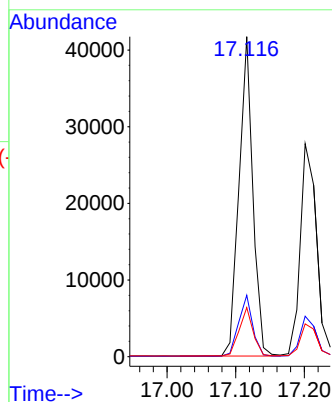

#26
Anthracene
Concen: 0.76 ng
RT: 17.201 min Scan# 1538
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09

Tgt Ion:178 Resp: 45835
Ion Ratio Lower Upper
178 100
176 18.5 14.8 22.2
179 15.4 12.2 18.4


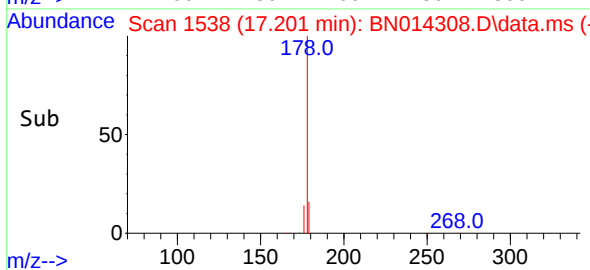

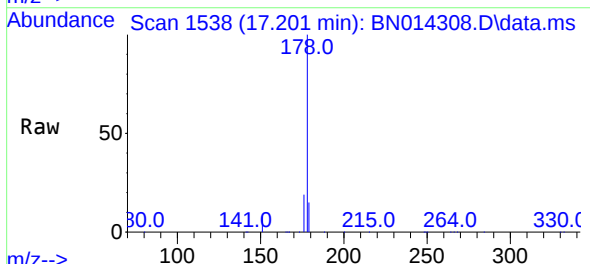




#27
Fluoranthene-d10
Concen: 0.74 ng
RT: 19.109 min Scan# 1825
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:212 Resp: 56803
Ion Ratio Lower Upper
212 100
106 12.0 9.7 14.5
104 6.7 5.5 8.3

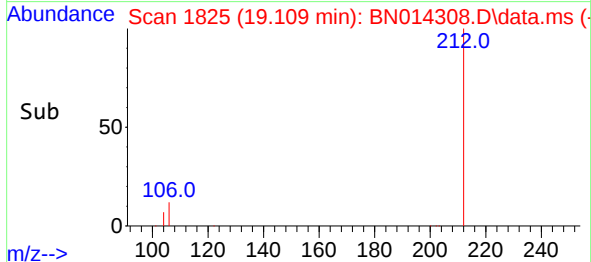

#28
Fluoranthene
Concen: 0.77 ng
RT: 19.139 min Scan# 1831
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09

Tgt Ion:202 Resp: 64237
Ion Ratio Lower Upper
202 100
101 10.2 8.3 12.5
203 17.2 13.8 20.6


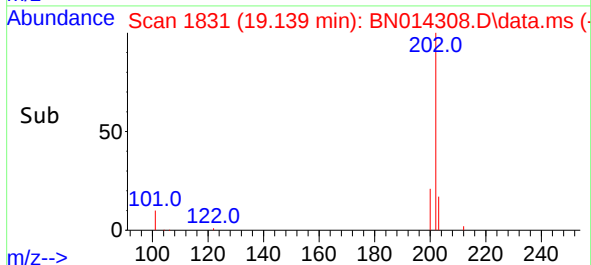
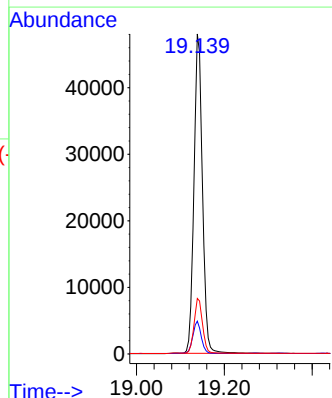
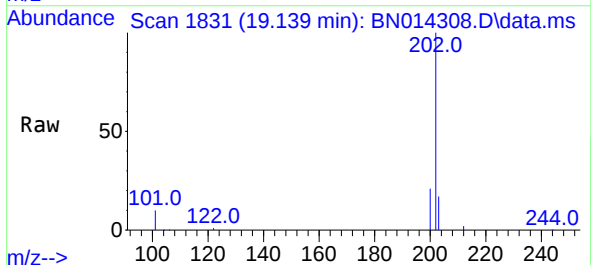




#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.271 min Scan# 2125
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09




Instrument :
BNA_N
ClientSampled :
SSTDICC0.8


Tgt Ion:240 Resp: 28162
Ion Ratio Lower Upper
240 100
120 6.7 5.4 8.0
236 26.0 20.4 30.6

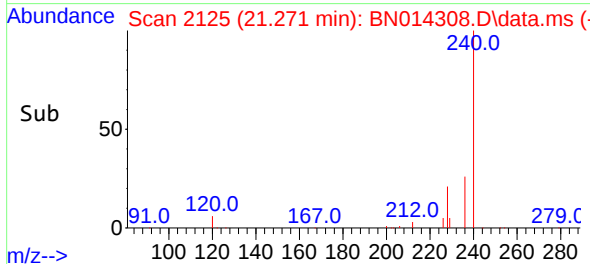

#30
Pyrene
Concen: 0.71 ng
RT: 19.506 min Scan# 1905
Delta R.T. 0.005 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09

Tgt Ion:202 Resp: 63083
Ion Ratio Lower Upper
202 100
200 20.7 16.6 24.8
203 17.4 14.0 21.0


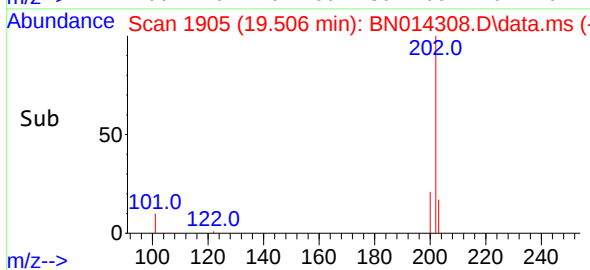

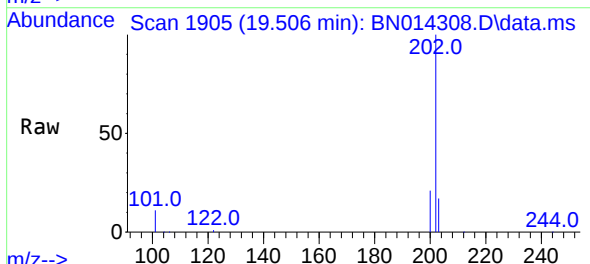




#31
 Terphenyl-d14
 Concen: 0.78 ng
 RT: 19.714 min Scan# 1947
 Delta R.T. -0.000 min
 Lab File: BN014308.D
 Acq: 16 Apr 2021 14:09




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8


Tgt Ion:244 Resp: 48319
 Ion Ratio Lower Upper
 244 100
 212 7.7 6.2 9.4
 122 11.3 9.0 13.6

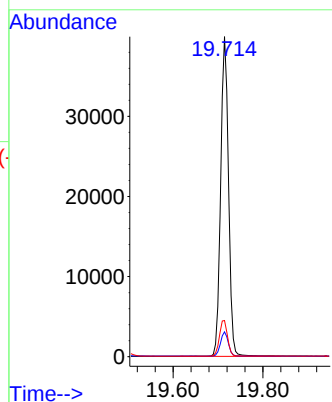

#32
 Benzo(a)anthracene
 Concen: 0.70 ng
 RT: 21.250 min Scan# 2123
 Delta R.T. -0.000 min
 Lab File: BN014308.D
 Acq: 16 Apr 2021 14:09

Tgt Ion:228 Resp: 56285
 Ion Ratio Lower Upper
 228 100
 226 27.4 21.7 32.5
 229 19.5 15.7 23.5






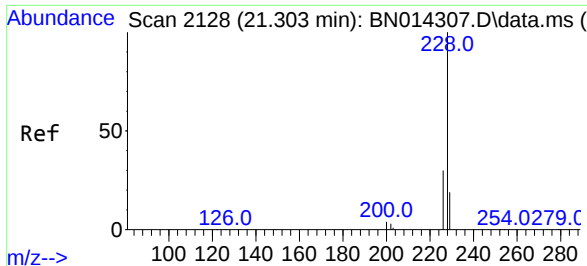


#33
Chrysene
Concen: 0.79 ng
RT: 21.303 min Scan# 2128
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8

Tgt Ion:228 Resp: 68601




Ion	Ratio	Lower	Upper
228	100		
226	29.8	23.8	35.6
229	19.5	15.6	23.4

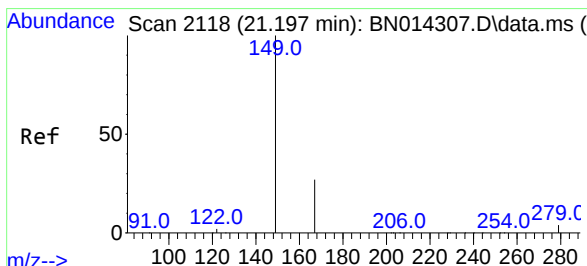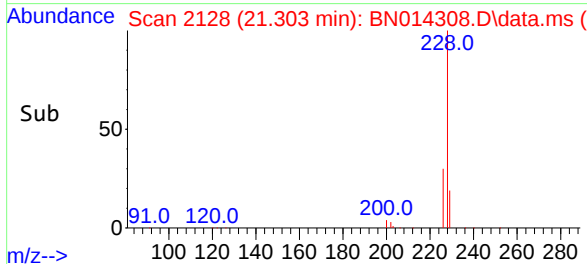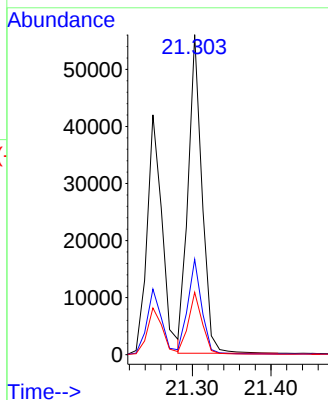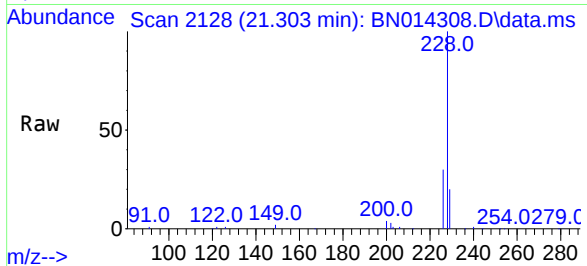


#34
Bis(2-ethylhexyl)phthalate
Concen: 0.53 ng
RT: 21.197 min Scan# 2118
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09

Tgt Ion:149 Resp: 15173

Ion	Ratio	Lower	Upper
149	100		
167	26.4	21.0	31.4
279	4.0	3.3	4.9


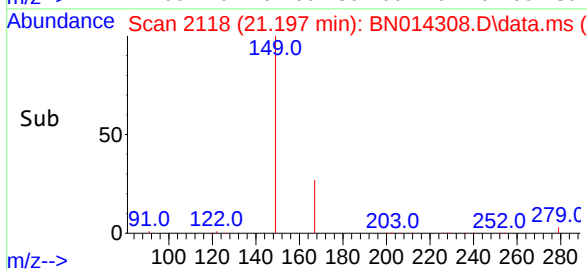
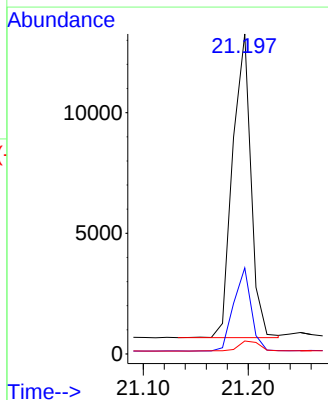
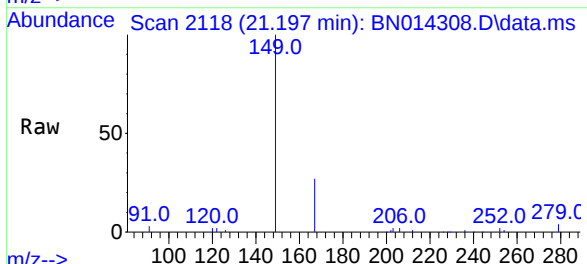




#35
Indeno(1,2,3-cd)pyrene
Concen: 0.78 ng
RT: 25.741 min Scan# 3206
Delta R.T. 0.003 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09




Instrument :
BNA_N
ClientSampled :
SSTDICC0.8


Tgt Ion:276 Resp: 79566
Ion Ratio Lower Upper
276 100
138 23.6 18.3 27.5
277 24.8 19.9 29.9

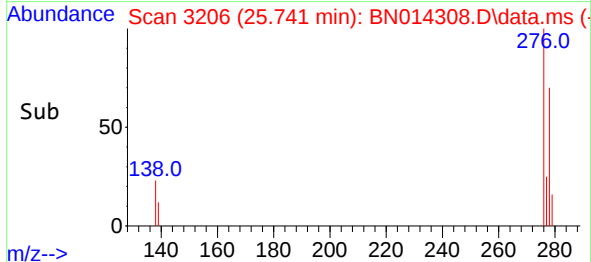

#36
Perylene-d12
Concen: 0.40 ng
RT: 23.499 min Scan# 2551
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09

Tgt Ion:264 Resp: 22700
Ion Ratio Lower Upper
264 100
260 24.4 20.0 30.0
265 47.4 37.8 56.8


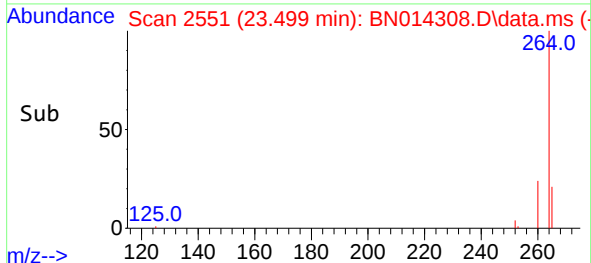

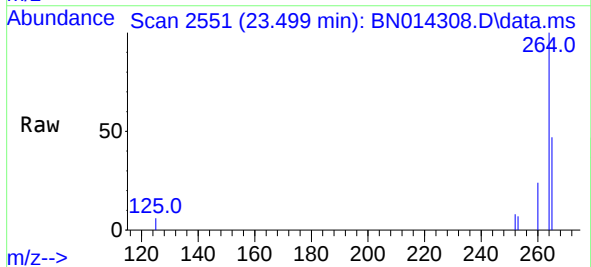




#37
Benzo(b)fluoranthene
Concen: 0.92 ng
RT: 22.828 min Scan# 2355
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:252 Resp: 73962
Ion Ratio Lower Upper
252 100
253 22.9 19.0 28.6
125 10.7 9.3 13.9

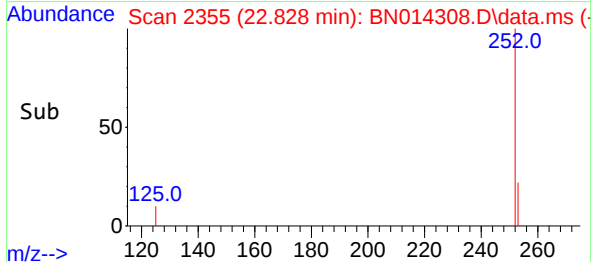

#38
Benzo(k)fluoranthene
Concen: 0.89 ng
RT: 22.873 min Scan# 2368
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09


Tgt Ion:252 Resp: 71918
Ion Ratio Lower Upper
252 100
253 22.9 19.1 28.7
125 10.4 9.1 13.7

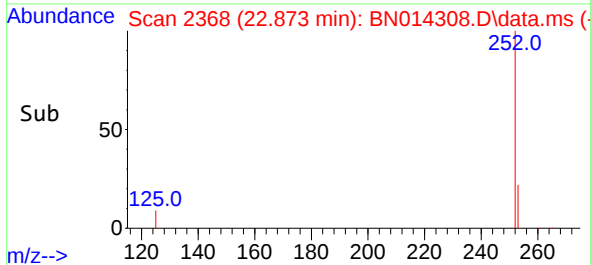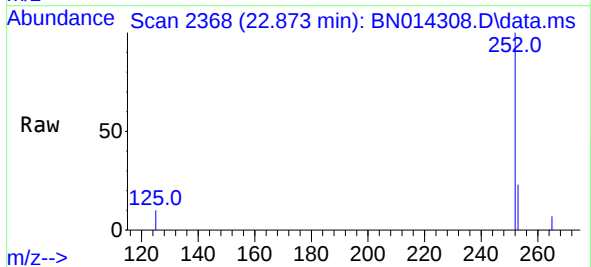






#39
Benzo(a)pyrene
Concen: 0.82 ng
RT: 23.400 min Scan# 2522
Delta R.T. -0.000 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09


Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8





Tgt Ion:252 Resp: 55924
Ion Ratio Lower Upper
252 100
253 24.0 20.2 30.2
125 13.3 12.4 18.6




#40
Dibenzo(a,h)anthracene
Concen: 0.85 ng
RT: 25.755 min Scan# 3210
Delta R.T. 0.003 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09

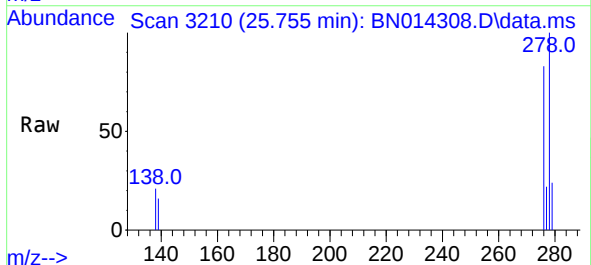


Tgt Ion:278 Resp: 66492
Ion Ratio Lower Upper
278 100
139 15.7 12.8 19.2
279 24.4 20.0 30.0

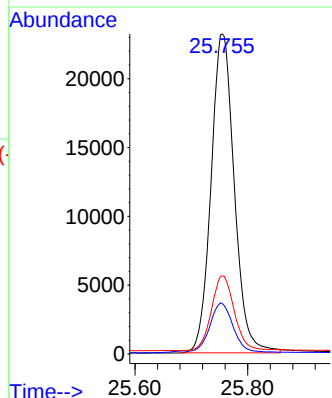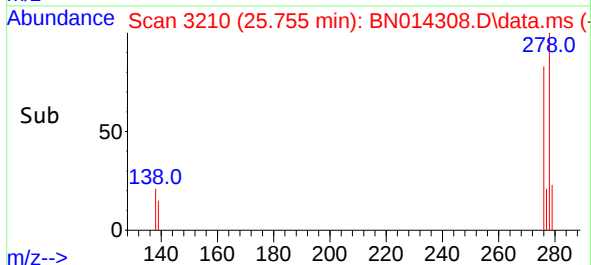

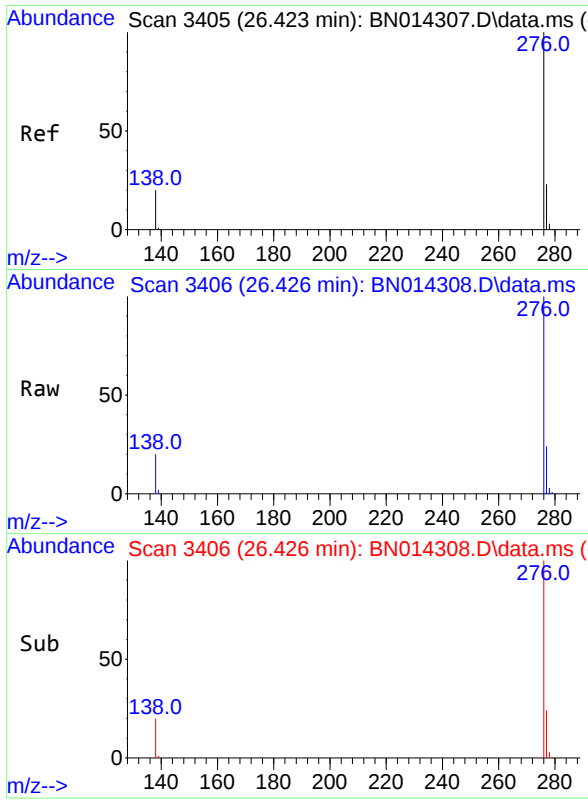

#41
Benzo(g,h,i)perylene
Concen: 0.89 ng
RT: 26.426 min Scan# 3406
Delta R.T. 0.003 min
Lab File: BN014308.D
Acq: 16 Apr 2021 14:09

Tgt Ion	Ratio	Lower	Upper
276	100		
277	24.0	18.9	28.3
138	20.4	16.6	24.8

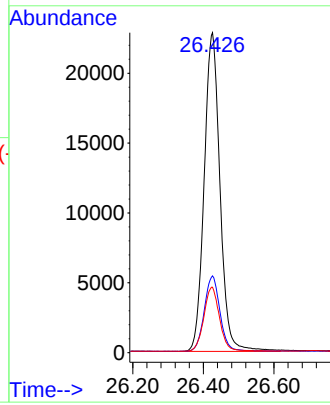

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8