

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042423\
 Data File : BN025116.D
 Acq On : 24 Apr 2023 16:07
 Operator : CG/JU
 Sample : 02400-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COMM4

Quant Time: Apr 25 01:26:18 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Apr 23 01:54:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.916	152	264619	20.000	ng/ul	0.00
20) Naphthalene-d8	10.728	136	1223944	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.563	164	803321	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.310	188	1779468	20.000	ng/ul	0.00
79) Chrysene-d12	21.498	240	1723833	20.000	ng/ul	-0.01
88) Perylene-d12	23.939	264	1828083	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	25361	3.648	ng/uL	0.00
4) Pyridine-d5	3.728	84	121171	5.820	ng/ul	0.01
7) Phenol-d5	7.075	99	127856	4.956	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.240	67	438332	25.402	ng/ul	0.00
11) 2-Chlorophenol-d4	7.440	132	368081	19.414	ng/ul	0.00
15) 4-Methylphenol-d8	8.628	113	256365	12.517	ng/ul	0.00
21) Nitrobenzene-d5	9.081	128	244769	24.699	ng/ul	0.00
24) 2-Nitrophenol-d4	9.810	143	260728	24.290	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.346	165	440870	22.979	ng/ul	0.00
31) 4-Chloroaniline-d4	10.869	131	525414	18.045	ng/ul	0.00
46) Dimethylphthalate-d6	13.969	166	1836359	29.488	ng/ul	0.00
49) Acenaphthylene-d8	14.257	160	1947527	27.290	ng/ul	0.00
54) 4-Nitrophenol-d4	14.763	143	48386	3.790	ng/ul	0.00
60) Fluorene-d10	15.551	176	1587505	30.193	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.675	200	172430	14.889	ng/ul	0.00
73) Anthracene-d10	17.410	188	2699644	32.302	ng/ul	0.00
81) Pyrene-d10	19.704	212	3279212	32.759	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.786	264	3099977	32.432	ng/ul	0.00
Target Compounds						
					Qvalue	
75) 1,2,3,4-Tetrachloroben...	13.363	216	34943	1.381	ng/uL	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042423\
Data File : BN025116.D
Acq On : 24 Apr 2023 16:07
Operator : CG/JU
Sample : 02400-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COMM4

Quant Time: Apr 25 01:26:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Apr 23 01:54:00 2023
Response via : Initial Calibration

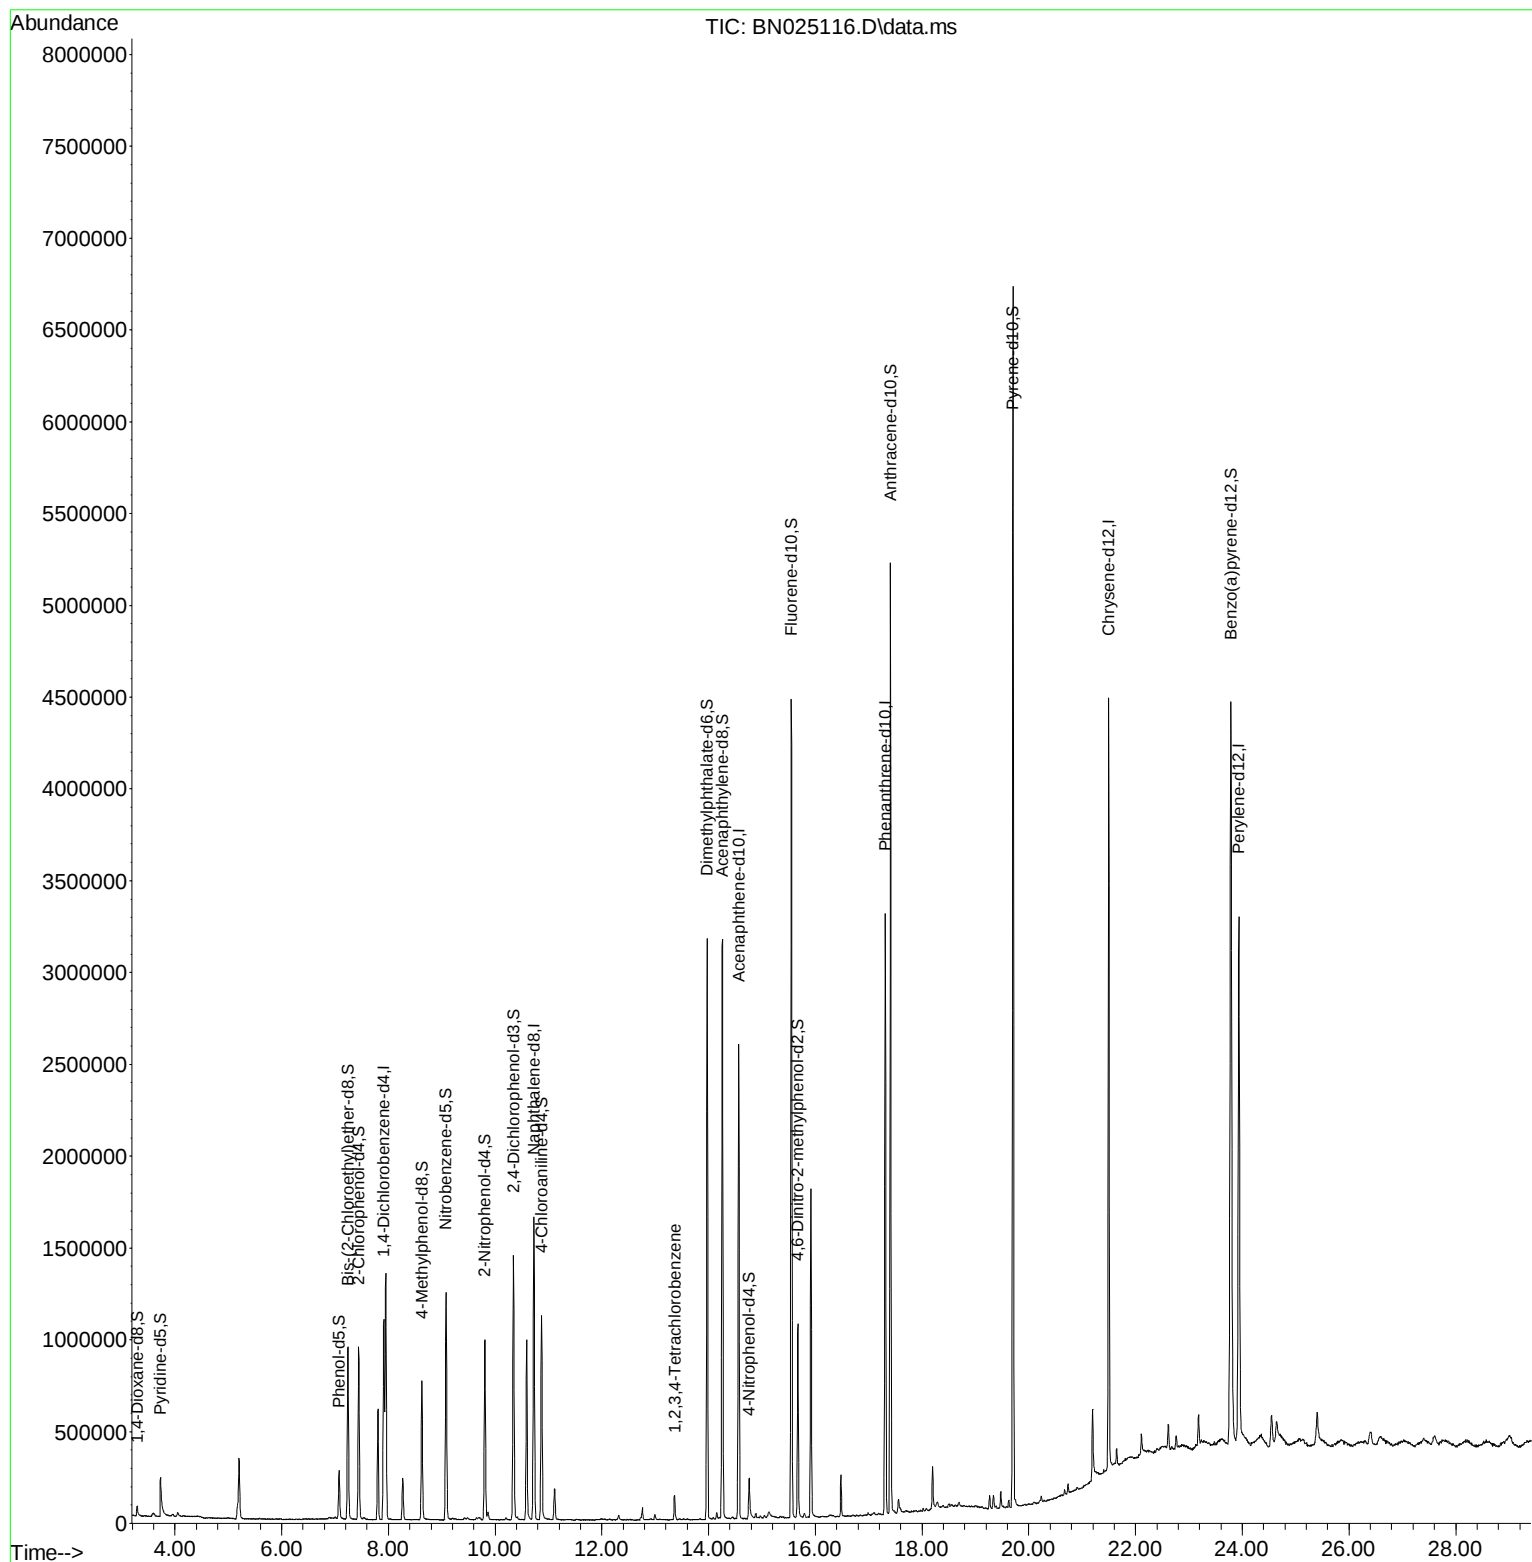

Abundance Scan 1730 (13.363 min): BN025107.D\data.ms (-1725) (-)

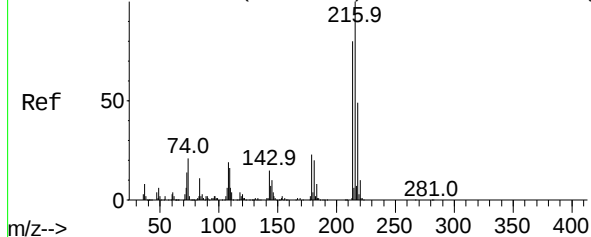

1,2,3,4-Tetrachlorobenzene

Concen: 1.381 ng/uL

RT: 13.363 min Scan# 1

Delta R.T. 0.000 min

Lab File: BN025116.D

Acq: 24 Apr 2023 16:07


Instrument :

BNA_N

ClientSampleId :

COMM4

Abundance Scan 1730 (13.363 min): BN025116.D\data.ms

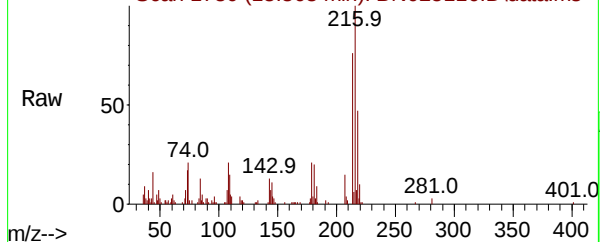


Tgt Ion:216 Resp: 34943

Ion Ratio Lower Upper

216 100

214 76.1 62.5 93.7

218 46.7 37.7 56.5

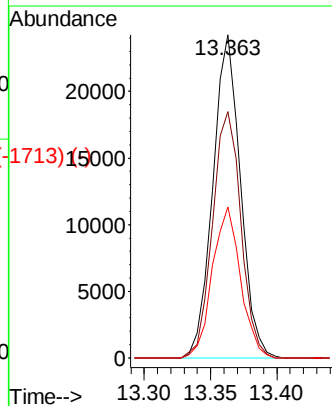

Abundance Scan 1730 (13.363 min): BN025116.D\data.ms (-1713)

