

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042423\
 Data File : BN025120.D
 Acq On : 24 Apr 2023 19:06
 Operator : CG/JU
 Sample : PB152288BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK288

Manual Integrations
 APPROVED

Reviewed By : Christian Giraldo 04/25/2023
 Supervised By : Jagrut Upadhyay 04/27/2023

Quant Time: Apr 25 01:26:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Apr 23 01:54:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.922	152	15197	20.000	ng/u1	0.00
20) Naphthalene-d8	10.728	136	50994	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.563	164	23817	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.310	188	47419	20.000	ng/u1	0.00
79) Chrysene-d12	21.498	240	44235	20.000	ng/u1	-0.01
88) Perylene-d12	23.927	264	46511	20.000	ng/u1	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	874	2.189	ng/uL	0.01
4) Pyridine-d5	3.781	84	32933m	27.544	ng/u1	0.06
7) Phenol-d5	7.087	99	41694	28.141	ng/u1	0.01
9) Bis-(2-Chloroethyl)eth...	7.252	67	31796	32.085	ng/u1	0.00
11) 2-Chlorophenol-d4	7.452	132	34258	31.463	ng/u1	0.00
15) 4-Methylphenol-d8	8.634	113	28154m	23.936	ng/u1	0.00
21) Nitrobenzene-d5	9.087	128	12198	29.543	ng/u1	0.00
24) 2-Nitrophenol-d4	9.810	143	11192	25.025	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.357	165	22278	27.870	ng/u1	0.01
31) 4-Chloroaniline-d4	10.875	131	34271	28.251	ng/u1	0.00
46) Dimethylphthalate-d6	13.969	166	66392	35.959	ng/u1	0.00
49) Acenaphthylene-d8	14.257	160	68088	32.181	ng/u1	0.00
54) 4-Nitrophenol-d4	14.793	143	4081m	10.783	ng/u1	0.03
60) Fluorene-d10	15.551	176	57476	36.870	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.681	200	1957	6.342	ng/u1	0.00
73) Anthracene-d10	17.410	188	80607	36.194	ng/u1	0.00
81) Pyrene-d10	19.704	212	106627	41.511	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.769	264	111464	45.834	ng/u1	-0.01
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.404	149	15518	7.727	ng/u1#	Qvalue 97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042423\
Data File : BN025120.D
Acq On : 24 Apr 2023 19:06
Operator : CG/JU
Sample : PB152288BL
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
SBLK288

Quant Time: Apr 25 01:26:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Apr 23 01:54:00 2023
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 04/25/2023
Supervised By :Jagrut Upadhyay 04/27/2023

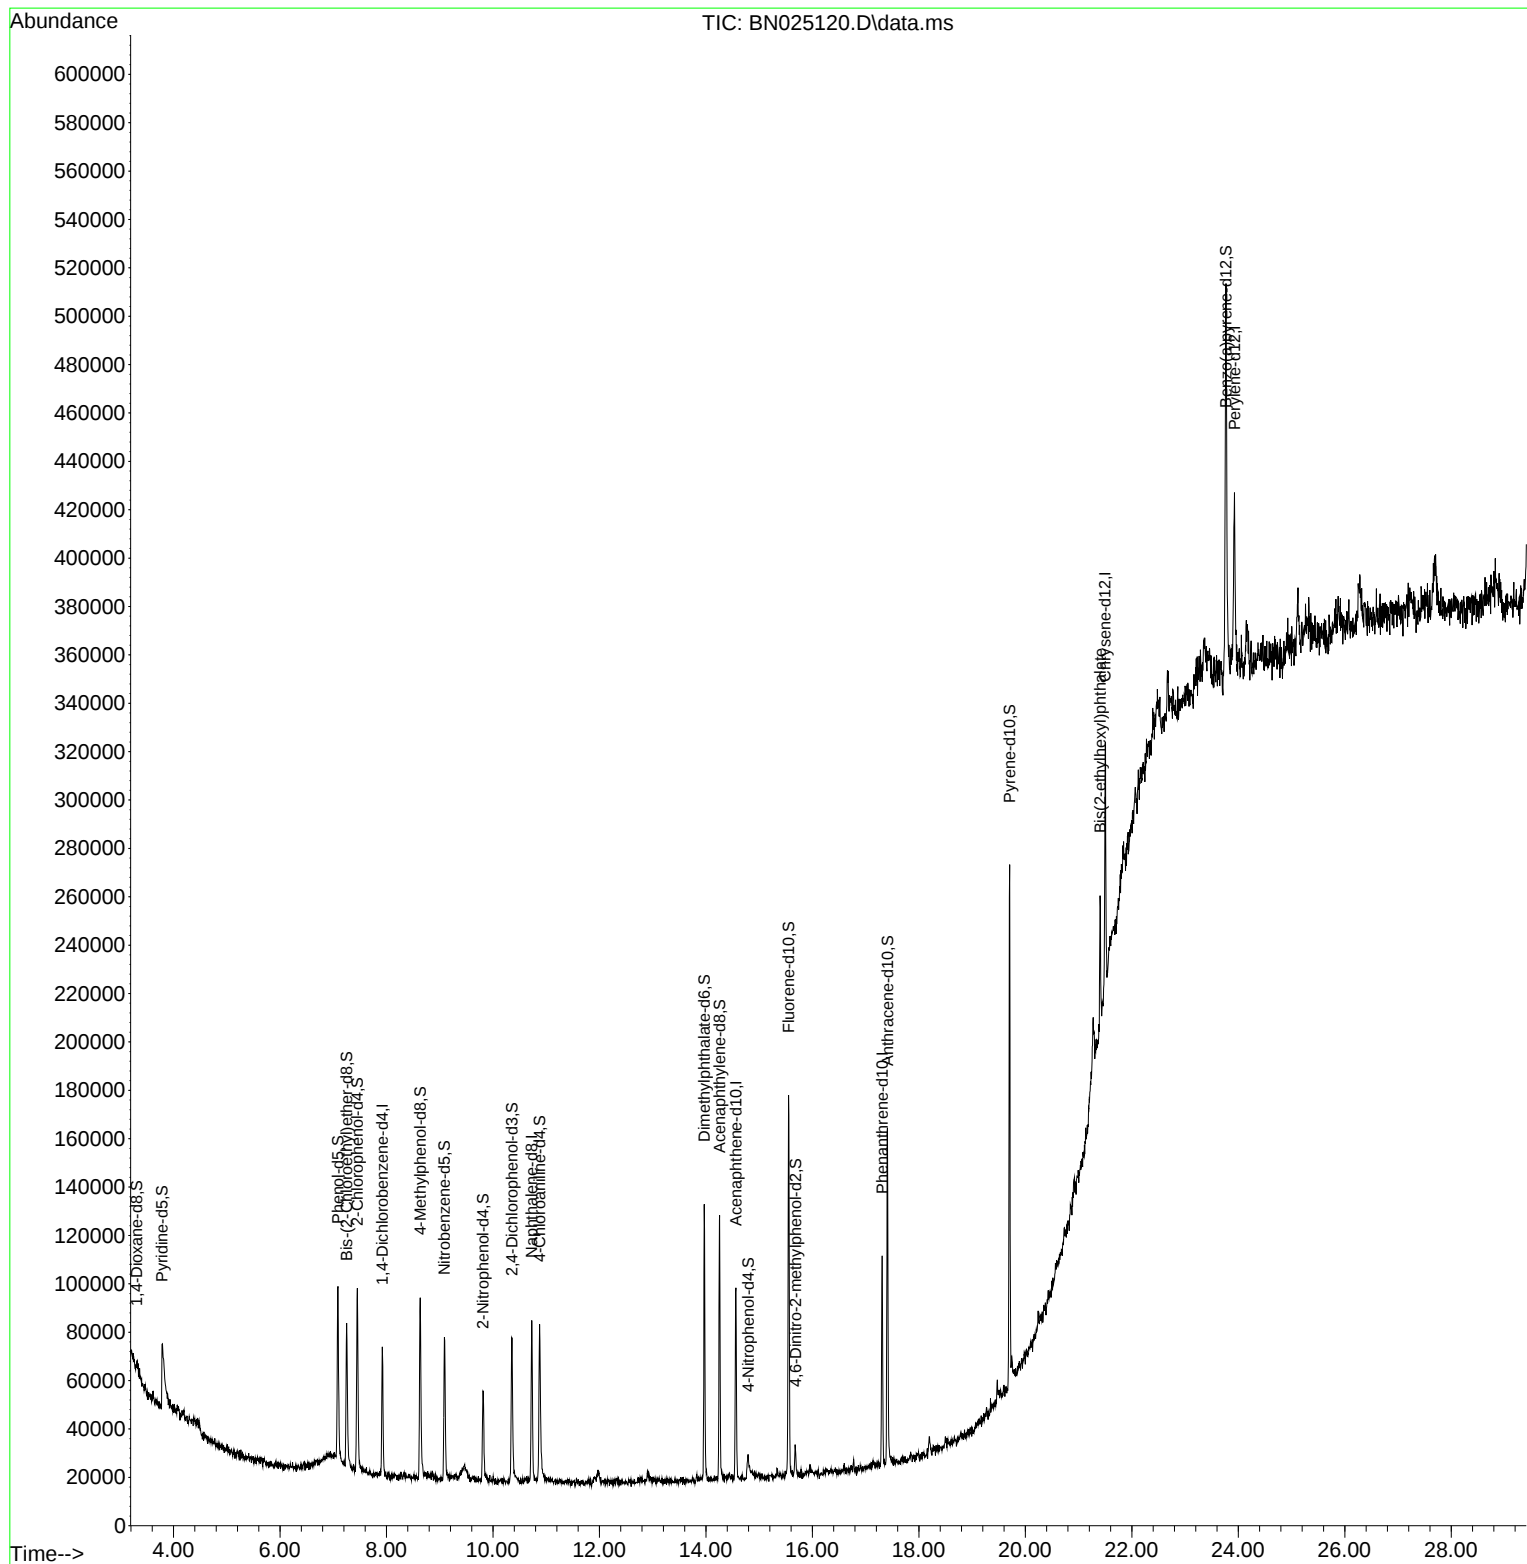

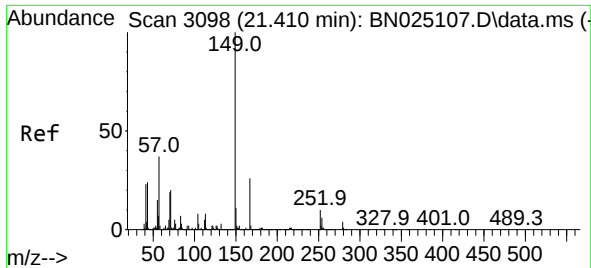

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 7.727 ng/ul
 RT: 21.404 min Scan# 3097
 Delta R.T. -0.006 min
 Lab File: BN025120.D
 Acq: 24 Apr 2023 19:06

Instrument :
 BNA_N
 ClientSampleId :
 SBLK288

Tgt Ion:	149	Resp:	15518
Ion Ratio	Lower	Upper	
149	100		
167	26.2	21.8	32.8
279	5.7	2.9	4.3

Manual Integrations
 APPROVED

Reviewed By :Christian Giraldo 04/25/2023
 Supervised By :Jagrut Upadhyay 04/27/2023

