

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042423\
 Data File : BN025119.D
 Acq On : 24 Apr 2023 18:30
 Operator : CG/JU
 Sample : PB152285BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK285

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Title : SVOA CALIBRATION

Signal : TIC: BN025119.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.287	14	17	24	rBV	73347	99370	1.03%	0.107%
2	3.587	64	68	78	rVB10	6498	15149	0.16%	0.016%
3	3.717	87	90	113	rBV	1030304	1767524	18.28%	1.906%
4	4.052	143	147	156	rVB2	30409	49617	0.51%	0.053%
5	7.075	654	661	675	rVB	1499295	2354720	24.35%	2.539%
6	7.246	682	690	700	rVB	1112129	1781784	18.42%	1.921%
7	7.440	715	723	731	rBV	1436397	2276456	23.54%	2.454%
8	7.916	797	804	814	rBV	1038995	1672997	17.30%	1.804%
9	8.628	917	925	938	rBV	1755282	2887855	29.86%	3.113%
10	9.081	995	1002	1012	rVB	1428312	2322724	24.02%	2.504%
11	9.810	1118	1126	1135	rBV	1201431	2014988	20.84%	2.172%
12	10.346	1207	1217	1227	rBV	1766022	2937713	30.38%	3.167%
13	10.728	1272	1282	1291	rBV	1553892	2637547	27.27%	2.843%
14	10.869	1297	1306	1320	rBV	1904520	3307210	34.20%	3.565%
15	11.975	1488	1494	1498	rBV9	5647	12986	0.13%	0.014%
16	12.316	1546	1552	1558	rBV	28593	46062	0.48%	0.050%
17	13.451	1740	1745	1751	rBV2	28392	46434	0.48%	0.050%
18	13.969	1826	1833	1845	rBV	3219361	4456105	46.08%	4.804%
19	14.257	1872	1882	1898	rBV	3585020	5275472	54.55%	5.687%
20	14.563	1926	1934	1943	rBV	2499999	3635704	37.60%	3.920%
21	14.757	1960	1967	1988	rBV	1801647	2645454	27.36%	2.852%
22	15.551	2094	2102	2115	rBV	4609846	6691759	69.20%	7.214%
23	15.675	2116	2123	2134	rVV	1558953	2056618	21.27%	2.217%
24	15.798	2137	2144	2149	rVB2	23246	41026	0.42%	0.044%
25	16.339	2231	2236	2240	rBV6	5781	10196	0.11%	0.011%
26	17.310	2394	2401	2411	rBV	3201585	4446933	45.98%	4.794%
27	17.410	2411	2418	2430	rBV	5493889	7573464	78.31%	8.165%
28	17.569	2439	2445	2449	rBV5	20225	40343	0.42%	0.043%
29	17.698	2463	2467	2471	rVB4	6850	10262	0.11%	0.011%
30	19.269	2729	2734	2740	rVB2	63616	87966	0.91%	0.095%
31	19.339	2741	2746	2751	rBV	57158	83039	0.86%	0.090%
32	19.704	2802	2808	2814	rBV	6601371	8988131	92.94%	9.690%
33	21.504	3109	3114	3123	rBV	3940015	5059156	52.31%	5.454%
34	23.186	3397	3400	3407	rVB	135183	196360	2.03%	0.212%
35	23.798	3495	3504	3518	rBV	4331272	9670635	100.00%	10.426%
36	23.945	3522	3529	3542	rVV2	2664425	5213398	53.91%	5.620%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042423\
Data File : BN025119.D
Acq On : 24 Apr 2023 18:30
Operator : CG/JU
Sample : PB152285BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK285

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Title : SVOA CALIBRATION

37	24.563	3630	3634	3642	rVB2	185061	344848	3.57%	0.372%
----	--------	------	------	------	------	--------	--------	-------	--------




Sum of corrected areas: 92758005

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042423\
Data File : BN025119.D
Acq On : 24 Apr 2023 18:30
Operator : CG/JU
Sample : PB152285BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK285

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

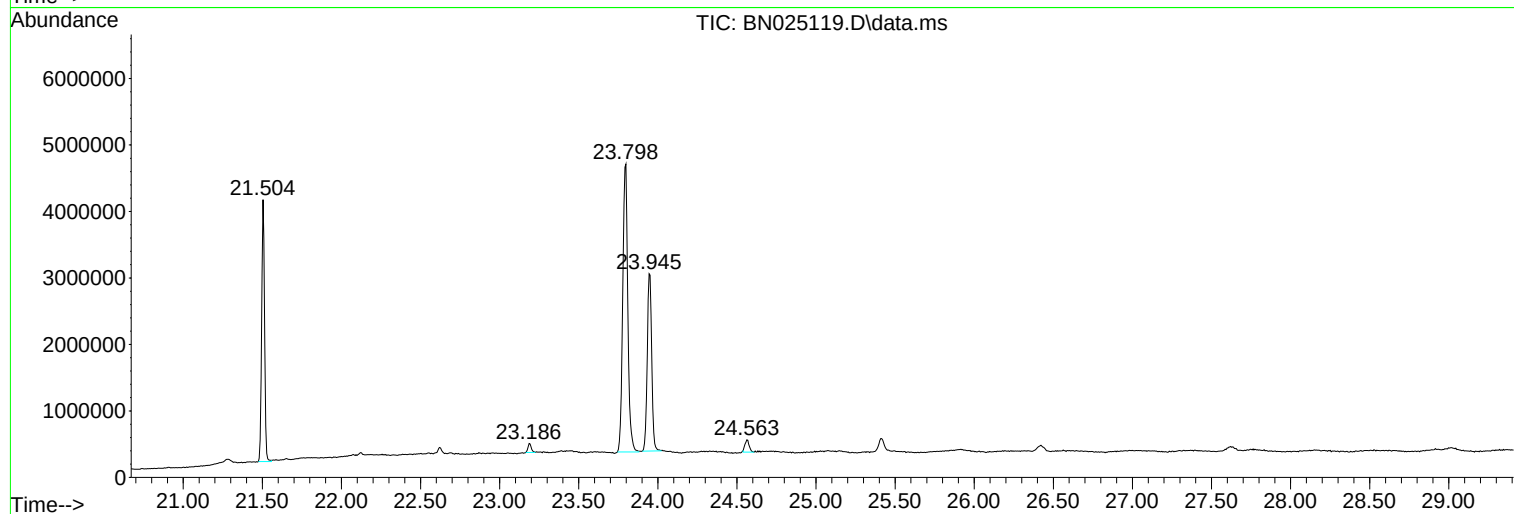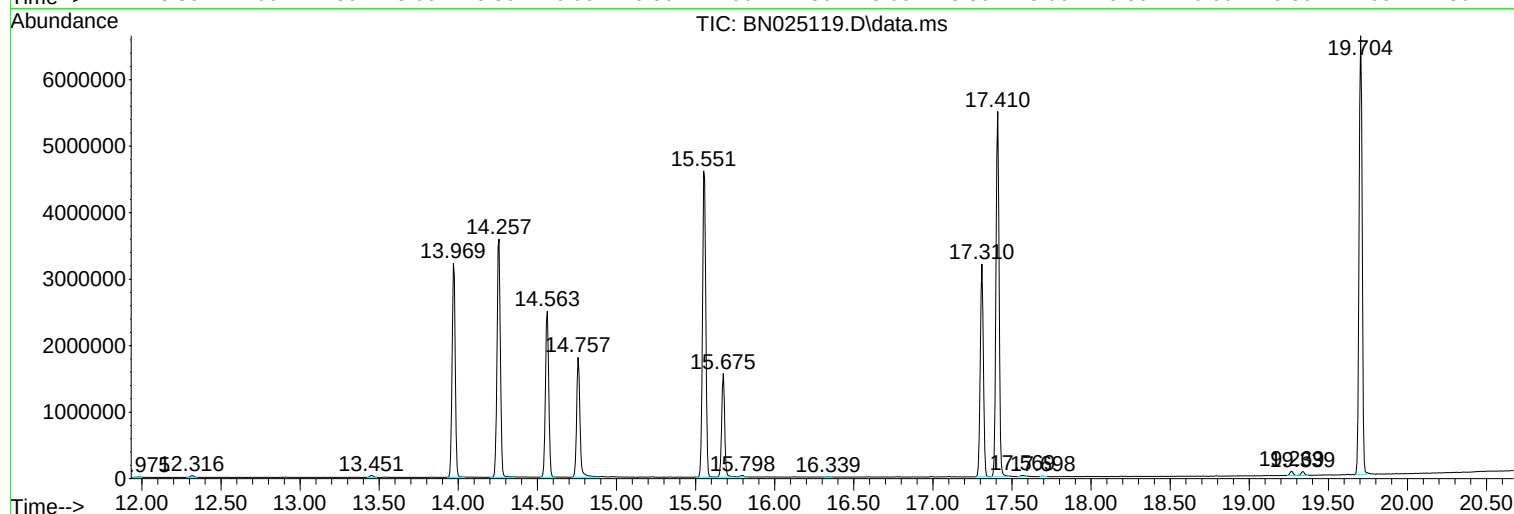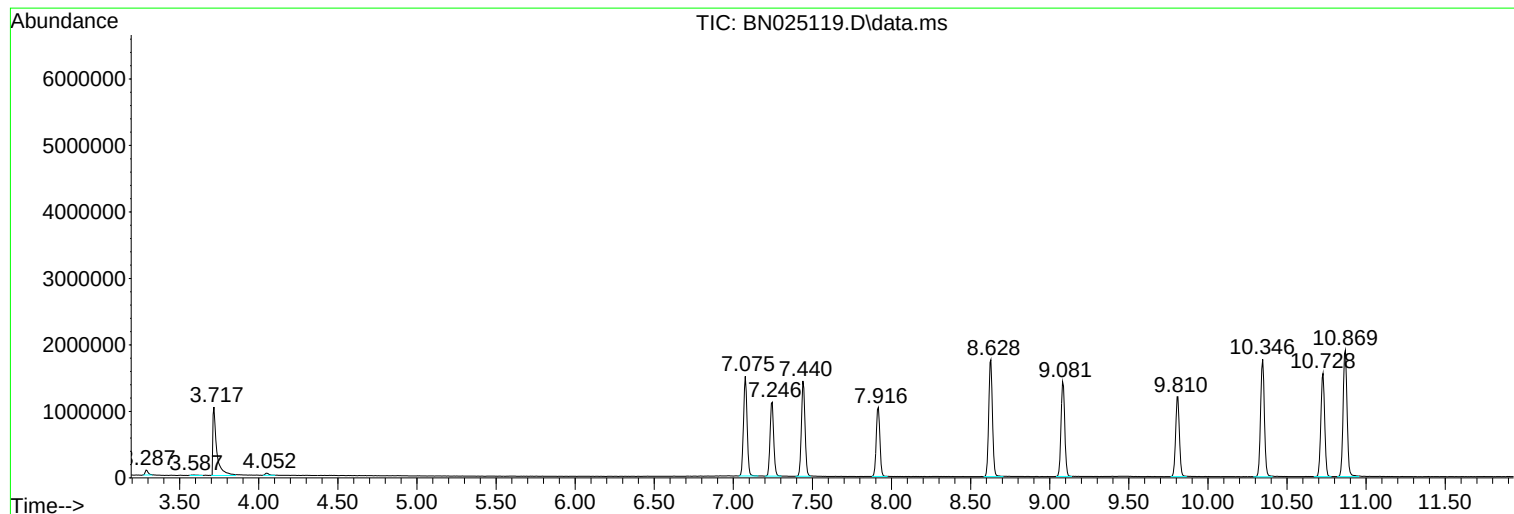

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042423\
Data File : BN025119.D
Acq On : 24 Apr 2023 18:30
Operator : CG/JU
Sample : PB152285BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK285

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042423\
Data File : BN025119.D
Acq On : 24 Apr 2023 18:30
Operator : CG/JU
Sample : PB152285BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK285

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------