

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042423\
 Data File : BN025120.D
 Acq On : 24 Apr 2023 19:06
 Operator : CG/JU
 Sample : PB152288BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK288

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Title : SVOA CALIBRATION

Signal : TIC: BN025120.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.793	99	103	118	rBV2	26986	97573	34.07%	3.405%
2	5.681	423	424	426	rBV2	3673	2836	0.99%	0.099%
3	6.316	530	532	534	rBV3	2719	2725	0.95%	0.095%
4	6.552	570	572	574	rBV3	2953	2821	0.99%	0.098%
5	7.087	657	663	670	rBV	70364	126841	44.29%	4.426%
6	7.252	686	691	704	rVB	59762	113532	39.65%	3.962%
7	7.452	719	725	734	rBV	75988	141603	49.45%	4.941%
8	7.922	797	805	813	rVV	54083	100949	35.25%	3.523%
9	7.981	813	815	818	rVV4	2523	2892	1.01%	0.101%
10	8.034	822	824	826	rVV3	2421	2225	0.78%	0.078%
11	8.099	832	835	836	rBV3	2762	2260	0.79%	0.079%
12	8.234	856	858	860	rBV3	2610	2712	0.95%	0.095%
13	8.328	870	874	875	rVV3	2795	3374	1.18%	0.118%
14	8.363	878	880	882	rBV3	2123	2083	0.73%	0.073%
15	8.475	898	899	903	rBV4	1636	2106	0.74%	0.073%
16	8.634	920	926	936	rBV	75287	146119	51.03%	5.099%
17	8.740	942	944	946	rVB3	2672	2090	0.73%	0.073%
18	8.846	961	962	964	rBV2	2401	2040	0.71%	0.071%
19	8.863	964	965	968	rVB3	4019	2950	1.03%	0.103%
20	8.916	972	974	976	rVB3	3339	2472	0.86%	0.086%
21	8.940	976	978	980	rBV3	2202	2117	0.74%	0.074%
22	9.087	997	1003	1010	rBV2	59054	108814	38.00%	3.797%
23	9.187	1019	1020	1022	rBV2	2631	2019	0.71%	0.070%
24	9.240	1025	1029	1031	rVV5	1329	2182	0.76%	0.076%
25	9.293	1036	1038	1040	rVV3	2141	2356	0.82%	0.082%
26	9.340	1044	1046	1049	rBV4	1873	2398	0.84%	0.084%
27	9.422	1057	1060	1062	rBV4	2955	4168	1.46%	0.145%
28	9.810	1121	1126	1135	rBV2	37130	74780	26.11%	2.609%
29	9.940	1145	1148	1150	rBV4	3079	2675	0.93%	0.093%
30	10.005	1157	1159	1163	rVB5	3439	3690	1.29%	0.129%
31	10.046	1163	1166	1169	rVV5	2594	3066	1.07%	0.107%
32	10.216	1192	1195	1198	rVB5	1919	2426	0.85%	0.085%
33	10.252	1198	1201	1204	rBV5	1236	1877	0.66%	0.065%
34	10.352	1211	1218	1225	rBV	59827	117502	41.03%	4.100%
35	10.522	1245	1247	1249	rBV3	2283	2134	0.75%	0.074%
36	10.599	1258	1260	1264	rVV5	2129	2947	1.03%	0.103%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042423\
 Data File : BN025120.D
 Acq On : 24 Apr 2023 19:06
 Operator : CG/JU
 Sample : PB152288BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK288

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Title : SVOA CALIBRATION

37	10.640	1264	1267	1269	rVB4	2850	3540	1.24%	0.124%
38	10.663	1269	1271	1272	rBV	2116	1758	0.61%	0.061%
39	10.728	1276	1282	1290	rVB	66391	114380	39.94%	3.991%
40	10.875	1300	1307	1323	rVV2	64536	138352	48.31%	4.828%
41	11.169	1352	1357	1358	rVB4	2371	3208	1.12%	0.112%
42	11.193	1358	1361	1363	rBV4	1915	2189	0.76%	0.076%
43	11.357	1386	1389	1391	rBV4	1444	1888	0.66%	0.066%
44	11.463	1405	1407	1410	rVB4	1722	1866	0.65%	0.065%
45	11.569	1422	1425	1428	rBV4	2711	3206	1.12%	0.112%
46	11.599	1428	1430	1433	rVB4	2565	2123	0.74%	0.074%
47	11.834	1467	1470	1473	rVB5	3019	3675	1.28%	0.128%
48	11.881	1473	1478	1479	rBV5	2883	4059	1.42%	0.142%
49	11.899	1479	1481	1482	rBV2	2187	1978	0.69%	0.069%
50	11.975	1490	1494	1495	rVV4	3161	3655	1.28%	0.128%
51	12.099	1512	1515	1518	rVB4	2202	1917	0.67%	0.067%
52	12.157	1523	1525	1526	rVV2	2783	2130	0.74%	0.074%
53	12.175	1526	1528	1530	rVB3	2346	2193	0.77%	0.077%
54	12.269	1541	1544	1545	rBV3	1890	1792	0.63%	0.063%
55	12.287	1545	1547	1550	rVV4	2216	1911	0.67%	0.067%
56	12.316	1550	1552	1554	rVV2	2585	2330	0.81%	0.081%
57	12.334	1554	1555	1558	rVB3	2780	1886	0.66%	0.066%
58	12.387	1561	1564	1566	rVB3	1818	1886	0.66%	0.066%
59	12.416	1566	1569	1570	rBV3	2120	2387	0.83%	0.083%
60	12.499	1582	1583	1589	rVB4	1634	2145	0.75%	0.075%
61	12.546	1589	1591	1594	rBV4	2280	2847	0.99%	0.099%
62	12.587	1596	1598	1599	rVB2	2947	1805	0.63%	0.063%
63	12.610	1599	1602	1605	rBV5	2525	3685	1.29%	0.129%
64	12.763	1627	1628	1630	rBV2	2257	1781	0.62%	0.062%
65	12.910	1649	1653	1659	rVB8	4194	8035	2.81%	0.280%
66	13.004	1666	1669	1670	rBV3	2767	1912	0.67%	0.067%
67	13.098	1682	1685	1688	rBV5	1701	2515	0.88%	0.088%
68	13.175	1696	1698	1700	rVB2	2459	1820	0.64%	0.064%
69	13.263	1712	1713	1716	rBV3	2693	2840	0.99%	0.099%
70	13.334	1722	1725	1728	rVB5	2148	2167	0.76%	0.076%
71	13.469	1746	1748	1751	rVB4	1800	2071	0.72%	0.072%
72	13.504	1751	1754	1757	rBV5	2034	3327	1.16%	0.116%
73	13.546	1759	1761	1764	rVB3	1905	2169	0.76%	0.076%
74	13.569	1764	1765	1768	rBV2	3056	2188	0.76%	0.076%
75	13.746	1792	1795	1799	rBV6	1936	2291	0.80%	0.080%
76	13.828	1805	1809	1811	rVV4	2757	3113	1.09%	0.109%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042423\
 Data File : BN025120.D
 Acq On : 24 Apr 2023 19:06
 Operator : CG/JU
 Sample : PB152288BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK288

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Title : SVOA CALIBRATION

77	13.863	1813	1815	1818	rBV4	1942	2148	0.75%	0.075%
78	13.969	1828	1833	1839	rBV	112683	158812	55.46%	5.542%
79	14.257	1876	1882	1892	rVB2	109200	171240	59.80%	5.975%
80	14.340	1894	1896	1897	rVB2	3452	2050	0.72%	0.072%
81	14.416	1908	1909	1911	rBV2	2120	1955	0.68%	0.068%
82	14.563	1928	1934	1940	rBV	79268	123425	43.10%	4.307%
83	14.681	1952	1954	1958	rBV5	2841	3428	1.20%	0.120%
84	14.793	1967	1973	1976	rBV8	9886	20840	7.28%	0.727%
85	14.945	1995	1999	2002	rBV6	1990	2636	0.92%	0.092%
86	15.334	2063	2065	2070	rVB6	3299	3885	1.36%	0.136%
87	15.551	2096	2102	2111	rVB	156591	236777	82.68%	8.262%
88	15.675	2119	2123	2131	rVB9	12999	21621	7.55%	0.754%
89	15.787	2139	2142	2145	rVB5	4007	5009	1.75%	0.175%
90	15.957	2167	2171	2173	rBV4	3943	4072	1.42%	0.142%
91	16.110	2195	2197	2200	rVB3	3952	3894	1.36%	0.136%
92	16.151	2200	2204	2205	rBV4	2086	3165	1.11%	0.110%
93	16.251	2220	2221	2223	rBV	2556	2072	0.72%	0.072%
94	16.775	2306	2310	2313	rBV5	5108	5840	2.04%	0.204%
95	16.845	2319	2322	2323	rBV3	3328	3674	1.28%	0.128%
96	16.863	2323	2325	2327	rVV3	3591	3030	1.06%	0.106%
97	16.898	2329	2331	2335	rVB2	2466	2985	1.04%	0.104%
98	17.310	2396	2401	2407	rVB	86202	121346	42.37%	4.234%
99	17.410	2412	2418	2428	rBV2	138798	227095	79.30%	7.924%
100	19.704	2803	2808	2812	rBV	213717	286365	100.00%	9.993%




Sum of corrected areas: 2865738

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042423\
Data File : BN025120.D
Acq On : 24 Apr 2023 19:06
Operator : CG/JU
Sample : PB152288BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK288

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

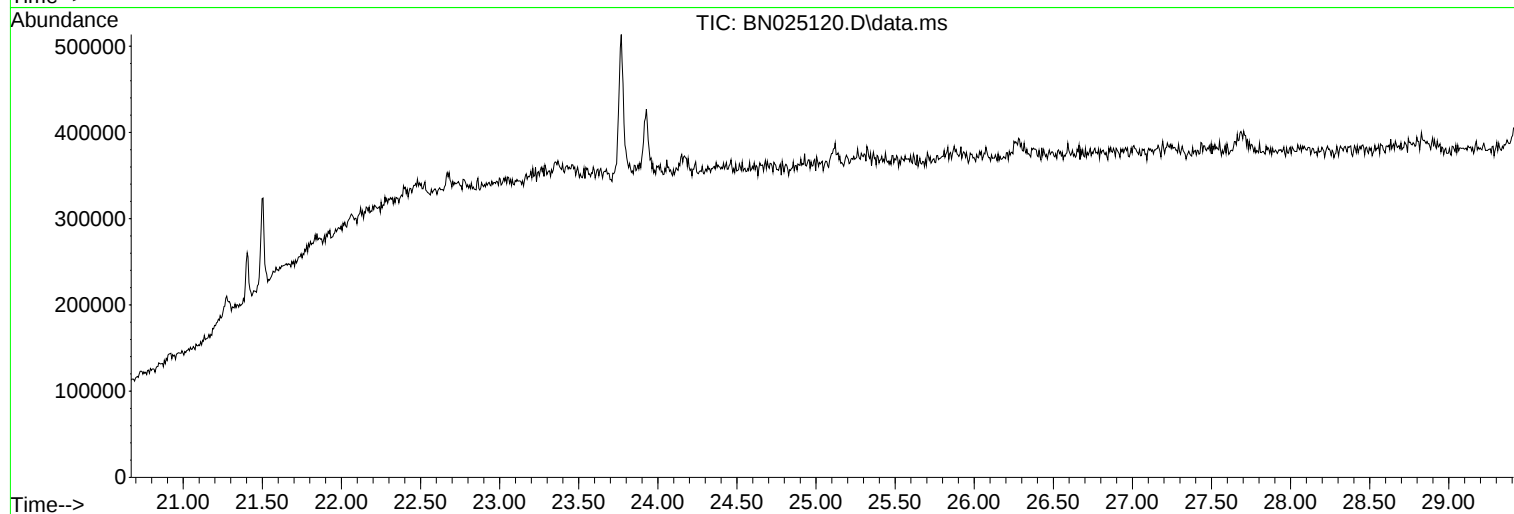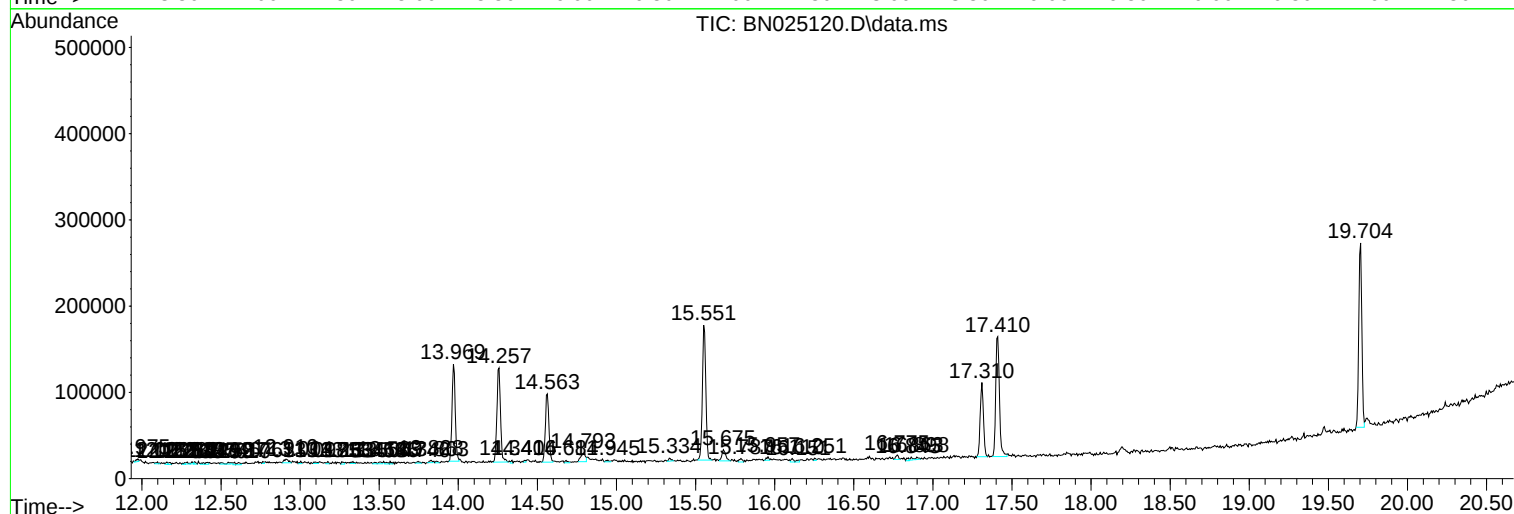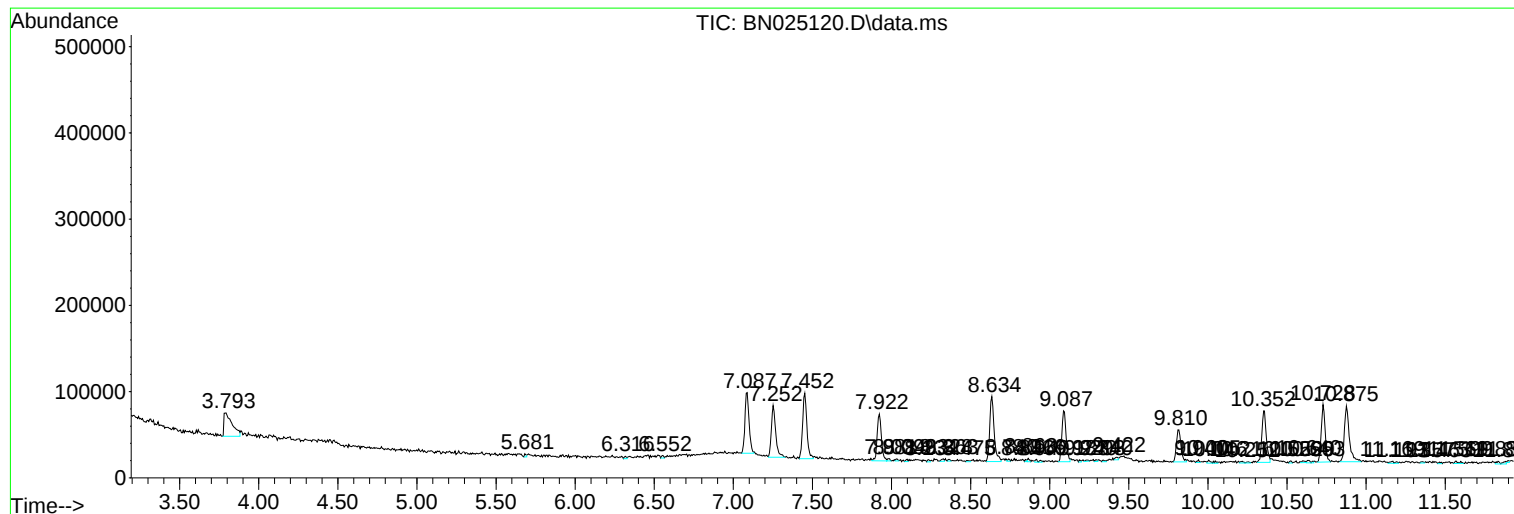

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042423\
Data File : BN025120.D
Acq On : 24 Apr 2023 19:06
Operator : CG/JU
Sample : PB152288BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK288

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042423\
Data File : BN025120.D
Acq On : 24 Apr 2023 19:06
Operator : CG/JU
Sample : PB152288BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK288

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------