

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042621\
 Data File : BN014438.D
 Acq On : 26 Apr 2021 11:25
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Quant Time: Apr 26 12:30:28 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN042221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 26 12:30:05 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.676	152	6394	0.40	ng	0.00
7) Naphthalene-d8	10.454	136	22248	0.40	ng	0.00
13) Acenaphthene-d10	14.308	164	10736	0.40	ng	0.00
19) Phenanthrene-d10	17.055	188	24370	0.40	ng	# 0.00
29) Chrysene-d12	21.261	240	25113	0.40	ng	# 0.00
36) Perylene-d12	23.482	264	21267	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.284	112	5030	0.38	ng	0.00
5) Phenol-d6	6.847	99	6715	0.42	ng	0.00
8) Nitrobenzene-d5	8.819	82	4312	0.23	ng	0.00
11) 2-Methylnaphthalene-d10	12.044	152	12393	0.37	ng	0.00
14) 2,4,6-Tribromophenol	15.805	330	1258	0.36	ng	0.00
15) 2-Fluorobiphenyl	12.925	172	17589	0.41	ng	0.00
27) Fluoranthene-d10	19.099	212	25291	0.39	ng	0.00
31) Terphenyl-d14	19.700	244	18314	0.34	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.247	88	3415	0.44	ng	# 95
3) n-Nitrosodimethylamine	3.585	42	1799	0.50	ng	# 73
6) bis(2-Chloroethyl)ether	7.104	93	6579	0.42	ng	98
9) Naphthalene	10.505	128	22673	0.41	ng	99
10) Hexachlorobutadiene	10.796	225	4821	0.40	ng	# 100
12) 2-Methylnaphthalene	12.120	142	13922	0.39	ng	99
16) Acenaphthylene	14.029	152	16495	0.36	ng	100
17) Acenaphthene	14.372	154	11765	0.39	ng	93
18) Fluorene	15.361	166	15760	0.42	ng	99
20) 4,6-Dinitro-2-methylph...	15.437	198	681	0.25	ng	# 1
21) 4-Bromophenyl-phenylether	16.252	248	4880	0.36	ng	# 88
22) Hexachlorobenzene	16.374	284	7626	0.40	ng	97
23) Atrazine	16.520	200	1798	0.23	ng	# 93
24) Pentachlorophenol	16.715	266	1280	0.37	ng	99
25) Phenanthrene	17.104	178	26536	0.39	ng	100
26) Anthracene	17.189	178	18998	0.35	ng	100
28) Fluoranthene	19.129	202	29387	0.40	ng	99
30) Pyrene	19.491	202	27349	0.37	ng	100
32) Benzo(a)anthracene	21.239	228	25376	0.38	ng	98
33) Chrysene	21.293	228	29027	0.37	ng	98
34) Bis(2-ethylhexyl)phtha...	21.186	149	20923	0.89	ng	97
35) Indeno(1,2,3-cd)pyrene	25.718	276	29445	0.34	ng	99
37) Benzo(b)fluoranthene	22.859	252	30747	0.39	ng	99
38) Benzo(k)fluoranthene	22.859	252	30932	0.39	ng	99
39) Benzo(a)pyrene	23.387	252	25243	0.38	ng	# 93
40) Dibenzo(a,h)anthracene	25.731	278	23514	0.32	ng	98
41) Benzo(g,h,i)perylene	26.395	276	25210	0.32	ng	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042621\
 Data File : BN014438.D
 Acq On : 26 Apr 2021 11:25
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4


Quant Time: Apr 26 12:30:28 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN042221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 26 12:30:05 2021
 Response via : Initial Calibration

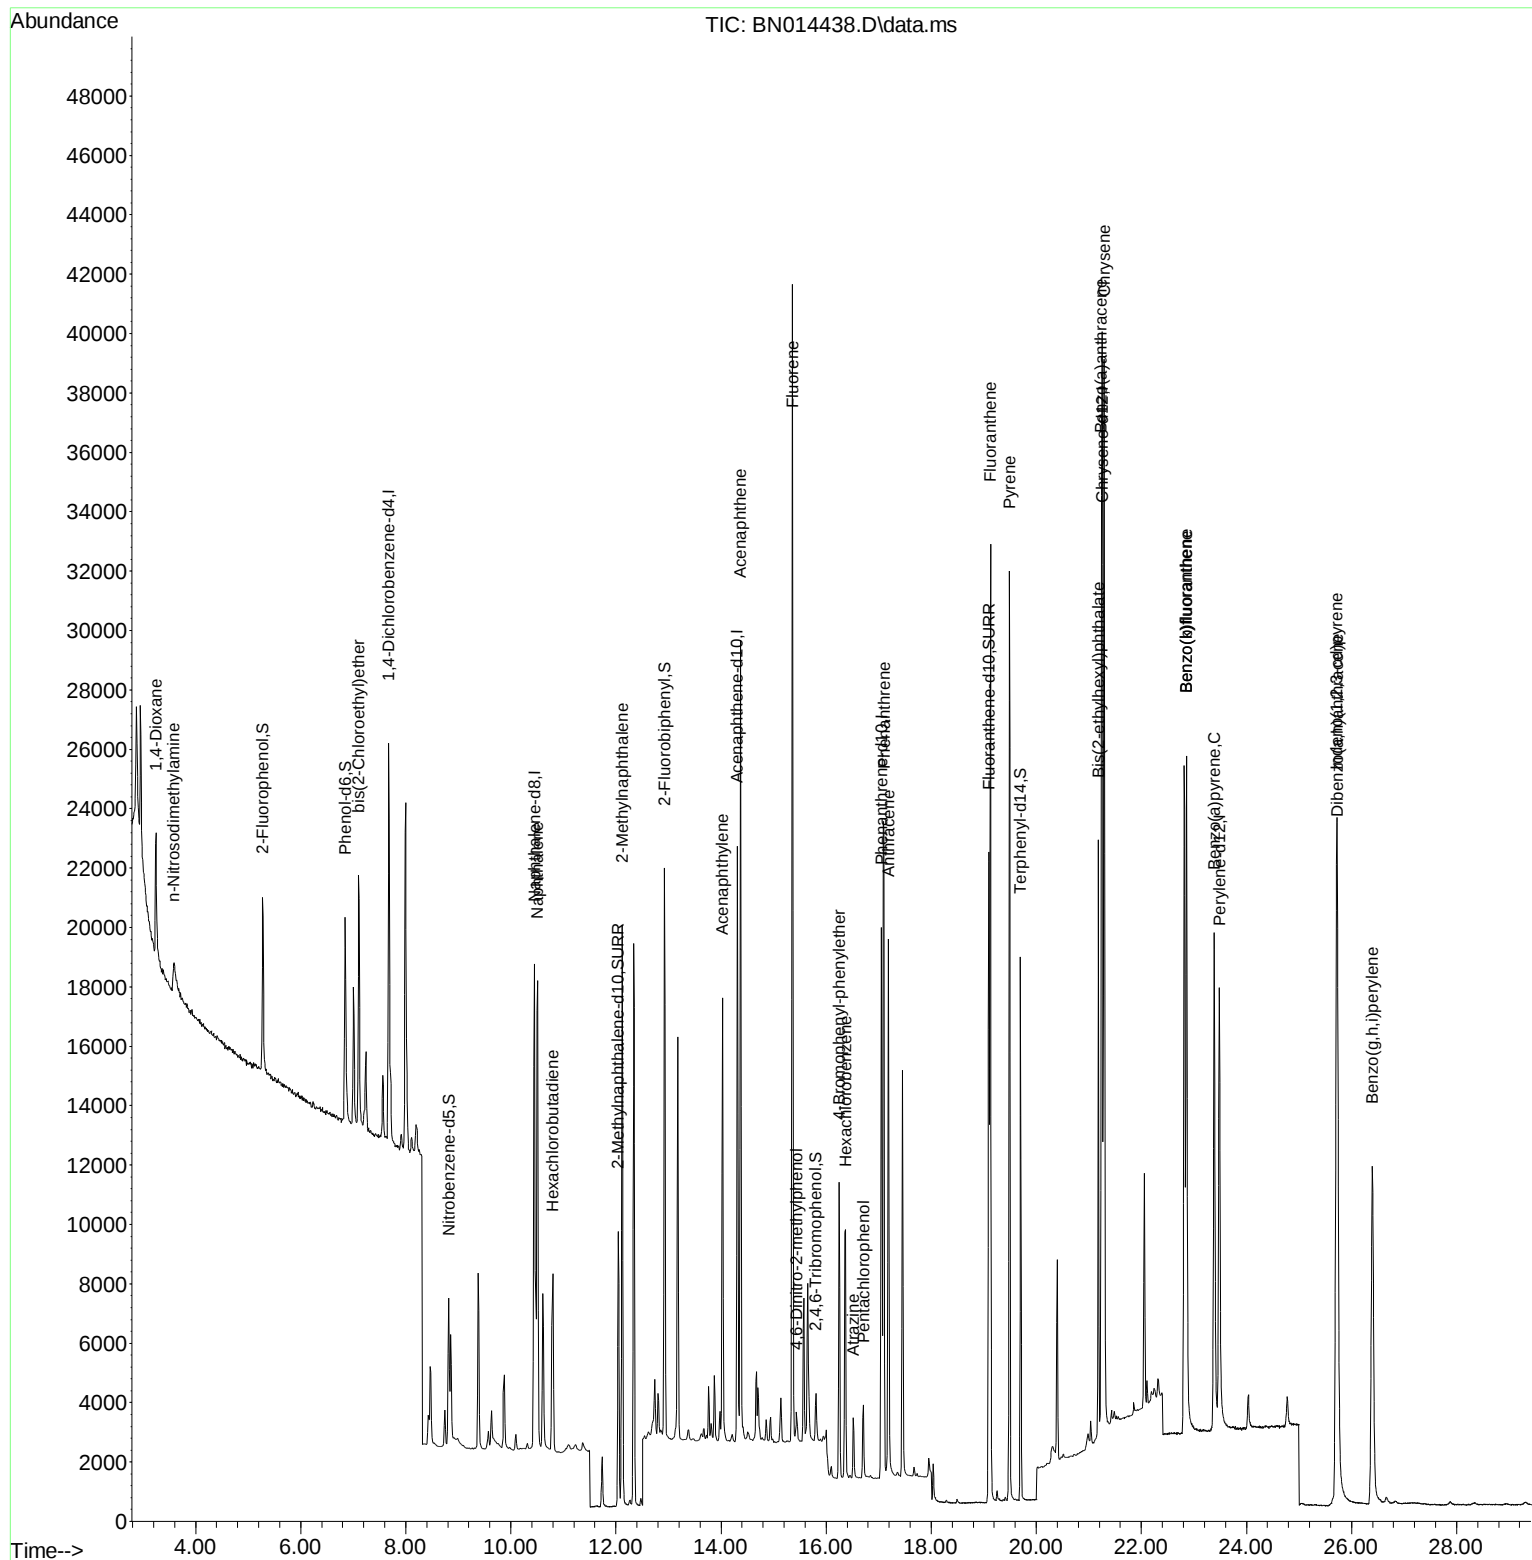



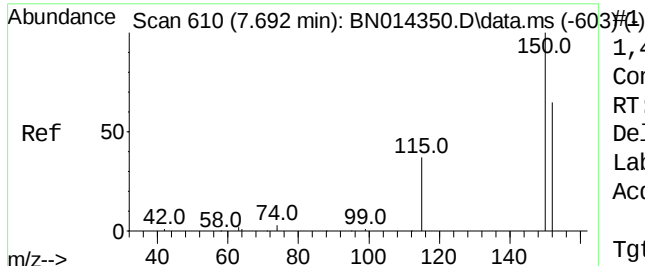


1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.676 min Scan# 608
 Delta R.T. 0.000 min
 Lab File: BN014438.D
 Acq: 26 Apr 2021 11:25


Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

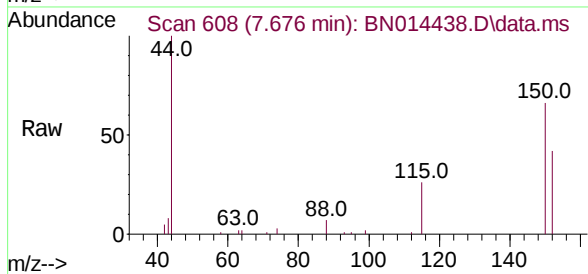



Tgt Ion:152 Resp: 6394
 Ion Ratio Lower Upper
 152 100
 150 157.0 123.4 185.2
 115 61.4 47.5 71.3

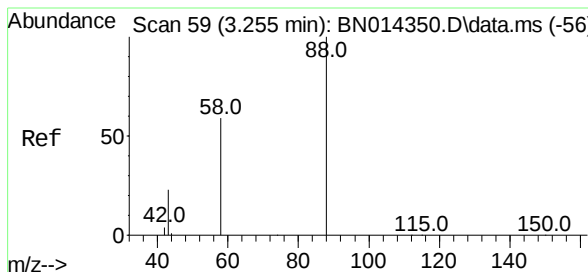


1,4-Dioxane
 Concen: 0.44 ng
 RT: 3.247 min Scan# 58
 Delta R.T. 0.000 min
 Lab File: BN014438.D
 Acq: 26 Apr 2021 11:25



Tgt Ion: 88 Resp: 3415
 Ion Ratio Lower Upper
 88 100
 58 67.2 52.2 78.2
 43 31.0 20.6 30.8#







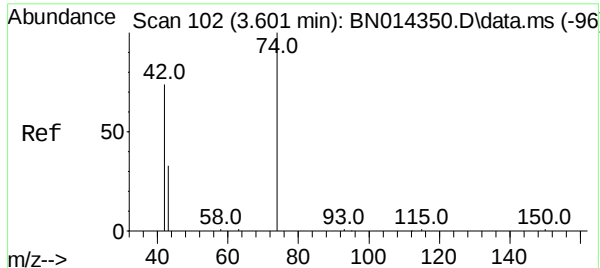

n-Nitrosodimethylamine
 Concen: 0.50 ng
 RT: 3.585 min Scan# 100
 Delta R.T. 0.000 min
 Lab File: BN014438.D
 Acq: 26 Apr 2021 11:25




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4


Tgt Ion: 42 Resp: 1799
 Ion Ratio Lower Upper
 42 100
 74 103.3 108.0 162.0#
 44 0.0 0.0 0.0

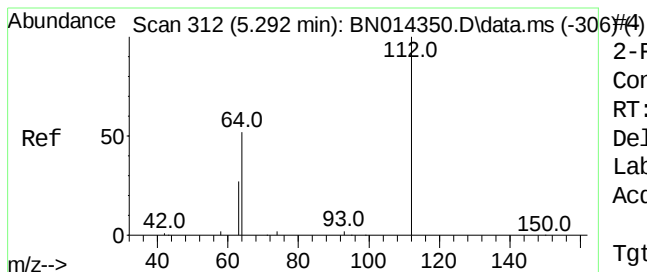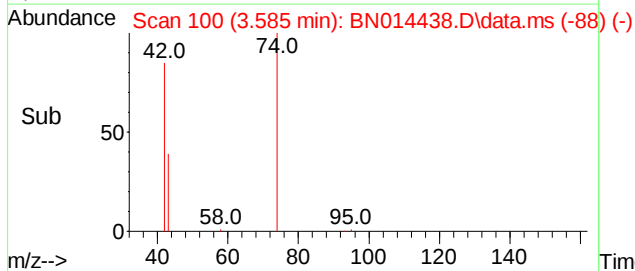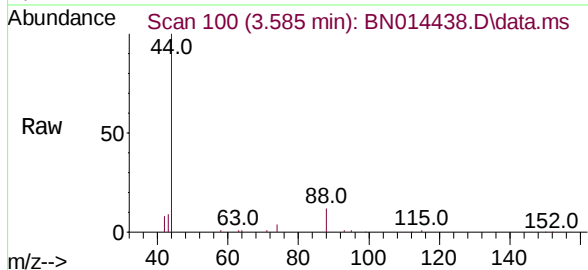

2-Fluorophenol
 Concen: 0.38 ng
 RT: 5.284 min Scan# 311
 Delta R.T. 0.000 min
 Lab File: BN014438.D
 Acq: 26 Apr 2021 11:25

Tgt Ion: 112 Resp: 5030
 Ion Ratio Lower Upper
 112 100
 64 55.7 43.0 64.6
 63 30.8 23.4 35.0


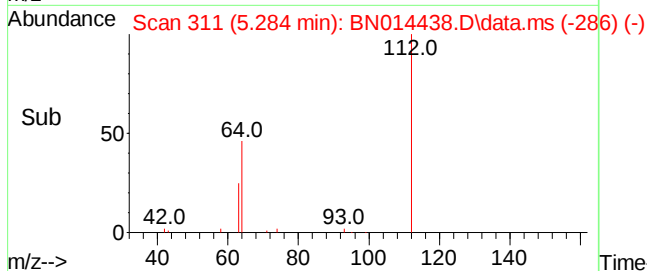




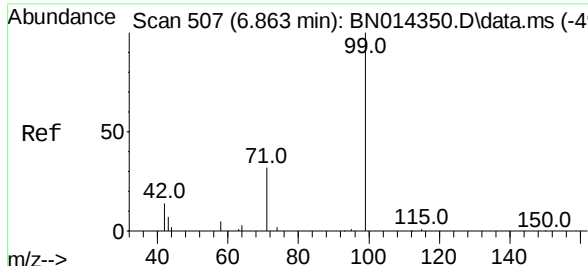

Phenol-d6
 Concen: 0.42 ng
 RT: 6.847 min Scan# 505
 Delta R.T. 0.000 min
 Lab File: BN014438.D
 Acq: 26 Apr 2021 11:25




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Tgt Ion:	99	Resp:	6715
Ion	Ratio	Lower	Upper
99	100		
42	21.3	16.0	24.0
71	34.2	27.8	41.8

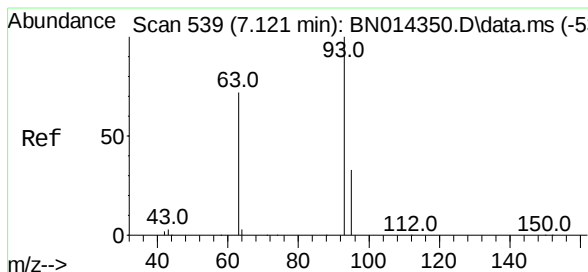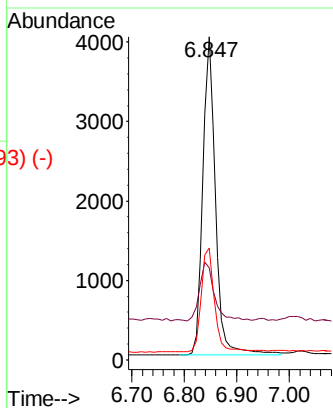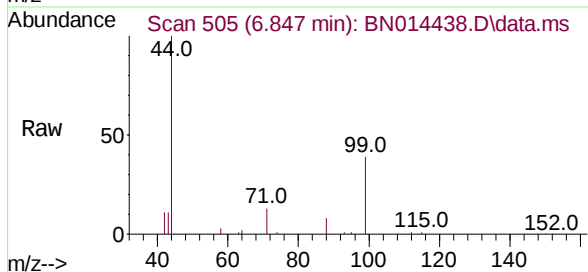


bis(2-Chloroethyl)ether
 Concen: 0.42 ng
 RT: 7.104 min Scan# 537
 Delta R.T. 0.000 min
 Lab File: BN014438.D
 Acq: 26 Apr 2021 11:25

Tgt Ion:	93	Resp:	6579
Ion	Ratio	Lower	Upper
93	100		
63	76.0	59.4	89.2
95	32.8	27.0	40.4






Abundance Scan 857 (10.467 min): BN014350.D\data.ms (-857) (-)

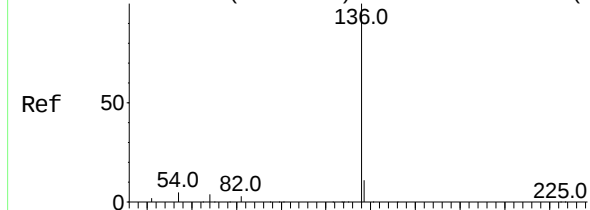


Naphthalene-d8
Concen: 0.40 ng
RT: 10.454 min Scan# 856
Delta R.T. 0.000 min
Lab File: BN014438.D
Acq: 26 Apr 2021 11:25

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:	136	Resp:	22248
Ion	Ratio	Lower	Upper
136	100		
137	11.3	9.0	13.6
54	5.7	4.4	6.6
68	5.5	3.9	5.9

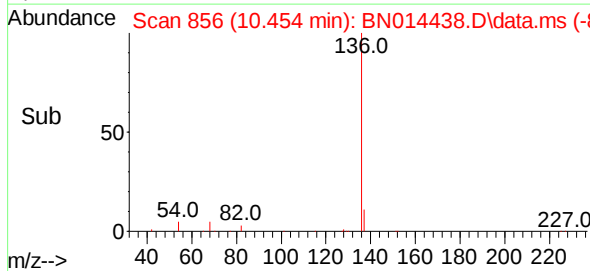
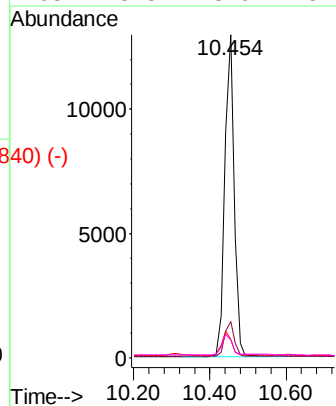
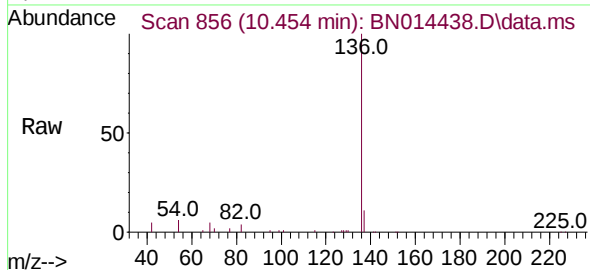


Abundance Scan 728 (8.832 min): BN014350.D\data.ms (-725) (-)

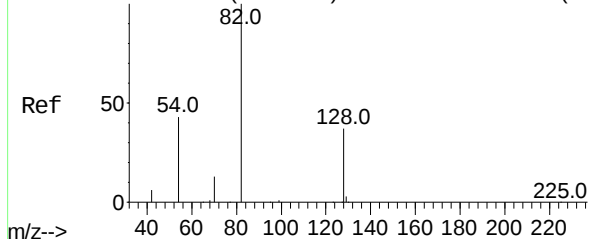


Nitrobenzene-d5
Concen: 0.23 ng
RT: 8.819 min Scan# 727
Delta R.T. 0.000 min
Lab File: BN014438.D
Acq: 26 Apr 2021 11:25

Tgt Ion:	82	Resp:	4312
Ion	Ratio	Lower	Upper
82	100		
128	33.0	30.3	45.5
54	47.5	35.8	53.8

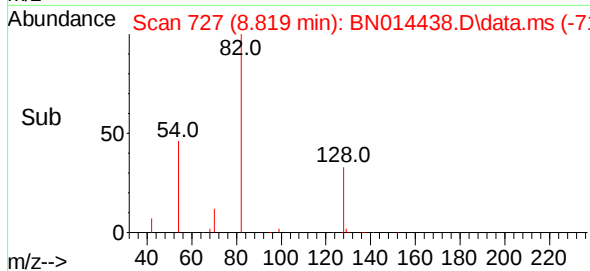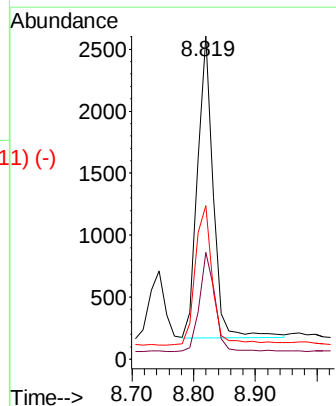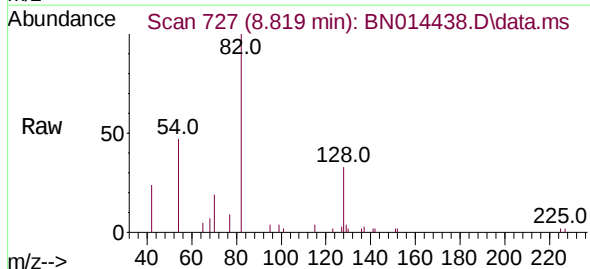




Abundance Scan 861 (10.518 min): BN014350.D\data.ms (-855) (-)




Naphthalene
Concen: 0.41 ng
RT: 10.505 min Scan# 860
Delta R.T. 0.000 min
Lab File: BN014438.D
Acq: 26 Apr 2021 11:25

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:	128	Resp:	22673
Ion	Ratio	Lower	Upper
128	100		
129	11.0	9.0	13.6
127	12.7	10.3	15.5


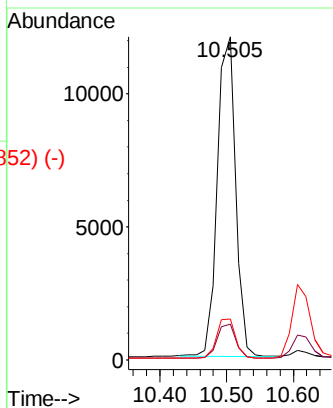
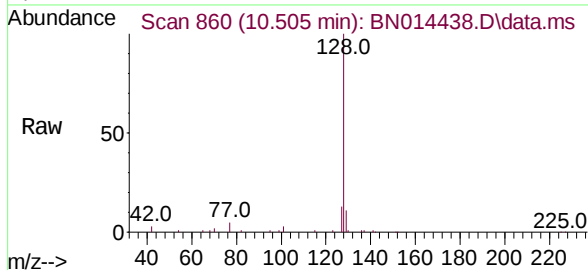


Abundance Scan 884 (10.809 min): BN014350.D\data.ms (-879) (-)




Hexachlorobutadiene
Concen: 0.40 ng
RT: 10.796 min Scan# 883
Delta R.T. 0.000 min
Lab File: BN014438.D
Acq: 26 Apr 2021 11:25

Tgt Ion:	225	Resp:	4821
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	63.3	50.6	75.8



Abundance Scan 1063 (12.058 min): BN014350.D\data.ms (-1051) (-)


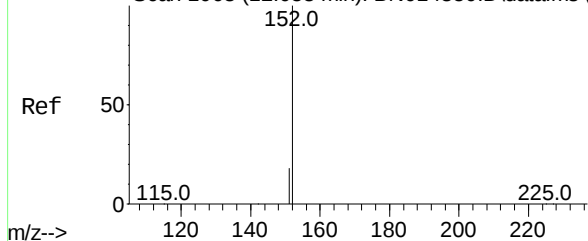


2-Methylnaphthalene-d10
Concen: 0.37 ng
RT: 12.044 min Scan# 1060
Delta R.T. 0.000 min
Lab File: BN014438.D
Acq: 26 Apr 2021 11:25


Tgt Ion:152 Resp: 12393
Ion Ratio Lower Upper
152 100
151 20.9 16.3 24.5

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Abundance Scan 1060 (12.044 min): BN014438.D\data.ms

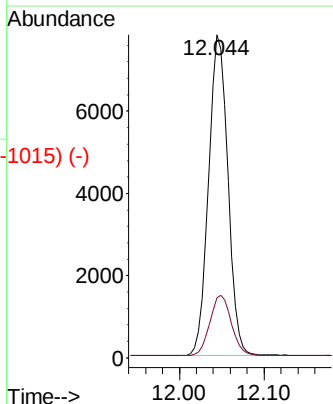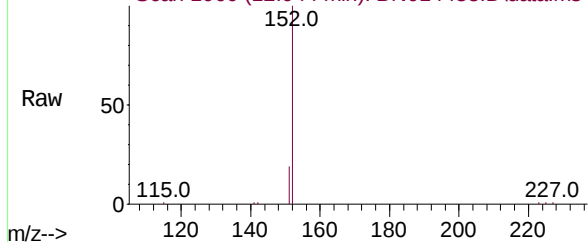

Abundance Scan 1060 (12.044 min): BN014438.D\data.ms (-1015) (-)





Abundance Scan 1080 (12.133 min): BN014350.D\data.ms (-1071) (-)

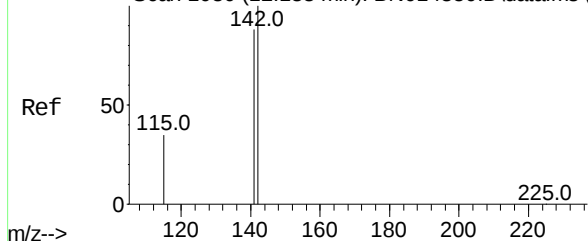


2-Methylnaphthalene
Concen: 0.39 ng
RT: 12.120 min Scan# 1077
Delta R.T. 0.000 min
Lab File: BN014438.D
Acq: 26 Apr 2021 11:25

Tgt Ion:142 Resp: 13922
Ion Ratio Lower Upper
142 100
141 89.1 70.6 105.8
115 36.7 29.0 43.6

Abundance Scan 1077 (12.120 min): BN014438.D\data.ms

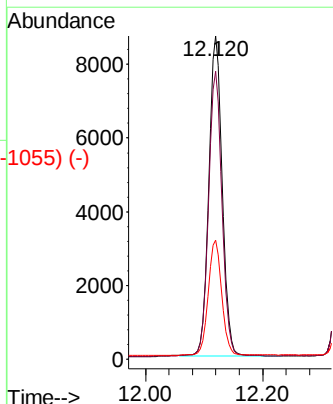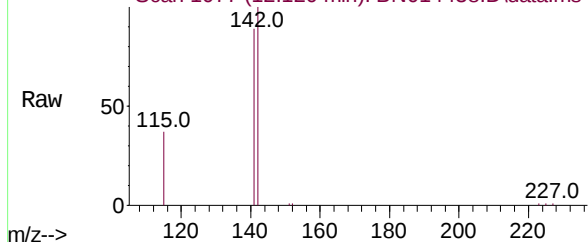


Abundance Scan 1077 (12.120 min): BN014438.D\data.ms (-1055) (-)






Abundance Scan 1307 (14.321 min): BN014350.D\data.ms (-1299) (-)

Acenaphthene-d10
Concen: 0.40 ng
RT: 14.308 min Scan# 1306
Delta R.T. 0.000 min
Lab File: BN014438.D
Acq: 26 Apr 2021 11:25

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

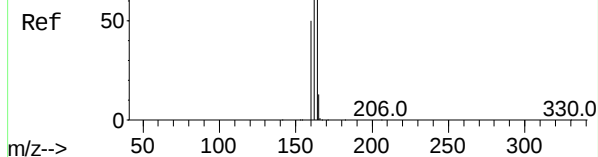


Tgt Ion:	164	Resp:	10736
Ion Ratio	Lower	Upper	
164	100		
162	102.1	81.0	121.6
160	60.7	40.7	61.1

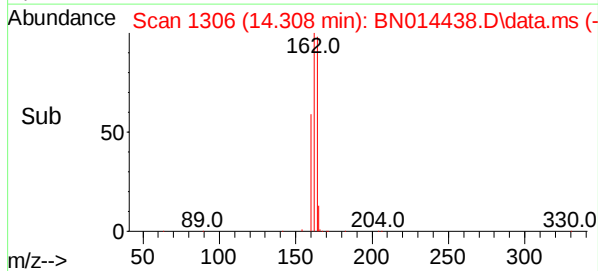
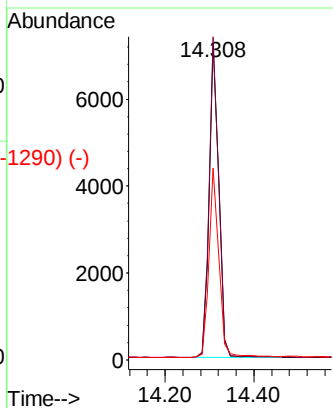
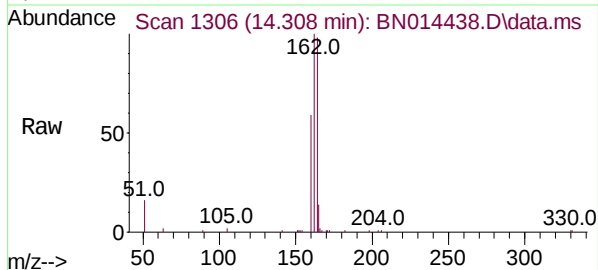


Abundance Scan 1425 (15.818 min): BN014350.D\data.ms (-1416) (-)


2,4,6-Tribromophenol
Concen: 0.36 ng
RT: 15.805 min Scan# 1424
Delta R.T. 0.000 min
Lab File: BN014438.D
Acq: 26 Apr 2021 11:25

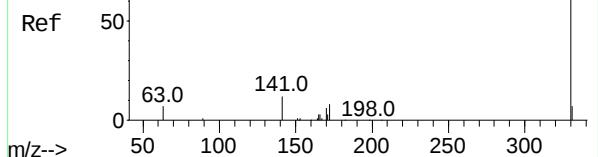

Tgt Ion:	330	Resp:	1258
Ion Ratio	Lower	Upper	
330	100		
332	0.0	0.0	0.0
141	36.9	26.2	39.2

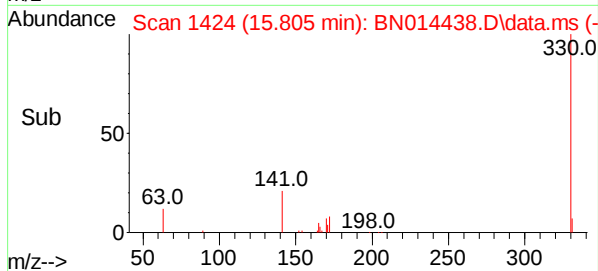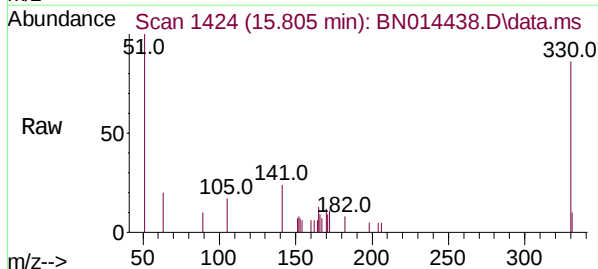




Abundance Scan 1198 (12.938 min): BN014350.D\data.ms (-1198) (-)




2-Fluorobiphenyl
Concen: 0.41 ng
RT: 12.925 min Scan# 1197
Delta R.T. 0.000 min
Lab File: BN014438.D
Acq: 26 Apr 2021 11:25

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:	172	Resp:	17589
Ion	Ratio	Lower	Upper
172	100		
171	35.4	28.2	42.2
170	24.5	19.6	29.4


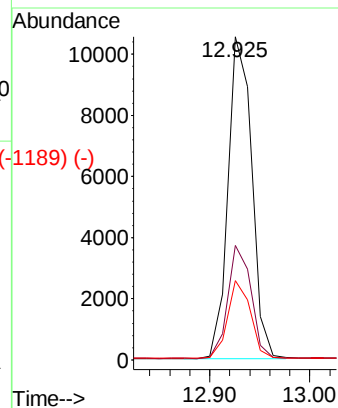
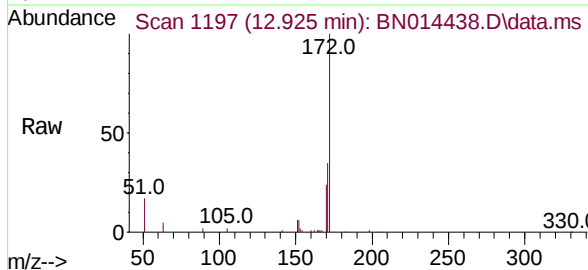


Abundance Scan 1285 (14.042 min): BN014350.D\data.ms (-1216) (-)




Acenaphthylene
Concen: 0.36 ng
RT: 14.029 min Scan# 1284
Delta R.T. 0.000 min
Lab File: BN014438.D
Acq: 26 Apr 2021 11:25

Tgt Ion:	152	Resp:	16495
Ion	Ratio	Lower	Upper
152	100		
151	19.3	15.6	23.4
153	13.2	10.5	15.7

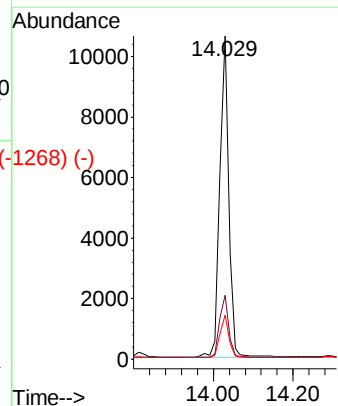




Abundance Scan 1312 (14.384 min): BN014350.D\data.ms (-1303) (-)

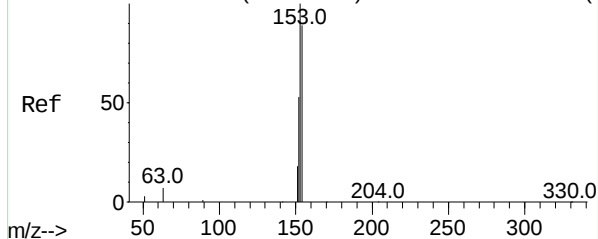


Acenaphthene
Concen: 0.39 ng
RT: 14.372 min Scan# 1311
Delta R.T. 0.000 min
Lab File: BN014438.D
Acq: 26 Apr 2021 11:25

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:	154	Resp:	11765
Ion Ratio	Lower	Upper	
154	100		
153	114.3	89.2	133.8
152	72.1	49.0	73.4

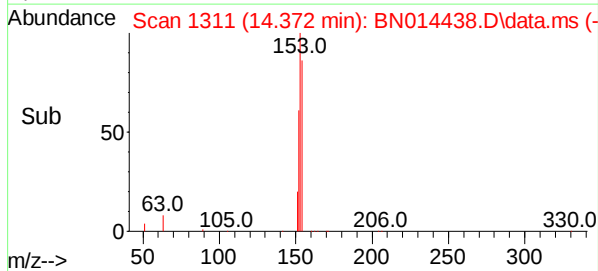
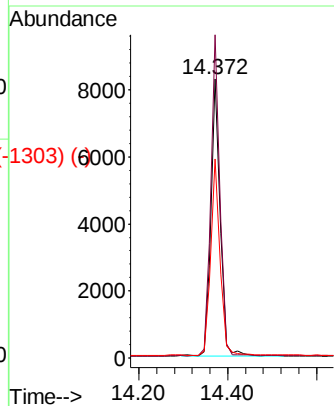
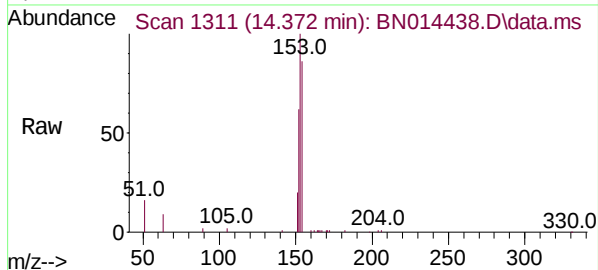


Abundance Scan 1390 (15.374 min): BN014350.D\data.ms (-1315) (-)

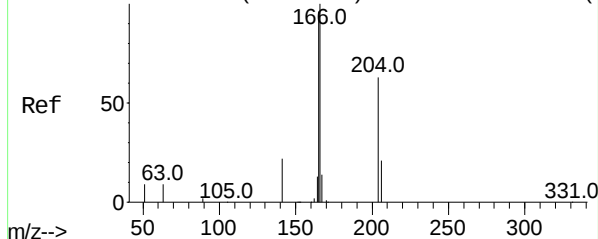

Fluorene
Concen: 0.42 ng
RT: 15.361 min Scan# 1389
Delta R.T. 0.000 min
Lab File: BN014438.D
Acq: 26 Apr 2021 11:25


Tgt Ion:	166	Resp:	15760
Ion Ratio	Lower	Upper	
166	100		
165	98.9	78.6	118.0
167	13.7	10.9	16.3

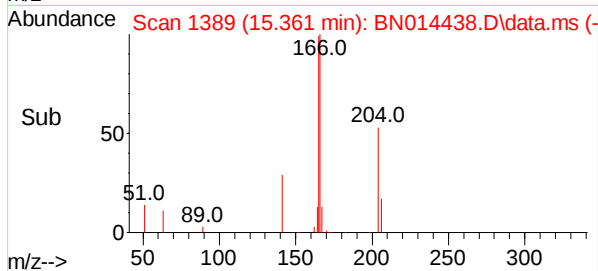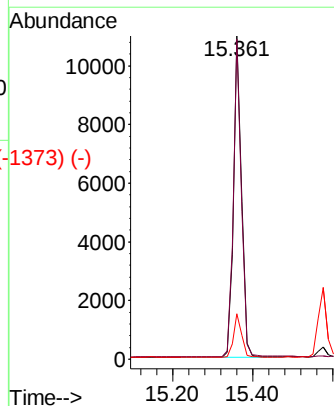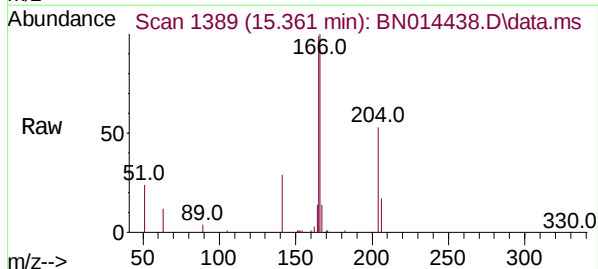




Abundance Scan 1527 (17.067 min): BN014350.D\data.ms (-1519) (-)

Phenanthrene-d10
Concen: 0.40 ng
RT: 17.055 min Scan# 1526
Delta R.T. 0.000 min
Lab File: BN014438.D
Acq: 26 Apr 2021 11:25

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

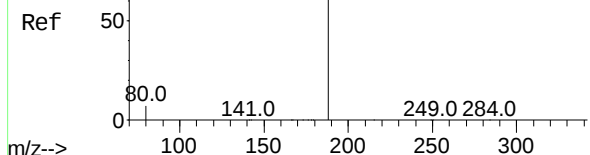


Tgt Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	11.3	6.2	9.4#

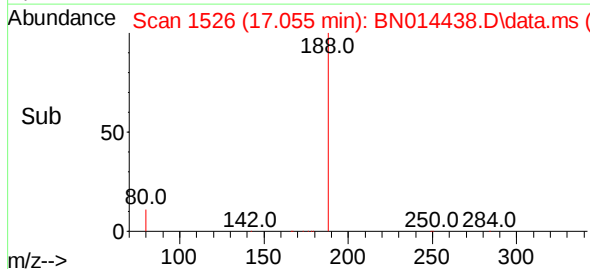
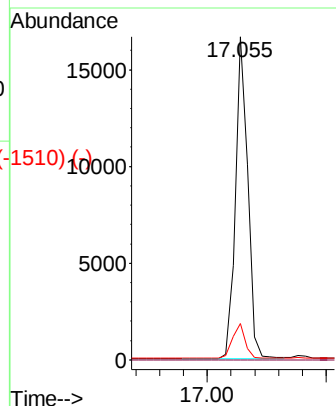
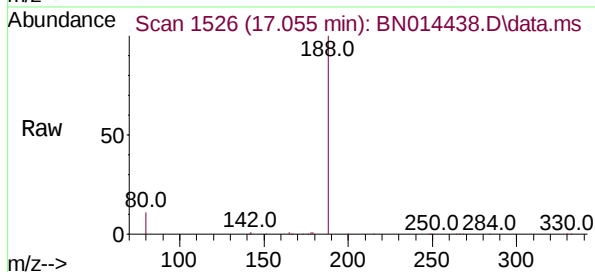


Abundance Scan 1396 (15.450 min): BN014350.D\data.ms (-1320) (-)


4,6-Dinitro-2-methylphenol
Concen: 0.25 ng
RT: 15.437 min Scan# 1395
Delta R.T. 0.000 min
Lab File: BN014438.D
Acq: 26 Apr 2021 11:25

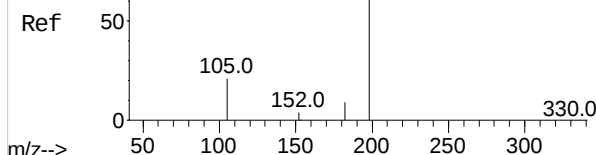

Tgt Ion	Ratio	Lower	Upper
198	100		
51	270.0	60.0	90.0#
105	75.9	31.5	47.3#

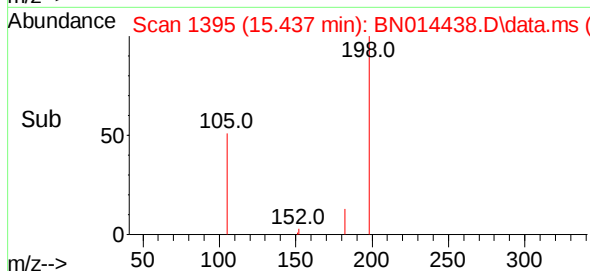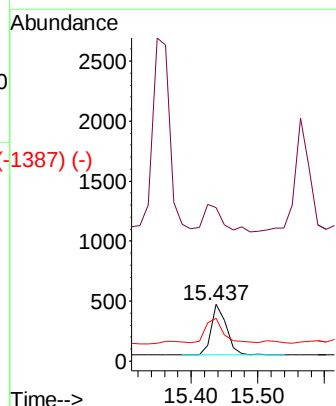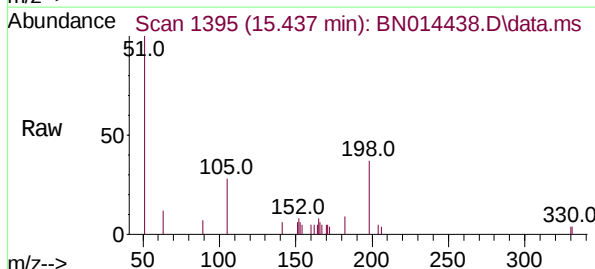




Abundance Scan 1461 (16.264 min): BN014350.D\data.ms (-1427) (-)

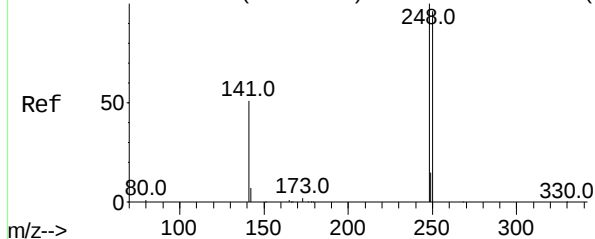


4-Bromophenyl-phenylether
Concen: 0.36 ng
RT: 16.252 min Scan# 1460
Delta R.T. 0.000 min
Lab File: BN014438.D
Acq: 26 Apr 2021 11:25

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:	248	Resp:	4880
Ion Ratio	Lower	Upper	
248	100		
250	92.7	77.4	116.0
141	70.1	41.4	62.0#

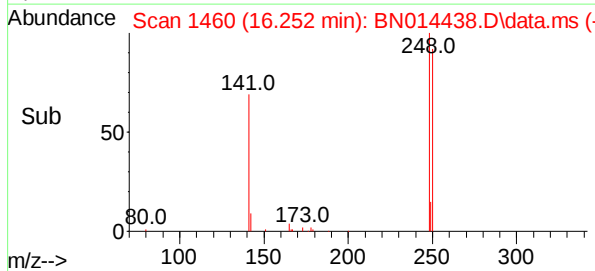
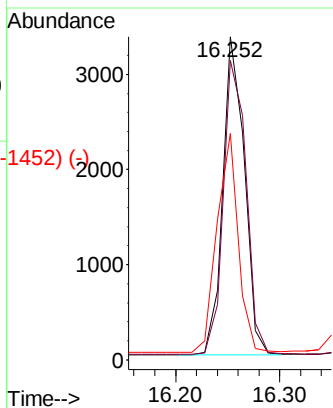
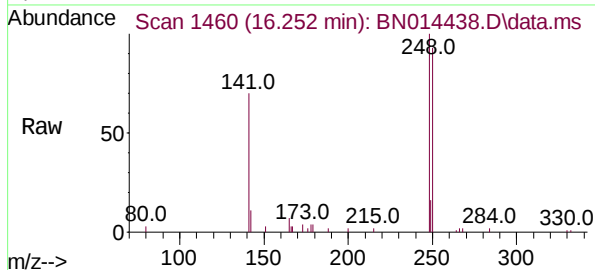


Abundance Scan 1470 (16.373 min): BN014350.D\data.ms (-1429) (-)

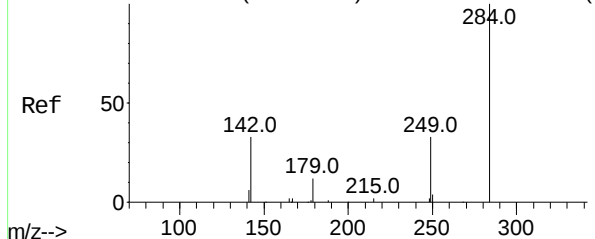

Hexachlorobenzene
Concen: 0.40 ng
RT: 16.374 min Scan# 1470
Delta R.T. 0.000 min
Lab File: BN014438.D
Acq: 26 Apr 2021 11:25


Tgt Ion:	284	Resp:	7626
Ion Ratio	Lower	Upper	
284	100		
142	35.4	26.5	39.7
249	29.5	24.0	36.0

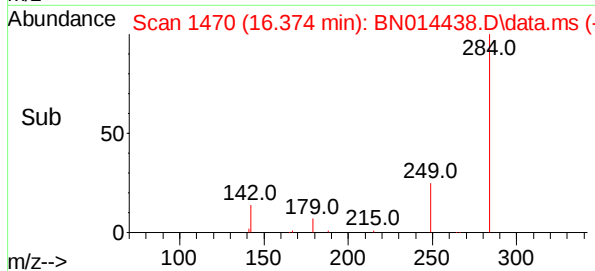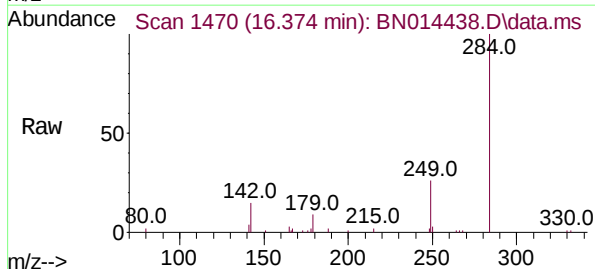



Abundance Scan 1483 (16.532 min): BN014350.D\data.ms (-1429) (-)

Atrazine
Concen: 0.23 ng
RT: 16.520 min Scan# 1482
Delta R.T. 0.000 min
Lab File: BN014438.D
Acq: 26 Apr 2021 11:25


Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

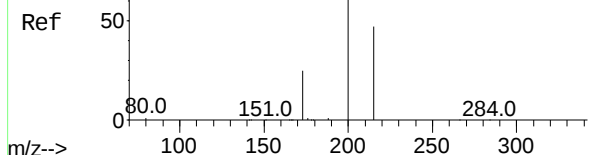

Tgt Ion	Ratio	Lower	Upper
200	100		
173	33.2	21.0	31.6#
215	46.0	38.7	58.1

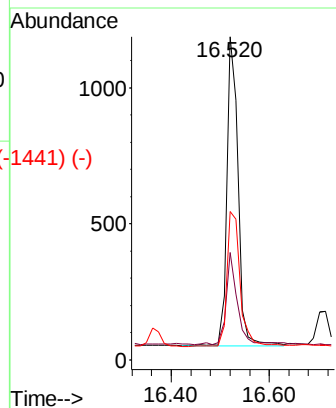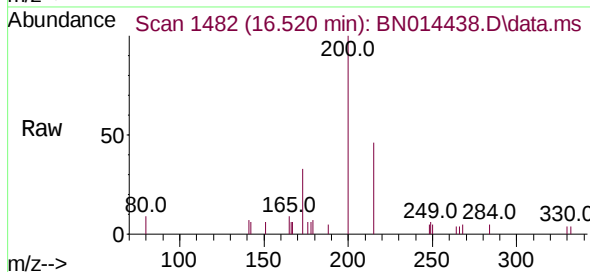


Abundance Scan 1482 (16.520 min): BN014438.D\data.ms (-1441) (-)


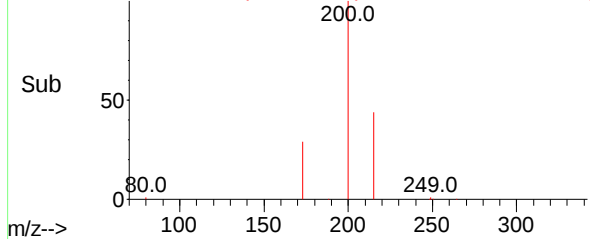


Abundance Scan 1498 (16.714 min): BN014350.D\data.ms (-1424) (-)


Pentachlorophenol
Concen: 0.37 ng
RT: 16.715 min Scan# 1498
Delta R.T. 0.000 min
Lab File: BN014438.D
Acq: 26 Apr 2021 11:25

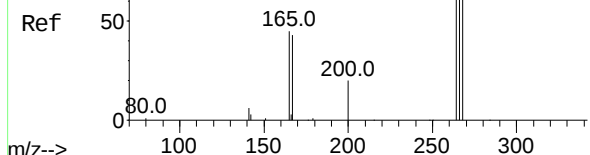

Tgt Ion	Ratio	Lower	Upper
266	100		
264	61.2	50.6	76.0
268	64.1	51.4	77.0

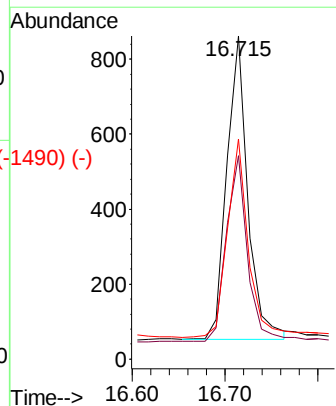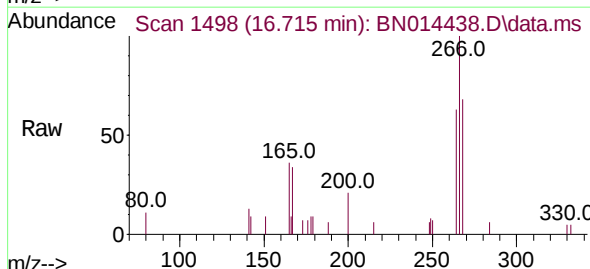


Abundance Scan 1498 (16.715 min): BN014438.D\data.ms (-1490) (-)

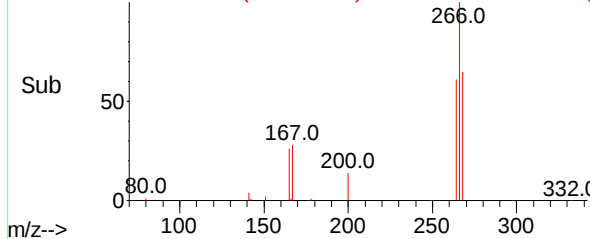




Abundance Scan 1530 (17.104 min): BN014350.D\data.ms (-1525) (-)

Phenanthrene
Concen: 0.39 ng
RT: 17.104 min Scan# 1530
Delta R.T. 0.000 min
Lab File: BN014438.D
Acq: 26 Apr 2021 11:25

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

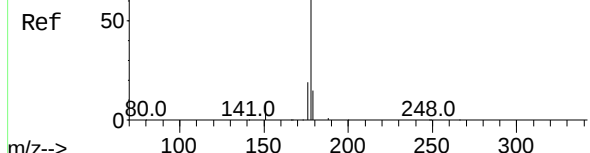


Tgt Ion:	178	Resp:	26536
Ion Ratio	Lower	Upper	
178	100		
176	19.1	15.2	22.8
179	15.4	12.2	18.4

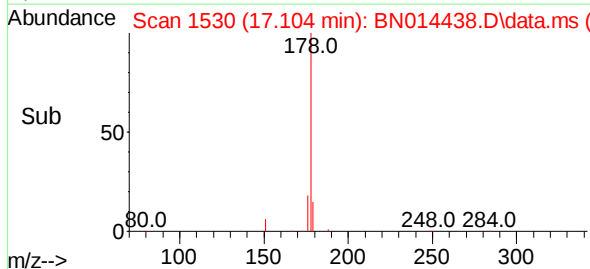

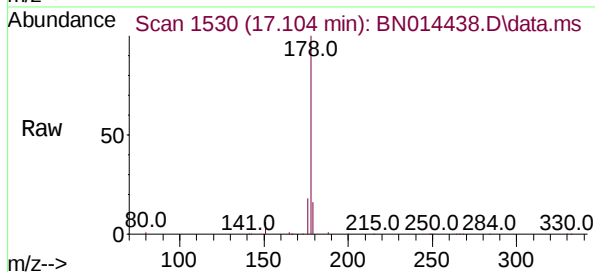


Abundance Scan 1538 (17.201 min): BN014350.D\data.ms (-1526) (-)


Anthracene
Concen: 0.35 ng
RT: 17.189 min Scan# 1537
Delta R.T. 0.000 min
Lab File: BN014438.D
Acq: 26 Apr 2021 11:25

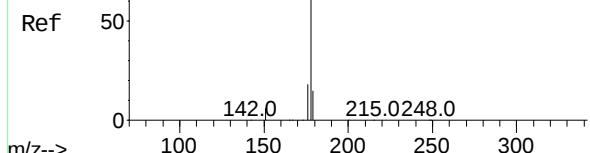

Tgt Ion:	178	Resp:	18998
Ion Ratio	Lower	Upper	
178	100		
176	18.5	15.0	22.4
179	15.3	12.2	18.2

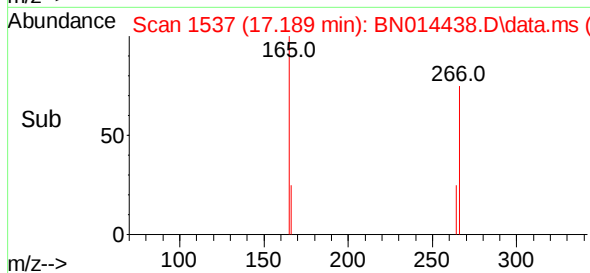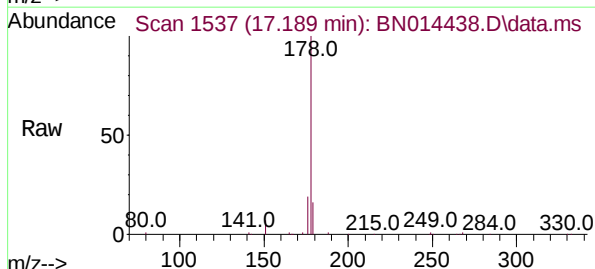




Abundance Scan 1825 (19.101 min): BN014350.D\data.ms (-1827) (-)




Fluoranthene-d10
Concen: 0.39 ng
RT: 19.099 min Scan# 1823
Delta R.T. 0.000 min
Lab File: BN014438.D
Acq: 26 Apr 2021 11:25

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:212 Resp: 25291
Ion Ratio Lower Upper
212 100
106 13.3 9.7 14.5
104 7.6 5.4 8.0



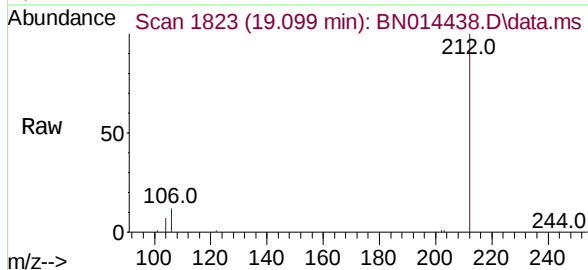


Abundance Scan 1831 (19.131 min): BN014350.D\data.ms (-1823) (-)




Fluoranthene
Concen: 0.40 ng
RT: 19.129 min Scan# 1829
Delta R.T. 0.000 min
Lab File: BN014438.D
Acq: 26 Apr 2021 11:25

Tgt Ion:202 Resp: 29387
Ion Ratio Lower Upper
202 100
101 11.4 8.2 12.4
203 17.2 13.8 20.6






Abundance Scan 2125 (21.258 min): BN014350.D\data.ms (-2125) (-)

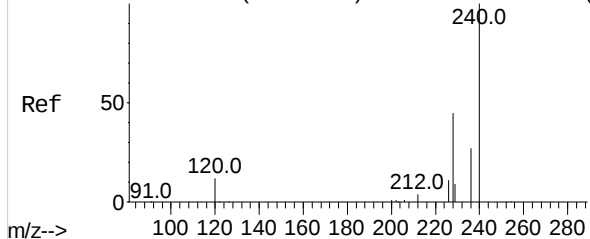


Chrysene-d12
Concen: 0.40 ng
RT: 21.261 min Scan# 2124
Delta R.T. 0.000 min
Lab File: BN014438.D
Acq: 26 Apr 2021 11:25

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:	240	Resp:	25113
Ion	Ratio	Lower	Upper
240	100		
120	7.9	10.7	16.1#
236	26.3	21.5	32.3

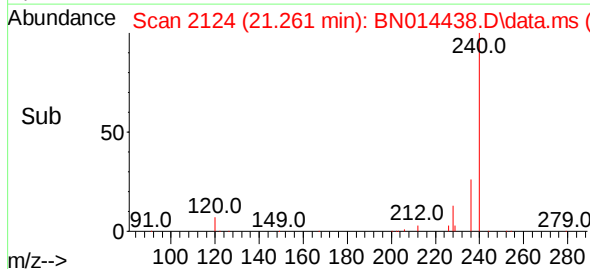
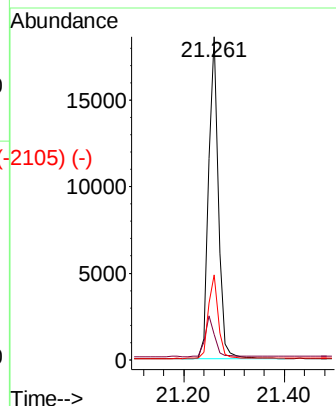
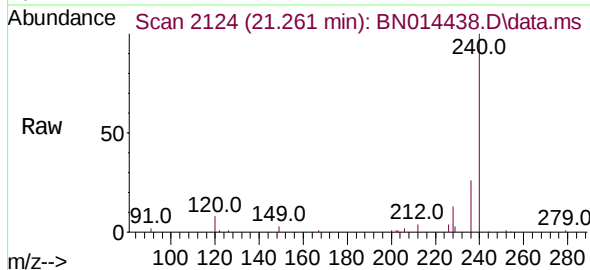


Abundance Scan 1905 (19.498 min): BN014350.D\data.ms (-1905) (-)

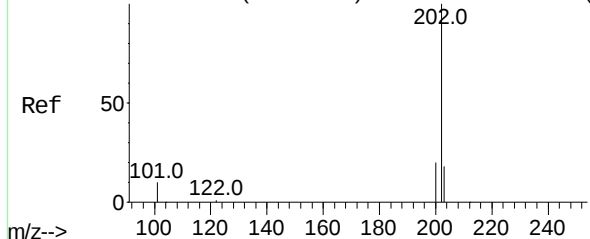

Pyrene
Concen: 0.37 ng
RT: 19.491 min Scan# 1902
Delta R.T. 0.000 min
Lab File: BN014438.D
Acq: 26 Apr 2021 11:25


Tgt Ion:	202	Resp:	27349
Ion	Ratio	Lower	Upper
202	100		
200	20.6	16.6	24.8
203	17.3	14.1	21.1

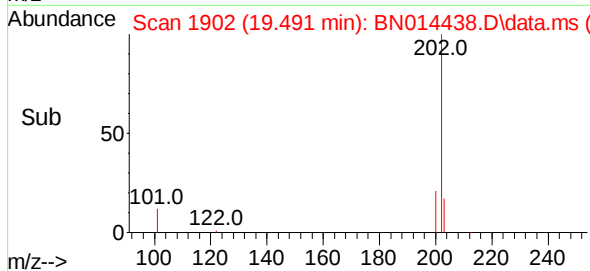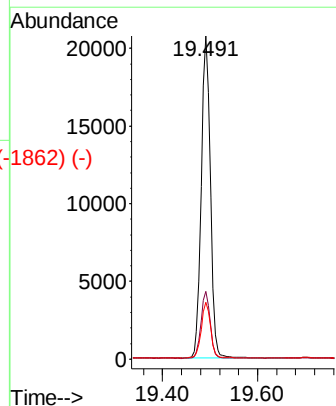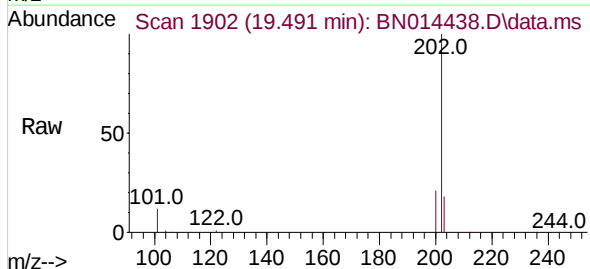



Abundance Scan 1947 (19.707 min): BN014350.D\data.ms (-1934) (-)

Terphenyl-d14
Concen: 0.34 ng
RT: 19.700 min Scan# 1944
Delta R.T. 0.000 min
Lab File: BN014438.D
Acq: 26 Apr 2021 11:25


Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

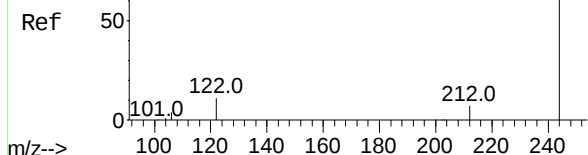

Tgt Ion	Ratio	Lower	Upper
244	100		
212	8.1	6.2	9.4
122	14.0	9.3	13.9#

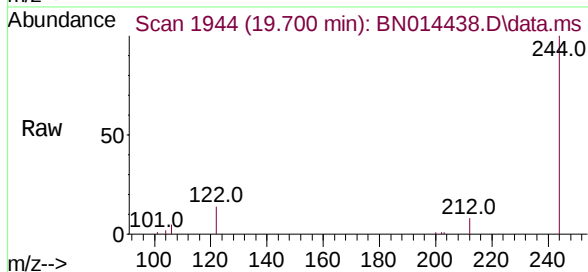




Abundance Scan 1944 (19.700 min): BN014438.D\data.ms (-1914) (-)

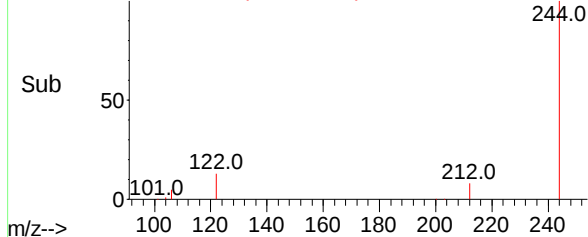


Abundance Scan 2124 (21.247 min): BN014350.D\data.ms (-2132) (-)

Benzo(a)anthracene
Concen: 0.38 ng
RT: 21.239 min Scan# 2122
Delta R.T. 0.000 min
Lab File: BN014438.D
Acq: 26 Apr 2021 11:25


Tgt Ion	Ratio	Lower	Upper
228	100		
226	27.7	21.3	31.9
229	19.2	15.7	23.5

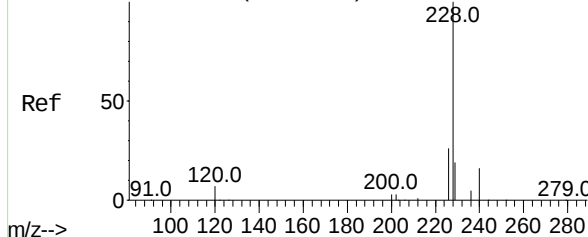

Abundance Scan 2122 (21.239 min): BN014438.D\data.ms (-2103) (-)

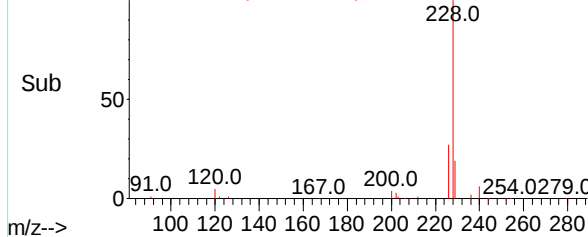



Abundance Scan 2129 (21.300 min): BN014350.D\data.ms (-2129) (-)

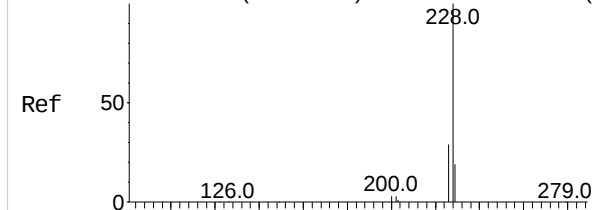


Chrysene
Concen: 0.37 ng
RT: 21.293 min Scan# 2127
Delta R.T. 0.000 min
Lab File: BN014438.D
Acq: 26 Apr 2021 11:25

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	228	Resp:	29027
Ion Ratio	Lower	Upper	
228	100		
226	30.2	23.1	34.7
229	19.4	15.7	23.5

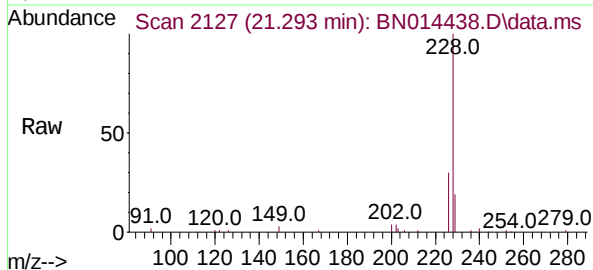

Abundance Scan 2127 (21.293 min): BN014438.D\data.ms (-2118) (-)


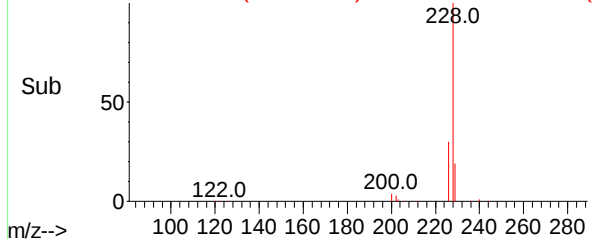


Abundance Scan 2118 (21.184 min): BN014350.D\data.ms (-2118) (-)

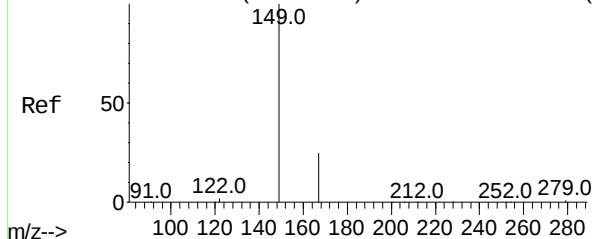


Bis(2-ethylhexyl)phthalate
Concen: 0.89 ng
RT: 21.186 min Scan# 2117
Delta R.T. 0.000 min
Lab File: BN014438.D
Acq: 26 Apr 2021 11:25


Tgt Ion:	149	Resp:	20923
Ion Ratio	Lower	Upper	
149	100		
167	24.8	21.3	31.9
279	3.6	3.1	4.7

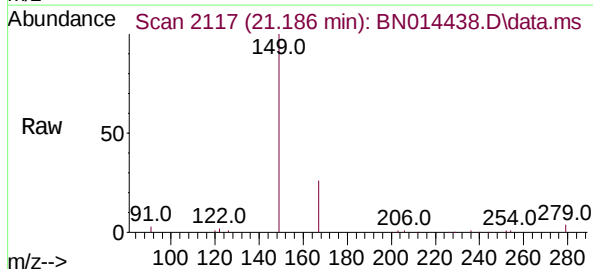

Abundance Scan 2117 (21.186 min): BN014438.D\data.ms (-2108) (-)

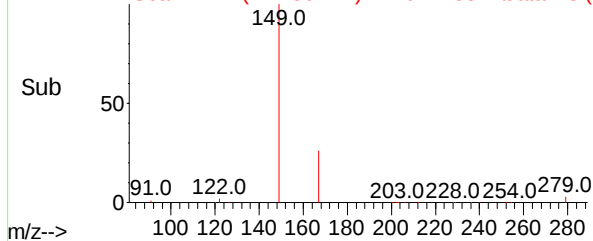


Abundance Scan 3203 (25.725 min): BN014350.D\data.ms (-3175) (-)


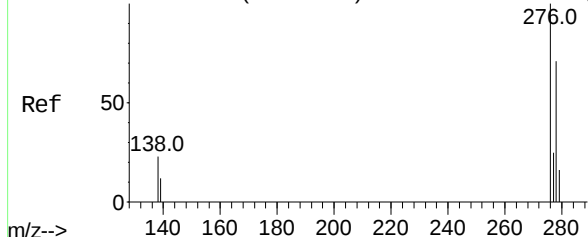


Indeno(1,2,3-cd)pyrene
Concen: 0.34 ng
RT: 25.718 min Scan# 3199
Delta R.T. 0.000 min
Lab File: BN014438.D
Acq: 26 Apr 2021 11:25


Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

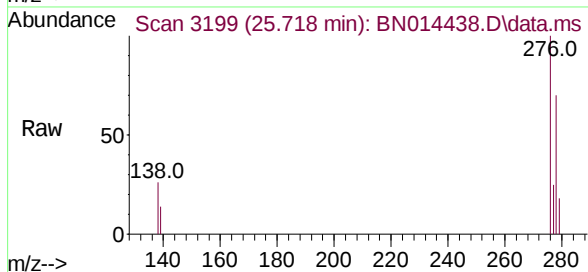


Tgt Ion	Ratio	Lower	Upper
276	100		
138	24.3	18.9	28.3
277	24.7	19.8	29.8





Abundance Scan 2550 (23.490 min): BN014350.D\data.ms (-2538) (-)

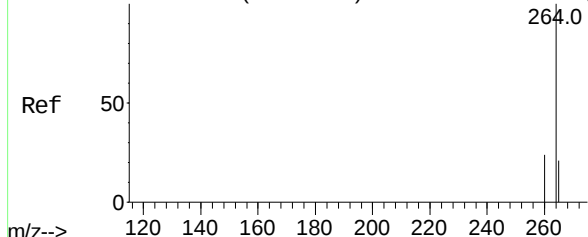


Perylene-d12
Concen: 0.40 ng
RT: 23.482 min Scan# 2546
Delta R.T. 0.000 min
Lab File: BN014438.D
Acq: 26 Apr 2021 11:25



Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.9	19.8	29.6
265	38.3	34.4	51.6

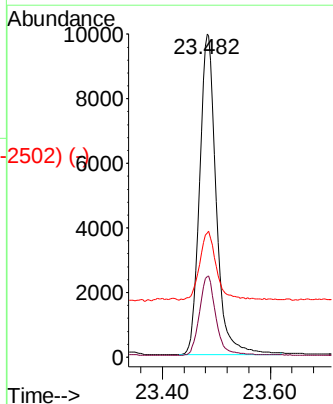




Abundance Scan 2354 (22.819 min): BN014350.D\data.ms (-2354) (-)




Benzo(b)fluoranthene
Concen: 0.39 ng
RT: 22.859 min Scan# 2364
Delta R.T. 0.041 min
Lab File: BN014438.D
Acq: 26 Apr 2021 11:25

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:	252	Resp:	30747
Ion Ratio	Lower	Upper	
252	100		
253	23.8	19.0	28.6
125	12.7	9.7	14.5



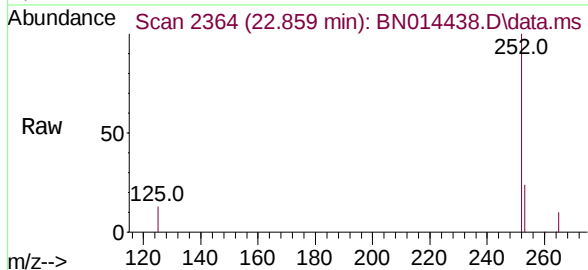


Abundance Scan 2367 (22.864 min): BN014350.D\data.ms (-2367) (-)




Benzo(k)fluoranthene
Concen: 0.39 ng
RT: 22.859 min Scan# 2364
Delta R.T. 0.000 min
Lab File: BN014438.D
Acq: 26 Apr 2021 11:25

Tgt Ion:	252	Resp:	30932
Ion Ratio	Lower	Upper	
252	100		
253	23.8	19.3	28.9
125	12.7	9.4	14.2



Abundance Scan 2521 (23.391 min): BN014350.D\data.ms (-2509) (-)


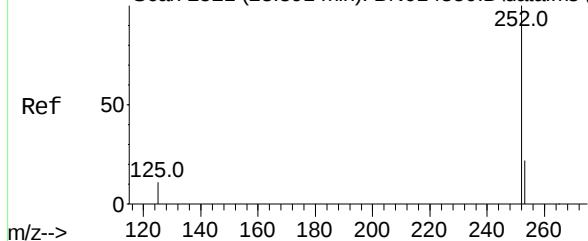


Benzo(a)pyrene
Concen: 0.38 ng
RT: 23.387 min Scan# 2518
Delta R.T. 0.000 min
Lab File: BN014438.D
Acq: 26 Apr 2021 11:25


Tgt Ion:	252	Resp:	25243
Ion Ratio	Lower	Upper	
252	100		
253	25.4	20.7	31.1
125	22.5	11.8	17.6#

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Abundance Scan 2518 (23.387 min): BN014438.D\data.ms

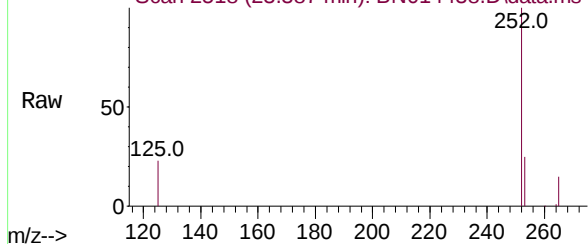

Abundance Scan 2518 (23.387 min): BN014438.D\data.ms (-2460) (-)

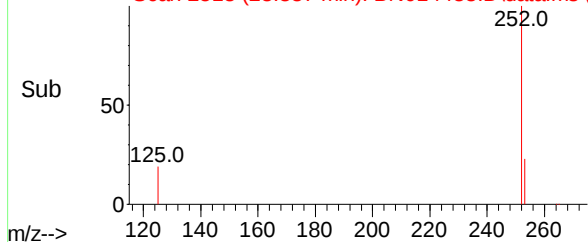



Abundance Scan 3207 (25.739 min): BN014350.D\data.ms (-3146) (-)

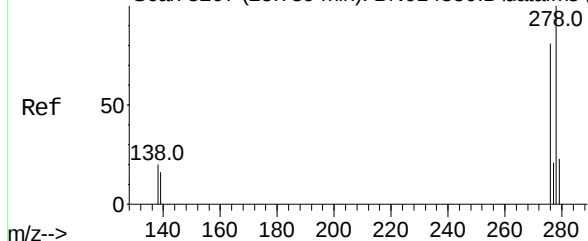


Dibenzo(a,h)anthracene
Concen: 0.32 ng
RT: 25.731 min Scan# 3203
Delta R.T. 0.000 min
Lab File: BN014438.D
Acq: 26 Apr 2021 11:25

Tgt Ion:	278	Resp:	23514
Ion Ratio	Lower	Upper	
278	100		
139	18.3	13.3	19.9
279	25.8	20.2	30.2


Abundance Scan 3203 (25.731 min): BN014438.D\data.ms

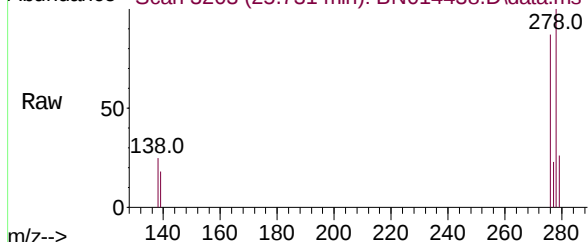

Abundance Scan 3203 (25.731 min): BN014438.D\data.ms (-3180) (-)

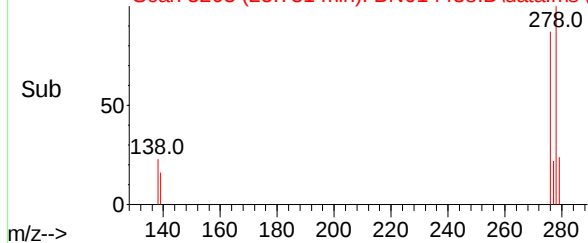


Abundance Scan 3403 (26.410 min): BN014350.D\data.ms (-3373) (-)




Benzo(g,h,i)perylene
Concen: 0.32 ng
RT: 26.395 min Scan# 3397
Delta R.T. 0.000 min
Lab File: BN014438.D
Acq: 26 Apr 2021 11:25

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Abundance Scan 3397 (26.395 min): BN014438.D\data.ms

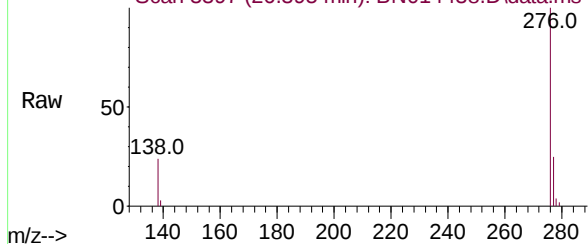

Tgt Ion:	276	Resp:	25210
Ion Ratio	Lower	Upper	
276	100		
277	24.5	19.1	28.7
138	23.7	16.7	25.1

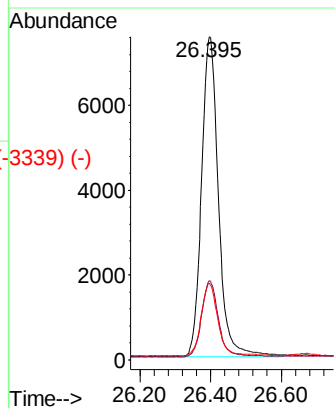

Abundance Scan 3397 (26.395 min): BN014438.D\data.ms (-3339) (-)

