

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042621\
 Data File : BN014442.D
 Acq On : 26 Apr 2021 13:46
 Operator : CG/JU
 Sample : M2164-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BP-VPB-RW8-GW-258-260

Quant Time: Apr 26 14:16:14 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN042221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 26 12:30:05 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.684	152	8439	0.40	ng	0.00
7) Naphthalene-d8	10.454	136	31355	0.40	ng	0.00
13) Acenaphthene-d10	14.308	164	16572	0.40	ng	0.00
19) Phenanthrene-d10	17.055	188	37144	0.40	ng	# 0.00
29) Chrysene-d12	21.261	240	34039	0.40	ng	# 0.00
36) Perylene-d12	23.482	264	26593	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.284	112	1324	0.08	ng	0.00
5) Phenol-d6	6.855	99	1064	0.05	ng	0.00
8) Nitrobenzene-d5	8.819	82	3042	0.12	ng	0.00
11) 2-Methylnaphthalene-d10	12.049	152	9318	0.20	ng	0.00
14) 2,4,6-Tribromophenol	15.805	330	639	0.12	ng	0.00
15) 2-Fluorobiphenyl	12.938	172	14675	0.22	ng	0.01
27) Fluoranthene-d10	19.094	212	22146	0.23	ng	0.00
31) Terphenyl-d14	19.700	244	23625	0.33	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.247	88	3083	0.30	ng	# 73
3) n-Nitrosodimethylamine	3.601	42	94	0.15	ng	# 1
32) Benzo(a)anthracene	21.239	228	2210	0.02	ng	93
33) Chrysene	21.292	228	2449	0.02	ng	94
34) Bis(2-ethylhexyl)phtha...	21.186	149	34559	1.09	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042621\
Data File : BN014442.D
Acq On : 26 Apr 2021 13:46
Operator : CG/JU
Sample : M2164-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BP-VPB-RW8-GW-258-260

Quant Time: Apr 26 14:16:14 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN042221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 26 12:30:05 2021
Response via : Initial Calibration




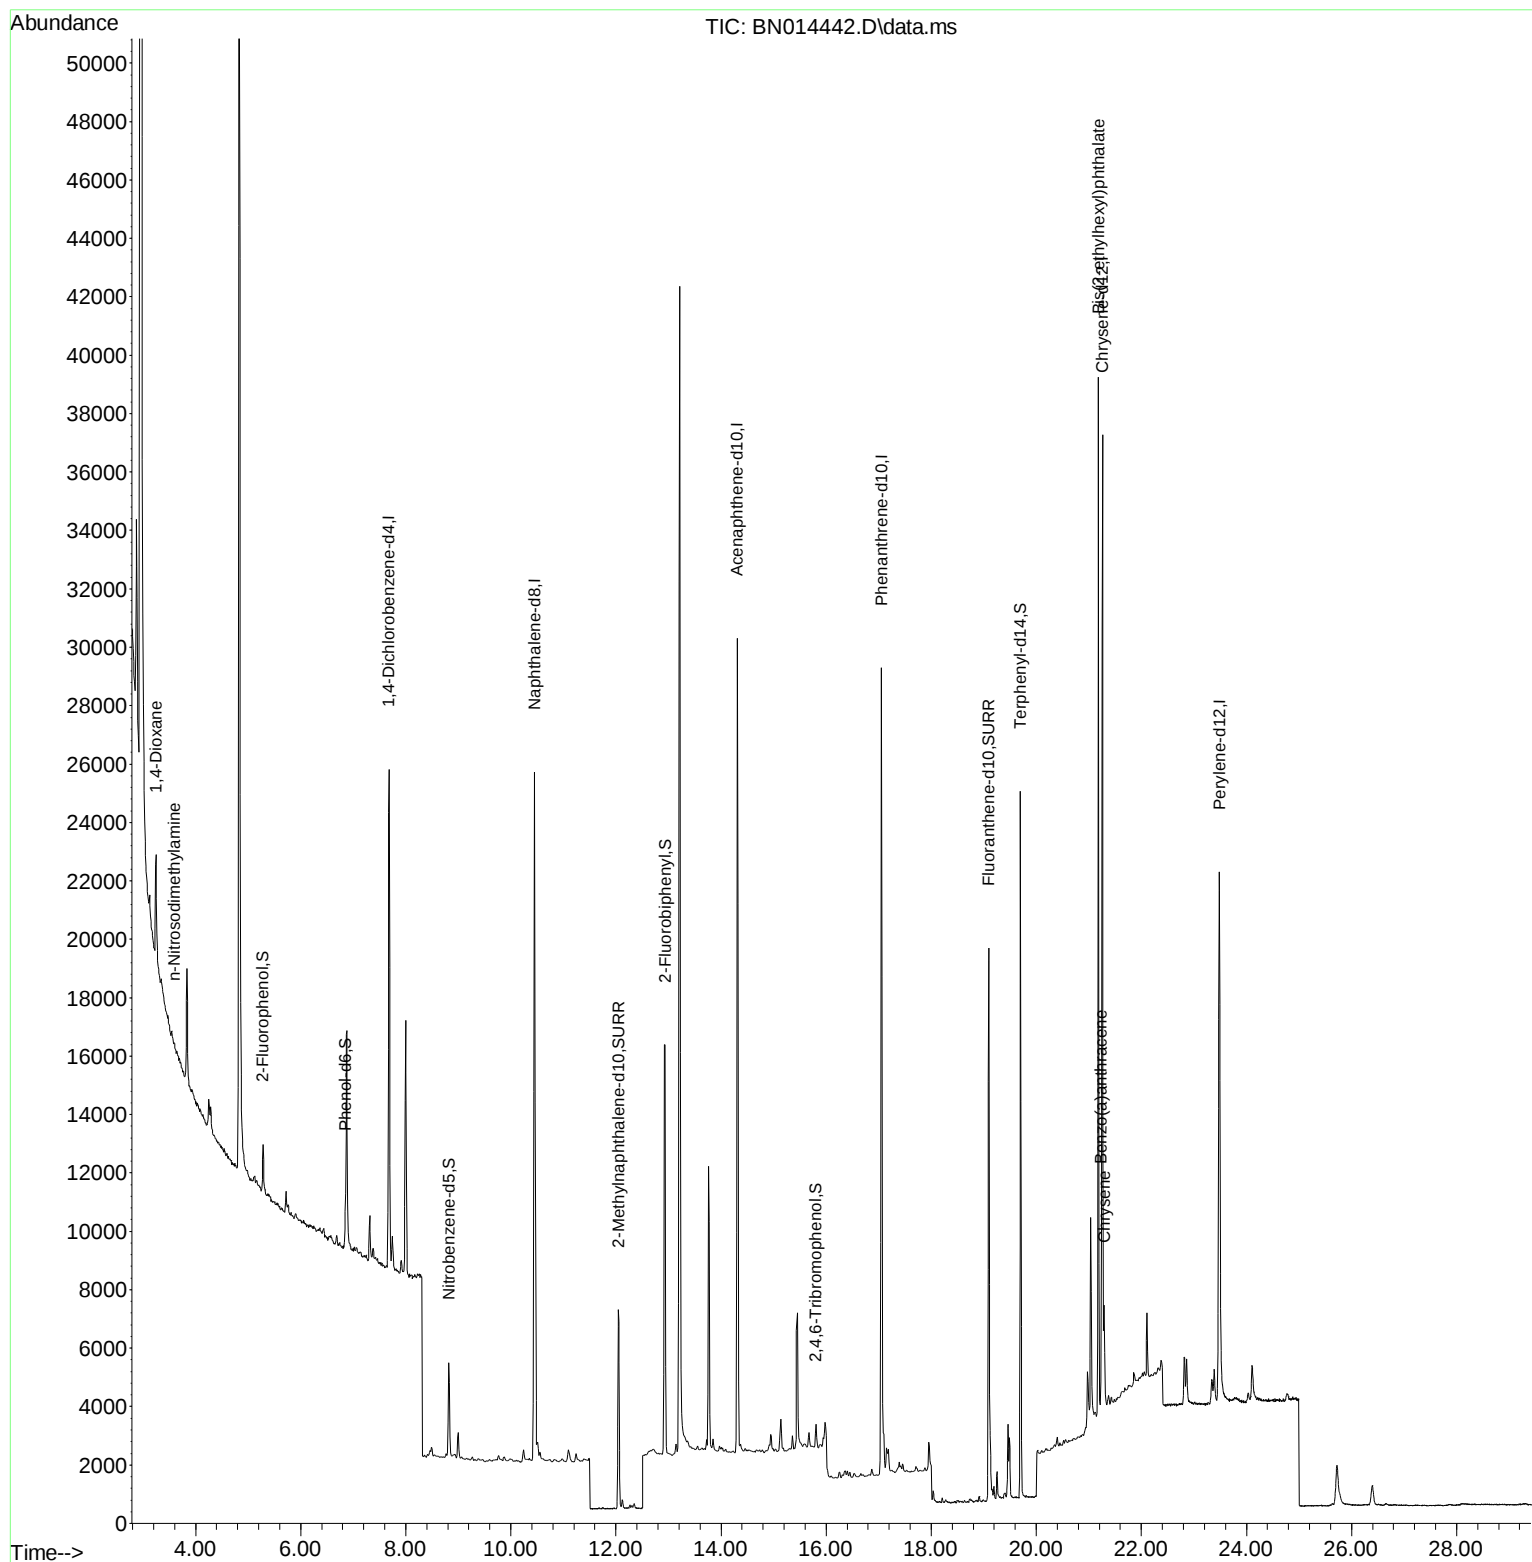


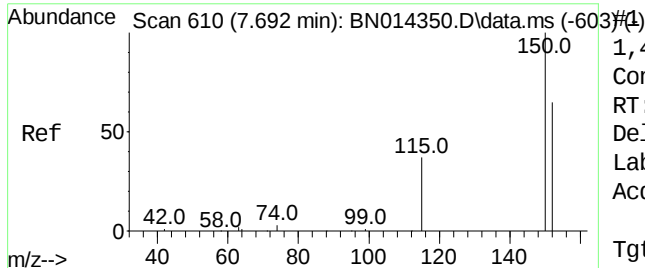

1,4-Dichlorobenzene-d4
Concen: 0.40 ng
RT: 7.684 min Scan# 609
Delta R.T. 0.008 min
Lab File: BN014442.D
Acq: 26 Apr 2021 13:46




Instrument :
BNA_N
ClientSampleId :
BP-VPB-RW8-GW-258-260


Tgt Ion:152 Resp: 8439
Ion Ratio Lower Upper
152 100
150 151.4 123.4 185.2
115 56.4 47.5 71.3

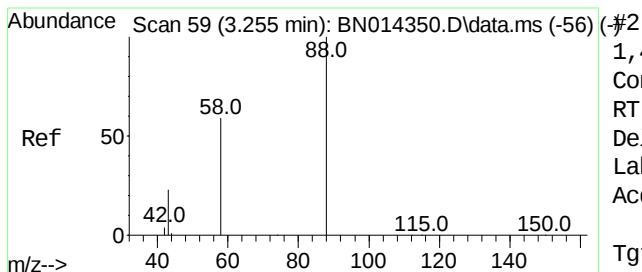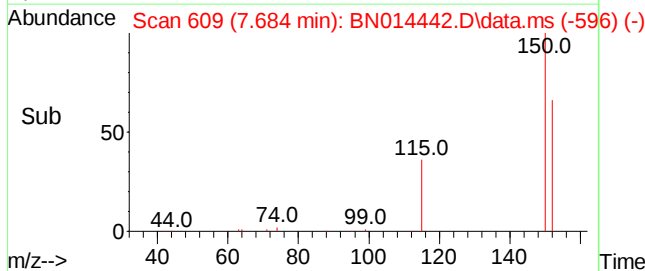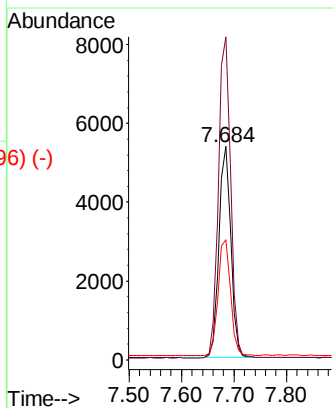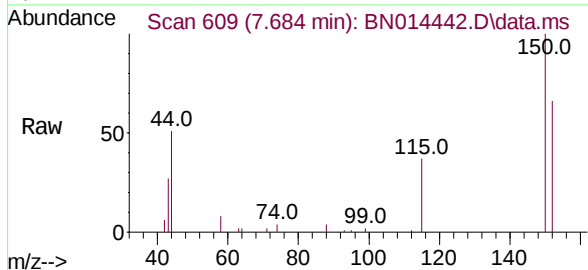

1,4-Dioxane
Concen: 0.30 ng
RT: 3.247 min Scan# 58
Delta R.T. -0.000 min
Lab File: BN014442.D
Acq: 26 Apr 2021 13:46

Tgt Ion: 88 Resp: 3083
Ion Ratio Lower Upper
88 100
58 72.4 52.2 78.2
43 61.6 20.6 30.8#


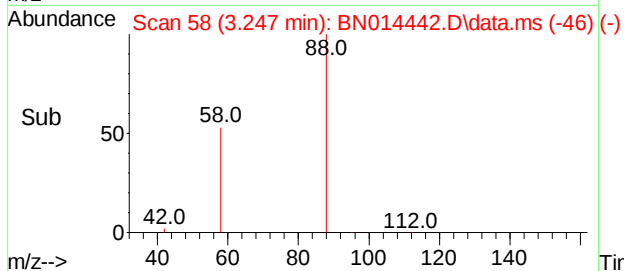
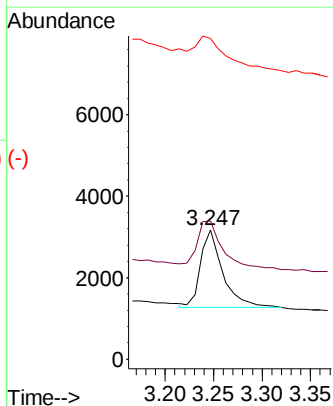
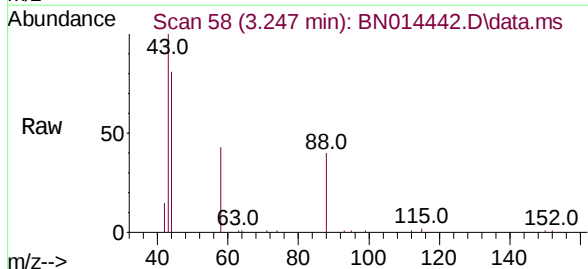


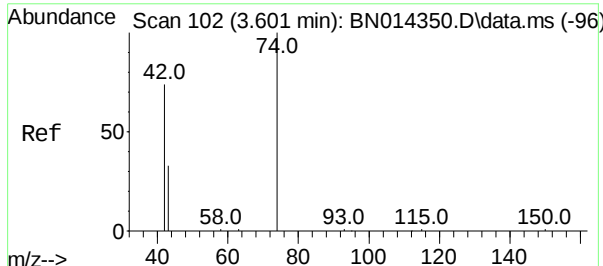

n-Nitrosodimethylamine
 Concen: 0.15 ng
 RT: 3.601 min Scan# 102
 Delta R.T. 0.016 min
 Lab File: BN014442.D
 Acq: 26 Apr 2021 13:46




Instrument :
 BNA_N
 ClientSampleId :
 BP-VPB-RW8-GW-258-260


Tgt Ion:	42	Resp:	94
Ion	Ratio	Lower	Upper
42	100		
74	10.6	108.0	162.0#
44	0.0	0.0	0.0

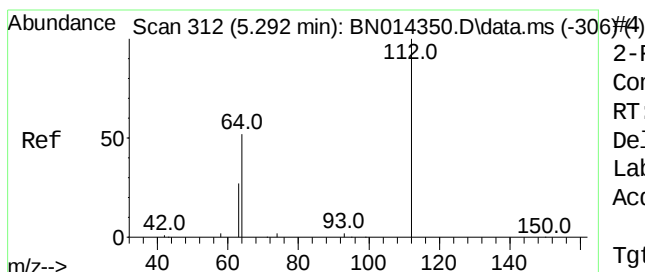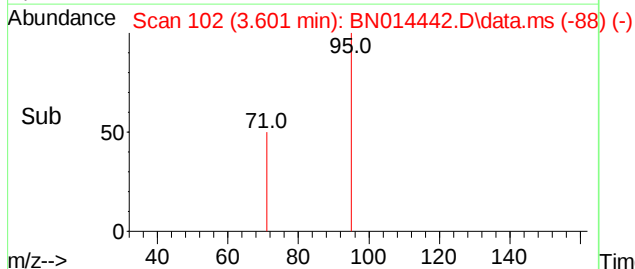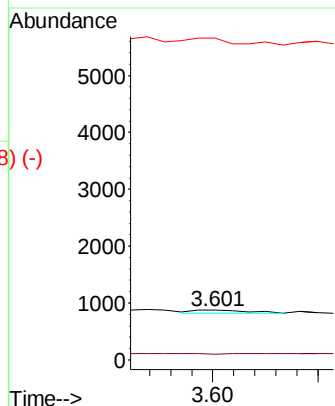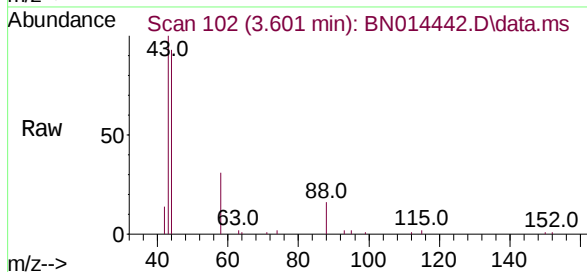

2-Fluorophenol
 Concen: 0.08 ng
 RT: 5.284 min Scan# 311
 Delta R.T. -0.000 min
 Lab File: BN014442.D
 Acq: 26 Apr 2021 13:46

Tgt Ion:	112	Resp:	1324
Ion	Ratio	Lower	Upper
112	100		
64	55.1	43.0	64.6
63	27.6	23.4	35.0


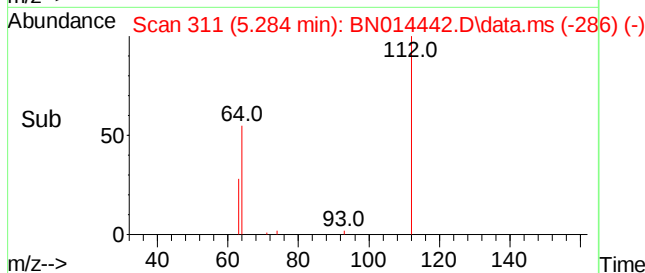
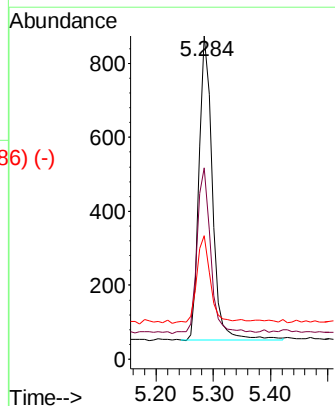
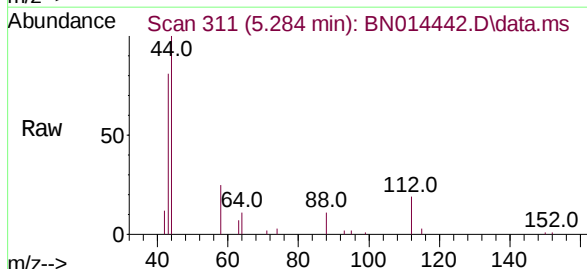


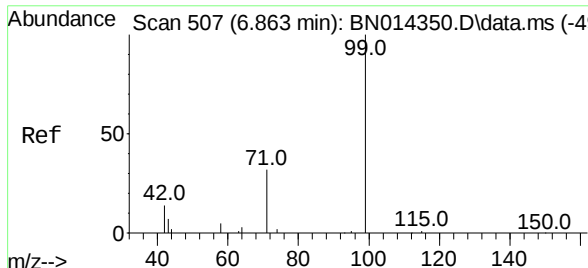

Phenol-d6
 Concen: 0.05 ng
 RT: 6.855 min Scan# 506
 Delta R.T. 0.008 min
 Lab File: BN014442.D
 Acq: 26 Apr 2021 13:46




Instrument :
 BNA_N
 ClientSampleId :
 BP-VPB-RW8-GW-258-260


Tgt Ion:	99	Resp:	1064
Ion	Ratio	Lower	Upper
99	100		
42	0.0	16.0	24.0#
71	46.3	27.8	41.8#

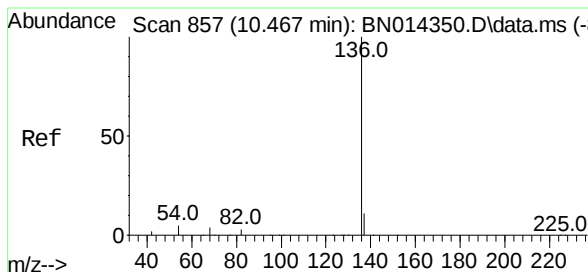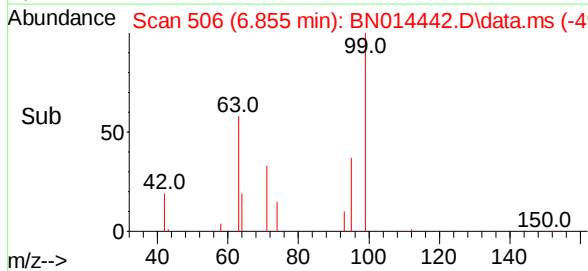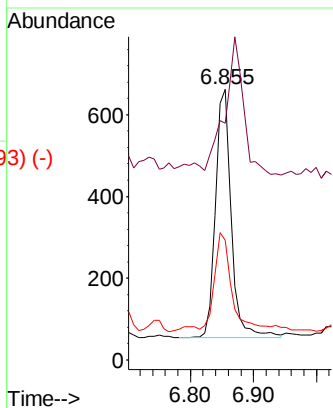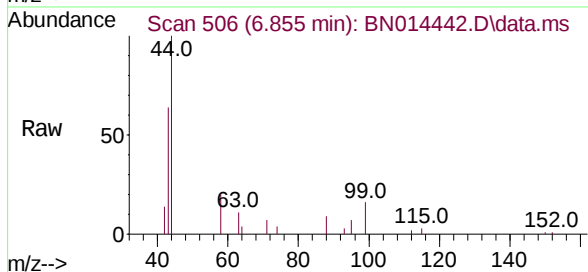

Naphthalene-d8
 Concen: 0.40 ng
 RT: 10.454 min Scan# 856
 Delta R.T. -0.000 min
 Lab File: BN014442.D
 Acq: 26 Apr 2021 13:46

Tgt Ion:	136	Resp:	31355
Ion	Ratio	Lower	Upper
136	100		
137	11.2	9.0	13.6
54	5.8	4.4	6.6
68	5.5	3.9	5.9


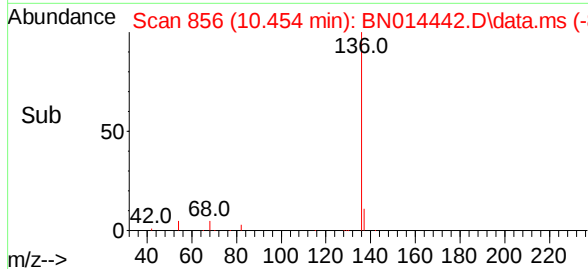
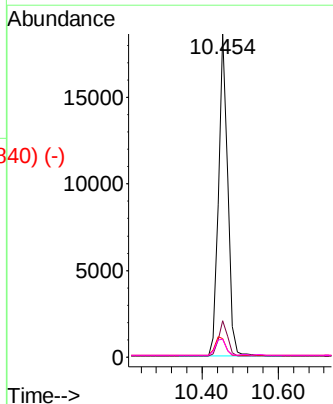
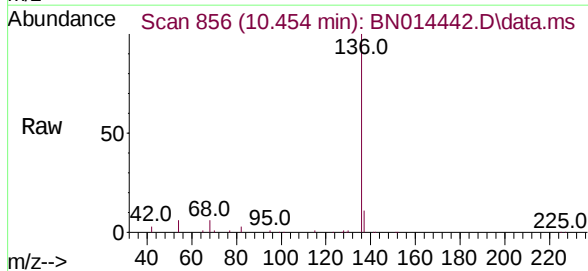


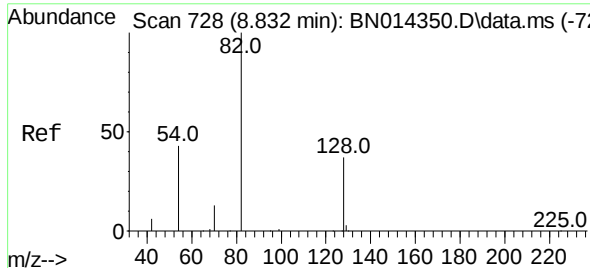

Nitrobenzene-d5
 Concen: 0.12 ng
 RT: 8.819 min Scan# 727
 Delta R.T. -0.000 min
 Lab File: BN014442.D
 Acq: 26 Apr 2021 13:46




Instrument :
 BNA_N
 ClientSampleId :
 BP-VPB-RW8-GW-258-260

Tgt Ion:	82	Resp:	3042
Ion	Ratio	Lower	Upper
82	100		
128	37.1	30.3	45.5
54	50.1	35.8	53.8

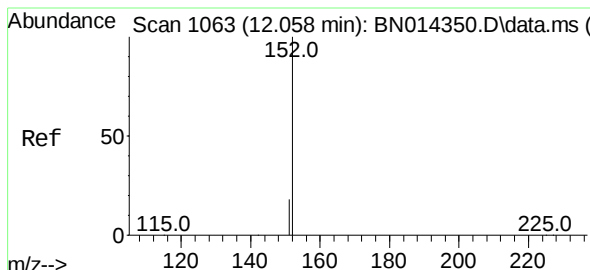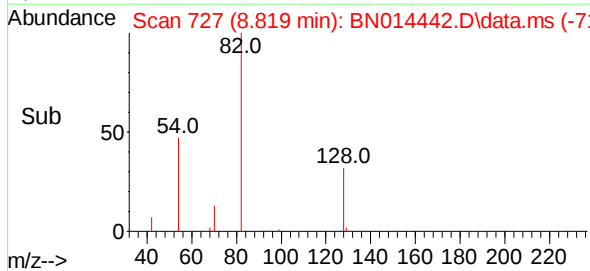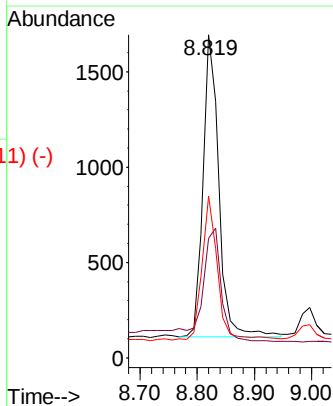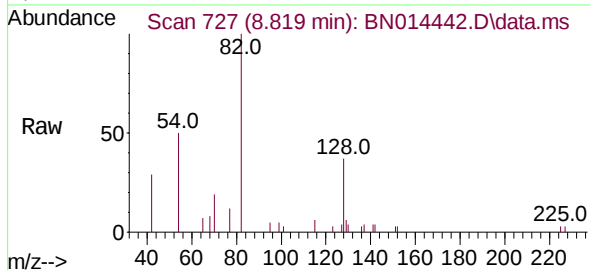

2-Methylnaphthalene-d10
 Concen: 0.20 ng
 RT: 12.049 min Scan# 1061
 Delta R.T. 0.004 min
 Lab File: BN014442.D
 Acq: 26 Apr 2021 13:46


Tgt Ion:	152	Resp:	9318
Ion	Ratio	Lower	Upper
152	100		
151	20.6	16.3	24.5

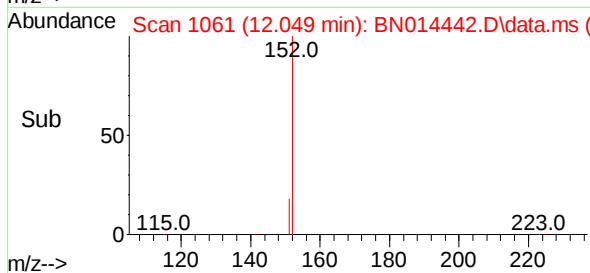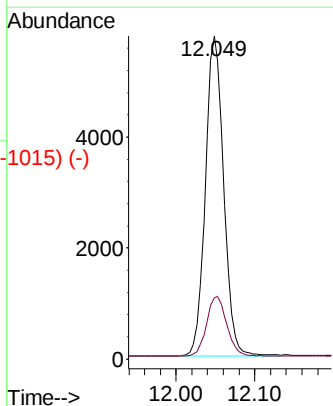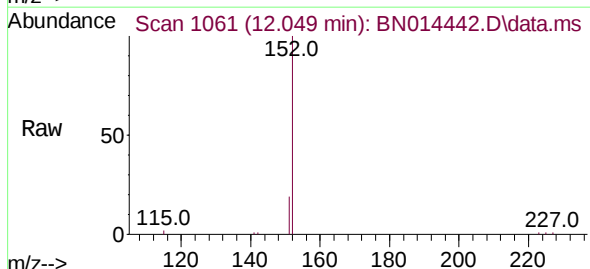




Abundance Scan 1307 (14.321 min): BN014350.D\data.ms (-1299) (-)

Acenaphthene-d10
Concen: 0.40 ng
RT: 14.308 min Scan# 1306
Delta R.T. -0.000 min
Lab File: BN014442.D
Acq: 26 Apr 2021 13:46

Instrument :
BNA_N
ClientSampleId :
BP-VPB-RW8-GW-258-260

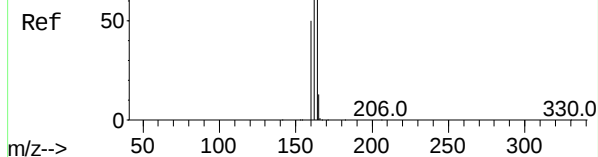




Tgt Ion:	164	Resp:	16572
Ion Ratio	Lower	Upper	
164	100		
162	102.1	81.0	121.6
160	50.2	40.7	61.1

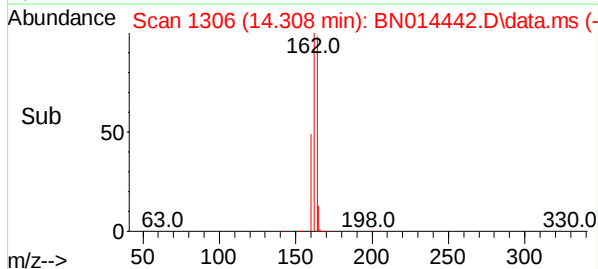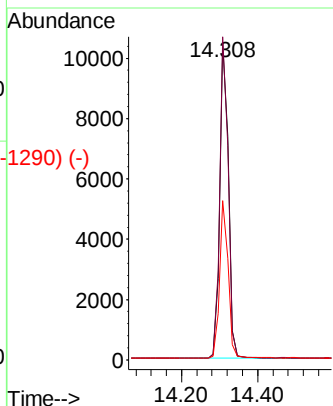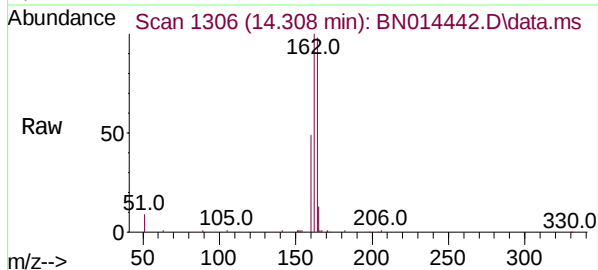

Abundance Scan 1425 (15.818 min): BN014350.D\data.ms (-1416) (-)

2,4,6-Tribromophenol
Concen: 0.12 ng
RT: 15.805 min Scan# 1424
Delta R.T. -0.000 min
Lab File: BN014442.D
Acq: 26 Apr 2021 13:46


Tgt Ion:	330	Resp:	639
Ion Ratio	Lower	Upper	
330	100		
332	0.0	0.0	0.0
141	38.5	26.2	39.2

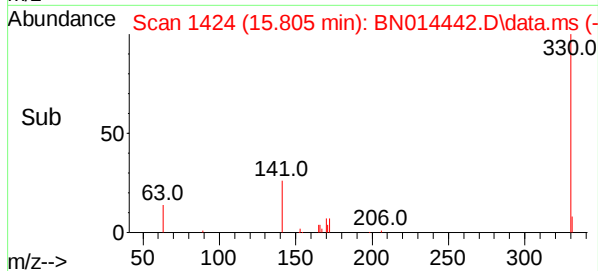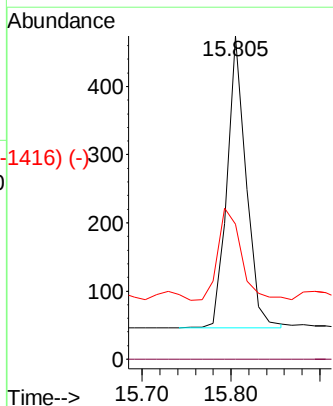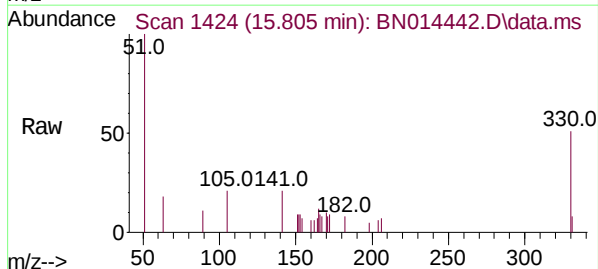



Abundance Scan 1198 (12.938 min): BN014350.D\data.ms (-1189) (-)

2-Fluorobiphenyl
Concen: 0.22 ng
RT: 12.938 min Scan# 1198
Delta R.T. 0.013 min
Lab File: BN014442.D
Acq: 26 Apr 2021 13:46


Instrument :
BNA_N
ClientSampleId :
BP-VPB-RW8-GW-258-260

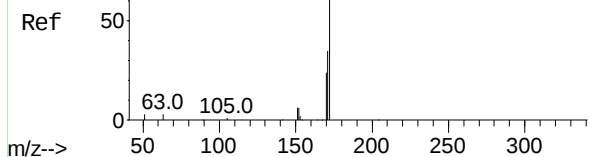

Tgt Ion:	172	Resp:	14675
Ion	Ratio	Lower	Upper
172	100		
171	32.7	28.2	42.2
170	21.9	19.6	29.4

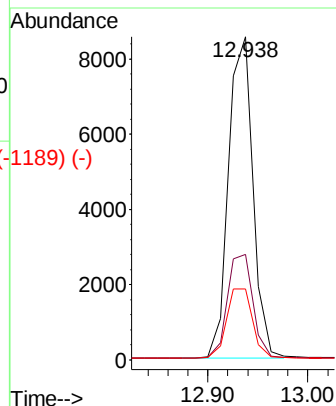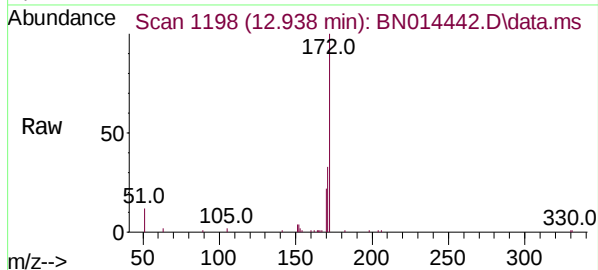



Abundance Scan 1198 (12.938 min): BN014442.D\data.ms (-1189) (-)

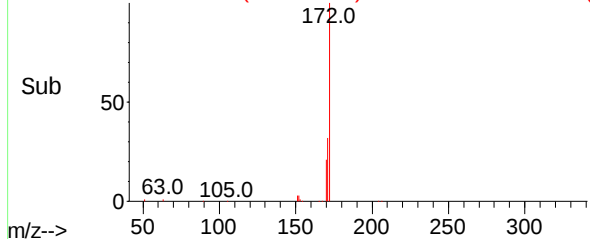


Abundance Scan 1527 (17.067 min): BN014350.D\data.ms (-1510) (-)

Phenanthrene-d10
Concen: 0.40 ng
RT: 17.055 min Scan# 1526
Delta R.T. -0.000 min
Lab File: BN014442.D
Acq: 26 Apr 2021 13:46


Tgt Ion:	188	Resp:	37144
Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	11.0	6.2	9.4#

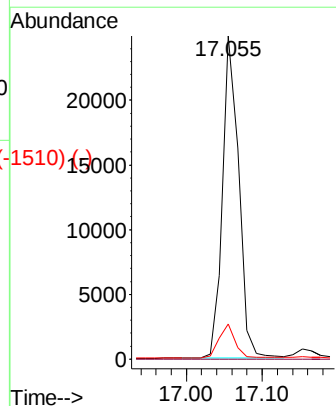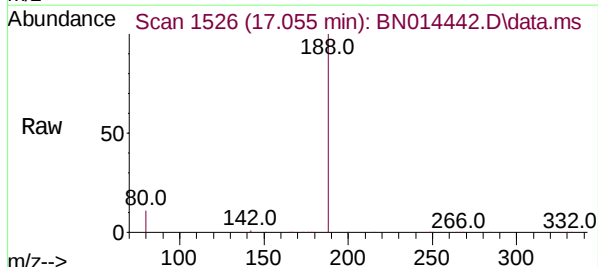

Abundance Scan 1526 (17.055 min): BN014442.D\data.ms (-1510) (-)

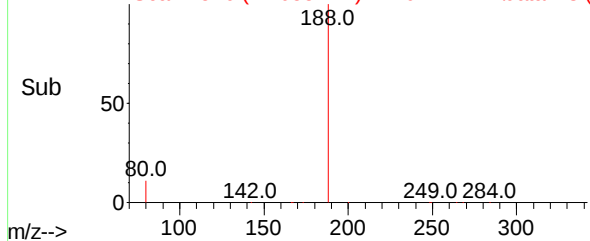




Abundance Scan 1825 (19.101 min): BN014350.D\data.ms (-1827) (-)

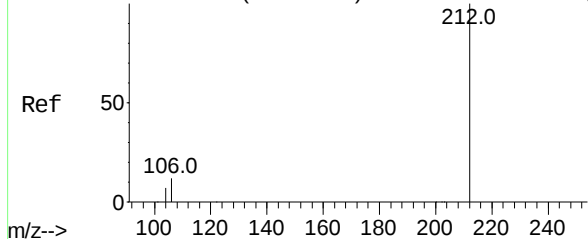


Fluoranthene-d10
Concen: 0.23 ng
RT: 19.094 min Scan# 1822
Delta R.T. -0.005 min
Lab File: BN014442.D
Acq: 26 Apr 2021 13:46

Instrument :
BNA_N
ClientSampleId :
BP-VPB-RW8-GW-258-260

Tgt Ion	Ratio	Lower	Upper
212	100		
106	13.3	9.7	14.5
104	7.3	5.4	8.0

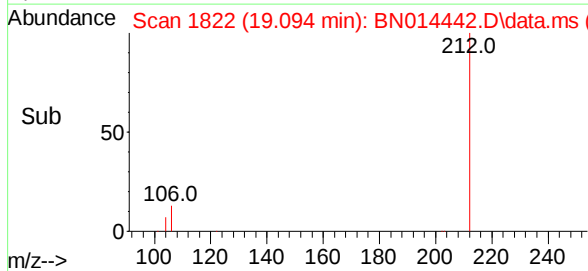
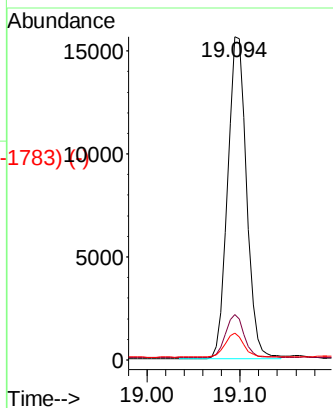
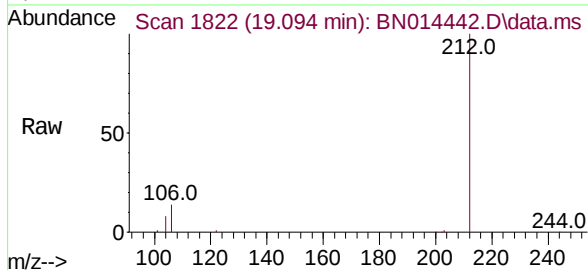


Abundance Scan 2125 (21.258 min): BN014350.D\data.ms (-2129) (-)

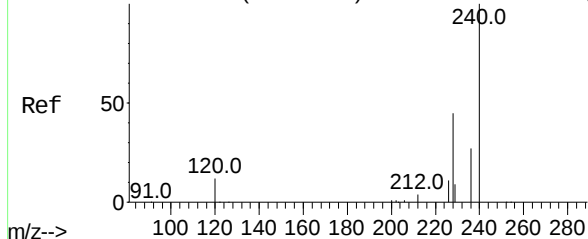

Chrysene-d12
Concen: 0.40 ng
RT: 21.261 min Scan# 2124
Delta R.T. -0.000 min
Lab File: BN014442.D
Acq: 26 Apr 2021 13:46

Tgt Ion	Ratio	Lower	Upper
240	100		
120	7.5	10.7	16.1#
236	25.8	21.5	32.3

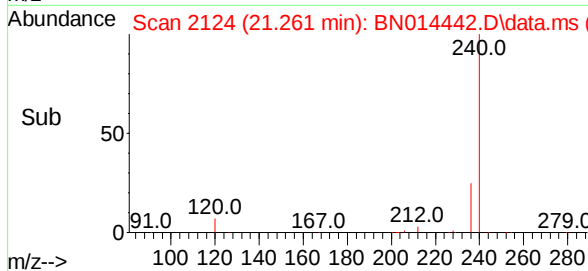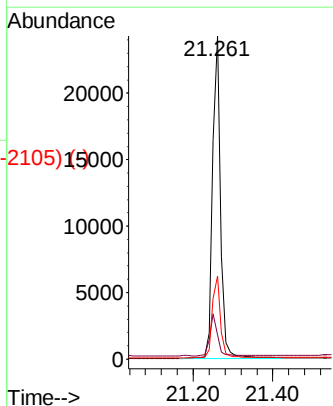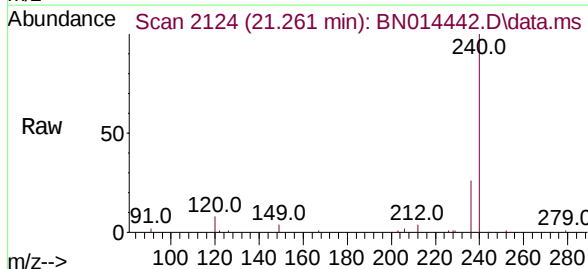

Abundance Scan 1947 (19.707 min): BN014350.D\data.ms (-1934) (-)

Terphenyl-d14
Concen: 0.33 ng
RT: 19.700 min Scan# 1944
Delta R.T. -0.000 min
Lab File: BN014442.D
Acq: 26 Apr 2021 13:46

Instrument :
BNA_N
ClientSampleId :
BP-VPB-RW8-GW-258-260

Ref 50 0 101.0 122.0 212.0 244.0

m/z--> 100 120 140 160 180 200 220 240

Tgt Ion:244 Resp: 23625
Ion Ratio Lower Upper
244 100
212 7.8 6.2 9.4
122 13.1 9.3 13.9

Abundance Scan 1944 (19.700 min): BN014442.D\data.ms

Raw 50 0 101.0 122.0 212.0 244.0

m/z--> 100 120 140 160 180 200 220 240

Abundance

19.700

15000

10000

5000

0

Time--> 19.60 19.80

Abundance Scan 1944 (19.700 min): BN014442.D\data.ms (-1914) (-)

Sub 50 0 101.0 122.0 212.0 244.0

m/z--> 100 120 140 160 180 200 220 240

Abundance Scan 2124 (21.247 min): BN014350.D\data.ms (-2132) (-)

Benzo(a)anthracene
Concen: 0.02 ng
RT: 21.239 min Scan# 2122
Delta R.T. -0.000 min
Lab File: BN014442.D
Acq: 26 Apr 2021 13:46

Ref 50 0 91.0 120.0 200.0 228.0 279.0

m/z--> 100 120 140 160 180 200 220 240 260 280

Tgt Ion:228 Resp: 2210
Ion Ratio Lower Upper
228 100
226 30.7 21.3 31.9
229 22.7 15.7 23.5

Abundance Scan 2122 (21.239 min): BN014442.D\data.ms

Raw 50 0 91.0 120.0 149.0 206.0 240.0 279.0

m/z--> 100 120 140 160 180 200 220 240 260 280

Abundance

21.239

1500

1000

500

0


Time--> 21.20

Abundance Scan 2122 (21.239 min): BN014442.D\data.ms (-2103) (-)

Sub 50 0 120.0 167.0 212.0 240.0 279.0

m/z--> 100 120 140 160 180 200 220 240 260 280

Abundance Scan 2129 (21.300 min): BN014350.D\data.ms (-2129) (-)


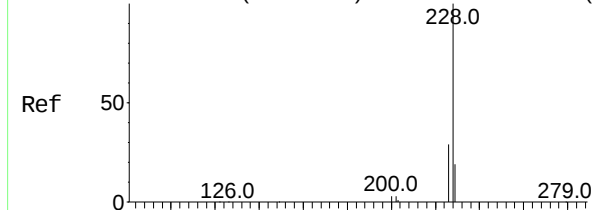


Chrysene
Concen: 0.02 ng
RT: 21.292 min Scan# 2127
Delta R.T. -0.000 min
Lab File: BN014442.D
Acq: 26 Apr 2021 13:46


Instrument :
BNA_N
ClientSampleId :
BP-VPB-RW8-GW-258-260

Tgt Ion:	228	Resp:	2449
Ion Ratio	Lower	Upper	
228	100		
226	32.3	23.1	34.7
229	22.2	15.7	23.5


Abundance Scan 2127 (21.292 min): BN014442.D\data.ms

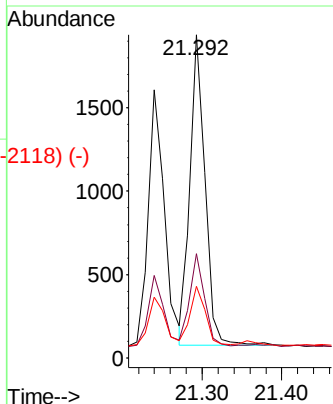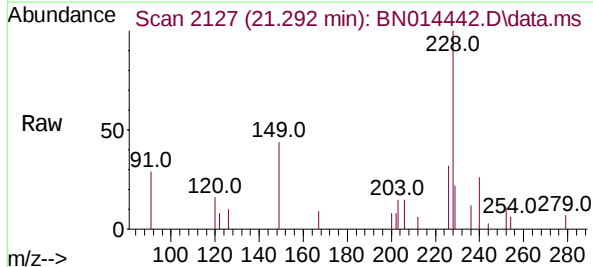

Abundance Scan 2127 (21.292 min): BN014442.D\data.ms (-2118) (-)

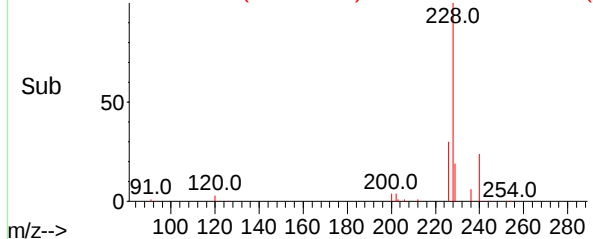



Abundance Scan 2118 (21.184 min): BN014350.D\data.ms (-2118) (-)

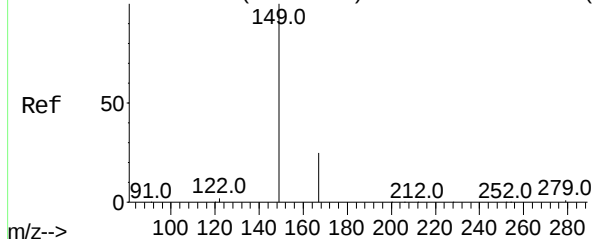


Bis(2-ethylhexyl)phthalate
Concen: 1.09 ng
RT: 21.186 min Scan# 2117
Delta R.T. -0.000 min
Lab File: BN014442.D
Acq: 26 Apr 2021 13:46

Tgt Ion:	149	Resp:	34559
Ion Ratio	Lower	Upper	
149	100		
167	26.6	21.3	31.9
279	3.6	3.1	4.7


Abundance Scan 2117 (21.186 min): BN014442.D\data.ms

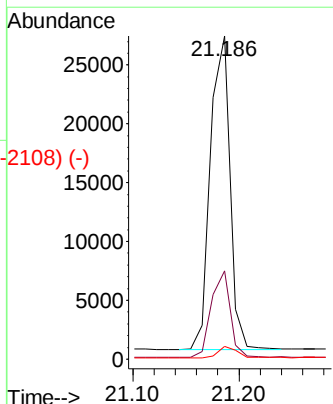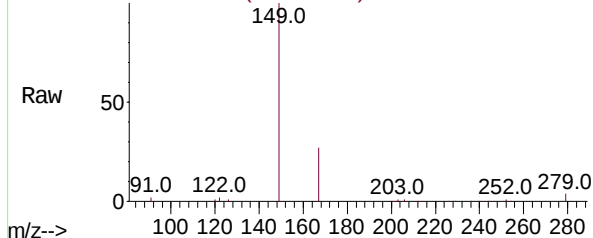

Abundance Scan 2117 (21.186 min): BN014442.D\data.ms (-2108) (-)

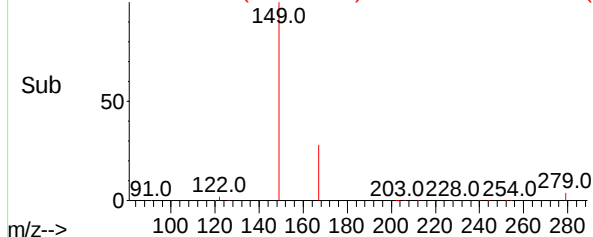



Abundance Scan 2550 (23.490 min): BN014350.D\data.ms (-2538) (-)

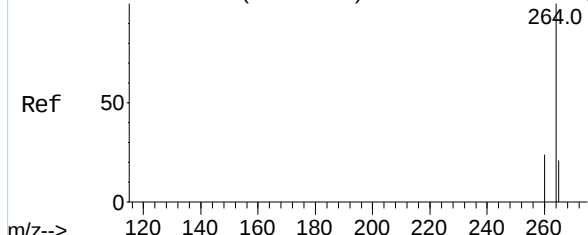

Perylene-d12
Concen: 0.40 ng
RT: 23.482 min Scan# 2546
Delta R.T. -0.000 min
Lab File: BN014442.D
Acq: 26 Apr 2021 13:46

Instrument :
BNA_N
ClientSampleId :
BP-VPB-RW8-GW-258-260

Tgt Ion:	264	Resp:	26593
Ion	Ratio	Lower	Upper
264	100		
260	24.8	19.8	29.6
265	40.4	34.4	51.6

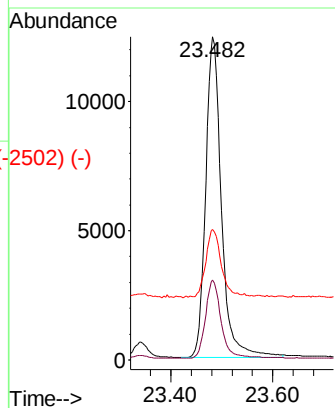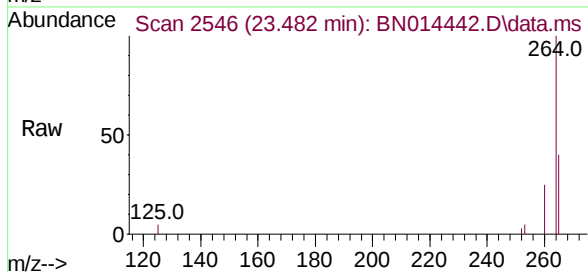

Abundance Scan 2546 (23.482 min): BN014442.D\data.ms (-2502) (-)

