

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042621\
 Data File : BN014449.D
 Acq On : 26 Apr 2021 18:31
 Operator : CG/JU
 Sample : PB135981BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB135981BL

Quant Time: Apr 27 03:30:57 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN042221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 26 12:30:05 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.684	152	9349	0.40	ng	0.00
7) Naphthalene-d8	10.454	136	35469	0.40	ng	0.00
13) Acenaphthene-d10	14.308	164	18930	0.40	ng	0.00
19) Phenanthrene-d10	17.055	188	38950	0.40	ng	# 0.00
29) Chrysene-d12	21.261	240	33138	0.40	ng	# 0.00
36) Perylene-d12	23.482	264	30728	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.284	112	7624	0.40	ng	0.00
5) Phenol-d6	6.855	99	9012	0.38	ng	0.00
8) Nitrobenzene-d5	8.819	82	6770	0.23	ng	0.00
11) 2-Methylnaphthalene-d10	12.048	152	17956	0.34	ng	0.00
14) 2,4,6-Tribromophenol	15.805	330	1414	0.23	ng	0.00
15) 2-Fluorobiphenyl	12.938	172	25707	0.34	ng	0.01
27) Fluoranthene-d10	19.099	212	30210	0.29	ng	0.00
31) Terphenyl-d14	19.700	244	26808	0.38	ng	0.00
Target Compounds						Qvalue
3) n-Nitrosodimethylamine	3.609	42	129	0.15	ng	# 1
34) Bis(2-ethylhexyl)phtha...	21.186	149	974	0.03	ng	# 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042621\
Data File : BN014449.D
Acq On : 26 Apr 2021 18:31
Operator : CG/JU
Sample : PB135981BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB135981BL

Quant Time: Apr 27 03:30:57 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN042221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 26 12:30:05 2021
Response via : Initial Calibration




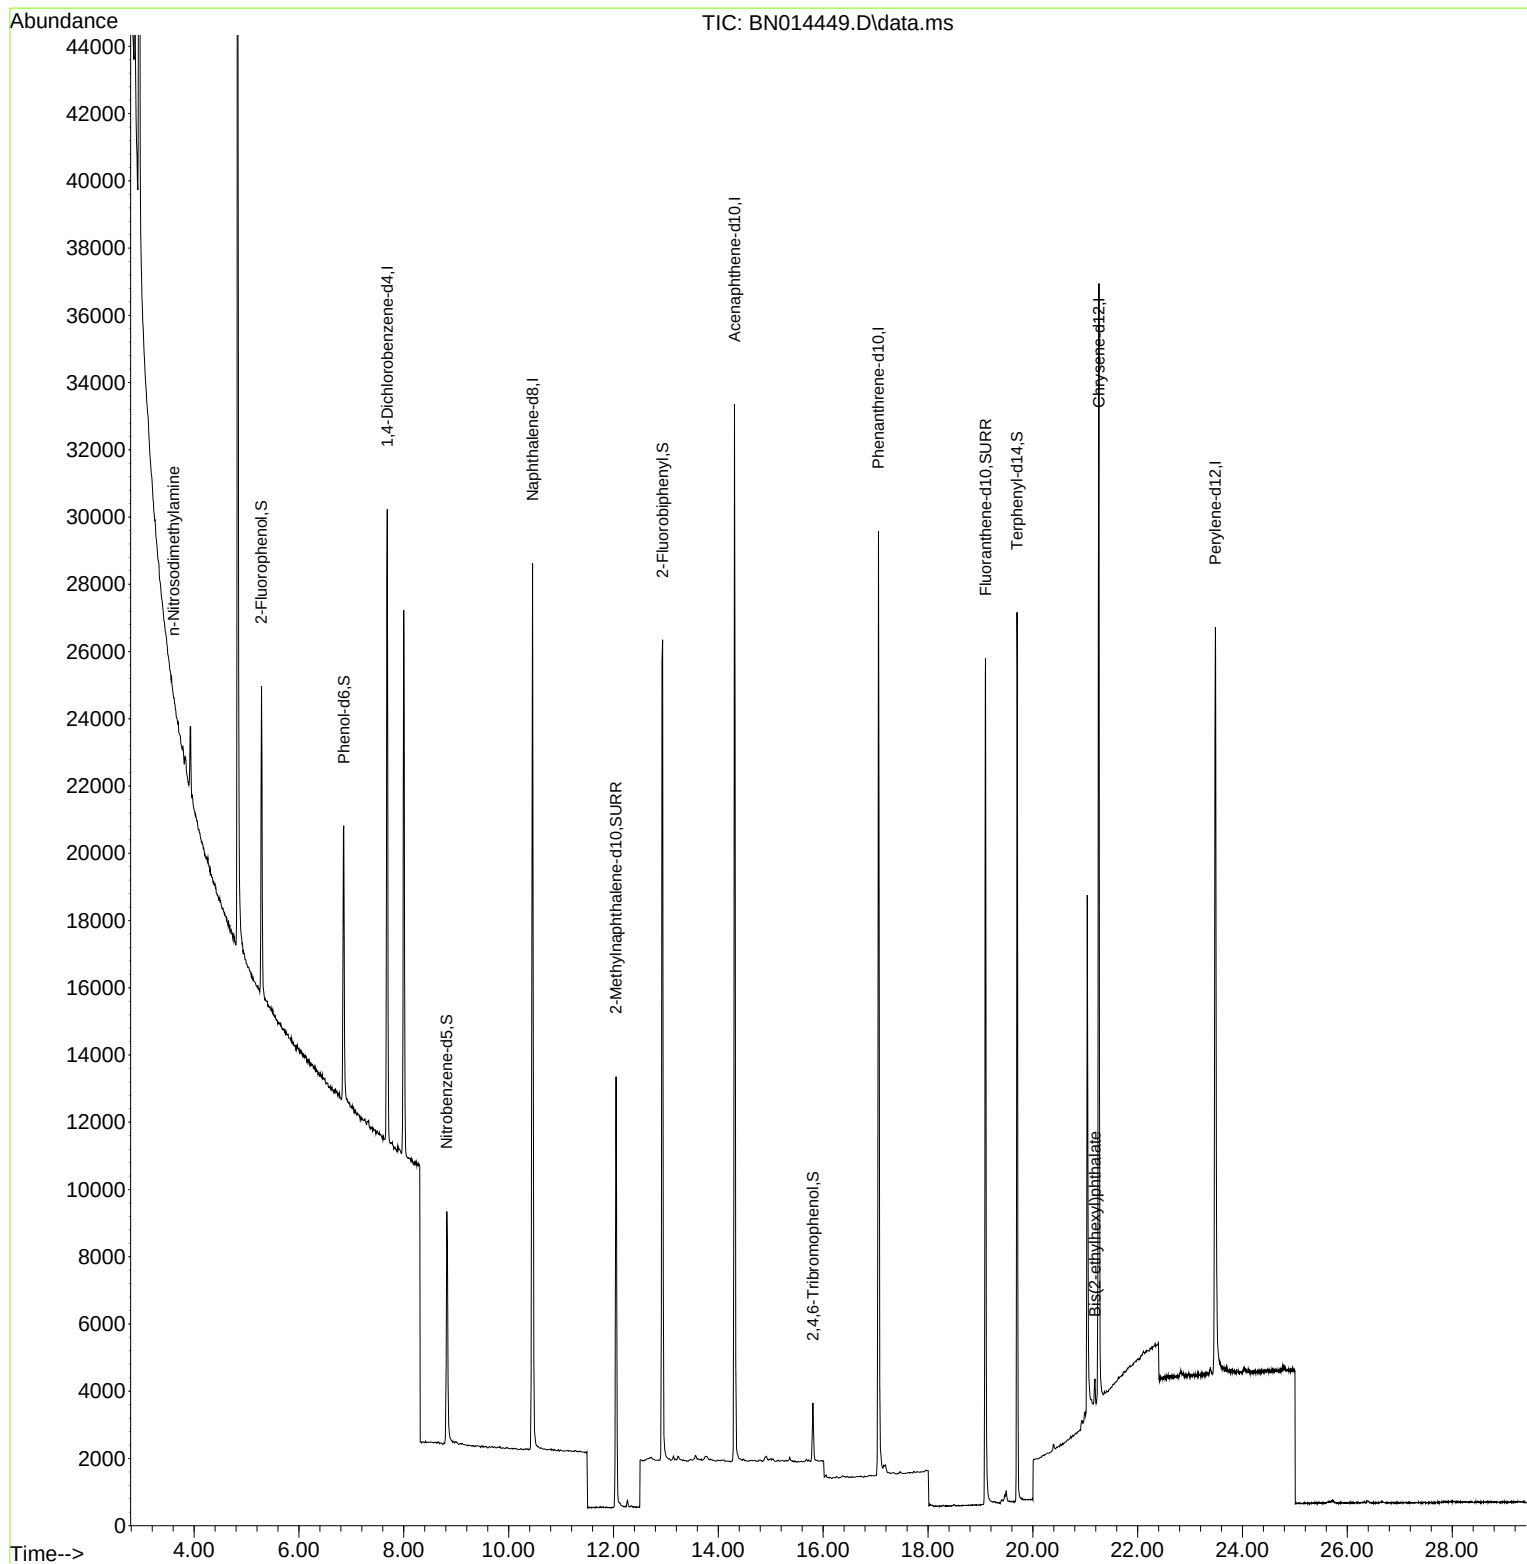


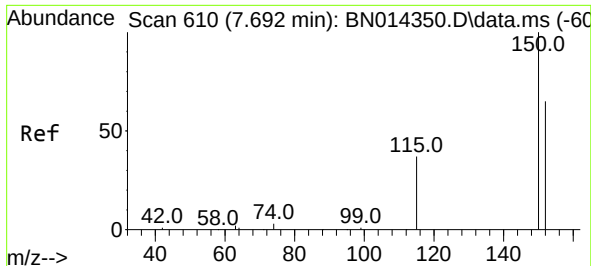

#1
1,4-Dichlorobenzene-d4
Concen: 0.40 ng
RT: 7.684 min Scan# 609
Delta R.T. 0.008 min
Lab File: BN014449.D
Acq: 26 Apr 2021 18:31




Instrument :
BNA_N
ClientSampleId :
PB135981BL


Tgt Ion:152 Resp: 9349
Ion Ratio Lower Upper
152 100
150 154.1 123.4 185.2
115 57.2 47.5 71.3

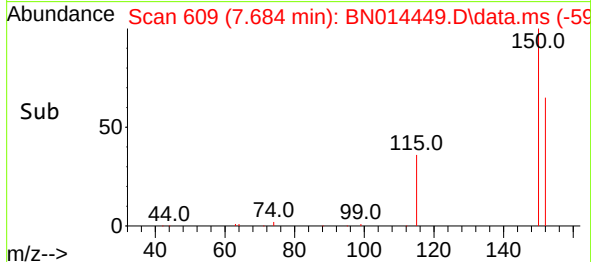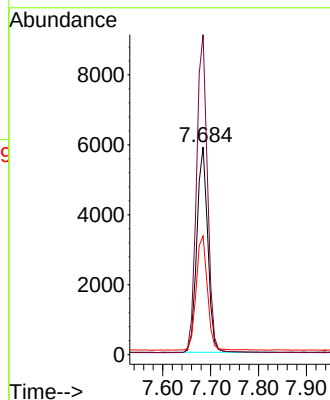

#3
n-Nitrosodimethylamine
Concen: 0.15 ng
RT: 3.609 min Scan# 103
Delta R.T. 0.024 min
Lab File: BN014449.D
Acq: 26 Apr 2021 18:31

Tgt Ion: 42 Resp: 129
Ion Ratio Lower Upper
42 100
74 7.8 108.0 162.0#
44 0.0 0.0 0.0


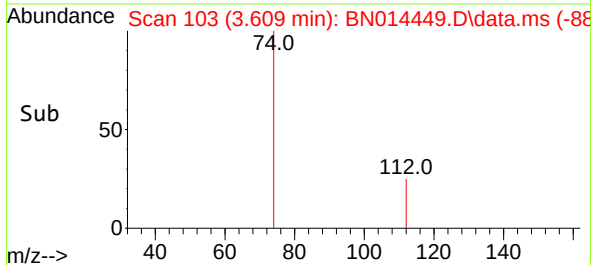
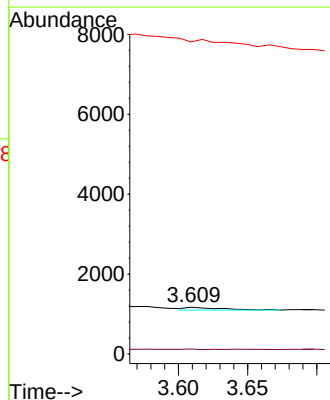
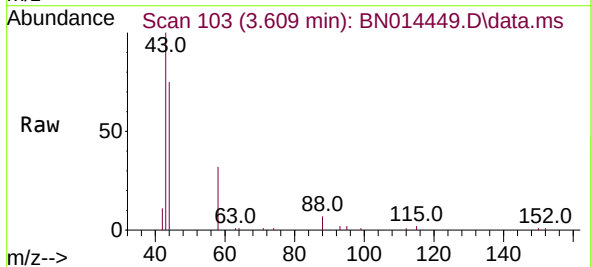


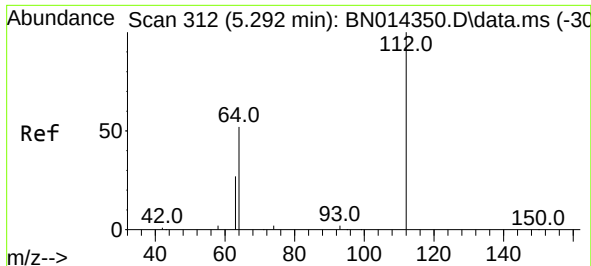

#4
2-Fluorophenol
Concen: 0.40 ng
RT: 5.284 min Scan# 311
Delta R.T. -0.000 min
Lab File: BN014449.D
Acq: 26 Apr 2021 18:31




Instrument :
BNA_N
ClientSampleId :
PB135981BL


Tgt Ion:112 Resp: 7624
Ion Ratio Lower Upper
112 100
64 52.1 43.0 64.6
63 26.9 23.4 35.0

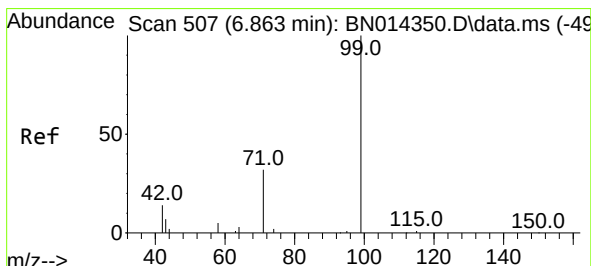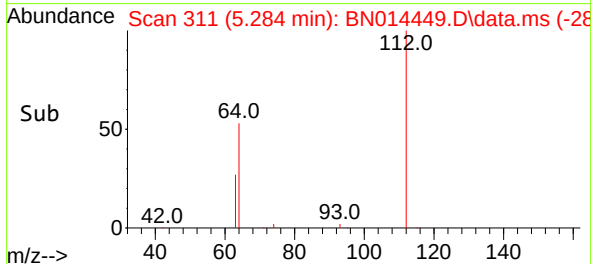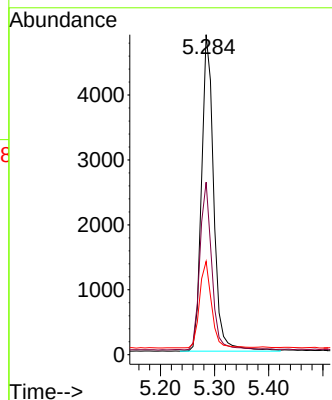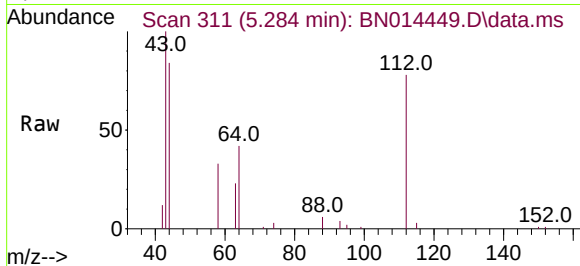

#5
Phenol-d6
Concen: 0.38 ng
RT: 6.855 min Scan# 506
Delta R.T. 0.008 min
Lab File: BN014449.D
Acq: 26 Apr 2021 18:31

Tgt Ion: 99 Resp: 9012
Ion Ratio Lower Upper
99 100
42 16.4 16.0 24.0
71 31.6 27.8 41.8



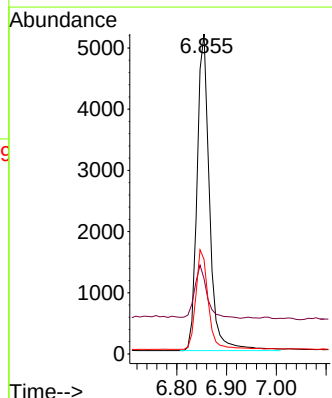
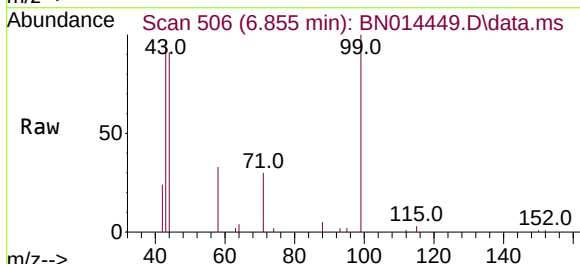


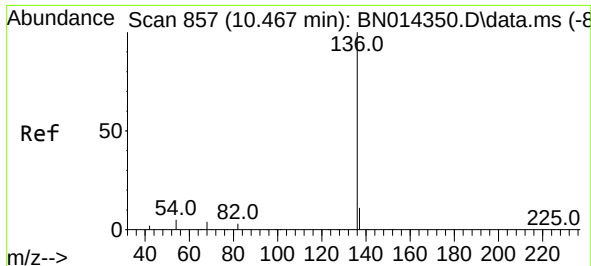

#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.454 min Scan# 856
Delta R.T. -0.000 min
Lab File: BN014449.D
Acq: 26 Apr 2021 18:31




Instrument :
BNA_N
ClientSampleId :
PB135981BL


Tgt Ion:136	Resp:	35469
Ion Ratio	Lower	Upper
136	100	
137	11.3	9.0 13.6
54	5.8	4.4 6.6
68	5.6	3.9 5.9

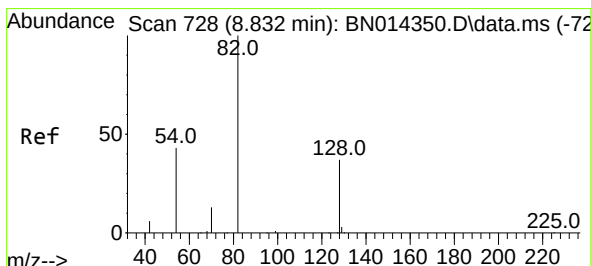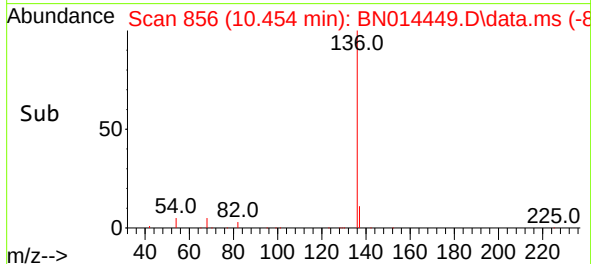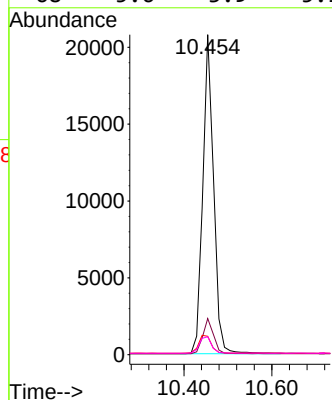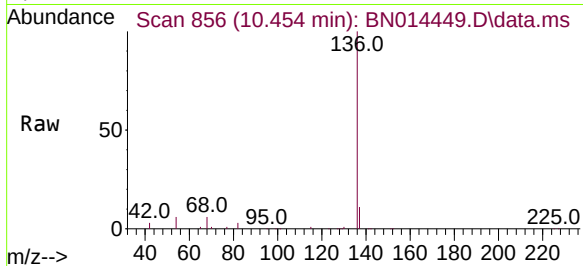

#8
Nitrobenzene-d5
Concen: 0.23 ng
RT: 8.819 min Scan# 727
Delta R.T. -0.000 min
Lab File: BN014449.D
Acq: 26 Apr 2021 18:31

Tgt Ion: 82	Resp:	6770
Ion Ratio	Lower	Upper
82	100	
128	36.2	30.3 45.5
54	48.3	35.8 53.8


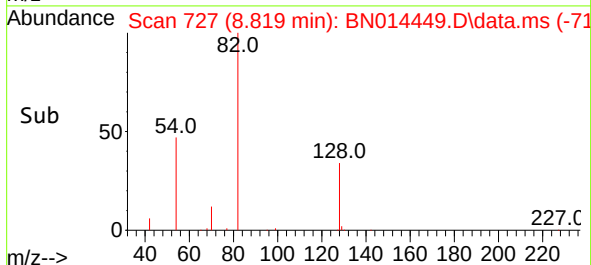
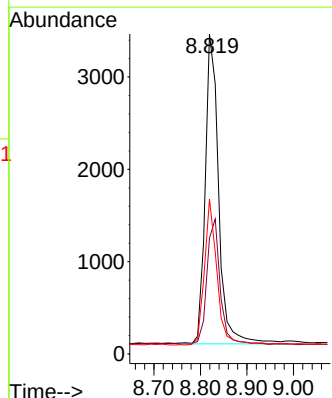
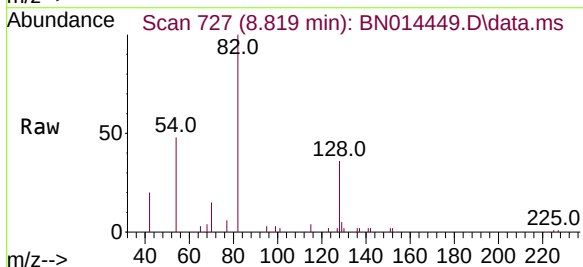


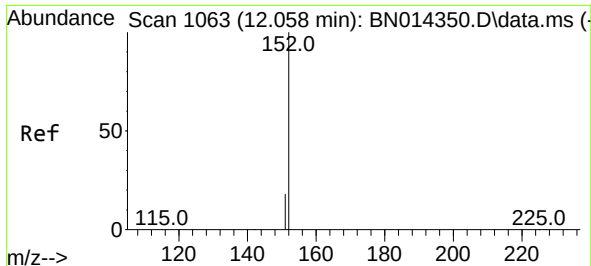

#11
2-Methylnaphthalene-d10
Concen: 0.34 ng
RT: 12.048 min Scan# 1061
Delta R.T. 0.004 min
Lab File: BN014449.D
Acq: 26 Apr 2021 18:31




Instrument :
BNA_N
ClientSampleId :
PB135981BL


Tgt Ion:152 Resp: 17956
Ion Ratio Lower Upper
152 100
151 20.2 16.3 24.5

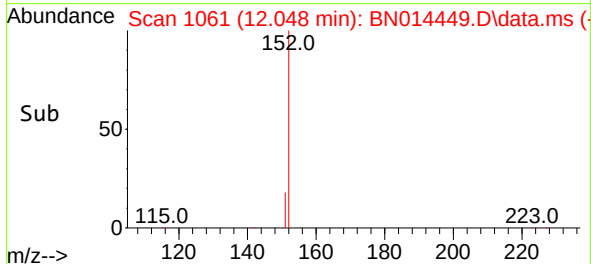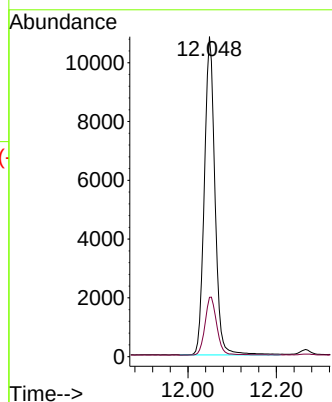

#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.308 min Scan# 1306
Delta R.T. -0.000 min
Lab File: BN014449.D
Acq: 26 Apr 2021 18:31

Tgt Ion:164 Resp: 18930
Ion Ratio Lower Upper
164 100
162 102.2 81.0 121.6
160 48.5 40.7 61.1



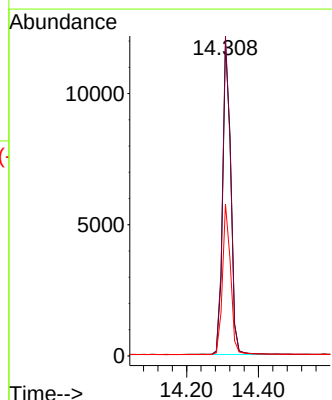
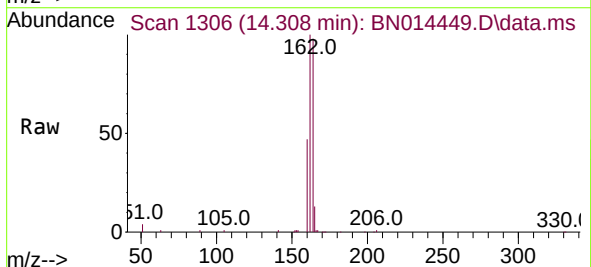


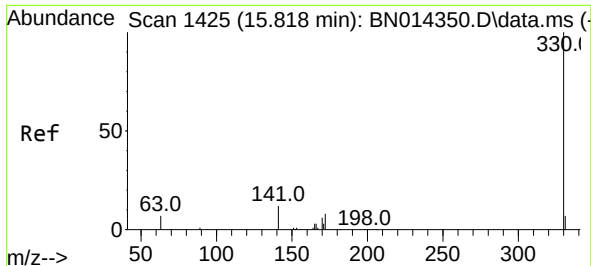

#14
2,4,6-Tribromophenol
Concen: 0.23 ng
RT: 15.805 min Scan# 1424
Delta R.T. -0.000 min
Lab File: BN014449.D
Acq: 26 Apr 2021 18:31




Instrument :
BNA_N
ClientSampleId :
PB135981BL


Tgt Ion:330 Resp: 1414
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 36.7 26.2 39.2

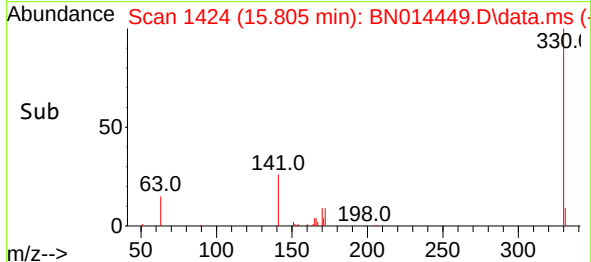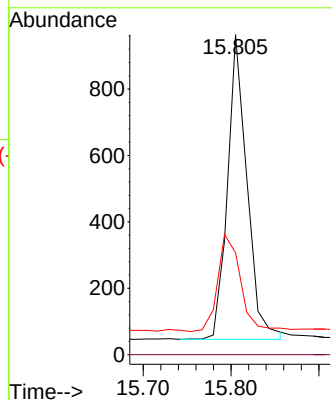

#15
2-Fluorobiphenyl
Concen: 0.34 ng
RT: 12.938 min Scan# 1198
Delta R.T. 0.013 min
Lab File: BN014449.D
Acq: 26 Apr 2021 18:31

Tgt Ion:172 Resp: 25707
Ion Ratio Lower Upper
172 100
171 33.3 28.2 42.2
170 22.0 19.6 29.4


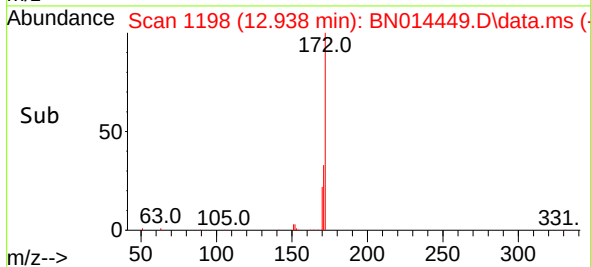
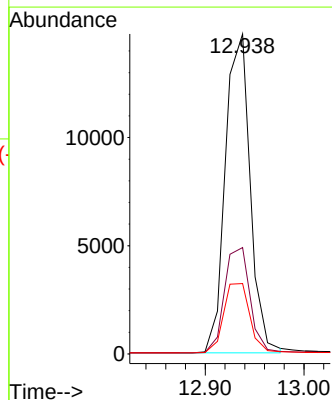
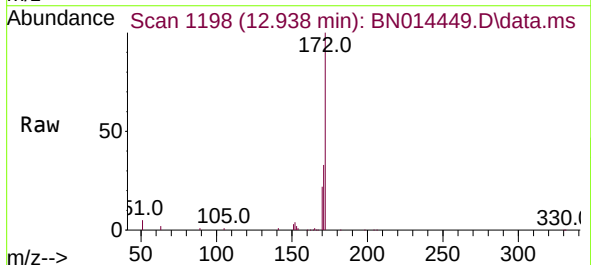


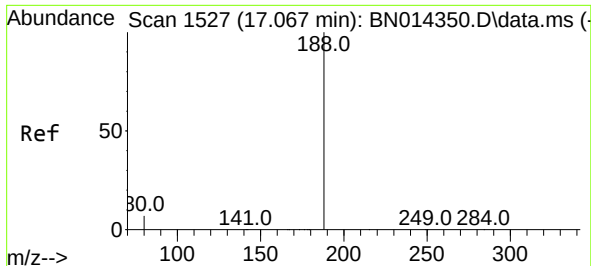

#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.055 min Scan# 1526
Delta R.T. -0.000 min
Lab File: BN014449.D
Acq: 26 Apr 2021 18:31




Instrument :
BNA_N
ClientSampleId :
PB135981BL


Tgt Ion:188 Resp: 38950
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 10.7 6.2 9.4#

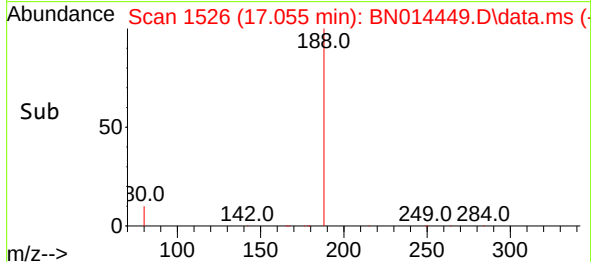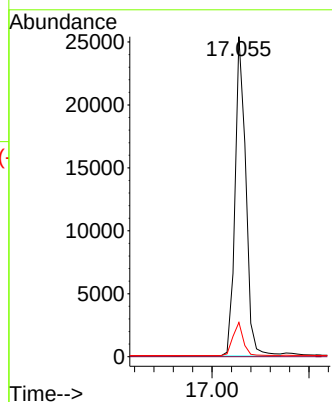

#27
Fluoranthene-d10
Concen: 0.29 ng
RT: 19.099 min Scan# 1823
Delta R.T. -0.000 min
Lab File: BN014449.D
Acq: 26 Apr 2021 18:31

Tgt Ion:212 Resp: 30210
Ion Ratio Lower Upper
212 100
106 12.8 9.7 14.5
104 6.9 5.4 8.0


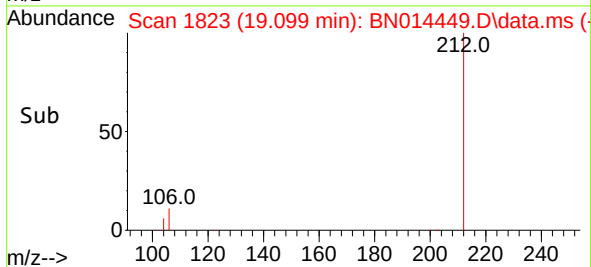
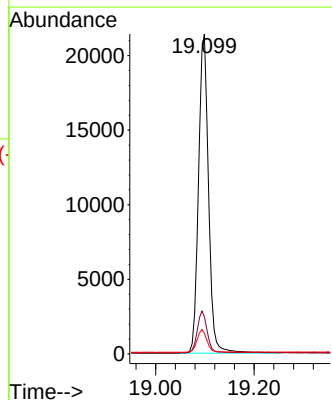
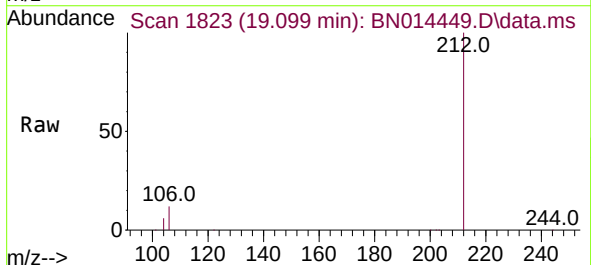


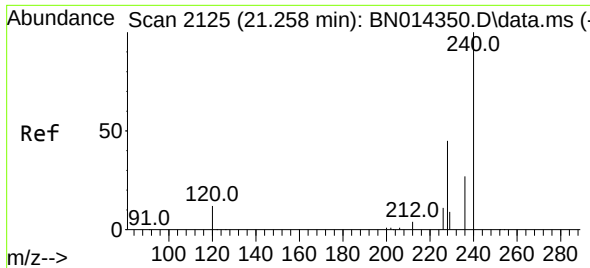

#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.261 min Scan# 2124
Delta R.T. -0.000 min
Lab File: BN014449.D
Acq: 26 Apr 2021 18:31




Instrument :
BNA_N
ClientSampleId :
PB135981BL


Tgt Ion:240 Resp: 33138
Ion Ratio Lower Upper
240 100
120 7.6 10.7 16.1#
236 26.0 21.5 32.3

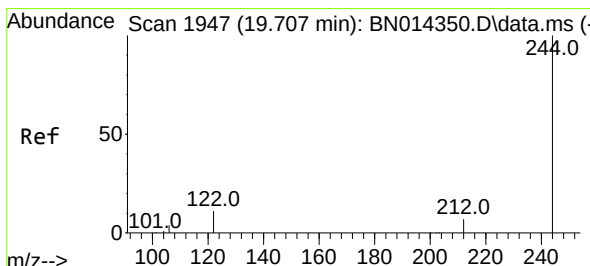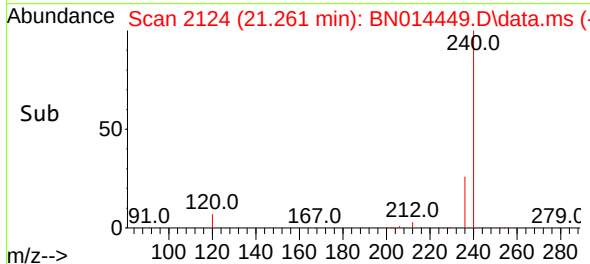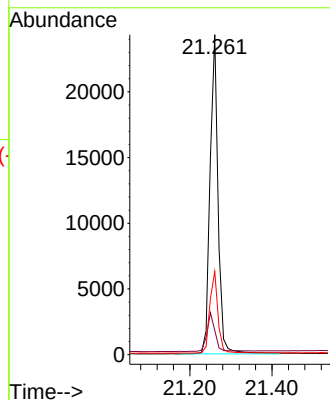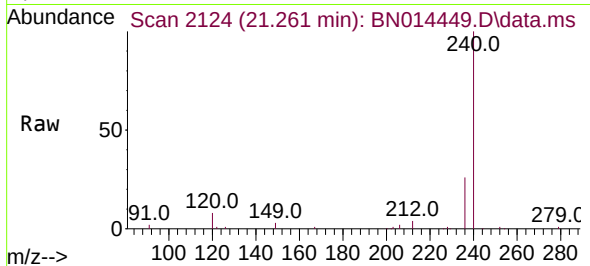

#31
Terphenyl-d14
Concen: 0.38 ng
RT: 19.700 min Scan# 1944
Delta R.T. -0.000 min
Lab File: BN014449.D
Acq: 26 Apr 2021 18:31

Tgt Ion:244 Resp: 26808
Ion Ratio Lower Upper
244 100
212 7.6 6.2 9.4
122 12.8 9.3 13.9


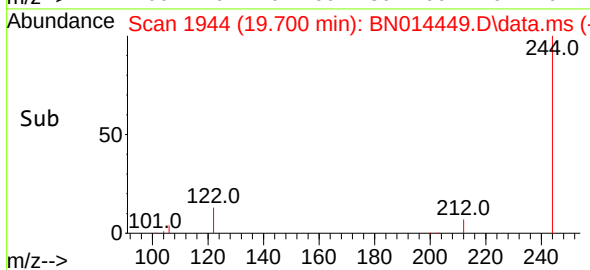
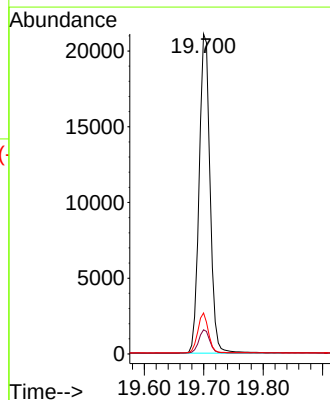
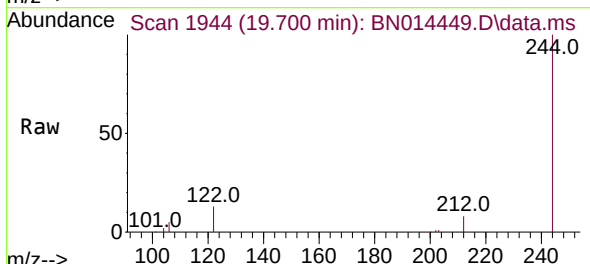


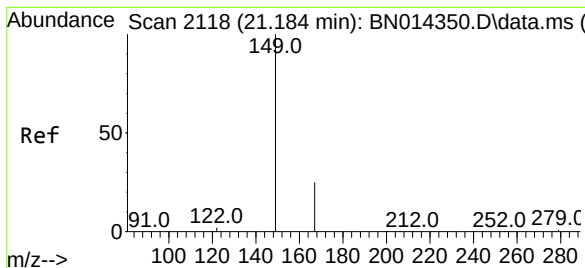

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.03 ng
 RT: 21.186 min Scan# 2117
 Delta R.T. -0.000 min
 Lab File: BN014449.D
 Acq: 26 Apr 2021 18:31

Instrument :
 BNA_N
 ClientSampleId :
 PB135981BL

Tgt Ion:149 Resp: 974
 Ion Ratio Lower Upper
 149 100
 167 25.7 21.3 31.9
 279 9.3 3.1 4.7#

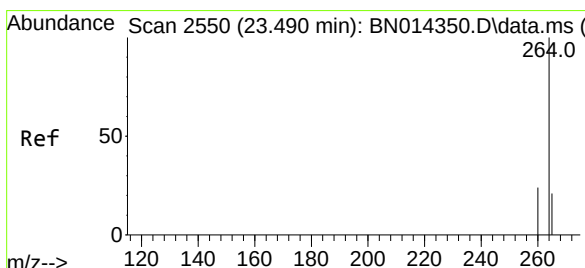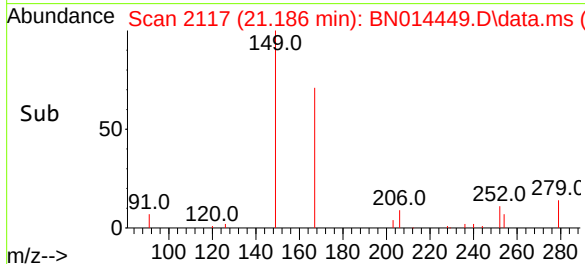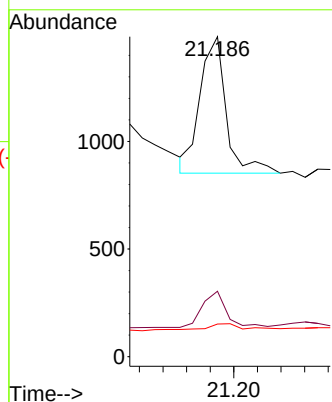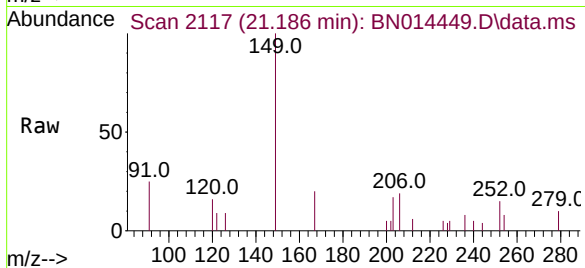

#36
 Perylene-d12
 Concen: 0.40 ng
 RT: 23.482 min Scan# 2546
 Delta R.T. -0.000 min
 Lab File: BN014449.D
 Acq: 26 Apr 2021 18:31

Tgt Ion:264 Resp: 30728
 Ion Ratio Lower Upper
 264 100
 260 24.7 19.8 29.6
 265 38.9 34.4 51.6

