
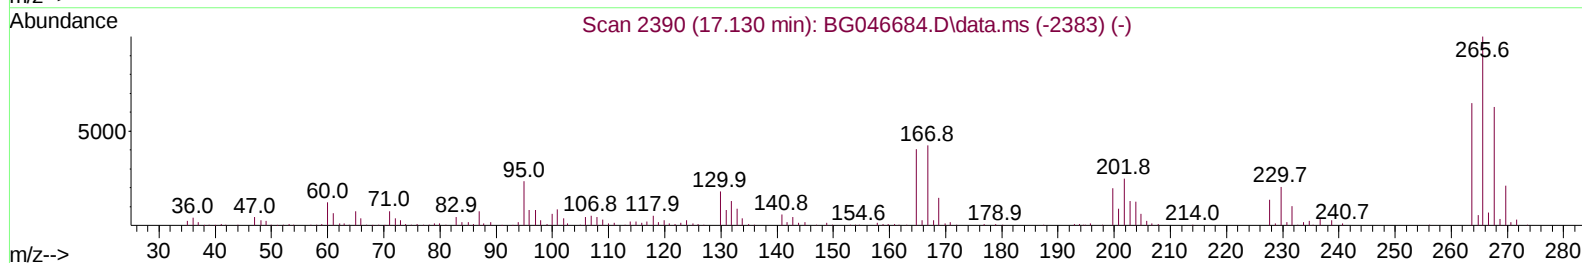
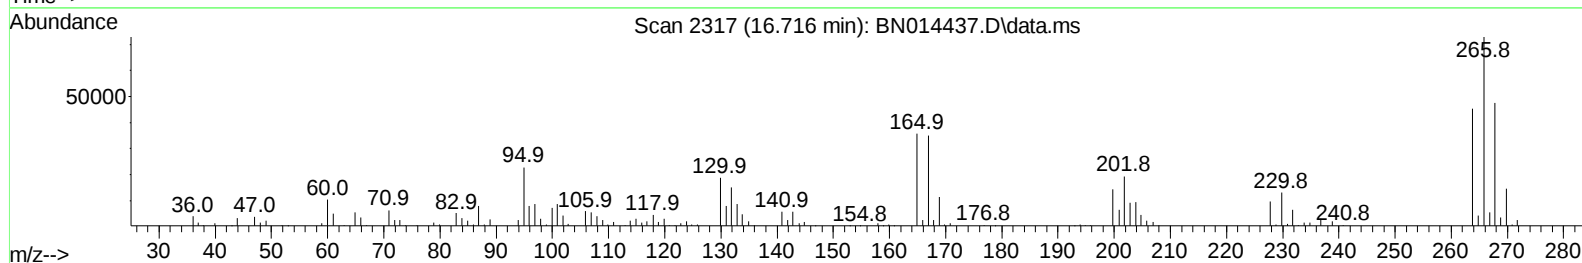


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042621\
Data File : BN014437.D
Acq On : 26 Apr 2021 09:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 26 12:13:05 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 09 09:55:03 2021
Response via : Initial Calibration

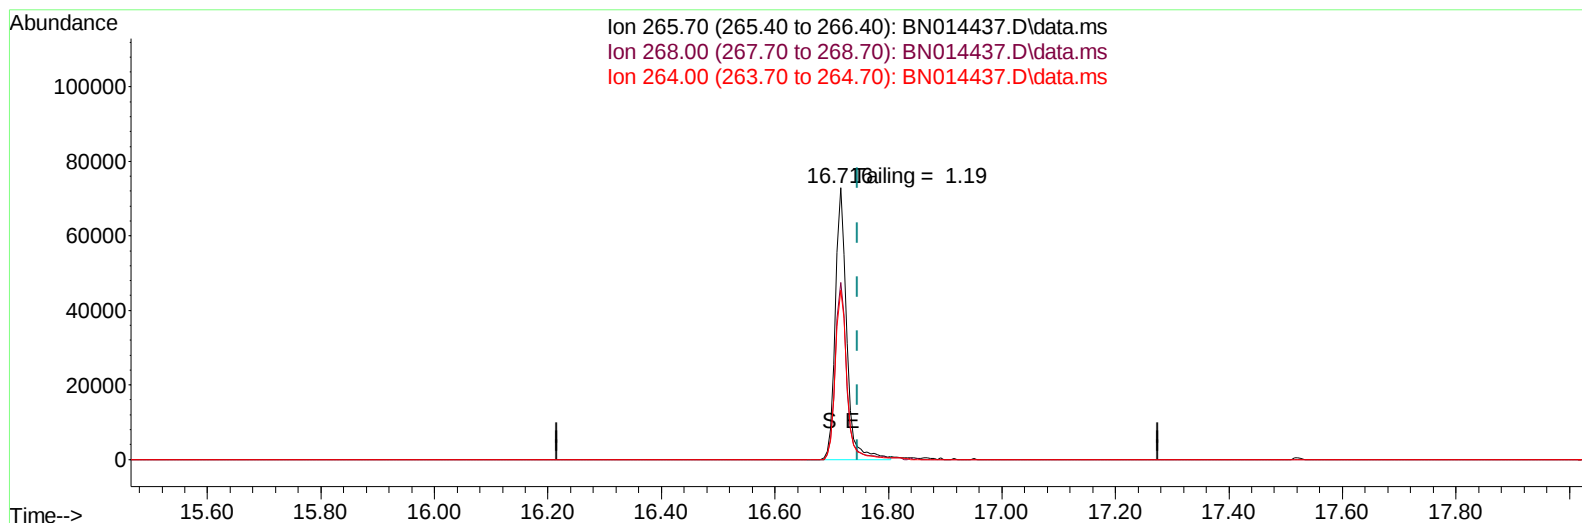




TIC: BN014437.D\data.ms

(70) Pentachlorophenol (C)**16.716min (-0.030) 17075.79 ng****response 102917**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.17
264.00	61.60	62.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042621\
Data File : BN014437.D
Acq On : 26 Apr 2021 09:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 26 12:13:05 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 09 09:55:03 2021
Response via : Initial Calibration

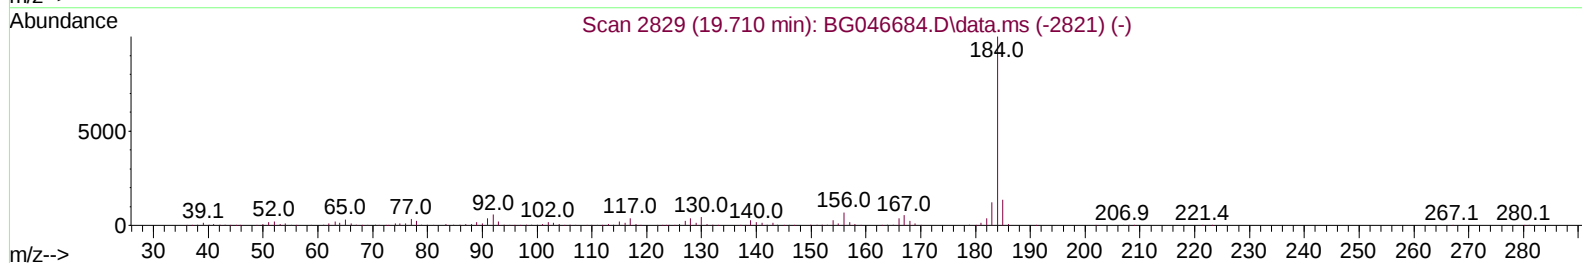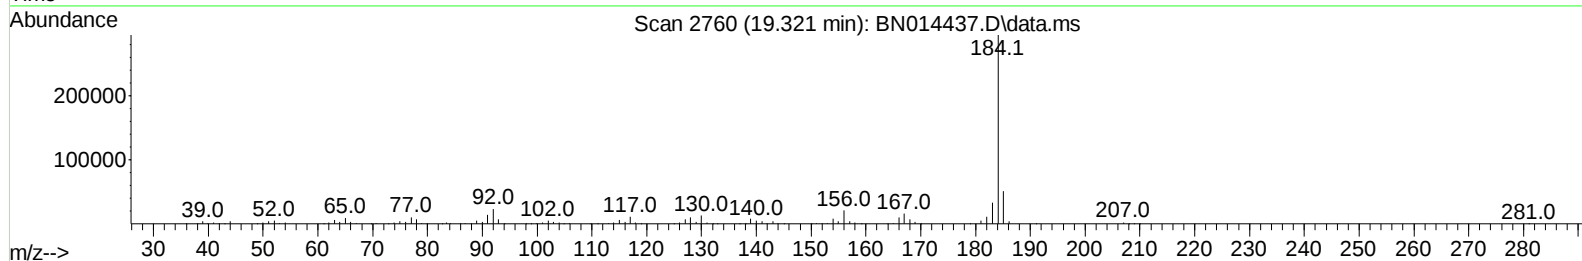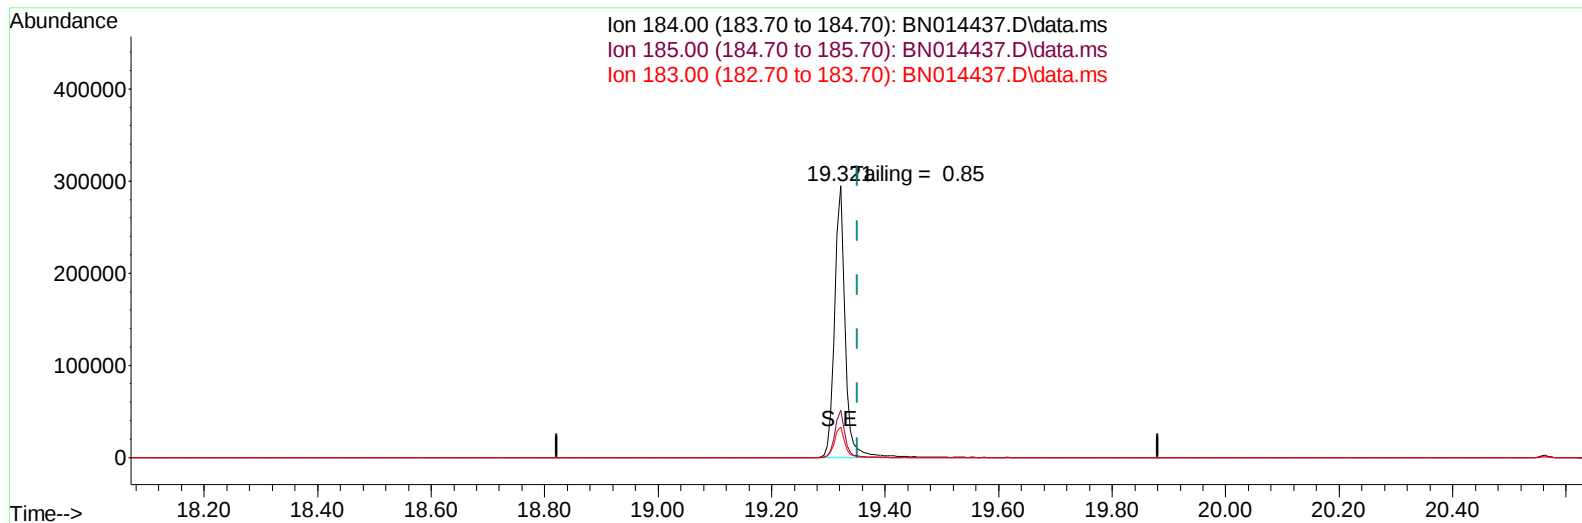

TIC: BN014437.D\data.ms

(77) Benzidine**19.321min (-0.030) 5970.62 ng****response 375455**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	17.36
183.00	13.20	11.18
0.00	0.00	0.00