
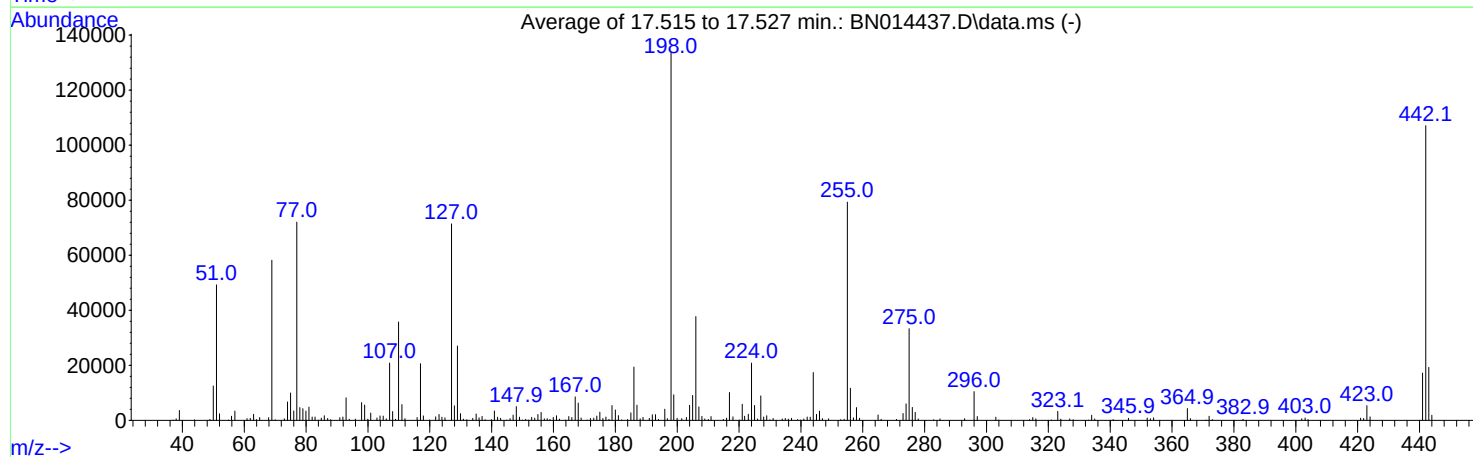


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042621\
 Data File : BN014437.D
 Acq On : 26 Apr 2021 09:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN042221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 27 11:43:13 2021

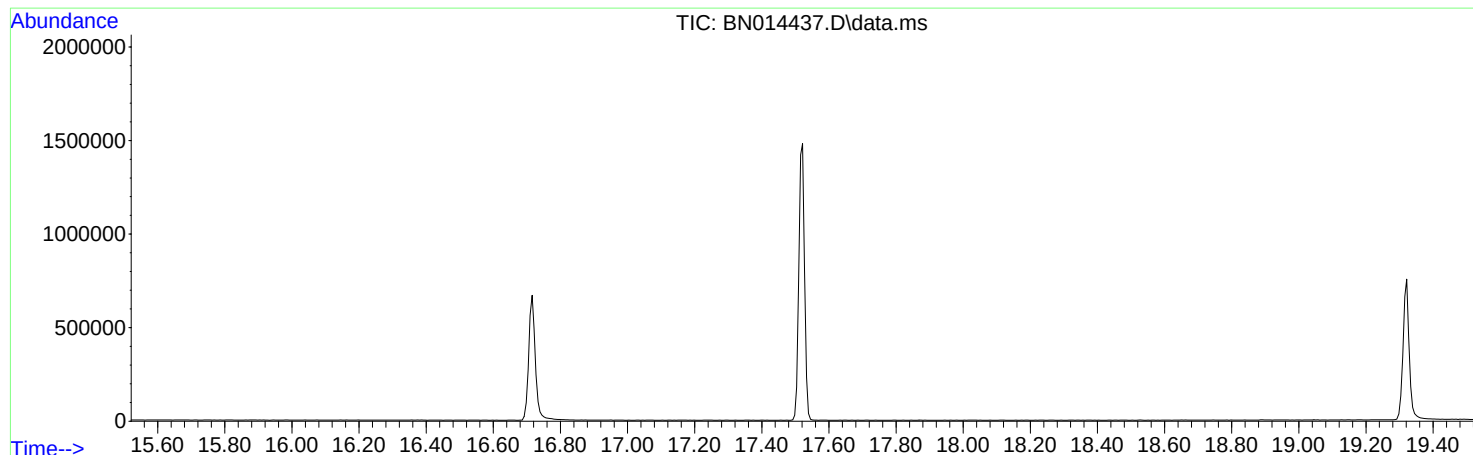




AutoFind: Scans 2453, 2454, 2455; Background Corrected with Scan 2446

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.8	49253	PASS
68	69	0.00	2	1.7	986	PASS
69	198	0.00	100	43.5	58205	PASS
70	69	0.00	2	0.4	243	PASS
127	198	10	80	53.4	71421	PASS
197	198	0.00	2	0.5	669	PASS
198	198	100	100	100.0	133677	PASS
199	198	5	9	7.0	9326	PASS
275	198	10	60	24.9	33301	PASS
365	198	1	100	3.2	4302	PASS
441	198	0.01	100	12.9	17194	PASS
442	442	50	100	100.0	107085	PASS
443	442	15	24	18.0	19259	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042621\
Data File : BN014437.D
Acq On : 26 Apr 2021 09:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 26 12:13:05 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 09 09:55:03 2021
Response via : Initial Calibration

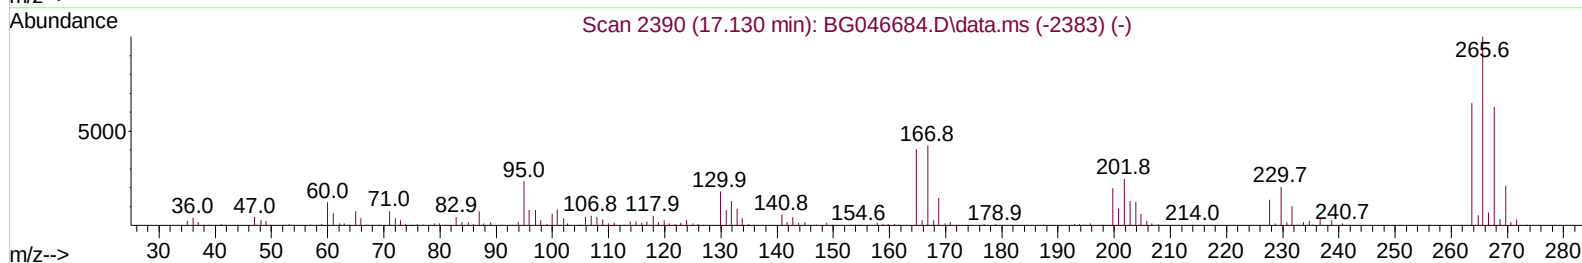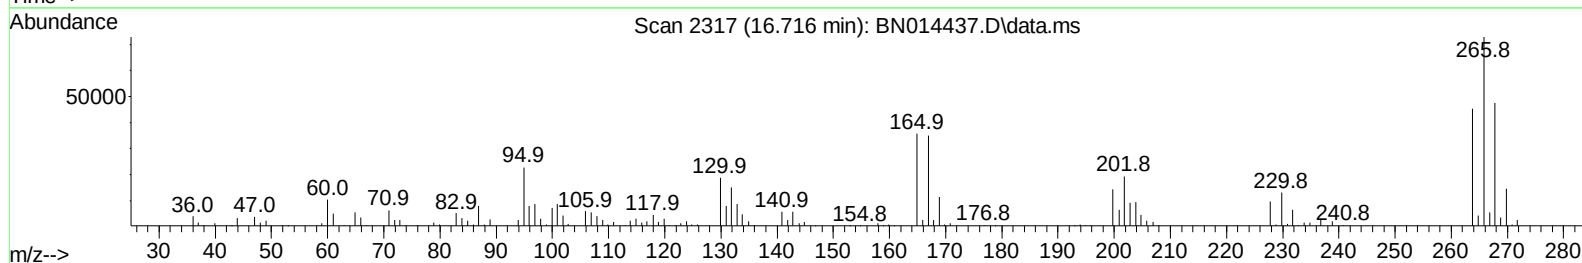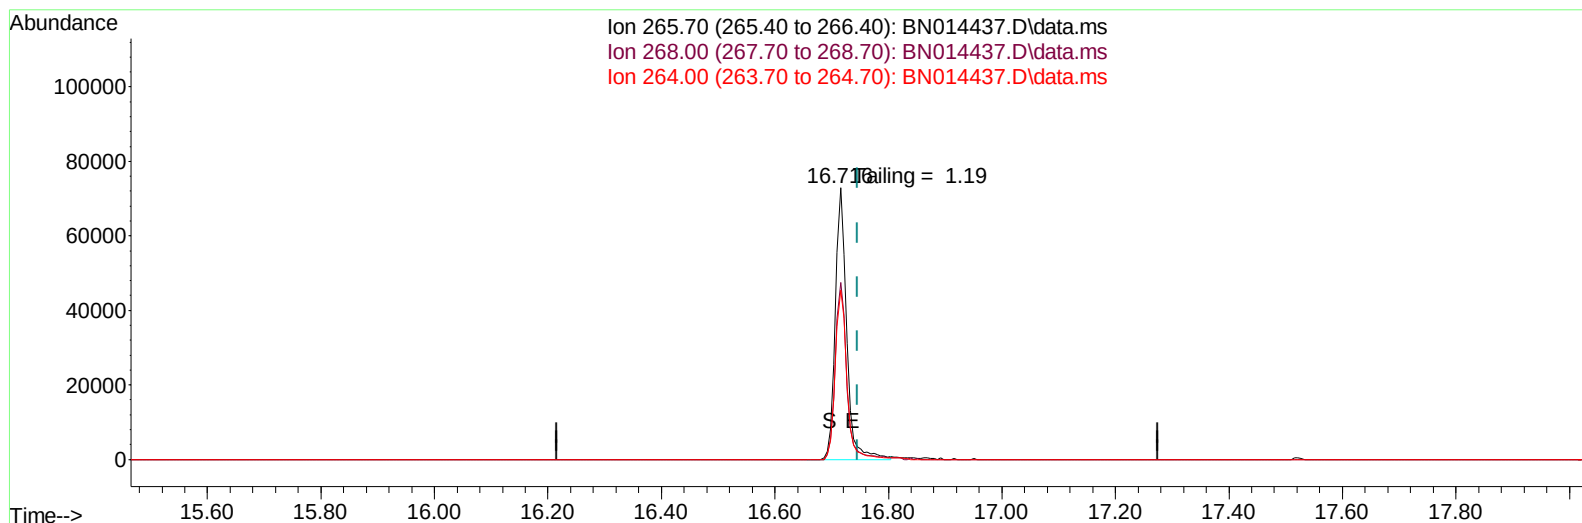

TIC: BN014437.D\data.ms

(70) Pentachlorophenol (C)

16.716min (-0.030) 17075.79 ng




response 102917

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.17
264.00	61.60	62.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042621\
Data File : BN014437.D
Acq On : 26 Apr 2021 09:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 26 12:13:05 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 09 09:55:03 2021
Response via : Initial Calibration

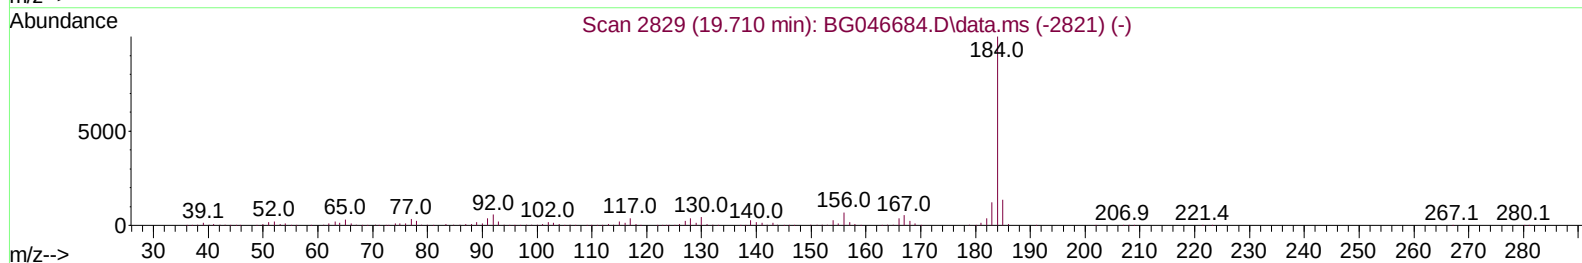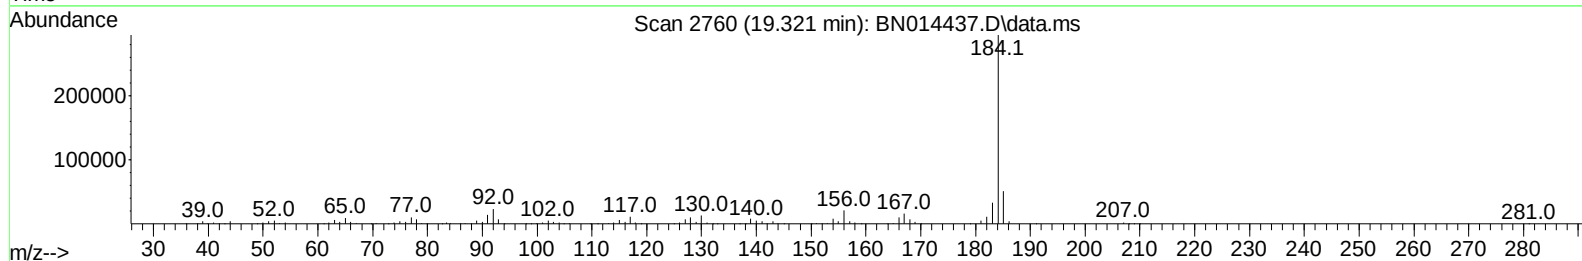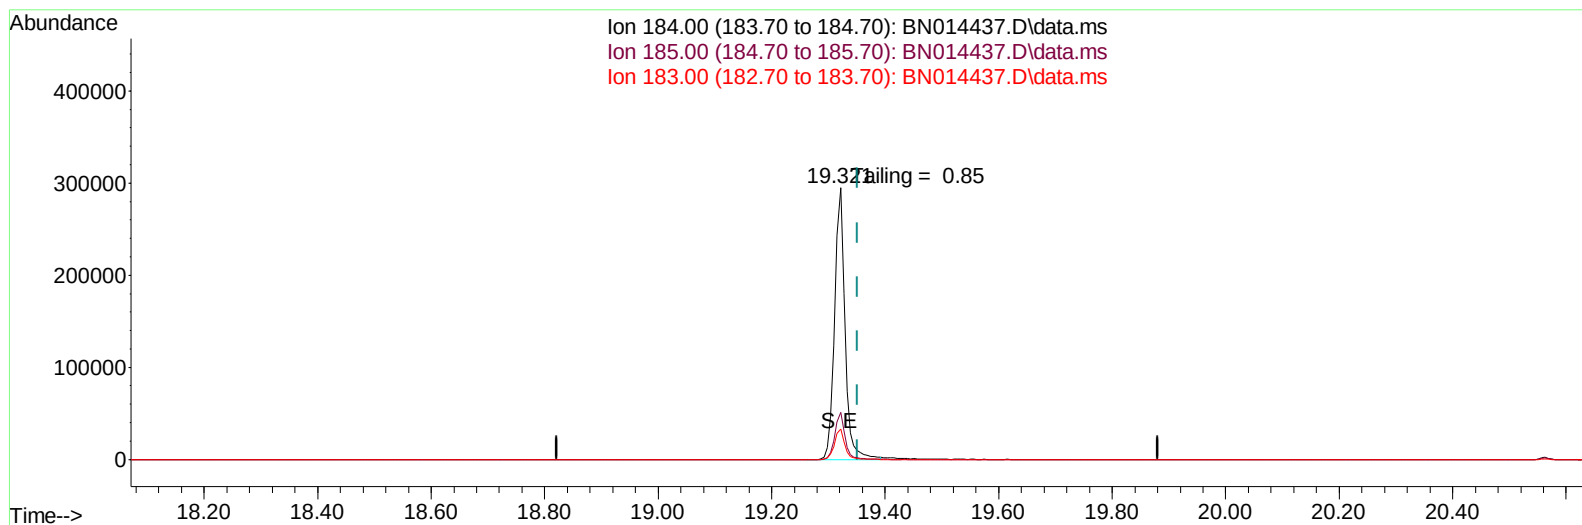

TIC: BN014437.D\data.ms

(77) Benzidine

19.321min (-0.030) 5970.62 ng

response 375455

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	17.36
183.00	13.20	11.18
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/26/2021	BNA_N	<u>BN014437.D</u>
Compound Name	Response	Retention Time
DDT	339644	20.562
DDD	16713	20.121
DDE	1166	19.61
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17879	357523	5.00