

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042623\
 Data File : BN025145.D
 Acq On : 26 Apr 2023 14:30
 Operator : CG/JU
 Sample : 02373-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB9D7

Quant Time: Apr 27 00:13:43 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 26 15:32:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.917	152	7402	0.400	ng/ul	0.00
4) Naphthalene-d8	10.725	136	23847	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.560	164	14911	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.308	188	32125	0.400	ng/ul	0.00
17) Chrysene-d12	21.507	240	24745	0.400	ng/ul	0.00
23) Perylene-d12	23.931	264	24717	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	37904	4.946	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.320	152	10765	0.352	ng/ul	0.00
18) Fluoranthene-d10	19.339	212	29235	0.448	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.706	202	4820	0.052	ng/ul#	1
26) Benzo(a)pyrene	23.776	252	8780	0.106	ng/ul#	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042623\
Data File : BN025145.D
Acq On : 26 Apr 2023 14:30
Operator : CG/JU
Sample : 02373-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB9D7

Quant Time: Apr 27 00:13:43 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 26 15:32:47 2023
Response via : Initial Calibration

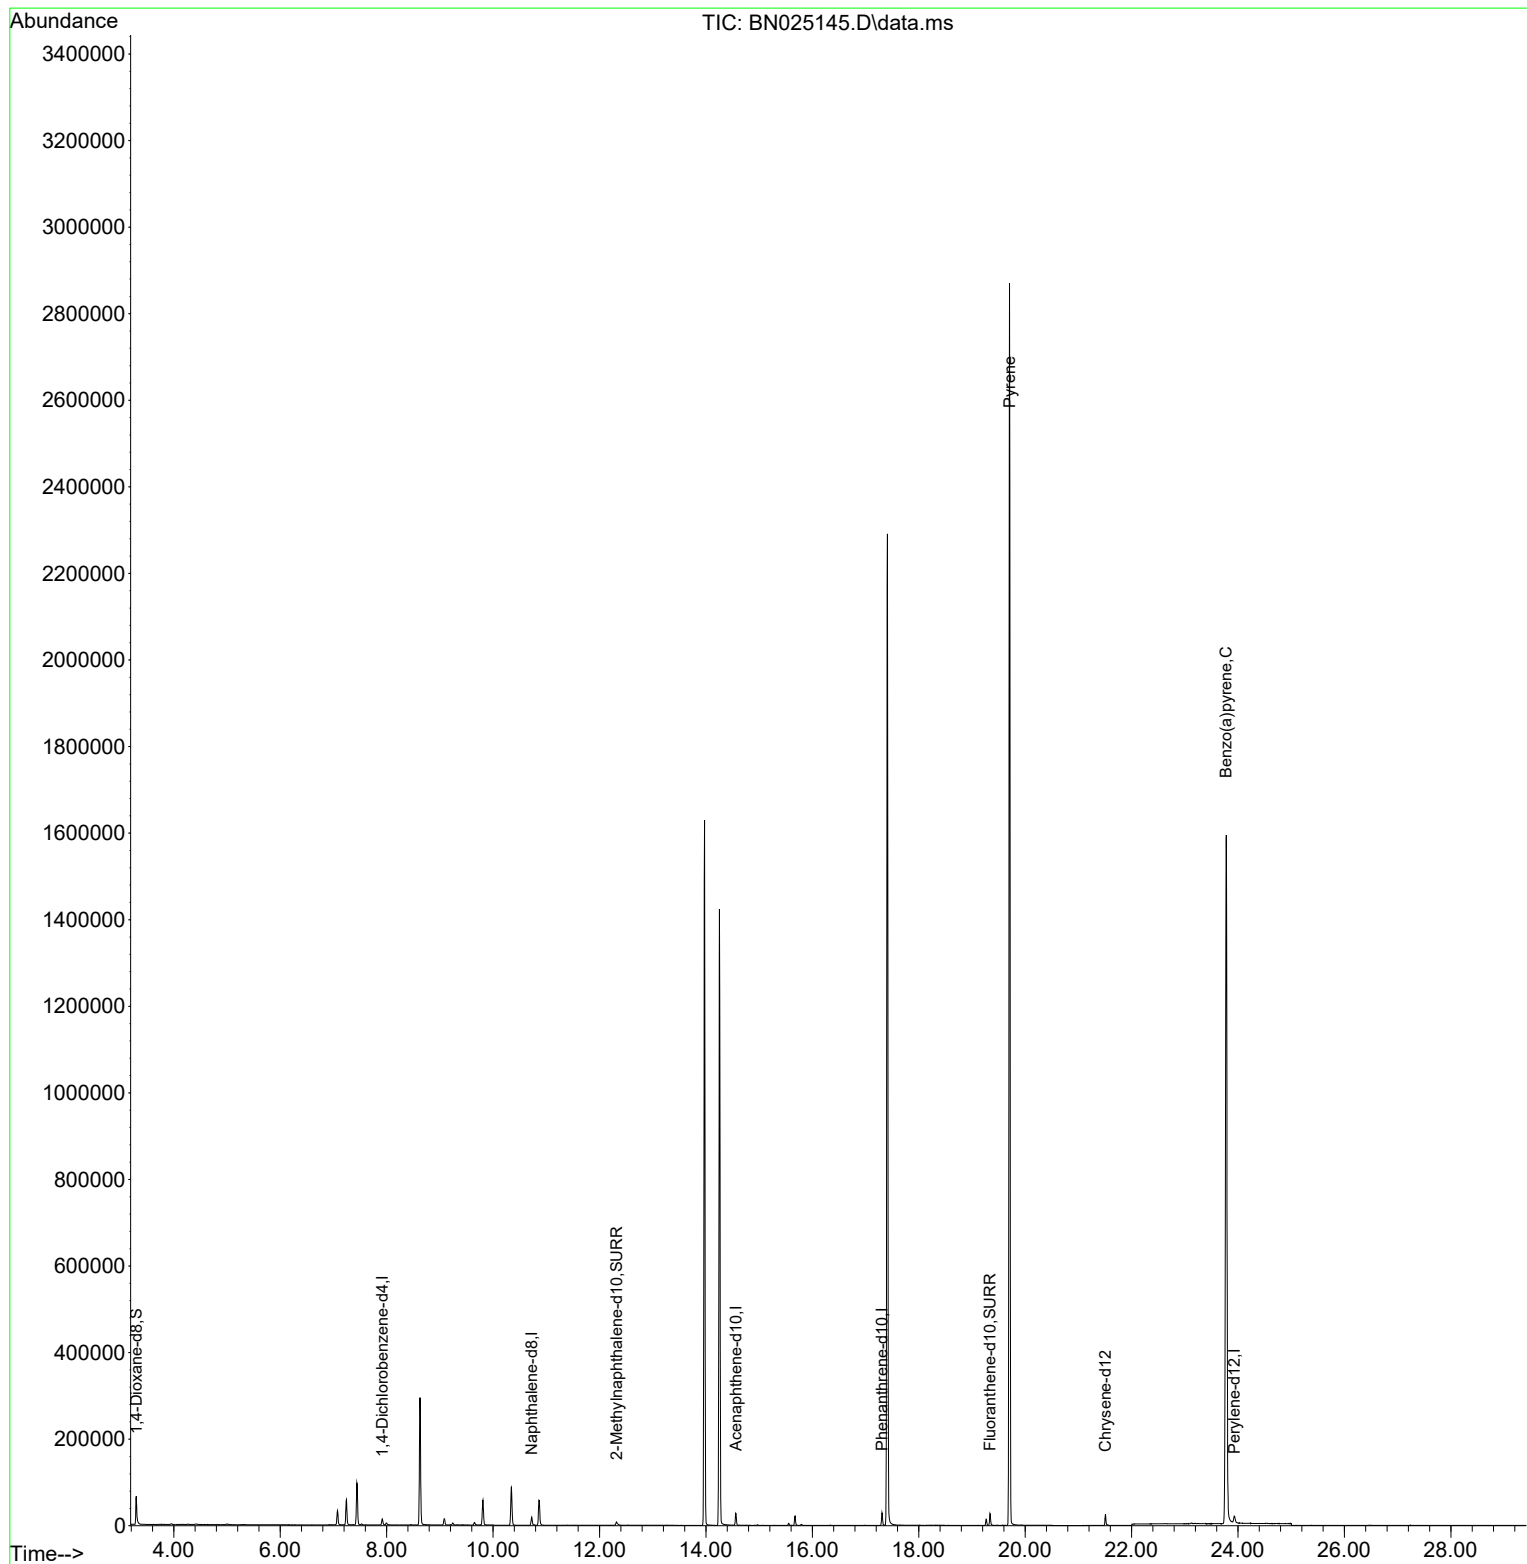

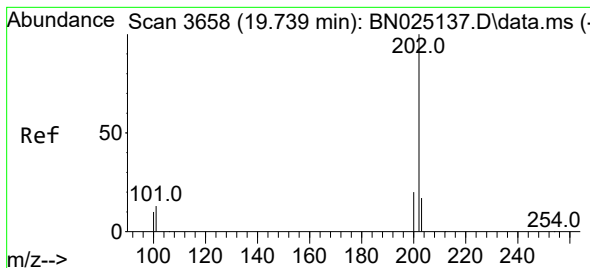

#20

Pyrene

Concen: 0.052 ng/ul

RT: 19.706 min Scan# 3

Delta R.T. -0.033 min

Lab File: BN025145.D

Acq: 26 Apr 2023 14:30

Instrument :

BNA_N

ClientSampleId :

CB9D7





Tgt Ion:202 Resp: 4820

Ion Ratio Lower Upper

202 100

101 173.6 11.3 16.9#

100 1278.7 9.2 13.8#

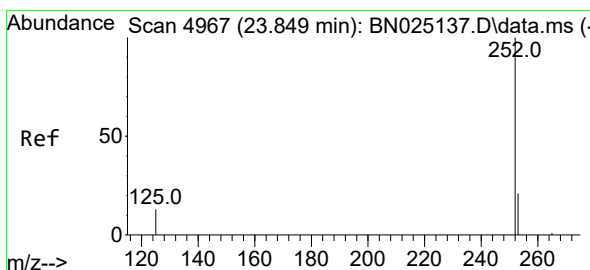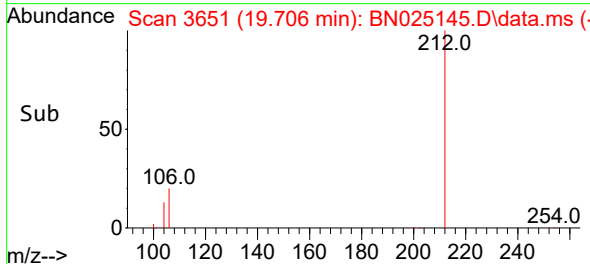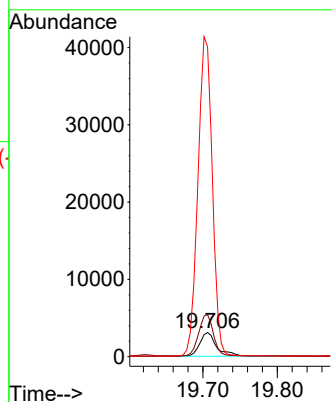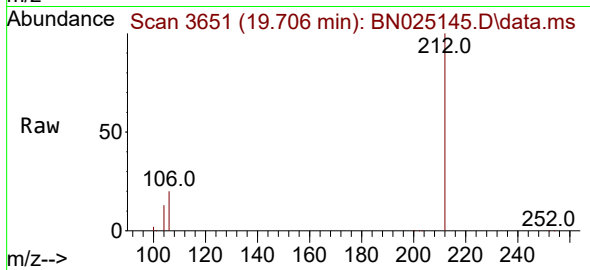

#26

Benzo(a)pyrene

Concen: 0.106 ng/ul

RT: 23.776 min Scan# 4942

Delta R.T. -0.073 min

Lab File: BN025145.D

Acq: 26 Apr 2023 14:30

Tgt Ion:252 Resp: 8780

Ion Ratio Lower Upper

252 100

253 44.5 21.4 32.2#

125 36.7 14.6 22.0#

