

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042623\
 Data File : BN025150.D
 Acq On : 26 Apr 2023 17:29
 Operator : CG/JU
 Sample : PB152353BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK353

Quant Time: Apr 27 00:28:50 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 26 15:32:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.917	152	7214	0.400	ng/ul	0.00
4) Naphthalene-d8	10.726	136	23887	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.562	164	14658	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.310	188	31186	0.400	ng/ul	0.00
17) Chrysene-d12	21.509	240	22729	0.400	ng/ul	0.00
23) Perylene-d12	23.947	264	22525	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	55262	7.398	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.321	152	11959	0.390	ng/ul	0.00
18) Fluoranthene-d10	19.341	212	26984	0.450	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.556	166	4388	0.085	ng/ul#	13
20) Pyrene	19.703	202	4190	0.050	ng/ul#	1
26) Benzo(a)pyrene	23.789	252	8186	0.108	ng/ul#	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042623\
Data File : BN025150.D
Acq On : 26 Apr 2023 17:29
Operator : CG/JU
Sample : PB152353BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK353

Quant Time: Apr 27 00:28:50 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 26 15:32:47 2023
Response via : Initial Calibration




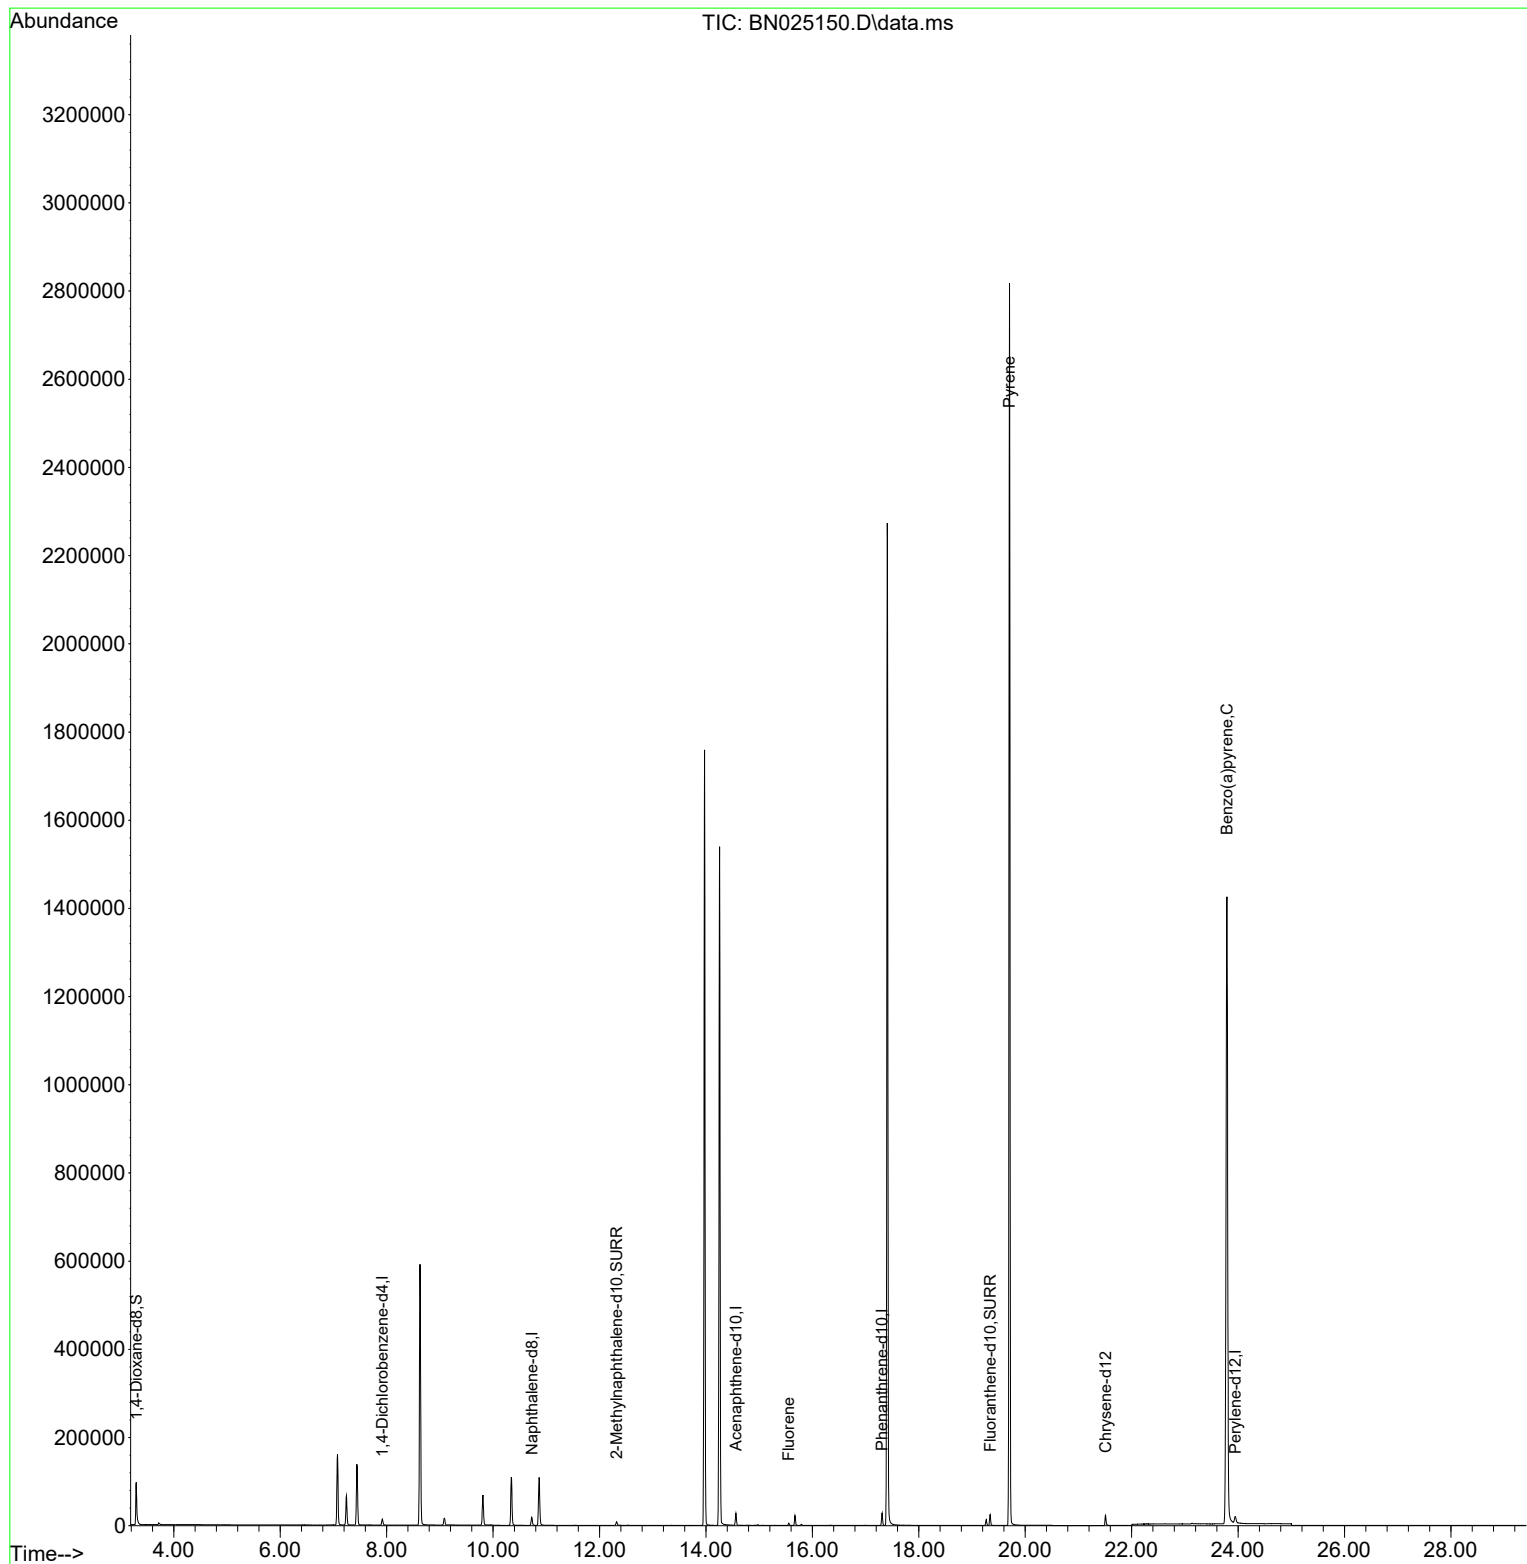


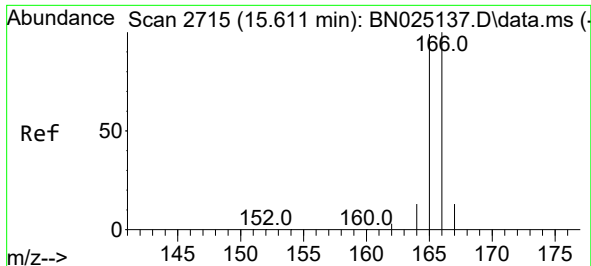

#12
Fluorene
Concen: 0.085 ng/ul
RT: 15.556 min Scan# 21
Delta R.T. -0.054 min
Lab File: BN025150.D
Acq: 26 Apr 2023 17:29




Instrument :
BNA_N
ClientSampleId :
SBLK353


Tgt Ion:166 Resp: 4388
Ion Ratio Lower Upper
166 100
165 7.0 78.1 117.1#
167 34.6 11.0 16.6#

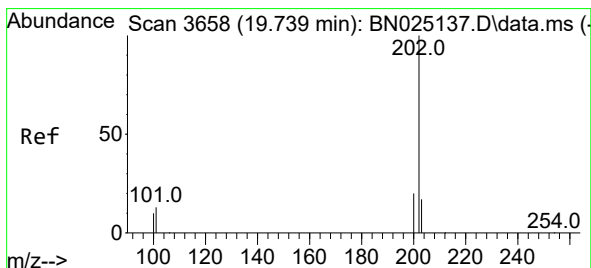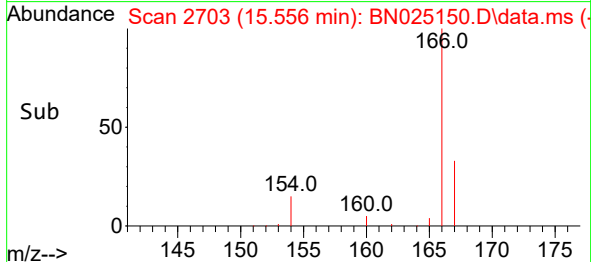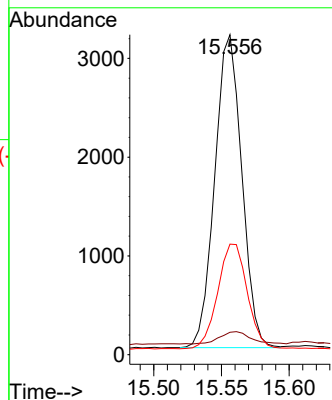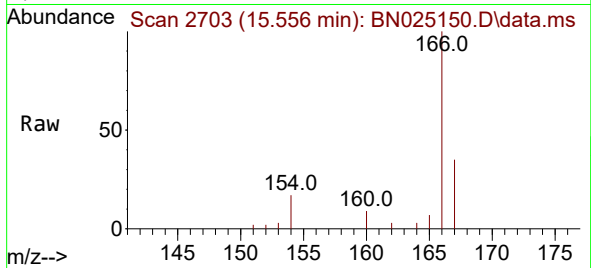

#20
Pyrene
Concen: 0.050 ng/ul
RT: 19.703 min Scan# 3650
Delta R.T. -0.036 min
Lab File: BN025150.D
Acq: 26 Apr 2023 17:29


Tgt Ion:202 Resp: 4190
Ion Ratio Lower Upper
202 100
101 173.9 11.3 16.9#
100 1322.7 9.2 13.8#

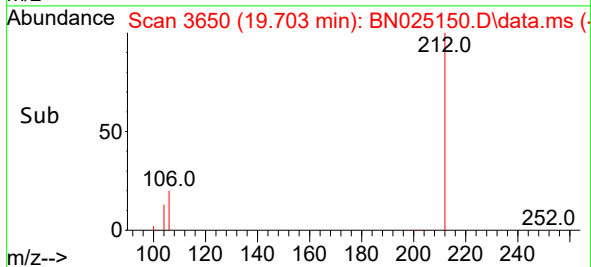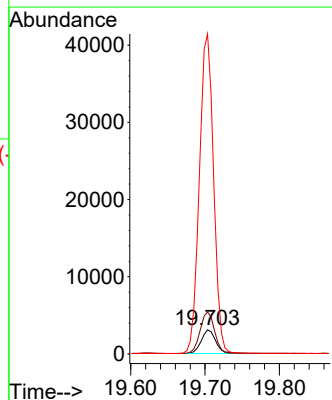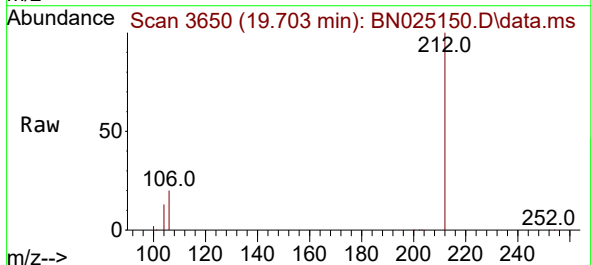

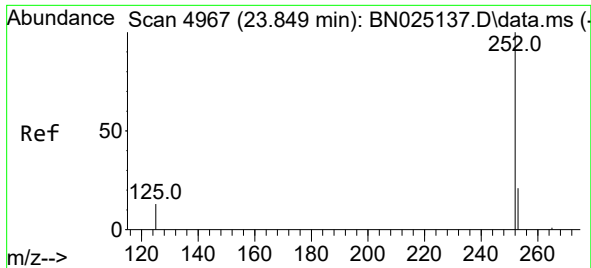

#26
 Benzo(a)pyrene
 Concen: 0.108 ng/ul
 RT: 23.789 min Scan# 4946
 Delta R.T. -0.060 min
 Lab File: BN025150.D
 Acq: 26 Apr 2023 17:29

Instrument :
 BNA_N
 ClientSampleId :
 SBLK353

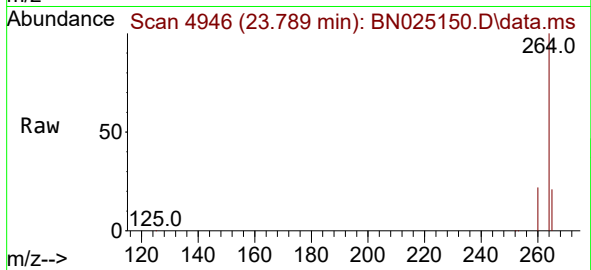

Tgt Ion:252 Resp: 8186
 Ion Ratio Lower Upper
 252 100
 253 43.8 21.4 32.2#
 125 35.9 14.6 22.0#

