

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042623\
 Data File : BN025155.D
 Acq On : 26 Apr 2023 20:28
 Operator : CG/JU
 Sample : 02433-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHE40

Quant Time: Apr 27 00:29:24 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 26 15:32:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.917	152	7018	0.400	ng/ul	0.00
4) Naphthalene-d8	10.726	136	23136	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.561	164	14434	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.309	188	31962	0.400	ng/ul	0.00
17) Chrysene-d12	21.506	240	24568	0.400	ng/ul	0.00
23) Perylene-d12	23.926	264	23629	0.400	ng/ul	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	36416	5.011	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.315	152	10950	0.369	ng/ul	0.00
18) Fluoranthene-d10	19.336	212	32530	0.502	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.330	88	1792	0.229	ng/ul#	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042623\
Data File : BN025155.D
Acq On : 26 Apr 2023 20:28
Operator : CG/JU
Sample : 02433-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHE40


Quant Time: Apr 27 00:29:24 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 26 15:32:47 2023
Response via : Initial Calibration

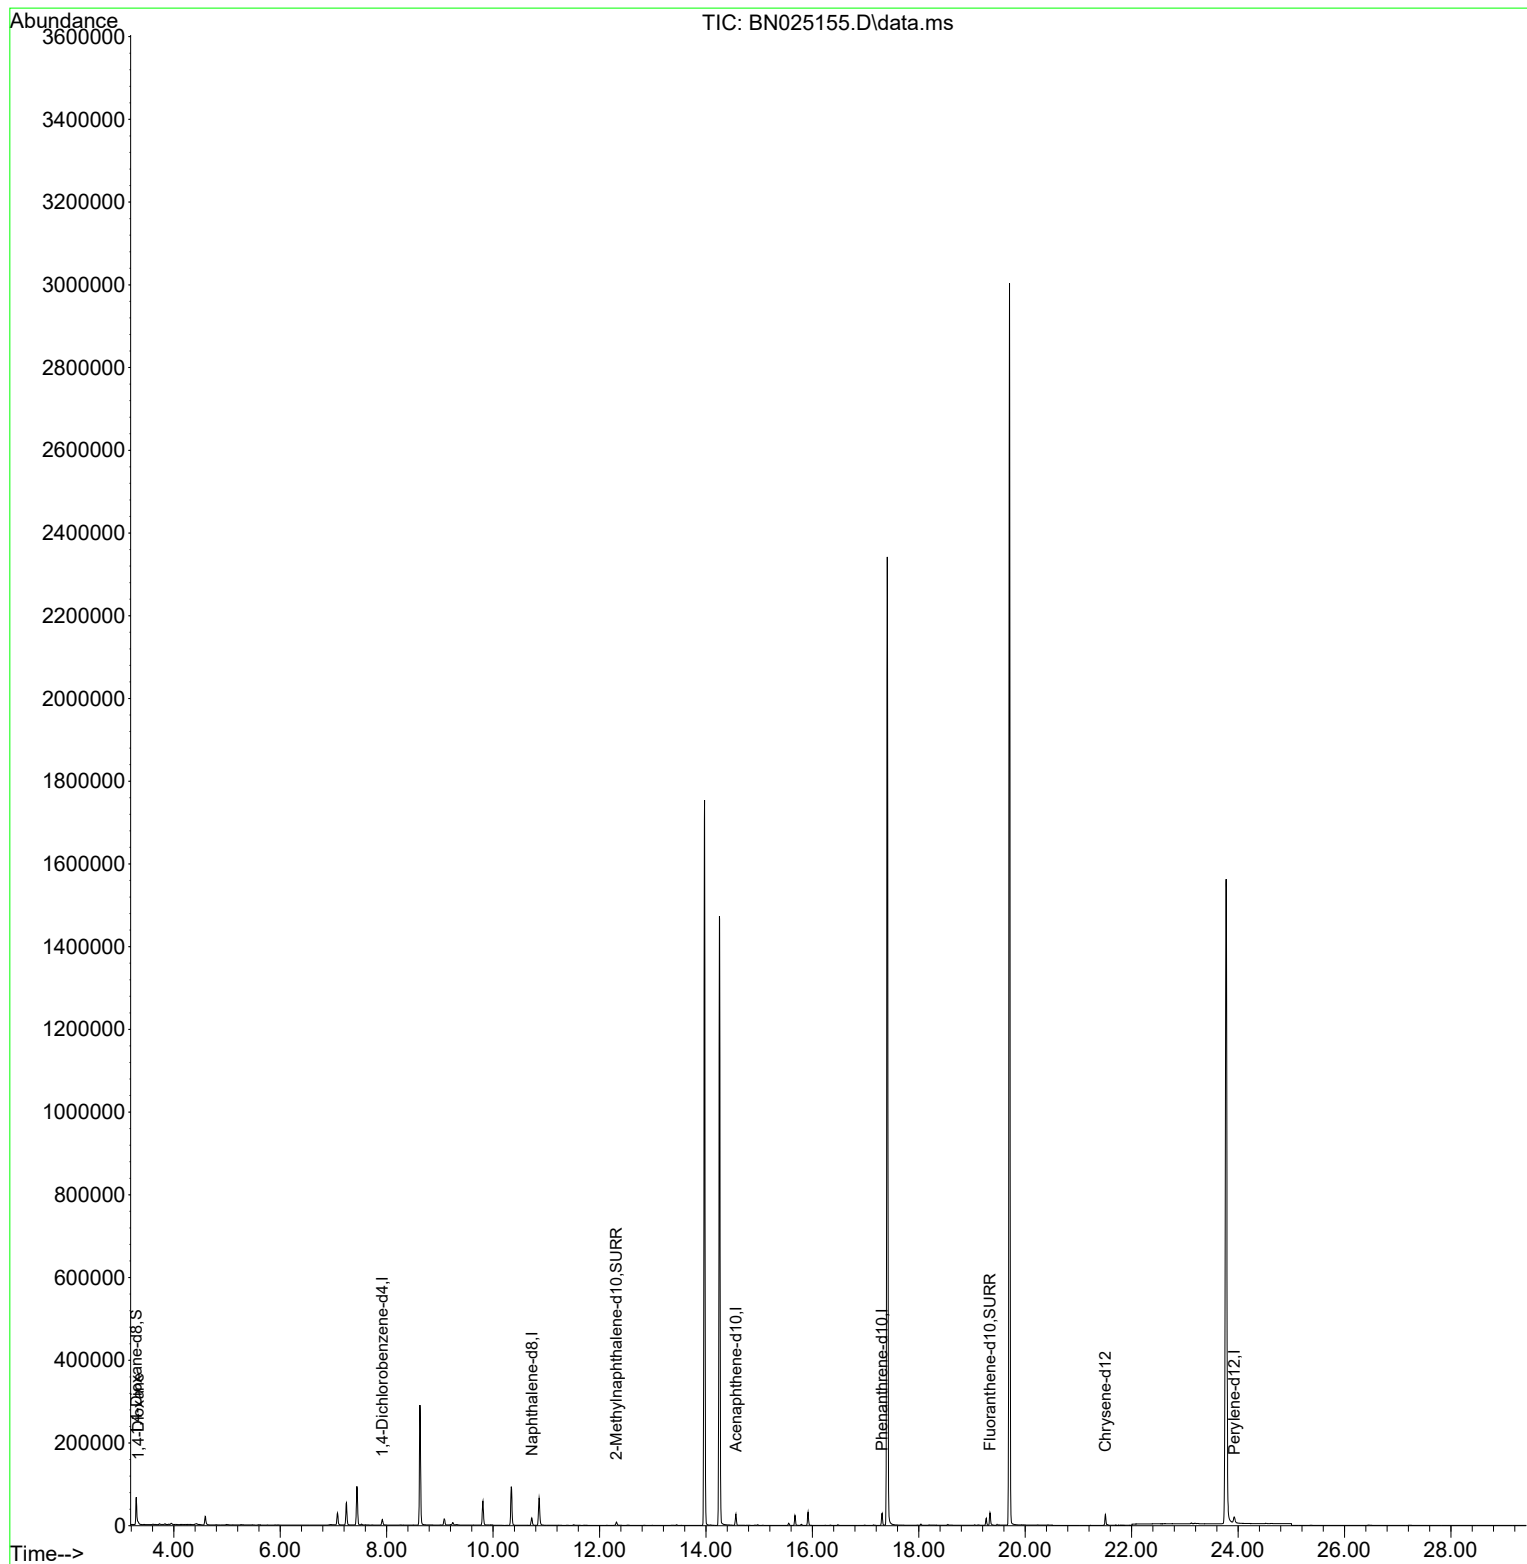

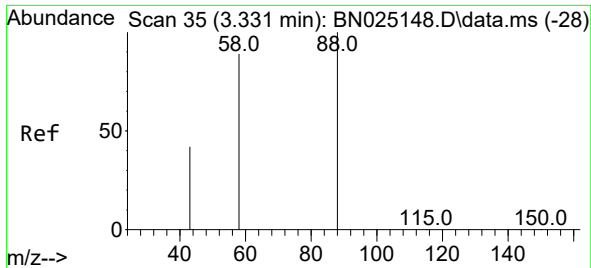

#2
 1,4-Dioxane
 Concen: 0.229 ng/ul
 RT: 3.330 min Scan# 31
 Delta R.T. 0.004 min
 Lab File: BN025155.D
 Acq: 26 Apr 2023 20:28

Instrument :
 BNA_N
 ClientSampleId :
 BHE40

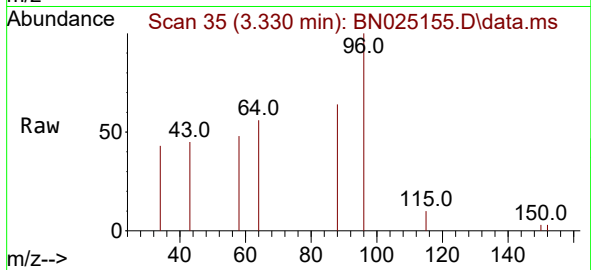

Tgt Ion: 88 Resp: 1792

Ion	Ratio	Lower	Upper
88	100		
43	71.3	37.0	55.4#
58	76.2	56.9	85.3

