

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050123\
 Data File : BN025210.D
 Acq On : 01 May 2023 16:16
 Operator : CG/JU
 Sample : PB152474BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK474

Quant Time: May 02 04:02:32 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 27 15:27:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.913	152	6418	0.400	ng/ul	0.00
4) Naphthalene-d8	10.721	136	21777	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.561	164	13382	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.309	188	27350	0.400	ng/ul	0.00
17) Chrysene-d12	21.506	240	16355	0.400	ng/ul	0.00
23) Perylene-d12	23.941	264	16556	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	43382	6.528	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.316	152	10973	0.392	ng/ul	0.00
18) Fluoranthene-d10	19.340	212	22531	0.522	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.556	166	3770	0.080	ng/ul#	14
20) Pyrene	19.703	202	3401	0.056	ng/ul#	1
26) Benzo(a)pyrene	23.791	252	5707	0.103	ng/ul#	59


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050123\
Data File : BN025210.D
Acq On : 01 May 2023 16:16
Operator : CG/JU
Sample : PB152474BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK474

Quant Time: May 02 04:02:32 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 27 15:27:43 2023
Response via : Initial Calibration




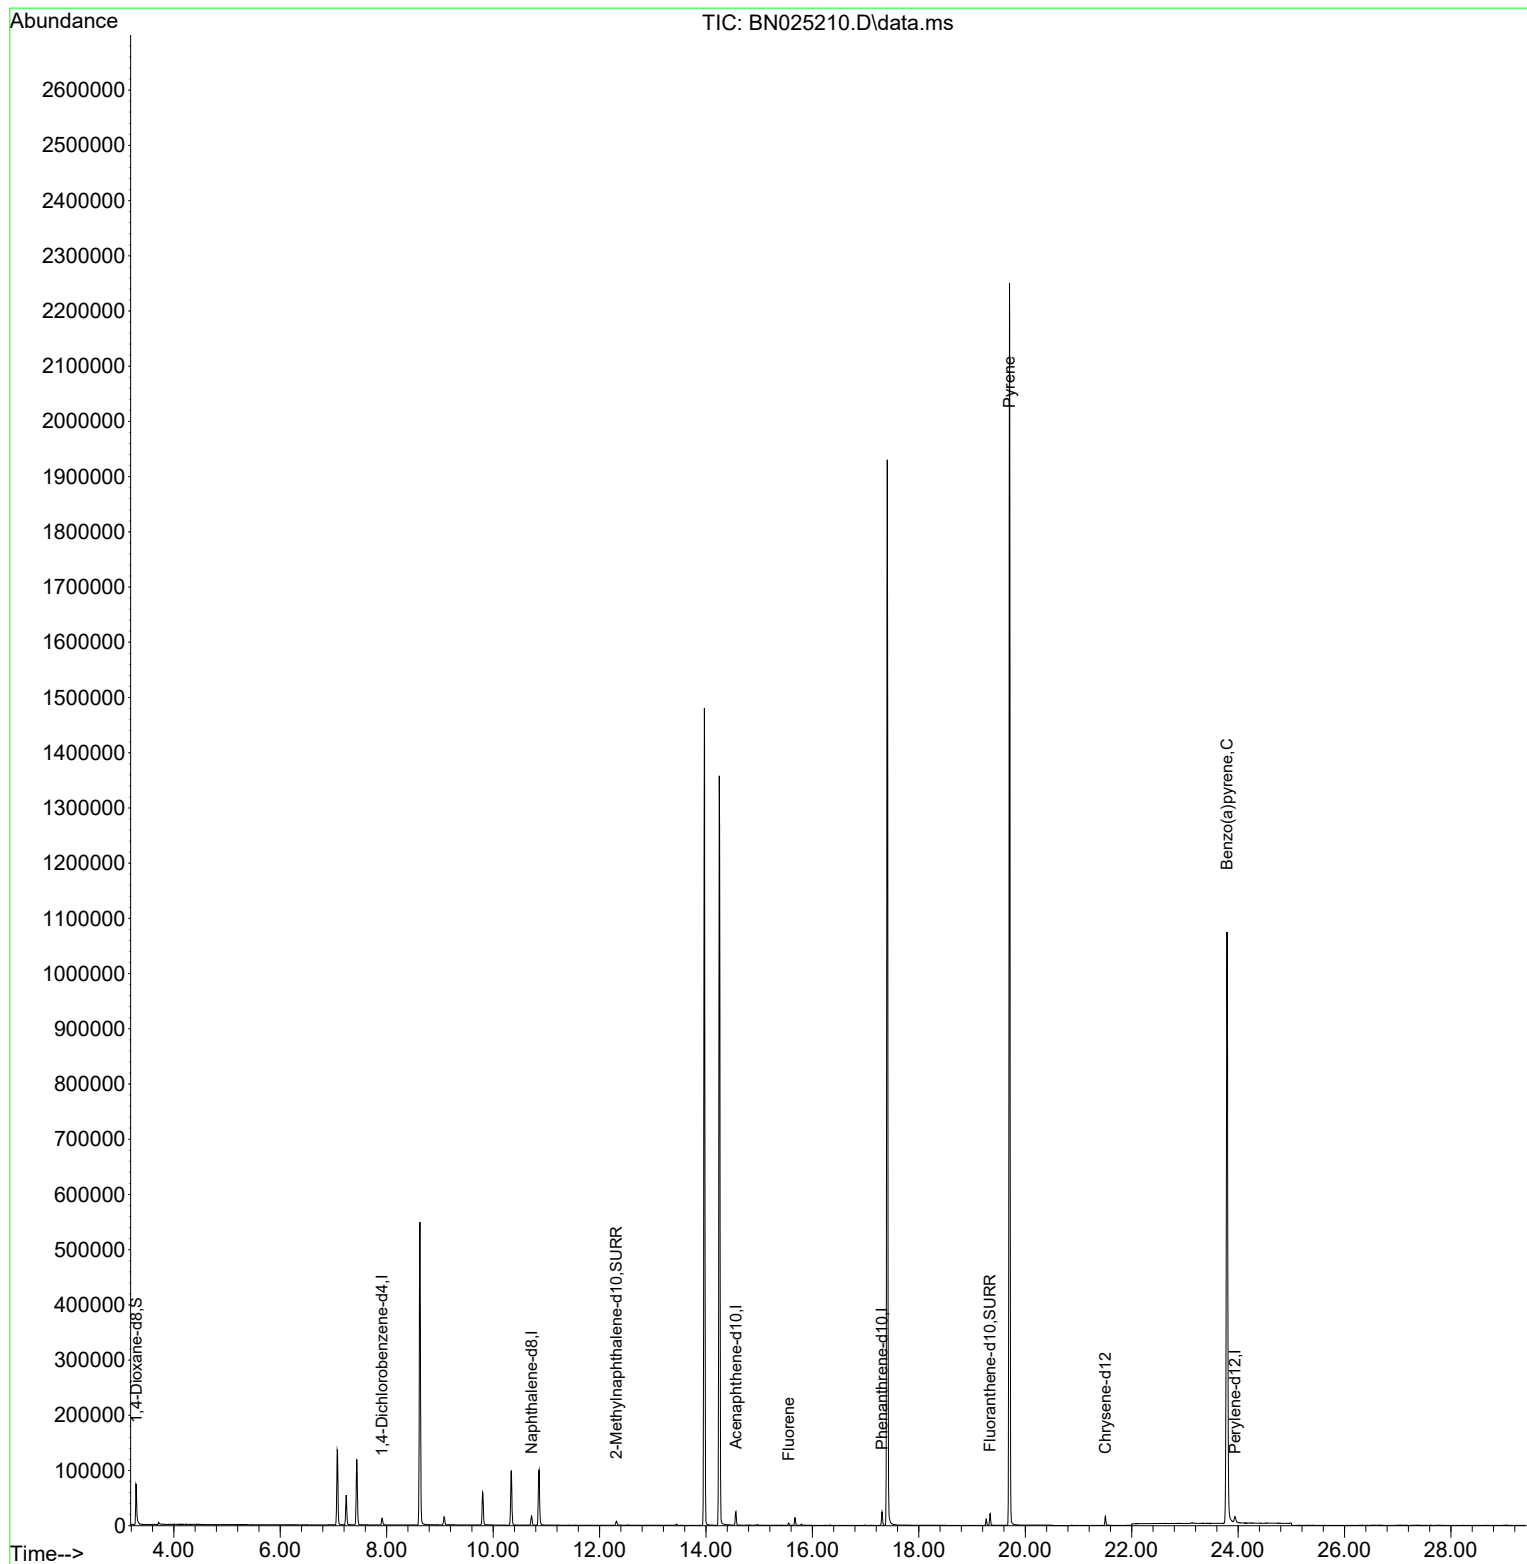


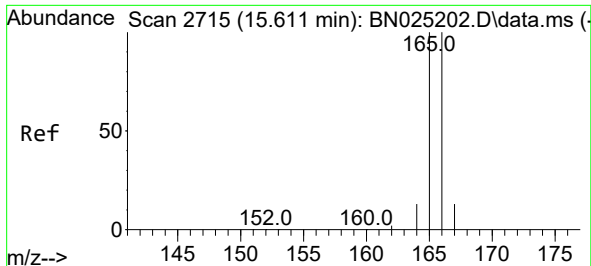

#12
Fluorene
Concen: 0.080 ng/ul
RT: 15.556 min Scan# 21
Delta R.T. -0.055 min
Lab File: BN025210.D
Acq: 01 May 2023 16:16




Instrument :
BNA_N
ClientSampleId :
SBLK474


Tgt Ion:166 Resp: 3770
Ion Ratio Lower Upper
166 100
165 8.0 78.1 117.1#
167 35.6 11.0 16.6#

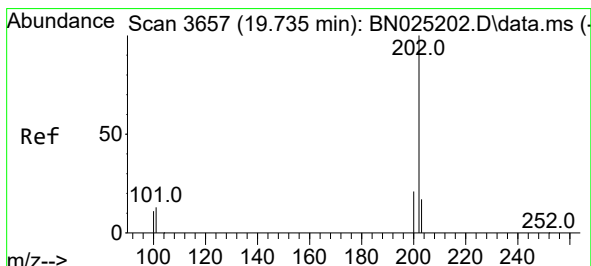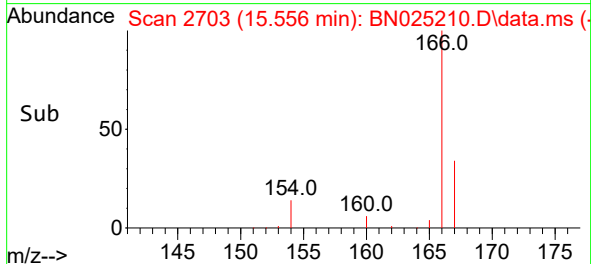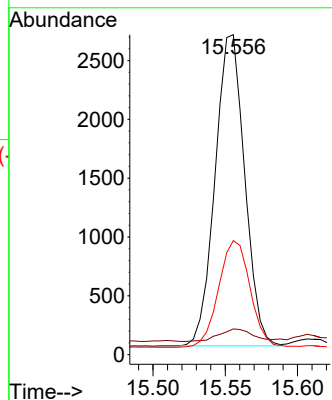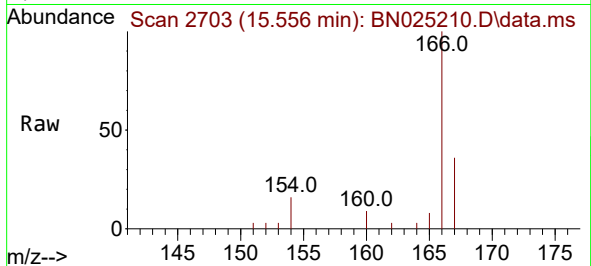

#20
Pyrene
Concen: 0.056 ng/ul
RT: 19.703 min Scan# 3650
Delta R.T. -0.031 min
Lab File: BN025210.D
Acq: 01 May 2023 16:16

Tgt Ion:202 Resp: 3401
Ion Ratio Lower Upper
202 100
101 183.4 11.3 16.9#
100 1401.4 9.2 13.8#

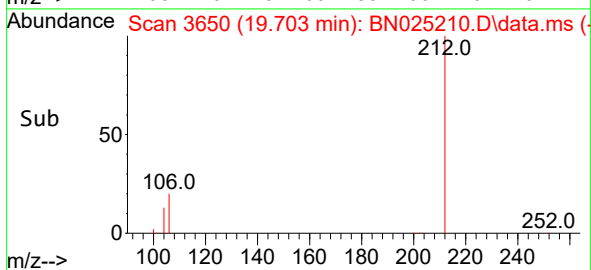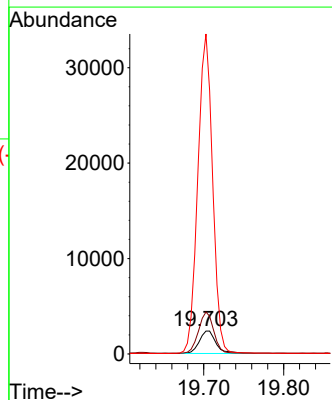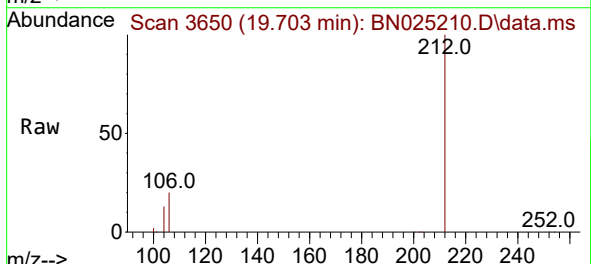

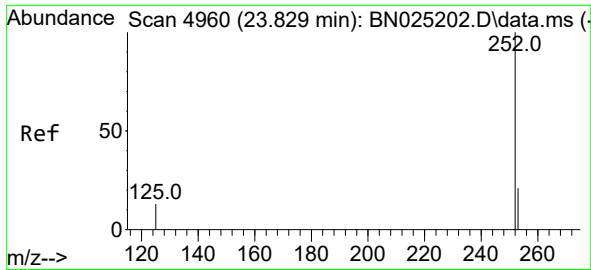

#26

Benzo(a)pyrene

Concen: 0.103 ng/ul

RT: 23.791 min Scan# 49

Delta R.T. -0.051 min

Lab File: BN025210.D


Acq: 01 May 2023 16:16

Instrument :

BNA_N

ClientSampleId :

SBLK474

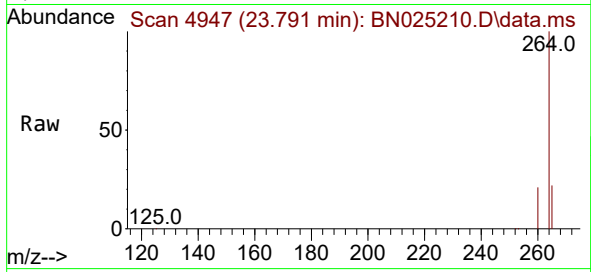

Tgt Ion:252 Resp: 5707

Ion Ratio Lower Upper

252 100

253 45.5 21.4 32.2#

125 39.3 14.6 22.0#

