
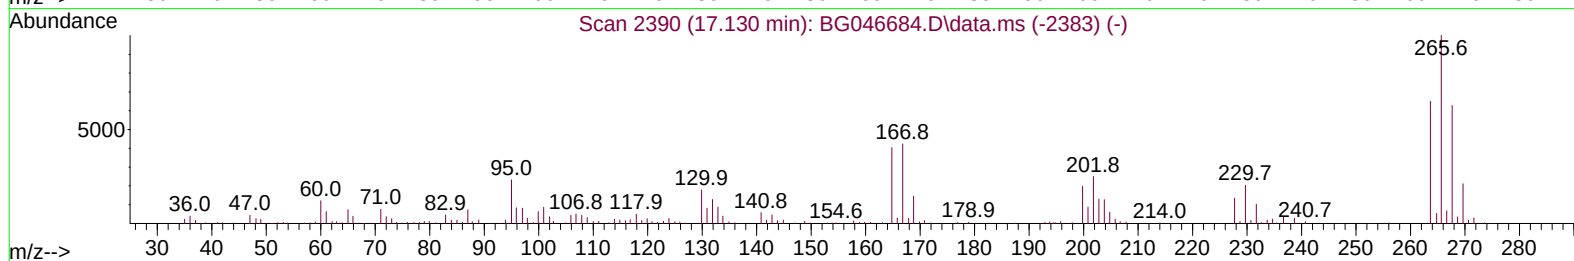
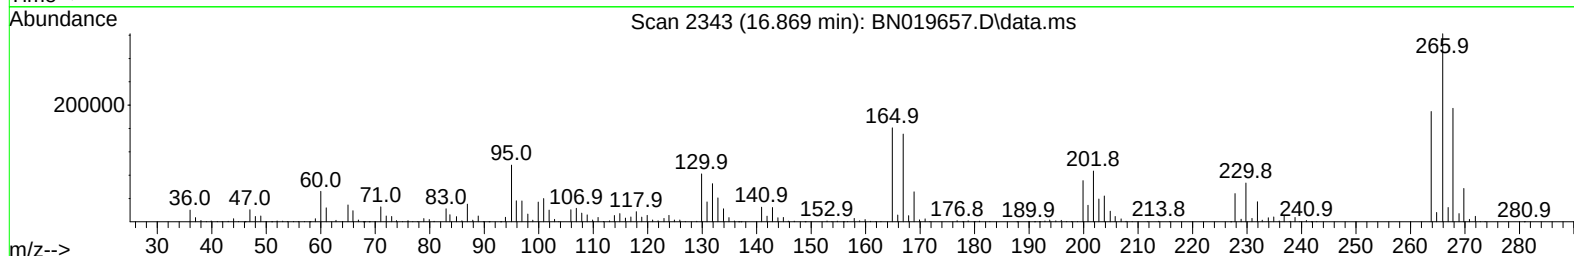


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050422\
 Data File : BN019657.D
 Acq On : 04 May 2022 10:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 04 14:53:54 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 23 16:56:32 2022
 Response via : Initial Calibration

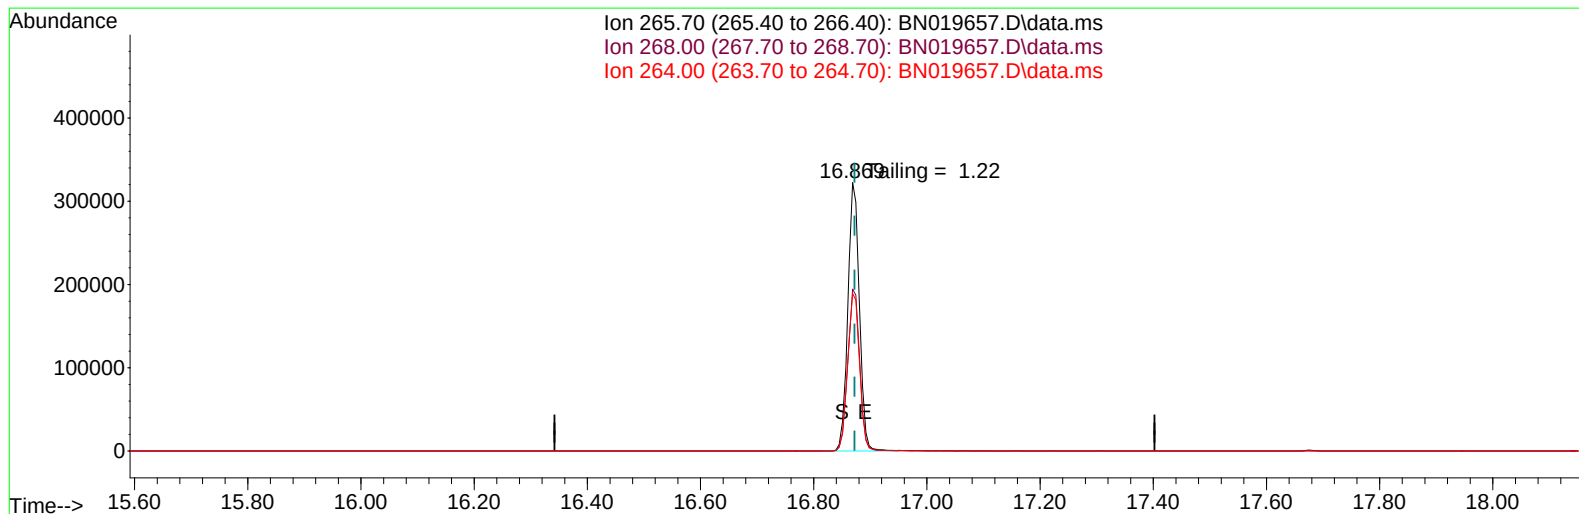

TIC: BN019657.D\data.ms

(70) Pentachlorophenol (C)




16.869min (-0.003) 21388.65 ng

response 459245

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.33
264.00	61.60	58.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050422\
Data File : BN019657.D
Acq On : 04 May 2022 10:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 04 14:53:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

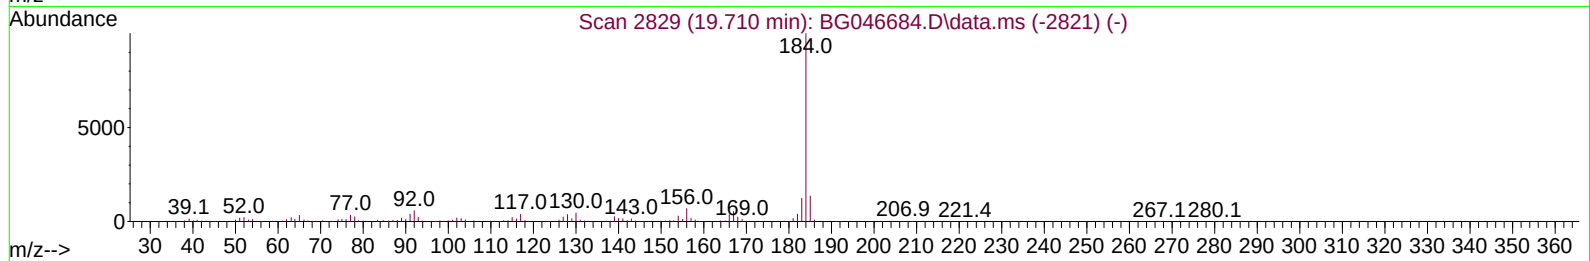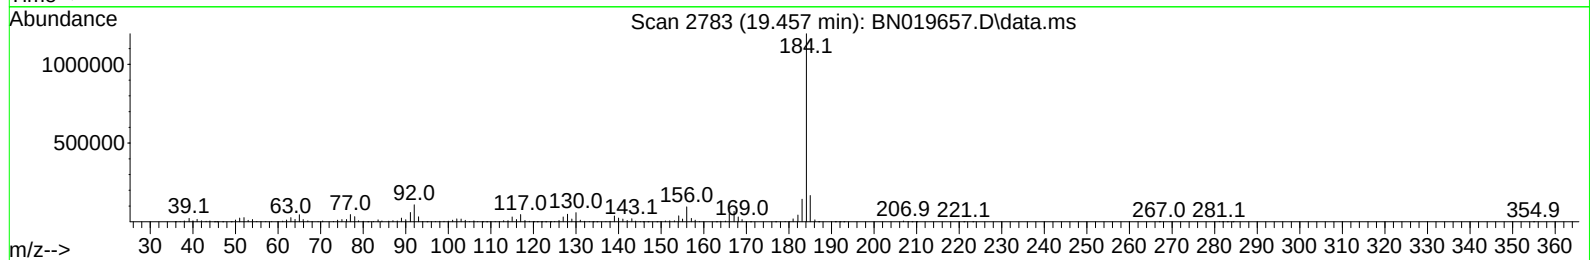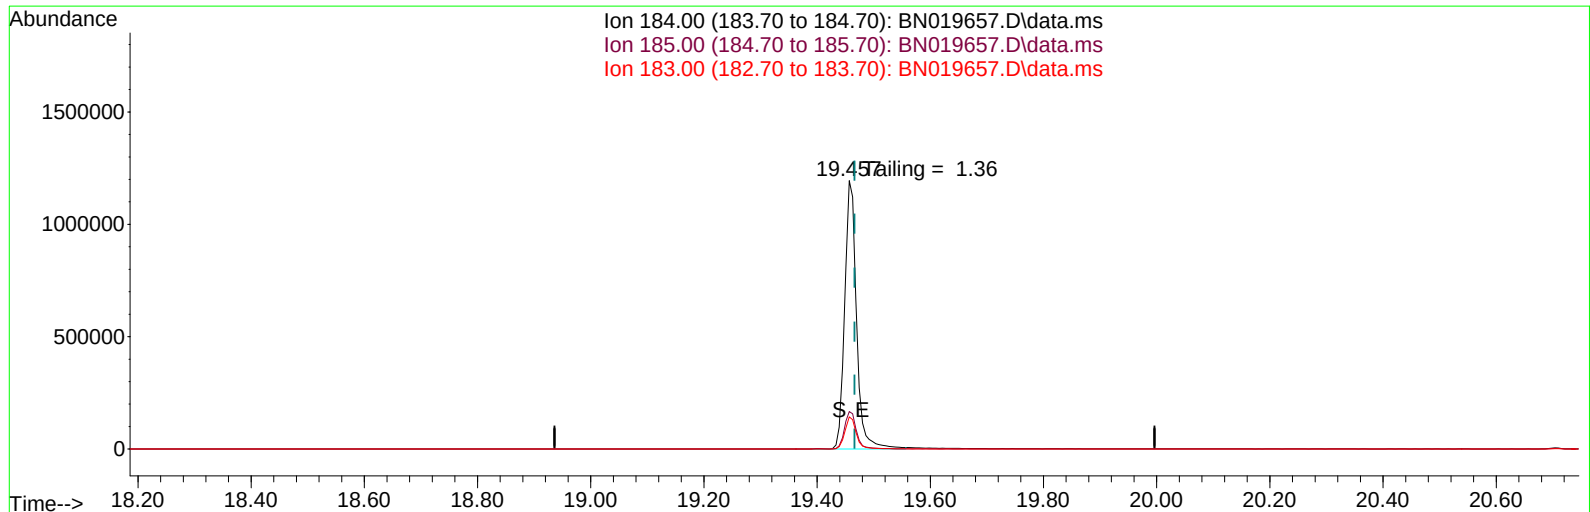

TIC: BN019657.D\data.ms

(77) Benzidine

19.457min (-0.009) 0.00 ng

response 1753782

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.98
183.00	13.20	11.98
0.00	0.00	0.00