


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050422\
 Data File : BN019657.D
 Acq On : 04 May 2022 10:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN050422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 04 15:20:22 2022

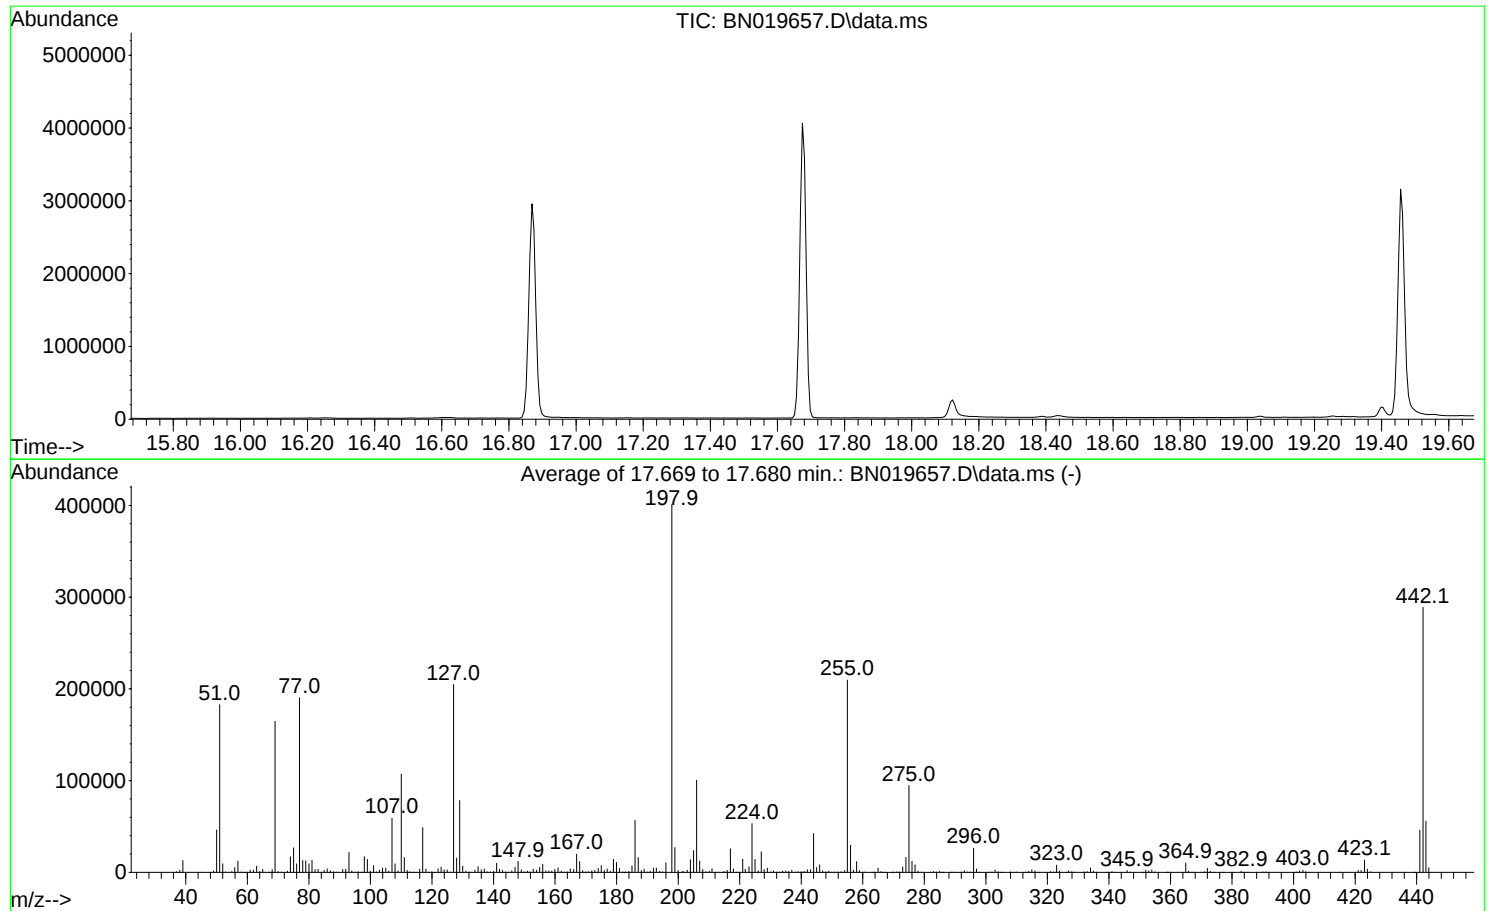

AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.6	182869	PASS
68	69	0.00	2	1.9	3056	PASS
69	198	0.00	100	41.1	164618	PASS
70	69	0.00	2	0.5	865	PASS
127	198	10	80	51.1	204757	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	400981	PASS
199	198	5	9	6.8	27115	PASS
275	198	10	60	23.6	94792	PASS
365	198	1	100	2.6	10282	PASS
441	198	0.01	100	11.4	45885	PASS
442	442	50	100	100.0	288789	PASS
443	442	15	24	19.3	55744	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/4/2022	BNA_N	<u>BN019657.D</u>
Compound Name	Response	Retention Time
DDT	1166386	20.7
DDD	4409	20.26
DDE	138	19.75
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4547	1170933	0.39

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050422\
 Data File : BN019657.D
 Acq On : 04 May 2022 10:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: May 04 14:53:54 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 23 16:56:32 2022
 Response via : Initial Calibration

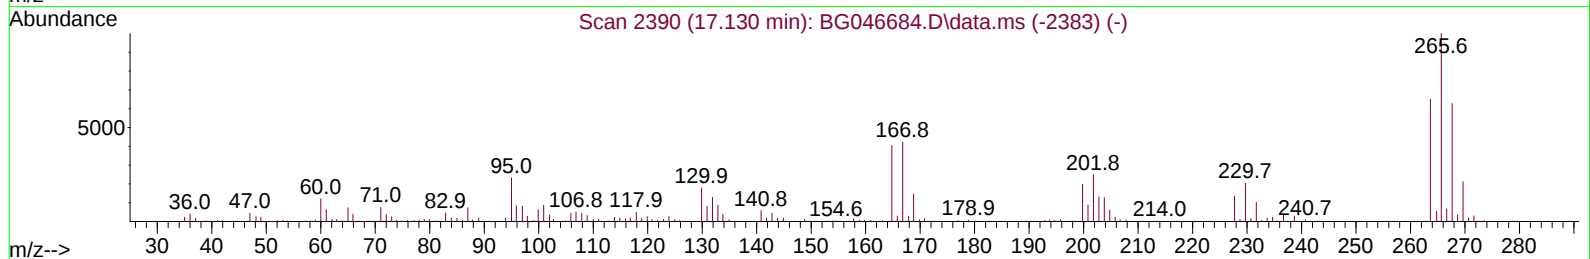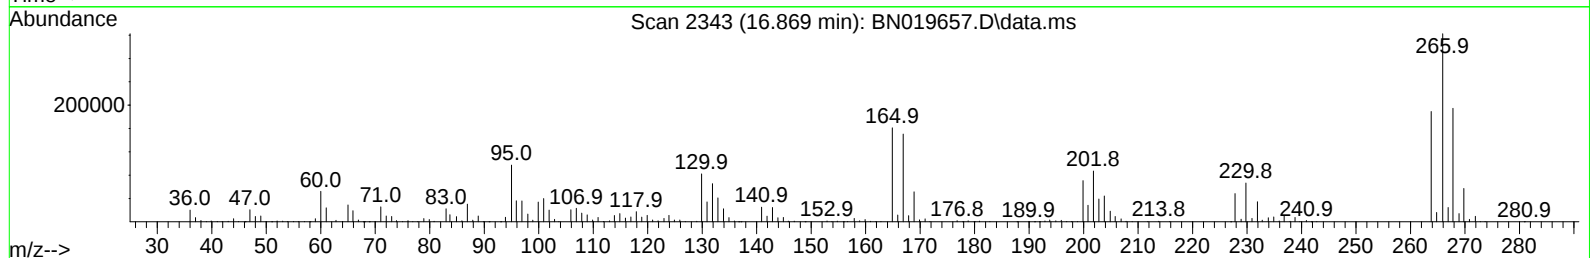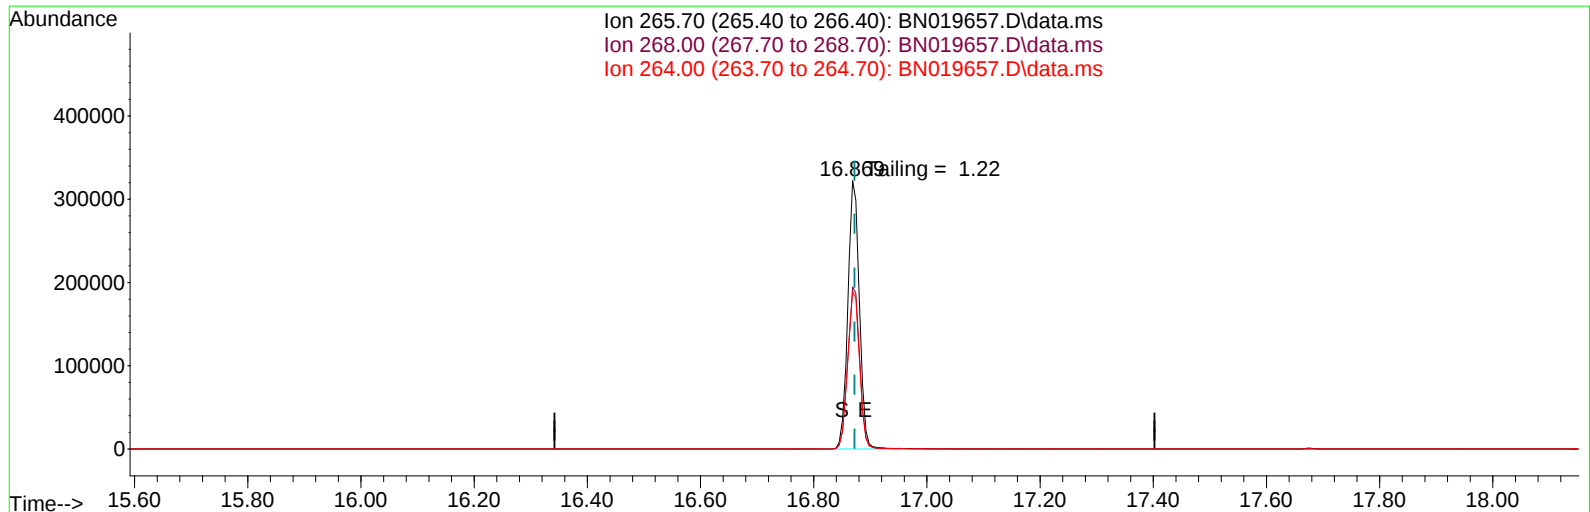

TIC: BN019657.D\data.ms

(70) Pentachlorophenol (C)

16.869min (-0.003) 21388.65 ng




response 459245

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.33
264.00	61.60	58.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050422\
Data File : BN019657.D
Acq On : 04 May 2022 10:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 04 14:53:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

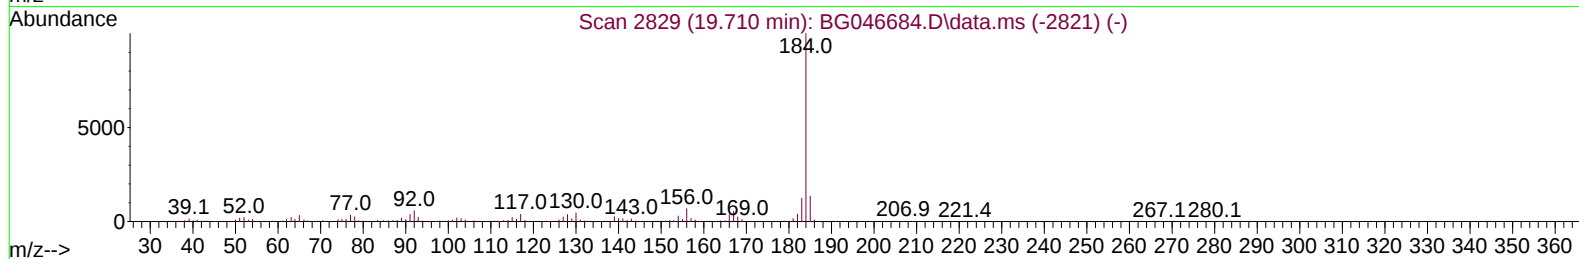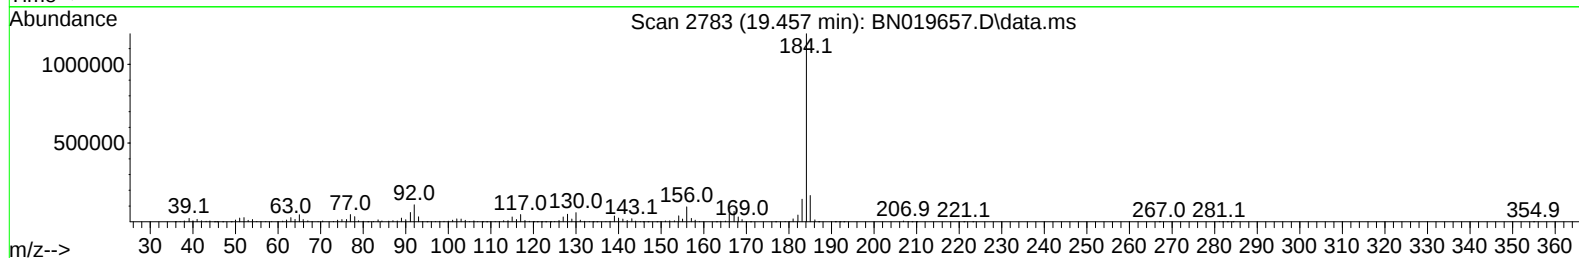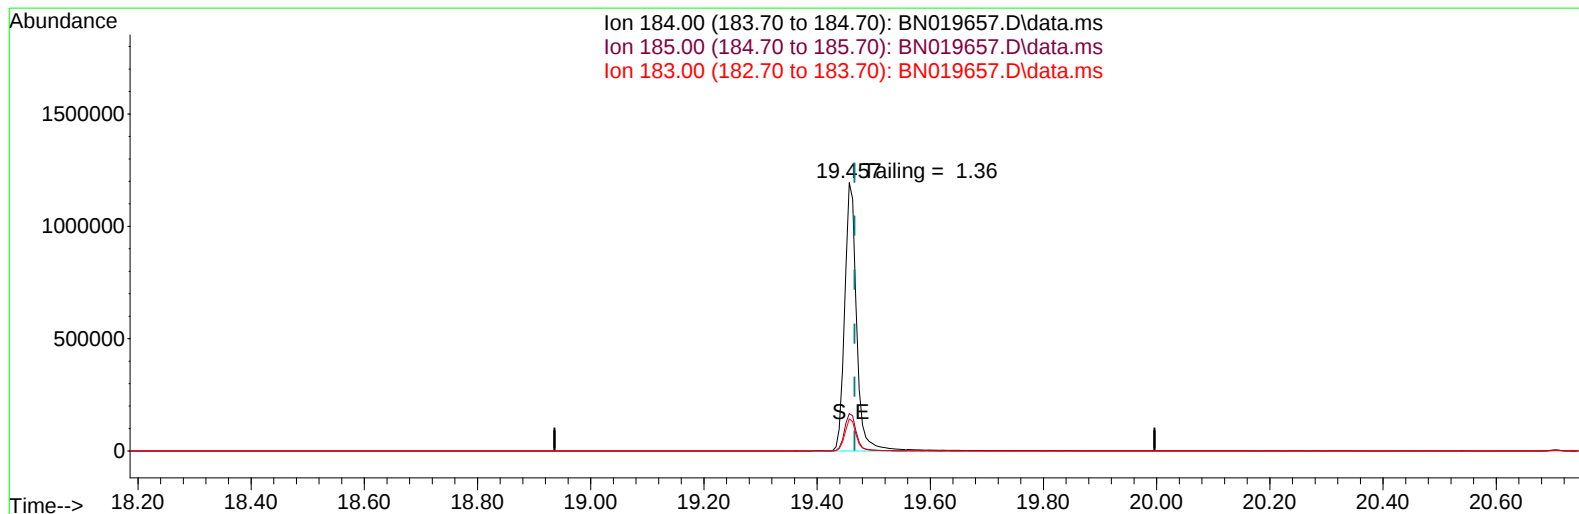

TIC: BN019657.D\data.ms

(77) Benzidine

19.457min (-0.009) 0.00 ng

response 1753782

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.98
183.00	13.20	11.98
0.00	0.00	0.00