
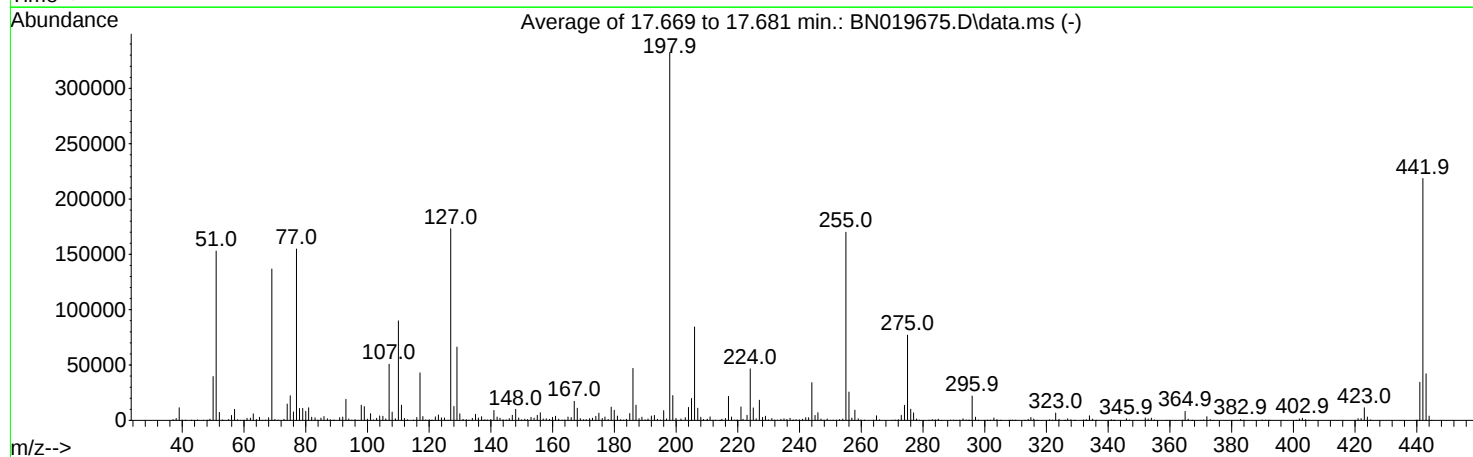


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050422\
 Data File : BN019675.D
 Acq On : 04 May 2022 22:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN050422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 04 15:20:22 2022

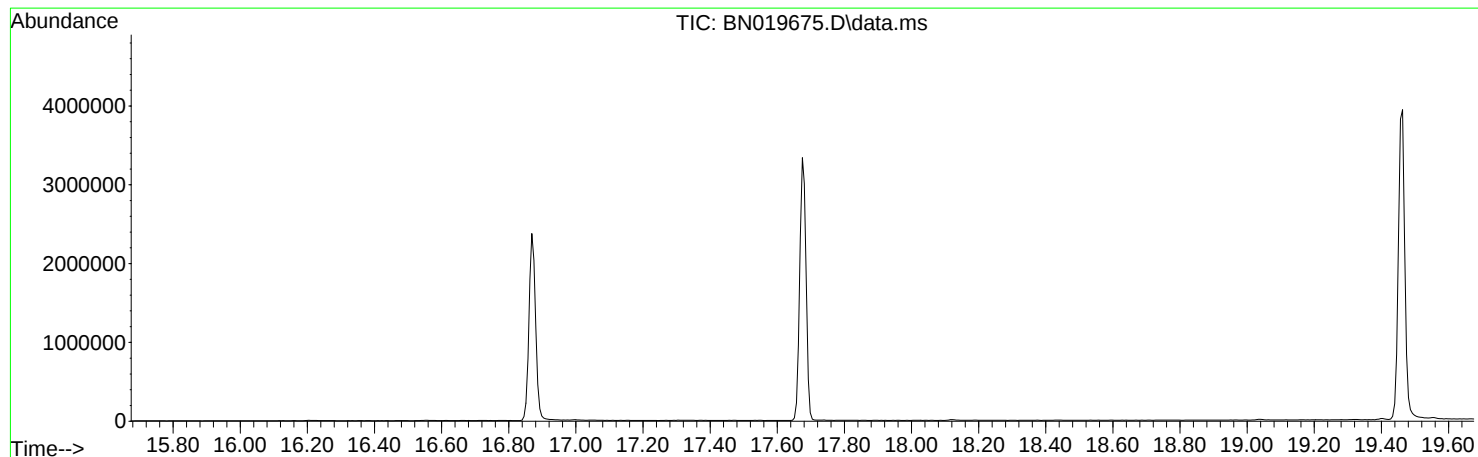

AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.0	152960	PASS
68	69	0.00	2	1.8	2519	PASS
69	198	0.00	100	41.2	136797	PASS
70	69	0.00	2	0.6	809	PASS
127	198	10	80	52.1	173269	PASS
197	198	0.00	2	0.4	1293	PASS
198	198	100	100	100.0	332373	PASS
199	198	5	9	6.8	22467	PASS
275	198	10	60	23.2	77016	PASS
365	198	1	100	2.4	8097	PASS
441	198	0.01	100	10.3	34395	PASS
442	442	50	100	100.0	218549	PASS
443	442	15	24	19.3	42125	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/4/2022	BNA_N	<u>BN019675.D</u>
Compound Name	Response	Retention Time
DDT	1036587	20.704
DDD	7068	20.257
DDE	56	19.757
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7124	1043711	0.68

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050422\
Data File : BN019675.D
Acq On : 04 May 2022 22:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 05 06:13:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

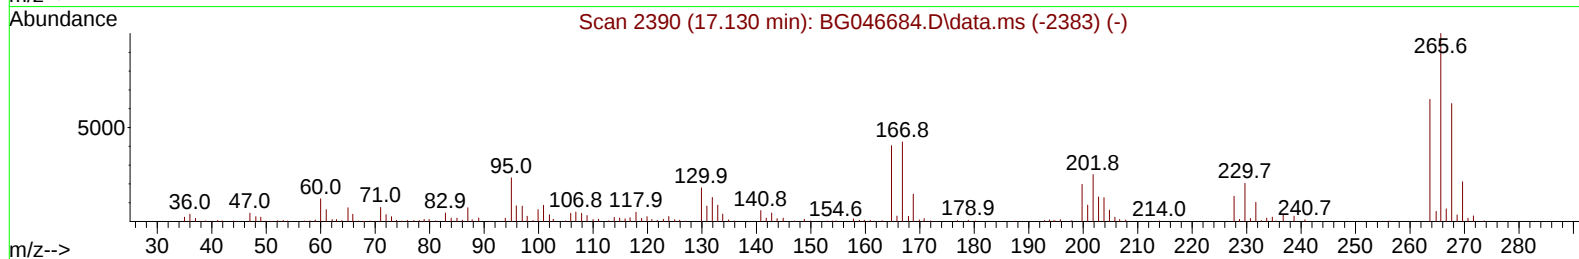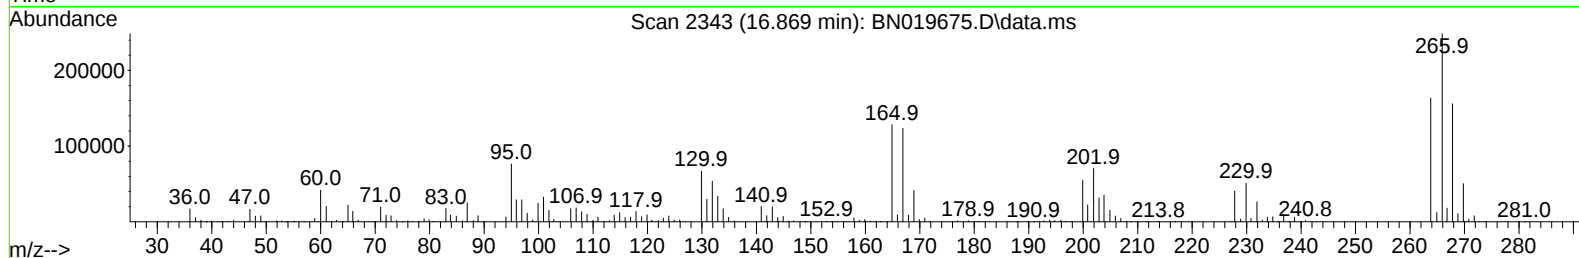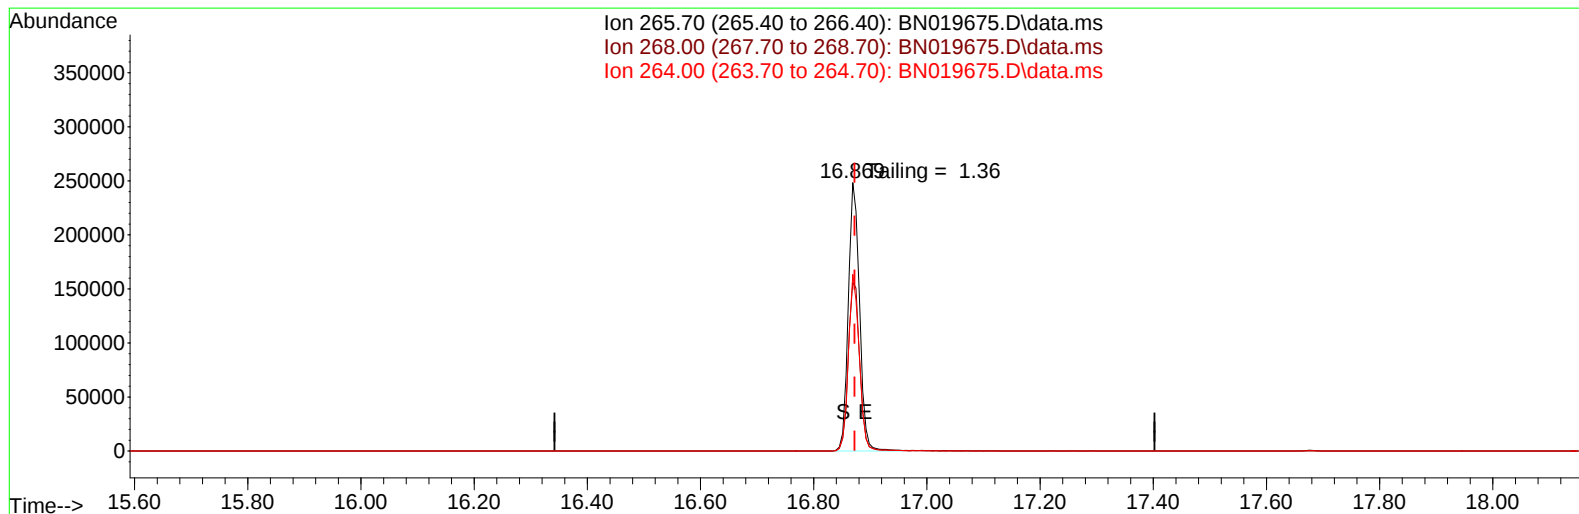

TIC: BN019675.D\data.ms

(70) Pentachlorophenol (C)

16.869min (-0.003) 18639.43 ng




response 343606

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.77
264.00	61.60	65.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050422\
Data File : BN019675.D
Acq On : 04 May 2022 22:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 05 06:13:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

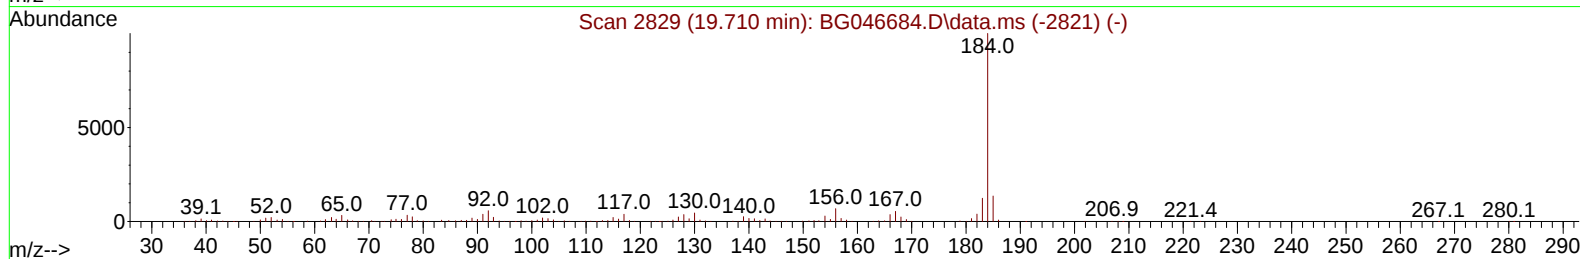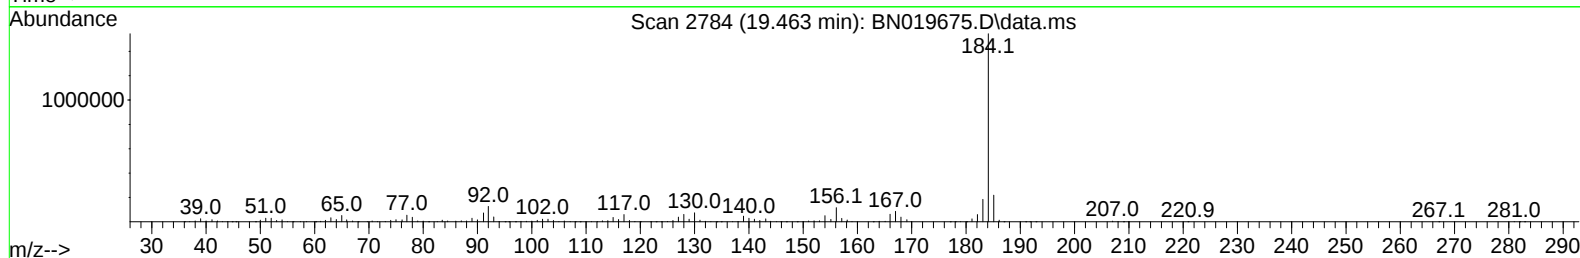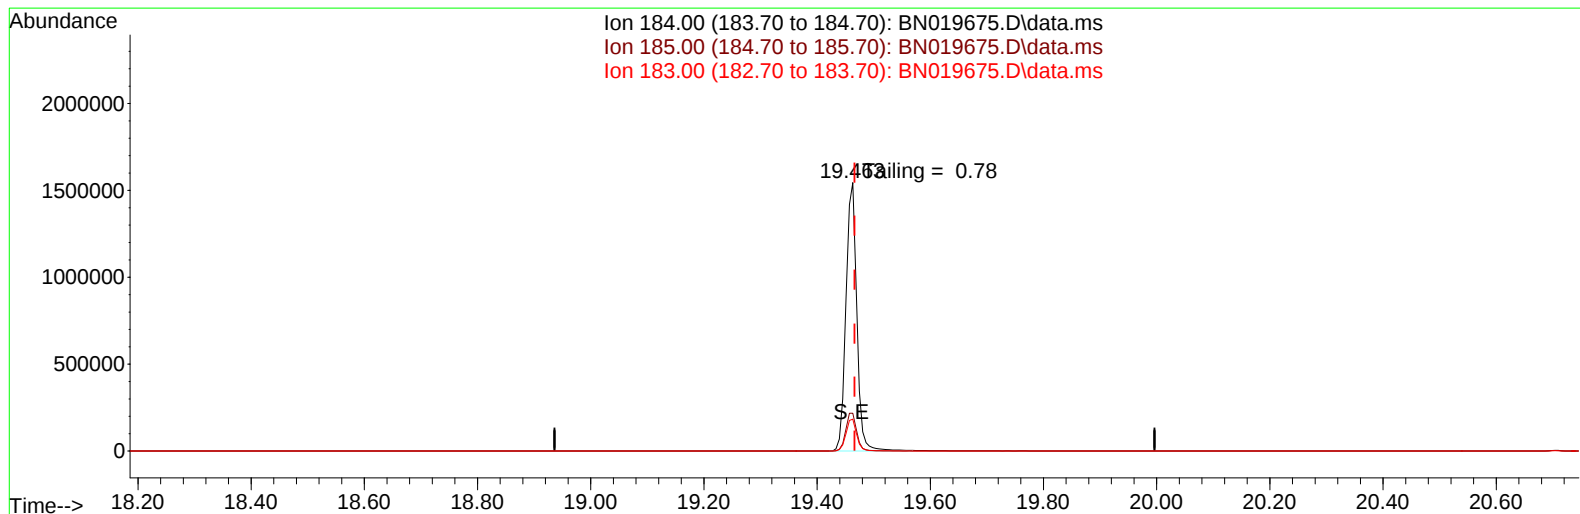

TIC: BN019675.D\data.ms

(77) Benzidine

19.463min (-0.003) 0.00 ng

response 2071524

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.10
183.00	13.20	11.89
0.00	0.00	0.00