
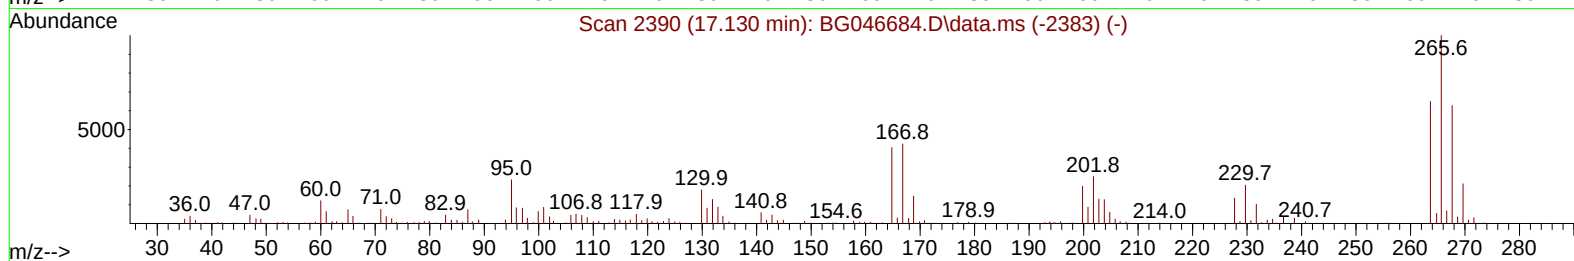
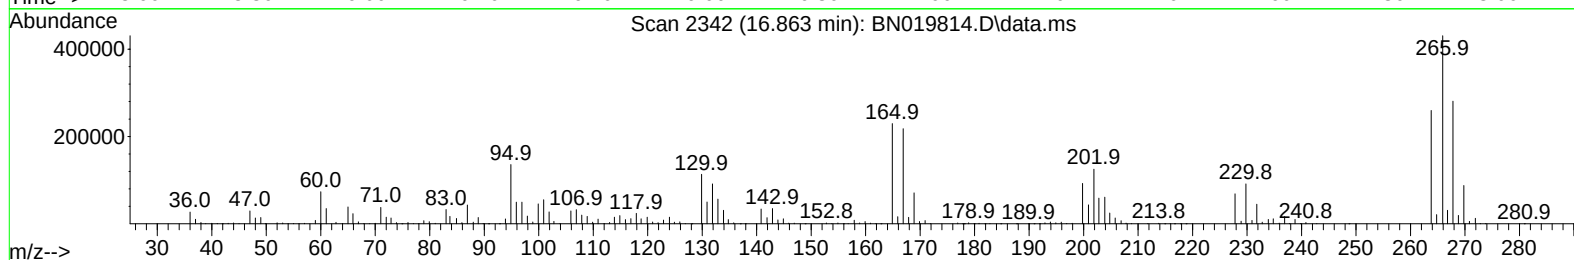


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051722\
Data File : BN019814.D
Acq On : 17 May 2022 10:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 18 04:36:48 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

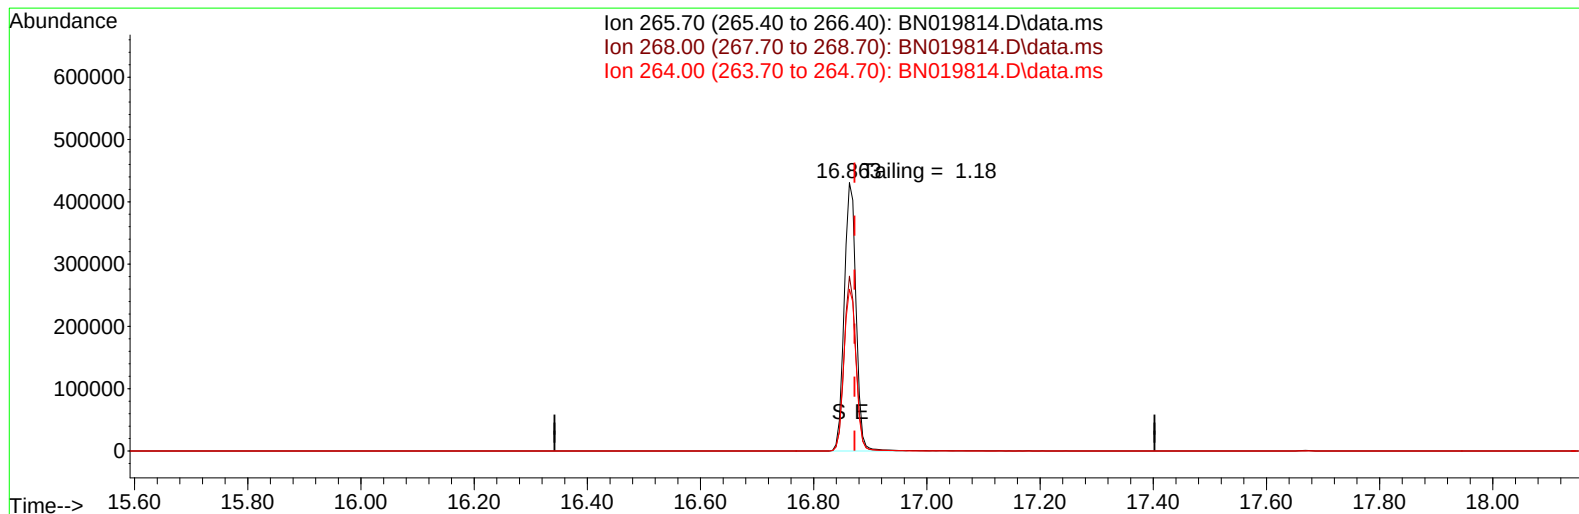

TIC: BN019814.D\data.ms

(70) Pentachlorophenol (C)




16.863min (-0.009) 24202.18 ng

response 626018

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.19
264.00	61.60	60.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051722\
Data File : BN019814.D
Acq On : 17 May 2022 10:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 18 04:36:48 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

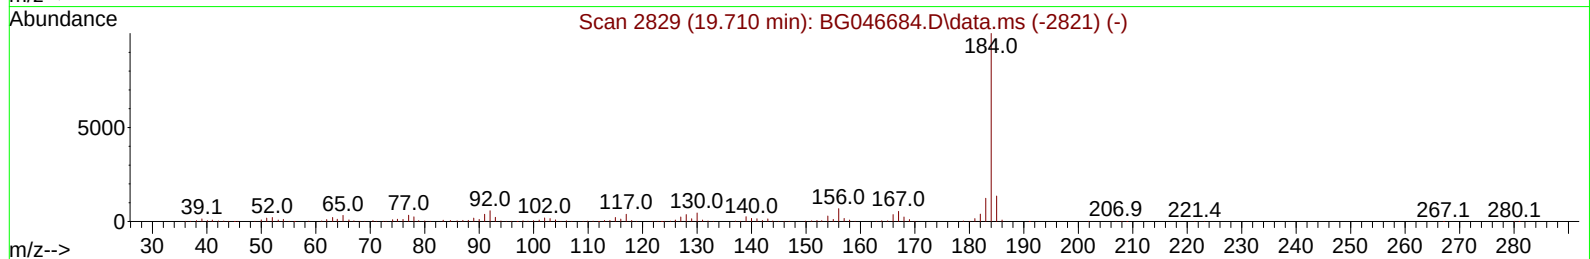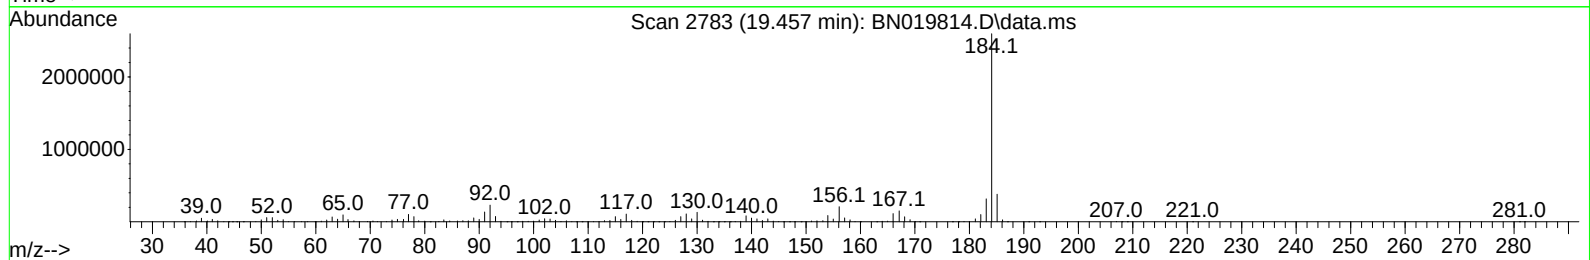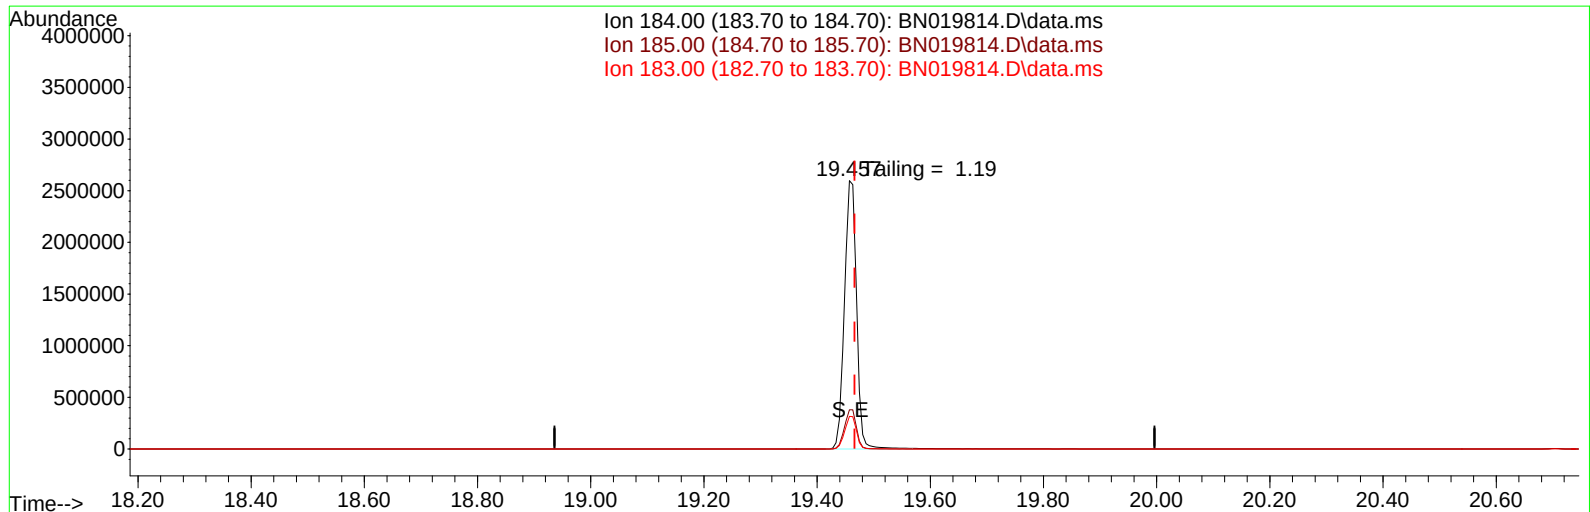

TIC: BN019814.D\data.ms

(77) Benzidine**19.457min (-0.009) 1023685.29 ng****response 3881324**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.62
183.00	13.20	12.19
0.00	0.00	0.00