


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051722\
 Data File : BN019814.D
 Acq On : 17 May 2022 10:27
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN051322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 18 07:42:52 2022

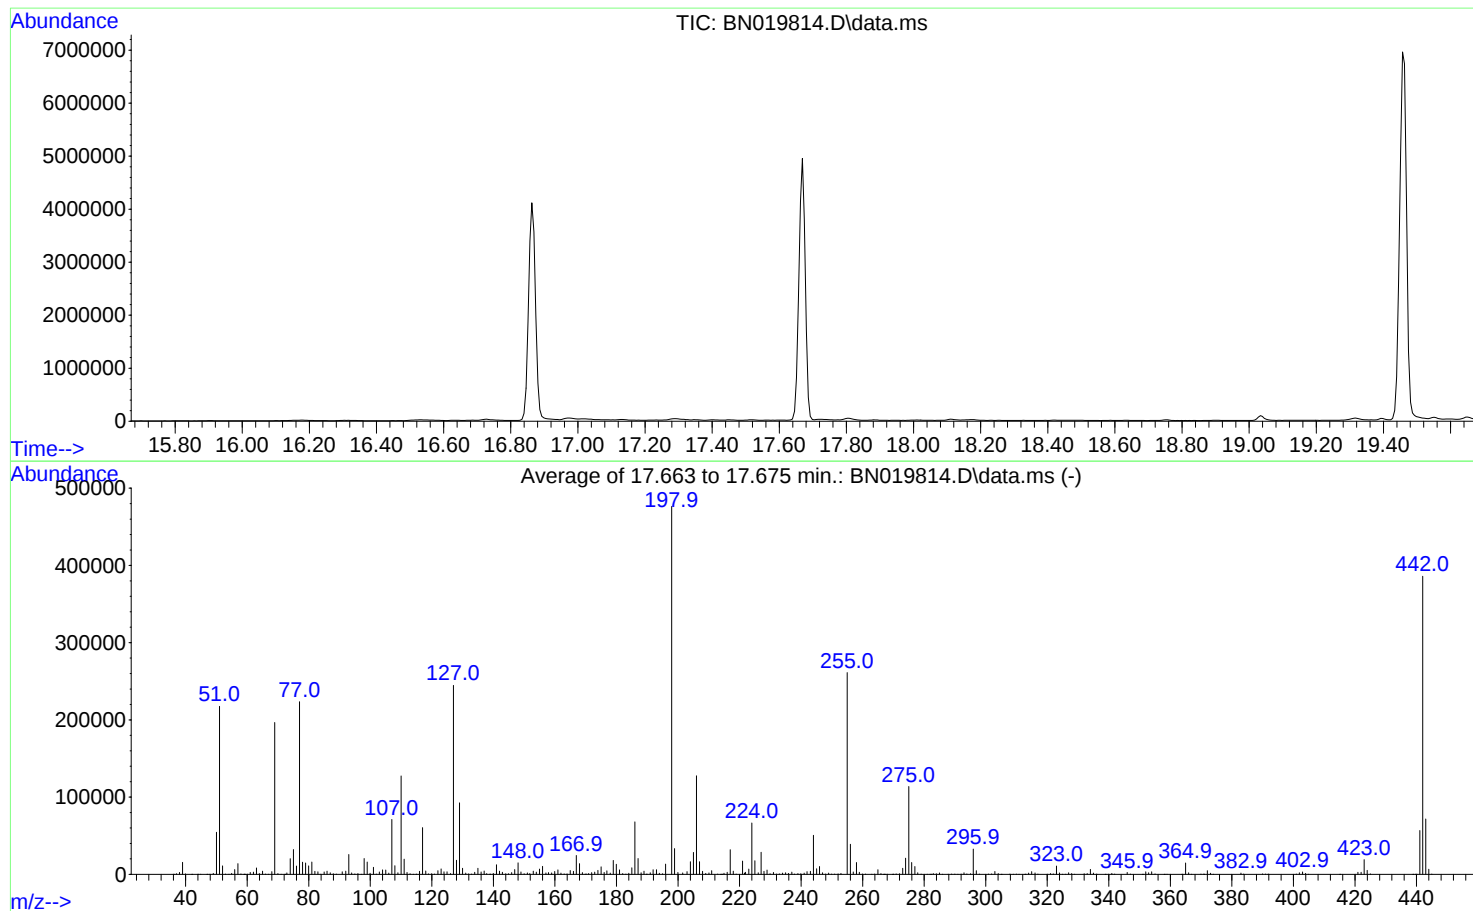




AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.7	217621	PASS
68	69	0.00	2	1.8	3468	PASS
69	198	0.00	100	41.3	196554	PASS
70	69	0.00	2	0.5	994	PASS
127	198	10	80	51.4	244779	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	476288	PASS
199	198	5	9	7.0	33451	PASS
275	198	10	60	23.9	113765	PASS
365	198	1	100	3.1	14688	PASS
441	198	0.01	100	11.9	56827	PASS
442	442	50	100	100.0	386005	PASS
443	442	15	24	18.5	71584	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051722\
Data File : BN019814.D
Acq On : 17 May 2022 10:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 18 04:36:48 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

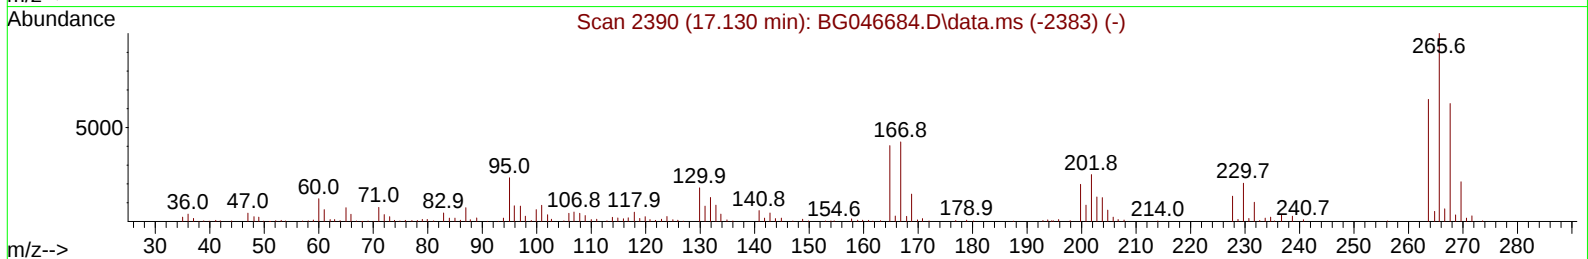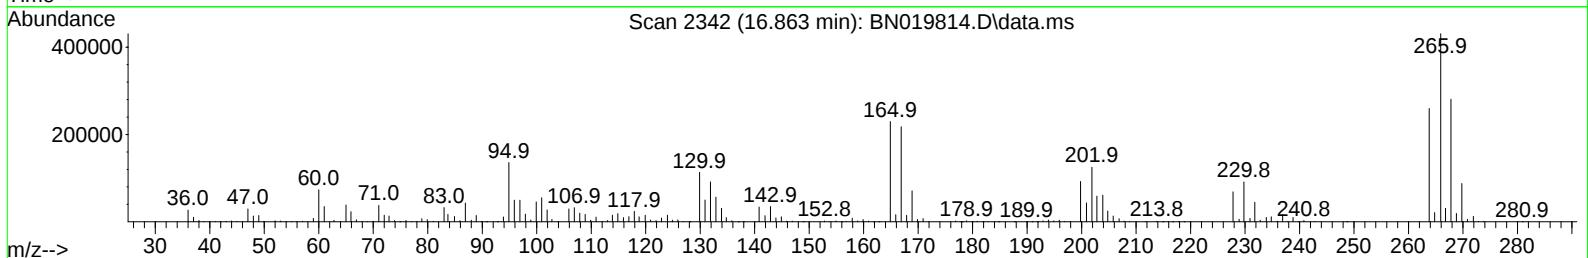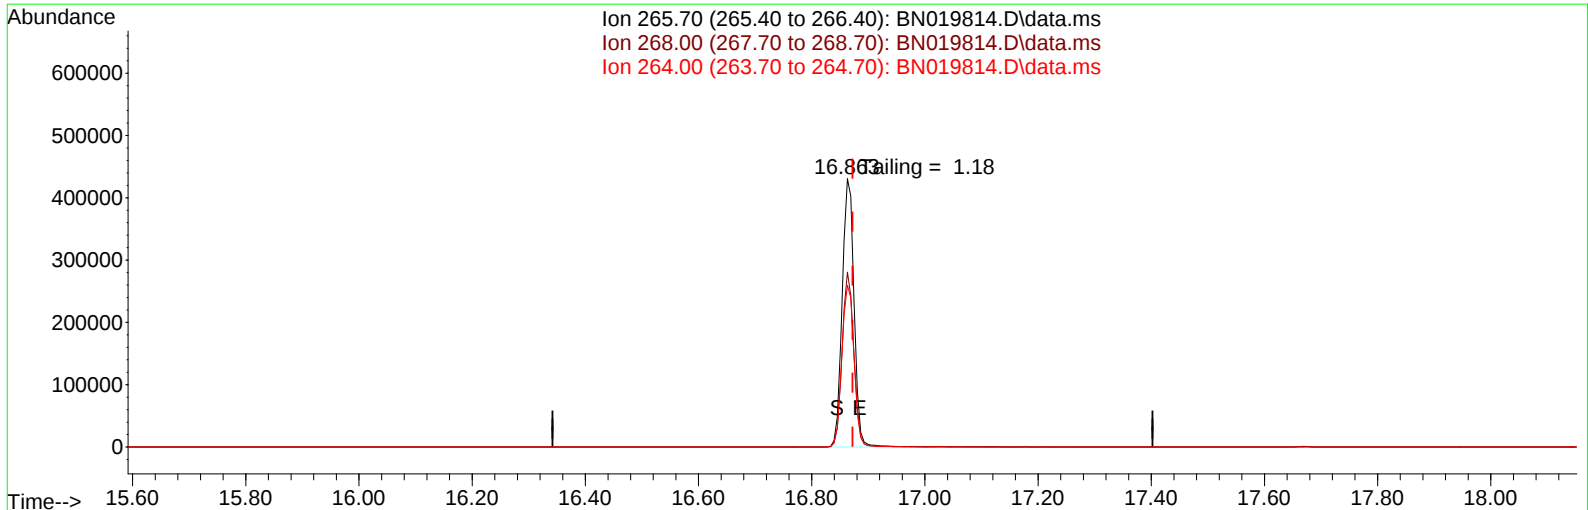

TIC: BN019814.D\data.ms

(70) Pentachlorophenol (C)

16.863min (-0.009) 24202.18 ng




response 626018

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.19
264.00	61.60	60.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051722\
Data File : BN019814.D
Acq On : 17 May 2022 10:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 18 04:36:48 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

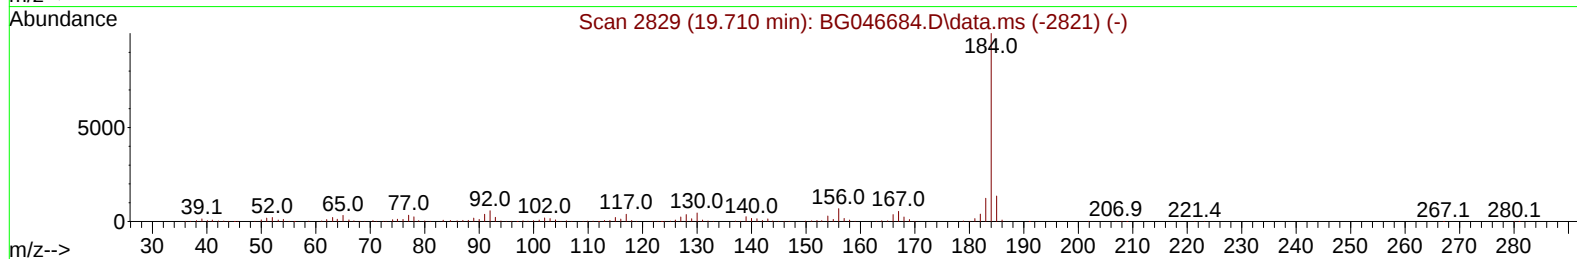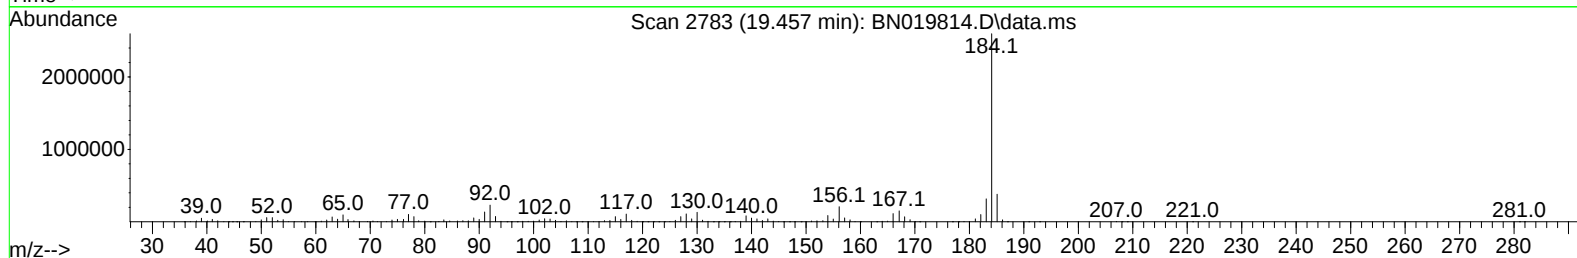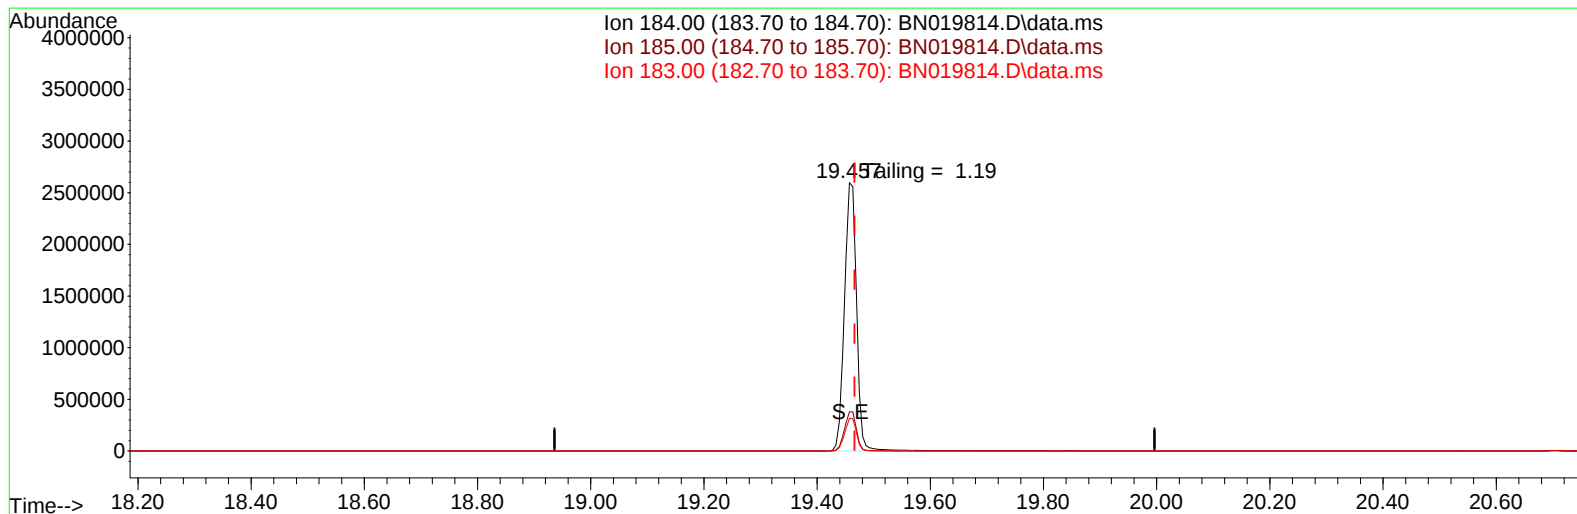

TIC: BN019814.D\data.ms

(77) Benzidine

19.457min (-0.009) 1023685.29 ng

response 3881324

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.62
183.00	13.20	12.19
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/17/2022	BNA_N	<u>BN019814.D</u>
Compound Name	Response	Retention Time
DDT	1629399	20.704
DDD	96876	20.263
DDE	2871	19.757
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
99747	1729146	5.77

Instrument :
BNA_N
ClientSampleId :
DFTPP