

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051822\
 Data File : BN019825.D
 Acq On : 18 May 2022 11:07
 Operator : CG/JU
 Sample : PB144854BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: May 19 03:19:11 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.851	152	4098	0.400	ng/ul	0.00
4) Naphthalene-d8	10.639	136	13443	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.474	164	8256	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.213	188	17739	0.400	ng/ul	0.00
17) Chrysene-d12	21.401	240	14175	0.400	ng/ul	0.00
23) Perylene-d12	23.740	264	14735	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.315	96	25033	5.161	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.229	152	6304	0.310	ng/ul	0.00
18) Fluoranthene-d10	19.239	212	14261	0.318	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.606	202	1964	0.030	ng/ul#	1
26) Benzo(a)pyrene	23.591	252	4540	0.071	ng/ul#	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051822\
Data File : BN019825.D
Acq On : 18 May 2022 11:07
Operator : CG/JU
Sample : PB144854BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: May 19 03:19:11 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

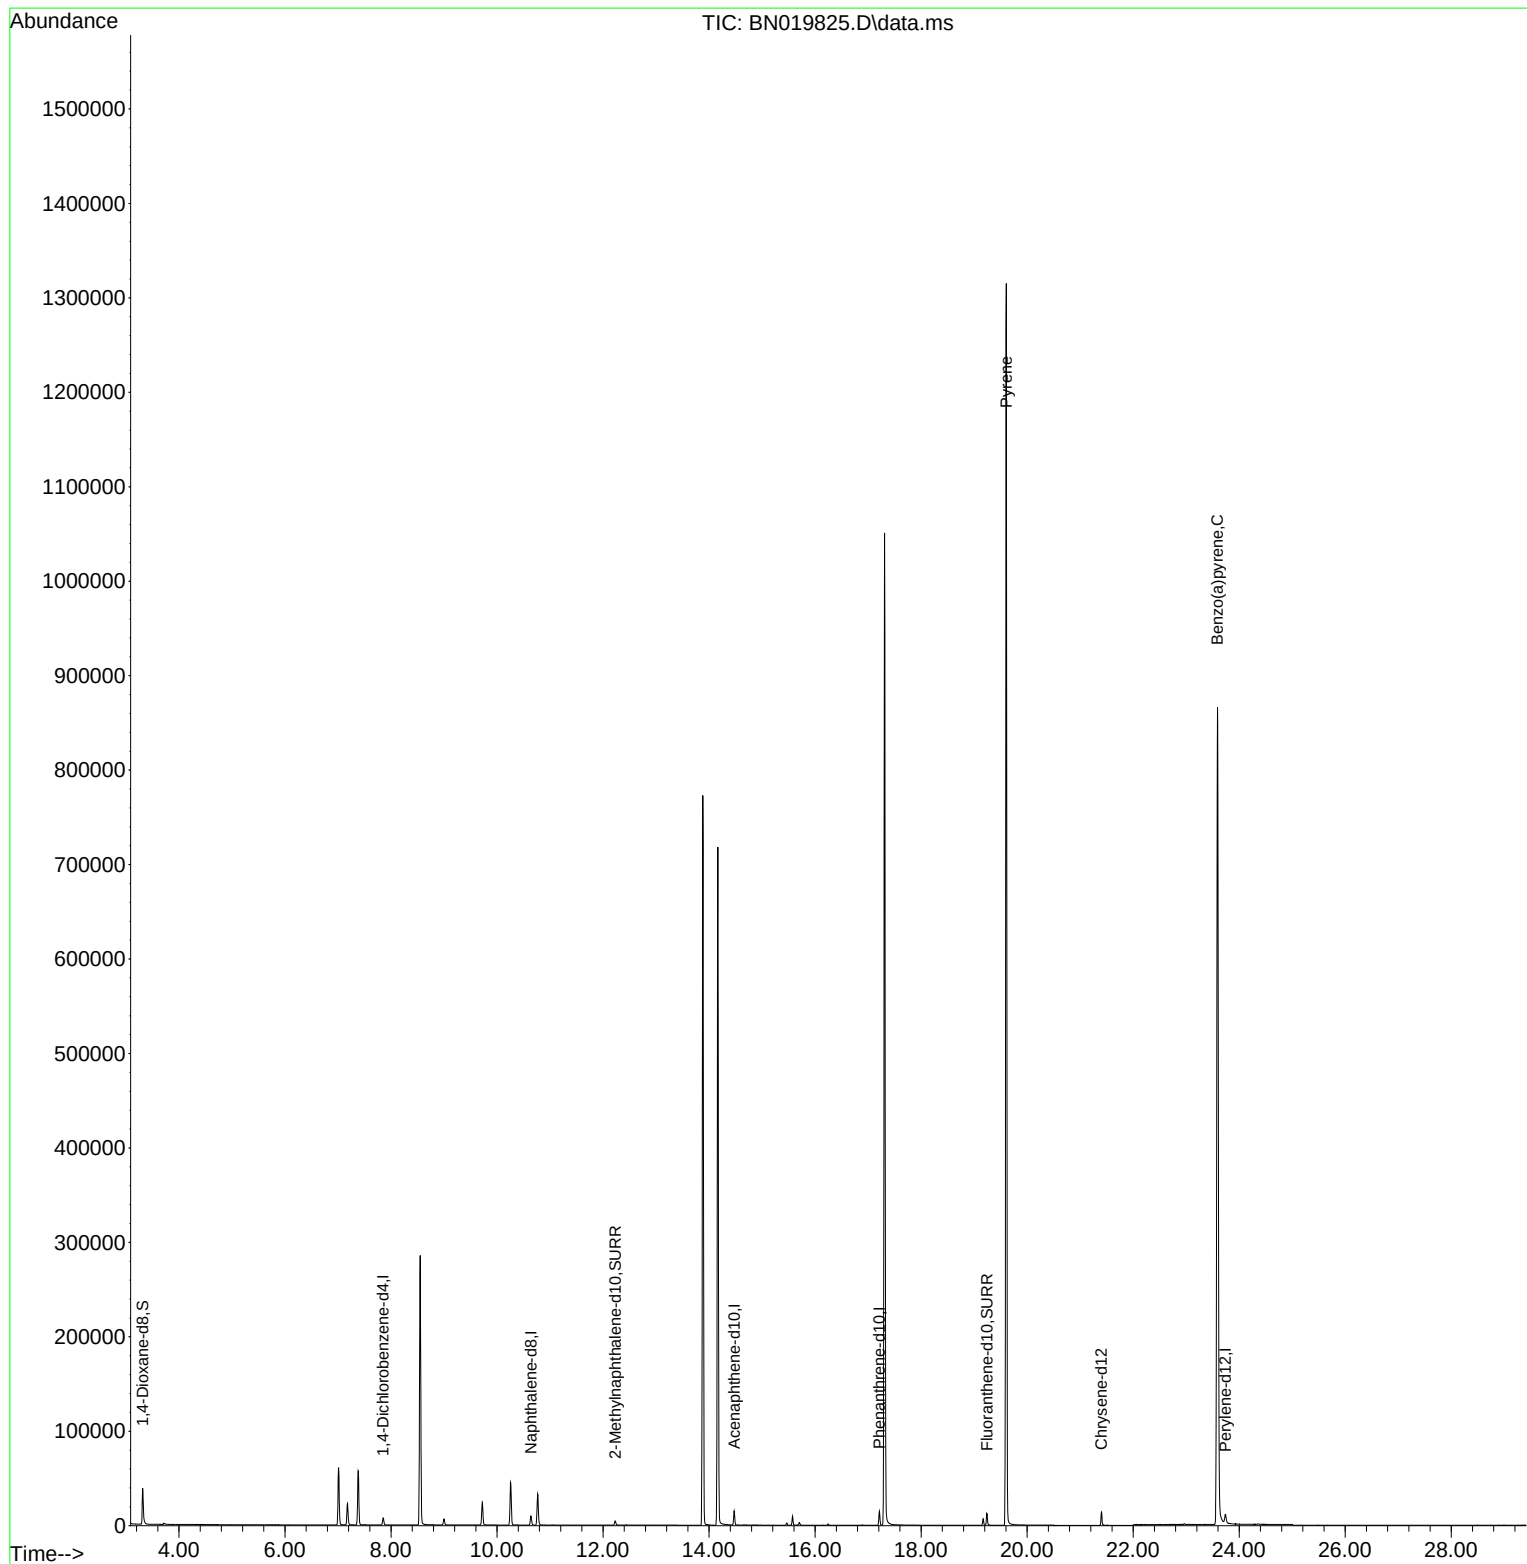



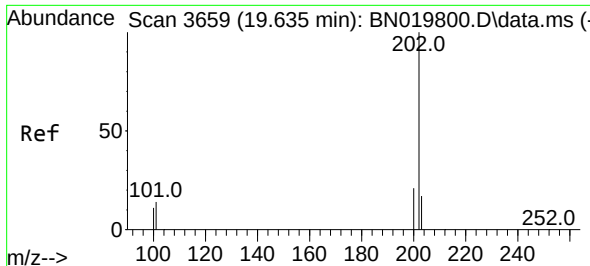


#20
Pyrene
Concen: 0.030 ng/ul
RT: 19.606 min Scan# 3653
Delta R.T. -0.028 min
Lab File: BN019825.D
Acq: 18 May 2022 11:07

Instrument :
BNA_N
ClientSampleId :

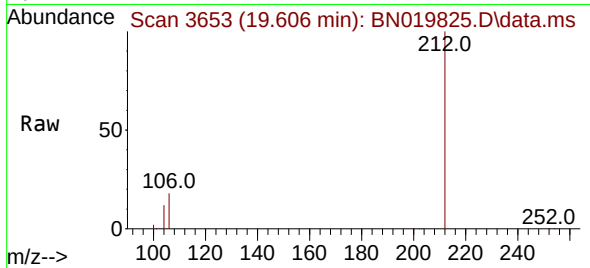

Tgt Ion:202 Resp: 1964
Ion Ratio Lower Upper
202 100
101 169.9 11.4 17.0#
100 1226.5 9.0 13.4#

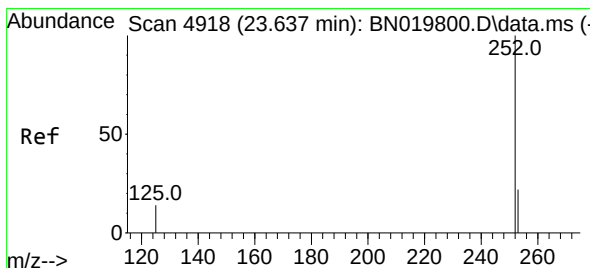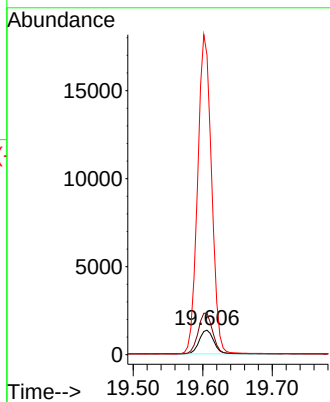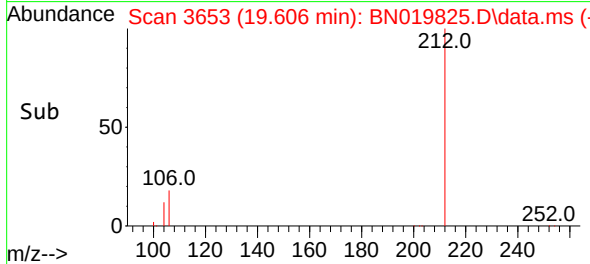

#26
Benzo(a)pyrene
Concen: 0.071 ng/ul
RT: 23.591 min Scan# 4902
Delta R.T. -0.048 min
Lab File: BN019825.D
Acq: 18 May 2022 11:07

Tgt Ion:252 Resp: 4540
Ion Ratio Lower Upper
252 100
253 38.9 23.4 35.0#
125 32.7 28.3 42.5

