




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051822\
 Data File : BN019835.D
 Acq On : 18 May 2022 17:31
 Operator : CG/JU
 Sample : N2766-10
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4G0

Manual IntegrationsAPPROVED

Quant Time: May 19 03:19:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
 Supervised By :mohammad ahmed 05/25/2022

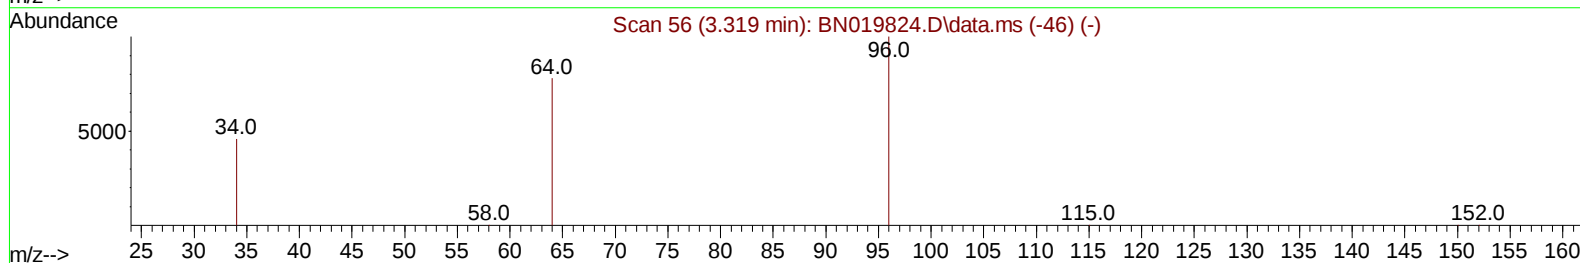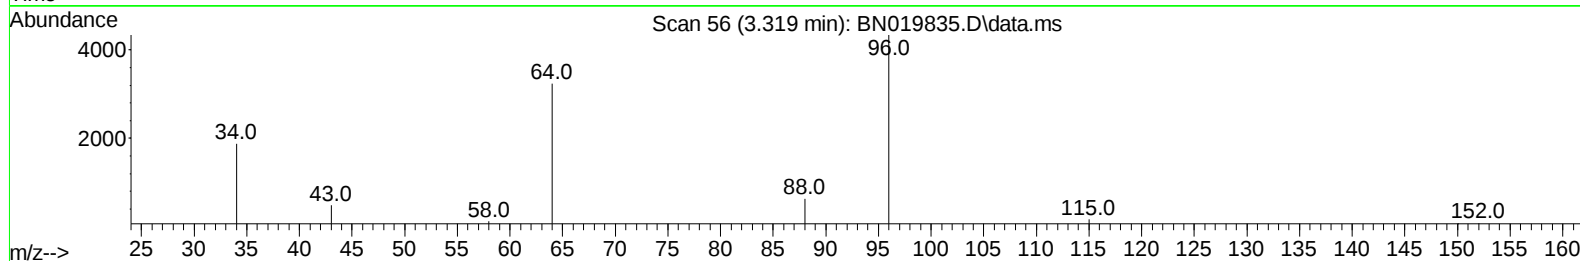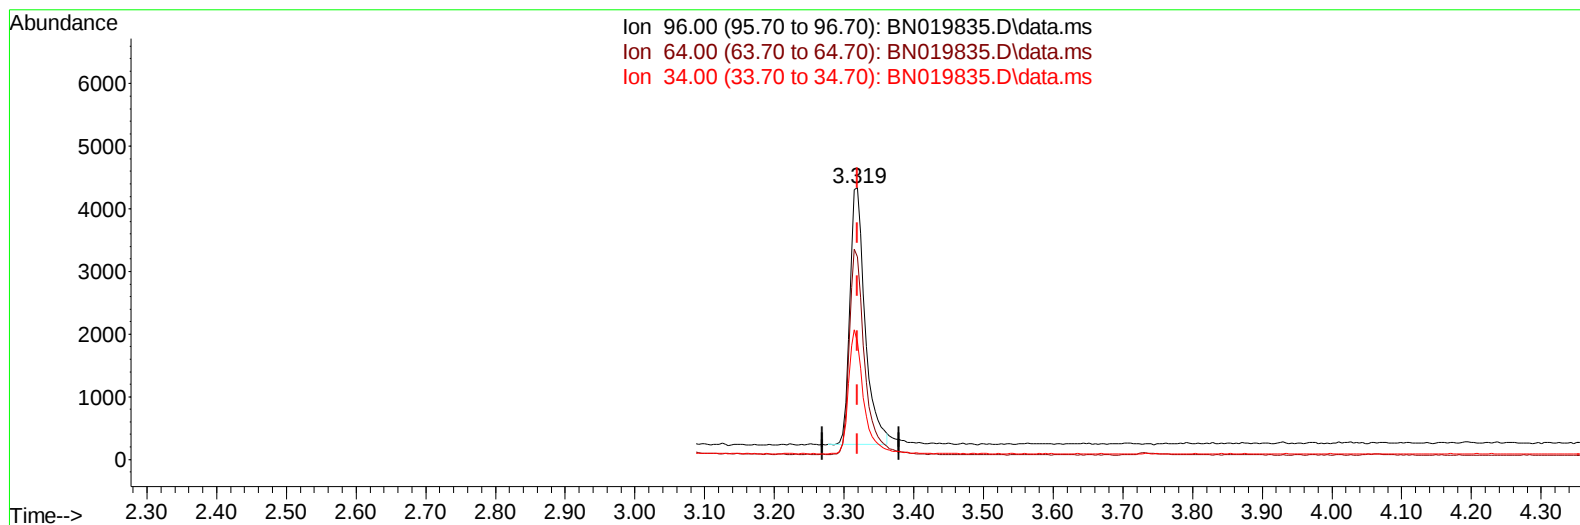

TIC: BN019835.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.319min (-0.000) 1.67 ng/u1

response 6199

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	74.51#
34.00	22.70	43.16#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051822\
 Data File : BN019835.D
 Acq On : 18 May 2022 17:31
 Operator : CG/JU
 Sample : N2766-10
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4G0

Manual IntegrationsAPPROVED

Quant Time: May 19 03:19:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
 Supervised By :mohammad ahmed 05/25/2022

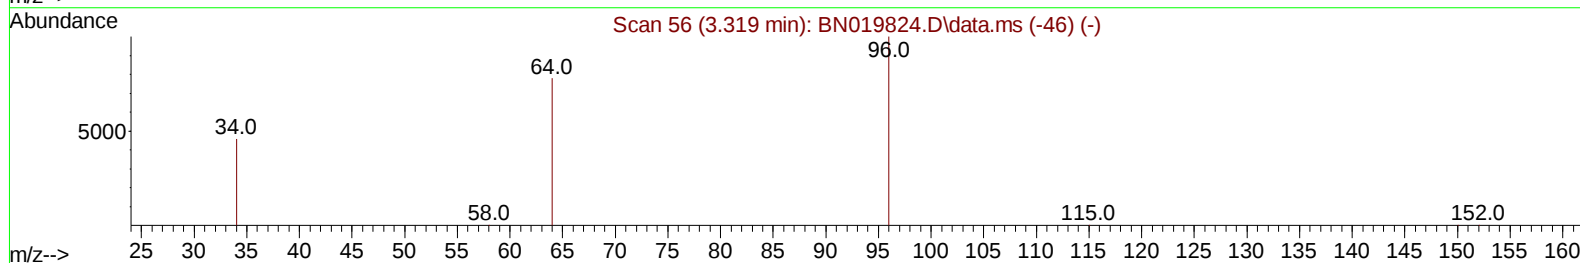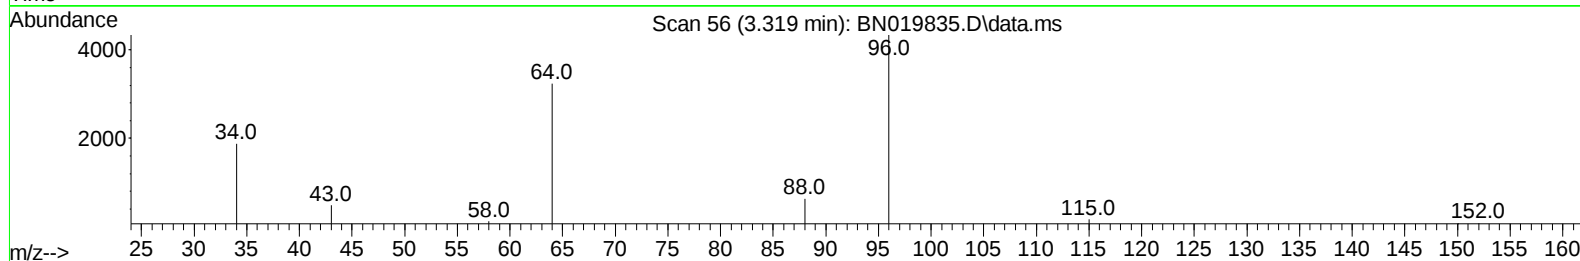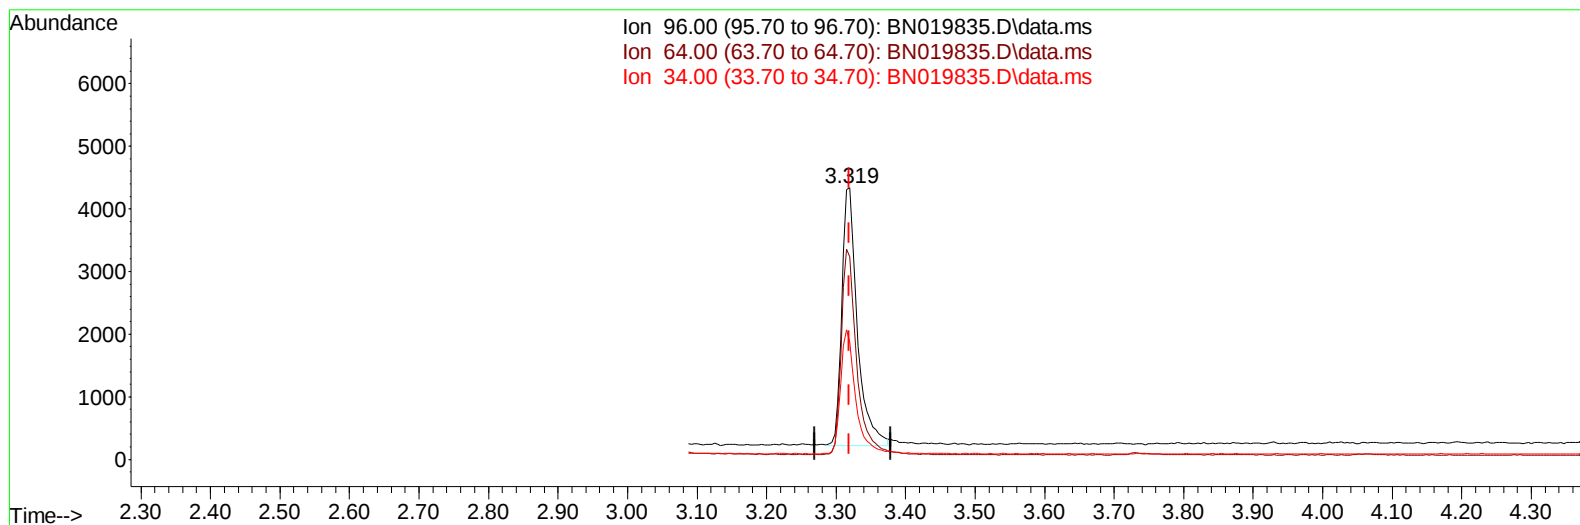

TIC: BN019835.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.319min (-0.000) 1.71 ng/ul m

response 6348

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	74.51#
34.00	22.70	43.16#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051822\
 Data File : BN019835.D
 Acq On : 18 May 2022 17:31
 Operator : CG/JU
 Sample : N2766-10
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4G0

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/19/2022
 Supervised By :mohammad ahmed 05/25/2022

Quant Time: May 19 03:19:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.855	152		3137	0.400	ng/ul	0.00
4) Naphthalene-d8	10.639	136		10907	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.474	164		7195	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.213	188		16090	0.400	ng/ul	0.00
17) Chrysene-d12	21.397	240		16121	0.400	ng/ul	0.00
23) Perylene-d12	23.735	264		15312	0.400	ng/ul	# 0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.319	96		6348m	1.710	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.228	152		2360	0.143	ng/ul	0.00
18) Fluoranthene-d10	19.239	212		6543	0.128	ng/ul	0.00
Target Compounds							
							Qvalue
15) Phenanthrene	17.255	178		1511	0.026	ng/ul#	84
22) Chrysene	21.435	228		1793	0.025	ng/ul#	75

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051822\
Data File : BN019835.D
Acq On : 18 May 2022 17:31
Operator : CG/JU
Sample : N2766-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4G0

Manual IntegrationsAPPROVED

Quant Time: May 19 03:19:48 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
Supervised By :mohammad ahmed 05/25/2022

