




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051822\
Data File : BN019836.D
Acq On : 18 May 2022 18:08
Operator : CG/JU
Sample : N2766-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4F4

Manual IntegrationsAPPROVED

Quant Time: May 19 03:19:51 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
Supervised By :mohammad ahmed 05/25/2022

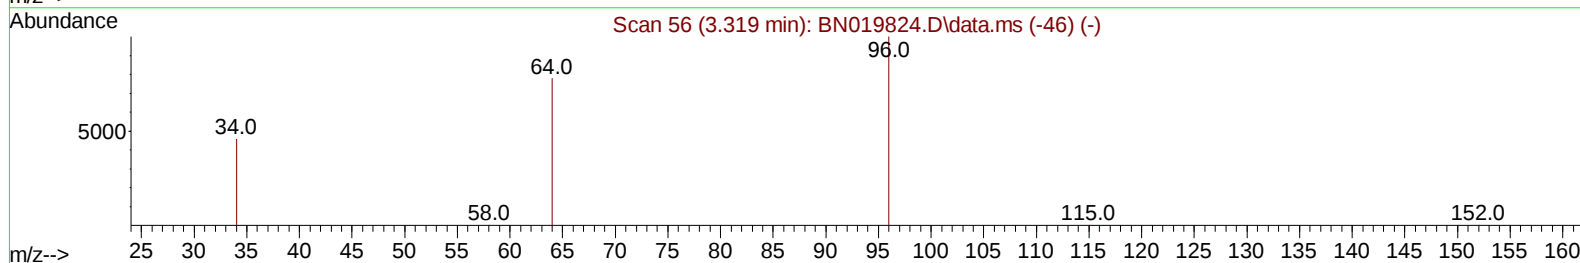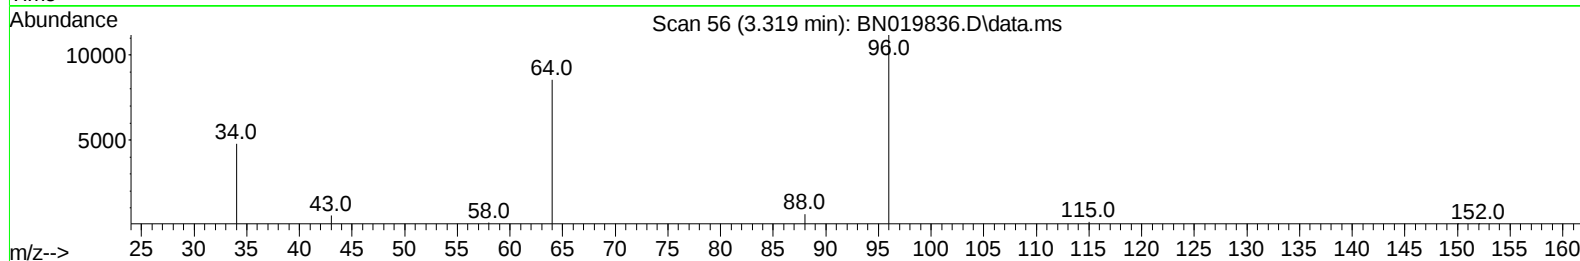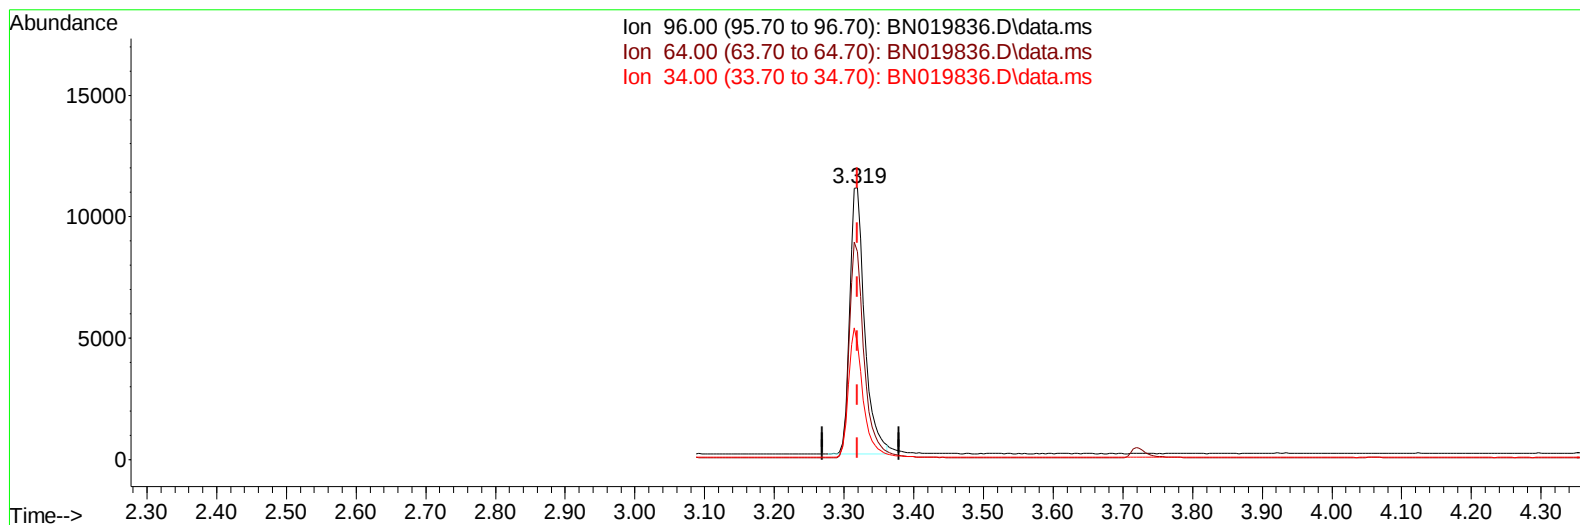

TIC: BN019836.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.319min (-0.000) 3.78 ng/u1

response 16157

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	76.44#
34.00	22.70	42.79#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051822\
Data File : BN019836.D
Acq On : 18 May 2022 18:08
Operator : CG/JU
Sample : N2766-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4F4

Manual IntegrationsAPPROVED

Quant Time: May 19 03:19:51 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
Supervised By :mohammad ahmed 05/25/2022

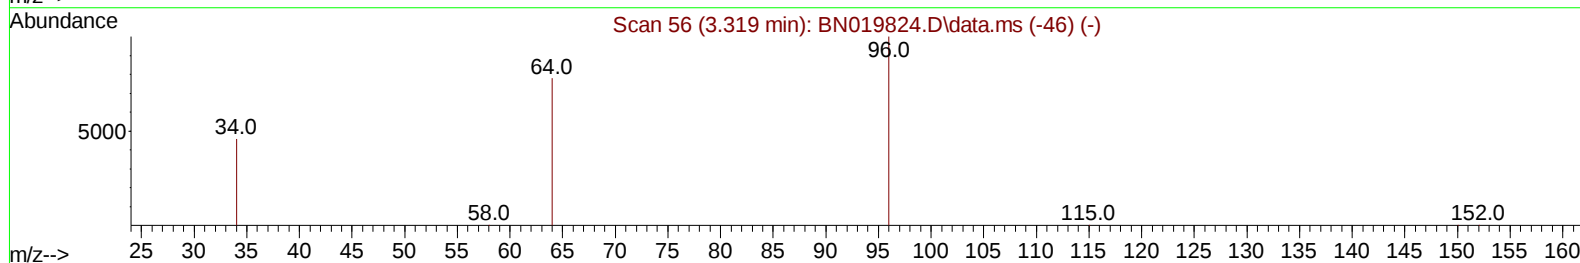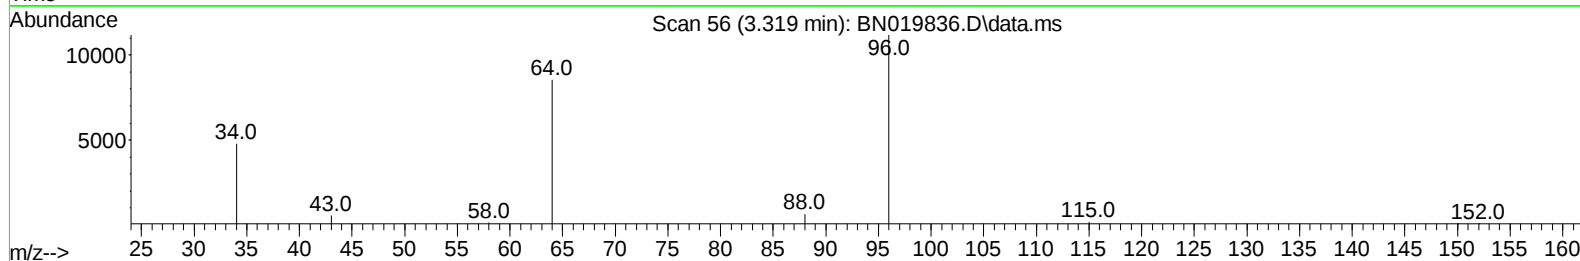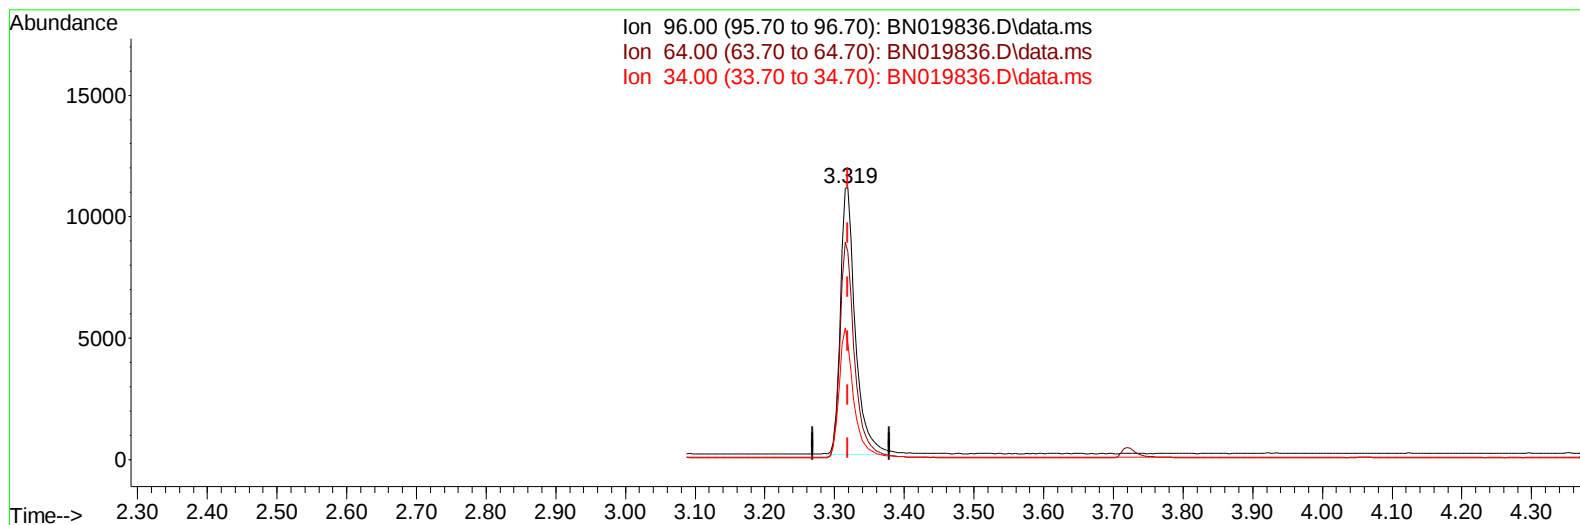

TIC: BN019836.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.319min (-0.000) 3.87 ng/ul m

response 16549

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	76.44#
34.00	22.70	42.79#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051822\
 Data File : BN019836.D
 Acq On : 18 May 2022 18:08
 Operator : CG/JU
 Sample : N2766-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4F4

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/19/2022
 Supervised By :mohammad ahmed 05/25/2022

Quant Time: May 19 03:19:51 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.855	152		3616	0.400	ng/ul	0.00
4) Naphthalene-d8	10.639	136		12735	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.474	164		8583	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.213	188		19289	0.400	ng/ul	0.00
17) Chrysene-d12	21.398	240		18688	0.400	ng/ul	0.00
23) Perylene-d12	23.734	264		17786	0.400	ng/ul	#-0.01
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.319	96		16549m	3.867	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.228	152		5343	0.277	ng/ul	0.00
18) Fluoranthene-d10	19.244	212		14302	0.242	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051822\
Data File : BN019836.D
Acq On : 18 May 2022 18:08
Operator : CG/JU
Sample : N2766-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4F4

Manual IntegrationsAPPROVED

Quant Time: May 19 03:19:51 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
Supervised By :mohammad ahmed 05/25/2022

