




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051822\
Data File : BN019845.D
Acq On : 19 May 2022 00:07
Operator : CG/JU
Sample : N2766-11
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4G1

Manual IntegrationsAPPROVED

Quant Time: May 19 05:38:21 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
Supervised By :mohammad ahmed 05/25/2022

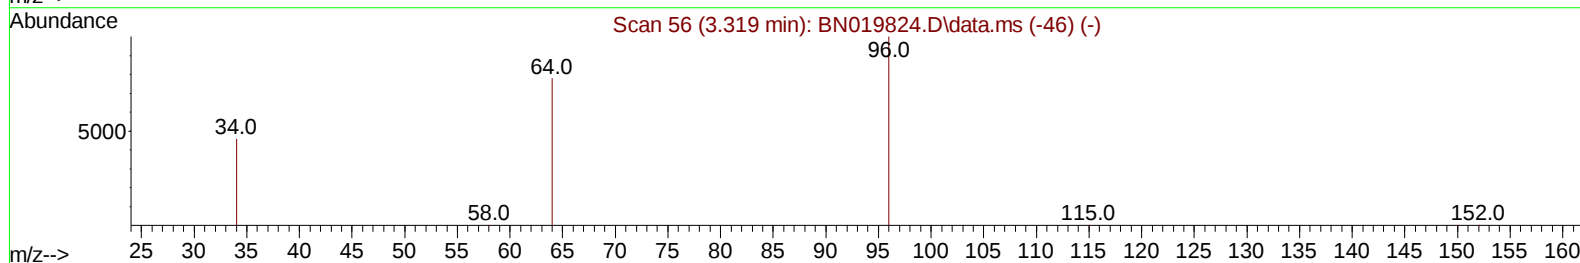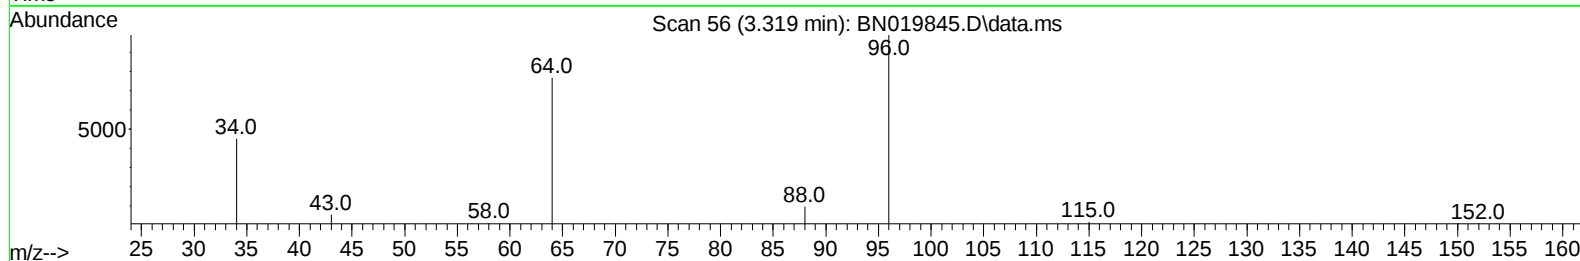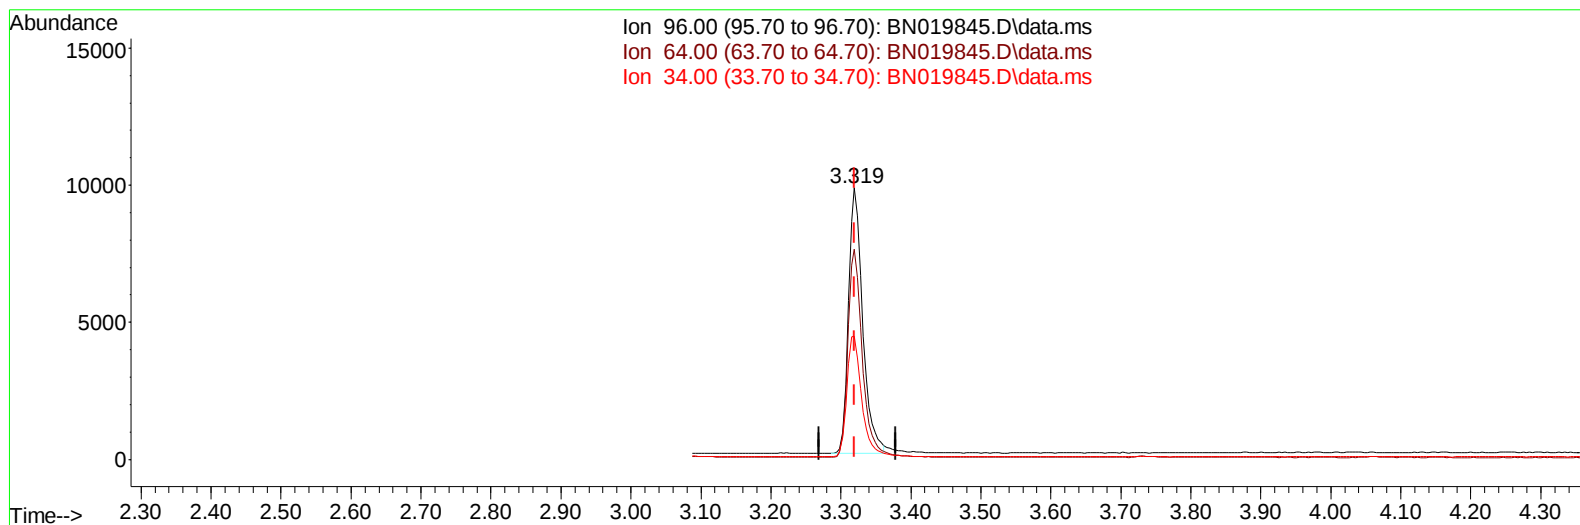

TIC: BN019845.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.319min (+ 0.000) 2.02 ng/u1

response 13619

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	77.38#
34.00	22.70	45.48#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051822\
Data File : BN019845.D
Acq On : 19 May 2022 00:07
Operator : CG/JU
Sample : N2766-11
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4G1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/19/2022
Supervised By :mohammad ahmed 05/25/2022

Quant Time: May 19 05:38:21 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

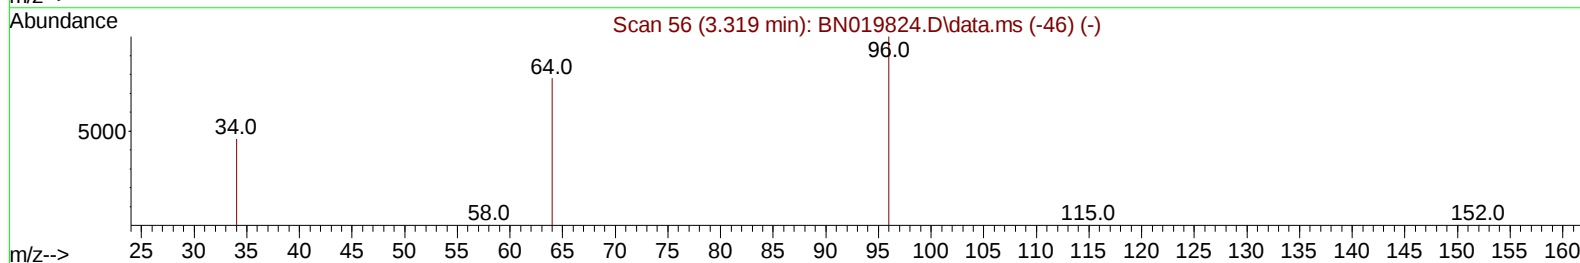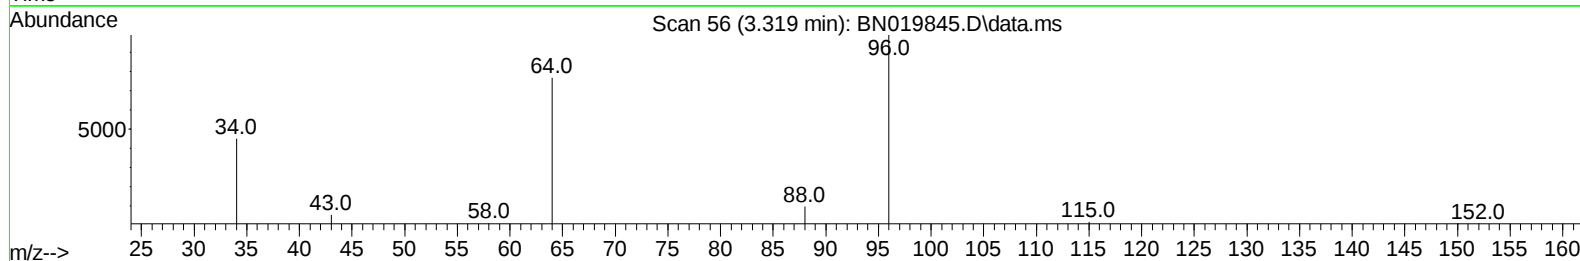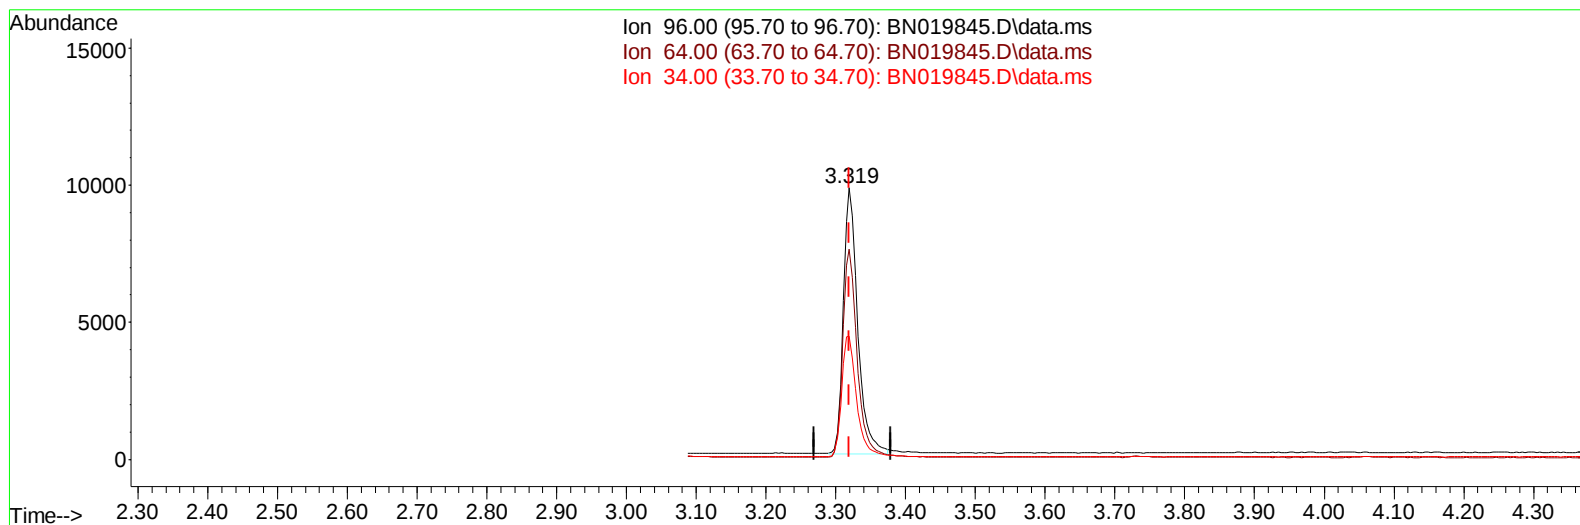

TIC: BN019845.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.319min (+ 0.000) 2.07 ng/ul m

response 13950

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	77.38#
34.00	22.70	45.48#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051822\
Data File : BN019845.D
Acq On : 19 May 2022 00:07
Operator : CG/JU
Sample : N2766-11
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4G1

Manual IntegrationsAPPROVED

Quant Time: May 19 05:38:21 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
Supervised By :mohammad ahmed 05/25/2022

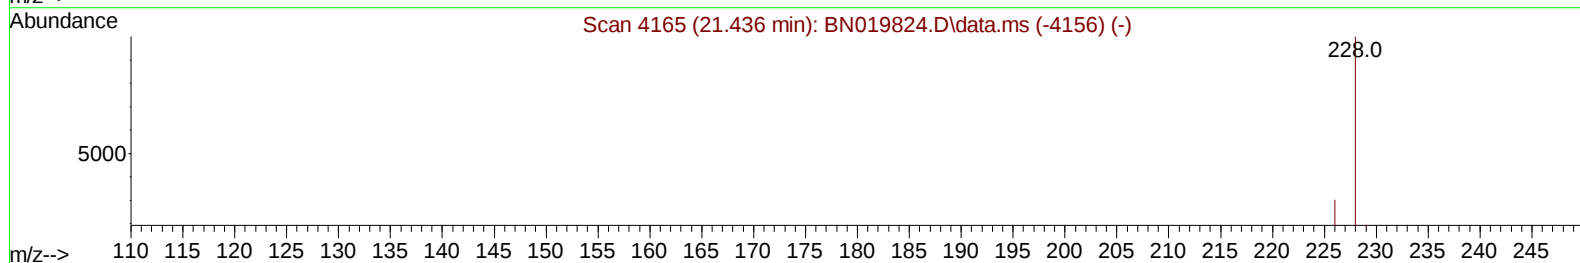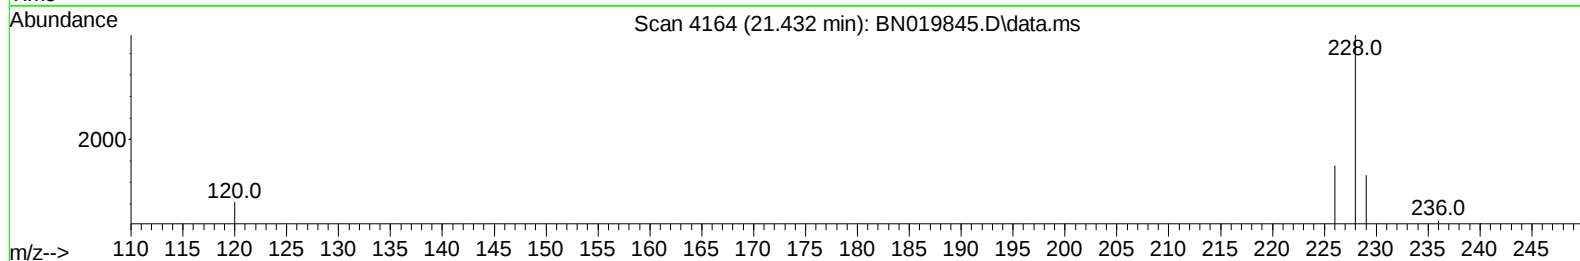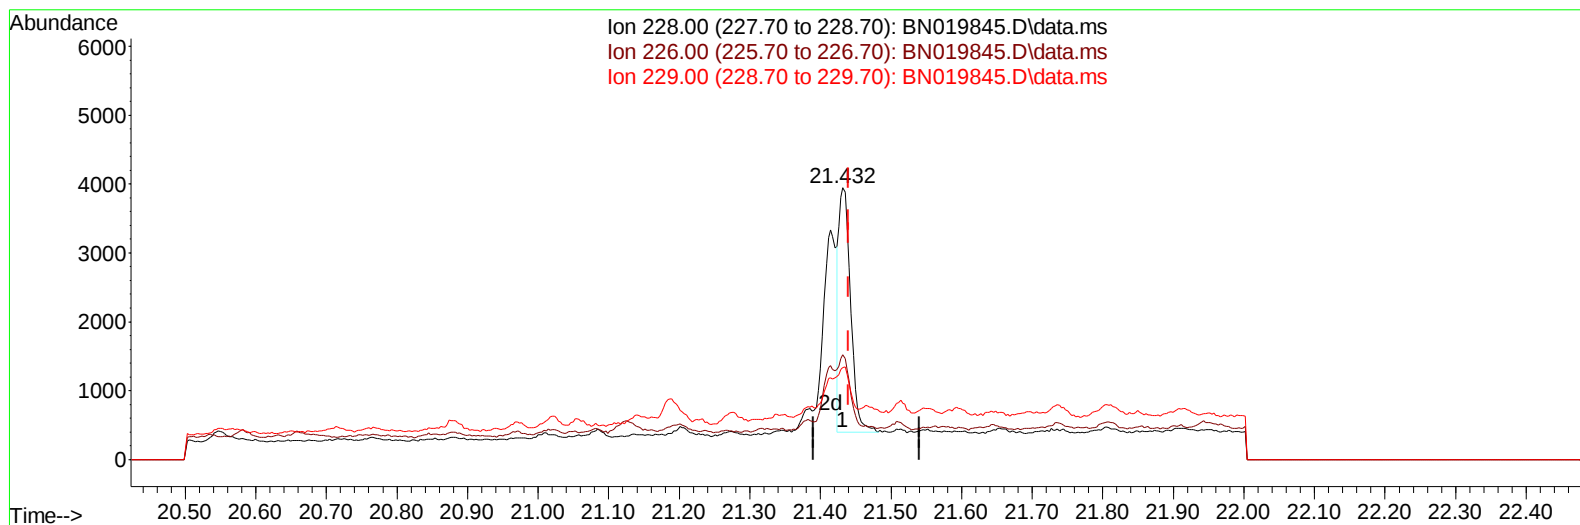

TIC: BN019845.D\data.ms

(22) Chrysene

21.432min (-0.009) 0.05 ng/u1

response 4104

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	30.20	38.45#
229.00	20.00	33.84#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051822\
 Data File : BN019845.D
 Acq On : 19 May 2022 00:07
 Operator : CG/JU
 Sample : N2766-11
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4G1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/19/2022
 Supervised By :mohammad ahmed 05/25/2022

Quant Time: May 19 05:38:21 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

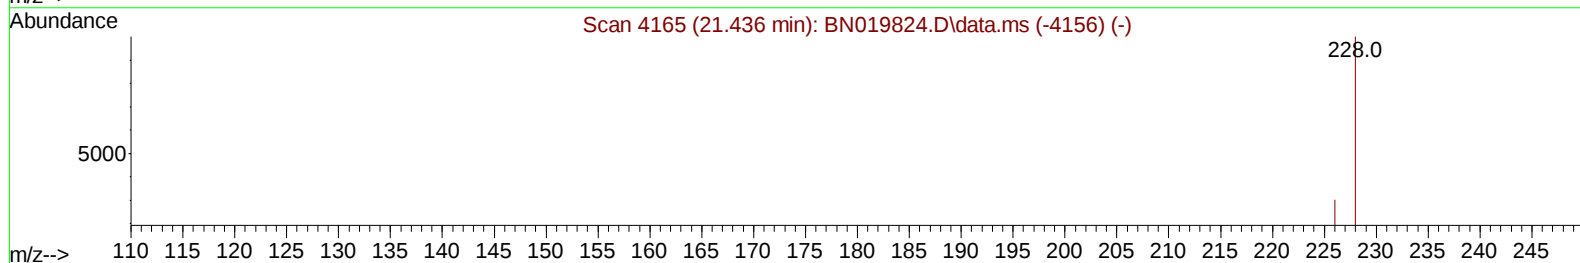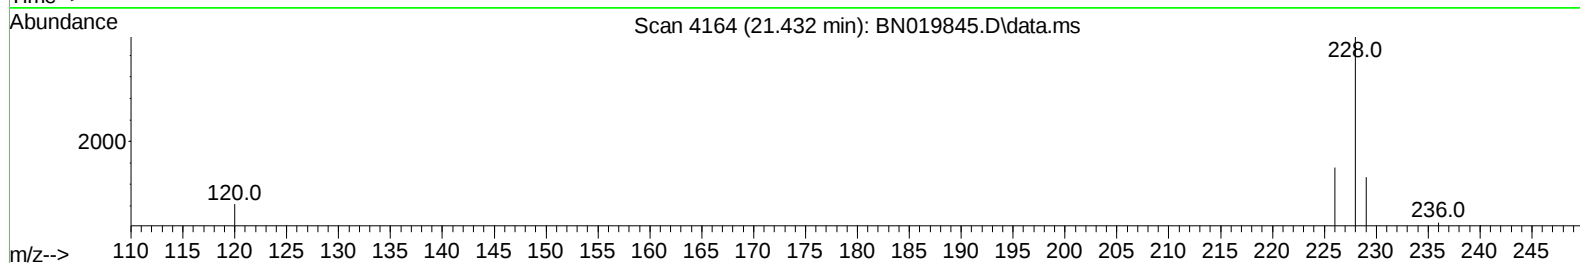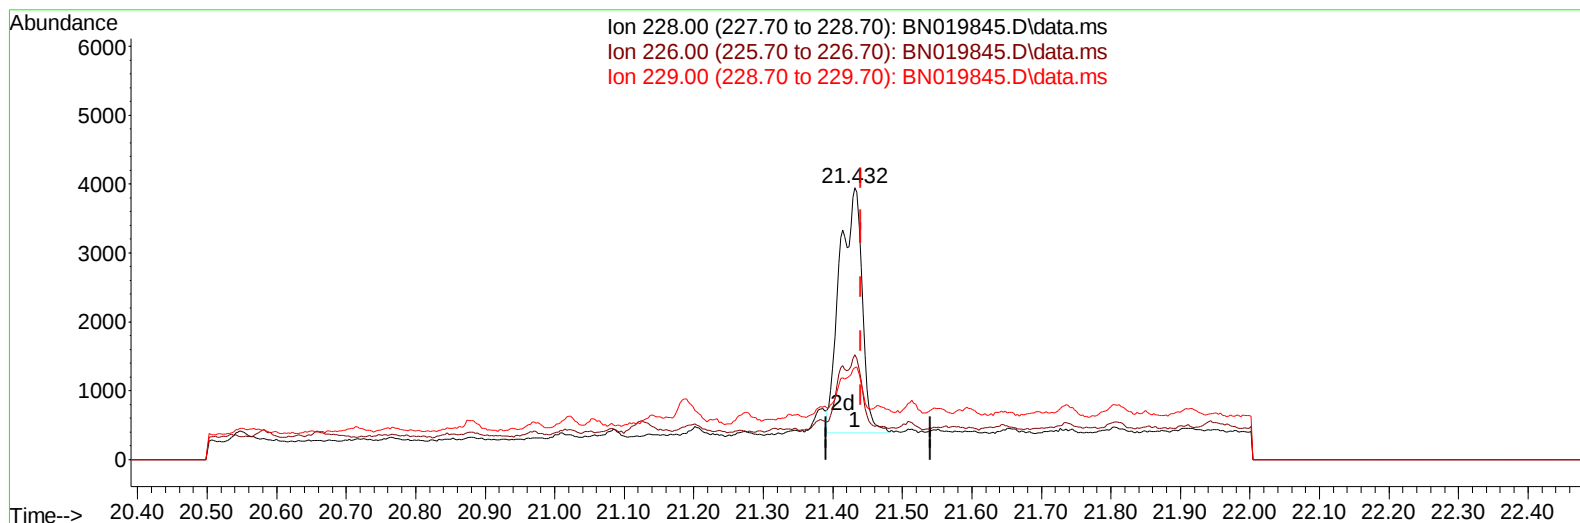

TIC: BN019845.D\data.ms

(22) Chrysene

21.432min (-0.009) 0.09 ng/u1 m

response 7961

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	30.20	38.45#
229.00	20.00	33.84#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051822\
 Data File : BN019845.D
 Acq On : 19 May 2022 00:07
 Operator : CG/JU
 Sample : N2766-11
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4G1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/19/2022
 Supervised By :mohammad ahmed 05/25/2022

Quant Time: May 19 05:38:21 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.855	152		5689	0.400	ng/ul	0.00
4) Naphthalene-d8	10.639	136		19729	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.474	164		12390	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.213	188		25929	0.400	ng/ul	0.00
17) Chrysene-d12	21.397	240		19787	0.400	ng/ul	0.00
23) Perylene-d12	23.735	264		15570	0.400	ng/ul	# 0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.319	96		13950m	2.072	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.229	152		4826	0.162	ng/ul	0.00
18) Fluoranthene-d10	19.239	212		13019	0.208	ng/ul	0.00
Target Compounds							Qvalue
15) Phenanthrene	17.255	178		10232	0.107	ng/ul#	94
20) Pyrene	19.634	202		4277	0.047	ng/ul#	69
22) Chrysene	21.432	228		7961m	0.091	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051822\
Data File : BN019845.D
Acq On : 19 May 2022 00:07
Operator : CG/JU
Sample : N2766-11
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4G1

Manual IntegrationsAPPROVED

Quant Time: May 19 05:38:21 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
Supervised By :mohammad ahmed 05/25/2022

