




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051822\
Data File : BN019846.D
Acq On : 19 May 2022 00:43
Operator : CG/JU
Sample : N2766-09
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4F9

Manual IntegrationsAPPROVED

Quant Time: May 19 05:39:59 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
Supervised By :mohammad ahmed 05/25/2022

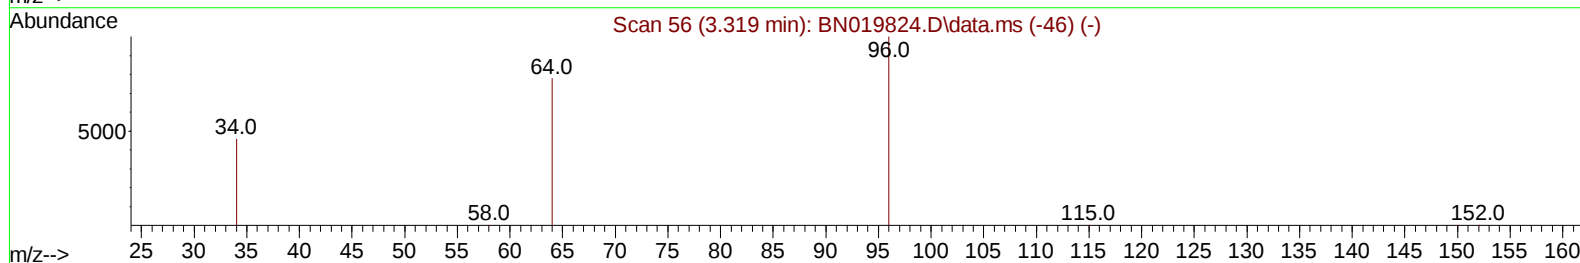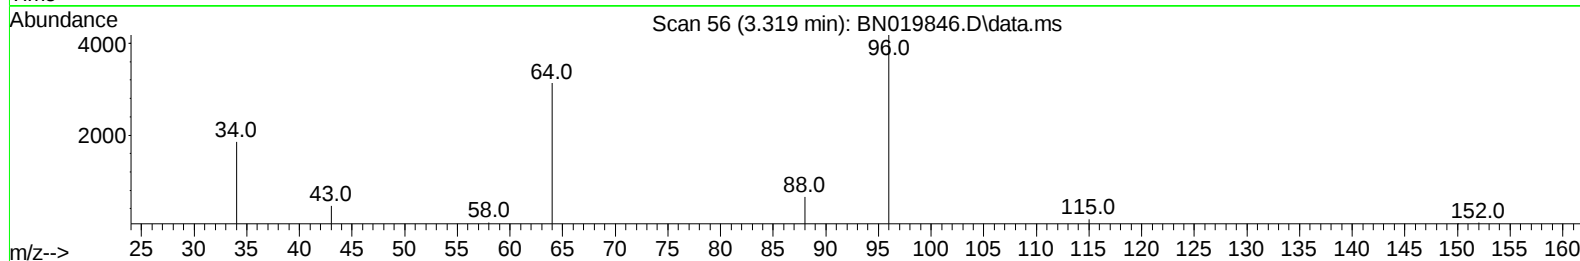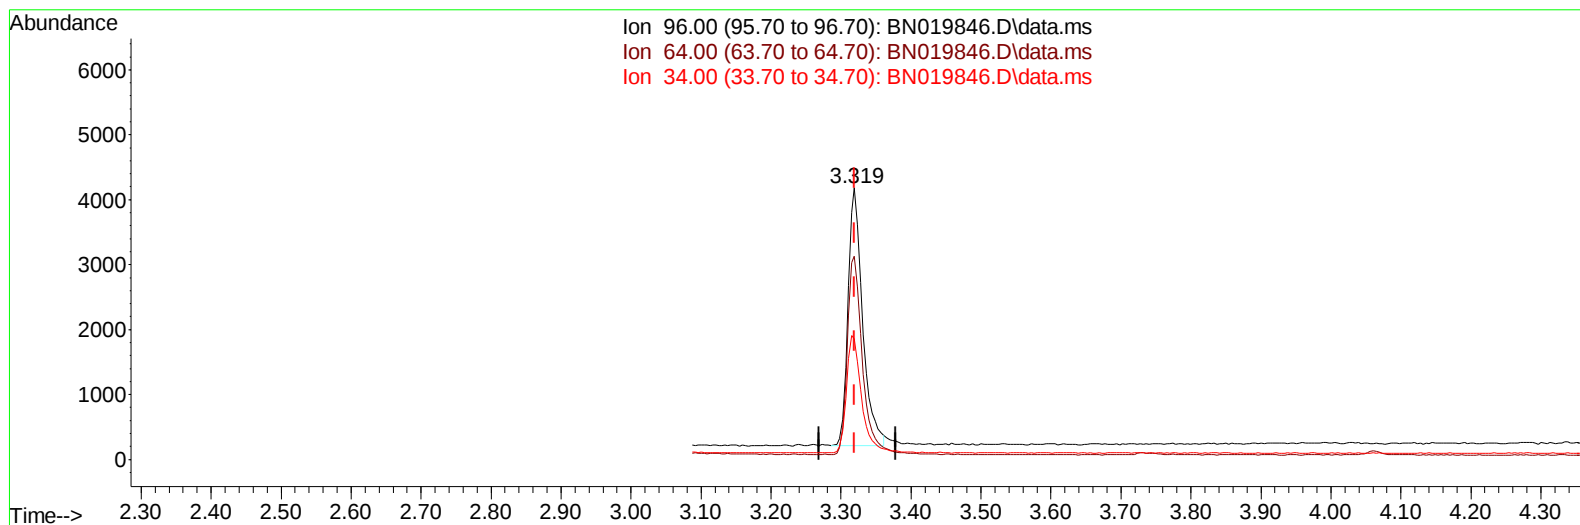

TIC: BN019846.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.319min (-0.000) 1.03 ng/u1

response 5727

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	74.91#
34.00	22.70	44.49#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051822\
 Data File : BN019846.D
 Acq On : 19 May 2022 00:43
 Operator : CG/JU
 Sample : N2766-09
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4F9

Manual IntegrationsAPPROVED

Quant Time: May 19 05:39:59 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
 Supervised By :mohammad ahmed 05/25/2022

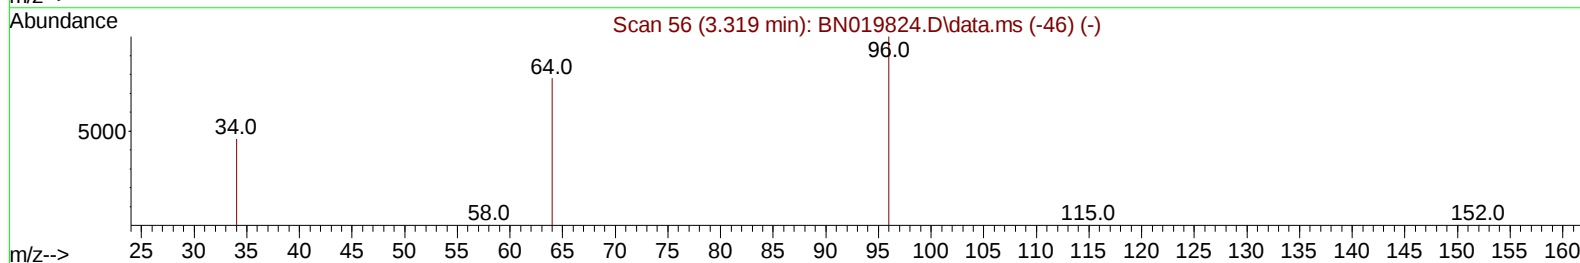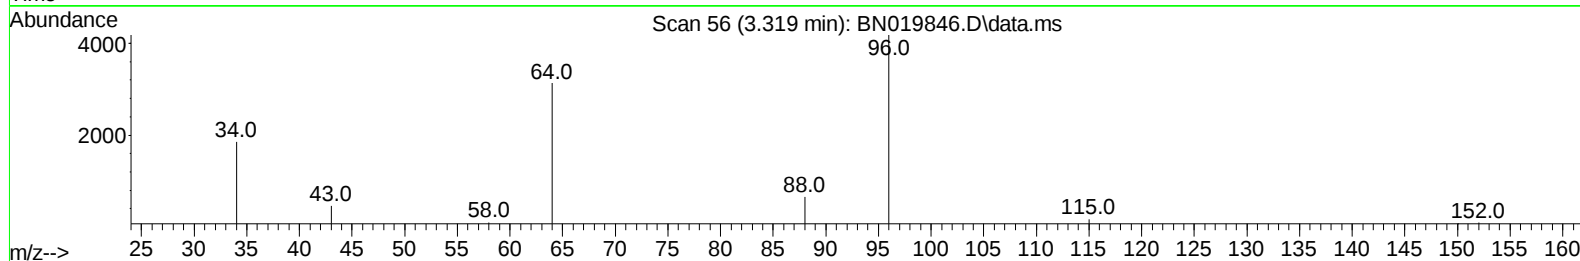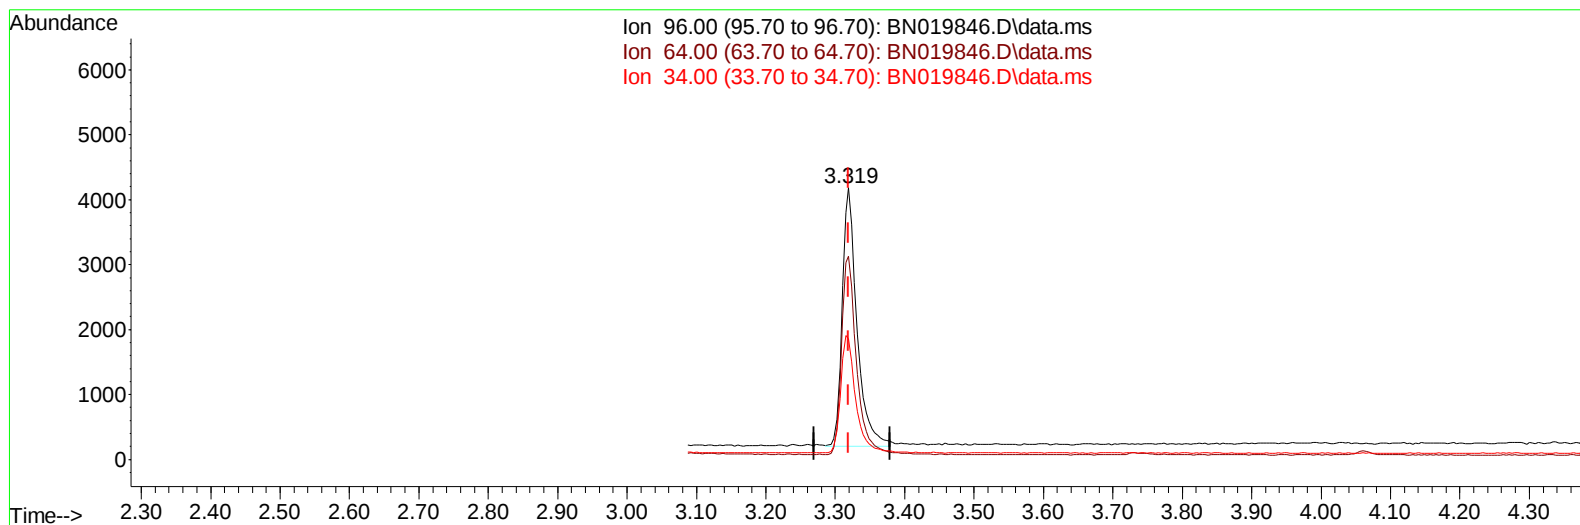

TIC: BN019846.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.319min (-0.000) 1.05 ng/ul m

response 5865

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	74.91#
34.00	22.70	44.49#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051822\
 Data File : BN019846.D
 Acq On : 19 May 2022 00:43
 Operator : CG/JU
 Sample : N2766-09
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4F9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/19/2022
 Supervised By :mohammad ahmed 05/25/2022

Quant Time: May 19 05:39:59 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.855	152	4714	0.400	ng/ul	0.00
4) Naphthalene-d8	10.639	136	16545	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.475	164	10303	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.214	188	21678	0.400	ng/ul	0.00
17) Chrysene-d12	21.398	240	17707	0.400	ng/ul	0.00
23) Perylene-d12	23.733	264	13856	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.319	96	5865m	1.051	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.228	152	2087	0.083	ng/ul	0.00
18) Fluoranthene-d10	19.240	212	4822	0.086	ng/ul	0.00
Target Compounds						Qvalue
7) 2-Methylnaphthalene	12.305	142	727	0.022	ng/ul#	100
8) 1-Methylnaphthalene	12.520	142	716	0.024	ng/ul#	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051822\
Data File : BN019846.D
Acq On : 19 May 2022 00:43
Operator : CG/JU
Sample : N2766-09
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4F9

Manual IntegrationsAPPROVED

Quant Time: May 19 05:39:59 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
Supervised By :mohammad ahmed 05/25/2022

