




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051822\
Data File : BN019847.D
Acq On : 19 May 2022 01:19
Operator : CG/JU
Sample : N2766-05
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4F5

Manual IntegrationsAPPROVED

Quant Time: May 19 05:41:31 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
Supervised By :mohammad ahmed 05/25/2022

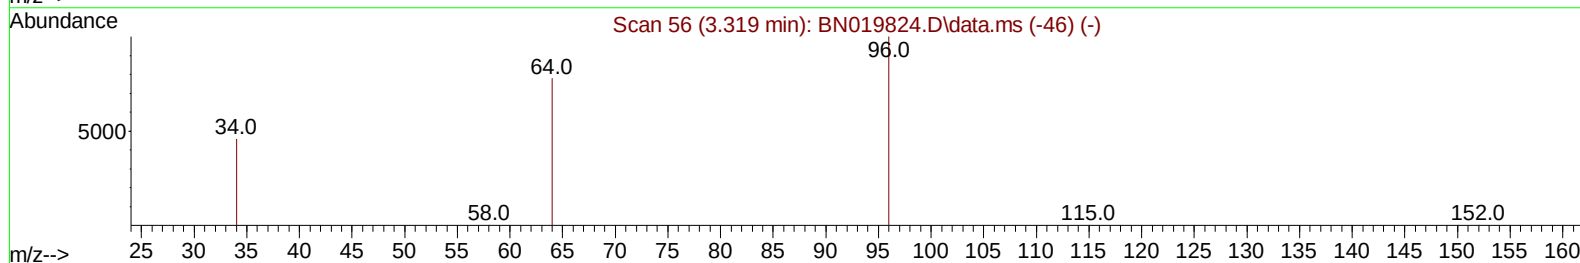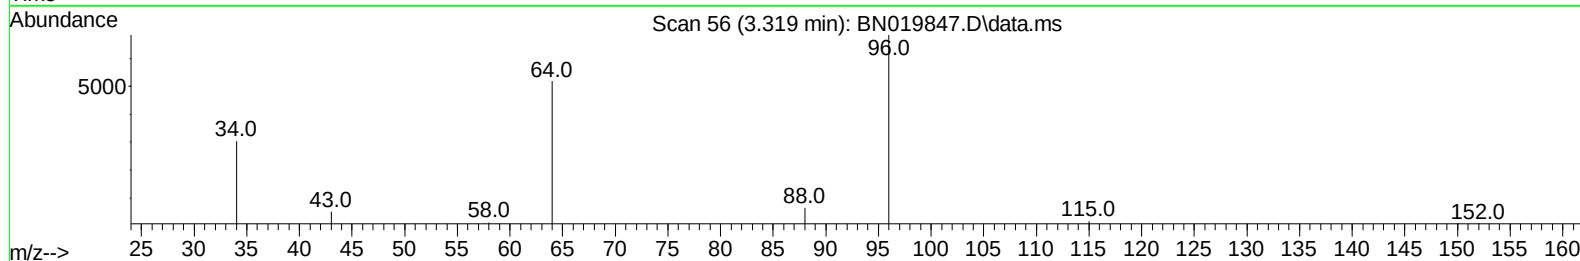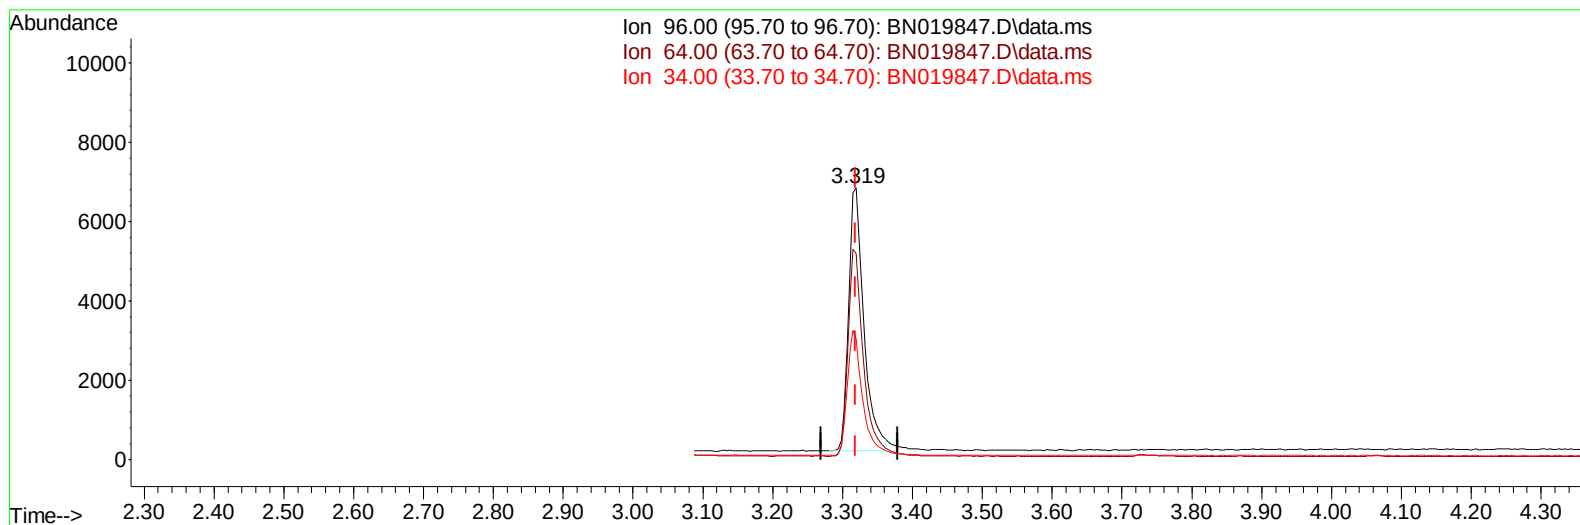

TIC: BN019847.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.319min (-0.000) 1.91 ng/u1

response 10043

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	75.77#
34.00	22.70	44.35#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051822\
 Data File : BN019847.D
 Acq On : 19 May 2022 01:19
 Operator : CG/JU
 Sample : N2766-05
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4F5

Manual IntegrationsAPPROVED

Quant Time: May 19 05:41:31 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
 Supervised By :mohammad ahmed 05/25/2022

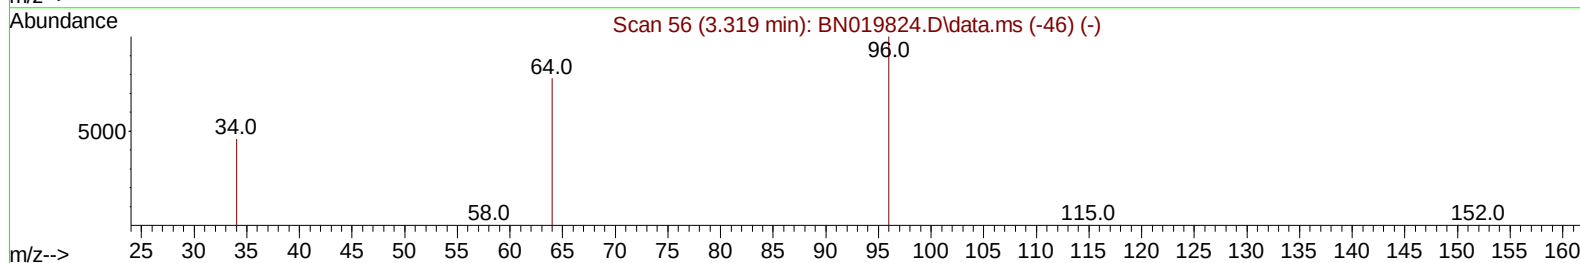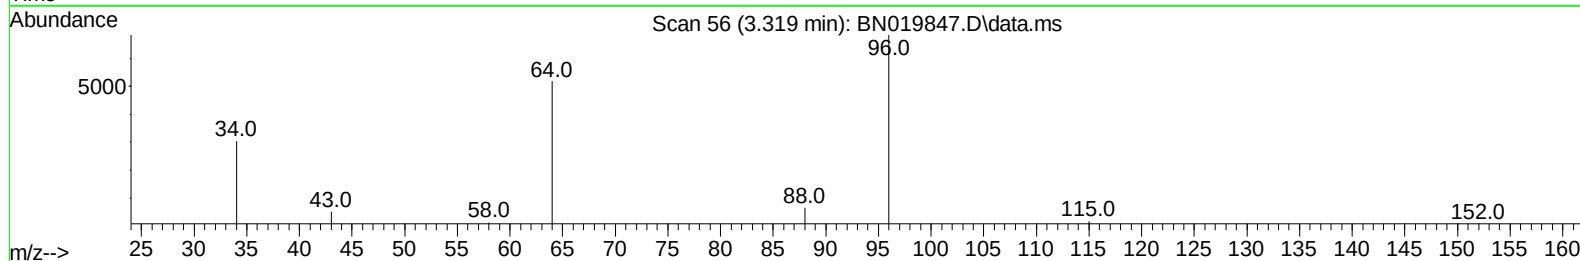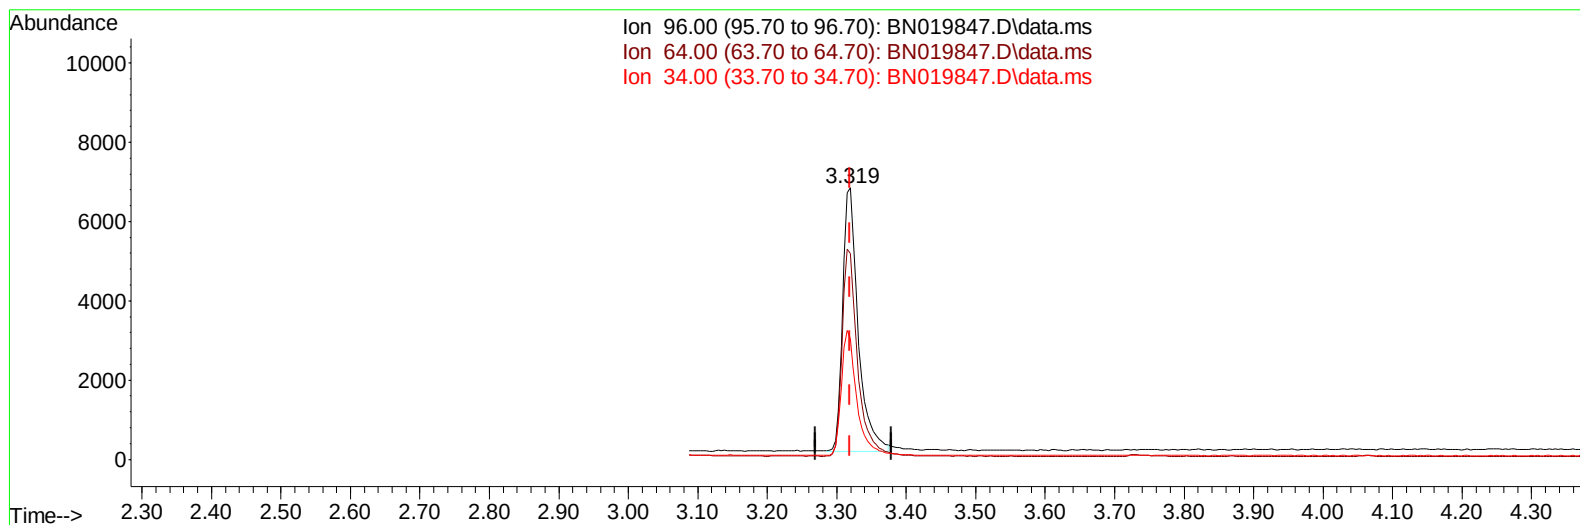

TIC: BN019847.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.319min (-0.000) 1.95 ng/ul m

response 10276

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	75.77#
34.00	22.70	44.35#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051822\
 Data File : BN019847.D
 Acq On : 19 May 2022 01:19
 Operator : CG/JU
 Sample : N2766-05
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4F5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/19/2022
 Supervised By :mohammad ahmed 05/25/2022

Quant Time: May 19 05:41:31 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.855	152		4446	0.400	ng/ul	0.00
4) Naphthalene-d8	10.639	136		15397	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.474	164		9505	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.213	188		20075	0.400	ng/ul	0.00
17) Chrysene-d12	21.401	240		17454	0.400	ng/ul	0.00
23) Perylene-d12	23.740	264		14088	0.400	ng/ul	# 0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.319	96		10276m	1.953	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.228	152		3709	0.159	ng/ul	0.00
18) Fluoranthene-d10	19.243	212		10774	0.195	ng/ul	0.00
Target Compounds							
						Qvalue	
15) Phenanthrene	17.255	178		1800	0.024	ng/ul#	82
22) Chrysene	21.436	228		1843	0.024	ng/ul#	56
29) Benzo(g,h,i)perylene	26.877	276		2509	0.036	ng/ul#	71

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051822\
Data File : BN019847.D
Acq On : 19 May 2022 01:19
Operator : CG/JU
Sample : N2766-05
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4F5

Manual IntegrationsAPPROVED

Quant Time: May 19 05:41:31 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
Supervised By :mohammad ahmed 05/25/2022

