




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051822\
 Data File : BN019849.D
 Acq On : 19 May 2022 02:30
 Operator : CG/JU
 Sample : N2766-22
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4H2

Manual IntegrationsAPPROVED

Quant Time: May 19 05:45:26 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
 Supervised By :mohammad ahmed 05/25/2022

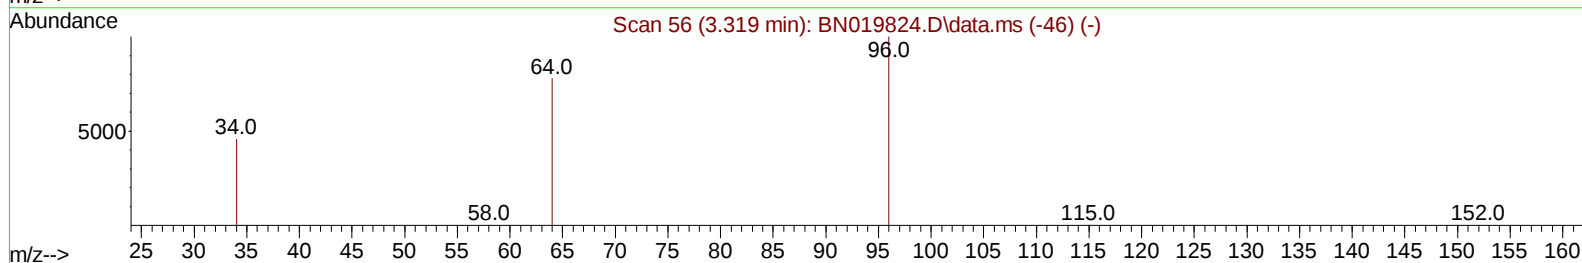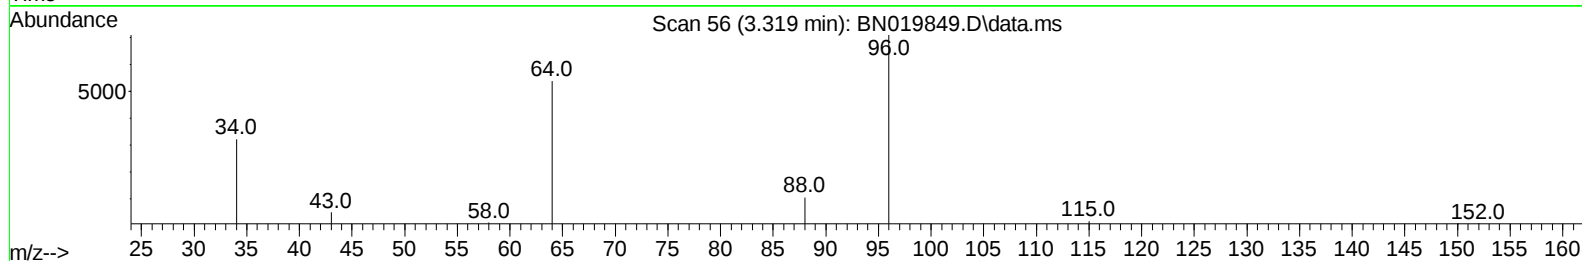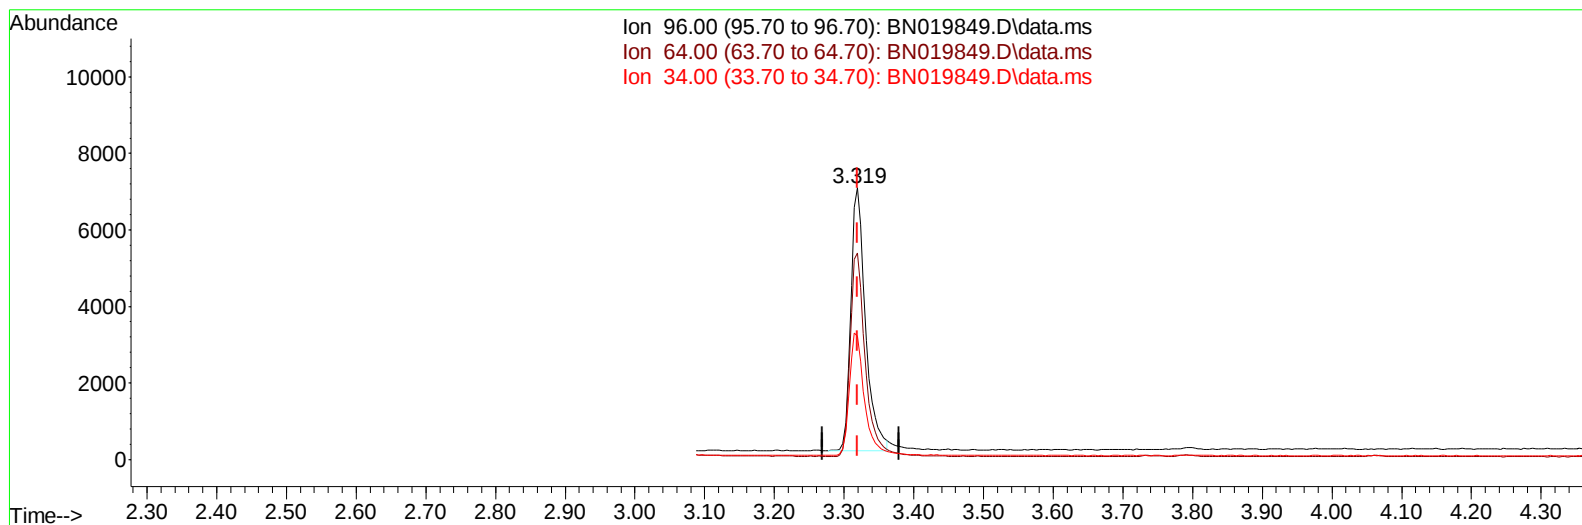

TIC: BN019849.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.319min (-0.000) 1.78 ng/u1

response 9965

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	75.98#
34.00	22.70	45.37#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051822\
Data File : BN019849.D
Acq On : 19 May 2022 02:30
Operator : CG/JU
Sample : N2766-22
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4H2

Manual IntegrationsAPPROVED

Quant Time: May 19 05:45:26 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
Supervised By :mohammad ahmed 05/25/2022

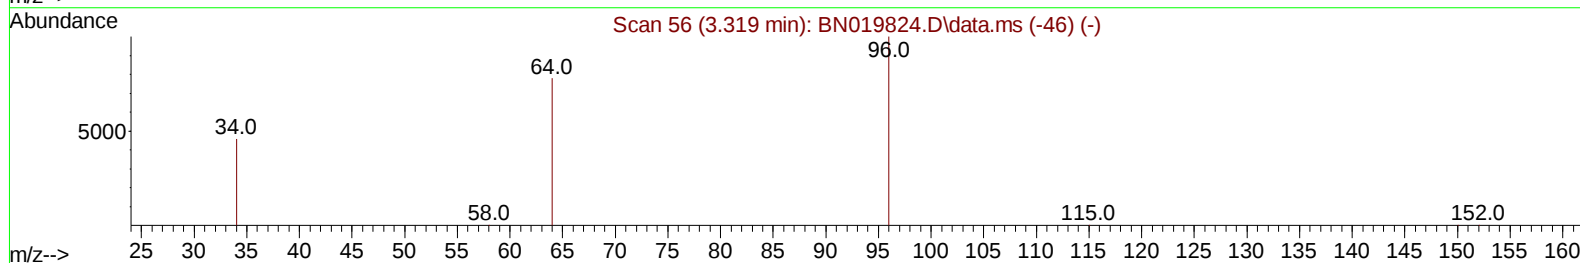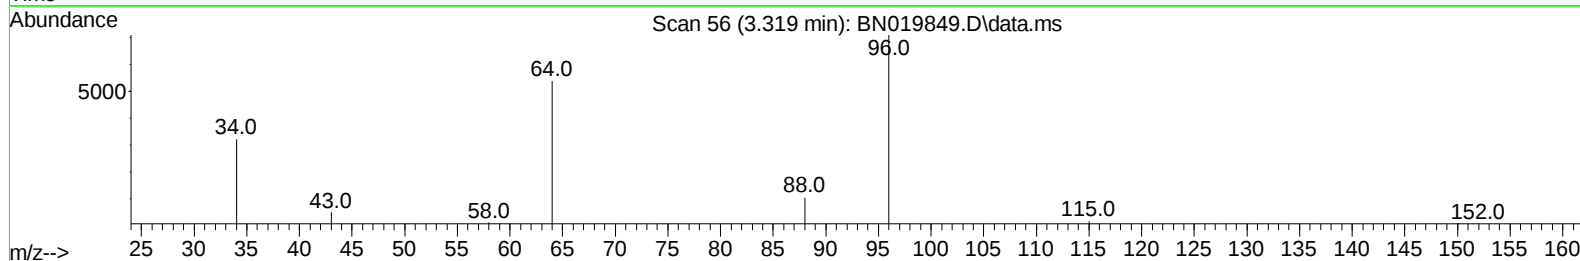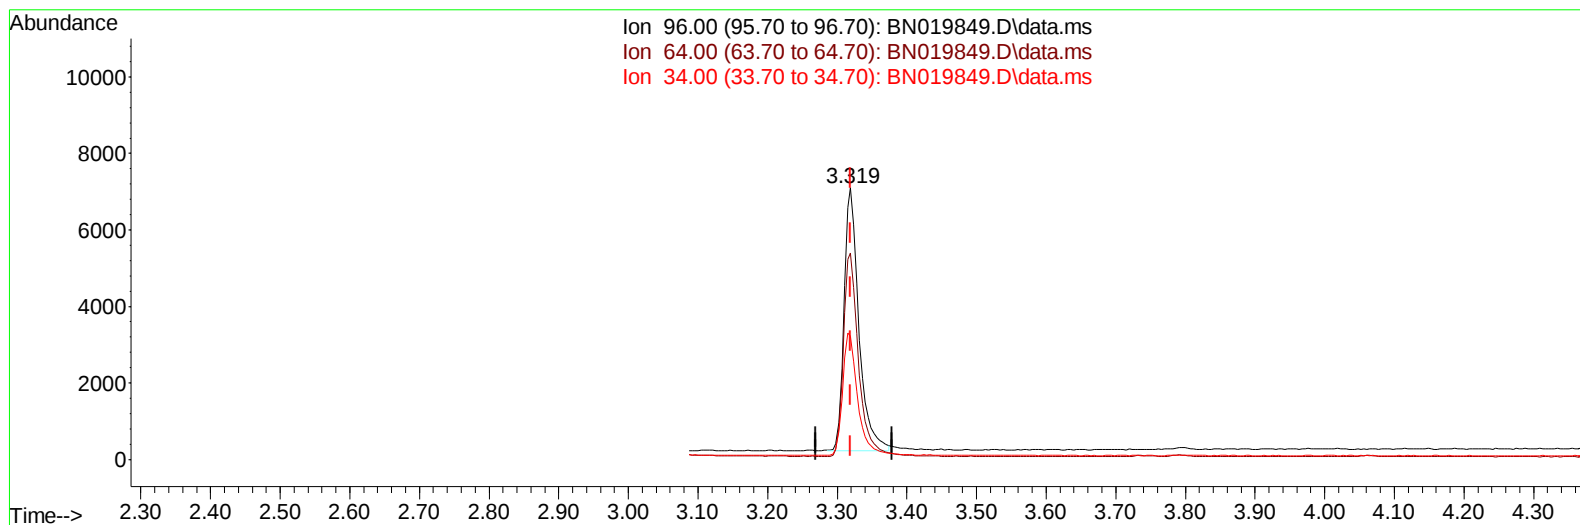

TIC: BN019849.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.319min (-0.000) 1.82 ng/ul m

response 10144

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	75.98#
34.00	22.70	45.37#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051822\
 Data File : BN019849.D
 Acq On : 19 May 2022 02:30
 Operator : CG/JU
 Sample : N2766-22
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4H2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/19/2022
 Supervised By :mohammad ahmed 05/25/2022

Quant Time: May 19 05:45:26 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.855	152		4720	0.400	ng/ul	0.00
4) Naphthalene-d8	10.639	136		16278	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.474	164		11772	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.213	188		20613	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.404	240		15432	0.400	ng/ul	# 0.00
23) Perylene-d12	23.748	264		14006	0.400	ng/ul	# 0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.319	96		10144m	1.816	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.228	152		3896	0.158	ng/ul	0.00
18) Fluoranthene-d10	19.243	212		10163	0.208	ng/ul	0.00
Target Compounds							
							Qvalue
5) Naphthalene	10.689	128		6020	0.114	ng/ul#	93
7) 2-Methylnaphthalene	12.300	142		25087	0.781	ng/ul#	100
8) 1-Methylnaphthalene	12.520	142		19212	0.646	ng/ul#	100
11) Acenaphthene	14.562	153		4950	0.106	ng/ul#	17
12) Fluorene	15.520	166		16398	0.319	ng/ul#	70
15) Phenanthrene	17.255	178		82659	1.090	ng/ul#	89
19) Fluoranthene	19.276	202		12590	0.178	ng/ul#	69
20) Pyrene	19.639	202		20255	0.287	ng/ul#	64
22) Chrysene	21.422	228		15807	0.233	ng/ul#	11

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051822\
Data File : BN019849.D
Acq On : 19 May 2022 02:30
Operator : CG/JU
Sample : N2766-22
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4H2

Manual IntegrationsAPPROVED

Quant Time: May 19 05:45:26 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
Supervised By :mohammad ahmed 05/25/2022

